

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032619\
 Data File : PL046469.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2019 12:41
 Operator : AJ\SJ
 Sample : MDL-CHL-S-03
 Misc : 25 PPB
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-CHL-S-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:05:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.359	3.978	135.6E6	43559198	18.647	19.025
28)	SA Decachlor...	8.036	9.029	166.6E6	48300455	19.808	20.833
Target Compounds							
23)	Chlordane-1	4.204	4.969	6464956	2269805	19.224	20.975
24)	Chlordane-2	4.696	5.436	9097627	2937909	23.978	25.151
25)	Chlordane-3	5.253	6.082	21513354	8982579	19.317	23.560
26)	Chlordane-4	5.309	6.155	20370276	10959893	19.699	23.752
27)	Chlordane-5	6.133	6.958	6078730	1867656	17.812	20.789



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032619\
Data File : PL046469.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2019 12:41
Operator : AJ\SJ
Sample : MDL-CHL-S-03
Misc : 25 PPB
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-S-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:05:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

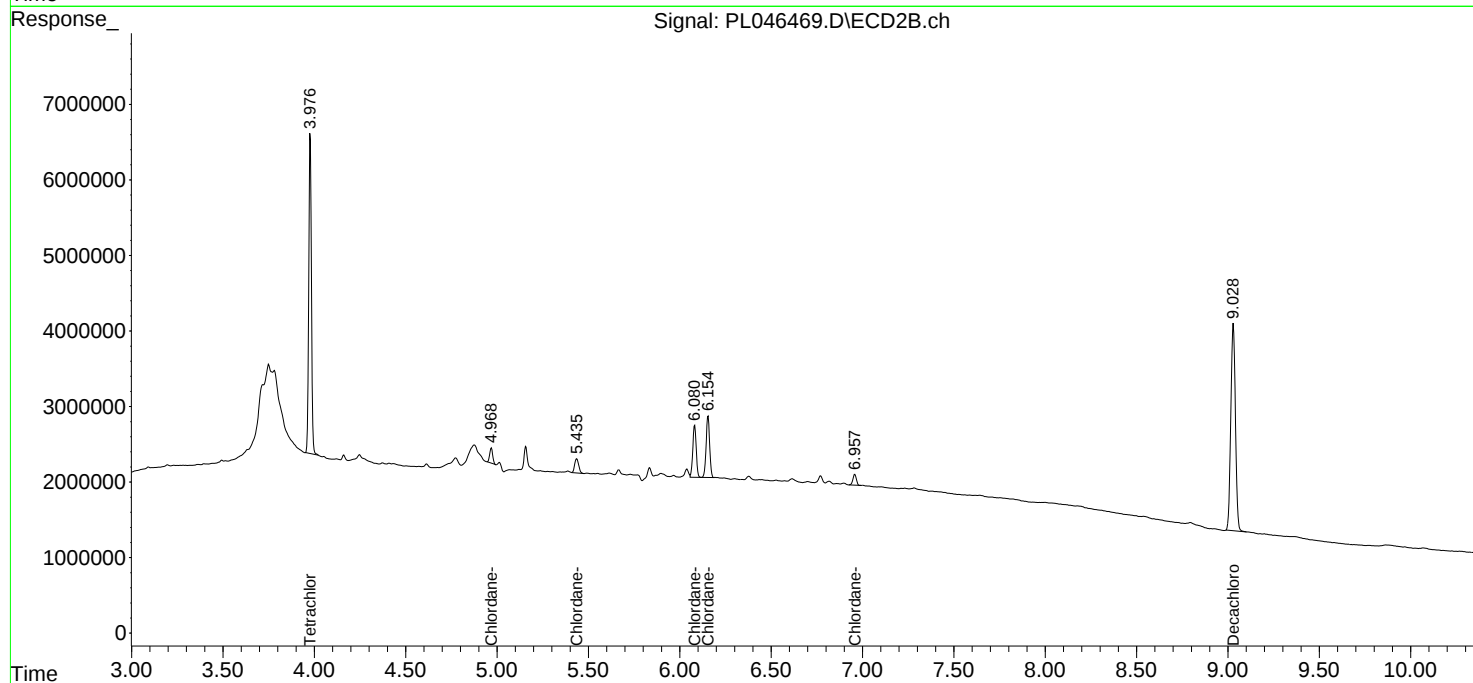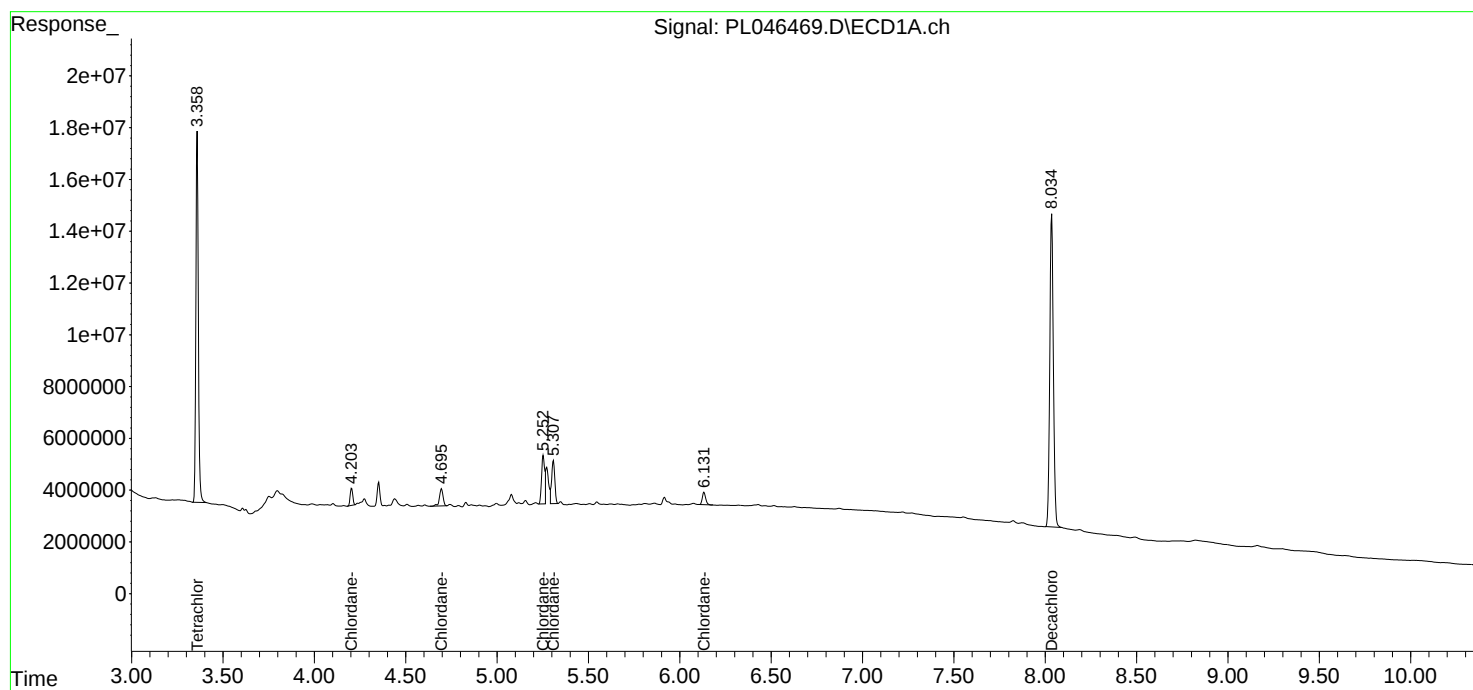


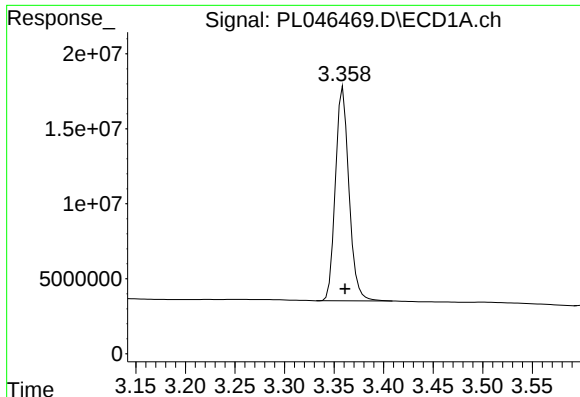

#1 Tetrachloro-m-xylene


R.T.: 3.359 min
Delta R.T.: -0.002 min
Response: 135649755
Conc: 18.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-S-03

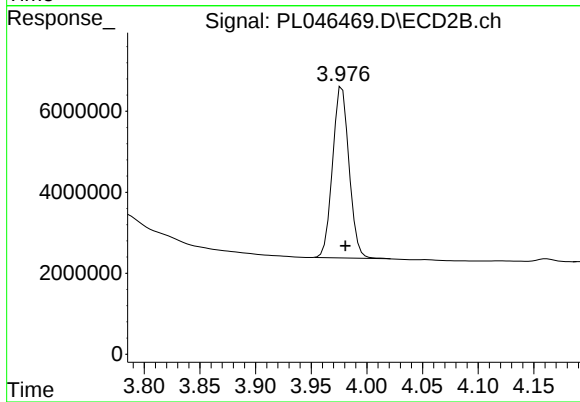


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.003 min
Response: 43559198
Conc: 19.02 ng/ml

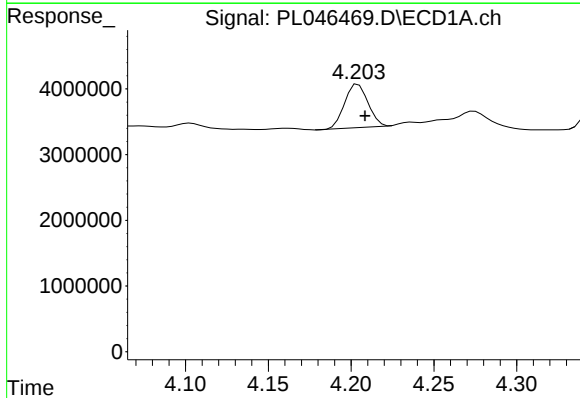


#23 Chlordane-1

R.T.: 4.204 min
Delta R.T.: -0.004 min
Response: 6464956
Conc: 19.22 ng/ml

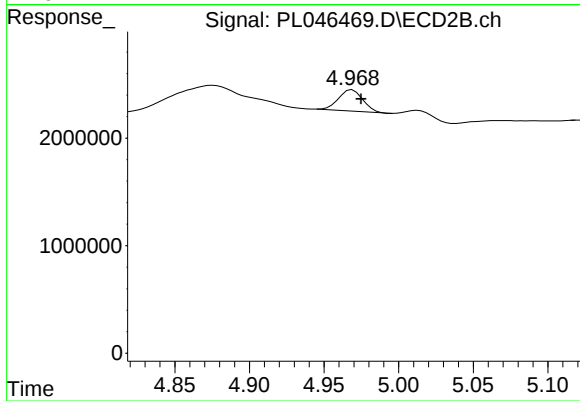

#23 Chlordane-1


R.T.: 4.969 min
Delta R.T.: -0.006 min
Response: 2269805
Conc: 20.97 ng/ml

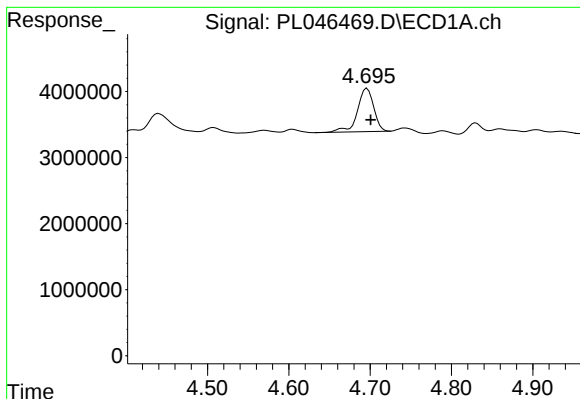

#24 Chlordane-2


R.T.: 4.696 min
Delta R.T.: -0.004 min
Response: 9097627
Conc: 23.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-S-03

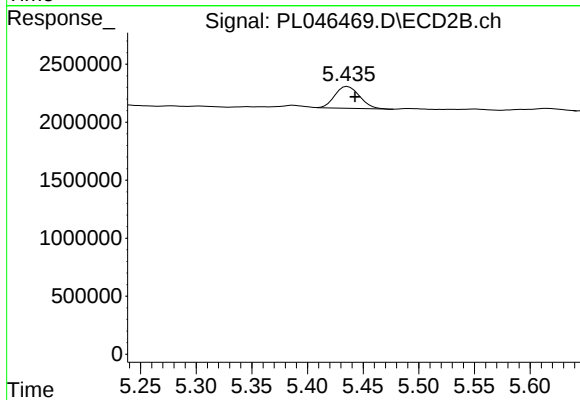


#24 Chlordane-2

R.T.: 5.436 min
Delta R.T.: -0.007 min
Response: 2937909
Conc: 25.15 ng/ml

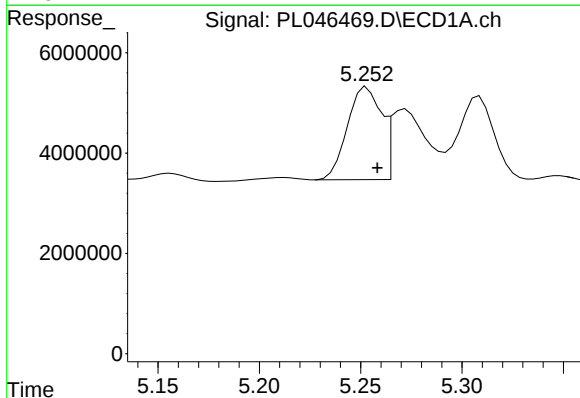


#25 Chlordane-3

R.T.: 5.253 min
Delta R.T.: -0.005 min
Response: 21513354
Conc: 19.32 ng/ml

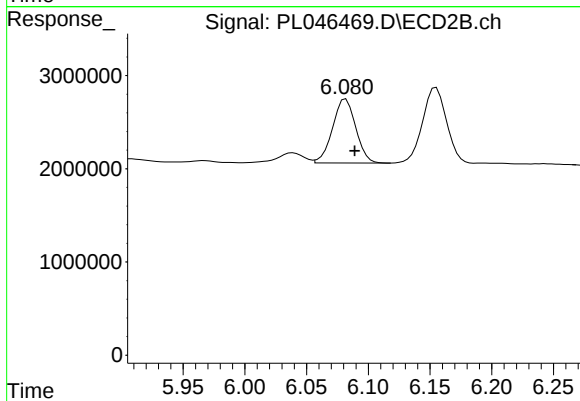

#25 Chlordane-3


R.T.: 6.082 min
Delta R.T.: -0.007 min
Response: 8982579
Conc: 23.56 ng/ml

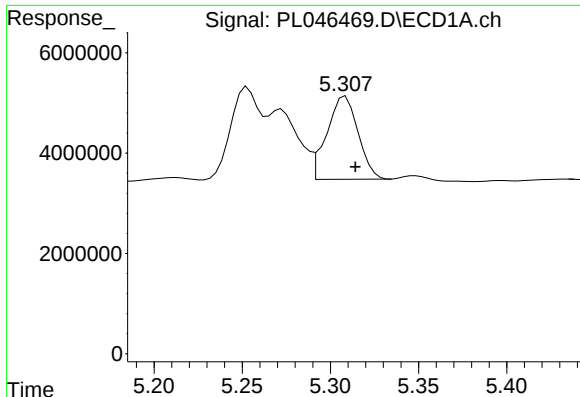

#26 Chlordane-4


R.T.: 5.309 min
Delta R.T.: -0.006 min
Response: 20370276
Conc: 19.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-S-03

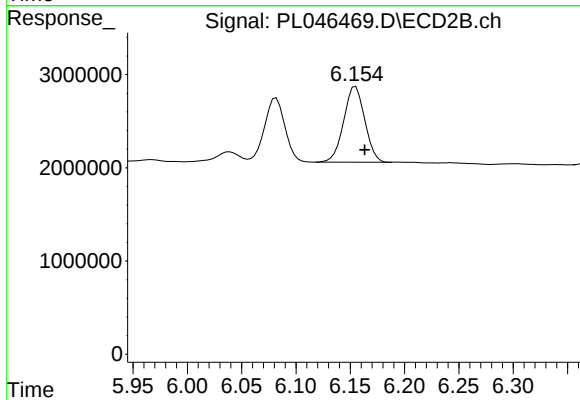


#26 Chlordane-4

R.T.: 6.155 min
Delta R.T.: -0.008 min
Response: 10959893
Conc: 23.75 ng/ml

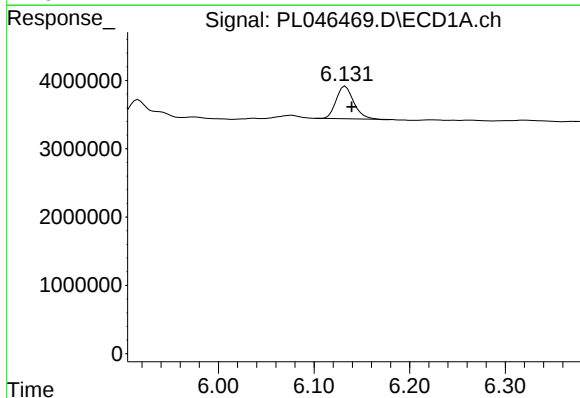


#27 Chlordane-5

R.T.: 6.133 min
Delta R.T.: -0.007 min
Response: 6078730
Conc: 17.81 ng/ml

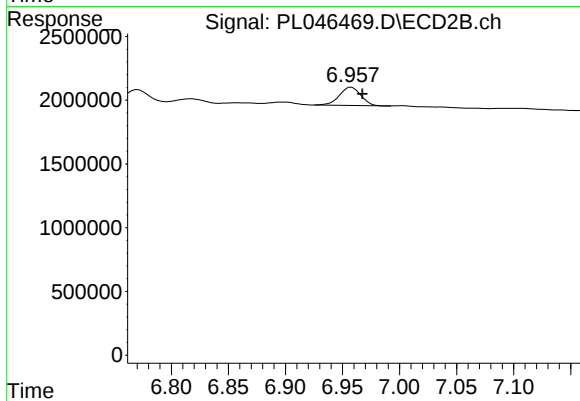

#27 Chlordane-5

R.T.: 6.958 min
Delta R.T.: -0.009 min
Response: 1867656
Conc: 20.79 ng/ml

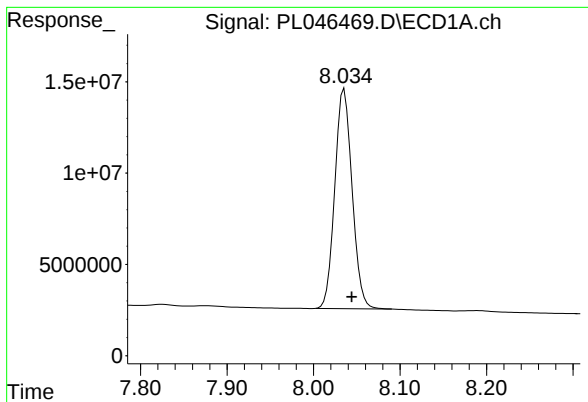

#28 Decachlorobiphenyl


R.T.: 8.036 min

Delta R.T.: -0.009 min

Response: 166605897

Conc: 19.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-S-03

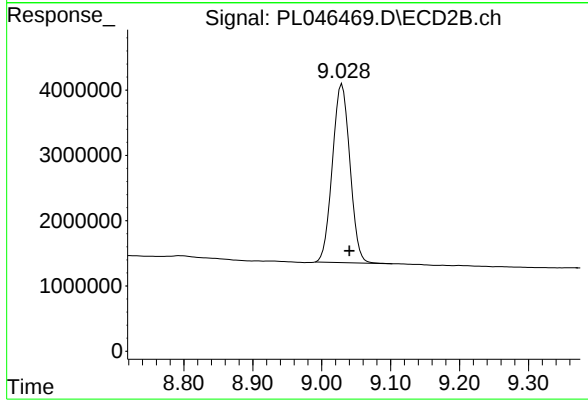

#28 Decachlorobiphenyl

R.T.: 9.029 min

Delta R.T.: -0.010 min

Response: 48300455

Conc: 20.83 ng/ml