

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032619\
 Data File : PL046470.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2019 12:55
 Operator : AJ\SJ
 Sample : MDL-BL-CHL-S-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-BL-CHL-S-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:05:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.359	3.978	127.6E6	41672943	17.544	18.201
28)	SA Decachlor...	8.036	9.030	158.3E6	45890126	18.815	19.793

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032619\
Data File : PL046470.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2019 12:55
Operator : AJ\SJ
Sample : MDL-BL-CHL-S-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MDL-BL-CHL-S-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:05:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

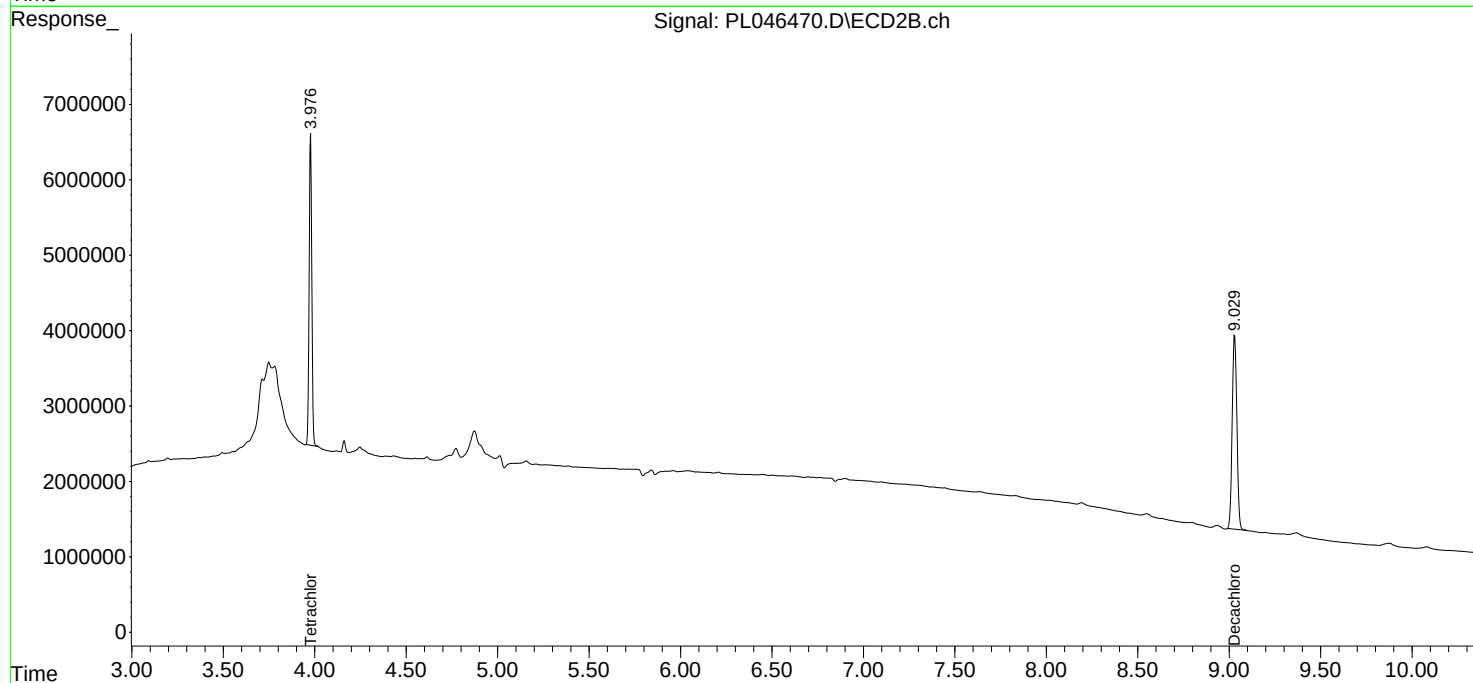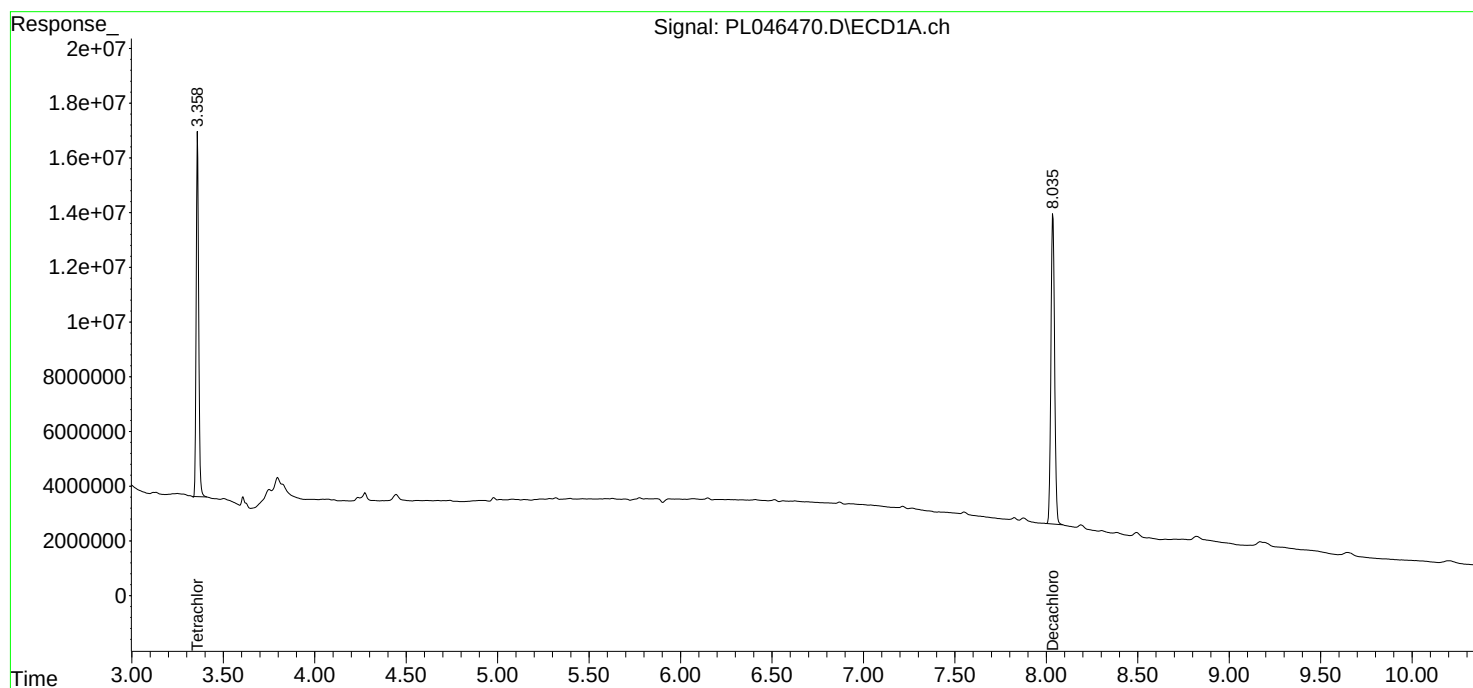


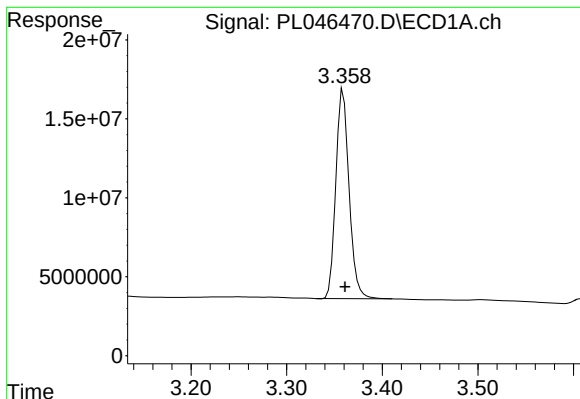

#1 Tetrachloro-m-xylene


R.T.: 3.359 min
Delta R.T.: -0.002 min
Response: 127626958
Conc: 17.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-BL-CHL-S-01

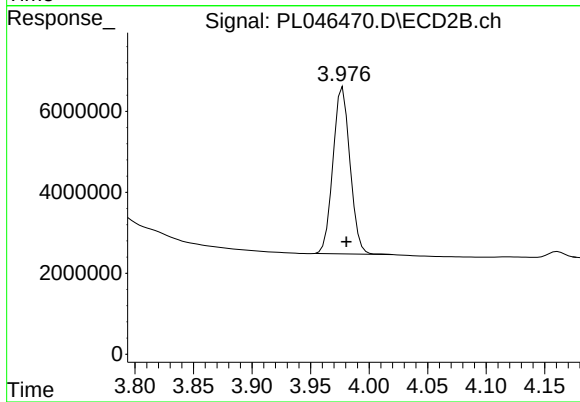


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.003 min
Response: 41672943
Conc: 18.20 ng/ml

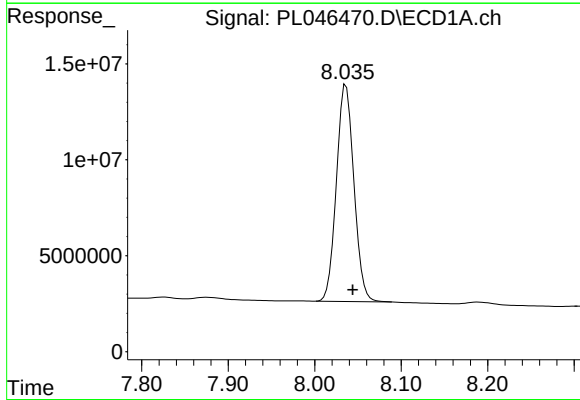

#28 Decachlorobiphenyl

R.T.: 8.036 min
Delta R.T.: -0.008 min
Response: 158251986
Conc: 18.81 ng/ml

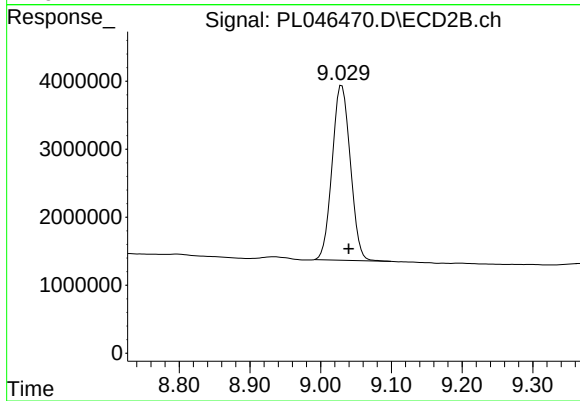

#28 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: -0.010 min
Response: 45890126
Conc: 19.79 ng/ml