

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032619\
 Data File : PL046474.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2019 13:53
 Operator : AJ\SJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:06:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.359	3.978	369.3E6	116.0E6	50.769	50.648
28)	SA Decachlor...	8.036	9.030	399.2E6	112.1E6	47.460	48.337
Target Compounds							
23)	Chlordane-1	4.205	4.970	159.9E6	53589823	475.404	495.207
24)	Chlordane-2	4.696	5.437	175.4E6	57944292	462.252	496.059
25)	Chlordane-3	5.253	6.082	524.8E6	195.0E6	471.224	511.413
26)	Chlordane-4	5.309	6.155	488.5E6	234.5E6	472.420	508.261
27)	Chlordane-5	6.133	6.959	154.0E6	42455942	451.362	472.585



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032619\
Data File : PL046474.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2019 13:53
Operator : AJ\SJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:06:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

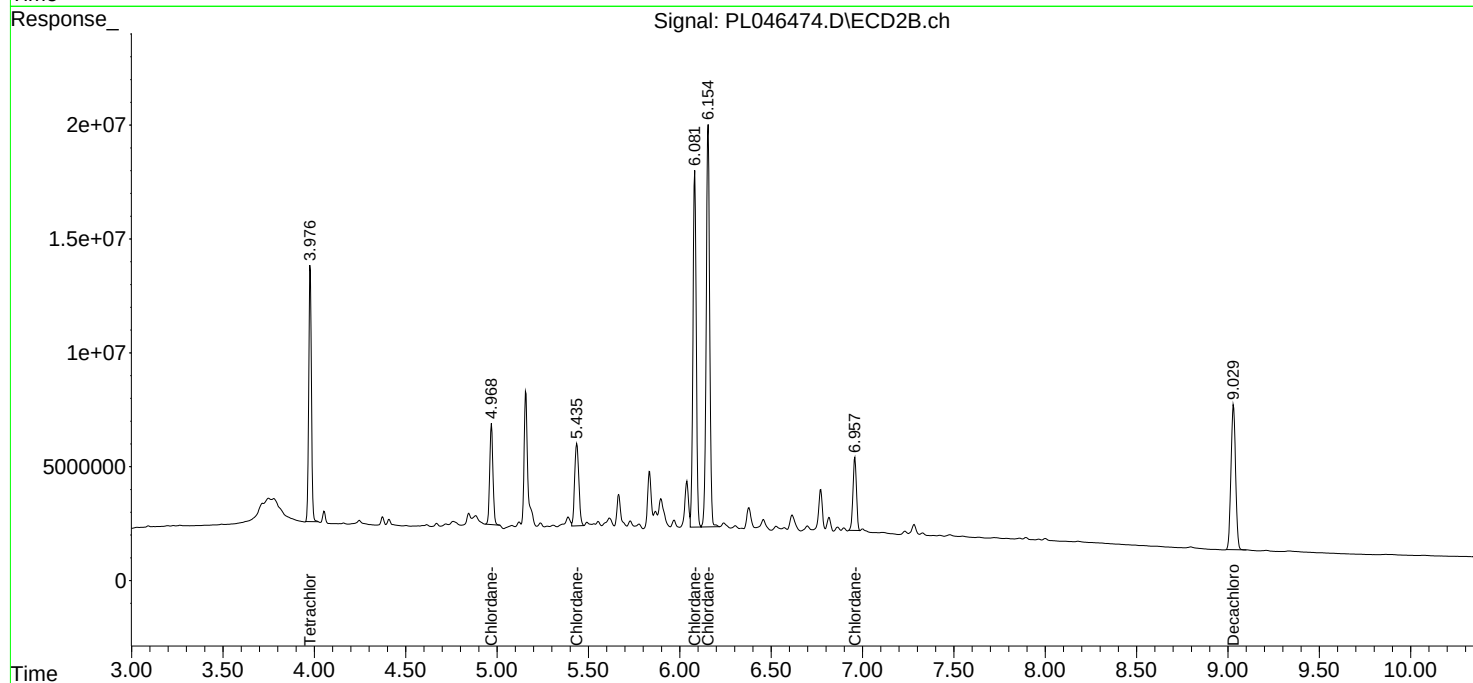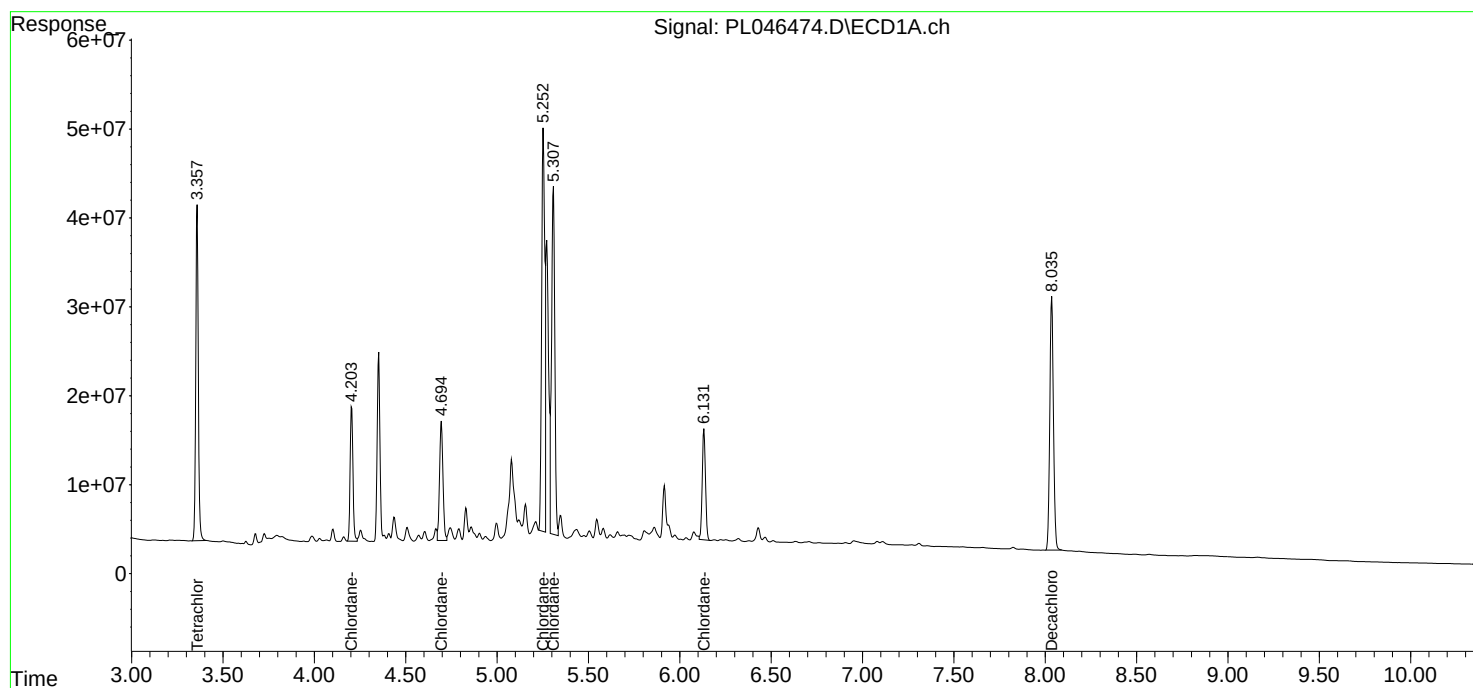


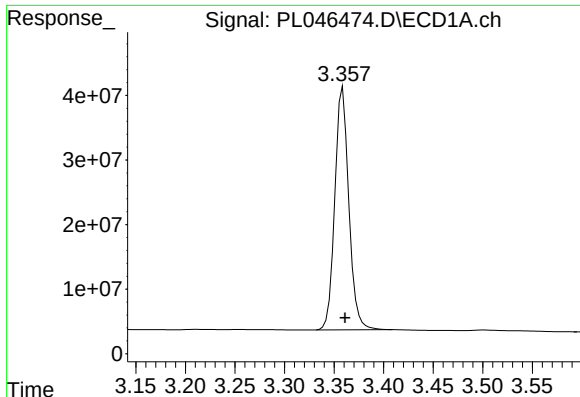

#1 Tetrachloro-m-xylene


R.T.: 3.359 min
Delta R.T.: -0.002 min
Response: 369328643
Conc: 50.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

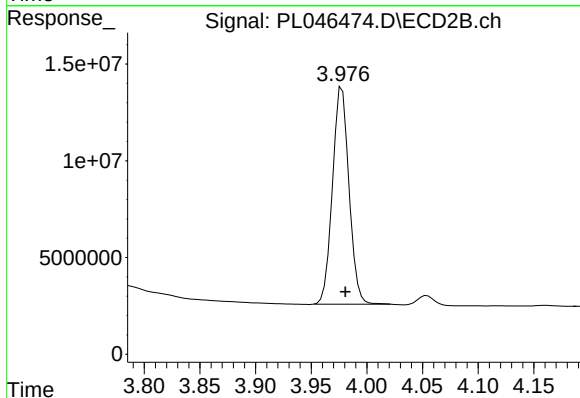


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.003 min
Response: 115963413
Conc: 50.65 ng/ml

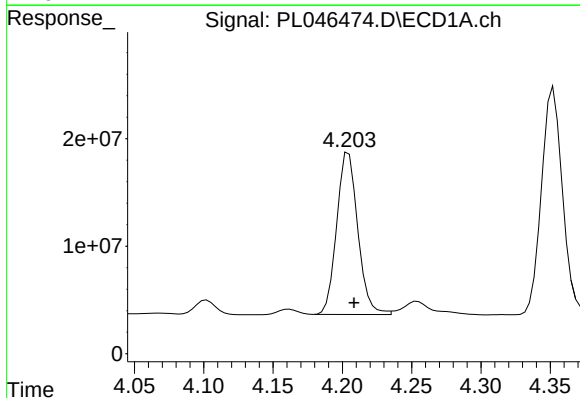


#23 Chlordane-1

R.T.: 4.205 min
Delta R.T.: -0.004 min
Response: 159875978
Conc: 475.40 ng/ml

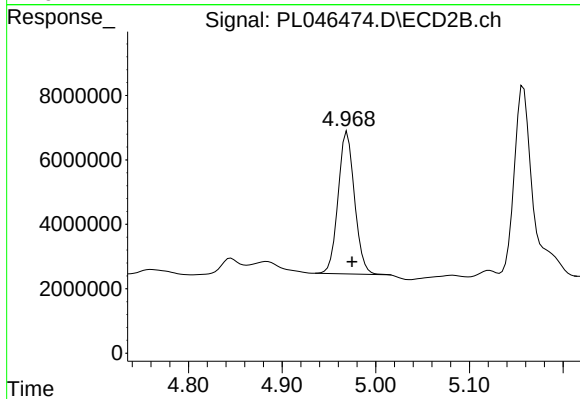

#23 Chlordane-1


R.T.: 4.970 min
Delta R.T.: -0.005 min
Response: 53589823
Conc: 495.21 ng/ml

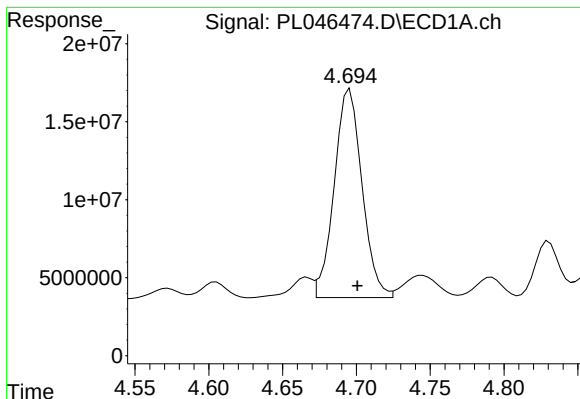

#24 Chlordane-2


R.T.: 4.696 min
Delta R.T.: -0.005 min
Response: 175387178
Conc: 462.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

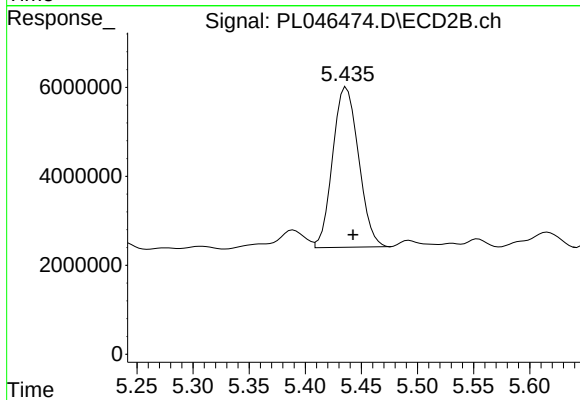


#24 Chlordane-2

R.T.: 5.437 min
Delta R.T.: -0.006 min
Response: 57944292
Conc: 496.06 ng/ml

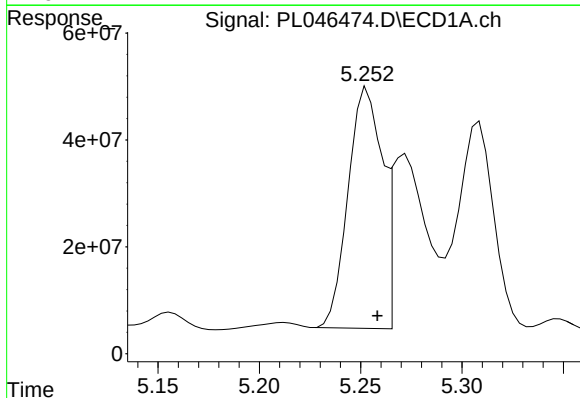


#25 Chlordane-3

R.T.: 5.253 min
Delta R.T.: -0.005 min
Response: 524789494
Conc: 471.22 ng/ml

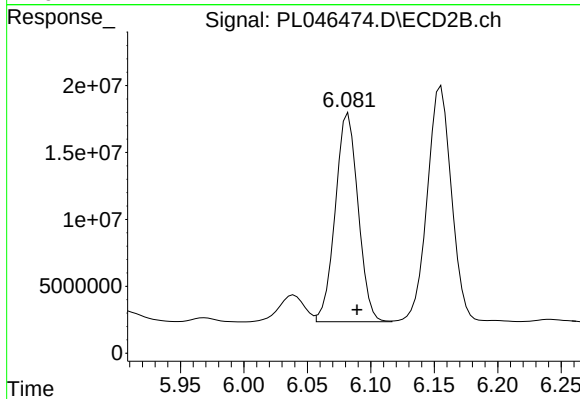

#25 Chlordane-3


R.T.: 6.082 min
Delta R.T.: -0.007 min
Response: 194985184
Conc: 511.41 ng/ml

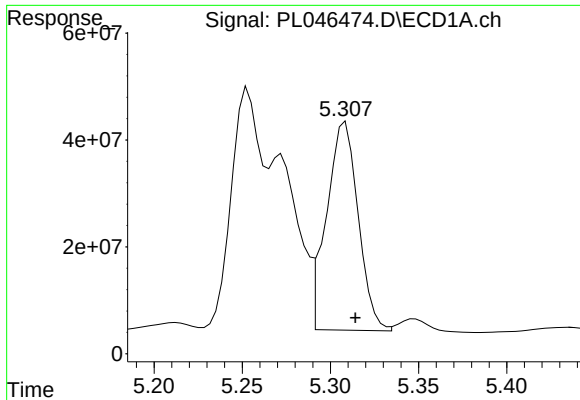

#26 Chlordane-4


R.T.: 5.309 min
Delta R.T.: -0.006 min
Response: 488510825
Conc: 472.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

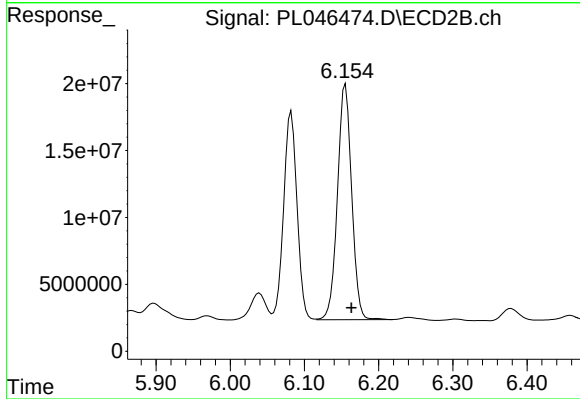


#26 Chlordane-4

R.T.: 6.155 min
Delta R.T.: -0.008 min
Response: 234524271
Conc: 508.26 ng/ml

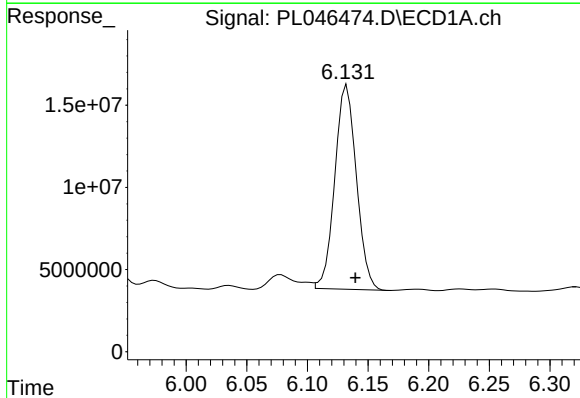


#27 Chlordane-5

R.T.: 6.133 min
Delta R.T.: -0.007 min
Response: 154034941
Conc: 451.36 ng/ml

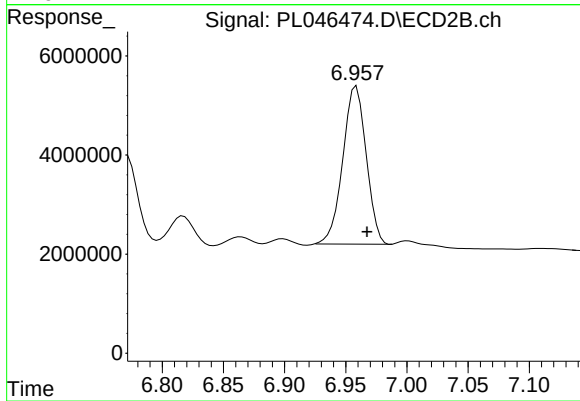

#27 Chlordane-5


R.T.: 6.959 min
Delta R.T.: -0.009 min
Response: 42455942
Conc: 472.58 ng/ml

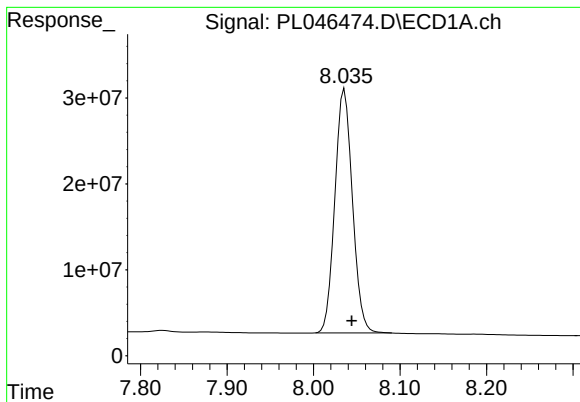

#28 Decachlorobiphenyl

R.T.: 8.036 min
Delta R.T.: -0.008 min
Response: 399188117
Conc: 47.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

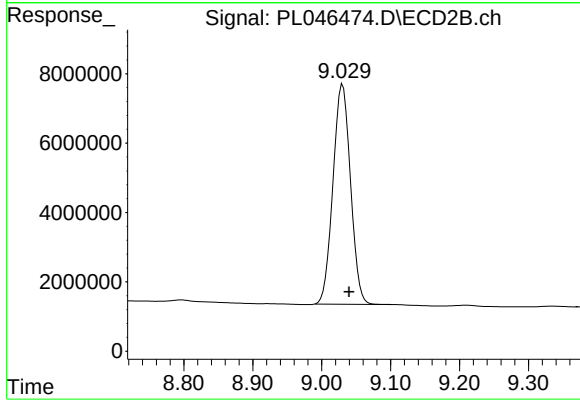

#28 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: -0.009 min
Response: 112068474
Conc: 48.34 ng/ml