

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032619\
 Data File : PL046475.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2019 14:38
 Operator : AJ\SJ
 Sample : MDL-CHL-W-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-CHL-W-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:06:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.361	3.977	134.8E6	44594560	18.534	19.477
28)	SA Decachlor...	8.039	9.031	170.1E6	48989894	20.220	21.130
Target Compounds							
23)	Chlordane-1	4.206	4.969	4986976	2505285	14.829	23.151 #
24)	Chlordane-2	4.698	5.436	9590948	3040385	25.278	26.029
25)	Chlordane-3	5.255	6.082	21819753	9375165	19.593	24.589 #
26)	Chlordane-4	5.310	6.156	20545435	11703769	19.869	25.364 #
27)	Chlordane-5	6.135	6.959	6478428	2045232	18.983	22.766



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032619\
Data File : PL046475.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2019 14:38
Operator : AJ\SJ
Sample : MDL-CHL-W-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-W-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:06:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

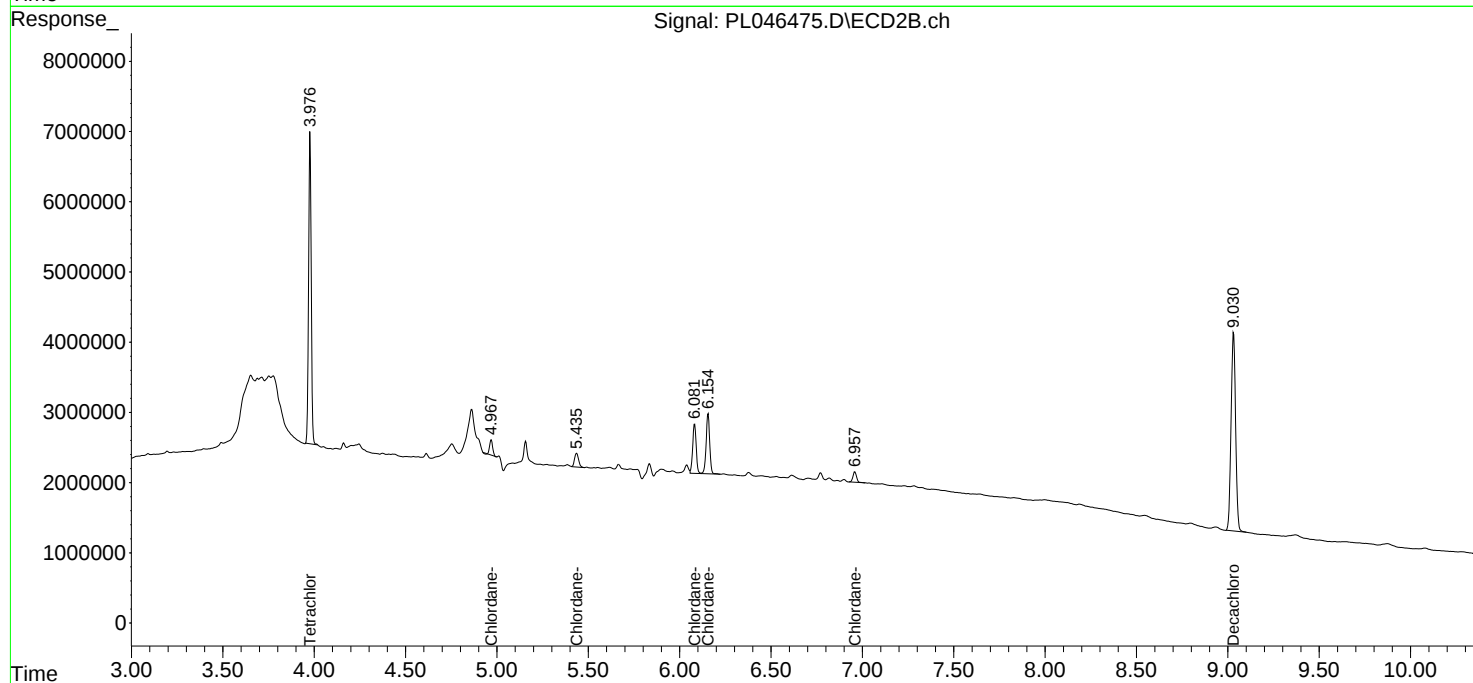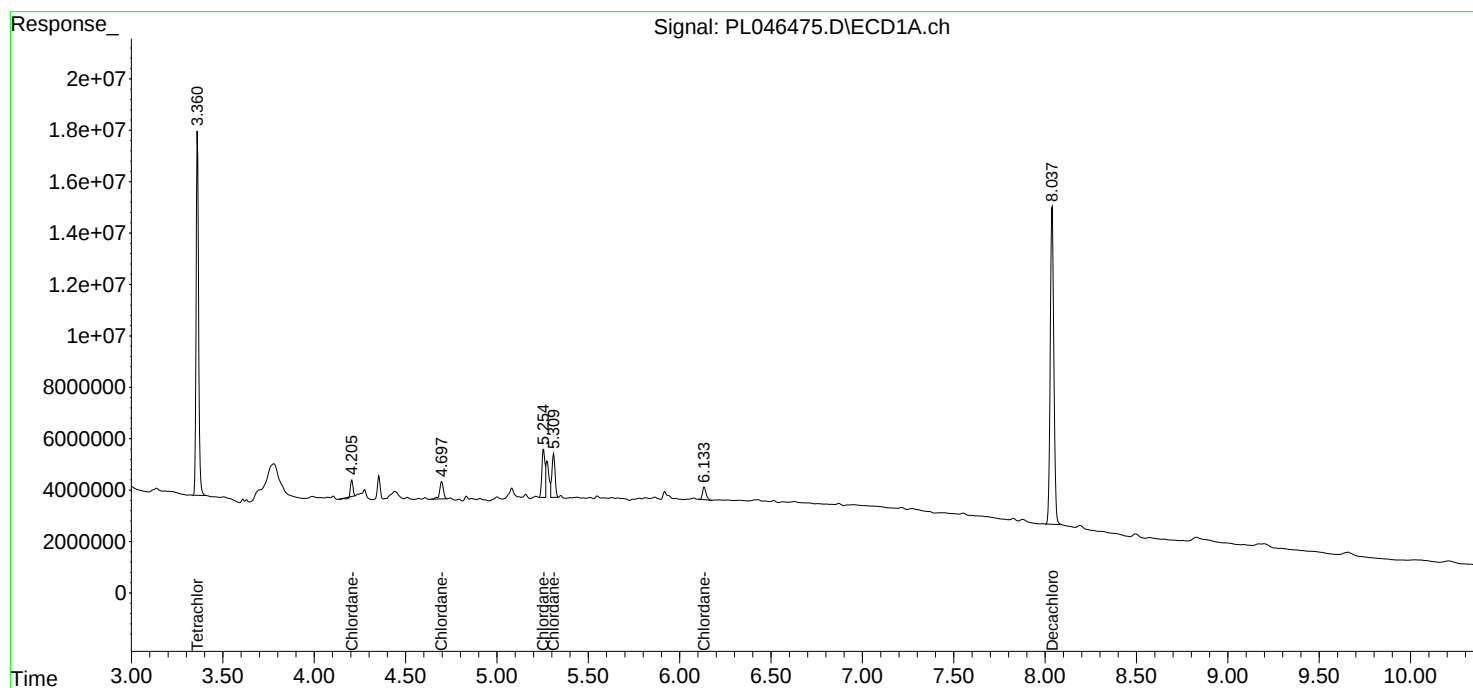


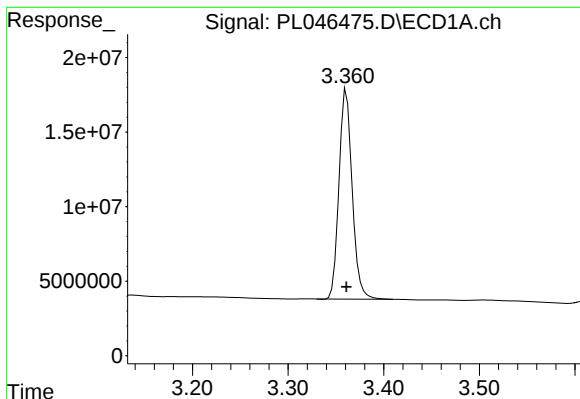

#1 Tetrachloro-m-xylene


R.T.: 3.361 min
Delta R.T.: 0.000 min
Response: 134825475
Conc: 18.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-W-01

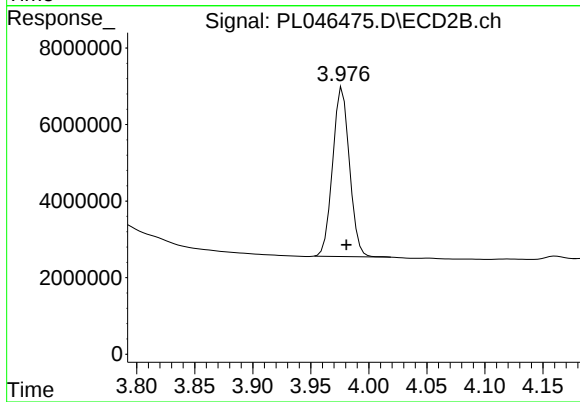


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.003 min
Response: 44594560
Conc: 19.48 ng/ml

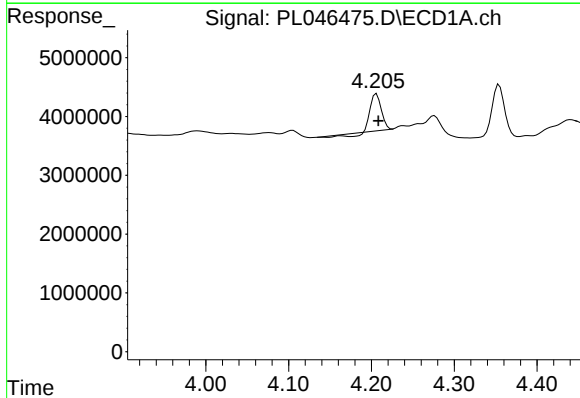


#23 Chlordane-1

R.T.: 4.206 min
Delta R.T.: -0.002 min
Response: 4986976
Conc: 14.83 ng/ml

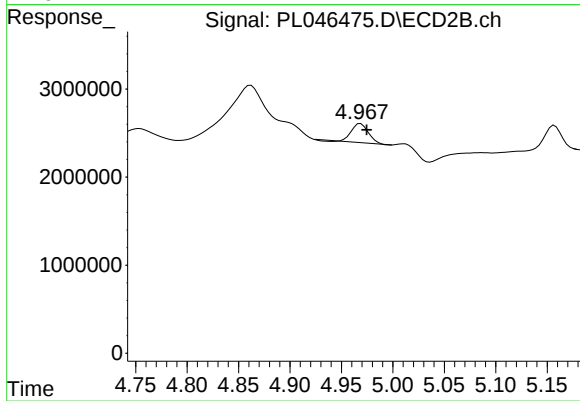

#23 Chlordane-1


R.T.: 4.969 min
Delta R.T.: -0.006 min
Response: 2505285
Conc: 23.15 ng/ml

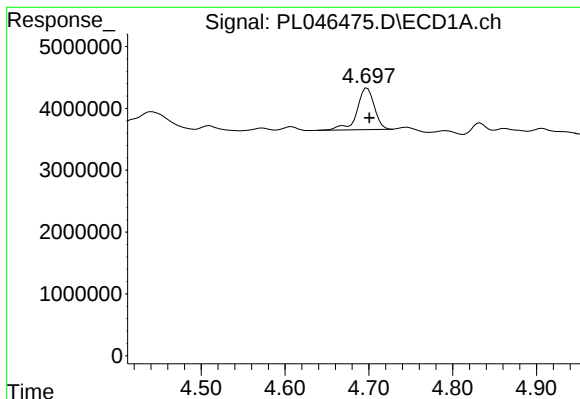

#24 Chlordane-2


R.T.: 4.698 min
Delta R.T.: -0.003 min
Response: 9590948
Conc: 25.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-W-01

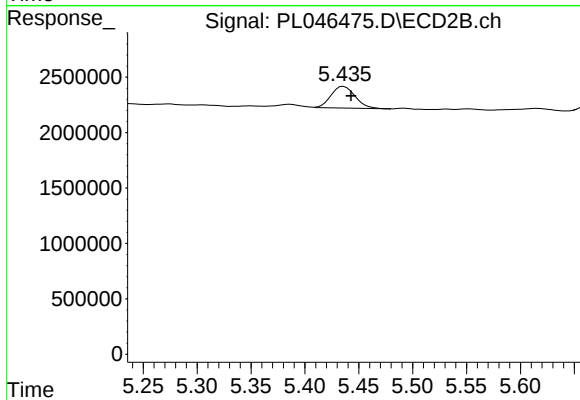


#24 Chlordane-2

R.T.: 5.436 min
Delta R.T.: -0.007 min
Response: 3040385
Conc: 26.03 ng/ml

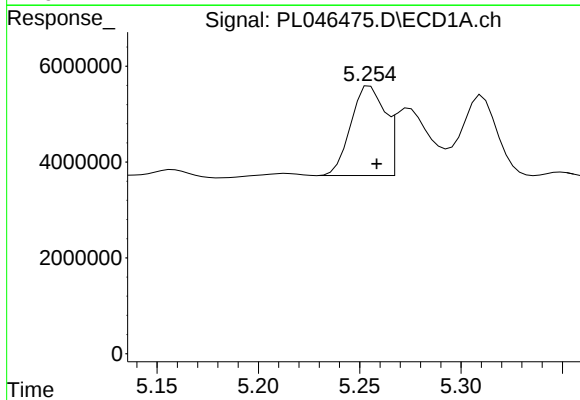


#25 Chlordane-3

R.T.: 5.255 min
Delta R.T.: -0.003 min
Response: 21819753
Conc: 19.59 ng/ml

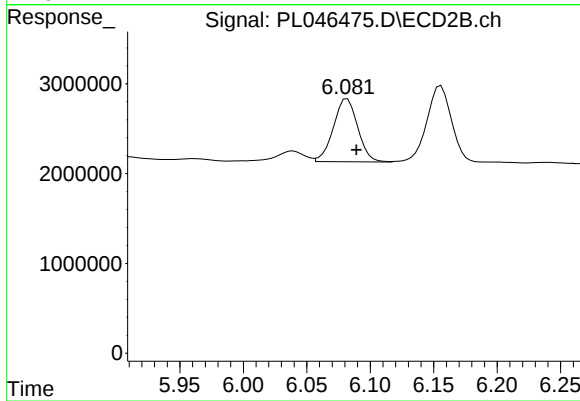

#25 Chlordane-3


R.T.: 6.082 min
Delta R.T.: -0.007 min
Response: 9375165
Conc: 24.59 ng/ml

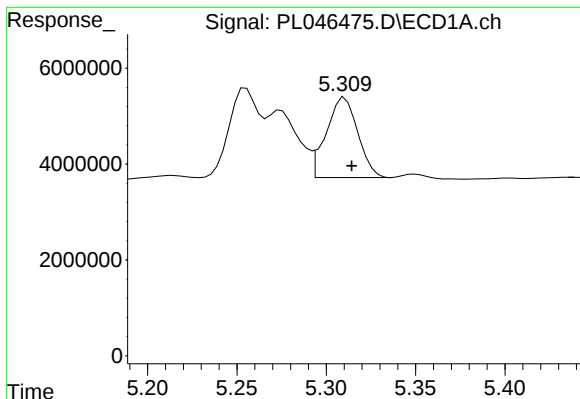

#26 Chlordane-4


R.T.: 5.310 min
Delta R.T.: -0.004 min
Response: 20545435
Conc: 19.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-W-01

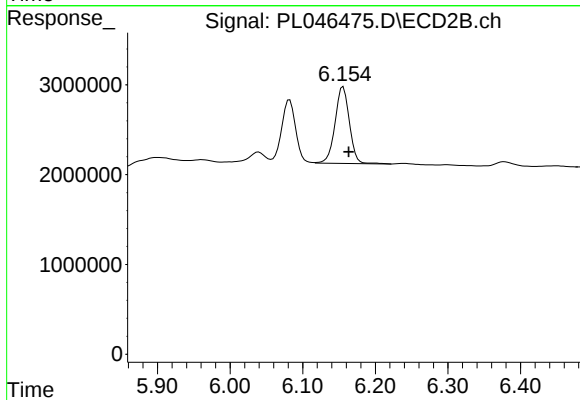


#26 Chlordane-4

R.T.: 6.156 min
Delta R.T.: -0.007 min
Response: 11703769
Conc: 25.36 ng/ml

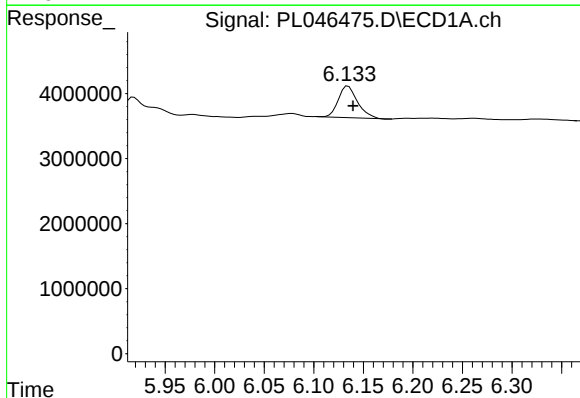


#27 Chlordane-5

R.T.: 6.135 min
Delta R.T.: -0.005 min
Response: 6478428
Conc: 18.98 ng/ml

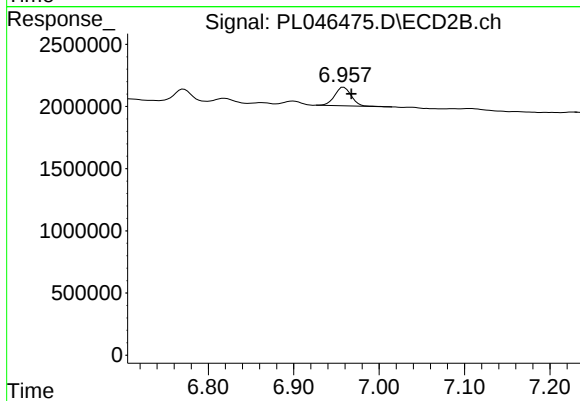

#27 Chlordane-5

R.T.: 6.959 min
Delta R.T.: -0.009 min
Response: 2045232
Conc: 22.77 ng/ml

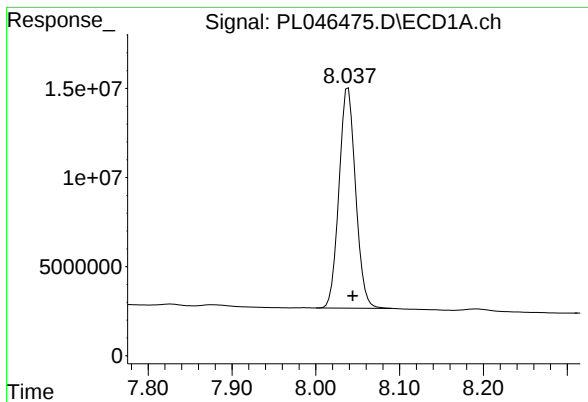

#28 Decachlorobiphenyl


R.T.: 8.039 min

Delta R.T.: -0.005 min

Response: 170073282

Conc: 20.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-W-01

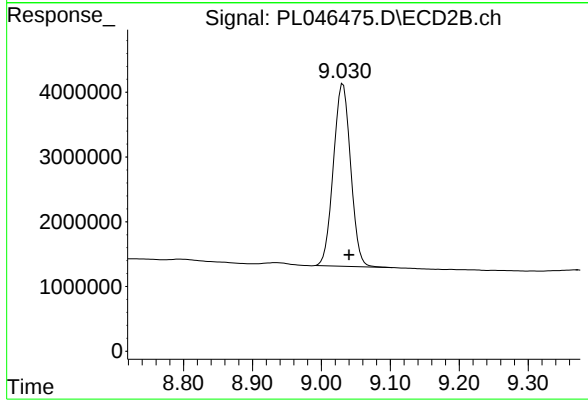

#28 Decachlorobiphenyl

R.T.: 9.031 min

Delta R.T.: -0.008 min

Response: 48989894

Conc: 21.13 ng/ml