

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032619\
 Data File : PL046477.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2019 15:07
 Operator : AJ\SJ
 Sample : MDL-CHL-W-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-CHL-W-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:07:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.359	3.977	133.3E6	43332533	18.330	18.926
28)	SA Decachlor...	8.036	9.030	167.1E6	48338768	19.868	20.849
Target Compounds							
23)	Chlordane-1	4.204	4.968	6218536	2294443	18.491	21.202
24)	Chlordane-2	4.696	5.437	9446691	3020706	24.898	25.860
25)	Chlordane-3	5.253	6.082	22004170	9139340	19.758	23.971
26)	Chlordane-4	5.308	6.155	20567531	11439829	19.890	24.792
27)	Chlordane-5	6.132	6.959	6243786	1962477	18.296	21.845



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032619\
Data File : PL046477.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2019 15:07
Operator : AJ\SJ
Sample : MDL-CHL-W-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-W-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:07:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

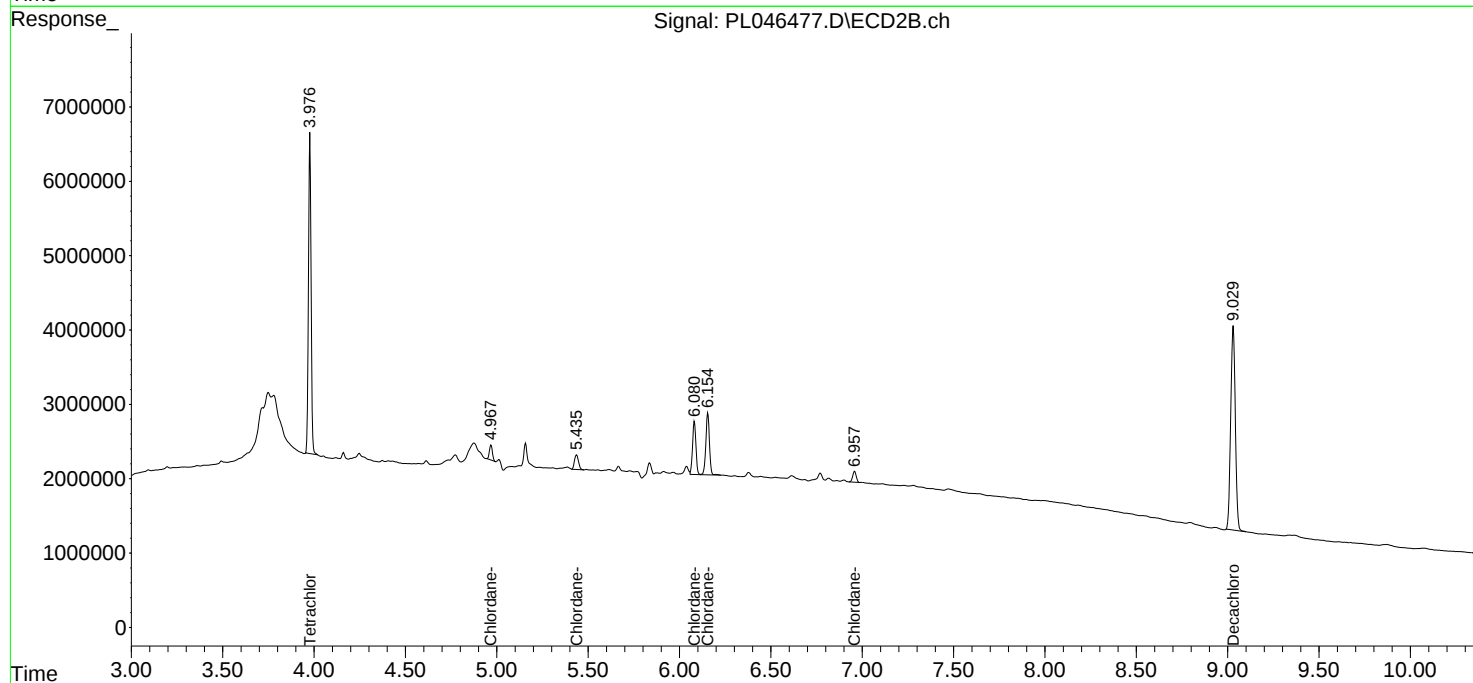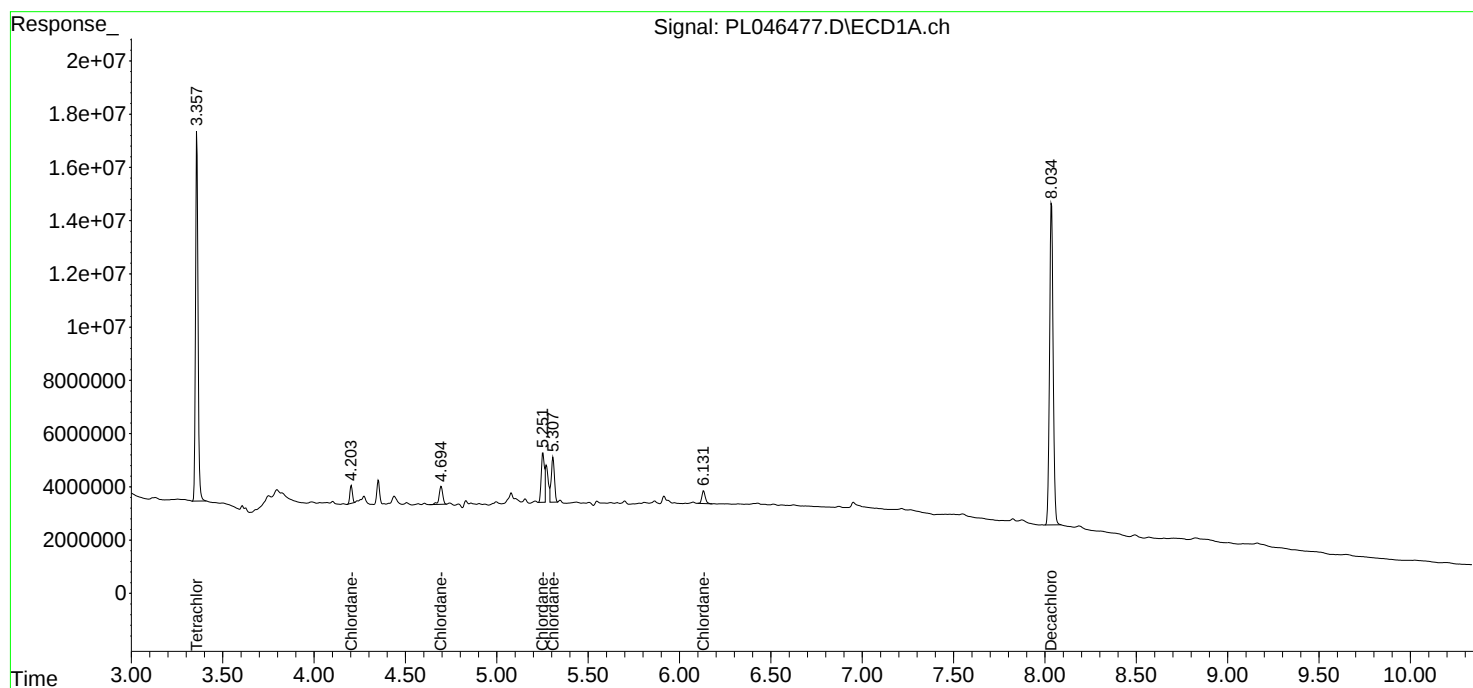


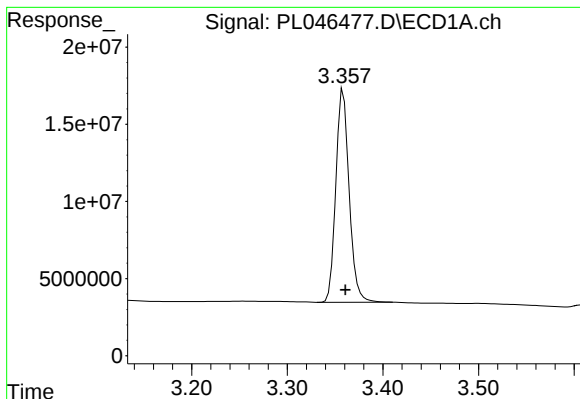

#1 Tetrachloro-m-xylene


R.T.: 3.359 min
Delta R.T.: -0.002 min
Response: 133346925
Conc: 18.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-W-03

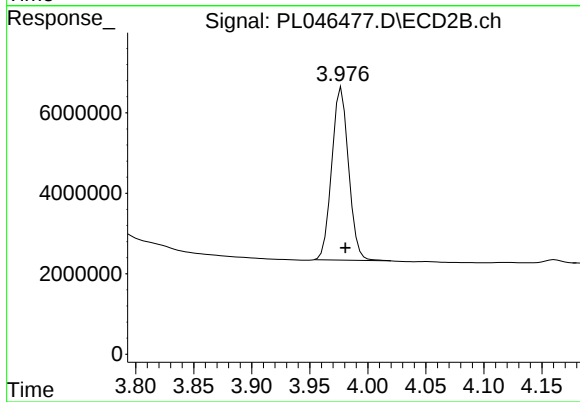


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.003 min
Response: 43332533
Conc: 18.93 ng/ml

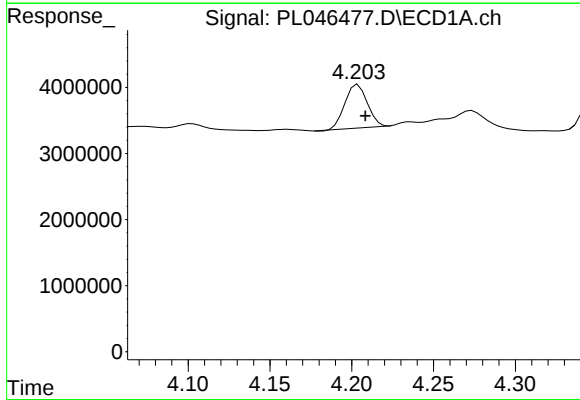


#23 Chlordane-1

R.T.: 4.204 min
Delta R.T.: -0.004 min
Response: 6218536
Conc: 18.49 ng/ml

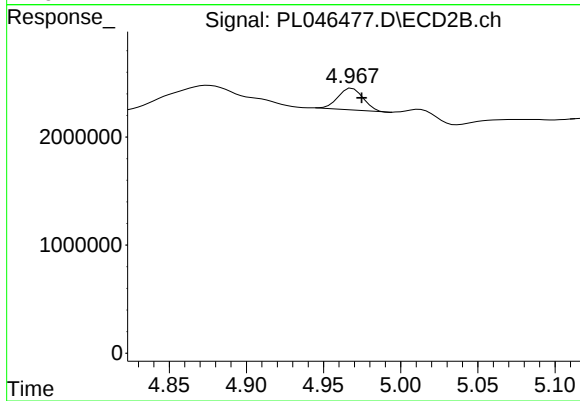

#23 Chlordane-1


R.T.: 4.968 min
Delta R.T.: -0.006 min
Response: 2294443
Conc: 21.20 ng/ml

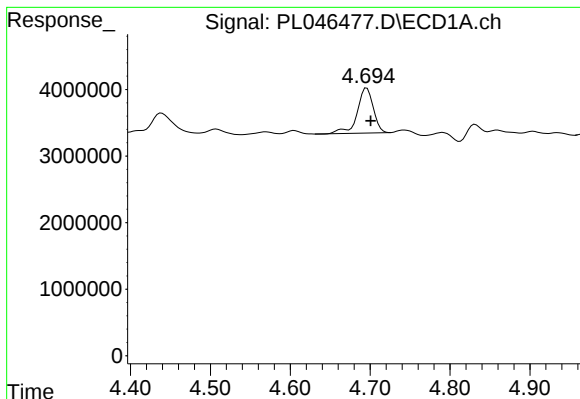

#24 Chlordane-2


R.T.: 4.696 min
Delta R.T.: -0.005 min
Response: 9446691
Conc: 24.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-W-03

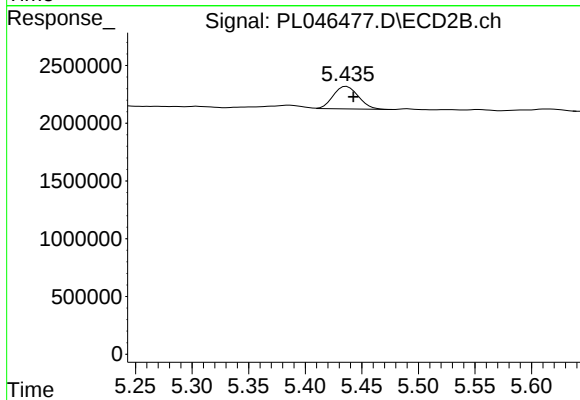


#24 Chlordane-2

R.T.: 5.437 min
Delta R.T.: -0.006 min
Response: 3020706
Conc: 25.86 ng/ml

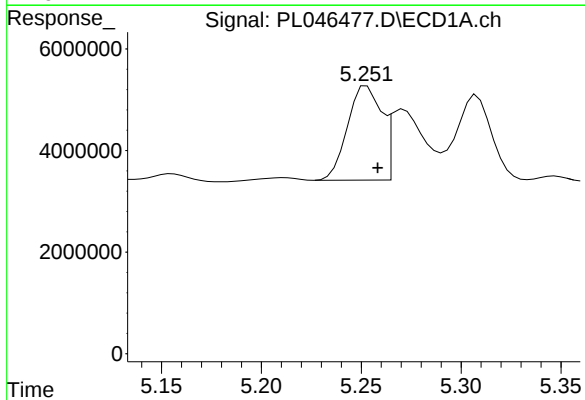


#25 Chlordane-3

R.T.: 5.253 min
Delta R.T.: -0.006 min
Response: 22004170
Conc: 19.76 ng/ml

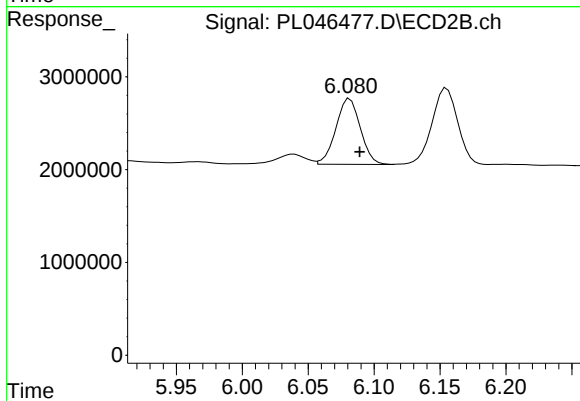

#25 Chlordane-3


R.T.: 6.082 min
Delta R.T.: -0.007 min
Response: 9139340
Conc: 23.97 ng/ml

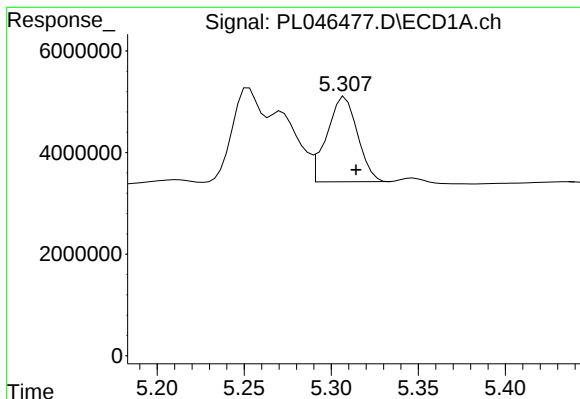

#26 Chlordane-4


R.T.: 5.308 min
Delta R.T.: -0.006 min
Response: 20567531
Conc: 19.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-W-03

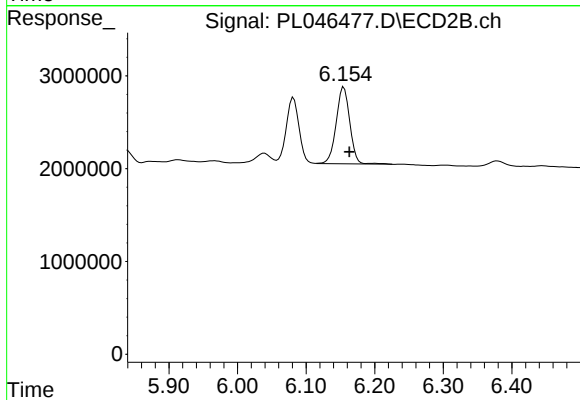


#26 Chlordane-4

R.T.: 6.155 min
Delta R.T.: -0.008 min
Response: 11439829
Conc: 24.79 ng/ml

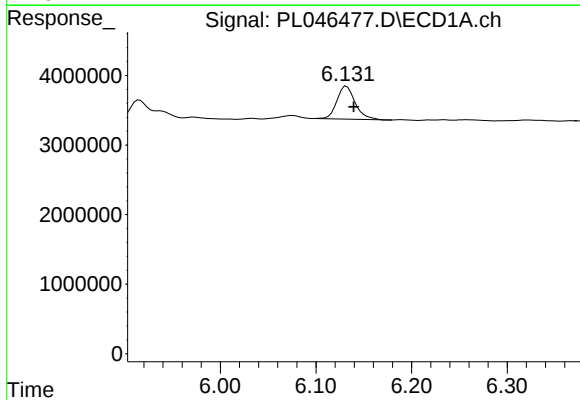


#27 Chlordane-5

R.T.: 6.132 min
Delta R.T.: -0.008 min
Response: 6243786
Conc: 18.30 ng/ml

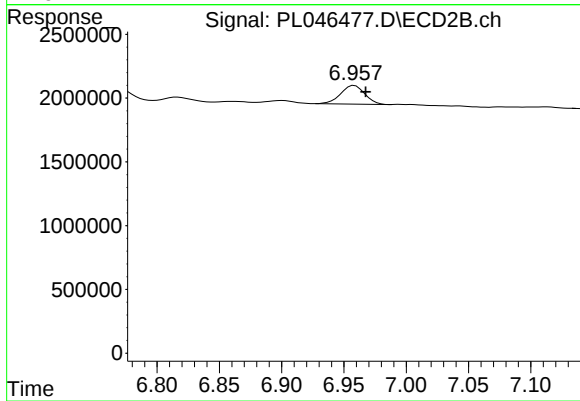

#27 Chlordane-5


R.T.: 6.959 min
Delta R.T.: -0.009 min
Response: 1962477
Conc: 21.84 ng/ml

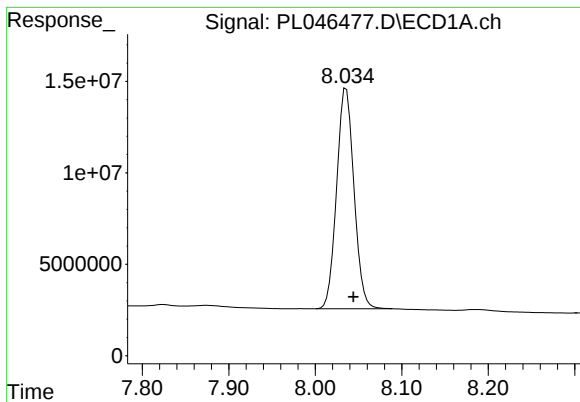

#28 Decachlorobiphenyl

R.T.: 8.036 min
Delta R.T.: -0.008 min
Response: 167110029
Conc: 19.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-W-03

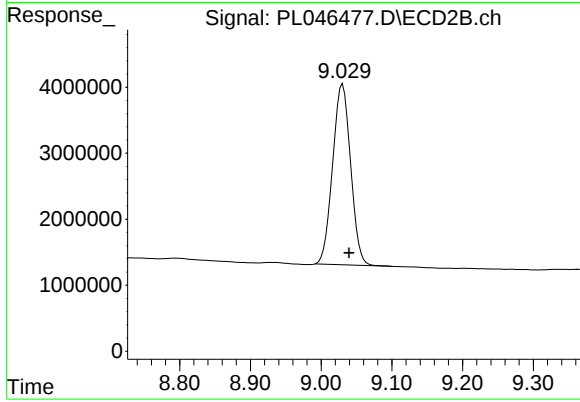

#28 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: -0.009 min
Response: 48338768
Conc: 20.85 ng/ml