

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032620\
 Data File : PL057578.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2020 16:04
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:11:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	3.956	233.7E6	52773442	25.214	24.325
2)	SA Decachlor...	8.206	8.978	229.5E6	50639129	21.689	22.838
Target Compounds							
2)	A alpha-BHC	3.889	0.000	4211677	0	0.264	N.D. #
4)	MA Heptachlor	0.000	5.136	0	4397711	N.D.	1.397 #
8)	B Heptachlo...	5.169	0.000	870865	0	0.068	N.D. #
9)	A Endosulfan I	5.504	0.000	410080	0	0.034	N.D. #
11)	B alpha-Chl...	5.429f	0.000	284862	0	0.022	N.D. #
14)	MA Endrin	6.005	0.000	513577	0	0.045	N.D. #
15)	B Endosulfa...	6.291	0.000	830470	0	0.076	N.D. #
17)	MA 4,4'-DDT	6.361	0.000	48210	0	0.005	N.D. #
20)	A Methoxychlor	6.899f	0.000	1297462	0	0.242	N.D. #
22)	Mirex	7.332	0.000	405821	0	0.050	N.D. #
23)	Chlordane-1	4.356f	0.000	2607808	0	8.035	N.D. #
24)	Chlordane-2	4.851f	0.000	427894	0	1.178	N.D. #
26)	Chlordane-4	5.429f	0.000	284862	0	0.297	N.D. #
27)	Chlordane-5	6.291	0.000	830470	0	2.282	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032620\
Data File : PL057578.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2020 16:04
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:11:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

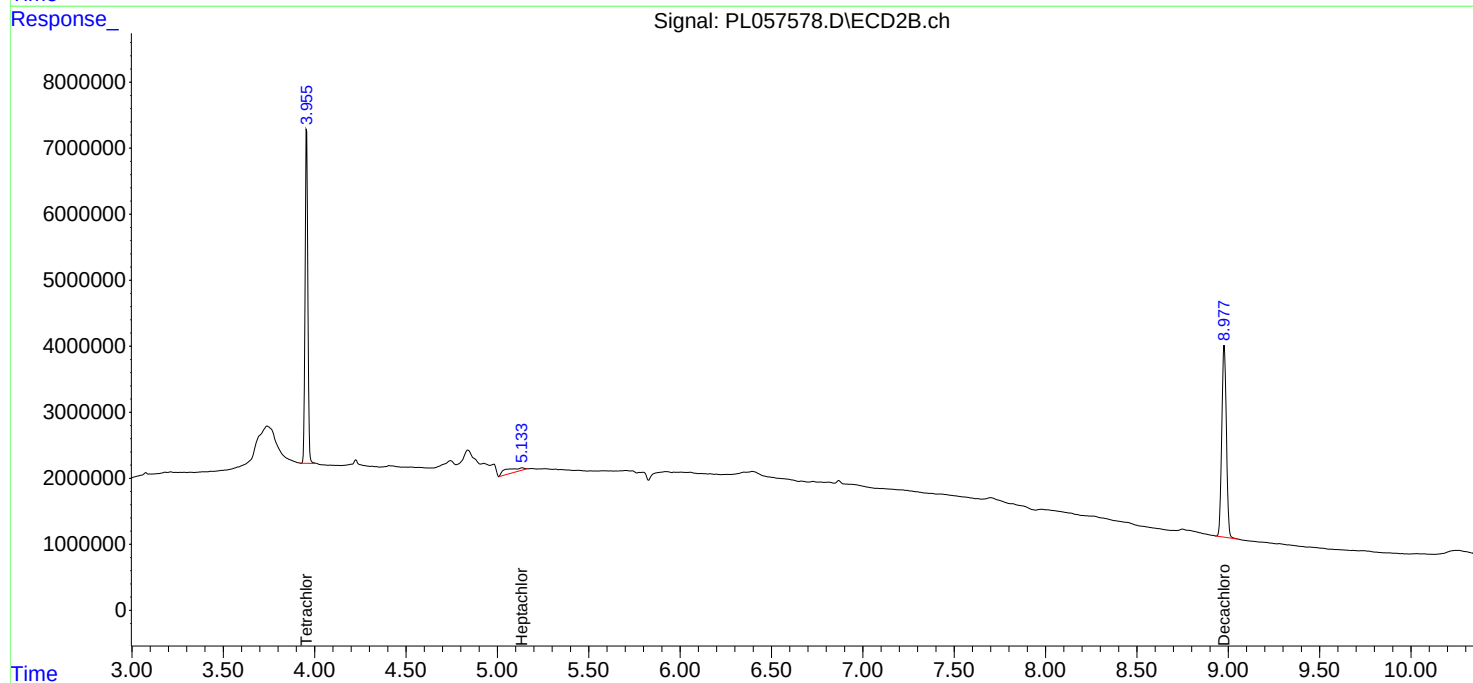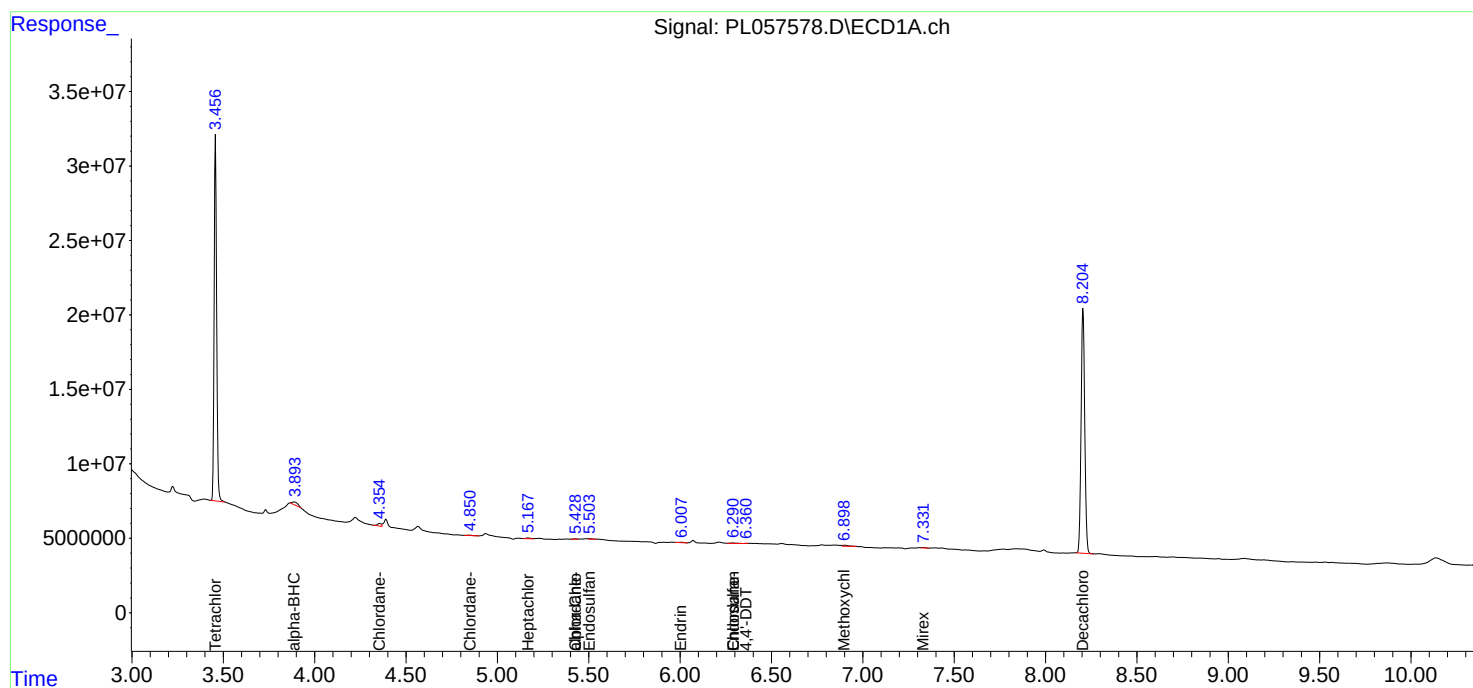


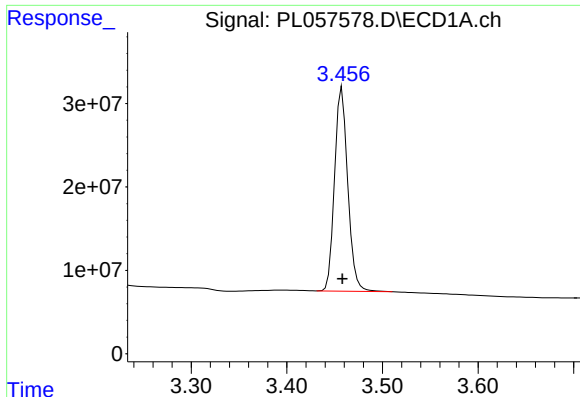

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 233721012
Conc: 25.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

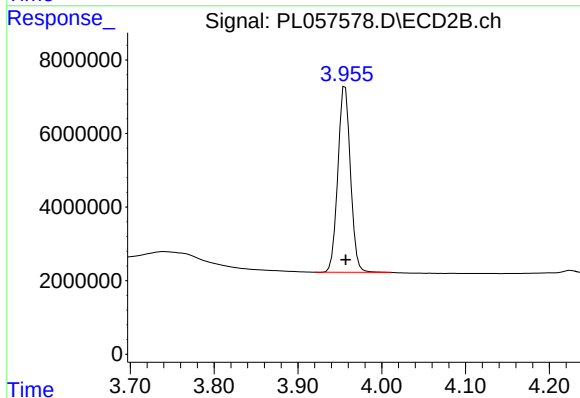


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: 0.000 min
Response: 52773442
Conc: 24.32 ng/ml

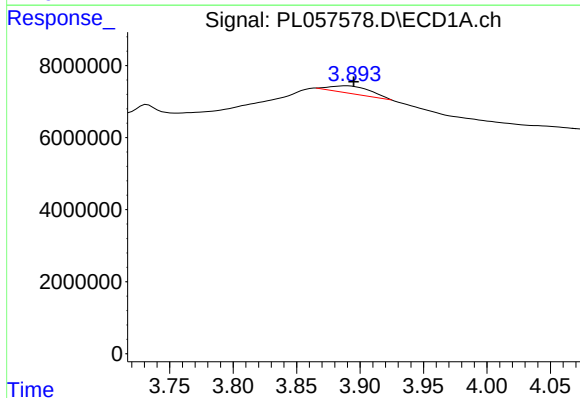


#2 alpha-BHC

R.T.: 3.889 min
Delta R.T.: -0.006 min
Response: 4211677
Conc: 0.26 ng/ml

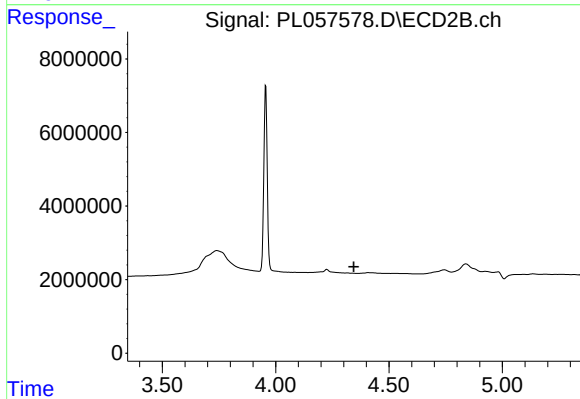

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.345 min
Response: 0
Conc: N.D.

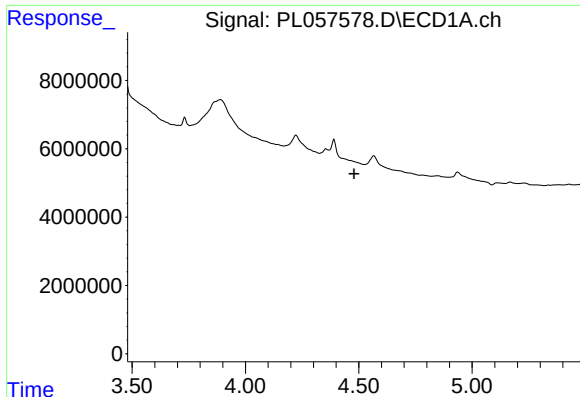

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

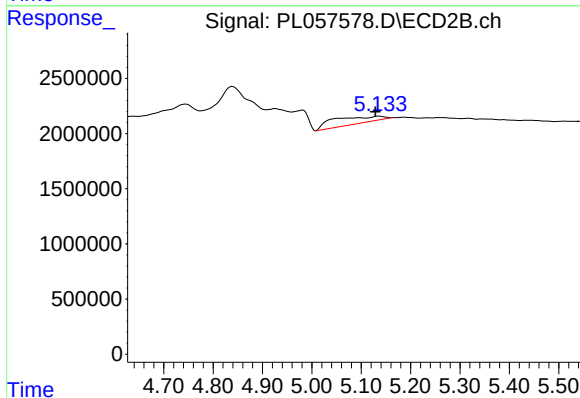


#4 Heptachlor

R.T.: 5.136 min
Delta R.T.: 0.007 min
Response: 4397711
Conc: 1.40 ng/ml

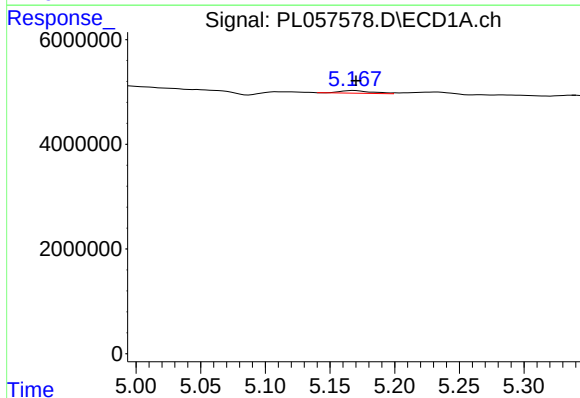


#8 Heptachlor epoxide

R.T.: 5.169 min
Delta R.T.: -0.001 min
Response: 870865
Conc: 0.07 ng/ml

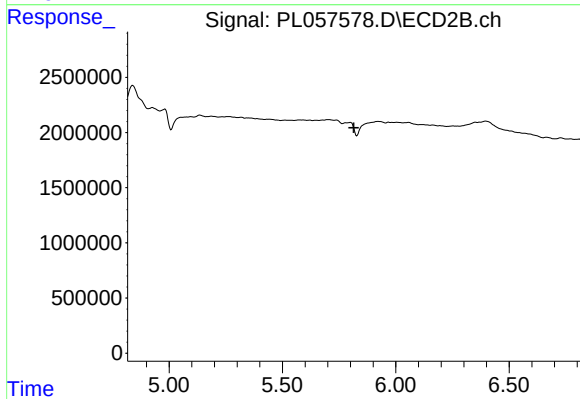

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.815 min
Response: 0
Conc: N.D.

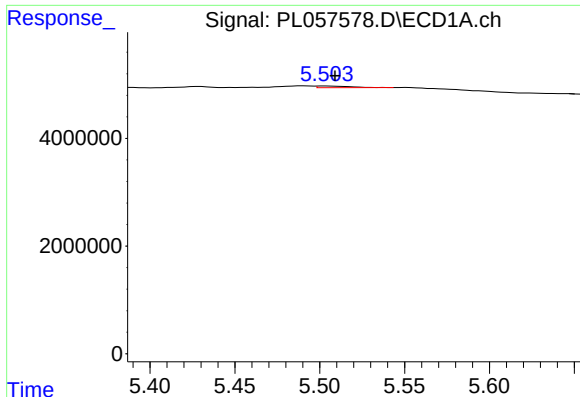

#9 Endosulfan I


R.T.: 5.504 min
Delta R.T.: -0.005 min
Response: 410080
Conc: 0.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

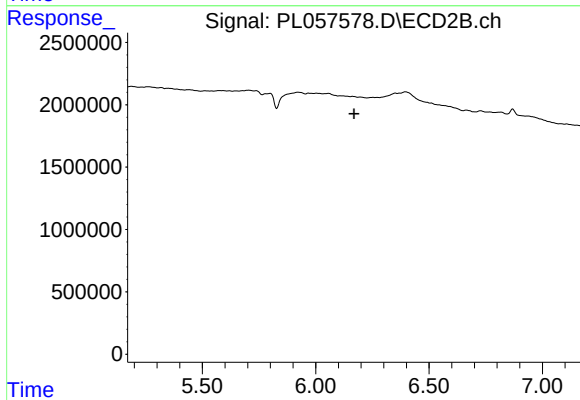


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

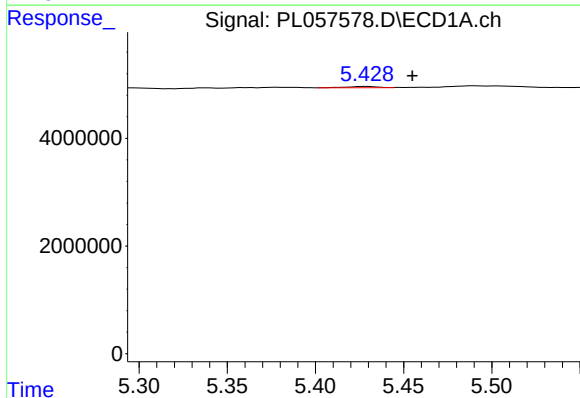


#11 alpha-Chlordane

R.T.: 5.429 min
Delta R.T.: -0.026 min
Response: 284862
Conc: 0.02 ng/ml

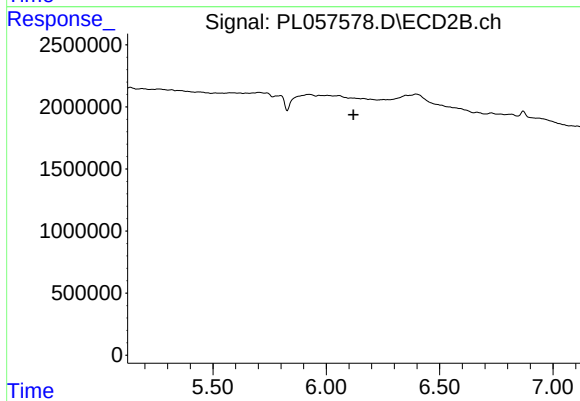

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.120 min
Response: 0
Conc: N.D.

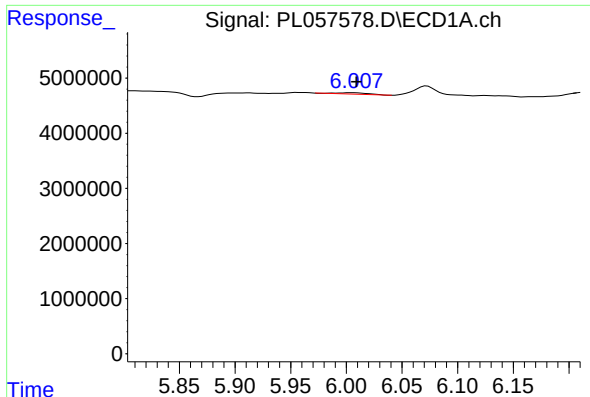

#14 Endrin


R.T.: 6.005 min
Delta R.T.: -0.004 min
Response: 513577
Conc: 0.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

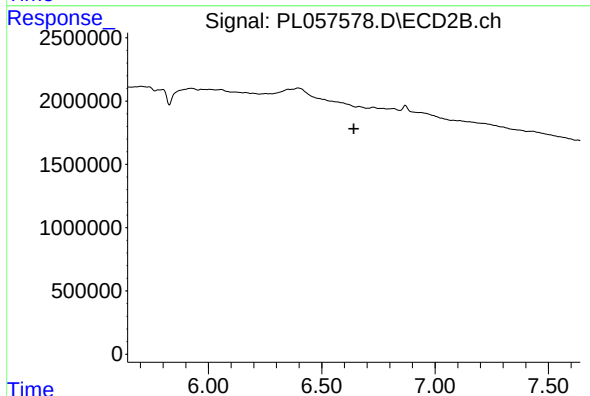


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.642 min
Response: 0
Conc: N.D.

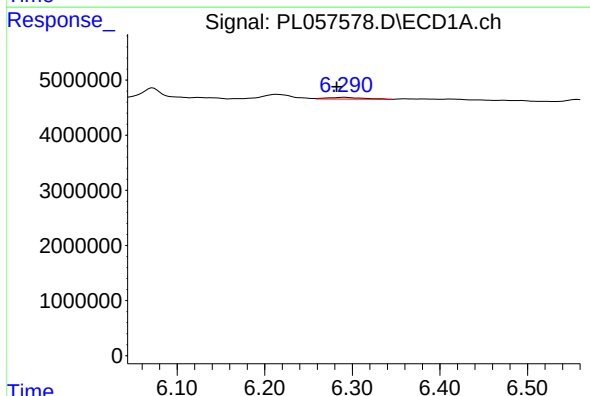


#15 Endosulfan II

R.T.: 6.291 min
Delta R.T.: 0.009 min
Response: 830470
Conc: 0.08 ng/ml

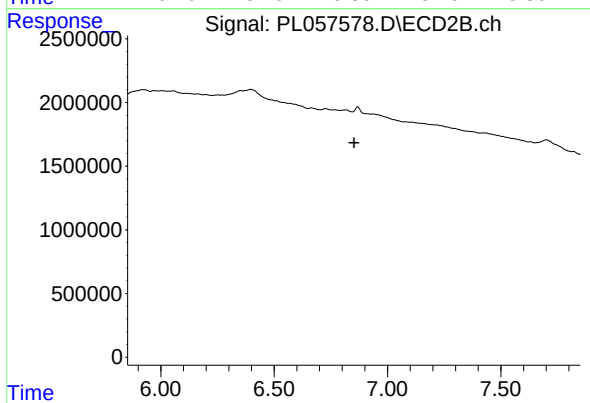

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.852 min
Response: 0
Conc: N.D.

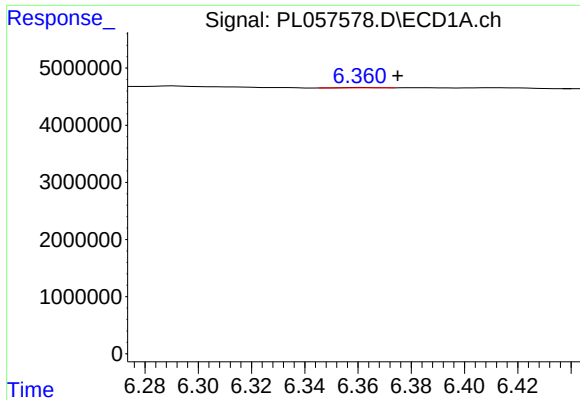

#17 4,4'-DDT


R.T.: 6.361 min
Delta R.T.: -0.014 min
Response: 48210
Conc: 0.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

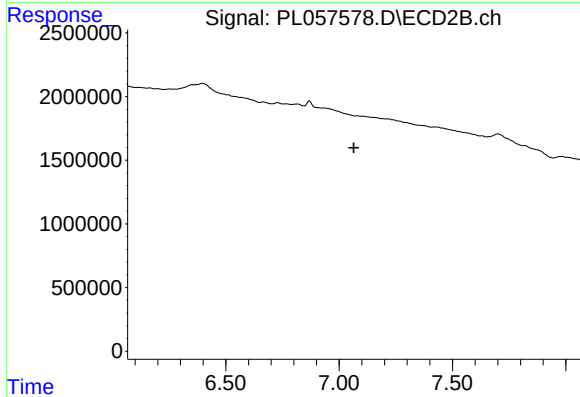


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.065 min
Response: 0
Conc: N.D.

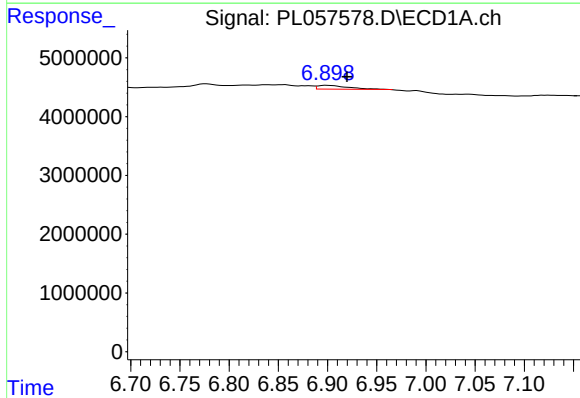


#20 Methoxychlor

R.T.: 6.899 min
Delta R.T.: -0.021 min
Response: 1297462
Conc: 0.24 ng/ml

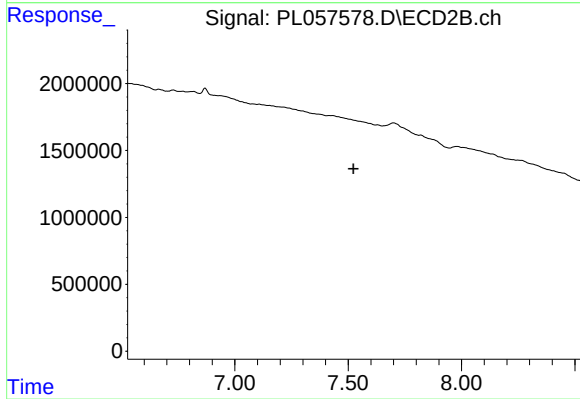

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.524 min
Response: 0
Conc: N.D.

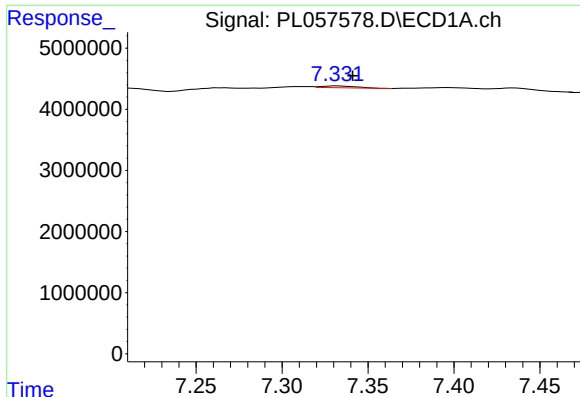

#22 Mirex


R.T.: 7.332 min
Delta R.T.: -0.009 min
Response: 405821
Conc: 0.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

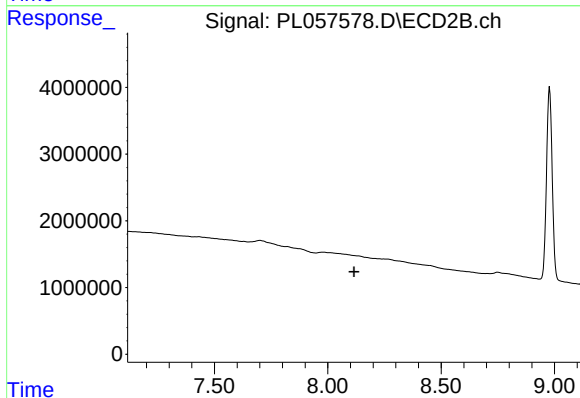


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

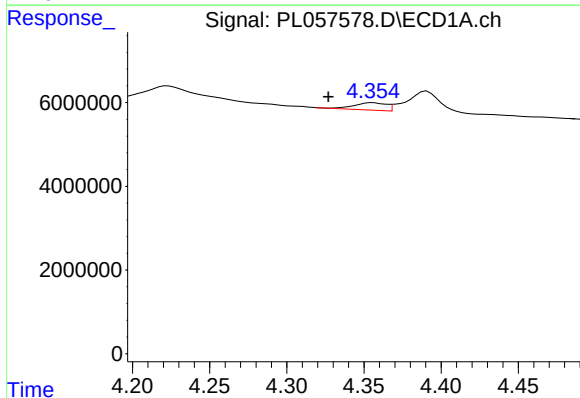


#23 Chlordane-1

R.T.: 4.356 min
Delta R.T.: 0.029 min
Response: 2607808
Conc: 8.03 ng/ml

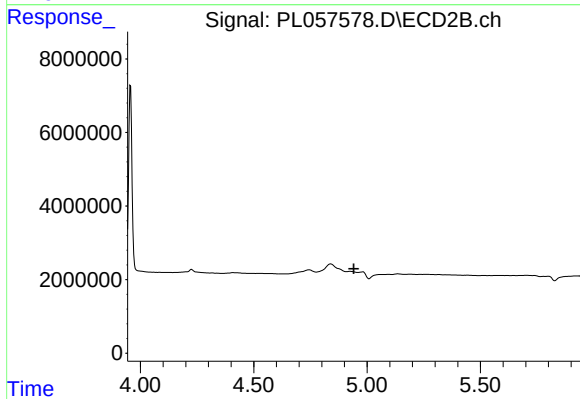

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

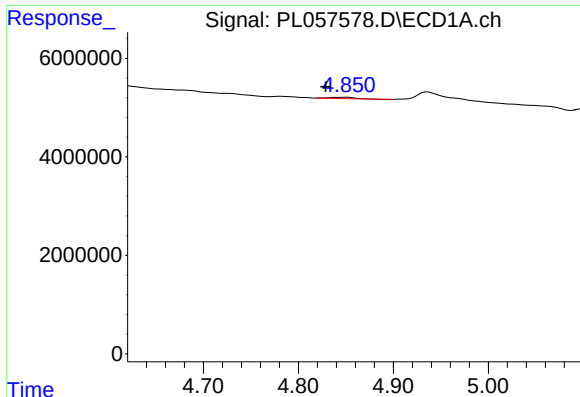

#24 Chlordane-2


R.T.: 4.851 min
Delta R.T.: 0.022 min
Response: 427894
Conc: 1.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

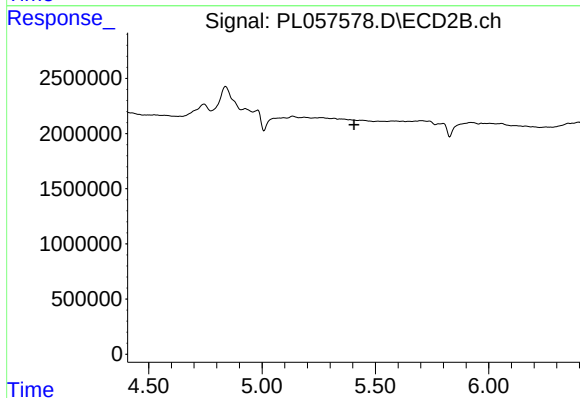


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.406 min
Response: 0
Conc: N.D.

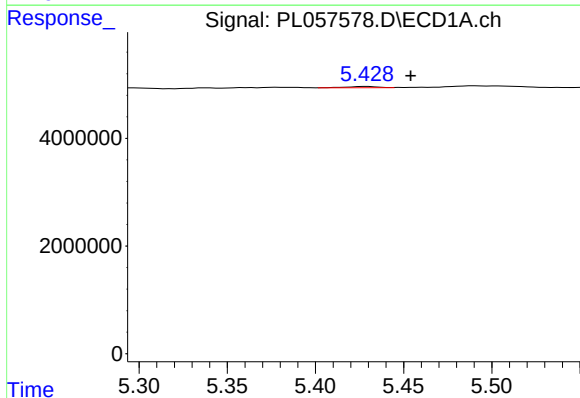


#26 Chlordane-4

R.T.: 5.429 min
Delta R.T.: -0.025 min
Response: 284862
Conc: 0.30 ng/ml

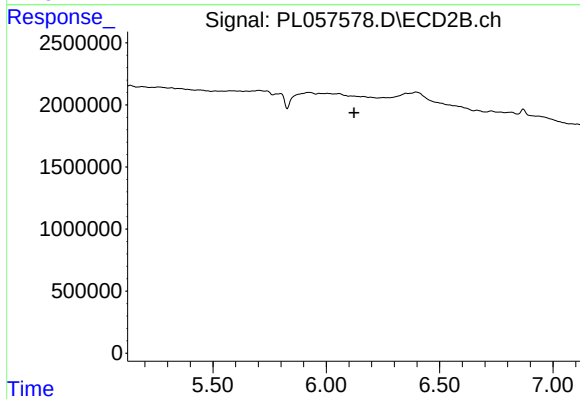

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.122 min
Response: 0
Conc: N.D.

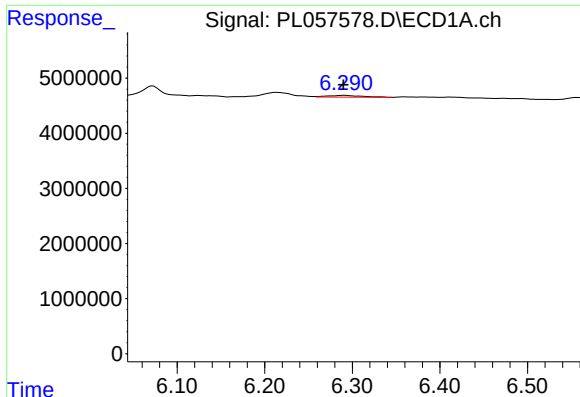

#27 Chlordane-5


R.T.: 6.291 min
Delta R.T.: 0.001 min
Response: 830470
Conc: 2.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

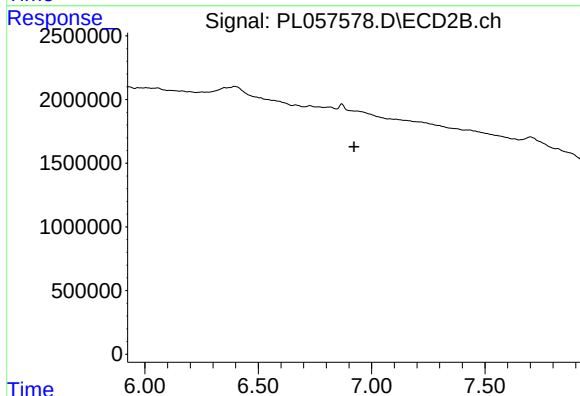


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

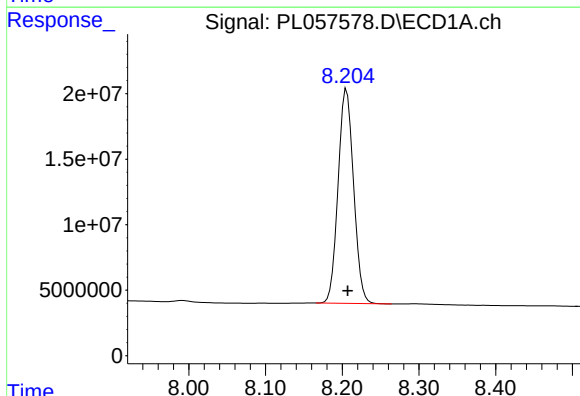

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.002 min
Response: 229492989
Conc: 21.69 ng/ml

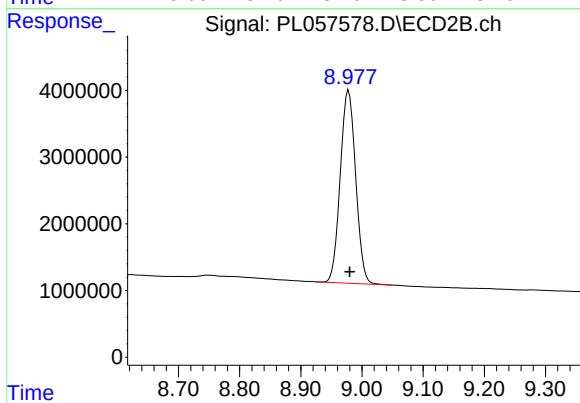

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: -0.002 min
Response: 50639129
Conc: 22.84 ng/ml