

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032620\
 Data File : PL057591.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2020 19:07
 Operator : AJ\MA
 Sample : PB127811BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB127811BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:14:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.957	194.0E6	43283379	20.928	19.950
28)	SA Decachlor...	8.206	8.980	163.1E6	40099340	15.417	18.084
Target Compounds							
2)	A alpha-BHC	3.889	0.000	3812367	0	0.239	N.D. #
4)	MA Heptachlor	0.000	5.137	0	3668055	N.D.	1.165 #
14)	MA Endrin	5.998	0.000	418883	0	0.037	N.D. #
18)	B Endrin al...	6.472f	0.000	106869	0	0.012	N.D. #
19)	B Endosulfa...	6.691f	0.000	527581	0	0.053	N.D. #
21)	B Endrin ke...	7.159	0.000	475728	0	0.042	N.D. #
22)	Mirex	7.328	0.000	98255	0	0.012	N.D. #
23)	Chlordane-1	4.356f	0.000	2749395	0	8.471	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032620\
Data File : PL057591.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2020 19:07
Operator : AJ\MA
Sample : PB127811BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB127811BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:14:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

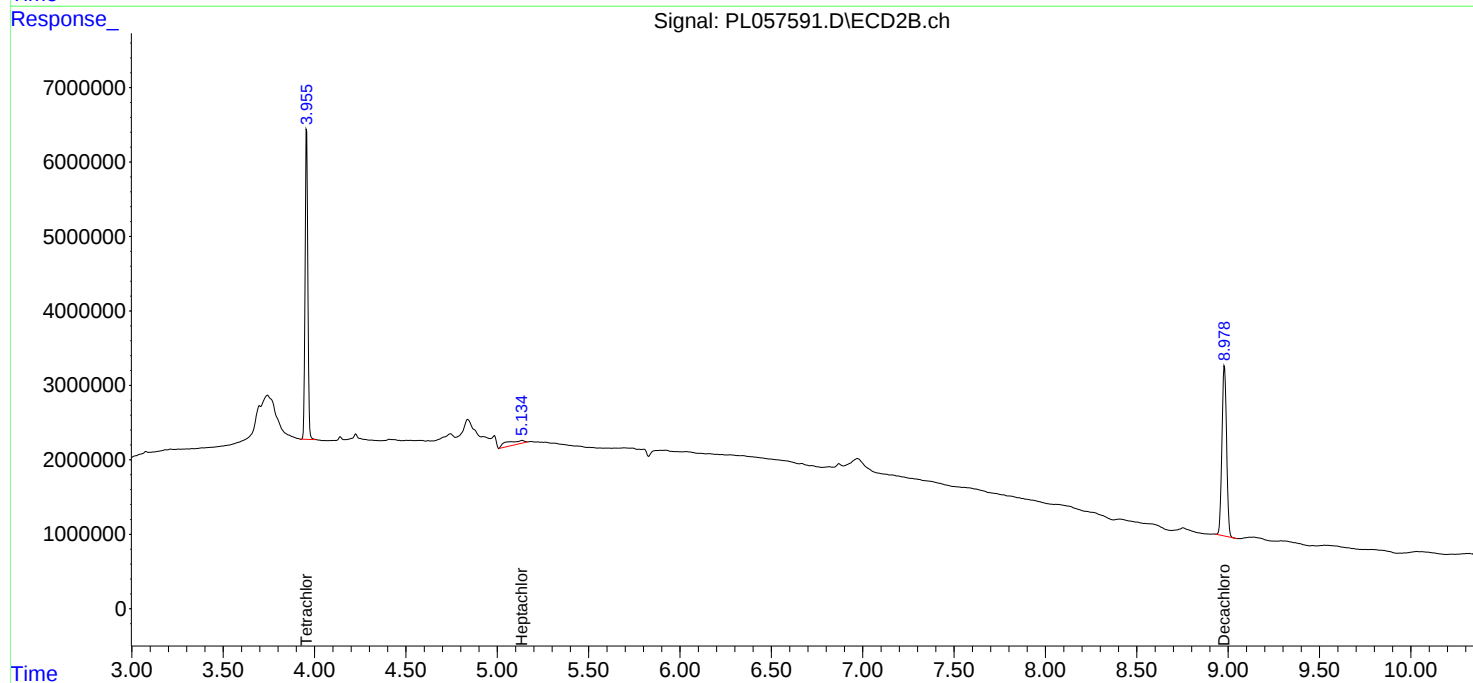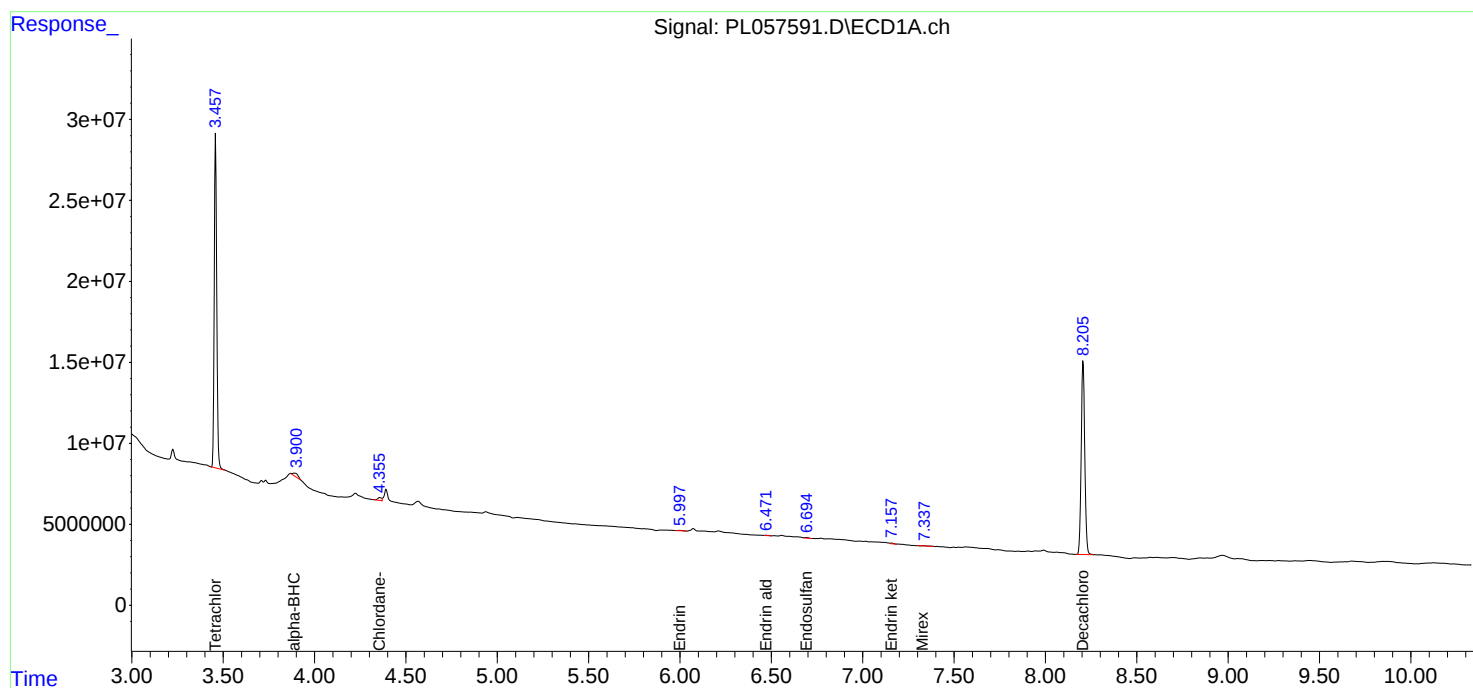


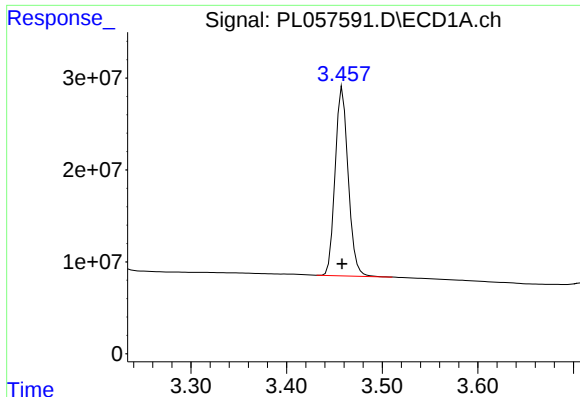

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 193988940
Conc: 20.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127811BL

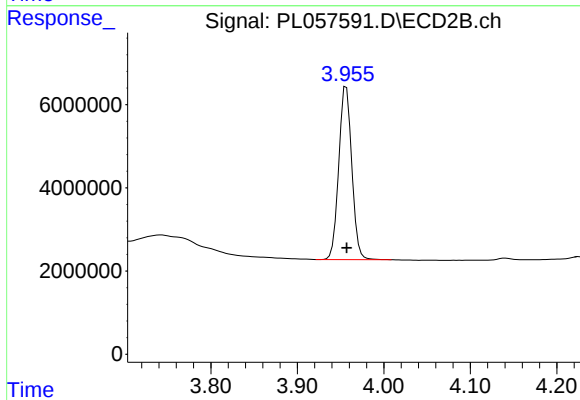


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 43283379
Conc: 19.95 ng/ml

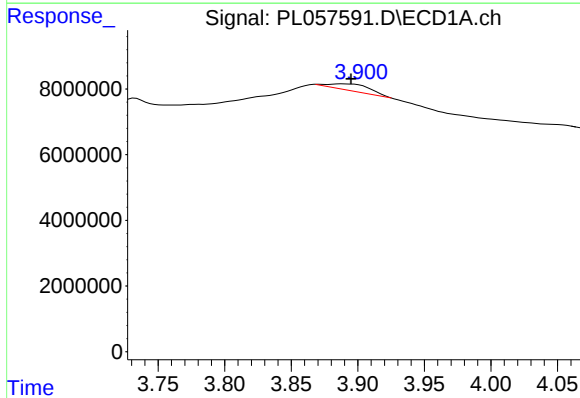


#2 alpha-BHC

R.T.: 3.889 min
Delta R.T.: -0.006 min
Response: 3812367
Conc: 0.24 ng/ml

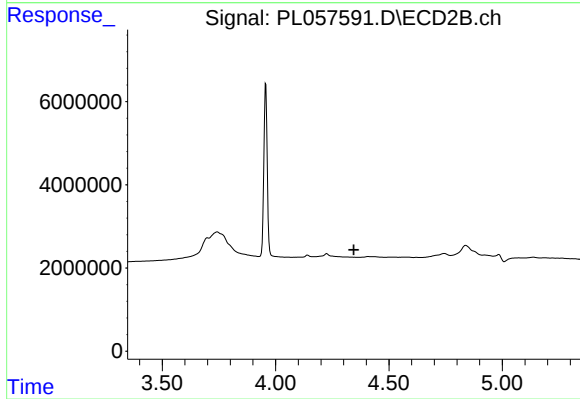

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

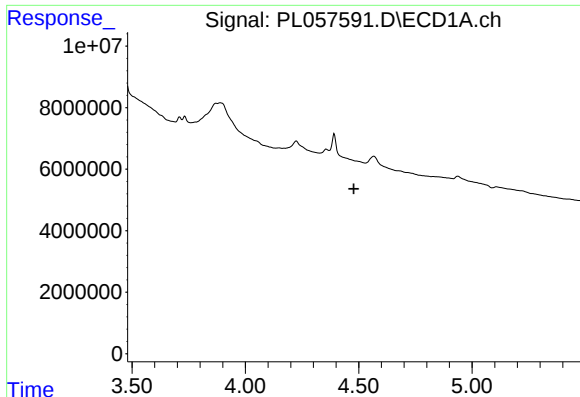

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB127811BL

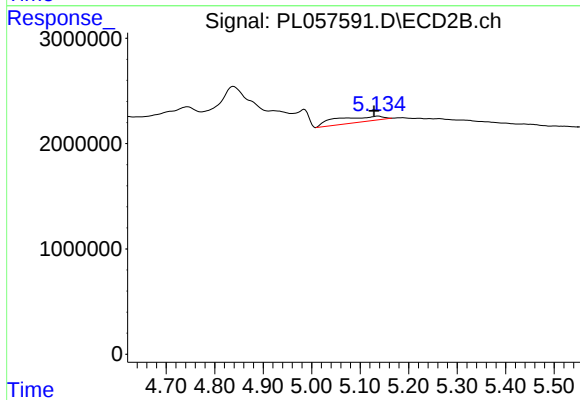


#4 Heptachlor

R.T.: 5.137 min
Delta R.T.: 0.008 min
Response: 3668055
Conc: 1.17 ng/ml

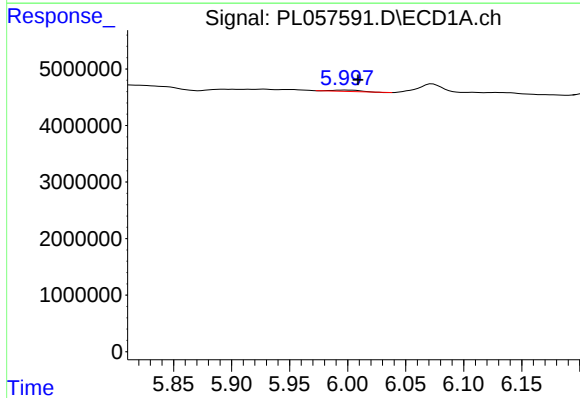


#14 Endrin

R.T.: 5.998 min
Delta R.T.: -0.011 min
Response: 418883
Conc: 0.04 ng/ml

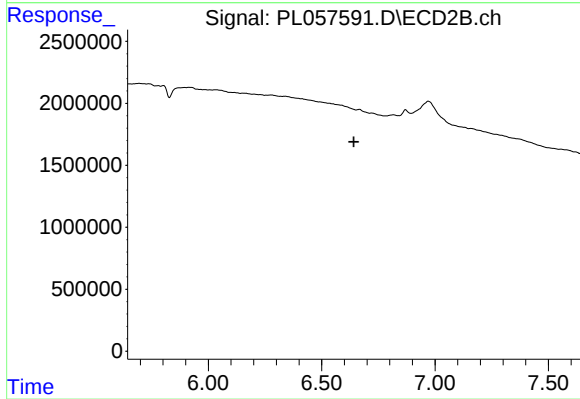

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.642 min
Response: 0
Conc: N.D.

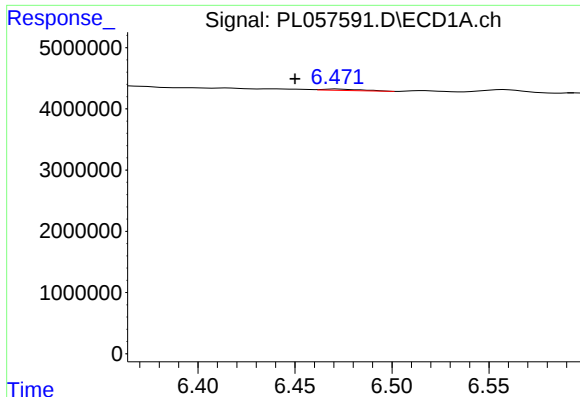

#18 Endrin aldehyde


R.T.: 6.472 min
Delta R.T.: 0.022 min
Response: 106869
Conc: 0.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127811BL

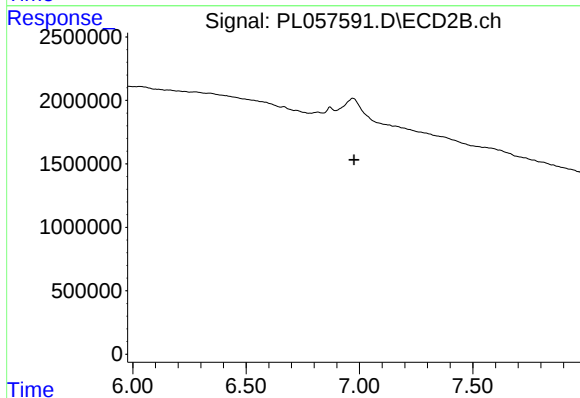


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.976 min
Response: 0
Conc: N.D.

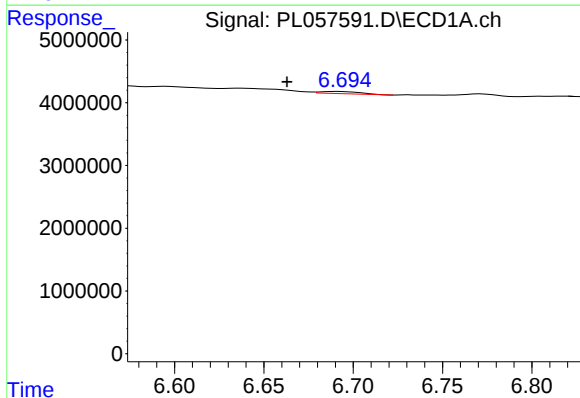


#19 Endosulfan Sulfate

R.T.: 6.691 min
Delta R.T.: 0.028 min
Response: 527581
Conc: 0.05 ng/ml

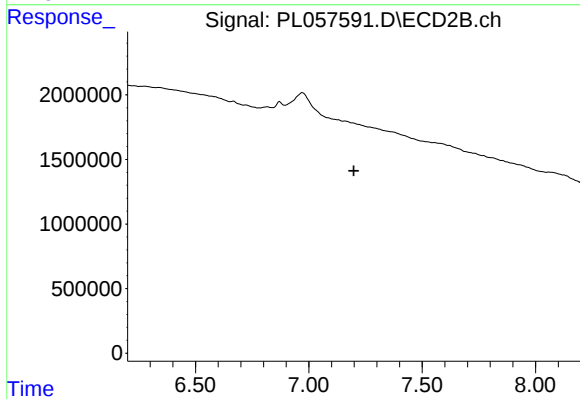

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

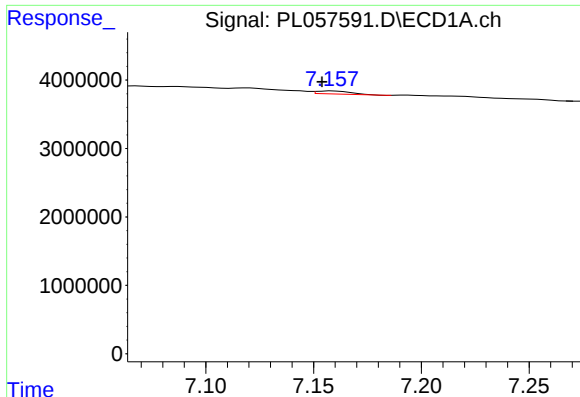

#21 Endrin ketone


R.T.: 7.159 min
Delta R.T.: 0.005 min
Response: 475728
Conc: 0.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127811BL

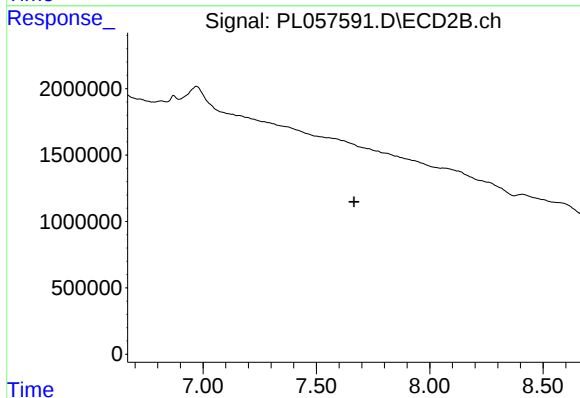


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.666 min
Response: 0
Conc: N.D.

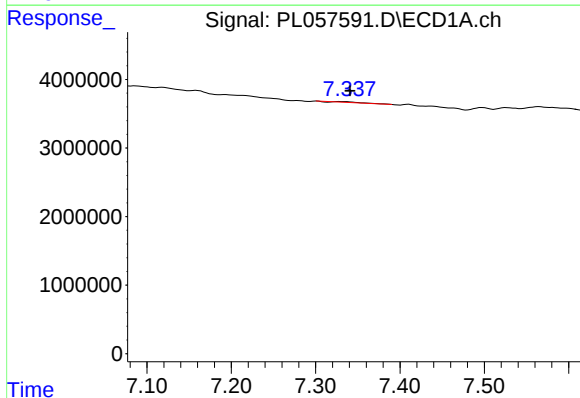


#22 Mirex

R.T.: 7.328 min
Delta R.T.: -0.013 min
Response: 98255
Conc: 0.01 ng/ml

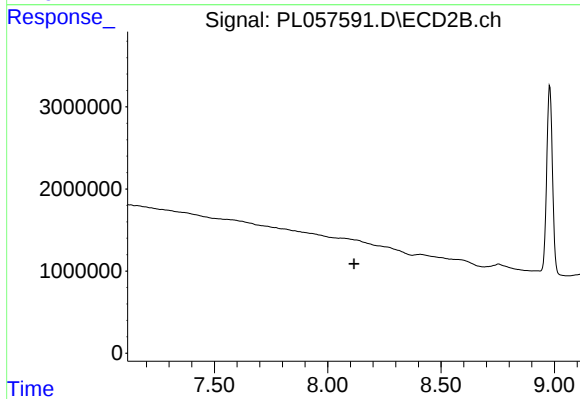

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

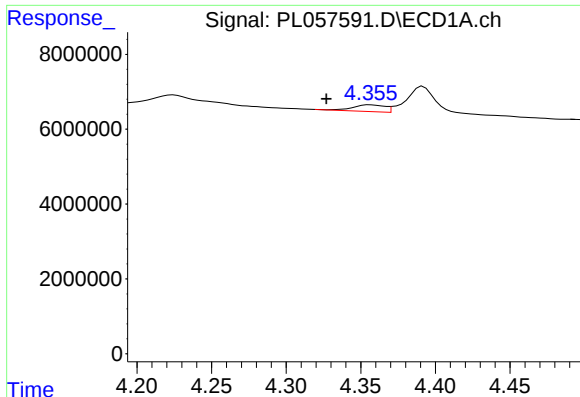

#23 Chlordane-1


R.T.: 4.356 min
Delta R.T.: 0.029 min
Response: 2749395
Conc: 8.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127811BL

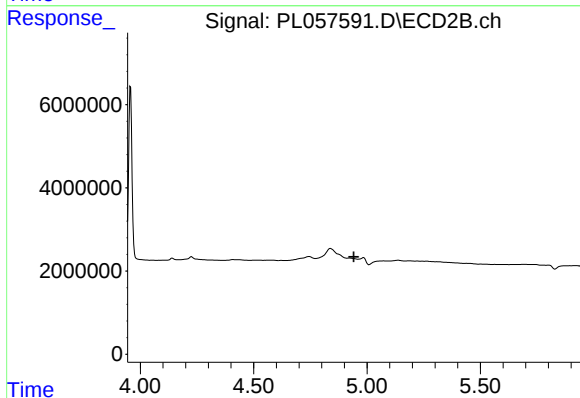


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

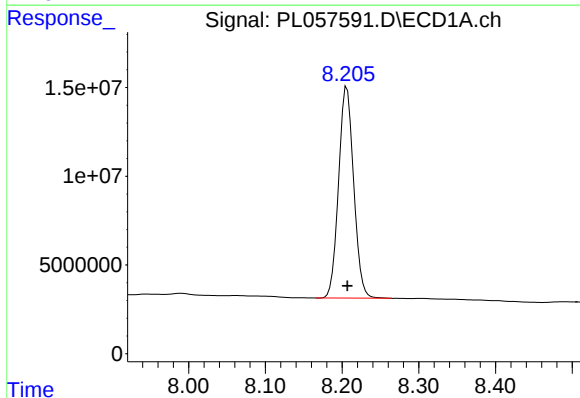

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 163127188
Conc: 15.42 ng/ml

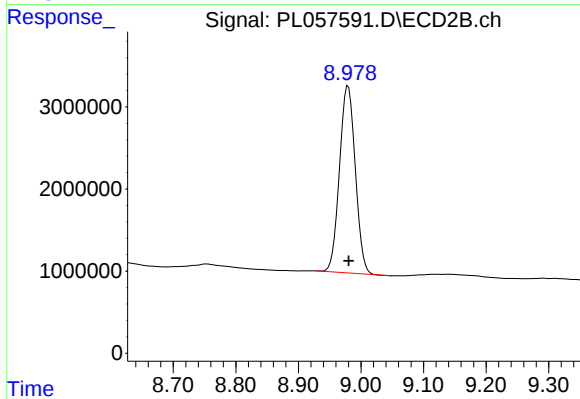

#28 Decachlorobiphenyl

R.T.: 8.980 min
Delta R.T.: 0.000 min
Response: 40099340
Conc: 18.08 ng/ml