

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032620\
 Data File : PL057593.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2020 19:36
 Operator : AJ\MA
 Sample : PB127811TB
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB127811TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:15:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	3.957	196.5E6	44207259	21.195	20.376
28)	SA Decachlor...	8.207	8.979	170.3E6	41990124	16.092	18.937
Target Compounds							
2)	A alpha-BHC	3.893	0.000	4438291	0	0.279	N.D. #
4)	MA Heptachlor	0.000	5.134	0	3512602	N.D.	1.116 #
15)	B Endosulfa...	6.288	0.000	743287	0	0.068	N.D. #
21)	B Endrin ke...	7.158	0.000	505046	0	0.045	N.D. #
22)	Mirex	7.343	0.000	309920	0	0.038	N.D. #
23)	Chlordane-1	4.355f	0.000	2404624	0	7.409	N.D. #
24)	Chlordane-2	4.843	0.000	235475	0	0.648	N.D. #
27)	Chlordane-5	6.288	0.000	743287	0	2.043	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032620\
Data File : PL057593.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2020 19:36
Operator : AJ\MA
Sample : PB127811TB
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB127811TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:15:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

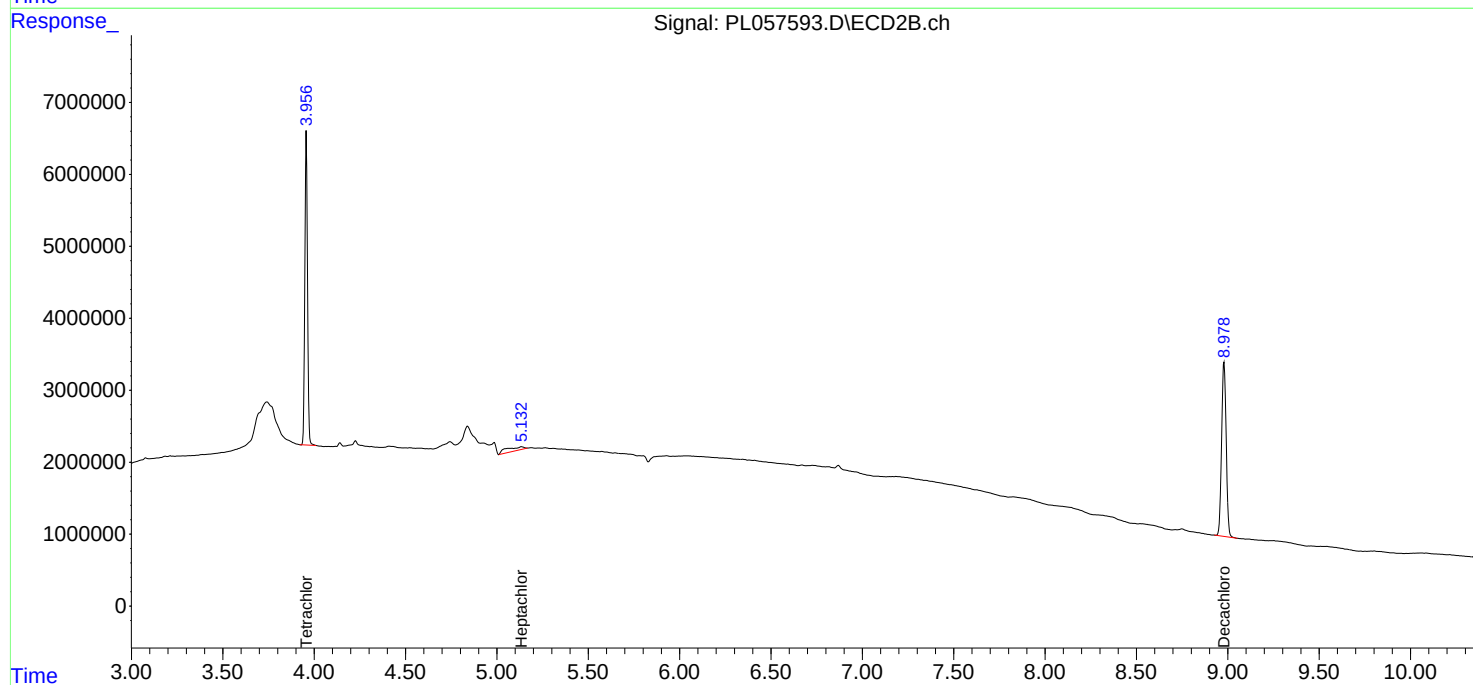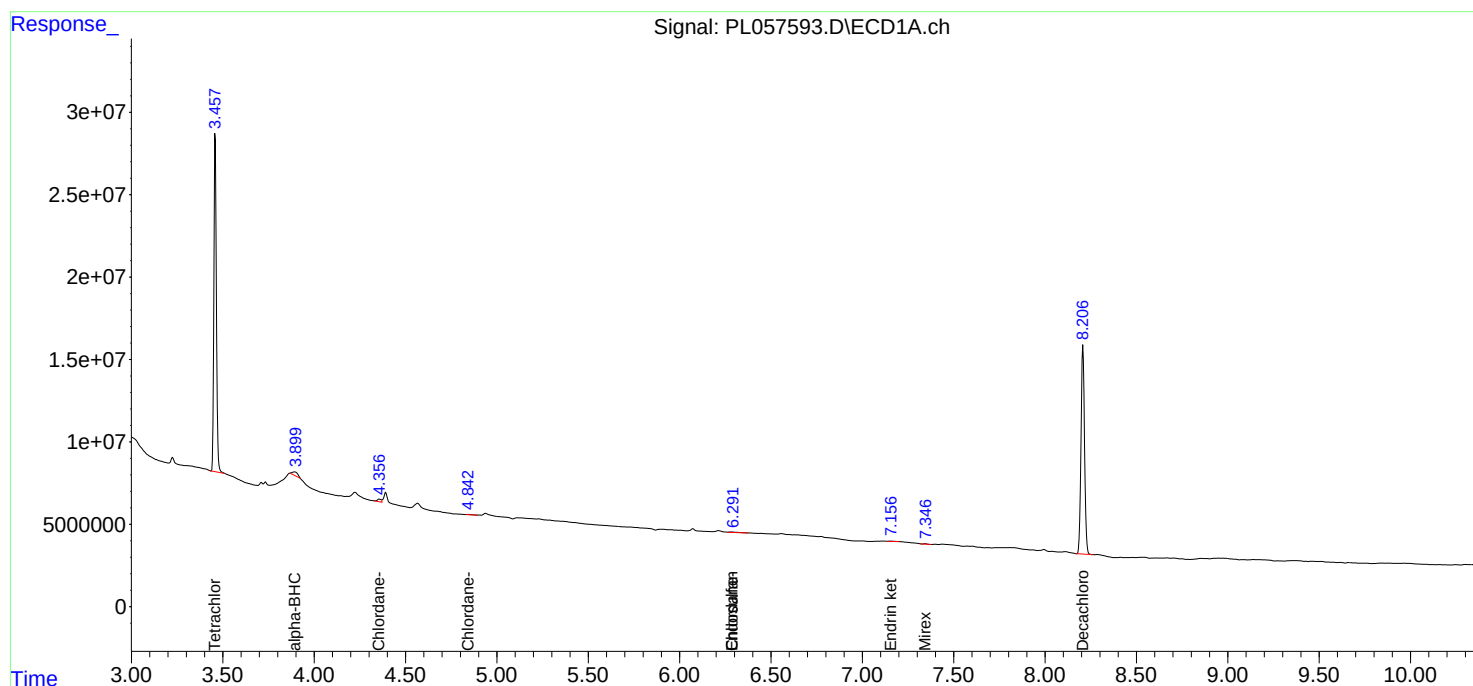


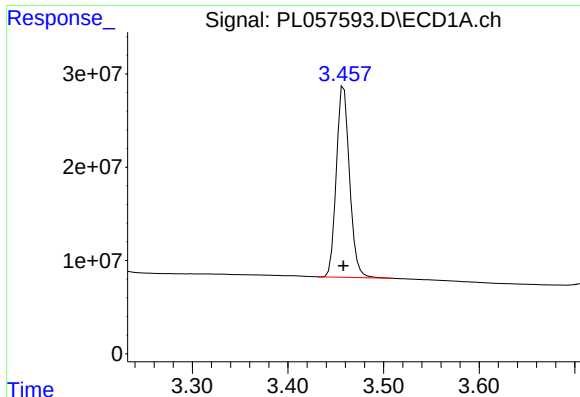

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 196460885
Conc: 21.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127811TB

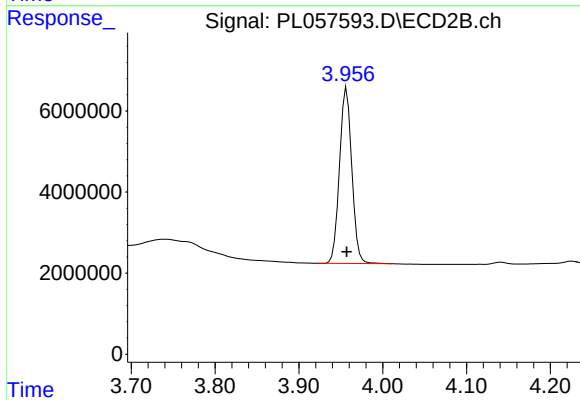


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 44207259
Conc: 20.38 ng/ml

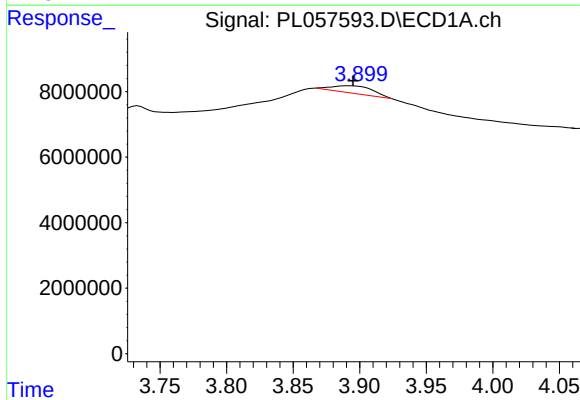


#2 alpha-BHC

R.T.: 3.893 min
Delta R.T.: -0.002 min
Response: 4438291
Conc: 0.28 ng/ml

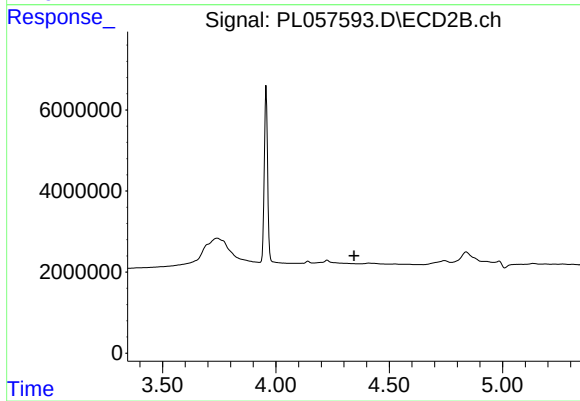

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

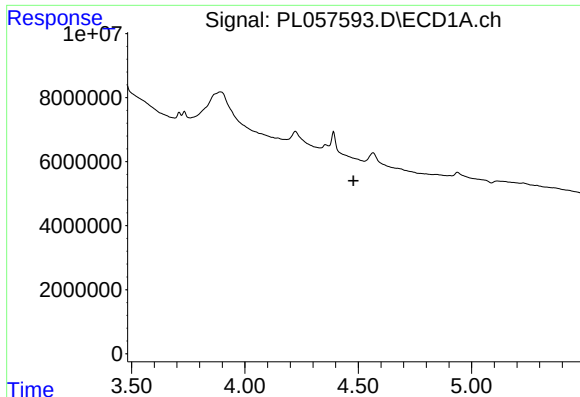

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB127811TB

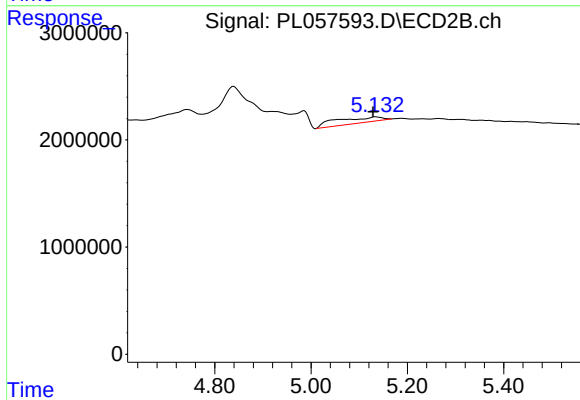


#4 Heptachlor

R.T.: 5.134 min
Delta R.T.: 0.005 min
Response: 3512602
Conc: 1.12 ng/ml

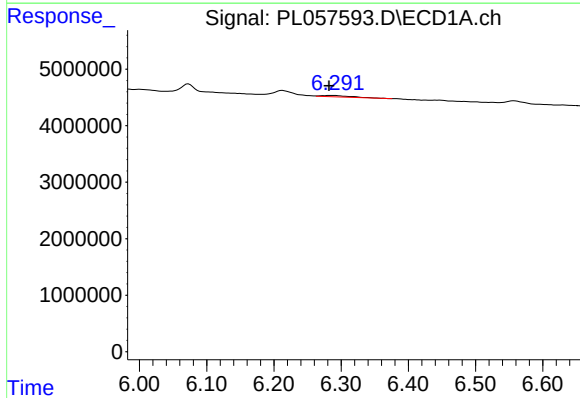


#15 Endosulfan II

R.T.: 6.288 min
Delta R.T.: 0.006 min
Response: 743287
Conc: 0.07 ng/ml

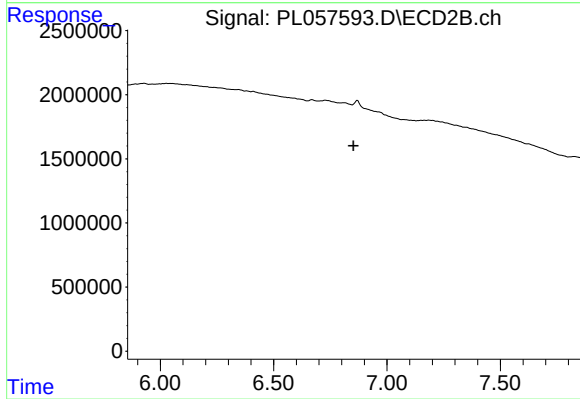

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

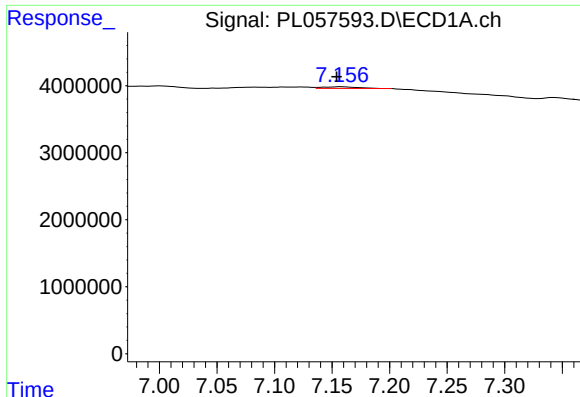

#21 Endrin ketone


R.T.: 7.158 min
Delta R.T.: 0.004 min
Response: 505046
Conc: 0.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127811TB

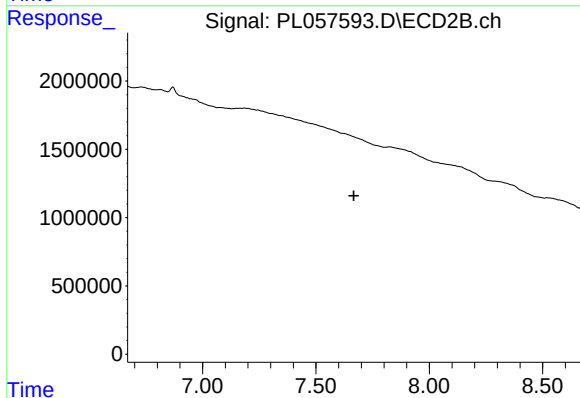


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.666 min
Response: 0
Conc: N.D.

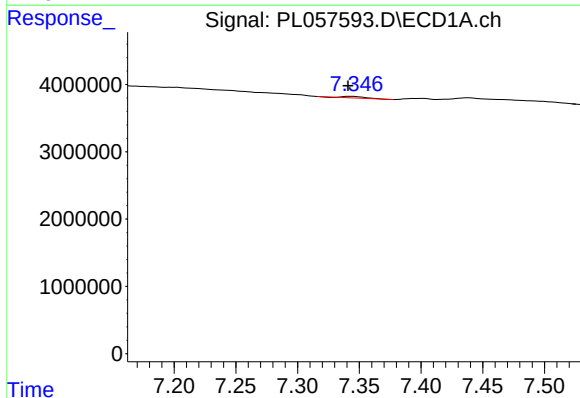


#22 Mirex

R.T.: 7.343 min
Delta R.T.: 0.002 min
Response: 309920
Conc: 0.04 ng/ml

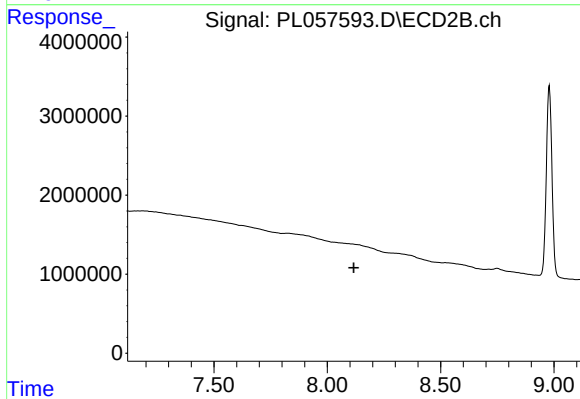

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

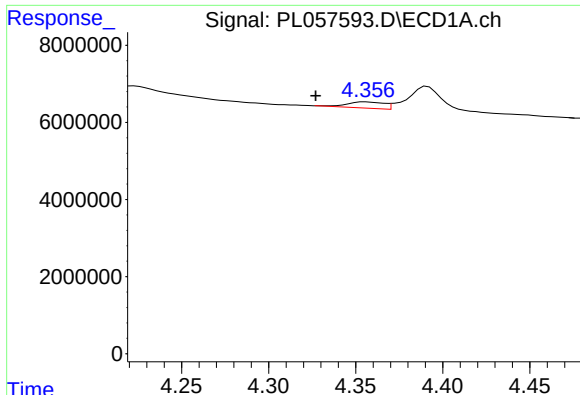

#23 Chlordane-1


R.T.: 4.355 min
Delta R.T.: 0.028 min
Response: 2404624
Conc: 7.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127811TB

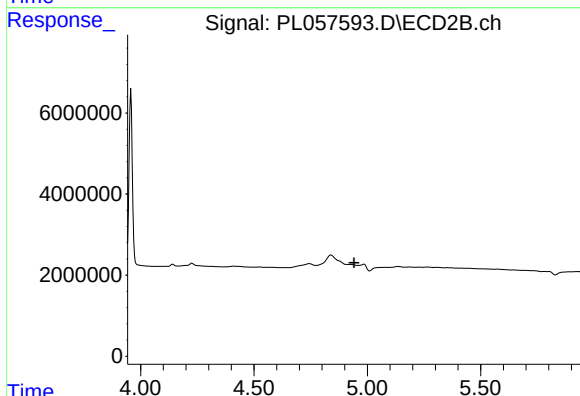


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

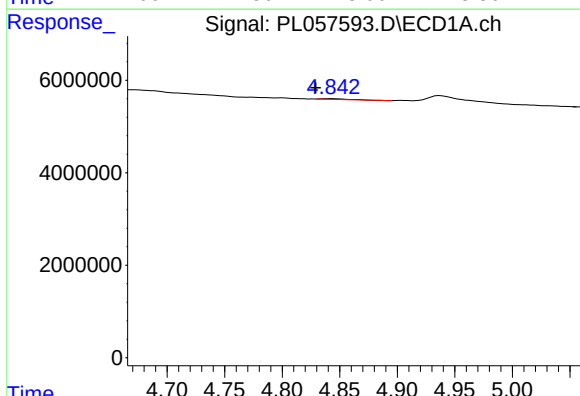


#24 Chlordane-2

R.T.: 4.843 min
Delta R.T.: 0.014 min
Response: 235475
Conc: 0.65 ng/ml

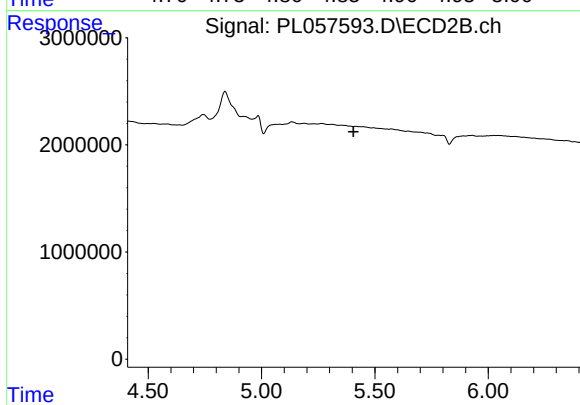

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.406 min
Response: 0
Conc: N.D.

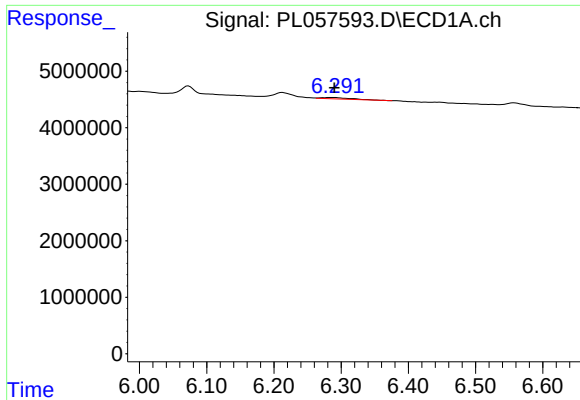

#27 Chlordane-5


R.T.: 6.288 min
Delta R.T.: -0.002 min
Response: 743287
Conc: 2.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127811TB

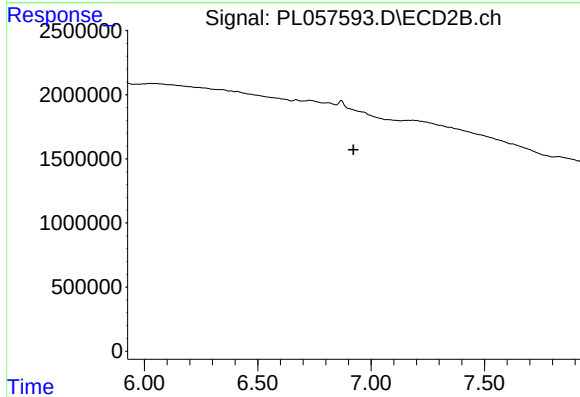


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.922 min
Response: 0
Conc: N.D.

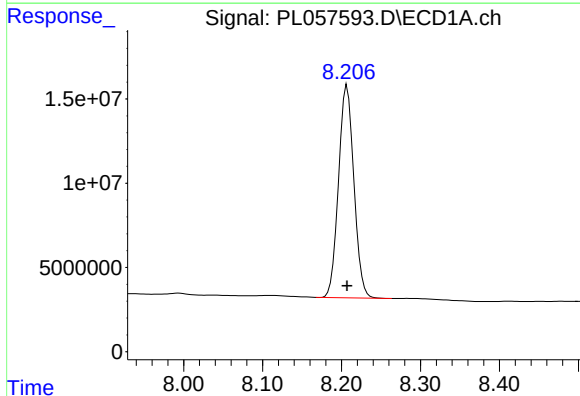

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 170271770
Conc: 16.09 ng/ml

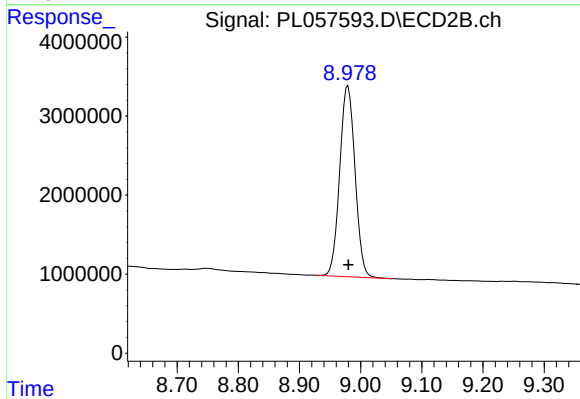

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: 0.000 min
Response: 41990124
Conc: 18.94 ng/ml