

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032620\
 Data File : PL057600.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2020 21:15
 Operator : AJ\MA
 Sample : PB127834TB
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB127834TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:16:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	3.957	189.4E6	43273652	20.431	19.946
28)	SA Decachlor...	8.206	8.980	180.9E6	45157473	17.101	20.365
Target Compounds							
2)	A alpha-BHC	3.893	0.000	4407711	0	0.277	N.D. #
4)	MA Heptachlor	0.000	5.136	0	5382384	N.D.	1.710 #
15)	B Endosulfa...	6.272	0.000	282657	0	0.026	N.D. #
18)	B Endrin al...	6.448	0.000	735935	0	0.080	N.D. #
19)	B Endosulfa...	6.688f	0.000	307942	0	0.031	N.D. #
22)	Mirex	7.339	0.000	535317	0	0.066	N.D. #
23)	Chlordane-1	4.356f	0.000	2525829	0	7.782	N.D. #
24)	Chlordane-2	4.837	0.000	341850	0	0.941	N.D. #
27)	Chlordane-5	6.272f	0.000	282657	0	0.777	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032620\
Data File : PL057600.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2020 21:15
Operator : AJ\MA
Sample : PB127834TB
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB127834TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:16:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

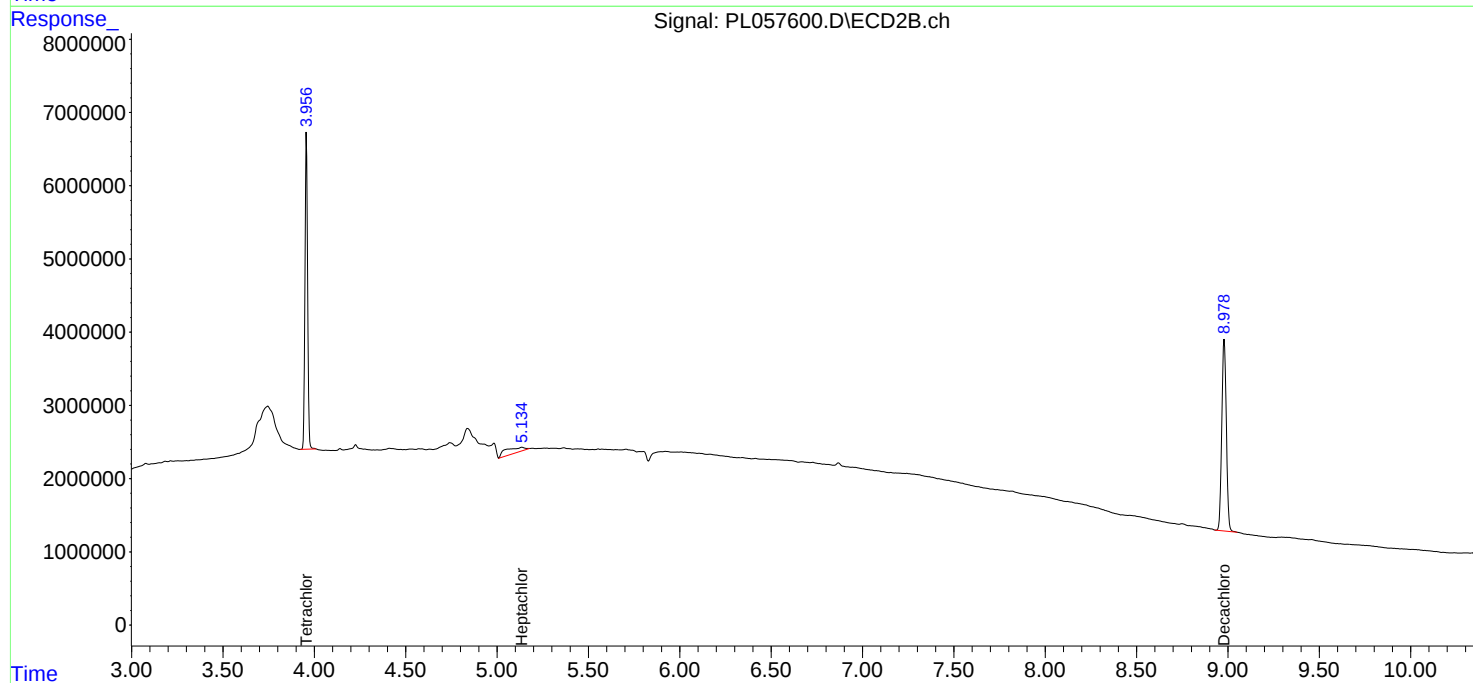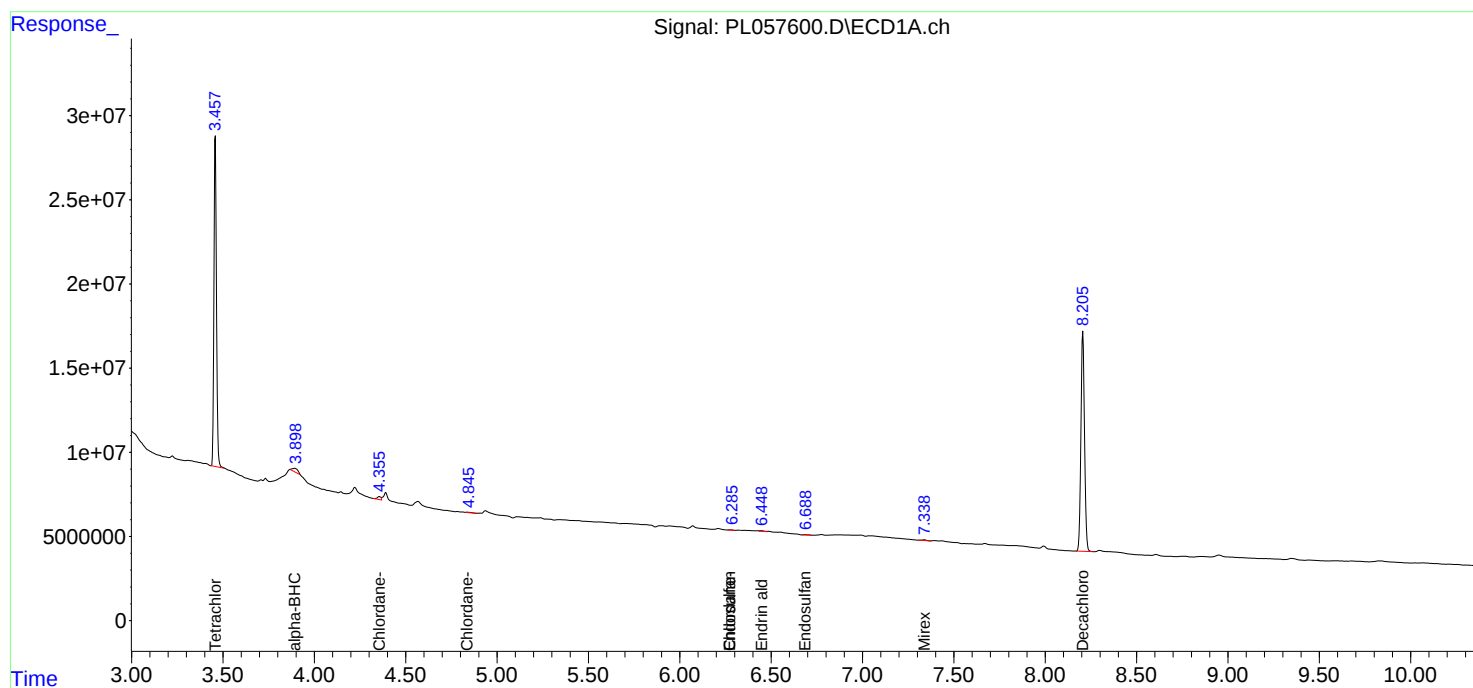


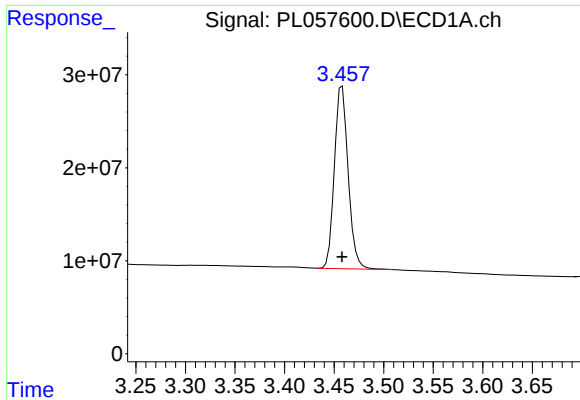

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 189383606
Conc: 20.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127834TB

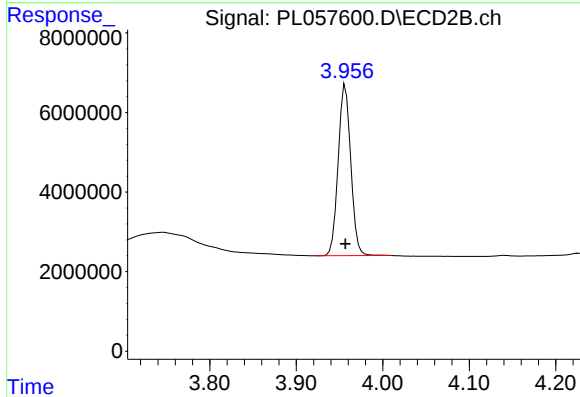


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 43273652
Conc: 19.95 ng/ml

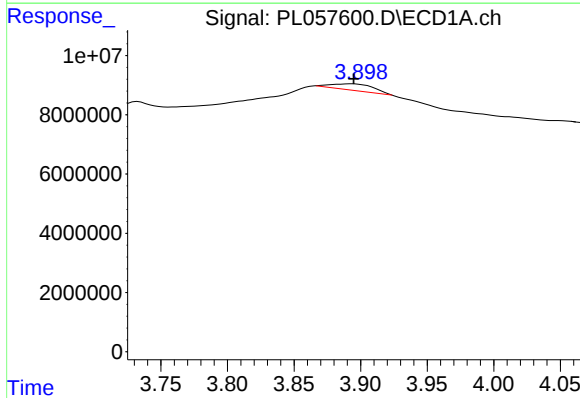


#2 alpha-BHC

R.T.: 3.893 min
Delta R.T.: -0.002 min
Response: 4407711
Conc: 0.28 ng/ml

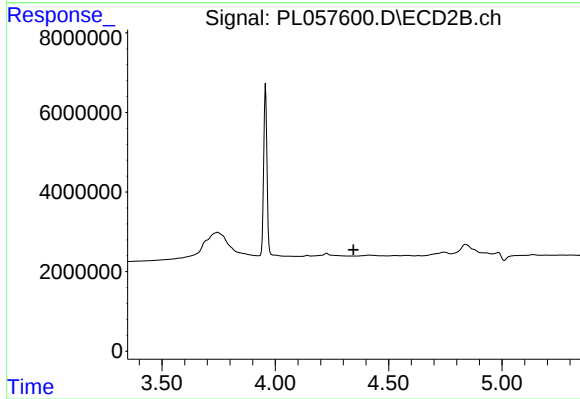

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.345 min
Response: 0
Conc: N.D.

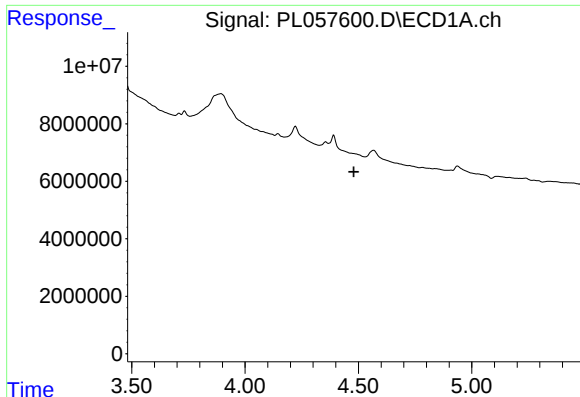

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB127834TB

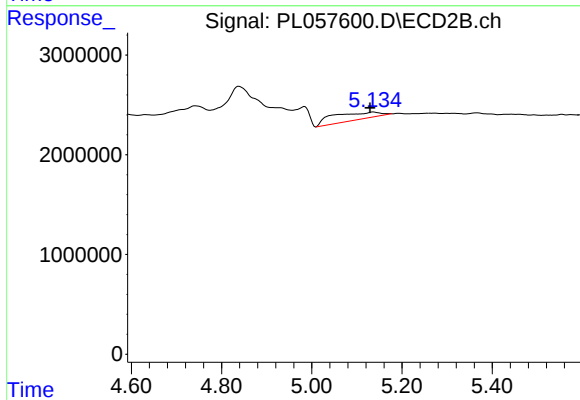


#4 Heptachlor

R.T.: 5.136 min
Delta R.T.: 0.007 min
Response: 5382384
Conc: 1.71 ng/ml

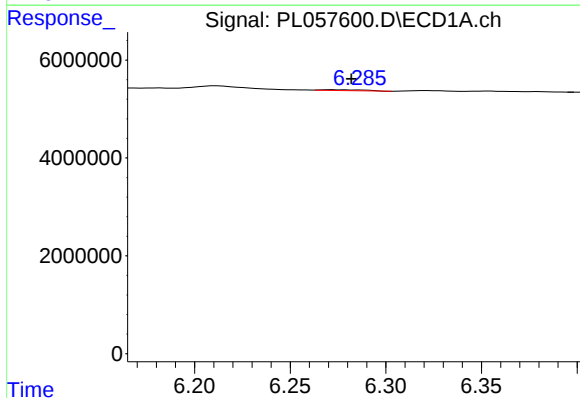


#15 Endosulfan II

R.T.: 6.272 min
Delta R.T.: -0.010 min
Response: 282657
Conc: 0.03 ng/ml

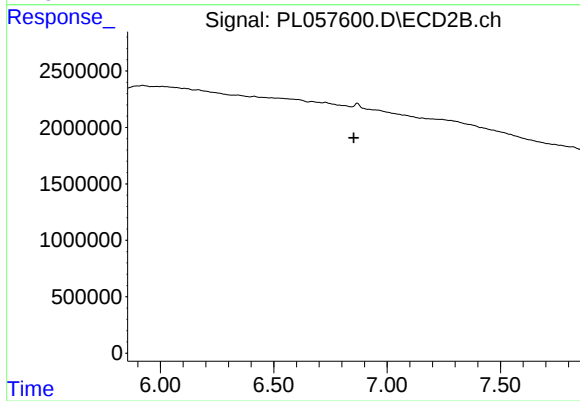

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

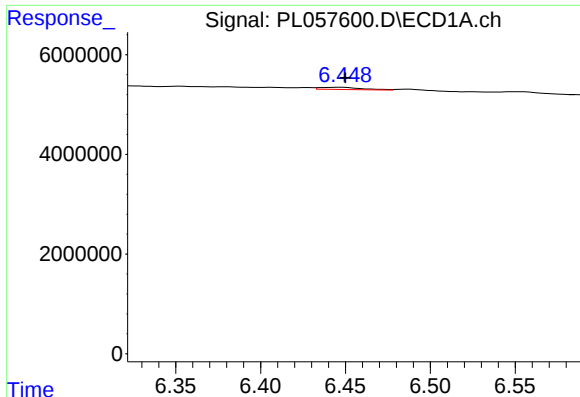

#18 Endrin aldehyde


R.T.: 6.448 min
Delta R.T.: -0.002 min
Response: 735935
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127834TB

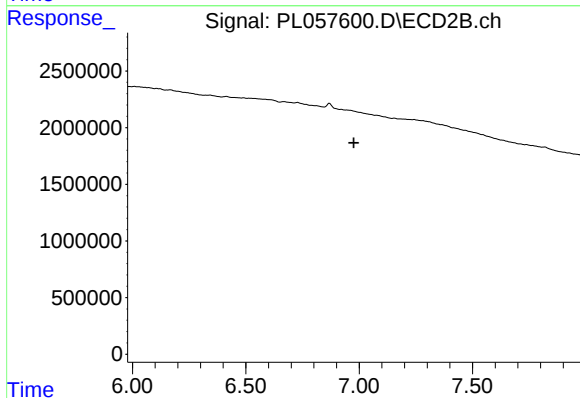


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.976 min
Response: 0
Conc: N.D.

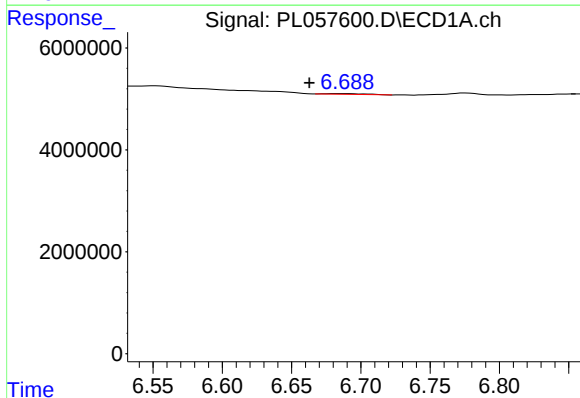


#19 Endosulfan Sulfate

R.T.: 6.688 min
Delta R.T.: 0.024 min
Response: 307942
Conc: 0.03 ng/ml

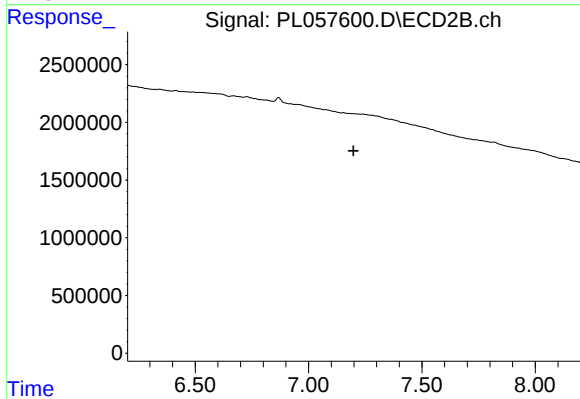

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

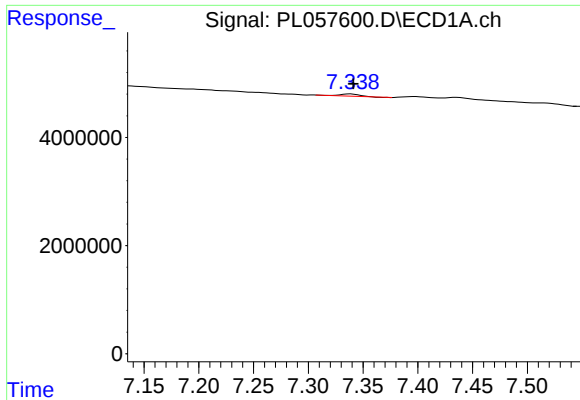

#22 Mirex


R.T.: 7.339 min
Delta R.T.: -0.002 min
Response: 535317
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127834TB

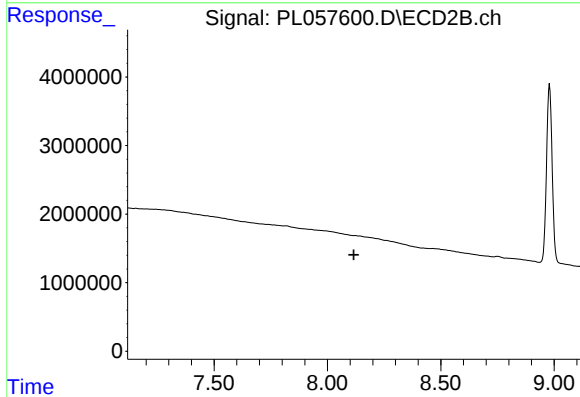


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

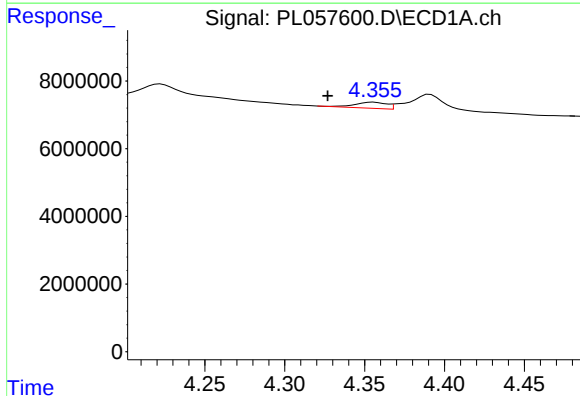


#23 Chlordane-1

R.T.: 4.356 min
Delta R.T.: 0.029 min
Response: 2525829
Conc: 7.78 ng/ml

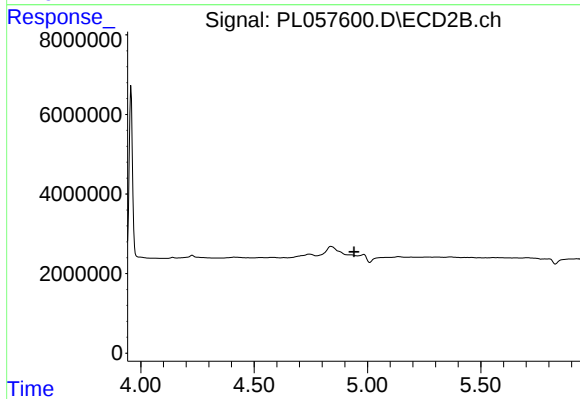

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

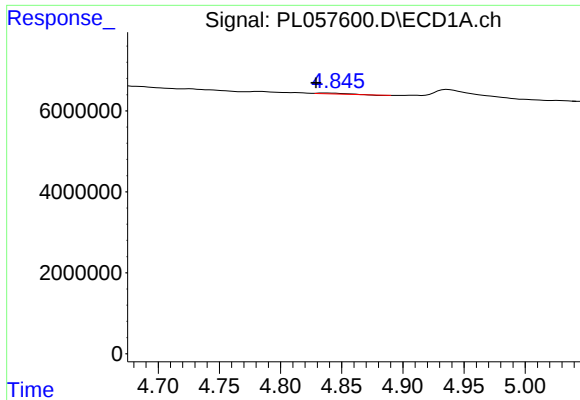

#24 Chlordane-2


R.T.: 4.837 min
Delta R.T.: 0.008 min
Response: 341850
Conc: 0.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127834TB

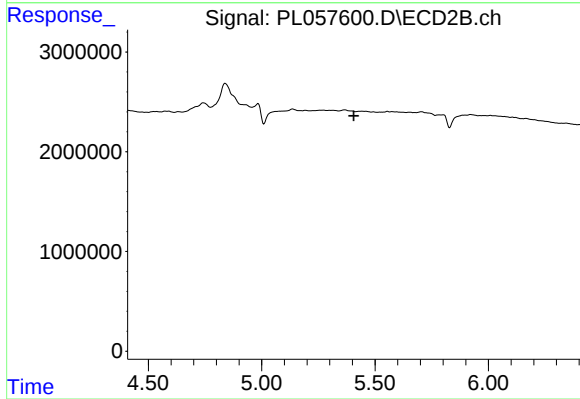


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.406 min
Response: 0
Conc: N.D.

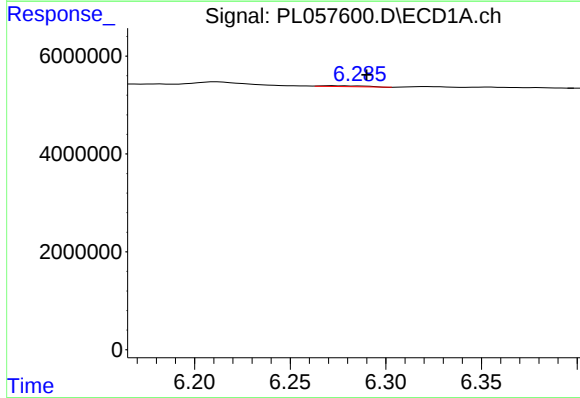


#27 Chlordane-5

R.T.: 6.272 min
Delta R.T.: -0.018 min
Response: 282657
Conc: 0.78 ng/ml

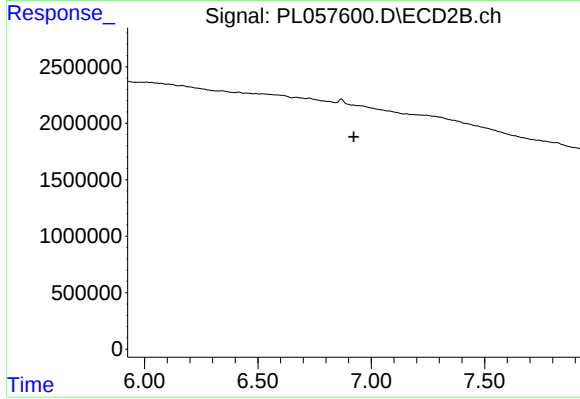

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

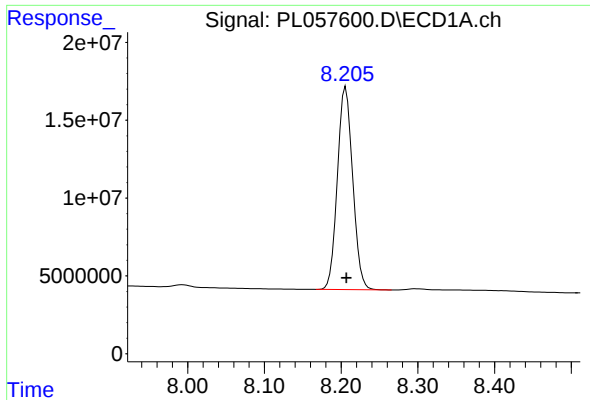

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.001 min
Response: 180948123
Conc: 17.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127834TB

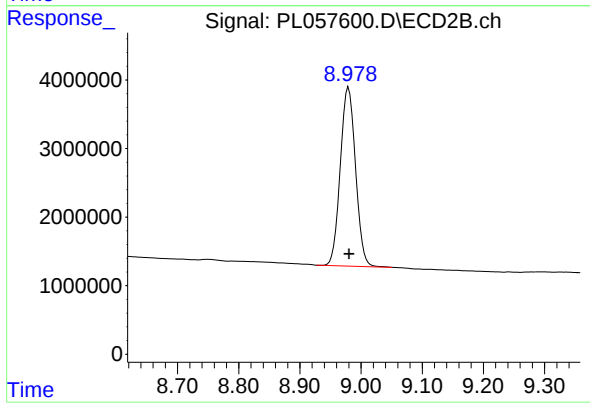

#28 Decachlorobiphenyl

R.T.: 8.980 min
Delta R.T.: 0.000 min
Response: 45157473
Conc: 20.37 ng/ml