

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032620\
 Data File : PL057601.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2020 21:29
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:17:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.957	235.9E6	54174217	25.446	24.970
28)	SA Decachlor...	8.207	8.980	205.7E6	53630976	19.439	24.187
Target Compounds							
2)	A alpha-BHC	3.891	0.000	4538382	0	0.285	N.D. #
8)	B Heptachlo...	5.170	0.000	989919	0	0.077	N.D. #
11)	B alpha-Chl...	5.430f	0.000	432188	0	0.033	N.D. #
13)	MA Dieldrin	5.760	0.000	248787	0	0.020	N.D. #
15)	B Endosulfa...	6.290	0.000	394239	0	0.036	N.D. #
20)	A Methoxychlor	6.908	0.000	165929	0	0.031	N.D. #
23)	Chlordane-1	4.357f	0.000	2736574	0	8.431	N.D. #
24)	Chlordane-2	4.847f	0.000	420359	0	1.157	N.D. #
26)	Chlordane-4	5.430f	0.000	432188	0	0.451	N.D. #
27)	Chlordane-5	6.290	0.000	394239	0	1.083	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032620\
Data File : PL057601.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2020 21:29
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:17:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

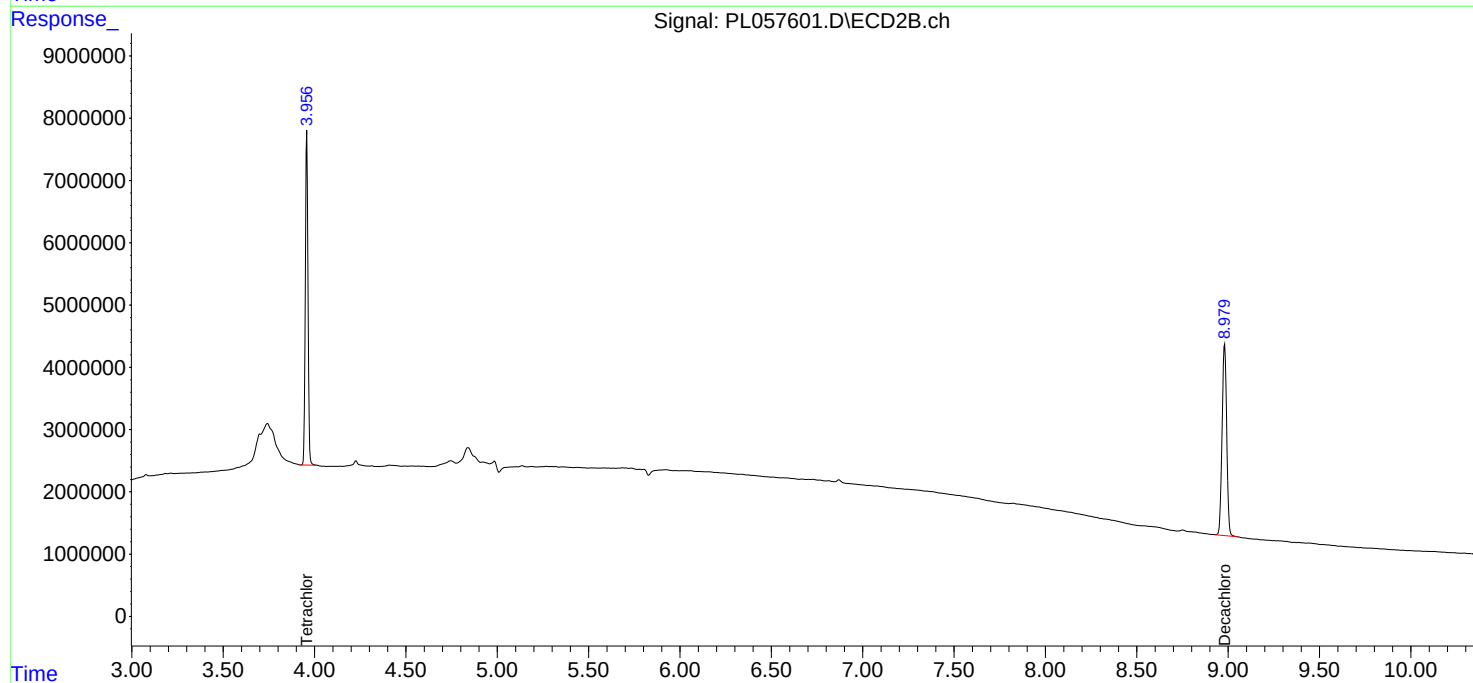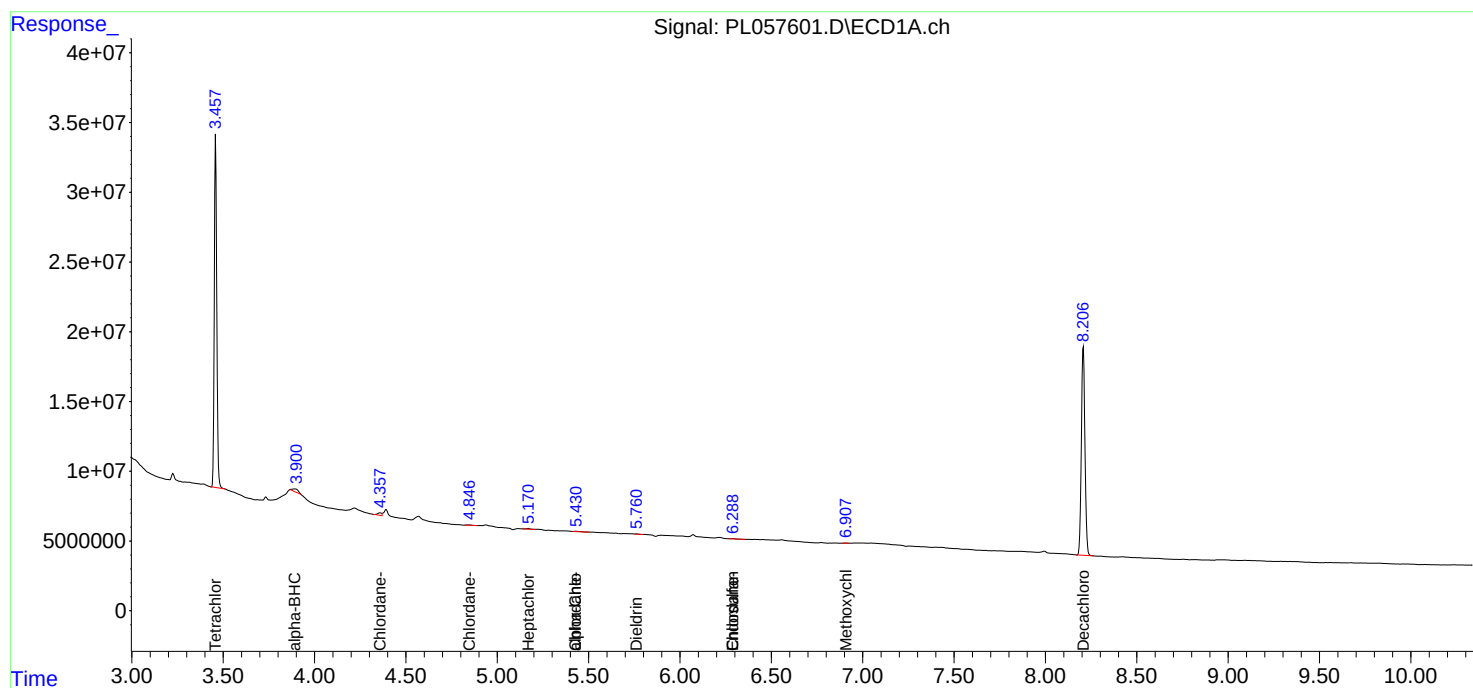


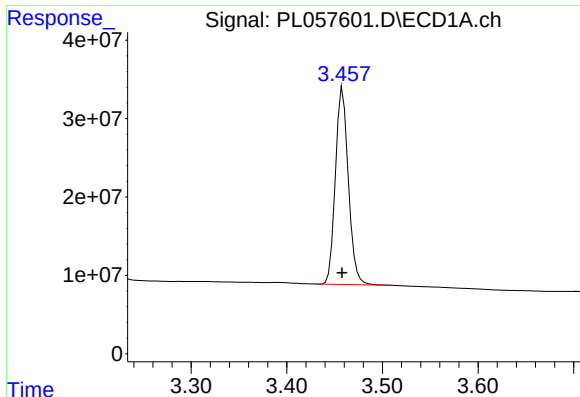

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 235867015
Conc: 25.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

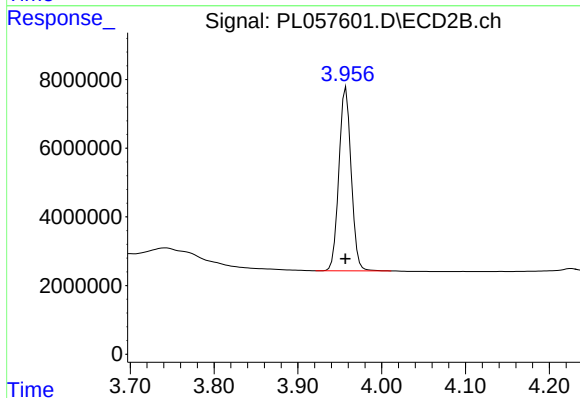


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 54174217
Conc: 24.97 ng/ml

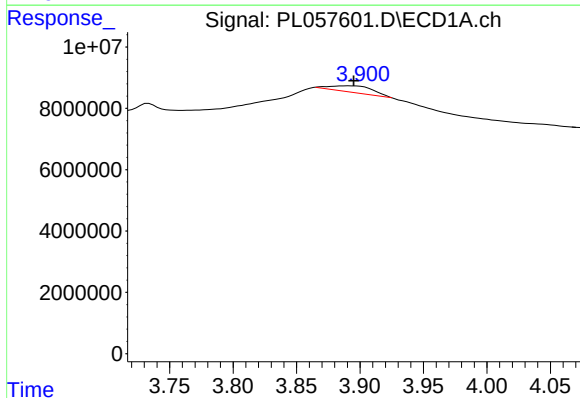


#2 alpha-BHC

R.T.: 3.891 min
Delta R.T.: -0.004 min
Response: 4538382
Conc: 0.28 ng/ml

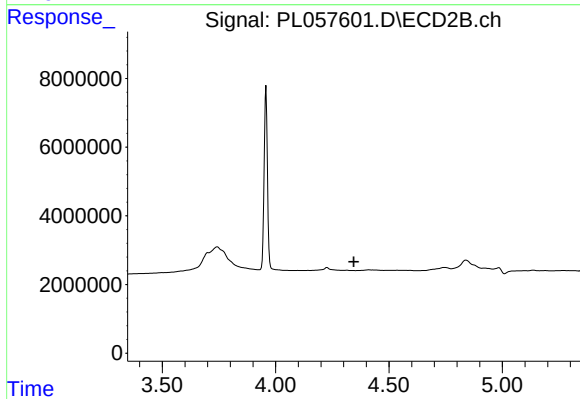

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

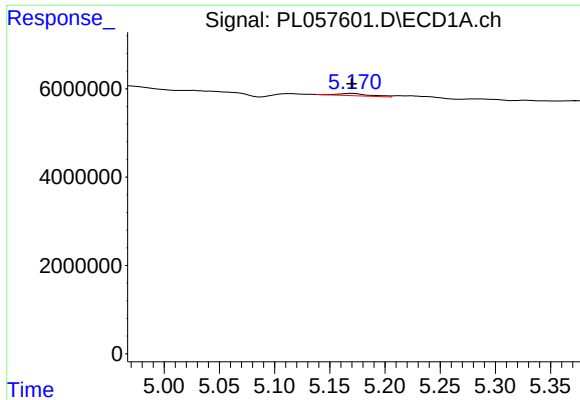

#8 Heptachlor epoxide


R.T.: 5.170 min
Delta R.T.: 0.000 min
Response: 989919
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

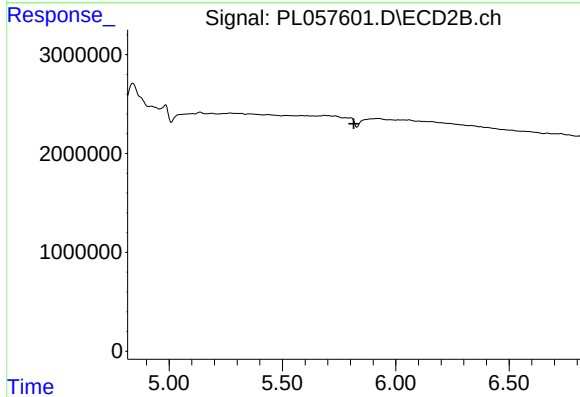


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.815 min
Response: 0
Conc: N.D.

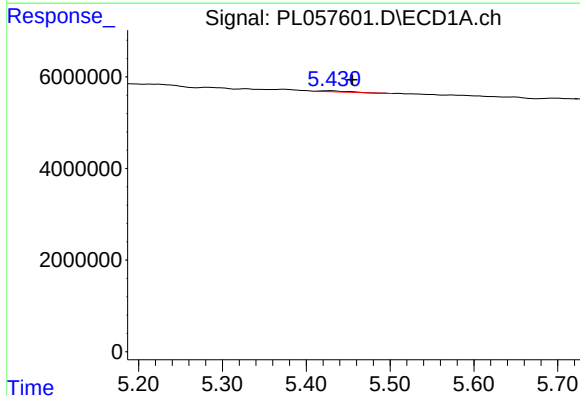


#11 alpha-Chlordane

R.T.: 5.430 min
Delta R.T.: -0.025 min
Response: 432188
Conc: 0.03 ng/ml

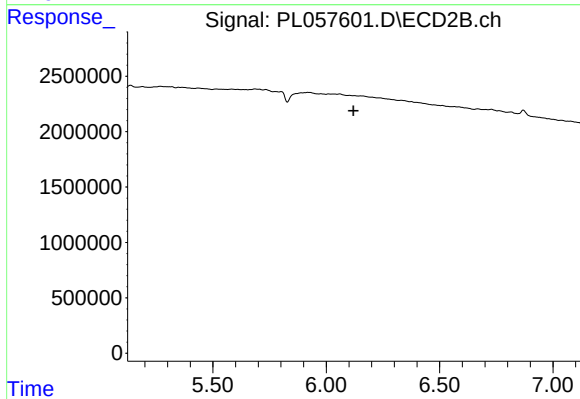

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.120 min
Response: 0
Conc: N.D.

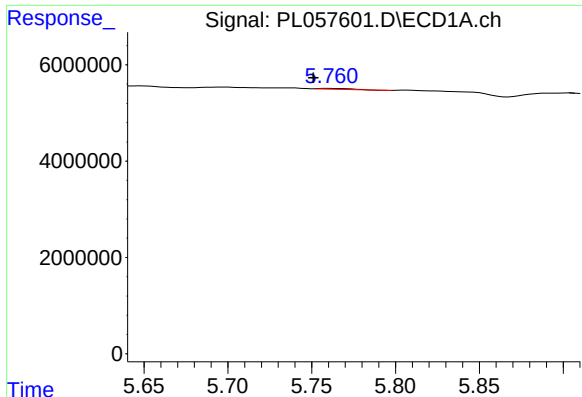

#13 Dieldrin


R.T.: 5.760 min
Delta R.T.: 0.009 min
Response: 248787
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

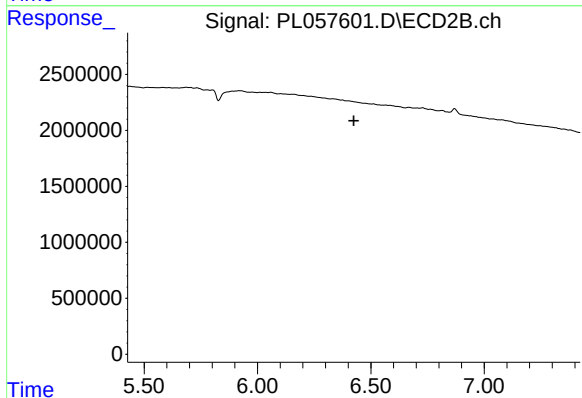


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.425 min
Response: 0
Conc: N.D.

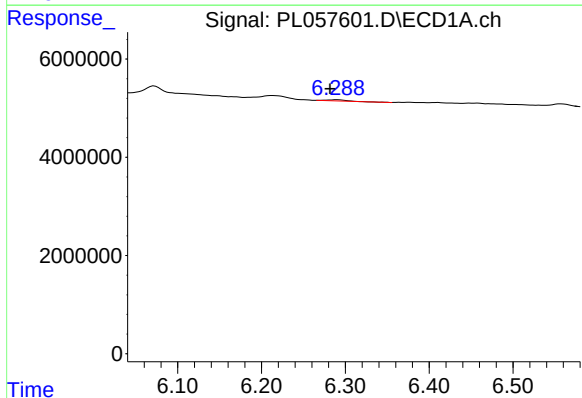


#15 Endosulfan II

R.T.: 6.290 min
Delta R.T.: 0.008 min
Response: 394239
Conc: 0.04 ng/ml

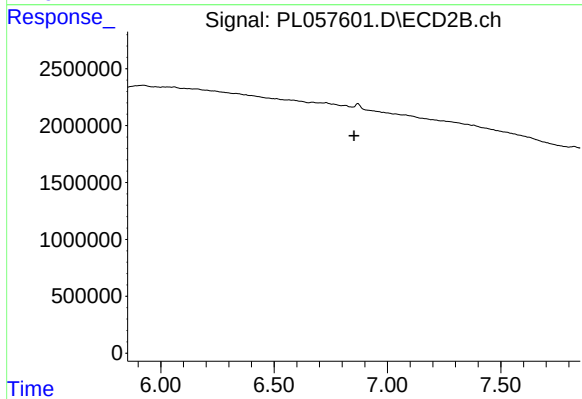

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.852 min
Response: 0
Conc: N.D.

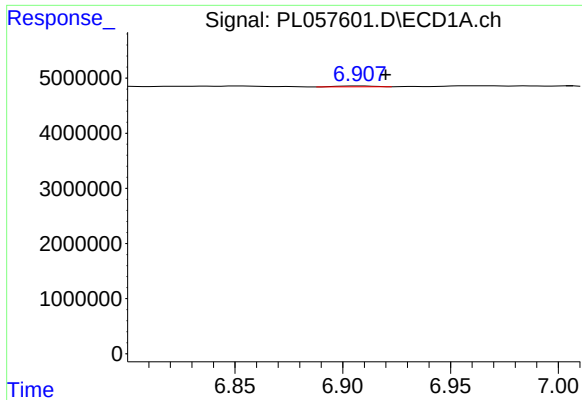

#20 Methoxychlor


R.T.: 6.908 min
Delta R.T.: -0.012 min
Response: 165929
Conc: 0.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

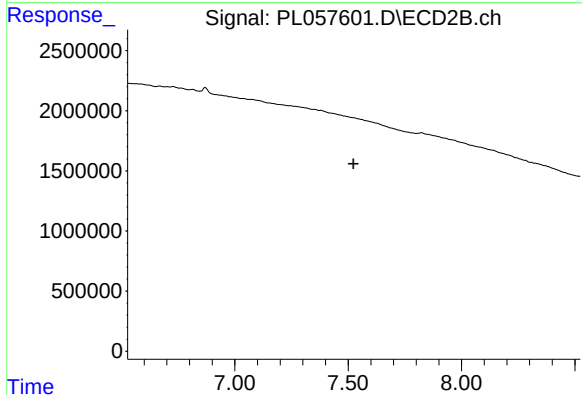


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.524 min
Response: 0
Conc: N.D.

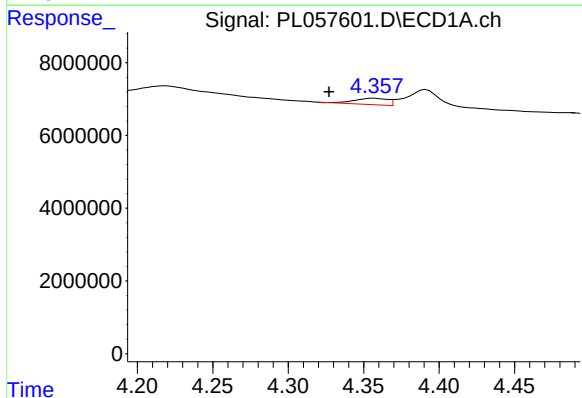


#23 Chlordane-1

R.T.: 4.357 min
Delta R.T.: 0.030 min
Response: 2736574
Conc: 8.43 ng/ml

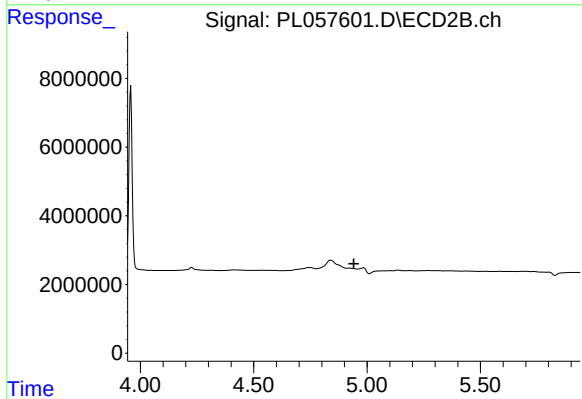

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

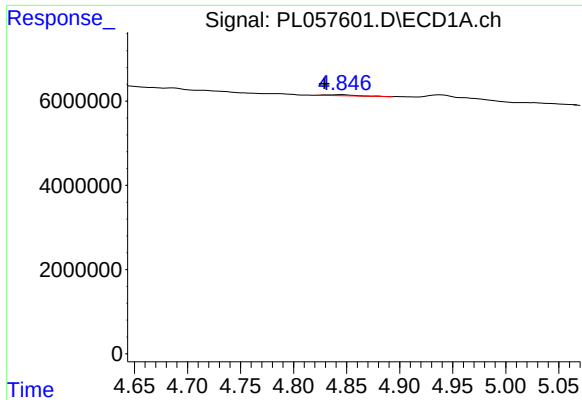

#24 Chlordane-2


R.T.: 4.847 min
Delta R.T.: 0.018 min
Response: 420359
Conc: 1.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

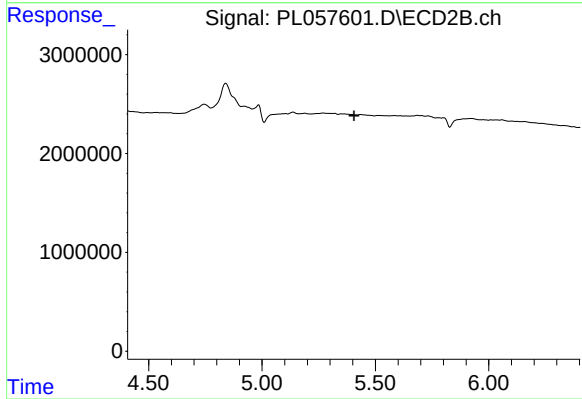


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.406 min
Response: 0
Conc: N.D.

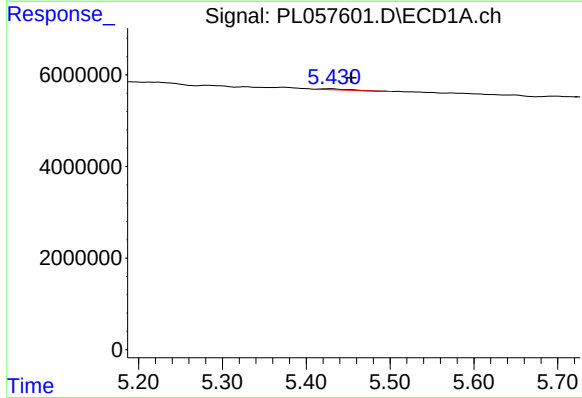


#26 Chlordane-4

R.T.: 5.430 min
Delta R.T.: -0.024 min
Response: 432188
Conc: 0.45 ng/ml

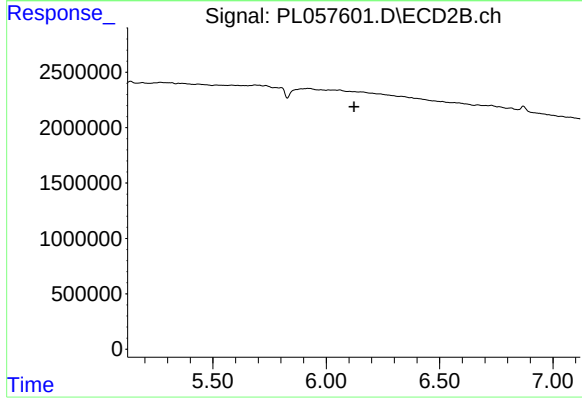

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.122 min
Response: 0
Conc: N.D.

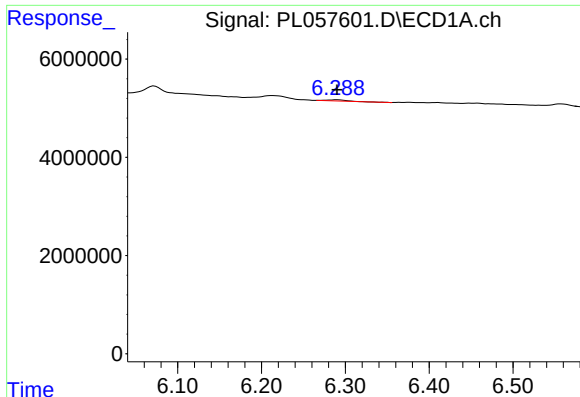

#27 Chlordane-5


R.T.: 6.290 min
Delta R.T.: 0.000 min
Response: 394239
Conc: 1.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

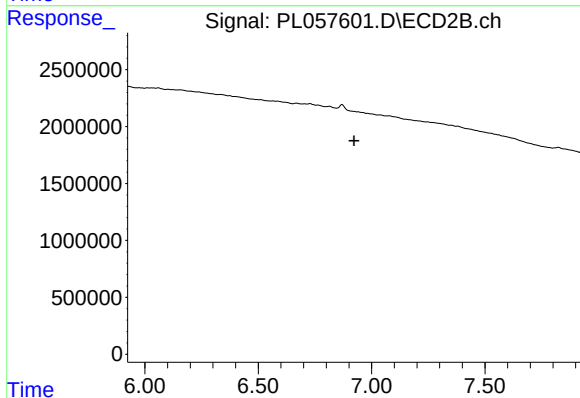


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.922 min
Response: 0
Conc: N.D.

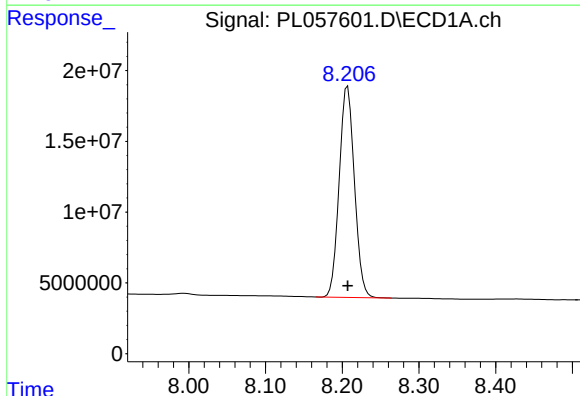

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 205692098
Conc: 19.44 ng/ml

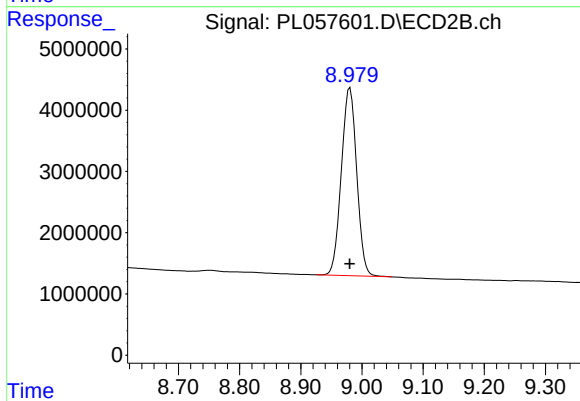

#28 Decachlorobiphenyl

R.T.: 8.980 min
Delta R.T.: 0.000 min
Response: 53630976
Conc: 24.19 ng/ml