

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032620\
 Data File : PL057616.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 01:15
 Operator : AJ\MA
 Sample : L1753-16MSD
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-032520MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 03:36:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	3.957	217.0E6	50793183	23.406	23.412
28)	SA Decachlor...	8.207	8.980	171.4E6	39673048	16.198	17.892
Target Compounds							
4)	MA Heptachlor	0.000	5.141	0	14234305	N.D.	4.522 #
16)	A 4,4'-DDD	6.137	0.000	651187	0	0.066	N.D. #
22)	Mirex	7.344	0.000	231446	0	0.029	N.D. #
23)	Chlordane-1	4.352f	0.000	1691076	0	5.210	N.D. #
24)	Chlordane-2	4.851f	0.000	1666894	0	4.587	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032620\
Data File : PL057616.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 01:15
Operator : AJ\MA
Sample : L1753-16MSD
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CL-02-032520MSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 03:36:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

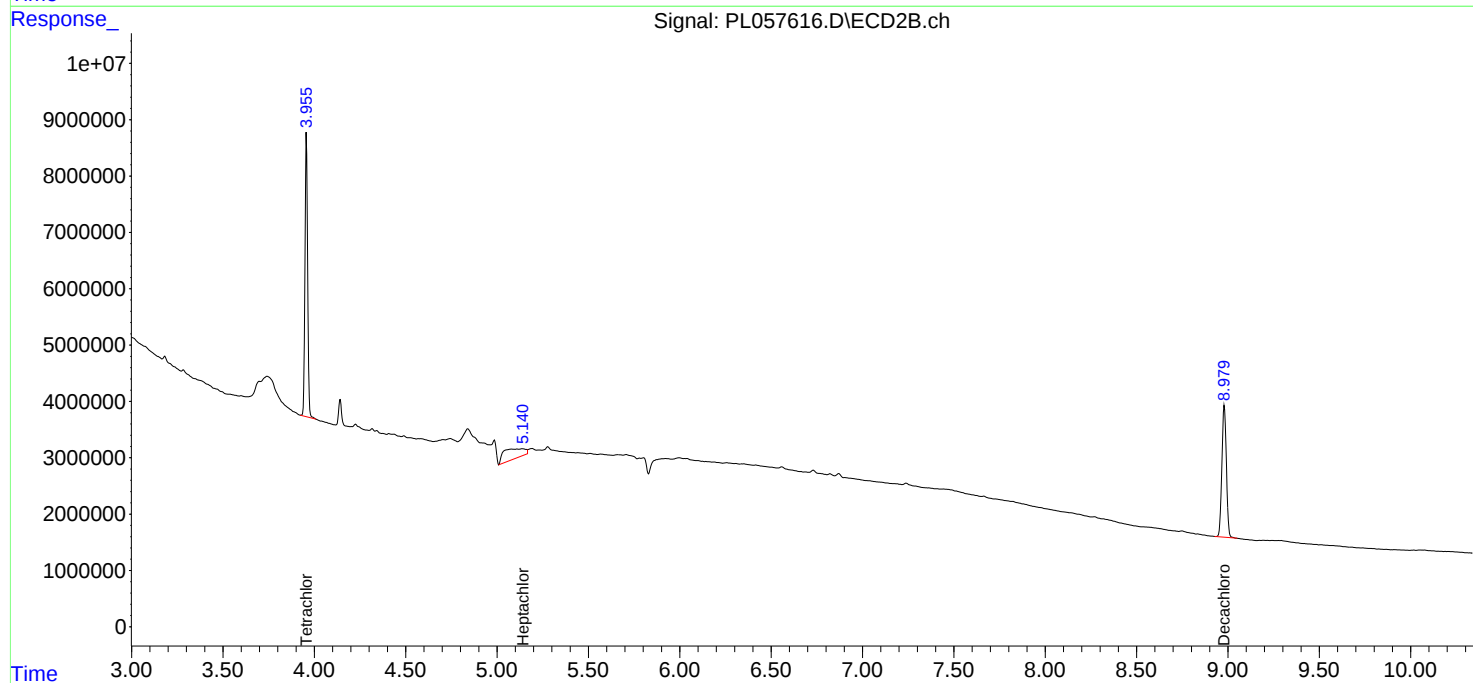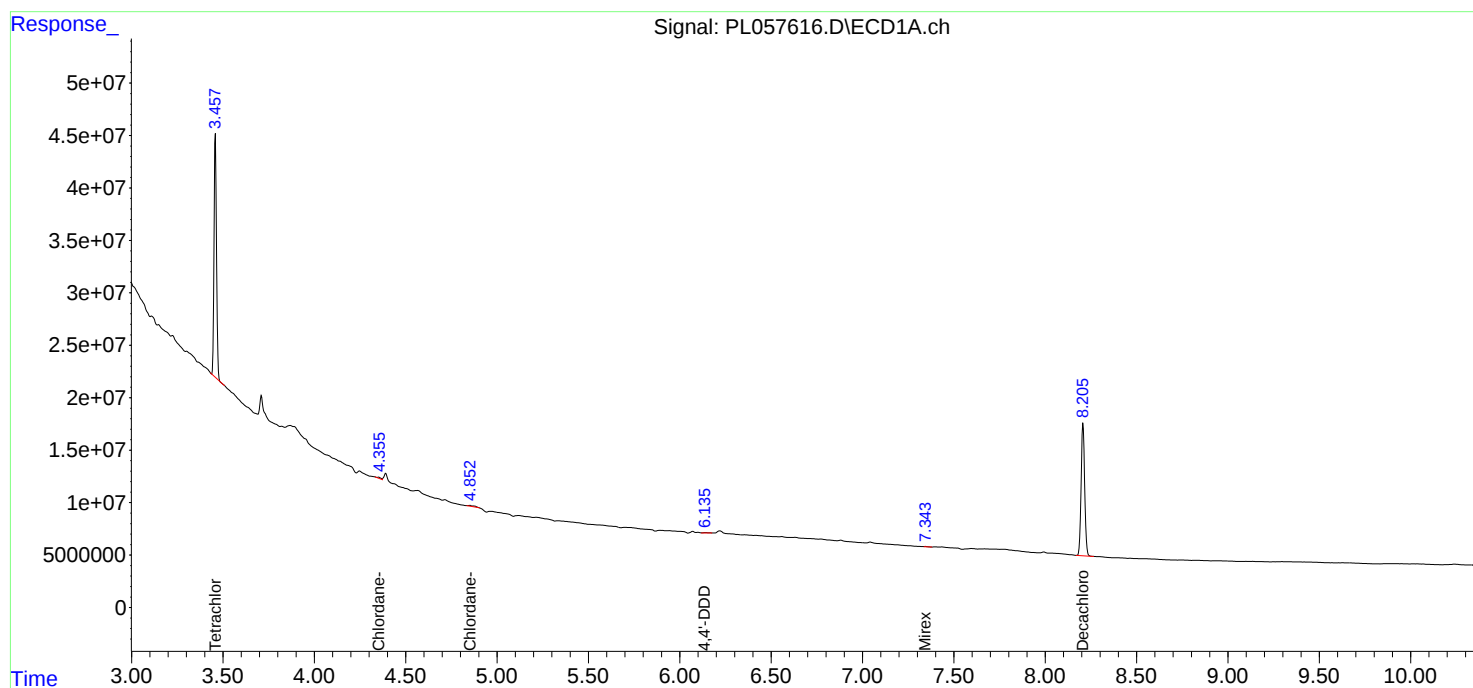


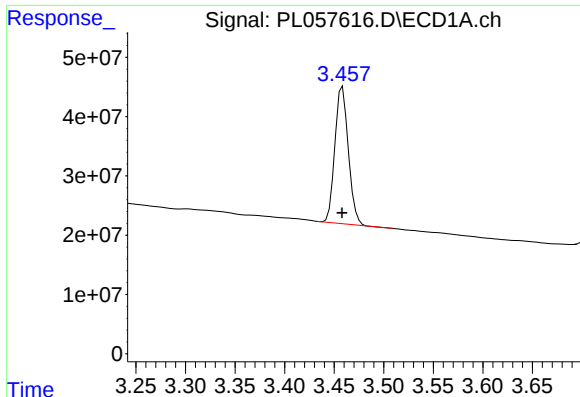

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 216962043
Conc: 23.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-032520MSD

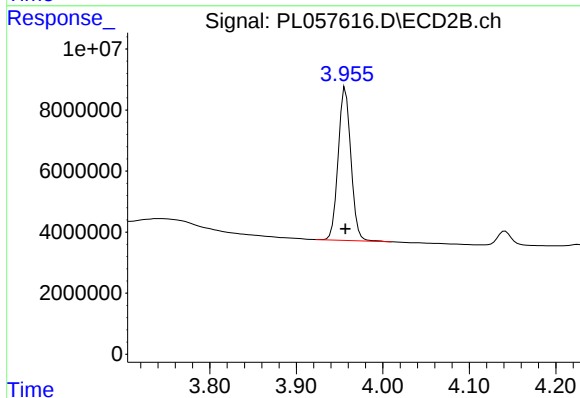


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 50793183
Conc: 23.41 ng/ml

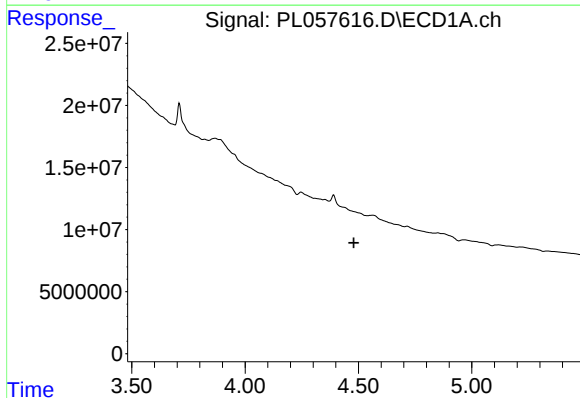


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

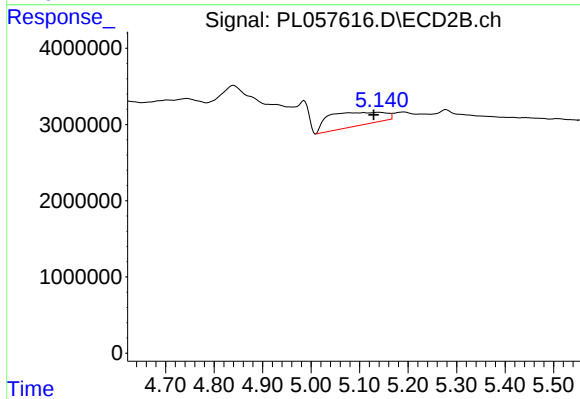

#4 Heptachlor


R.T.: 5.141 min
Delta R.T.: 0.012 min
Response: 14234305
Conc: 4.52 ng/ml

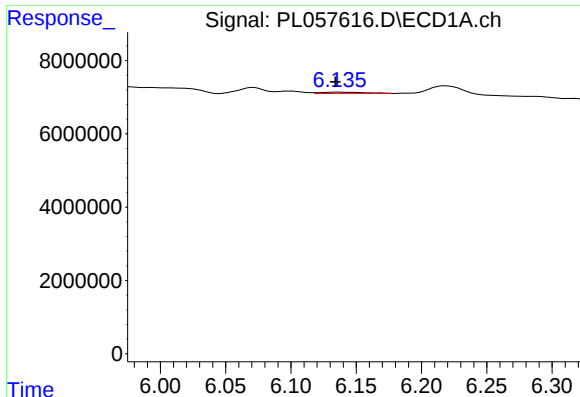

#16 4,4'-DDD


R.T.: 6.137 min
Delta R.T.: 0.003 min
Response: 651187
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-032520MSD

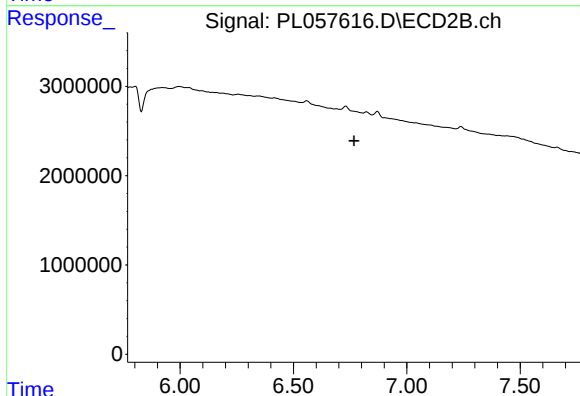


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.768 min
Response: 0
Conc: N.D.

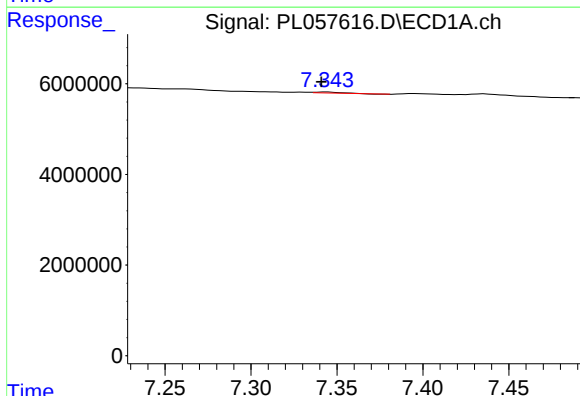


#22 Mirex

R.T.: 7.344 min
Delta R.T.: 0.003 min
Response: 231446
Conc: 0.03 ng/ml

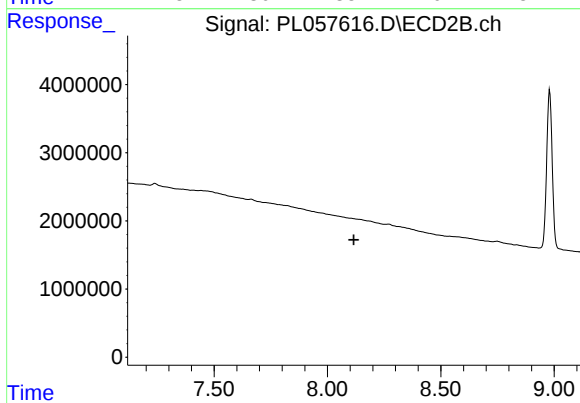

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

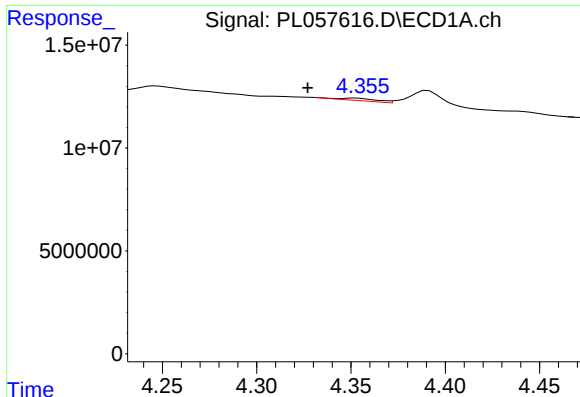

#23 Chlordane-1


R.T.: 4.352 min
Delta R.T.: 0.025 min
Response: 1691076
Conc: 5.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-032520MSD

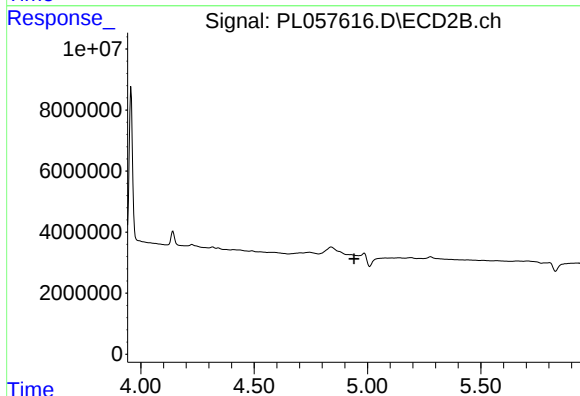


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

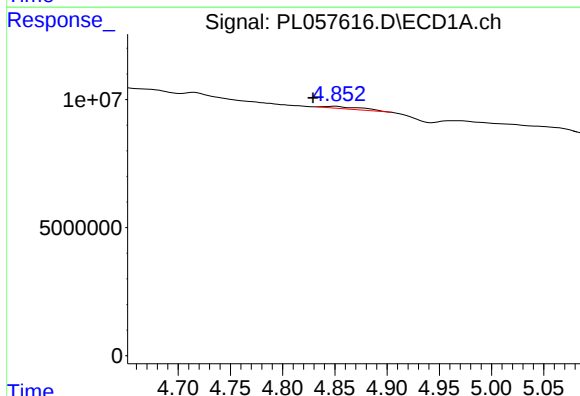


#24 Chlordane-2

R.T.: 4.851 min
Delta R.T.: 0.022 min
Response: 1666894
Conc: 4.59 ng/ml

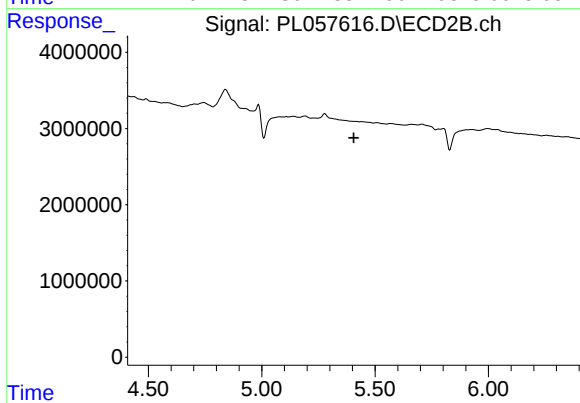

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.406 min
Response: 0
Conc: N.D.

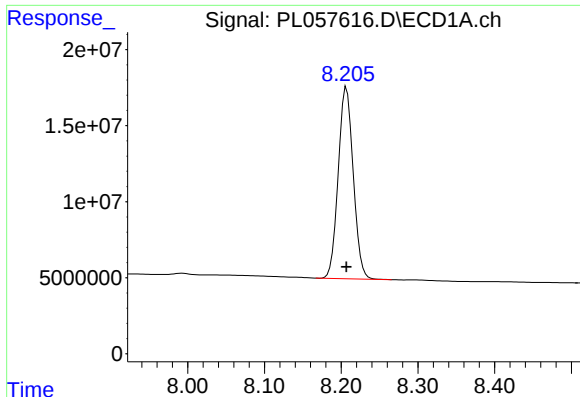

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 171399592
Conc: 16.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-032520MSD

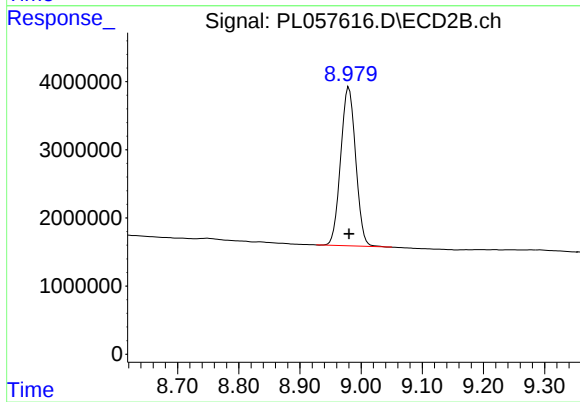

#28 Decachlorobiphenyl

R.T.: 8.980 min
Delta R.T.: 0.000 min
Response: 39673048
Conc: 17.89 ng/ml