

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032620\
 Data File : PL057631.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 05:16
 Operator : AJ\MA
 Sample : L2043-06
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 07:00:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.958	127.9E6	29976516	13.793	13.817
2)	SA Decachlor...	8.207	8.981	157.3E6	35581498	14.869	16.047
Target Compounds							
2)	A alpha-BHC	3.890	0.000	4451745	0	0.279	N.D. #
4)	MA Heptachlor	0.000	5.137	0	3898269	N.D.	1.238 #
8)	B Heptachlo...	5.148f	0.000	930674	0	0.073	N.D. #
9)	A Endosulfan I	5.498	0.000	798023	0	0.067	N.D. #
11)	B alpha-Chl...	5.452	0.000	369458	0	0.029	N.D. #
12)	B 4,4'-DDE	5.614	0.000	1413805	0	0.114	N.D. #
13)	MA Dieldrin	5.744	0.000	829461	0	0.066	N.D. #
16)	A 4,4'-DDD	6.139	0.000	384121	0	0.039	N.D. #
17)	MA 4,4'-DDT	6.368	0.000	361767	0	0.036	N.D. #
20)	A Methoxychlor	6.902f	0.000	640009	0	0.119	N.D. #
23)	Chlordane-1	4.354f	0.000	2039565	0	6.284	N.D. #
26)	Chlordane-4	5.452	0.000	369458	0	0.385	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032620\
Data File : PL057631.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 05:16
Operator : AJ\MA
Sample : L2043-06
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-1A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 07:00:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

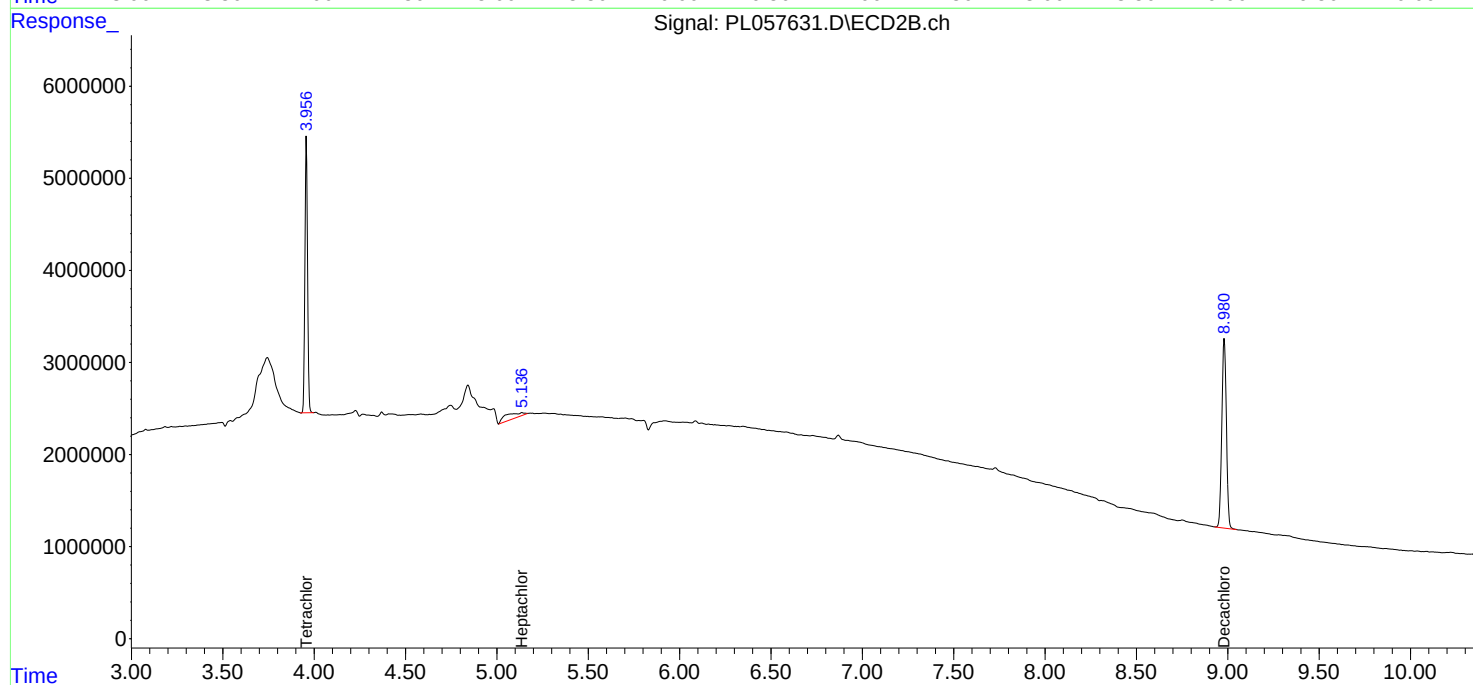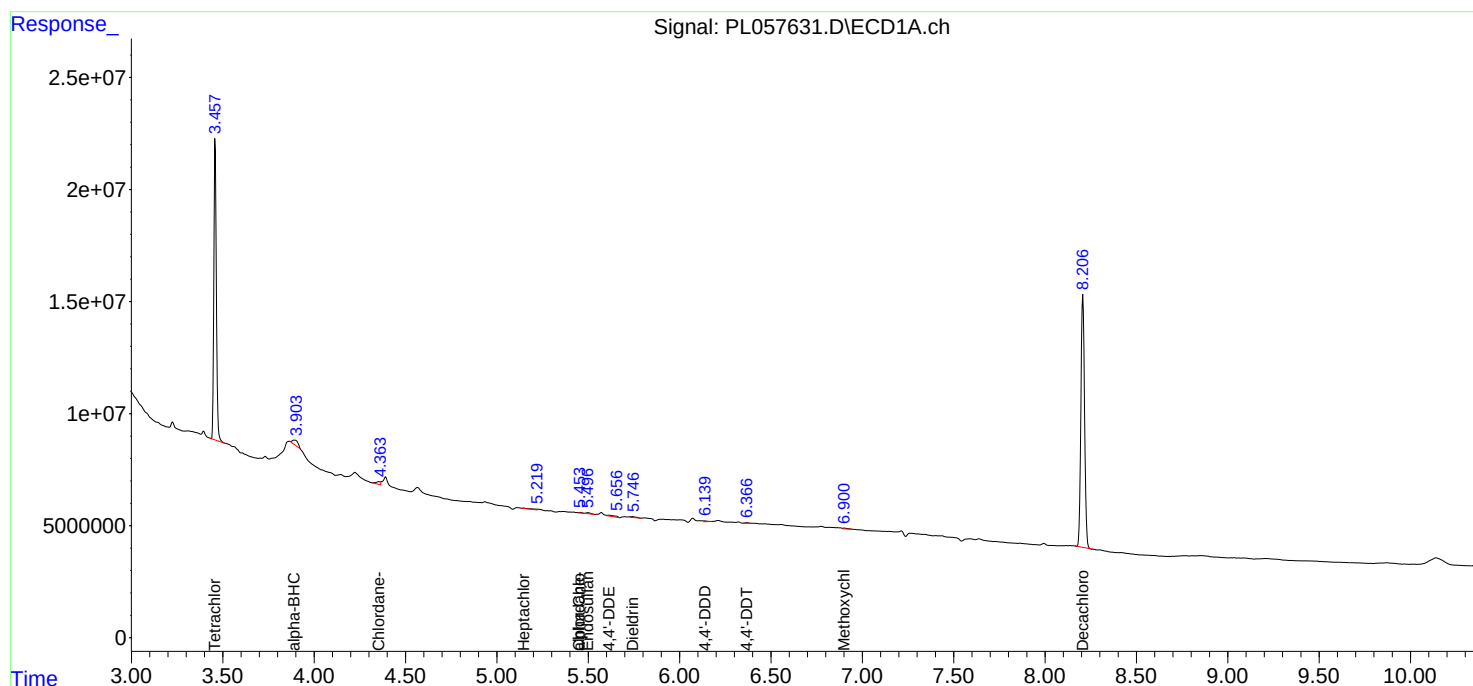


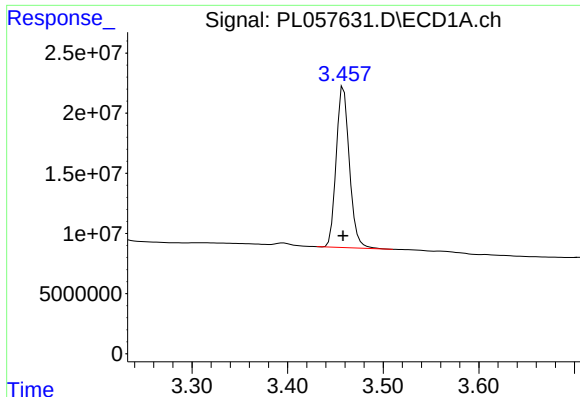

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 127850065
Conc: 13.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1A

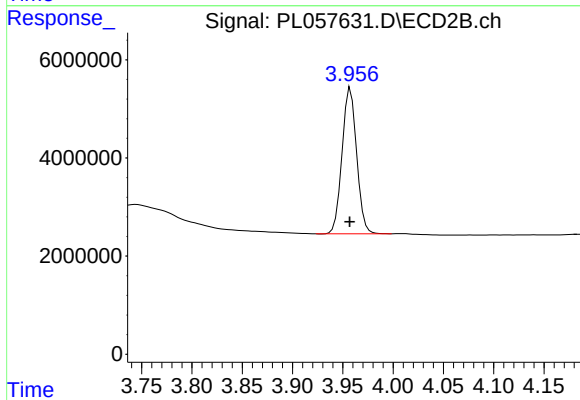


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 29976516
Conc: 13.82 ng/ml

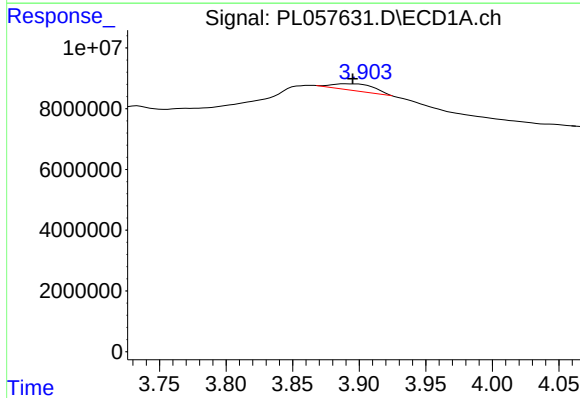


#2 alpha-BHC

R.T.: 3.890 min
Delta R.T.: -0.005 min
Response: 4451745
Conc: 0.28 ng/ml

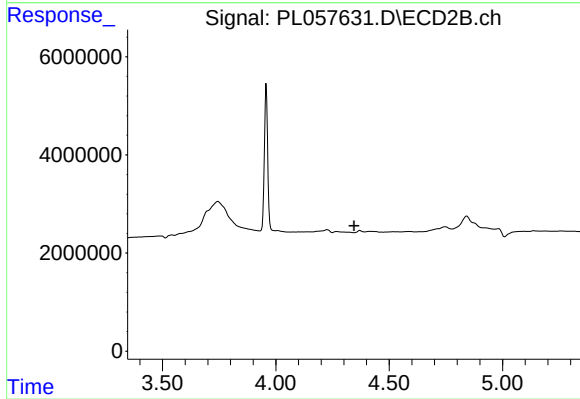

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

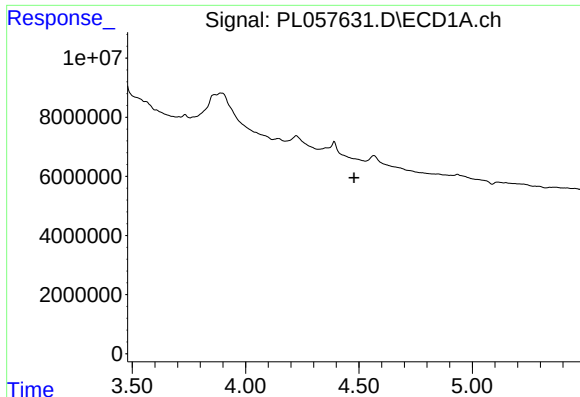

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-1A

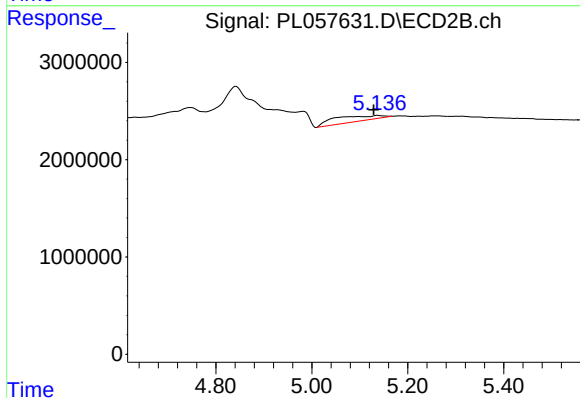


#4 Heptachlor

R.T.: 5.137 min
Delta R.T.: 0.008 min
Response: 3898269
Conc: 1.24 ng/ml

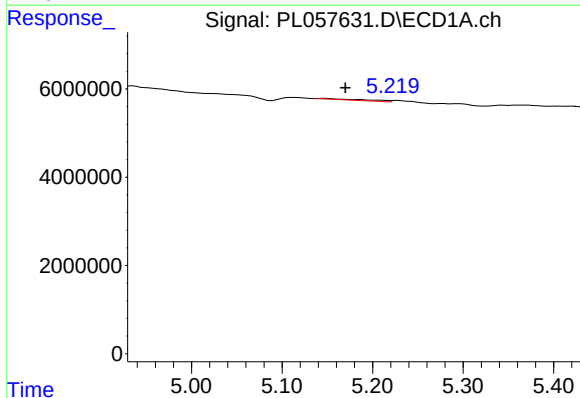


#8 Heptachlor epoxide

R.T.: 5.148 min
Delta R.T.: -0.022 min
Response: 930674
Conc: 0.07 ng/ml

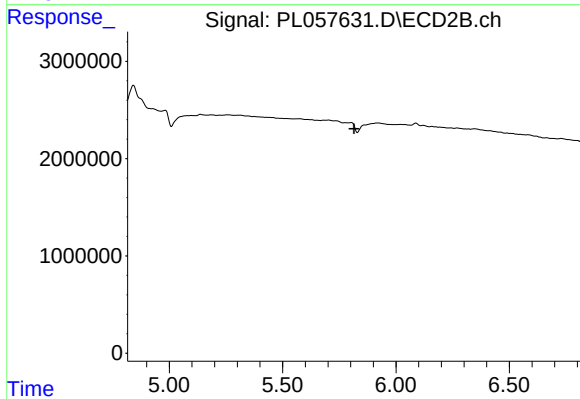

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.815 min
Response: 0
Conc: N.D.

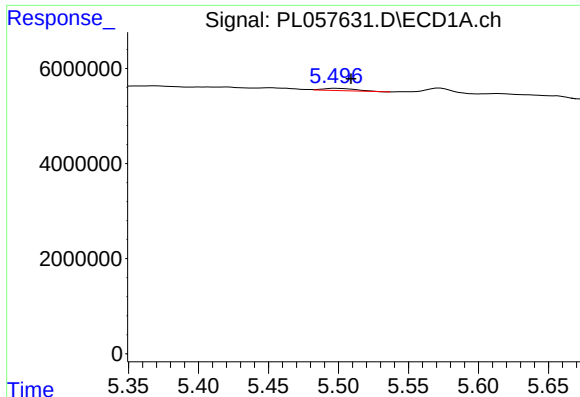

#9 Endosulfan I


R.T.: 5.498 min
Delta R.T.: -0.011 min
Response: 798023
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1A

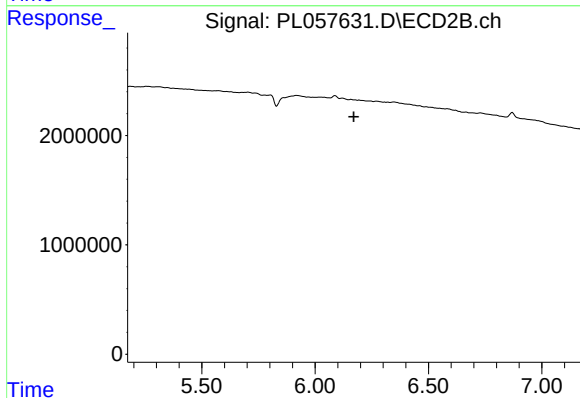


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

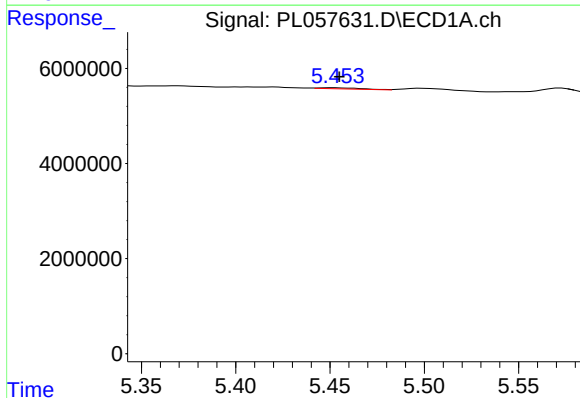


#11 alpha-Chlordane

R.T.: 5.452 min
Delta R.T.: -0.003 min
Response: 369458
Conc: 0.03 ng/ml

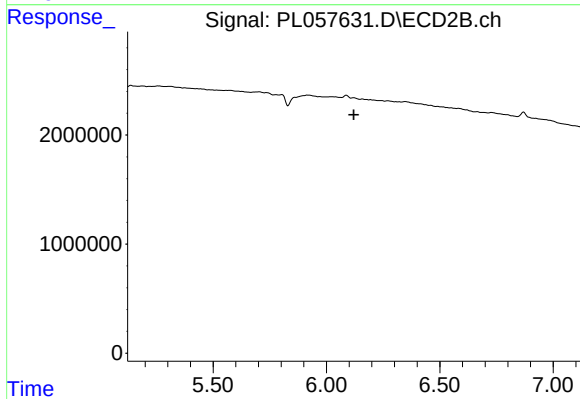

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.120 min
Response: 0
Conc: N.D.

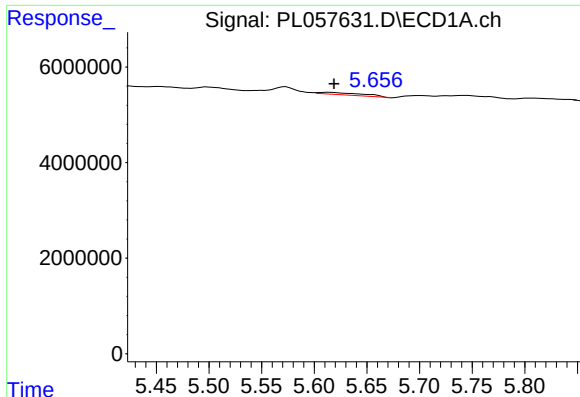

#12 4,4'-DDE


R.T.: 5.614 min
Delta R.T.: -0.005 min
Response: 1413805
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1A

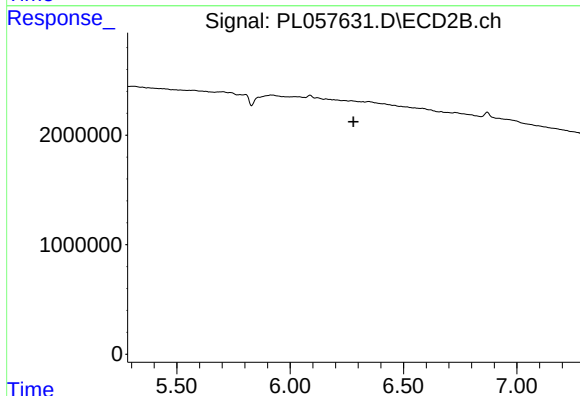


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.280 min
Response: 0
Conc: N.D.

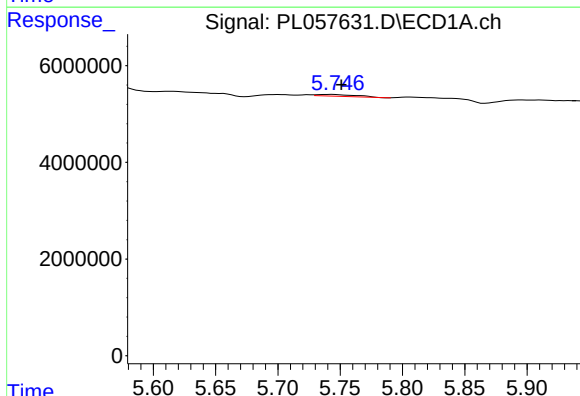


#13 Dieldrin

R.T.: 5.744 min
Delta R.T.: -0.007 min
Response: 829461
Conc: 0.07 ng/ml

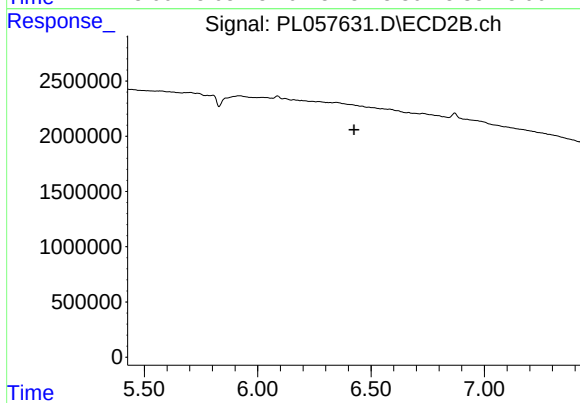

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.425 min
Response: 0
Conc: N.D.

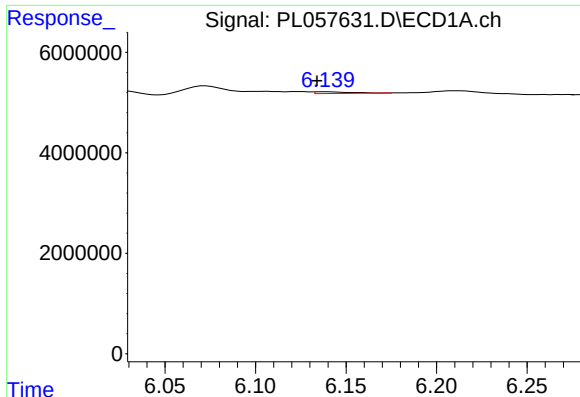

#16 4,4'-DDD


R.T.: 6.139 min
Delta R.T.: 0.005 min
Response: 384121
Conc: 0.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1A

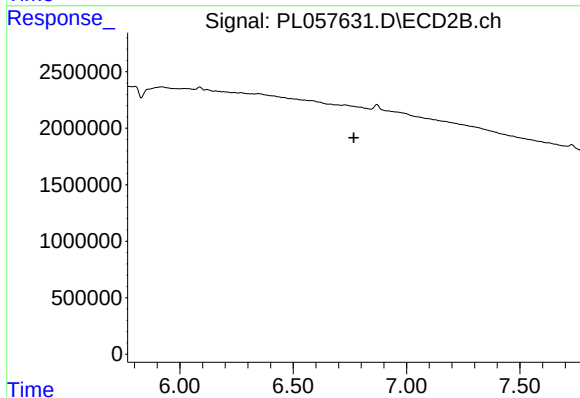


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.768 min
Response: 0
Conc: N.D.

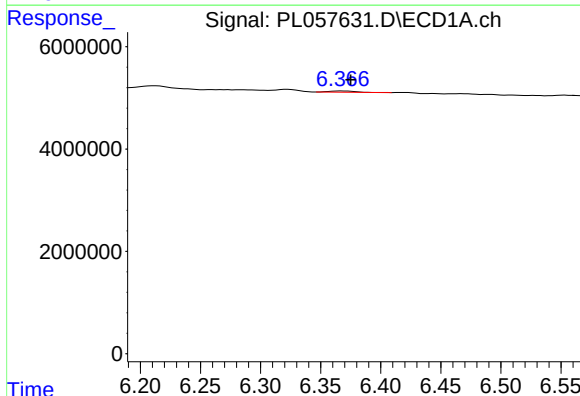


#17 4,4'-DDT

R.T.: 6.368 min
Delta R.T.: -0.007 min
Response: 361767
Conc: 0.04 ng/ml

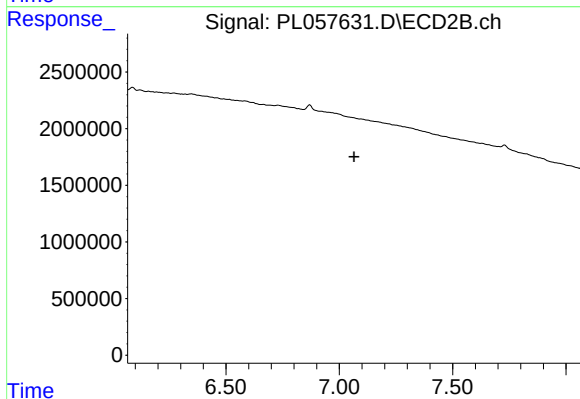

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.065 min
Response: 0
Conc: N.D.

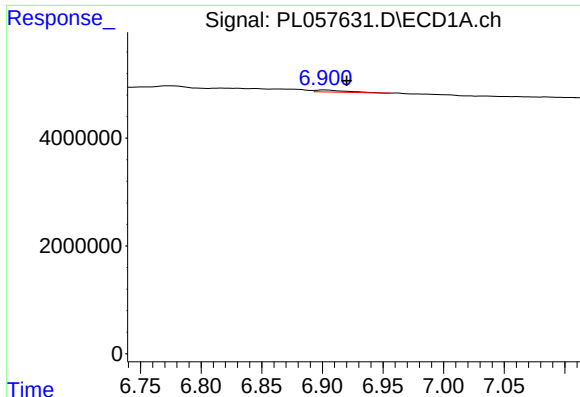

#20 Methoxychlor


R.T.: 6.902 min
Delta R.T.: -0.018 min
Response: 640009
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1A

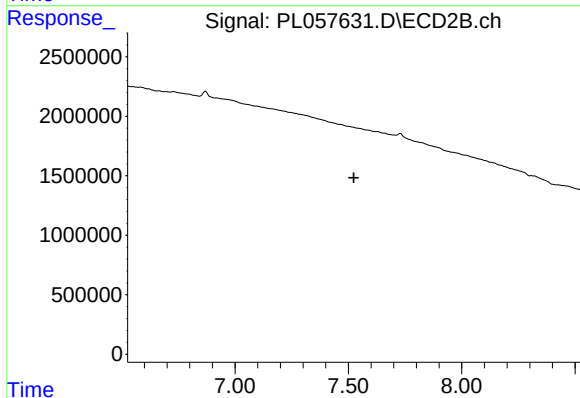


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.524 min
Response: 0
Conc: N.D.

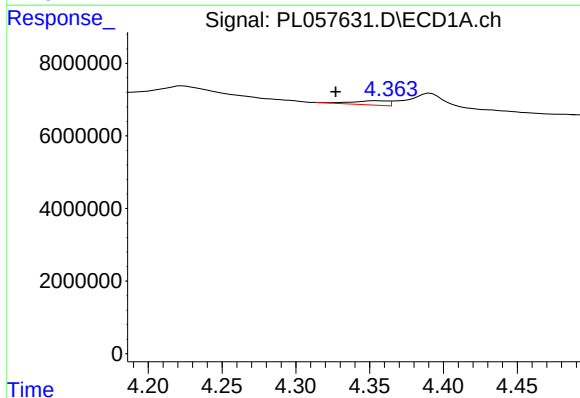


#23 Chlordane-1

R.T.: 4.354 min
Delta R.T.: 0.027 min
Response: 2039565
Conc: 6.28 ng/ml

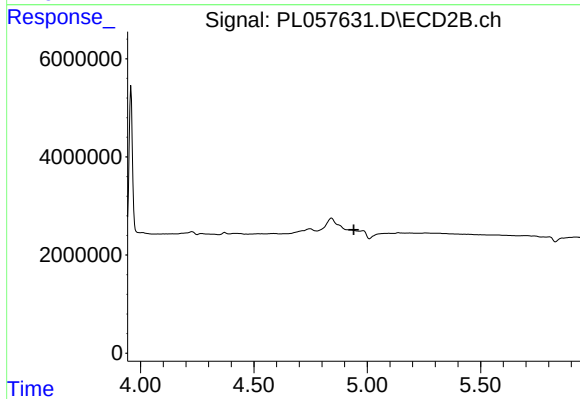

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

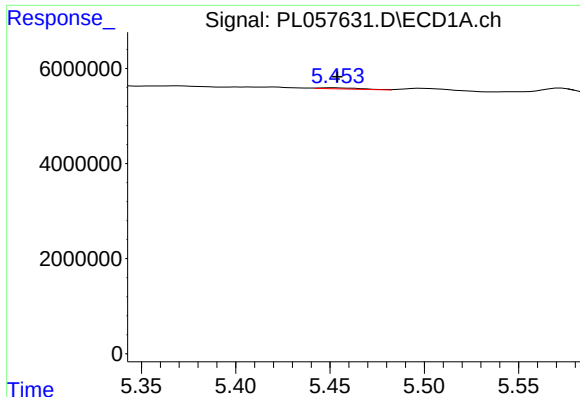

#26 Chlordane-4


R.T.: 5.452 min
Delta R.T.: -0.002 min
Response: 369458
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1A

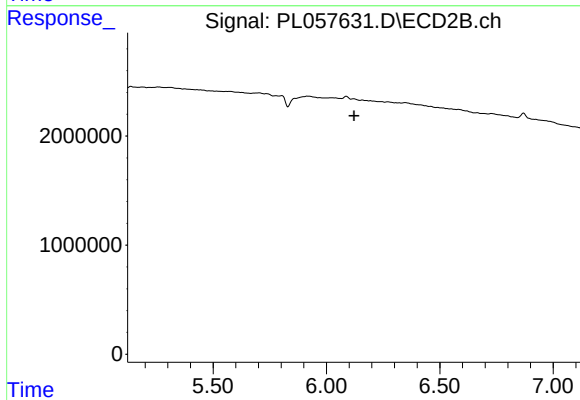


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.122 min
Response: 0
Conc: N.D.

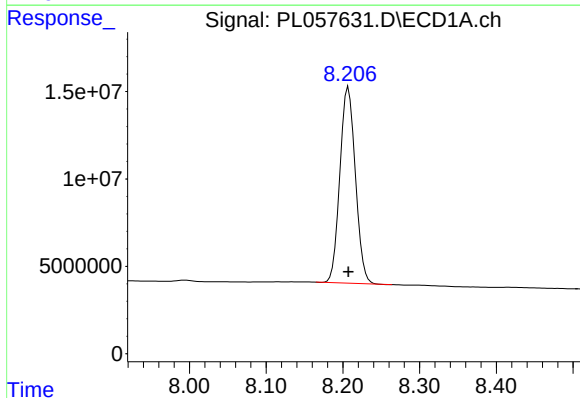

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 157332724
Conc: 14.87 ng/ml

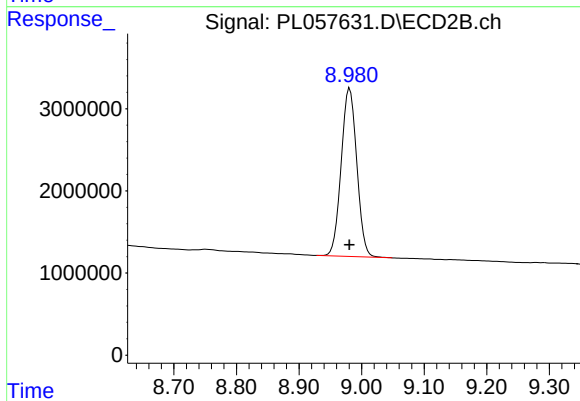

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: 0.000 min
Response: 35581498
Conc: 16.05 ng/ml