

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032620\
 Data File : PL057637.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 06:42
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 07:02:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.957	235.1E6	53179525	25.367	24.512
28)	SA Decachlor...	8.207	8.981	227.4E6	49276937	21.494	22.223
Target Compounds							
2)	A alpha-BHC	3.888	0.000	4538211	0	0.285	N.D. #
3)	MA gamma-BHC...	4.187	0.000	48033	0	0.003	N.D. #
4)	MA Heptachlor	0.000	5.139	0	4221591	N.D.	1.341 #
8)	B Heptachlo...	5.169	0.000	939390	0	0.073	N.D. #
9)	A Endosulfan I	5.488f	0.000	235153	0	0.020	N.D. #
14)	MA Endrin	6.011	0.000	884203	0	0.077	N.D. #
16)	A 4,4'-DDD	6.139	0.000	68759	0	0.007	N.D. #
17)	MA 4,4'-DDT	6.375	0.000	216773	0	0.022	N.D. #
23)	Chlordane-1	4.356f	0.000	3231383	0	9.956	N.D. #
24)	Chlordane-2	4.844	0.000	824005	0	2.268	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032620\
Data File : PL057637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 06:42
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 07:02:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

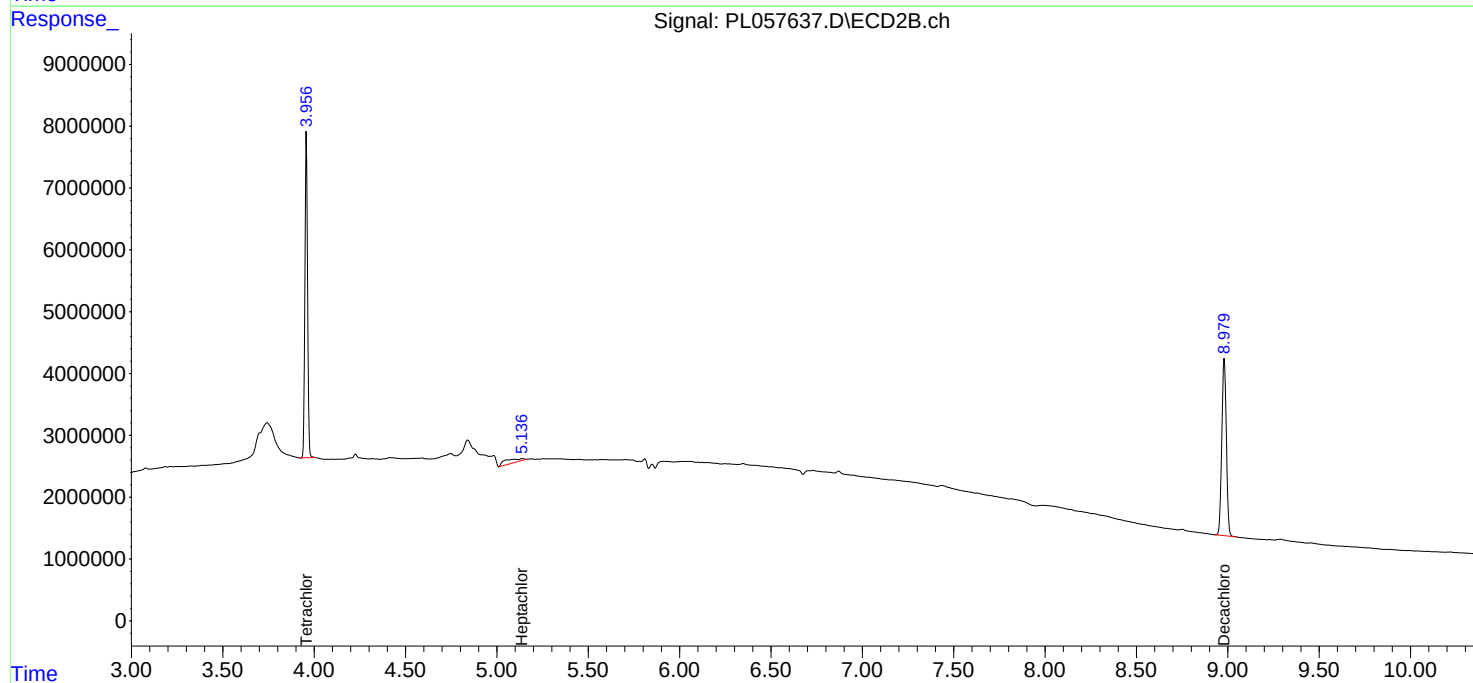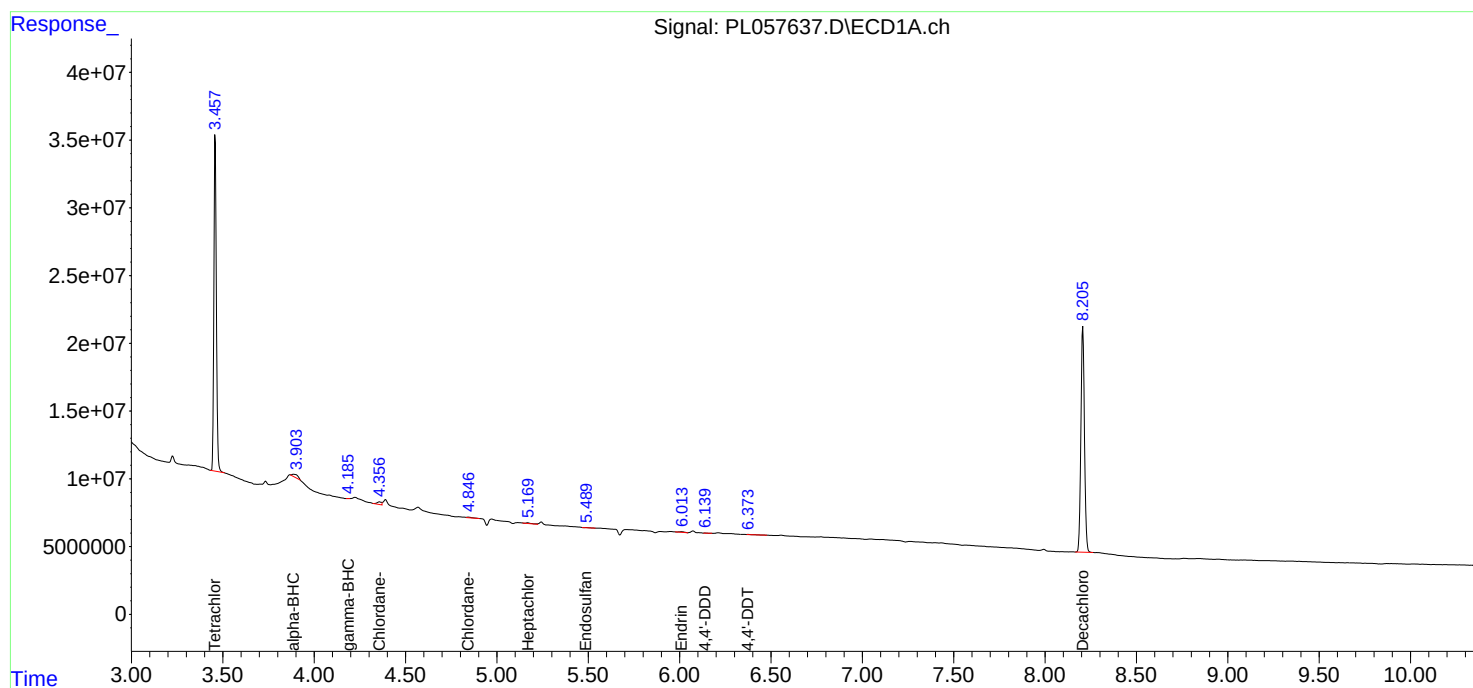


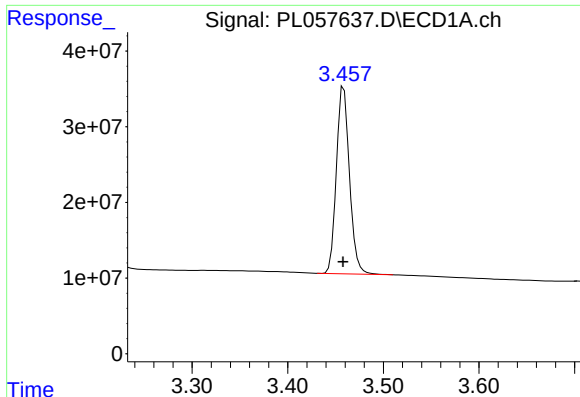

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 235141946
Conc: 25.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

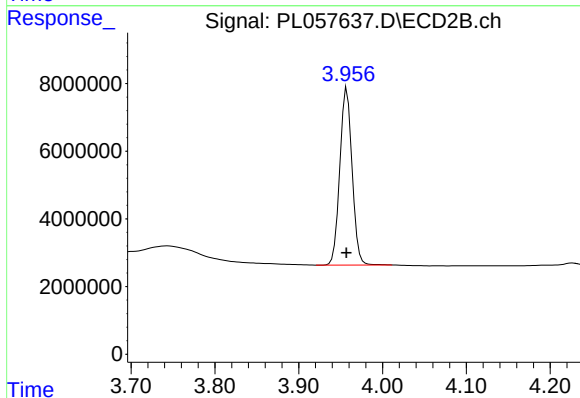


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 53179525
Conc: 24.51 ng/ml

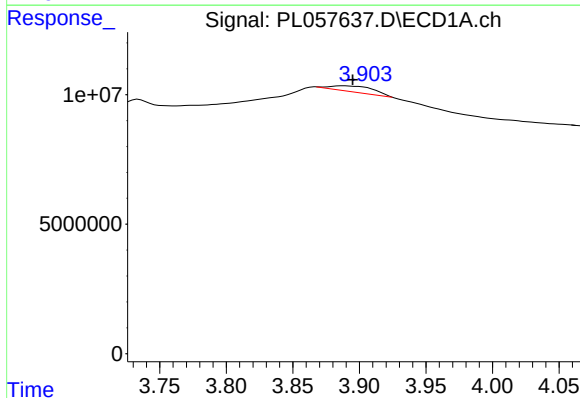


#2 alpha-BHC

R.T.: 3.888 min
Delta R.T.: -0.007 min
Response: 4538211
Conc: 0.28 ng/ml

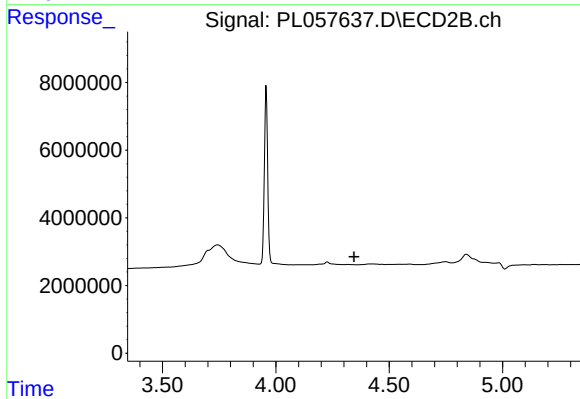

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

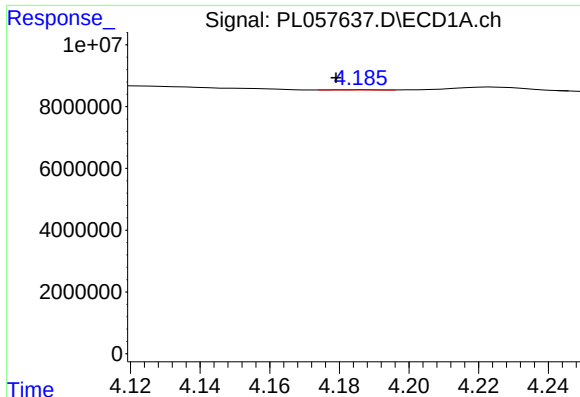

#3 gamma-BHC (Lindane)


R.T.: 4.187 min
Delta R.T.: 0.008 min
Response: 48033
Conc: 0.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

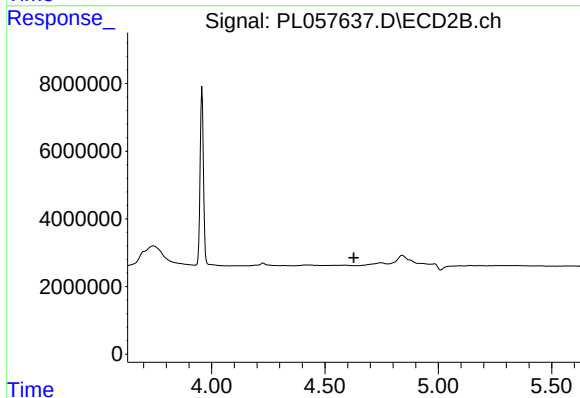


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.627 min
Response: 0
Conc: N.D.

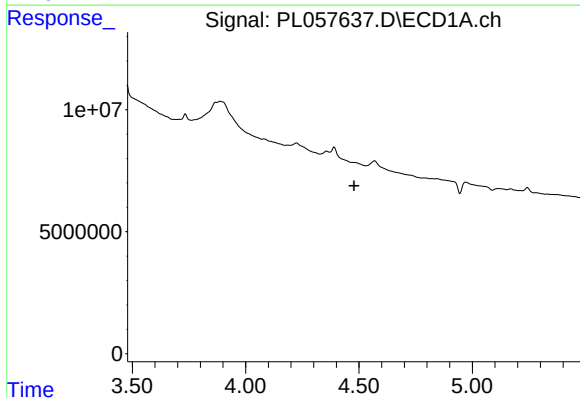


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

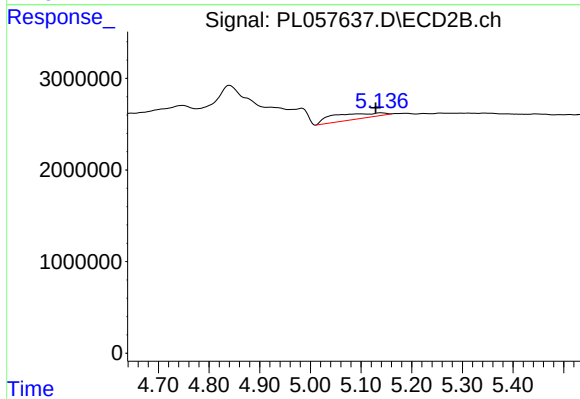

#4 Heptachlor


R.T.: 5.139 min
Delta R.T.: 0.010 min
Response: 4221591
Conc: 1.34 ng/ml

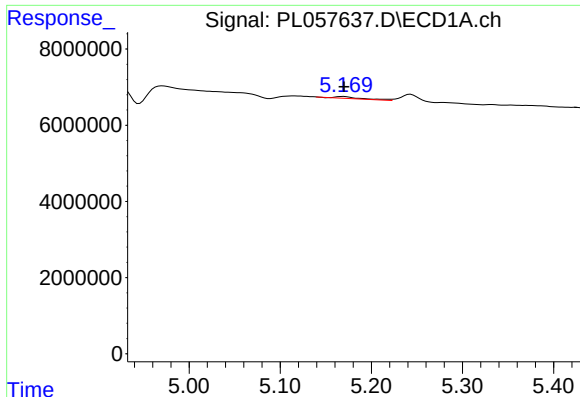

#8 Heptachlor epoxide


R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 939390
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

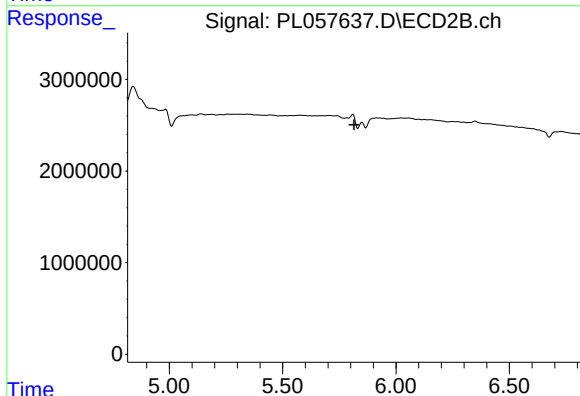


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.815 min
Response: 0
Conc: N.D.

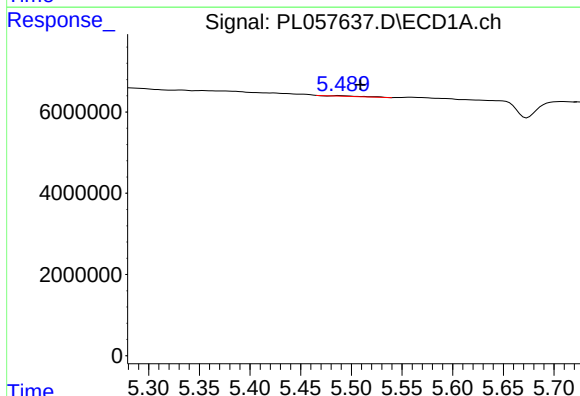


#9 Endosulfan I

R.T.: 5.488 min
Delta R.T.: -0.021 min
Response: 235153
Conc: 0.02 ng/ml

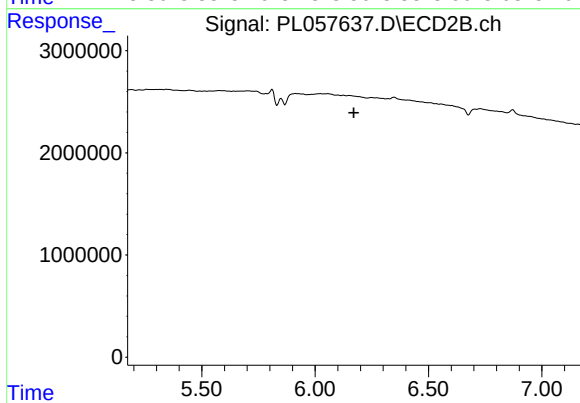

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

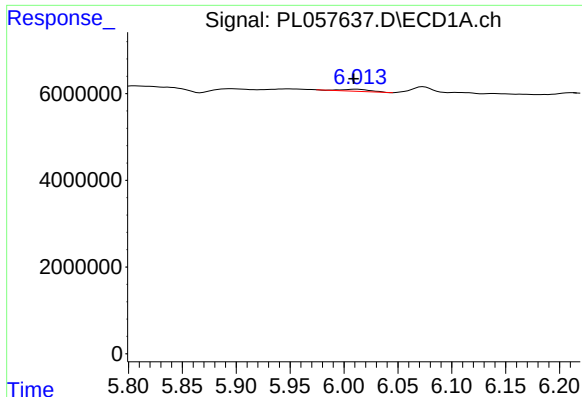

#14 Endrin


R.T.: 6.011 min
Delta R.T.: 0.002 min
Response: 884203
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

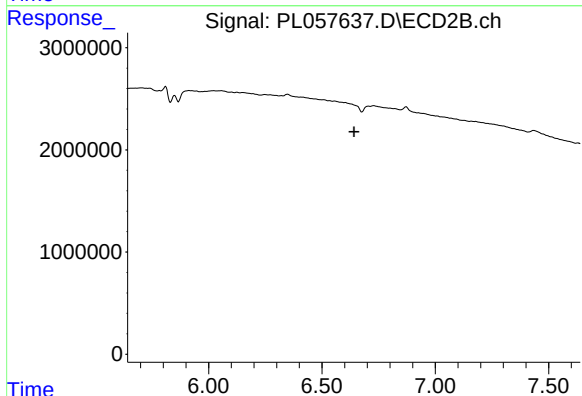


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.642 min
Response: 0
Conc: N.D.

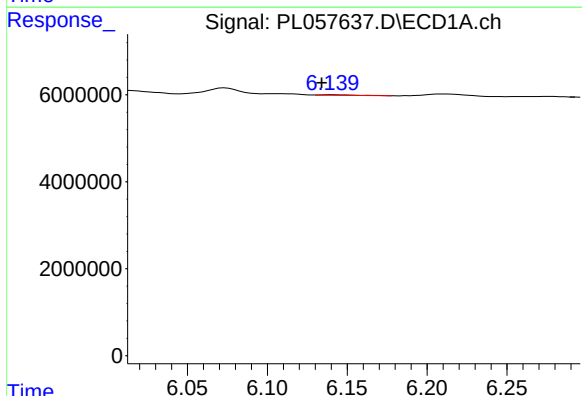


#16 4,4'-DDD

R.T.: 6.139 min
Delta R.T.: 0.005 min
Response: 68759
Conc: 0.01 ng/ml

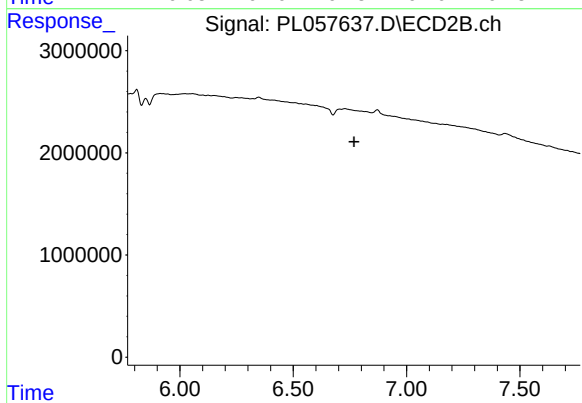

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.768 min
Response: 0
Conc: N.D.

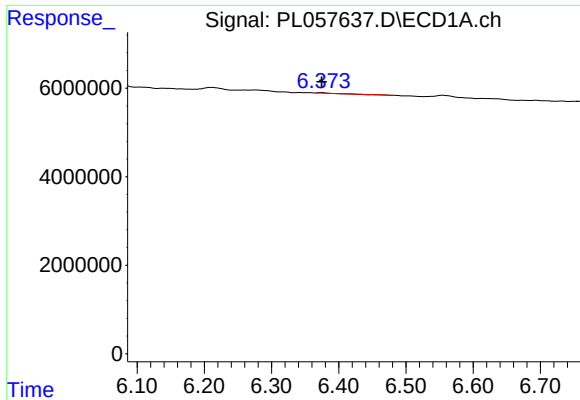

#17 4,4'-DDT


R.T.: 6.375 min
Delta R.T.: 0.000 min
Response: 216773
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

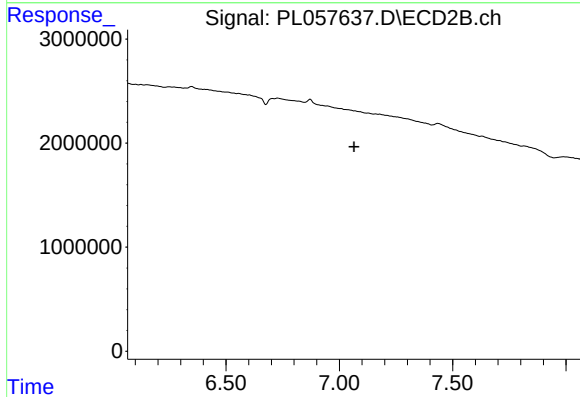


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.065 min
Response: 0
Conc: N.D.

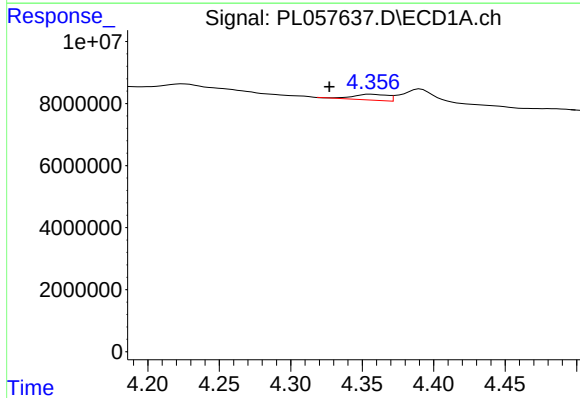


#23 Chlordane-1

R.T.: 4.356 min
Delta R.T.: 0.029 min
Response: 3231383
Conc: 9.96 ng/ml

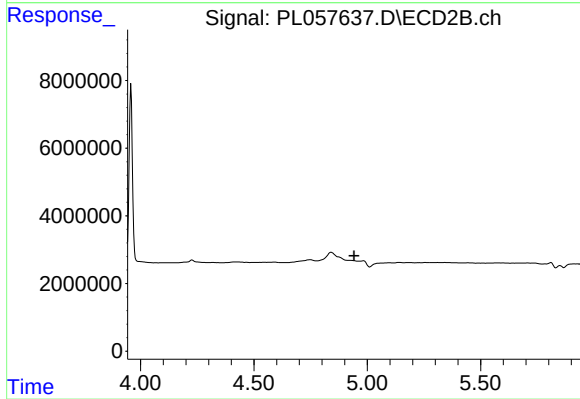

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

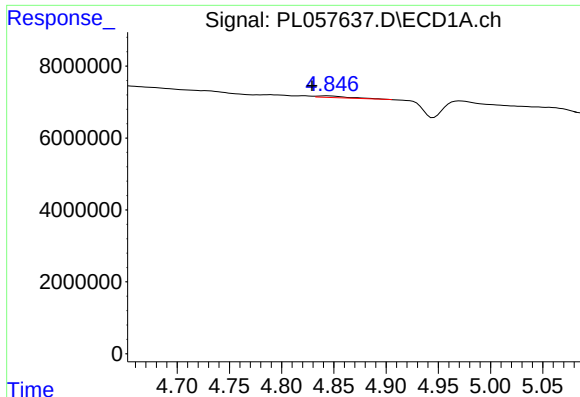

#24 Chlordane-2


R.T.: 4.844 min
Delta R.T.: 0.015 min
Response: 824005
Conc: 2.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

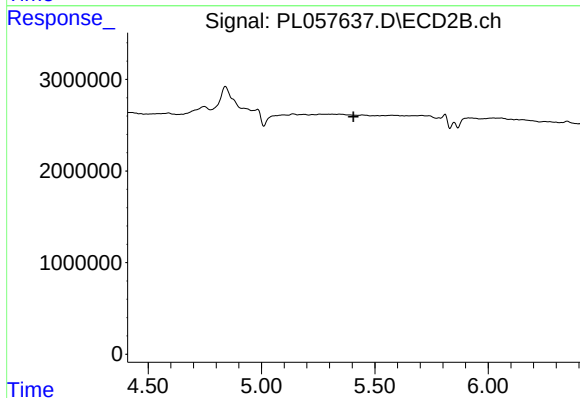


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.406 min
Response: 0
Conc: N.D.

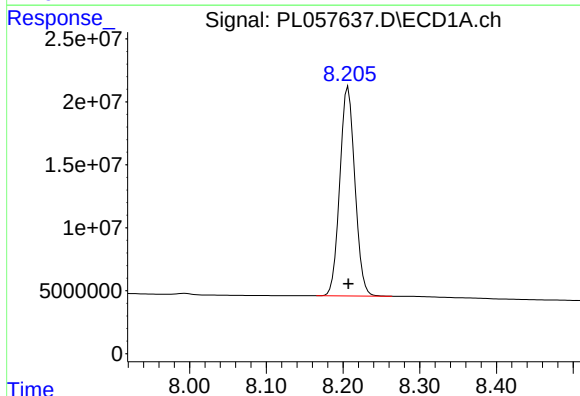

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 227437893
Conc: 21.49 ng/ml

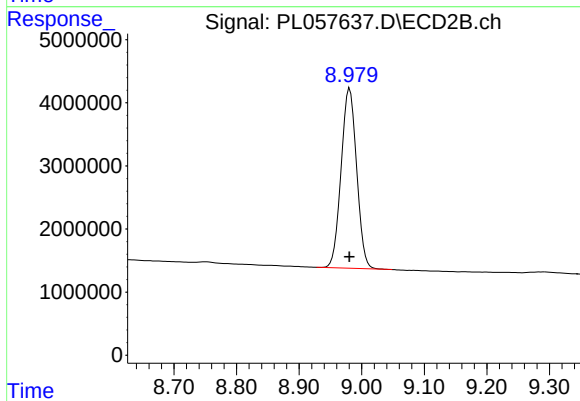

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: 0.000 min
Response: 49276937
Conc: 22.22 ng/ml