

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032620\
 Data File : PL057616.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 01:15
 Operator : AJ\MA
 Sample : L1753-16MSD
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-032520MSD

Manual Integrations
 APPROVED

mohammad
 3/30/2020 10:35:06 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 03:36:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.457	3.957	219.3E6	50793183	23.661m	23.412
28) SA Decachlor...	8.207	8.980	171.4E6	39673048	16.198	17.892

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032620\
Data File : PL057616.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 01:15
Operator : AJ\MA
Sample : L1753-16MSD
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CL-02-032520MSD


Manual Integrations
APPROVED

mohammad
3/30/2020 10:35:06 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 03:36:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

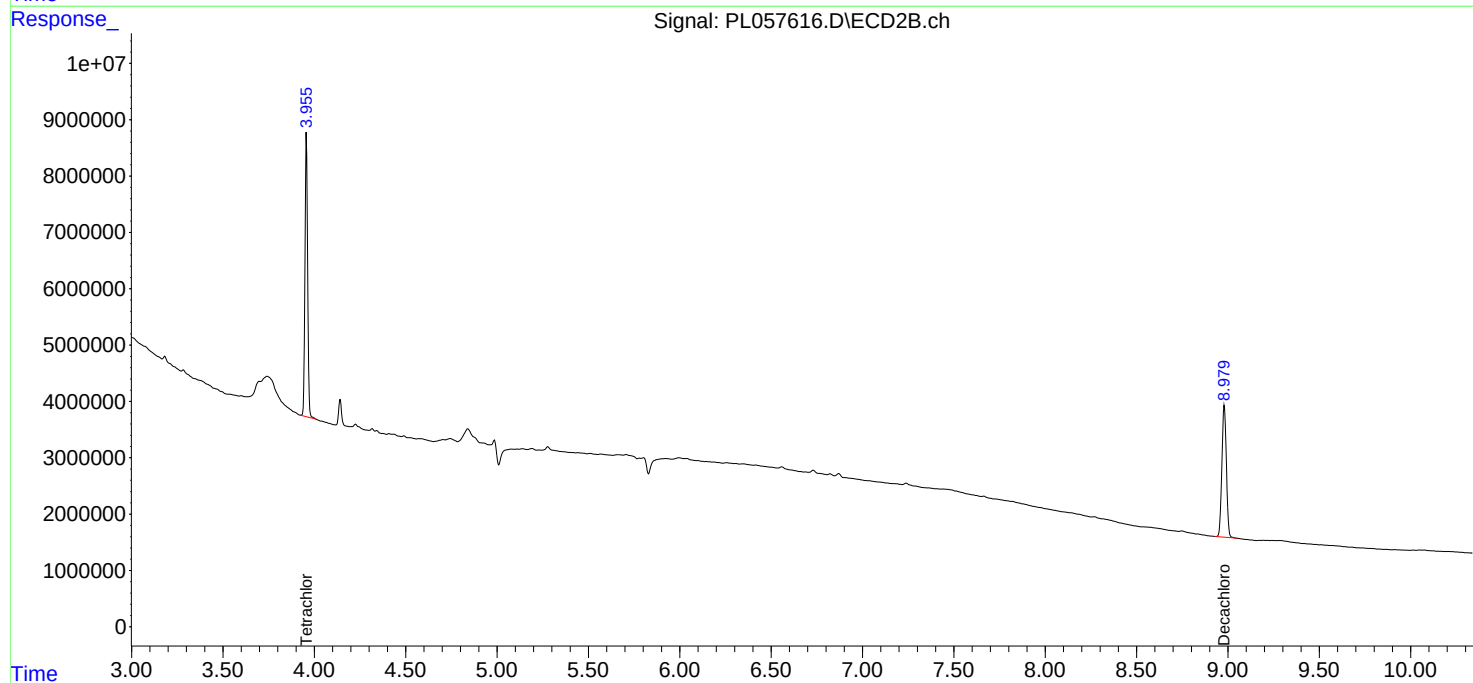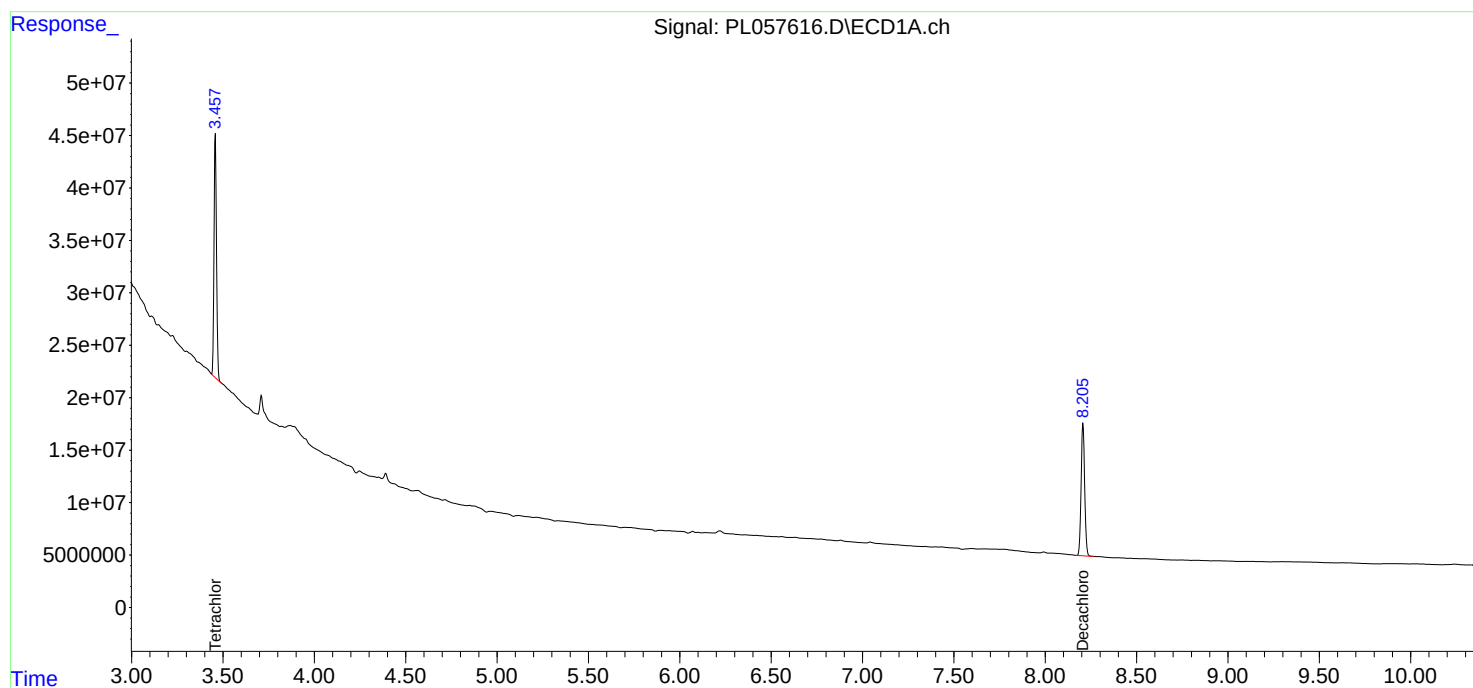

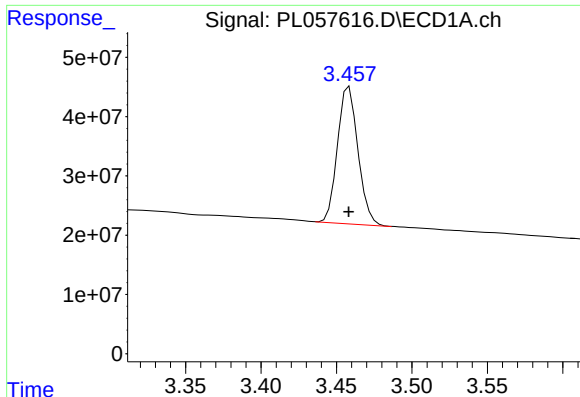


#1 Tetrachloro-m-xylene

R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 219322980
Conc: 23.66 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CL-02-032520MSD


Manual Integrations
APPROVED

mohammad
3/30/2020 10:35:06 AM

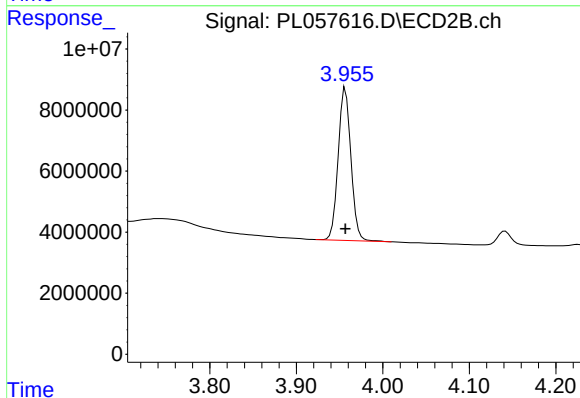


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 50793183
Conc: 23.41 ng/ml

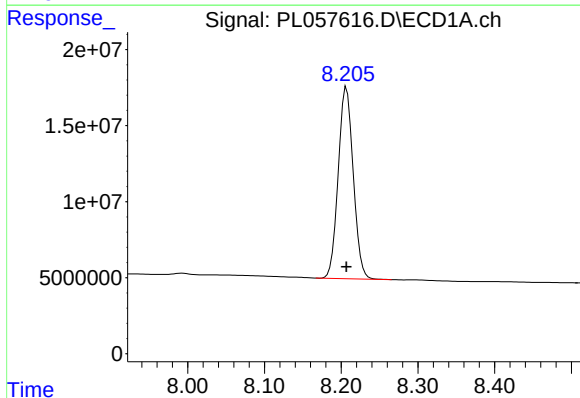

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 171399592
Conc: 16.20 ng/ml

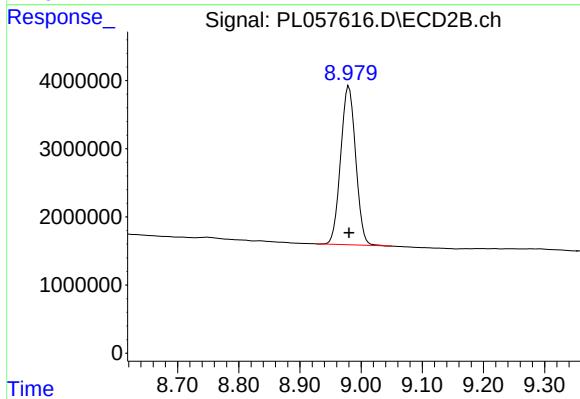

#28 Decachlorobiphenyl

R.T.: 8.980 min
Delta R.T.: 0.000 min
Response: 39673048
Conc: 17.89 ng/ml