

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032621\
 Data File : PL065573.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2021 09:07
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:15:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.284	3.785	64018378	66480723	26.958	24.221
28)	SA Decachlor...	7.924	8.735	54562475	49973183	22.583	25.212
Target Compounds							
4)	MA Heptachlor	0.000	4.947	0	1119299	N.D.	0.336 #
6)	B beta-BHC	4.241	4.634	1389446	4959881	0.983	2.879 #
8)	B Heptachlo...	0.000	5.621	0	1327750	N.D.	0.459 #
9)	A Endosulfan I	0.000	5.998f	0	339548	N.D.	0.129 #
14)	MA Endrin	5.763	0.000	1104261	0	0.442	N.D. #
15)	B Endosulfa...	6.014f	6.687f	147416	2281066	0.060	1.011 #
17)	MA 4,4'-DDT	6.129	0.000	1380312	0	0.729	N.D. #
18)	B Endrin al...	6.193	0.000	696988	0	0.363	N.D. #
19)	B Endosulfa...	6.420	0.000	340291	0	0.138	N.D. #
27)	Chlordane-5	6.014f	6.700f	147416	195579	1.474	2.444 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032621\
Data File : PL065573.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2021 09:07
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:15:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

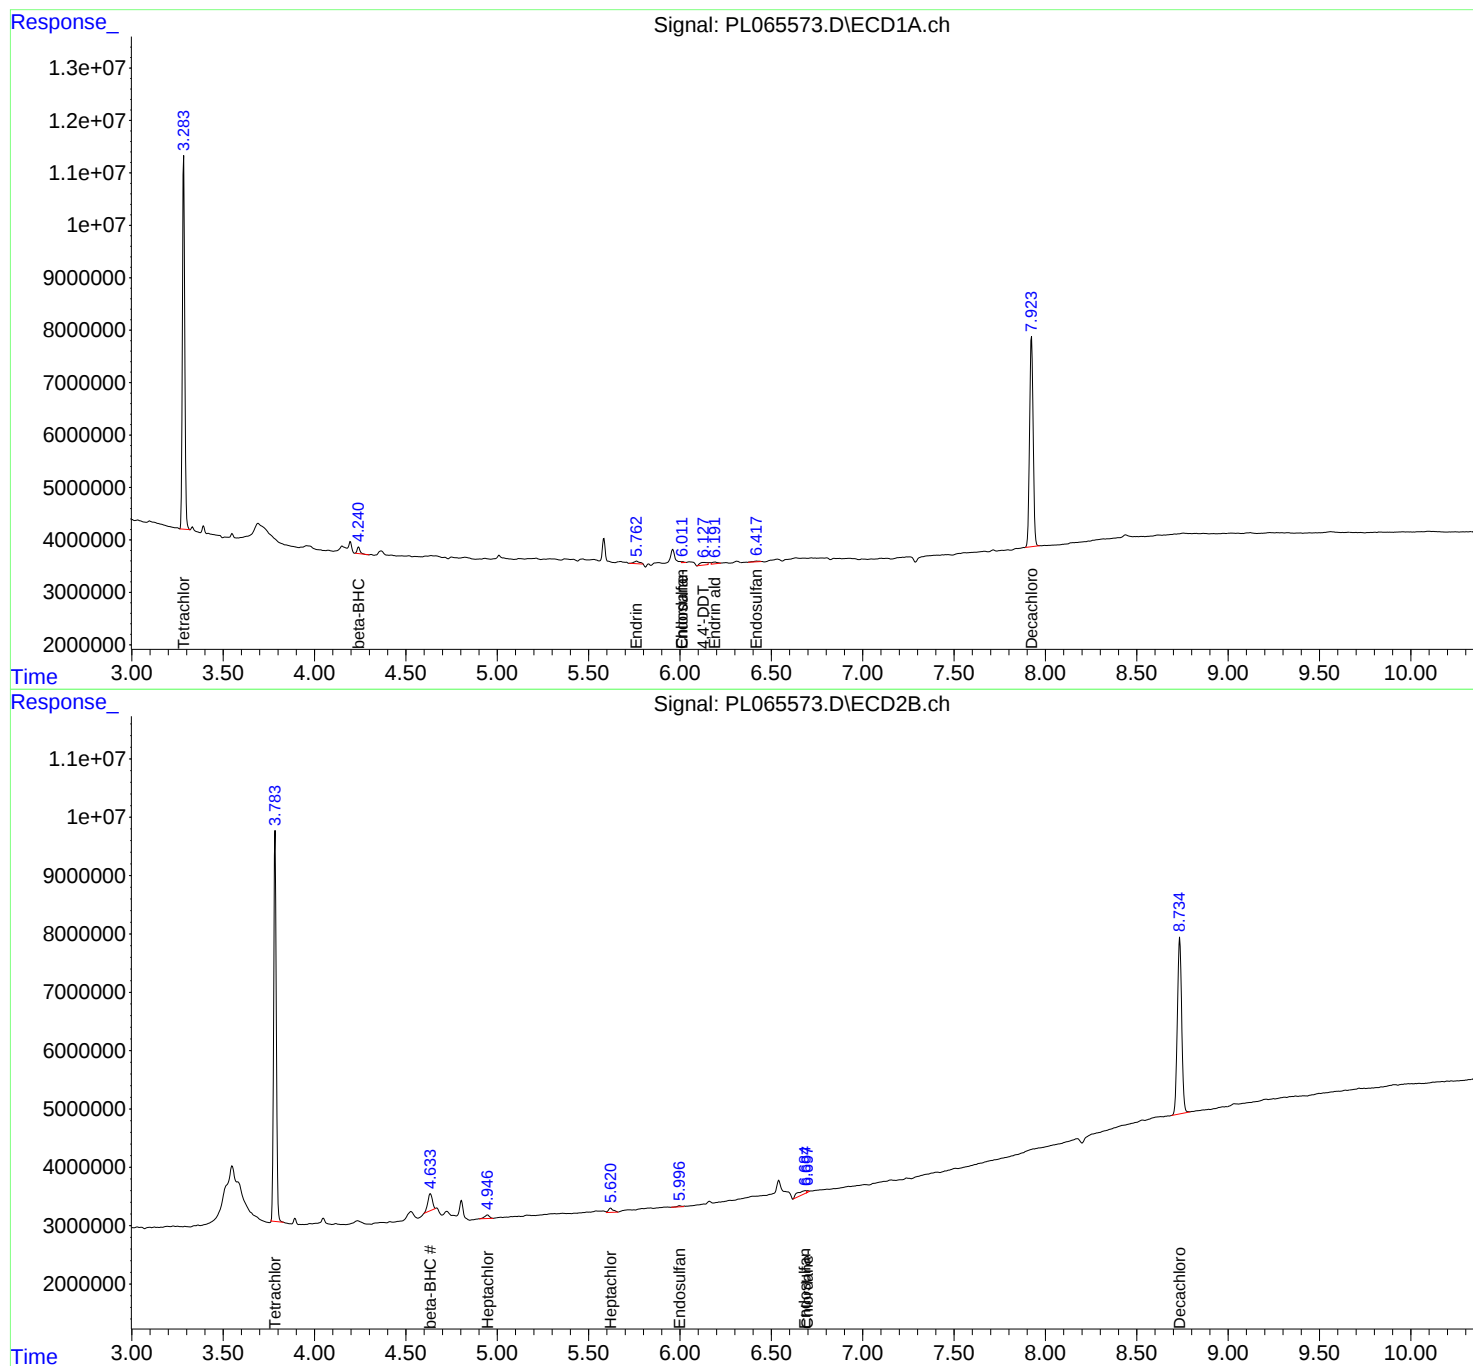


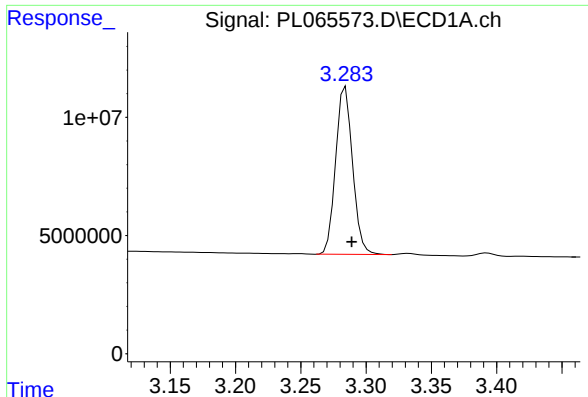

#1 Tetrachloro-m-xylene


R.T.: 3.284 min
Delta R.T.: -0.005 min
Response: 64018378
Conc: 26.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

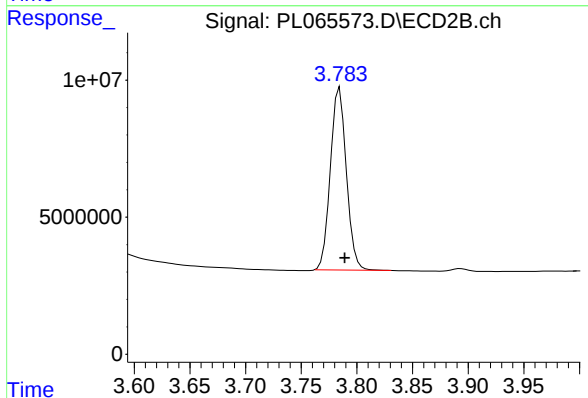


#1 Tetrachloro-m-xylene

R.T.: 3.785 min
Delta R.T.: -0.004 min
Response: 66480723
Conc: 24.22 ng/ml

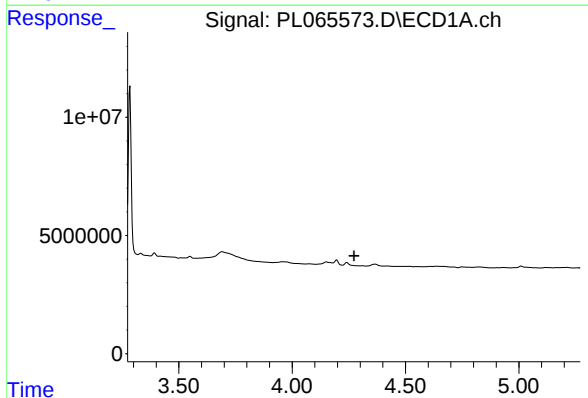


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.274 min
Response: 0
Conc: N.D.

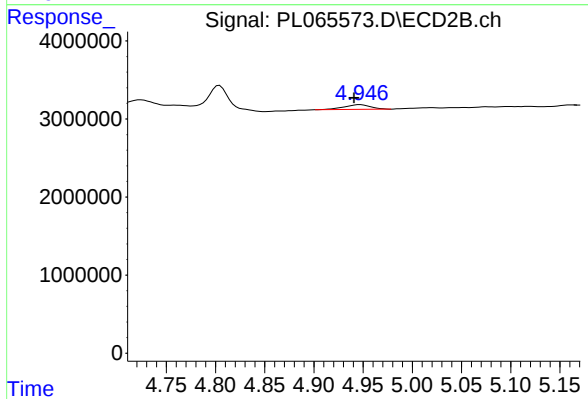

#4 Heptachlor


R.T.: 4.947 min
Delta R.T.: 0.006 min
Response: 1119299
Conc: 0.34 ng/ml

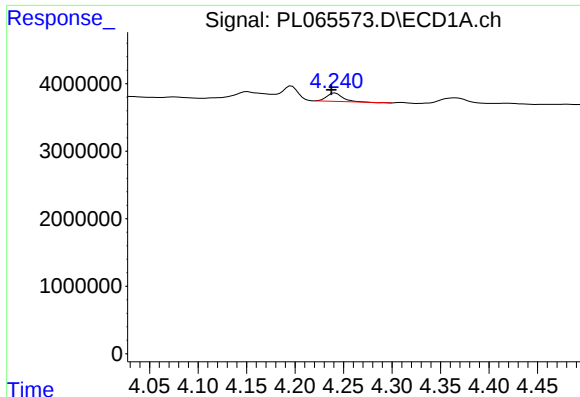

#6 beta-BHC


R.T.: 4.241 min
Delta R.T.: 0.004 min
Response: 1389446
Conc: 0.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

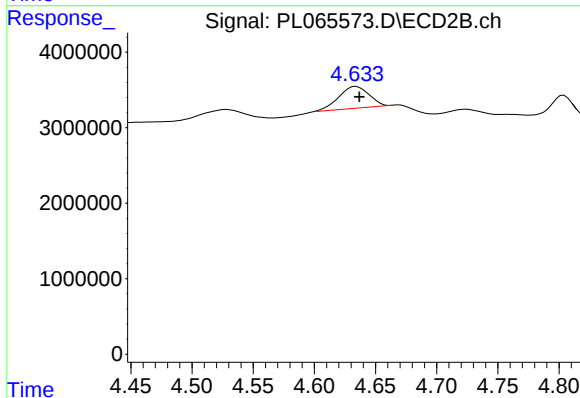


#6 beta-BHC

R.T.: 4.634 min
Delta R.T.: -0.003 min
Response: 4959881
Conc: 2.88 ng/ml

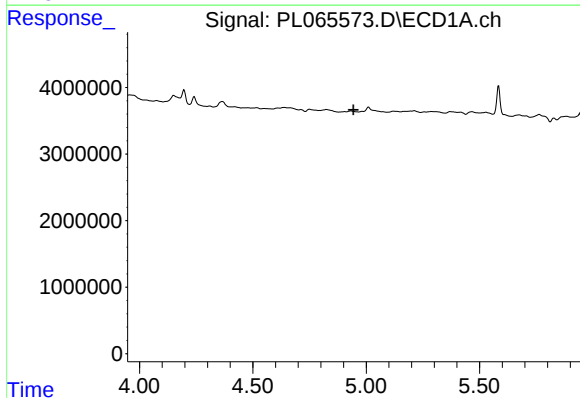


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.944 min
Response: 0
Conc: N.D.

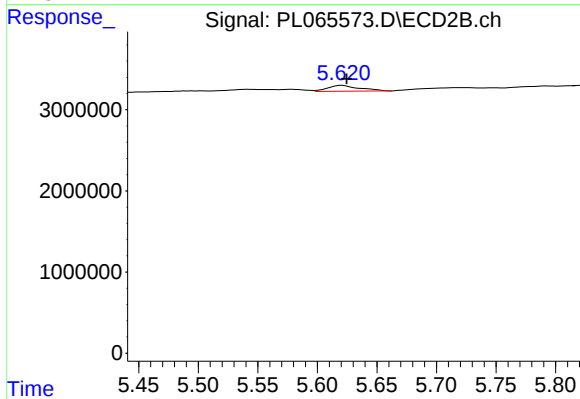

#8 Heptachlor epoxide


R.T.: 5.621 min
Delta R.T.: -0.004 min
Response: 1327750
Conc: 0.46 ng/ml

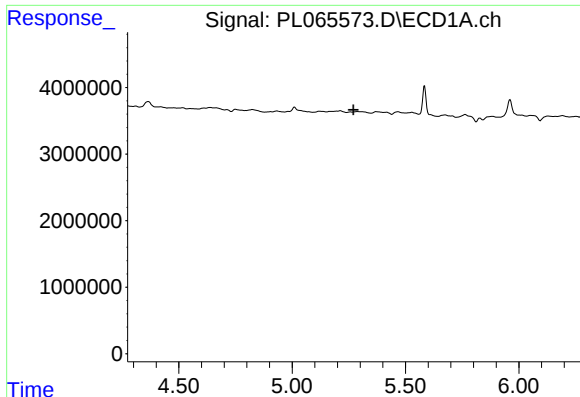

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.271 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

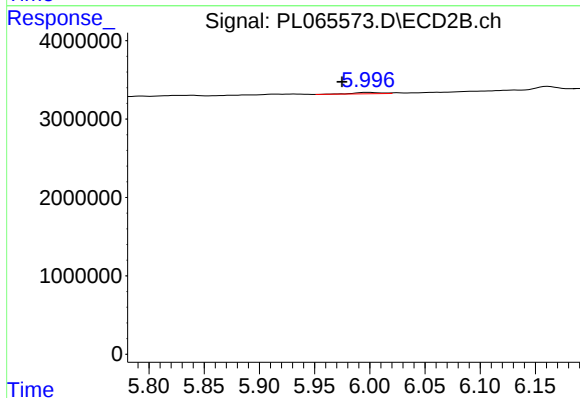


#9 Endosulfan I

R.T.: 5.998 min
Delta R.T.: 0.023 min
Response: 339548
Conc: 0.13 ng/ml

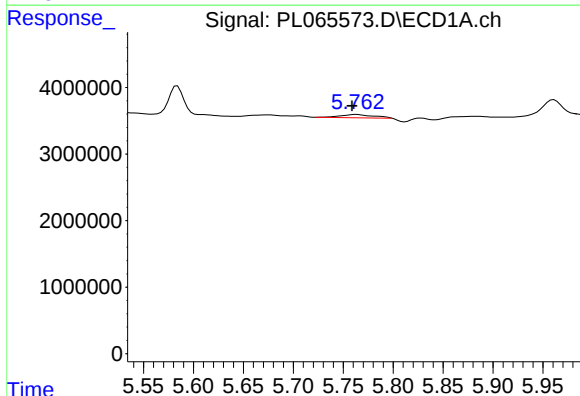


#14 Endrin

R.T.: 5.763 min
Delta R.T.: 0.004 min
Response: 1104261
Conc: 0.44 ng/ml

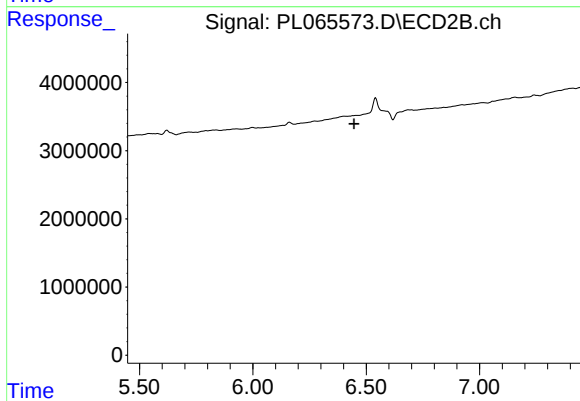

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.446 min
Response: 0
Conc: N.D.

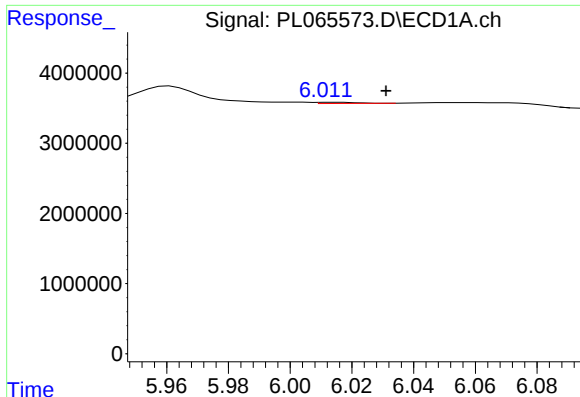

#15 Endosulfan II


R.T.: 6.014 min
Delta R.T.: -0.017 min
Response: 147416
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

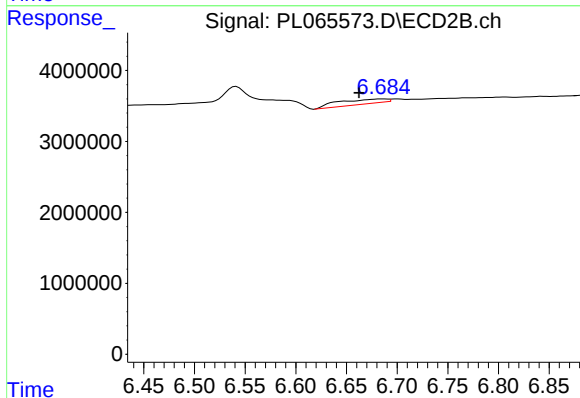


#15 Endosulfan II

R.T.: 6.687 min
Delta R.T.: 0.024 min
Response: 2281066
Conc: 1.01 ng/ml

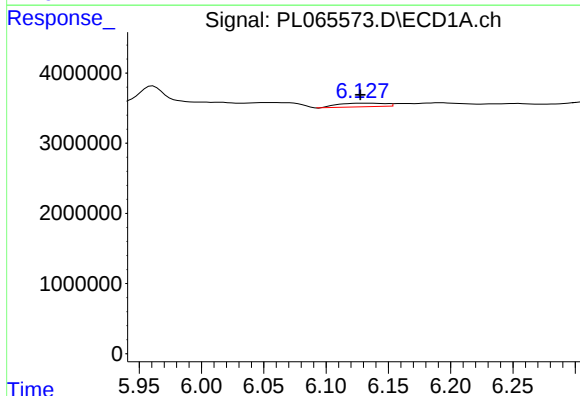


#17 4,4'-DDT

R.T.: 6.129 min
Delta R.T.: 0.001 min
Response: 1380312
Conc: 0.73 ng/ml

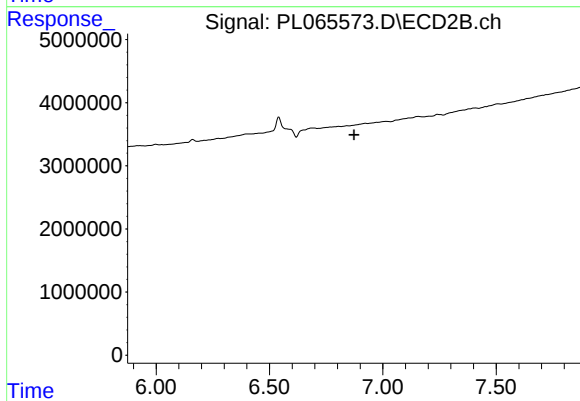

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.873 min
Response: 0
Conc: N.D.

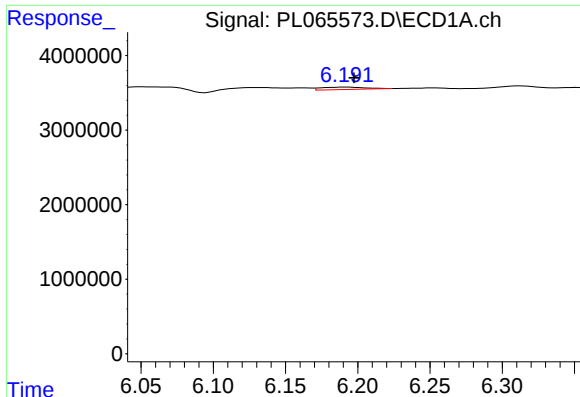

#18 Endrin aldehyde


R.T.: 6.193 min
Delta R.T.: -0.005 min
Response: 696988
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

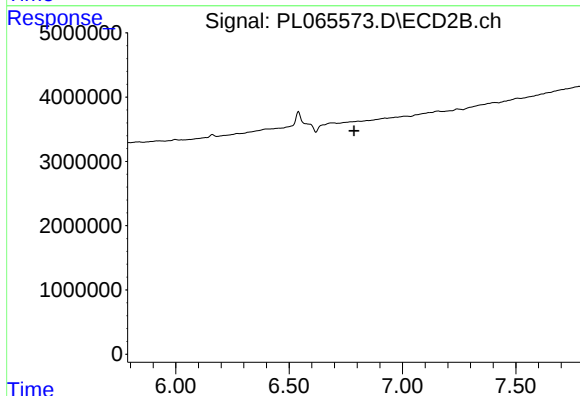


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.787 min
Response: 0
Conc: N.D.

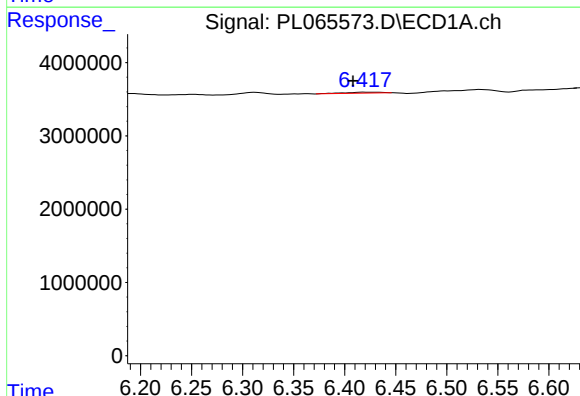


#19 Endosulfan Sulfate

R.T.: 6.420 min
Delta R.T.: 0.012 min
Response: 340291
Conc: 0.14 ng/ml

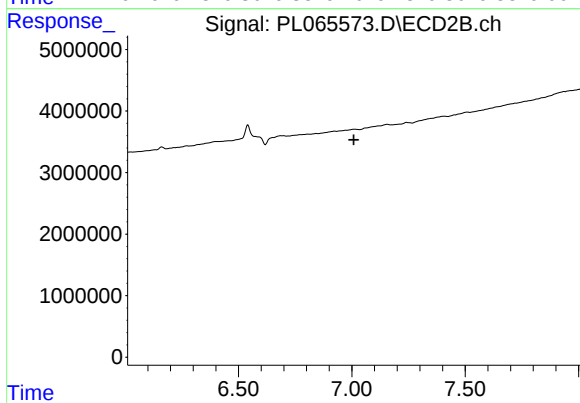

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.009 min
Response: 0
Conc: N.D.

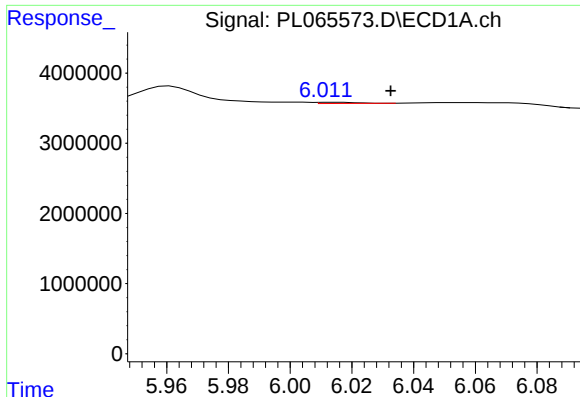

#27 Chlordane-5


R.T.: 6.014 min
Delta R.T.: -0.019 min
Response: 147416
Conc: 1.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

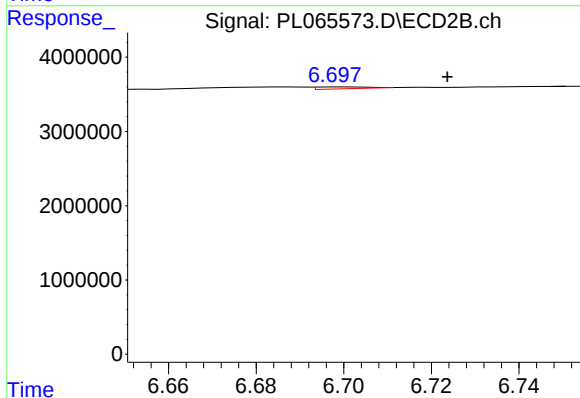


#27 Chlordane-5

R.T.: 6.700 min
Delta R.T.: -0.024 min
Response: 195579
Conc: 2.44 ng/ml

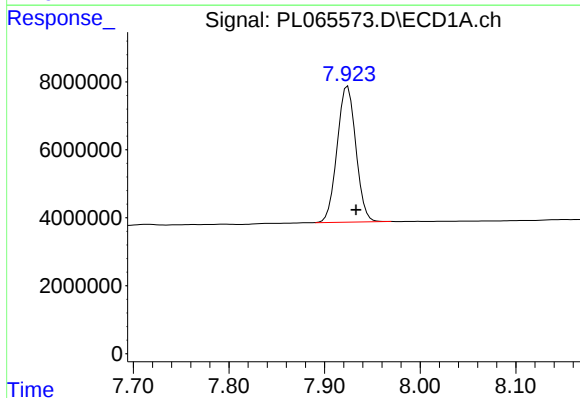

#28 Decachlorobiphenyl

R.T.: 7.924 min
Delta R.T.: -0.009 min
Response: 54562475
Conc: 22.58 ng/ml

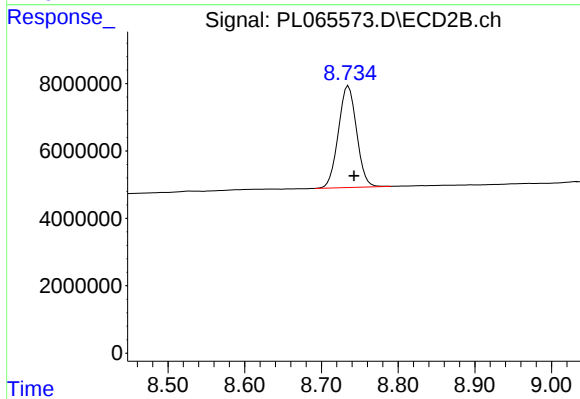

#28 Decachlorobiphenyl

R.T.: 8.735 min
Delta R.T.: -0.007 min
Response: 49973183
Conc: 25.21 ng/ml