

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032621\
 Data File : PL065591.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2021 15:44
 Operator : AR\AJ
 Sample : PB135379BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:21:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.284	3.784	47803635	51457646	20.130	18.748
28)	SA Decachlor...	7.925	8.735	45084794	41097814	18.661	20.734
Target Compounds							
2)	A alpha-BHC	3.710	0.000	2314337	0	0.619	N.D. #
4)	MA Heptachlor	0.000	4.947	0	661063	N.D.	0.198 #
6)	B beta-BHC	0.000	4.637	0	7997951	N.D.	4.643 #
8)	B Heptachlo...	0.000	5.642f	0	126247	N.D.	0.044 #
16)	A 4,4'-DDD	0.000	6.582	0	100401	N.D.	0.046 #
18)	B Endrin al...	6.202	0.000	353132	0	0.184	N.D. #
22)	Mirex	0.000	7.939f	0	529054	N.D.	0.318 #
27)	Chlordane-5	0.000	6.699f	0	330050	N.D.	4.125 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032621\
Data File : PL065591.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2021 15:44
Operator : AR\AJ
Sample : PB135379BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:21:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

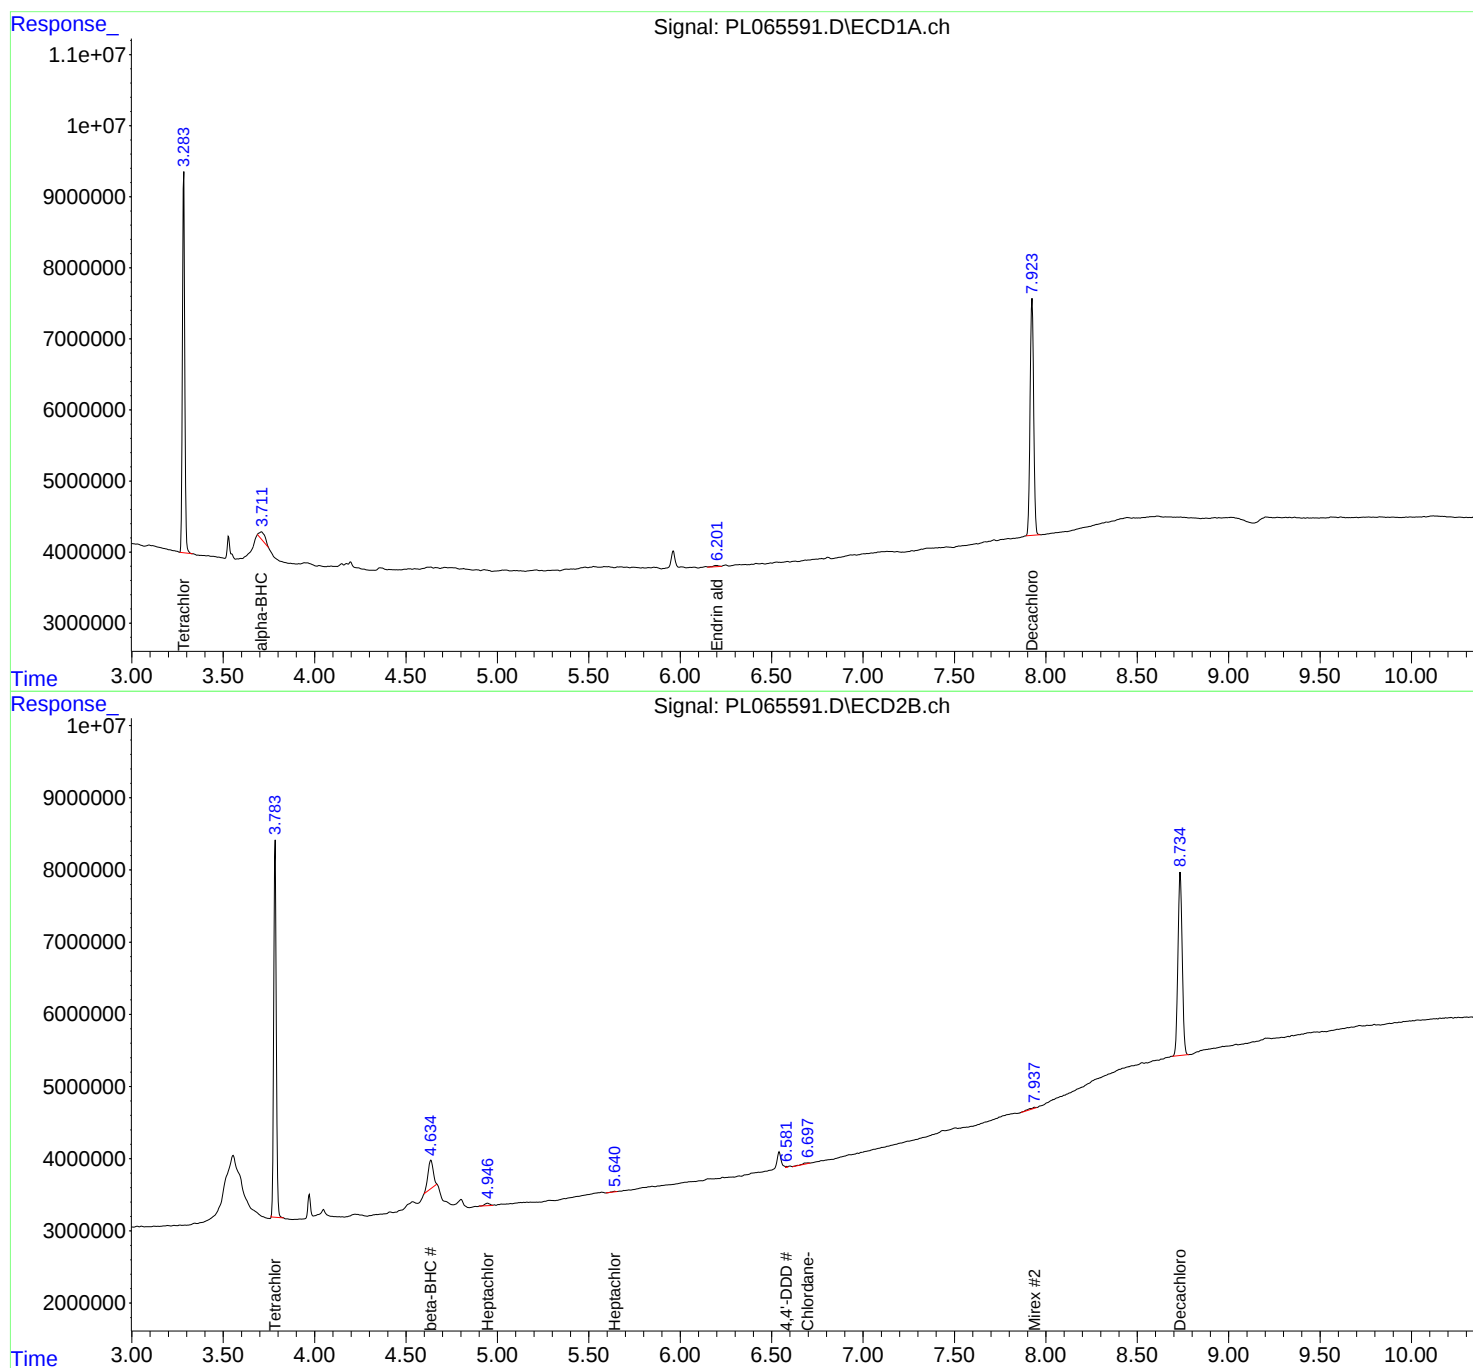


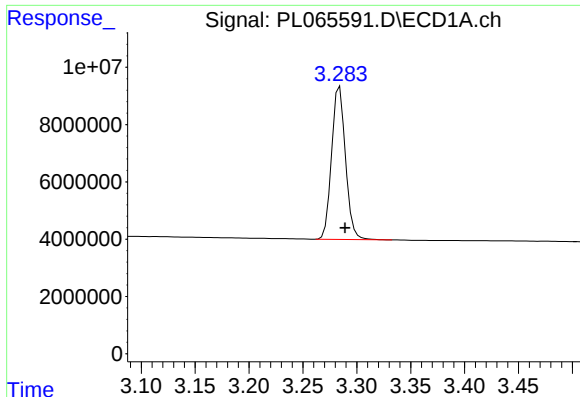

#1 Tetrachloro-m-xylene


R.T.: 3.284 min
Delta R.T.: -0.005 min
Response: 47803635
Conc: 20.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

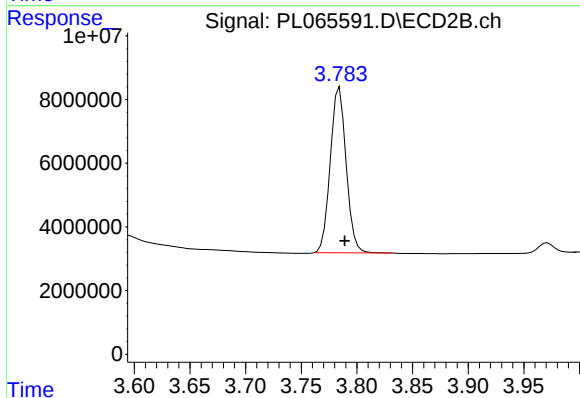


#1 Tetrachloro-m-xylene

R.T.: 3.784 min
Delta R.T.: -0.005 min
Response: 51457646
Conc: 18.75 ng/ml

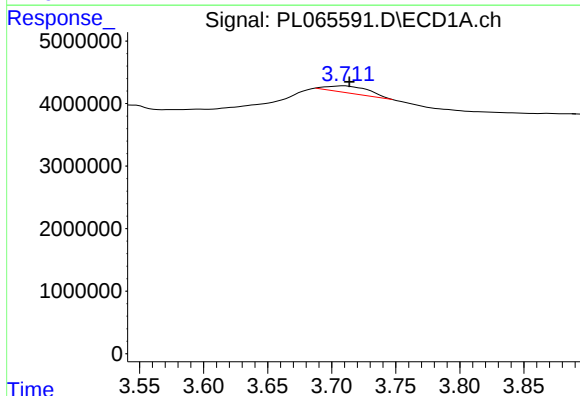


#2 alpha-BHC

R.T.: 3.710 min
Delta R.T.: -0.004 min
Response: 2314337
Conc: 0.62 ng/ml

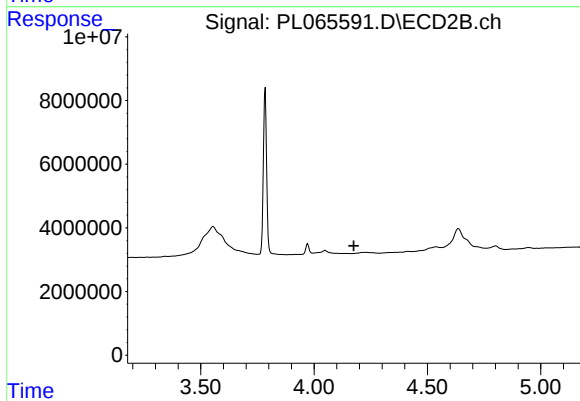

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.175 min
Response: 0
Conc: N.D.

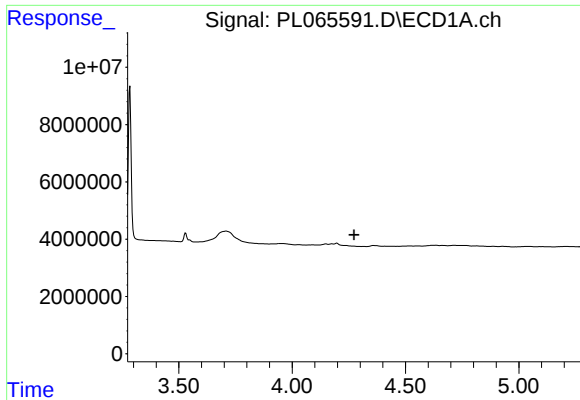

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

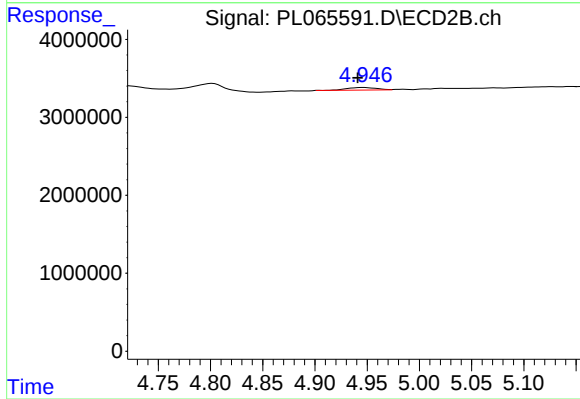


#4 Heptachlor

R.T.: 4.947 min
Delta R.T.: 0.006 min
Response: 661063
Conc: 0.20 ng/ml

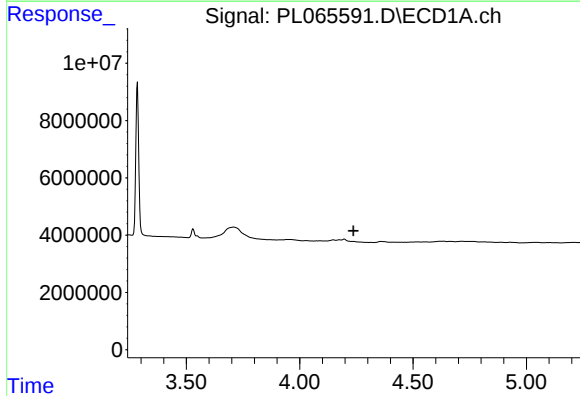


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.238 min
Response: 0
Conc: N.D.

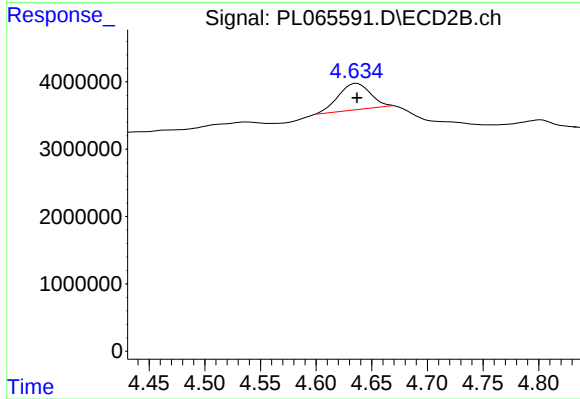

#6 beta-BHC


R.T.: 4.637 min
Delta R.T.: 0.000 min
Response: 7997951
Conc: 4.64 ng/ml

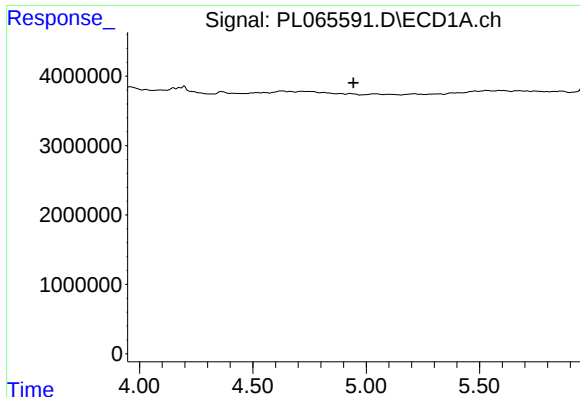

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.944 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

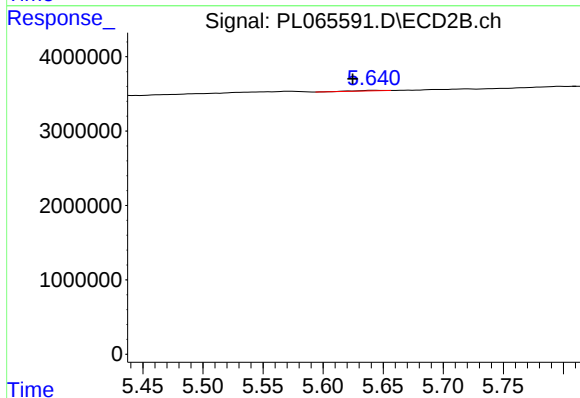


#8 Heptachlor epoxide

R.T.: 5.642 min
Delta R.T.: 0.017 min
Response: 126247
Conc: 0.04 ng/ml

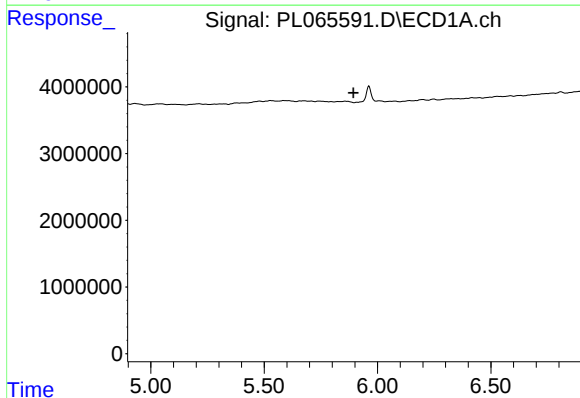


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.894 min
Response: 0
Conc: N.D.

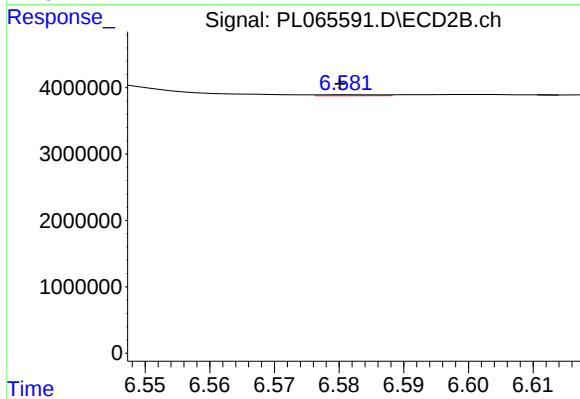

#16 4,4'-DDD


R.T.: 6.582 min
Delta R.T.: 0.002 min
Response: 100401
Conc: 0.05 ng/ml

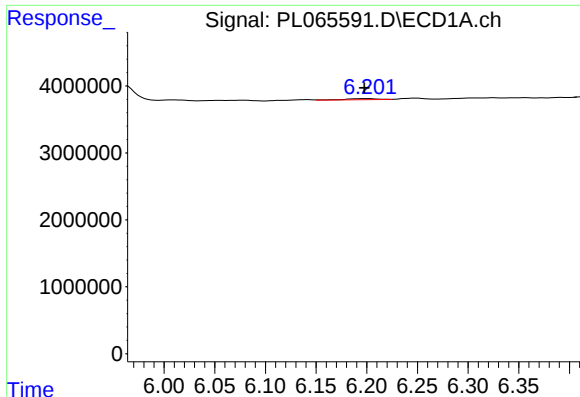

#18 Endrin aldehyde


R.T.: 6.202 min
Delta R.T.: 0.005 min
Response: 353132
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

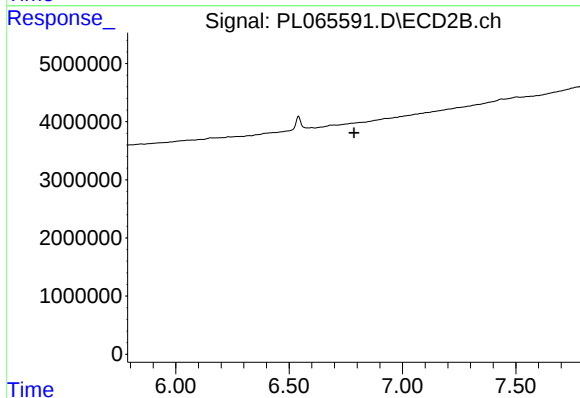


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.787 min
Response: 0
Conc: N.D.

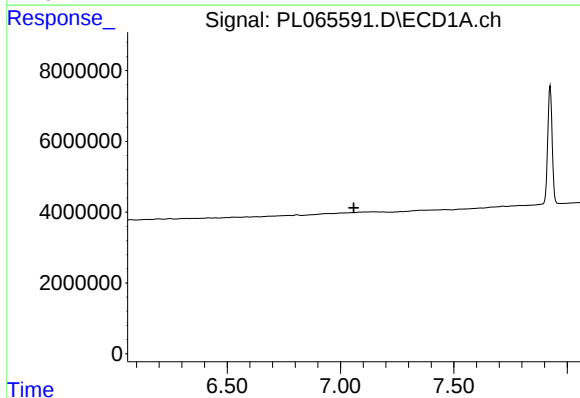


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.059 min
Response: 0
Conc: N.D.

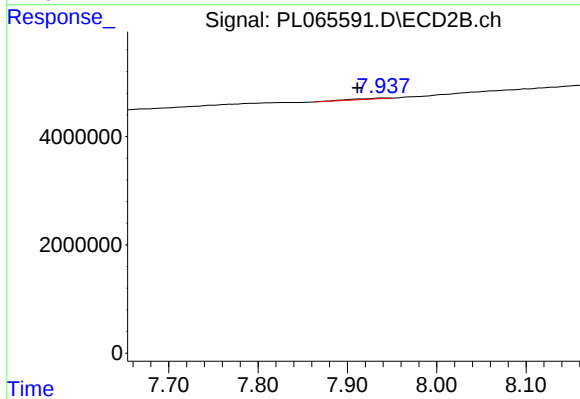

#22 Mirex


R.T.: 7.939 min
Delta R.T.: 0.027 min
Response: 529054
Conc: 0.32 ng/ml

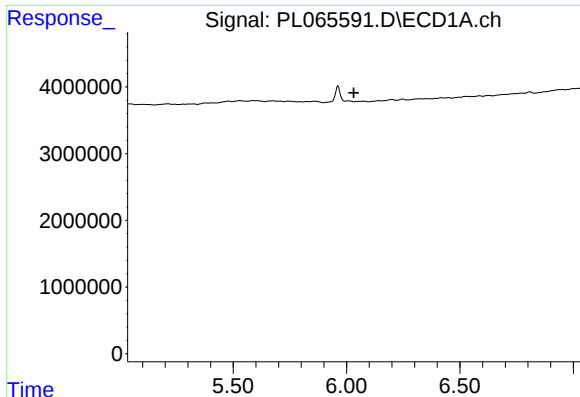

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

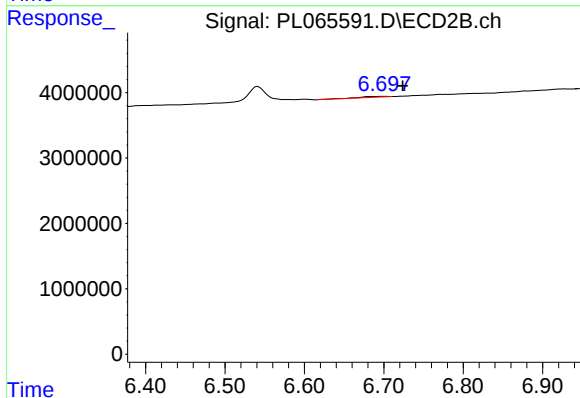


#27 Chlordane-5

R.T.: 6.699 min
Delta R.T.: -0.024 min
Response: 330050
Conc: 4.12 ng/ml

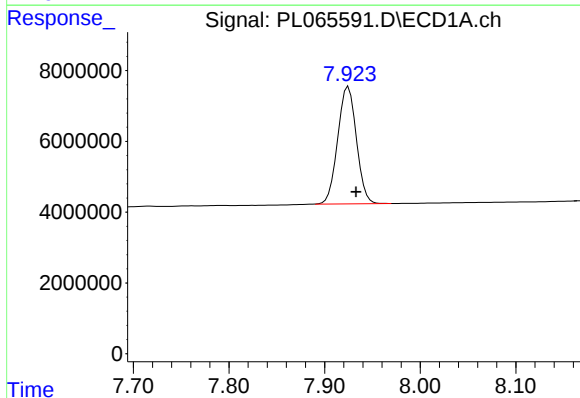

#28 Decachlorobiphenyl

R.T.: 7.925 min
Delta R.T.: -0.008 min
Response: 45084794
Conc: 18.66 ng/ml

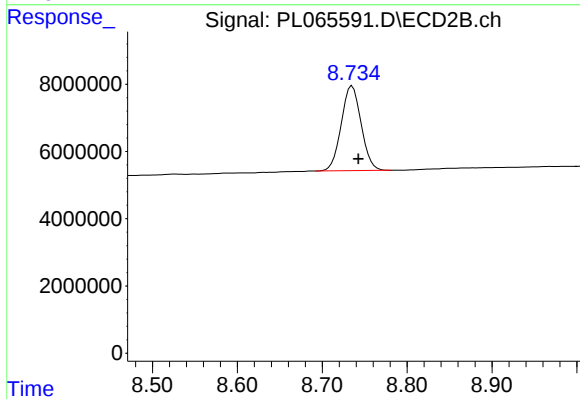

#28 Decachlorobiphenyl

R.T.: 8.735 min
Delta R.T.: -0.007 min
Response: 41097814
Conc: 20.73 ng/ml