

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032621\
 Data File : PL065597.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2021 17:10
 Operator : AR\AJ
 Sample : M1791-19
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:23:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.284	3.784	41258700	44696854	17.374	16.285
28)	SA Decachlor...	7.923	8.735	40774684	37428784	16.877	18.883
Target Compounds							
5)	MB Aldrin	4.508	0.000	233877	0	0.074	N.D. #
6)	B beta-BHC	0.000	4.636	0	3082176	N.D.	1.789 #
8)	B Heptachlo...	0.000	5.647f	0	212188	N.D.	0.073 #
15)	B Endosulfa...	0.000	6.647f	0	316814	N.D.	0.140 #
18)	B Endrin al...	6.189	0.000	367988	0	0.192	N.D. #
19)	B Endosulfa...	0.000	7.011	0	200625	N.D.	0.091 #
20)	A Methoxychlor	0.000	7.336	0	180150	N.D.	0.172 #
21)	B Endrin ke...	0.000	7.502f	0	630025	N.D.	0.267 #
27)	Chlordane-5	0.000	6.722	0	232911	N.D.	2.911 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032621\
Data File : PL065597.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2021 17:10
Operator : AR\AJ
Sample : M1791-19
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:23:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

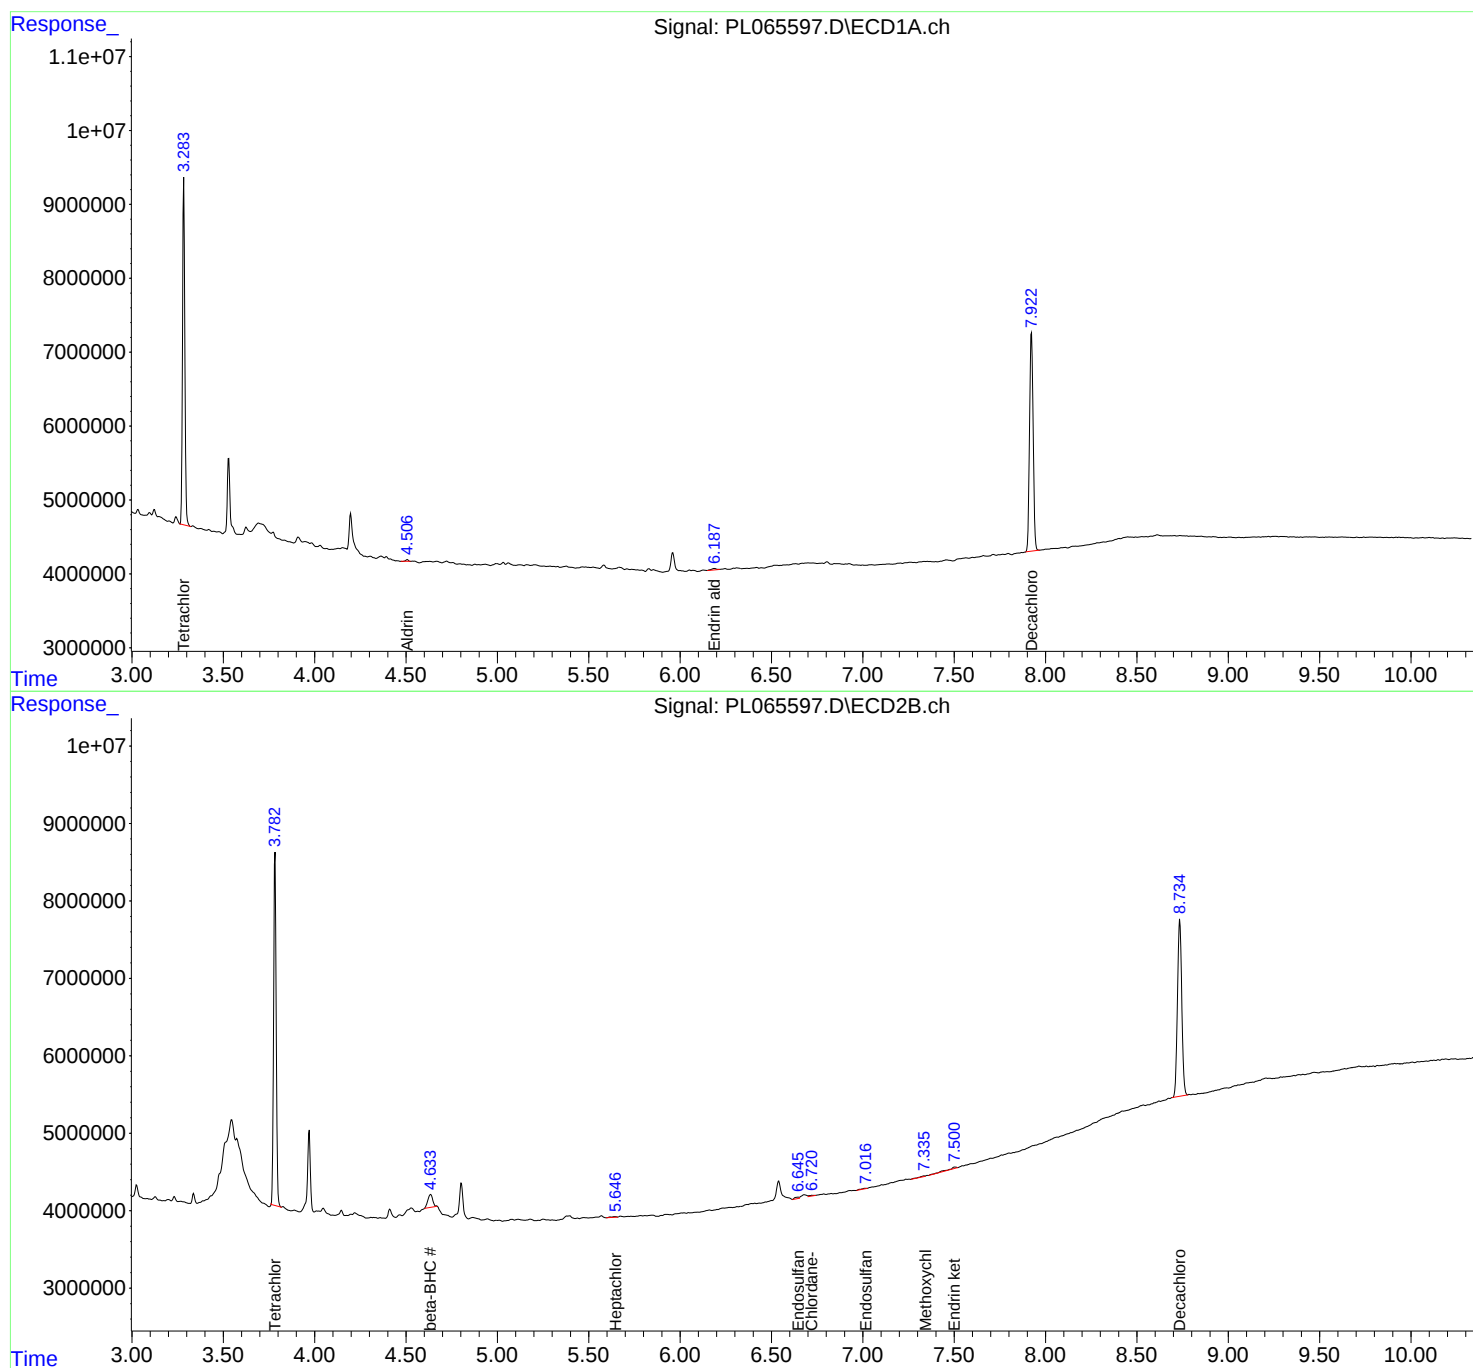


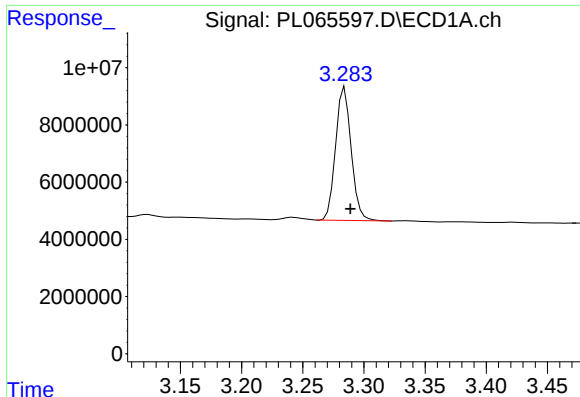

#1 Tetrachloro-m-xylene


R.T.: 3.284 min
Delta R.T.: -0.005 min
Response: 41258700
Conc: 17.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

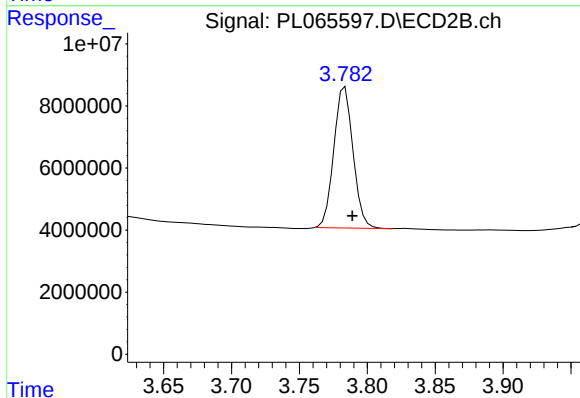


#1 Tetrachloro-m-xylene

R.T.: 3.784 min
Delta R.T.: -0.005 min
Response: 44696854
Conc: 16.28 ng/ml

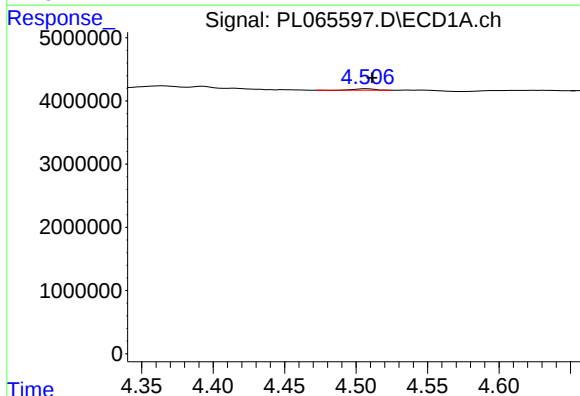


#5 Aldrin

R.T.: 4.508 min
Delta R.T.: -0.003 min
Response: 233877
Conc: 0.07 ng/ml

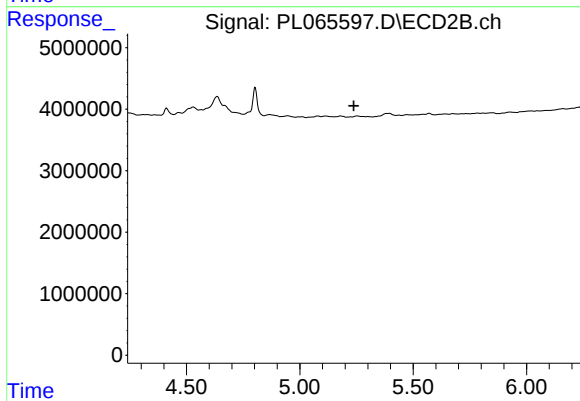

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.238 min
Response: 0
Conc: N.D.

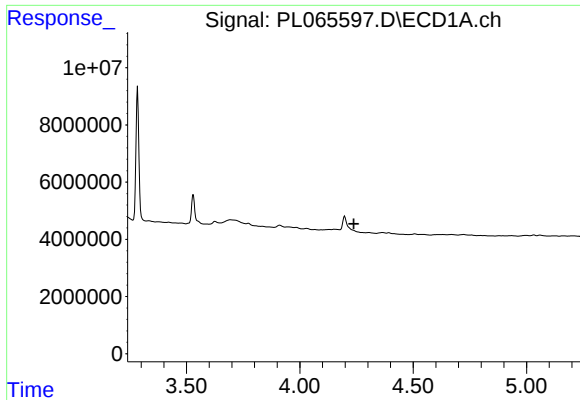

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.238 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

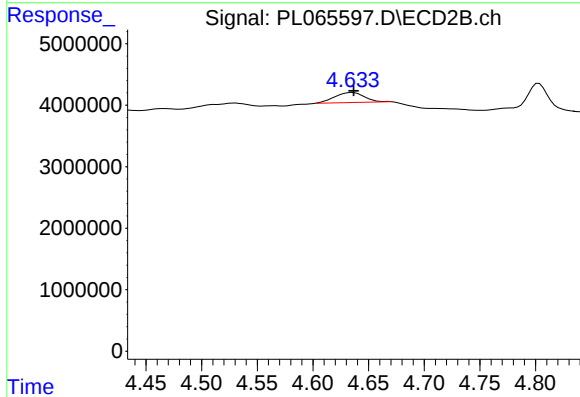


#6 beta-BHC

R.T.: 4.636 min
Delta R.T.: -0.001 min
Response: 3082176
Conc: 1.79 ng/ml

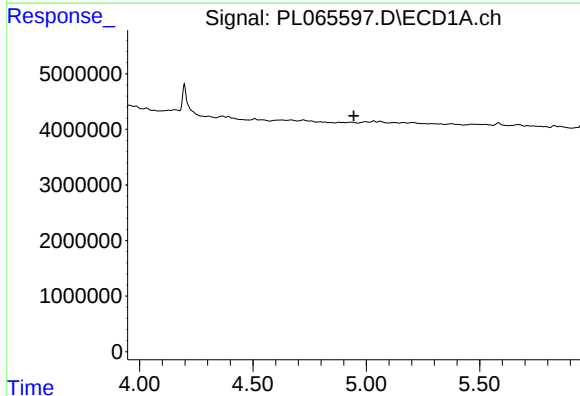


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.944 min
Response: 0
Conc: N.D.

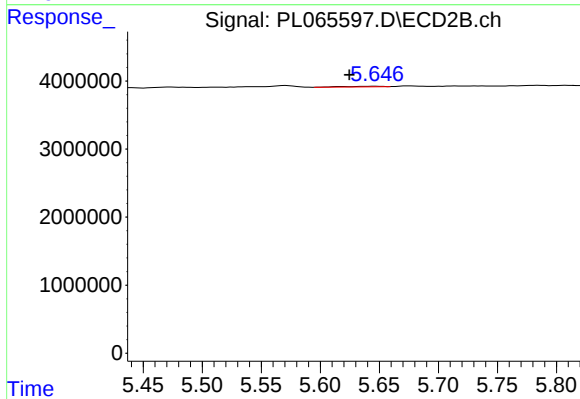

#8 Heptachlor epoxide


R.T.: 5.647 min
Delta R.T.: 0.022 min
Response: 212188
Conc: 0.07 ng/ml

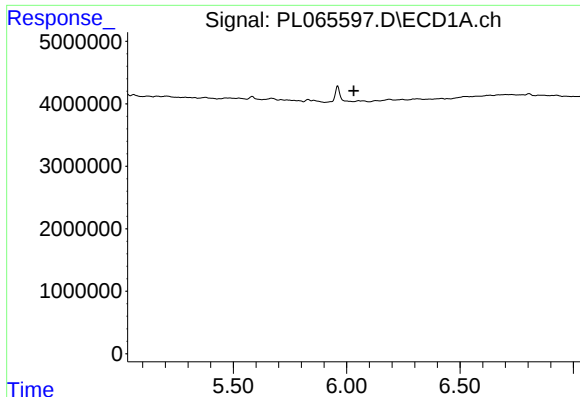

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.031 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

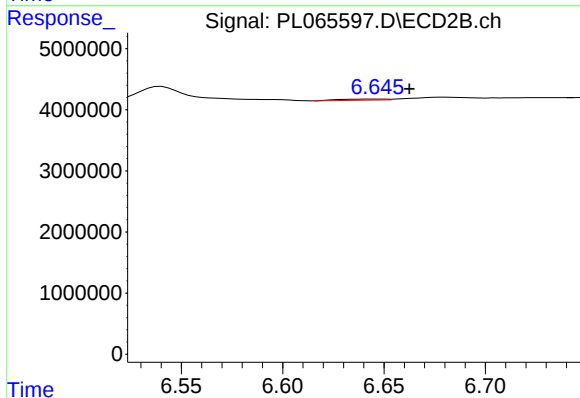


#15 Endosulfan II

R.T.: 6.647 min
Delta R.T.: -0.016 min
Response: 316814
Conc: 0.14 ng/ml

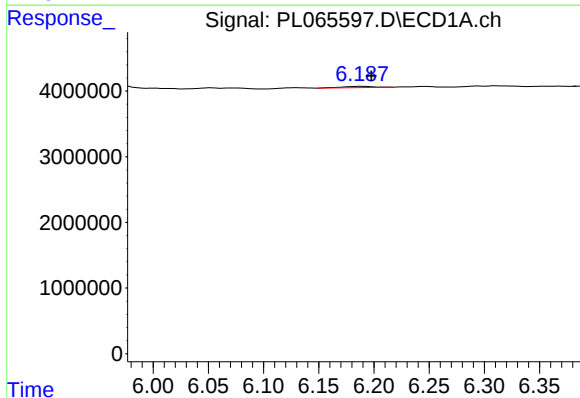


#18 Endrin aldehyde

R.T.: 6.189 min
Delta R.T.: -0.009 min
Response: 367988
Conc: 0.19 ng/ml

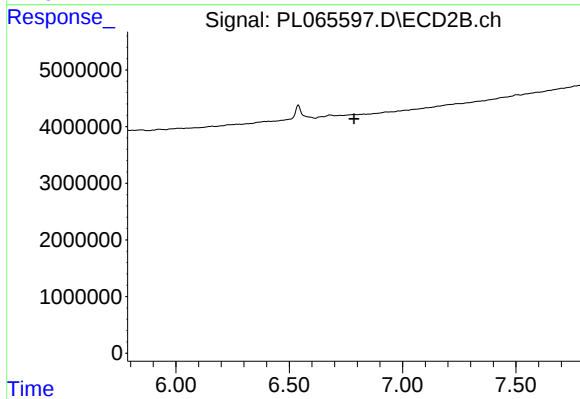

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.787 min
Response: 0
Conc: N.D.

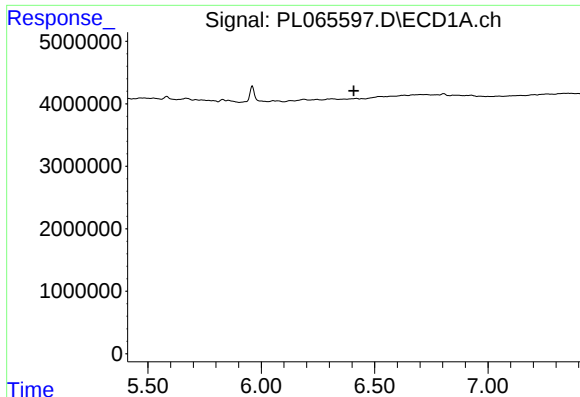

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.408 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

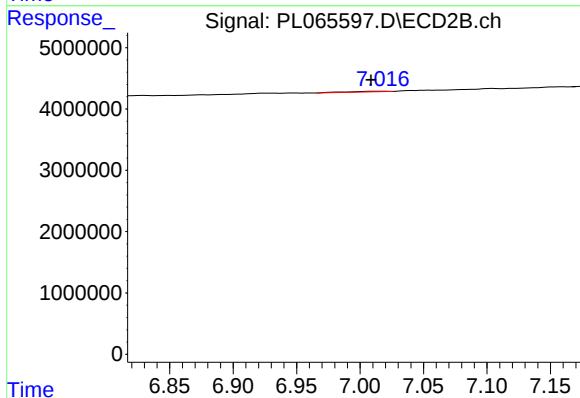


#19 Endosulfan Sulfate

R.T.: 7.011 min
Delta R.T.: 0.003 min
Response: 200625
Conc: 0.09 ng/ml

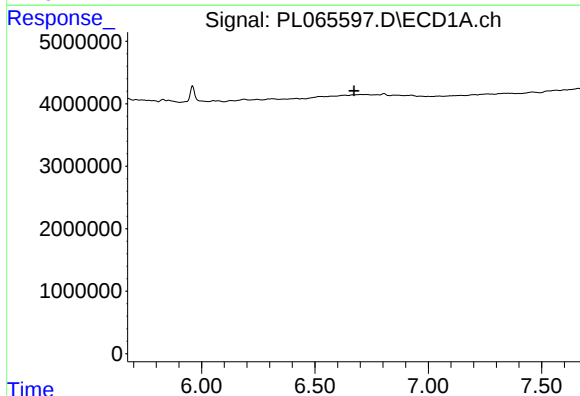


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.673 min
Response: 0
Conc: N.D.

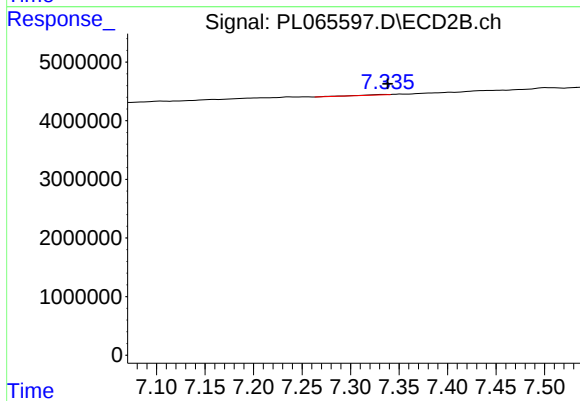

#20 Methoxychlor


R.T.: 7.336 min
Delta R.T.: -0.003 min
Response: 180150
Conc: 0.17 ng/ml

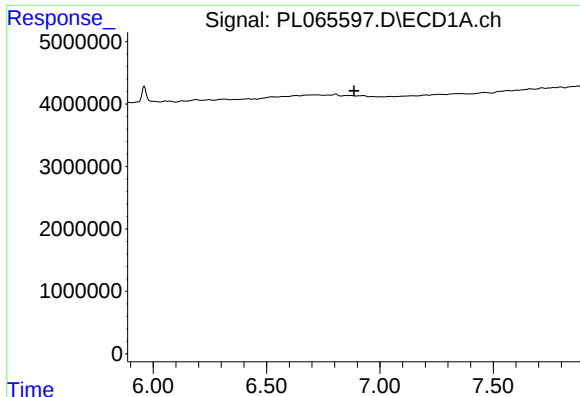

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.886 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

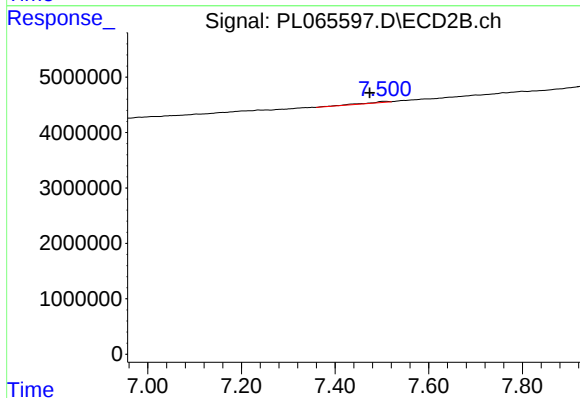


#21 Endrin ketone

R.T.: 7.502 min
Delta R.T.: 0.028 min
Response: 630025
Conc: 0.27 ng/ml

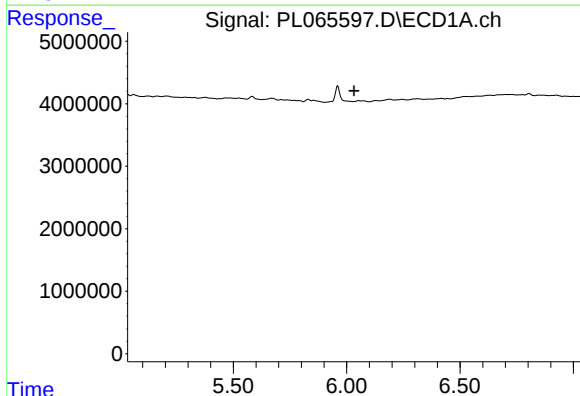


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.033 min
Response: 0
Conc: N.D.

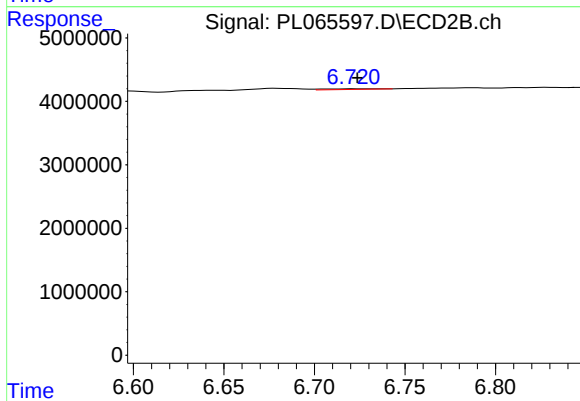

#27 Chlordane-5


R.T.: 6.722 min
Delta R.T.: -0.001 min
Response: 232911
Conc: 2.91 ng/ml

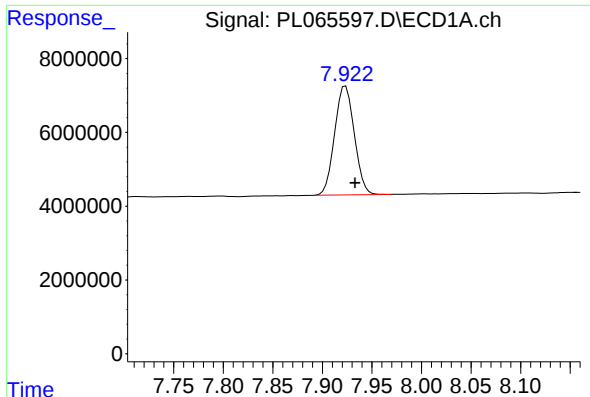

#28 Decachlorobiphenyl

R.T.: 7.923 min
Delta R.T.: -0.010 min
Response: 40774684
Conc: 16.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

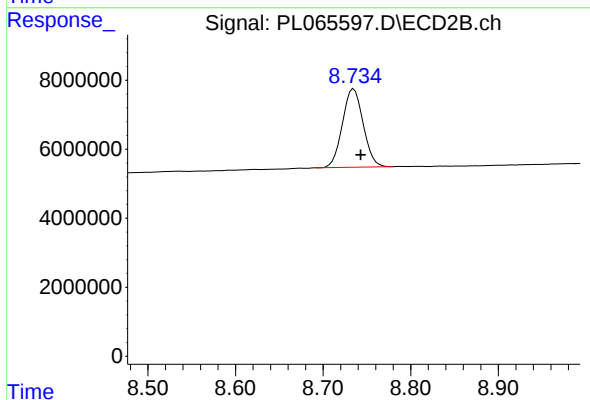

#28 Decachlorobiphenyl

R.T.: 8.735 min
Delta R.T.: -0.008 min
Response: 37428784
Conc: 18.88 ng/ml