

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032621\
 Data File : PL065600.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2021 17:53
 Operator : AR\AJ
 Sample : M1796-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:24:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.283	3.784	40711619	45221482	17.143	16.476
28)	SA Decachlor...	7.922	8.733	37255851	34804410	15.420	17.559
Target Compounds							
4)	MA Heptachlor	0.000	4.940	0	781746	N.D.	0.234 #
5)	MB Aldrin	4.521	0.000	284002	0	0.090	N.D. #
6)	B beta-BHC	0.000	4.628	0	2127752	N.D.	1.235 #
8)	B Heptachlo...	0.000	5.614	0	2296965	N.D.	0.795 #
9)	A Endosulfan I	0.000	5.997f	0	552190	N.D.	0.210 #
15)	B Endosulfa...	0.000	6.682f	0	975743	N.D.	0.432 #
21)	B Endrin ke...	0.000	7.503f	0	370348	N.D.	0.157 #
22)	Mirex	0.000	7.925	0	34717	N.D.	0.021 #
23)	Chlordane-1	4.148f	0.000	6068	0	0.070	N.D. #
24)	Chlordane-2	4.616	0.000	1748380	0	16.120	N.D. #
27)	Chlordane-5	0.000	6.720	0	101523	N.D.	1.269 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032621\
Data File : PL065600.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2021 17:53
Operator : AR\AJ
Sample : M1796-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:24:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

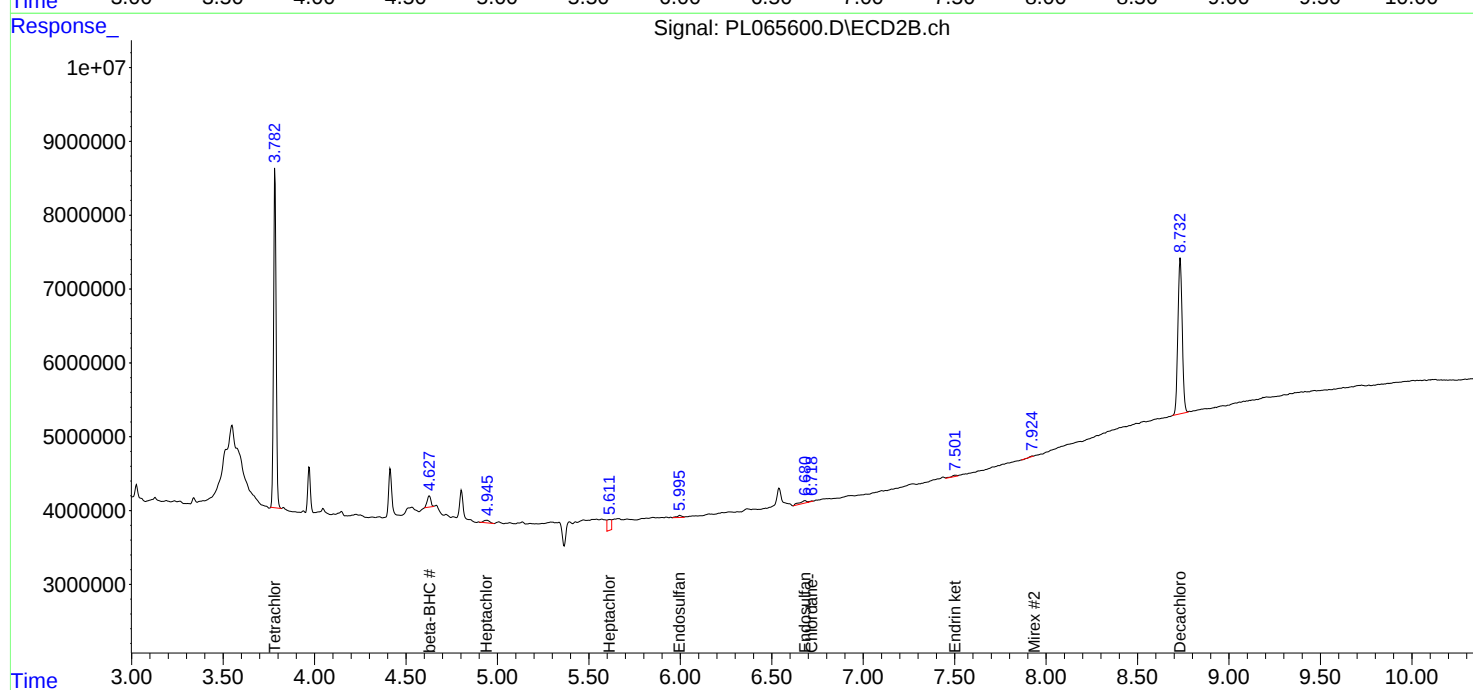


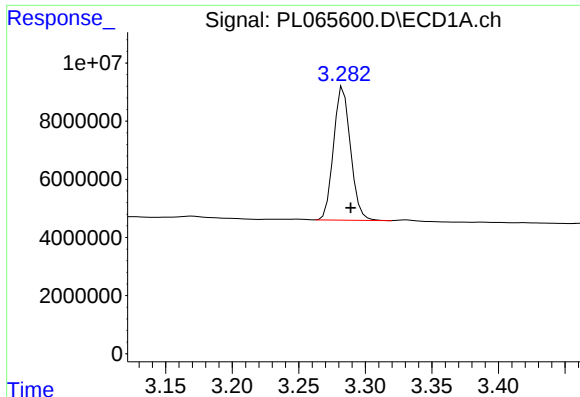

#1 Tetrachloro-m-xylene


R.T.: 3.283 min
Delta R.T.: -0.006 min
Response: 40711619
Conc: 17.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

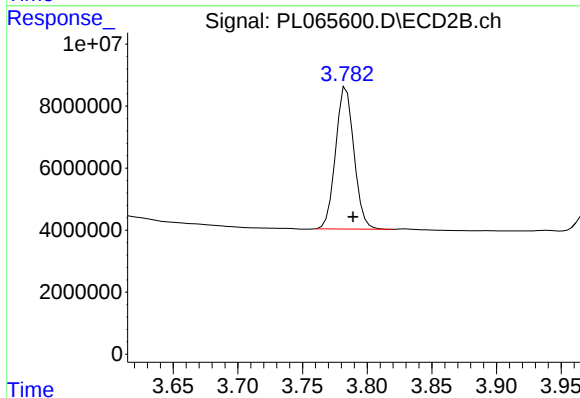


#1 Tetrachloro-m-xylene

R.T.: 3.784 min
Delta R.T.: -0.005 min
Response: 45221482
Conc: 16.48 ng/ml

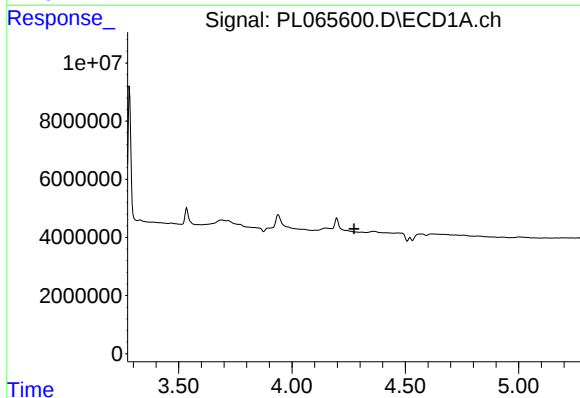


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.274 min
Response: 0
Conc: N.D.

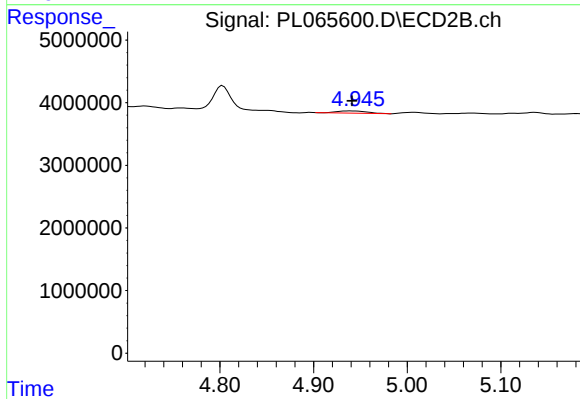

#4 Heptachlor


R.T.: 4.940 min
Delta R.T.: -0.001 min
Response: 781746
Conc: 0.23 ng/ml

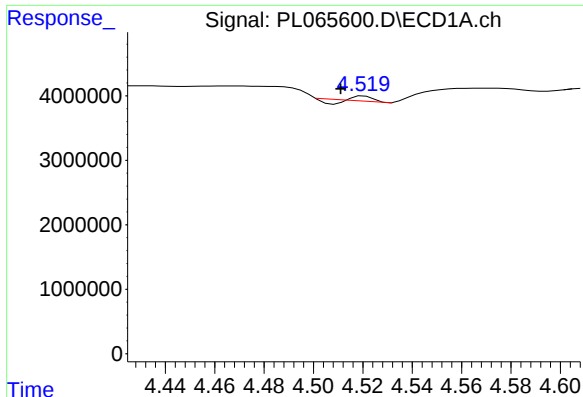

#5 Aldrin


R.T.: 4.521 min
Delta R.T.: 0.010 min
Response: 284002
Conc: 0.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

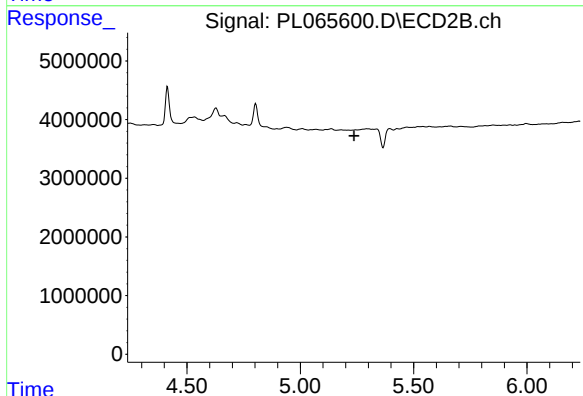


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.238 min
Response: 0
Conc: N.D.

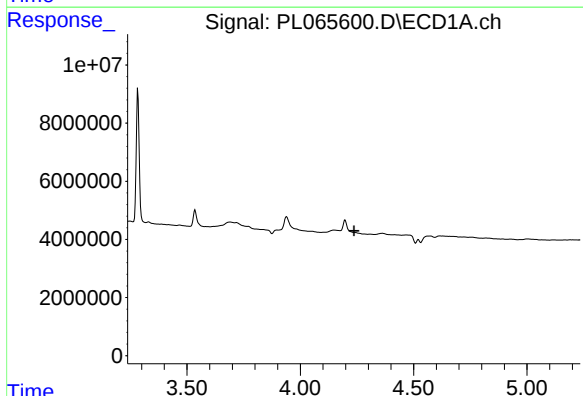


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.238 min
Response: 0
Conc: N.D.

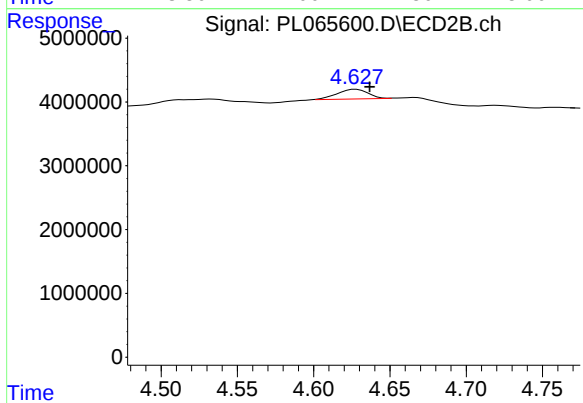

#6 beta-BHC


R.T.: 4.628 min
Delta R.T.: -0.009 min
Response: 2127752
Conc: 1.24 ng/ml

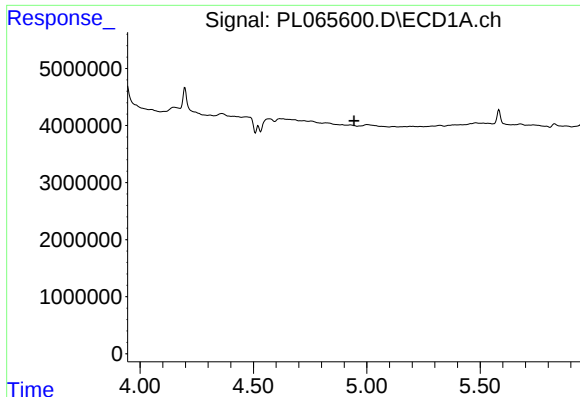

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.944 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

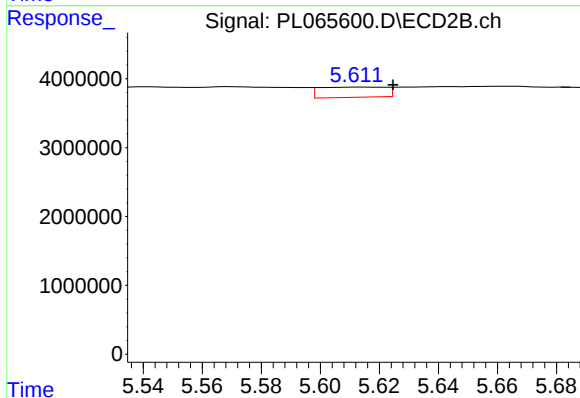


#8 Heptachlor epoxide

R.T.: 5.614 min
Delta R.T.: -0.011 min
Response: 2296965
Conc: 0.79 ng/ml

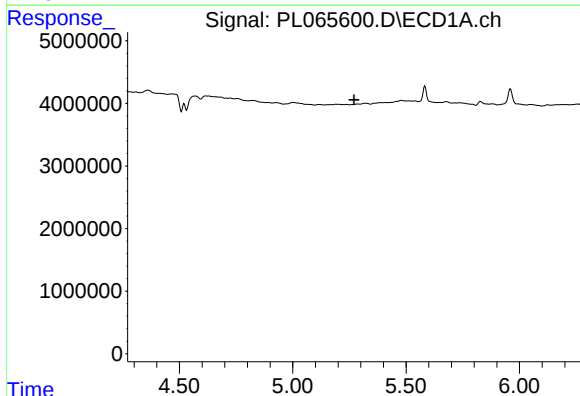


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.271 min
Response: 0
Conc: N.D.

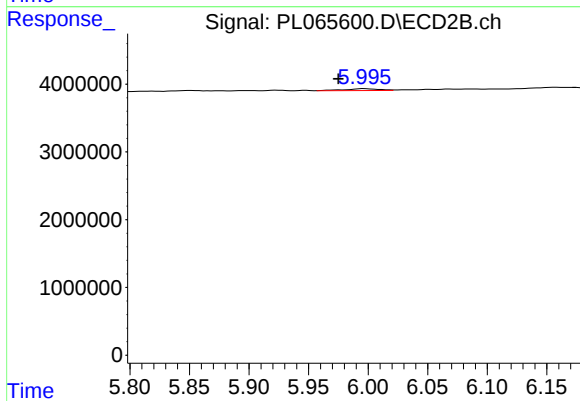

#9 Endosulfan I


R.T.: 5.997 min
Delta R.T.: 0.021 min
Response: 552190
Conc: 0.21 ng/ml

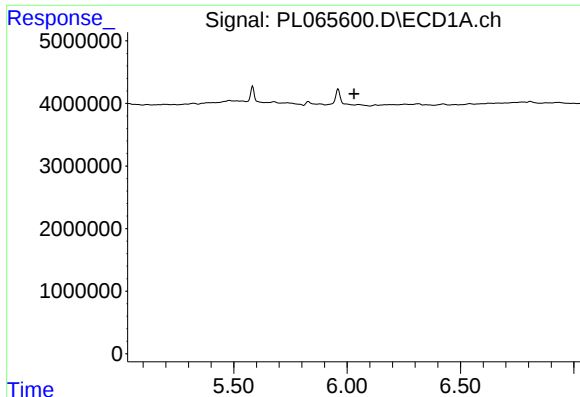

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.031 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

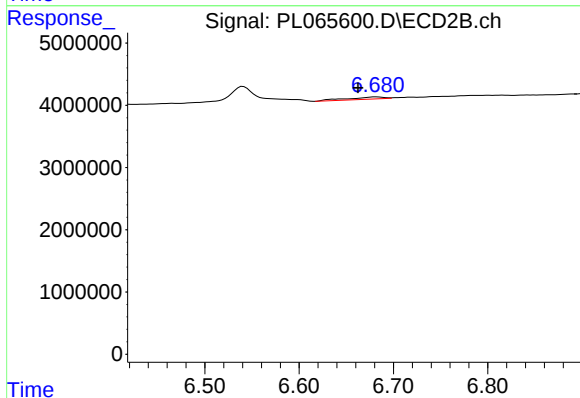


#15 Endosulfan II

R.T.: 6.682 min
Delta R.T.: 0.019 min
Response: 975743
Conc: 0.43 ng/ml

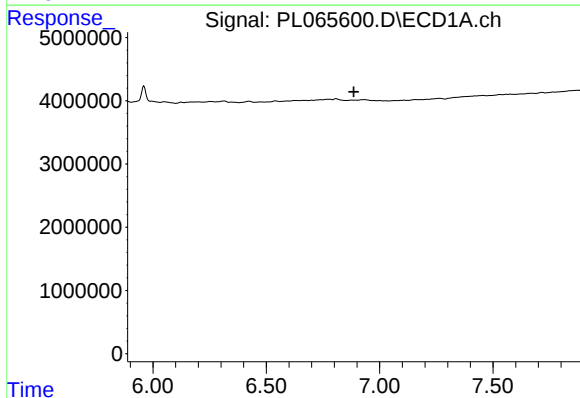


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 6.886 min
Response: 0
Conc: N.D.

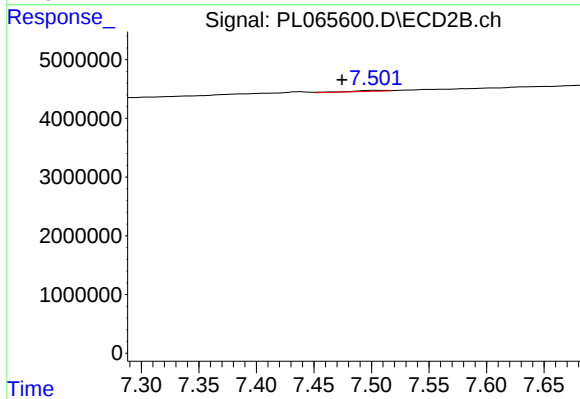

#21 Endrin ketone


R.T.: 7.503 min
Delta R.T.: 0.028 min
Response: 370348
Conc: 0.16 ng/ml

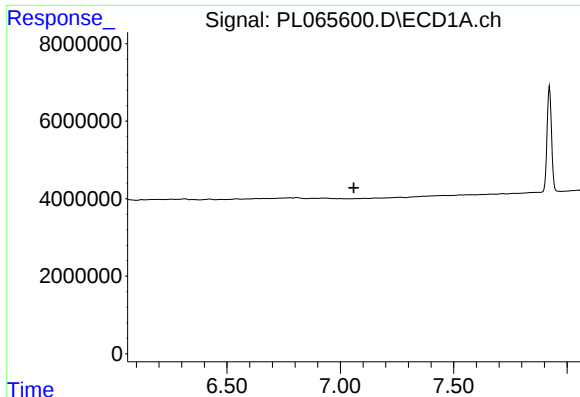

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

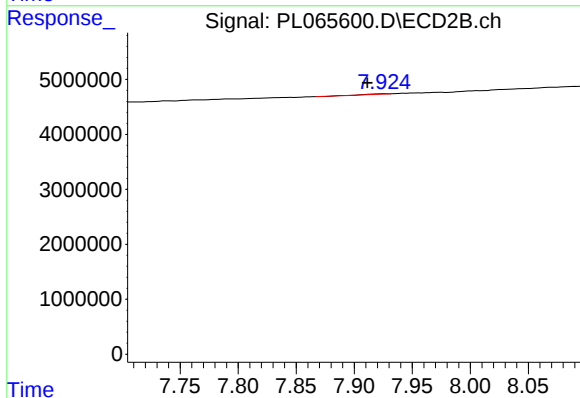


#22 Mirex

R.T.: 7.925 min
Delta R.T.: 0.014 min
Response: 34717
Conc: 0.02 ng/ml

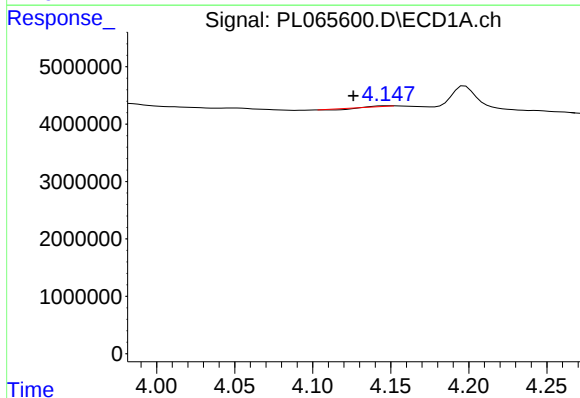


#23 Chlordane-1

R.T.: 4.148 min
Delta R.T.: 0.022 min
Response: 6068
Conc: 0.07 ng/ml

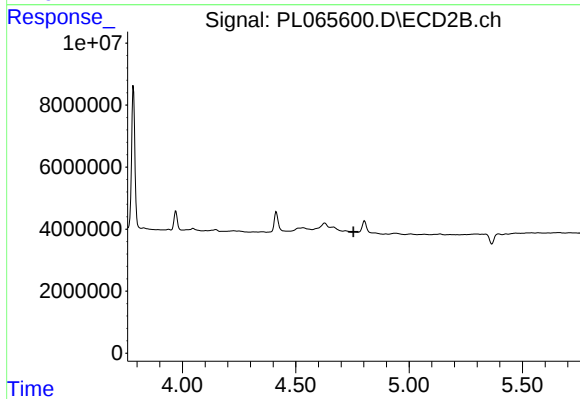

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.755 min
Response: 0
Conc: N.D.

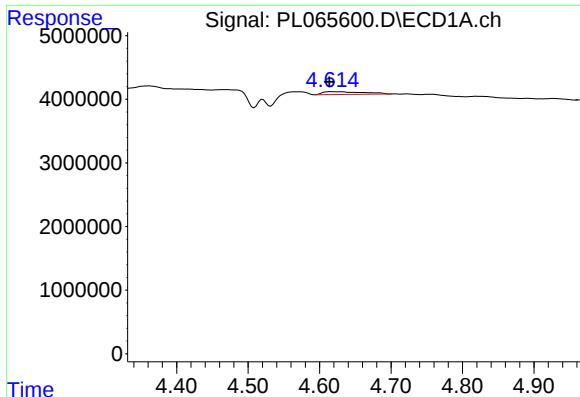

#24 Chlordane-2


R.T.: 4.616 min
Delta R.T.: 0.002 min
Response: 1748380
Conc: 16.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

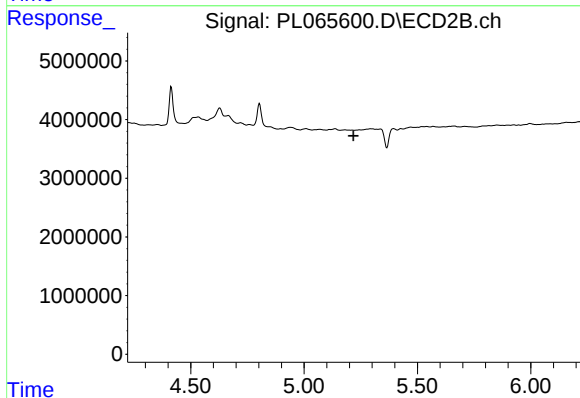


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.219 min
Response: 0
Conc: N.D.

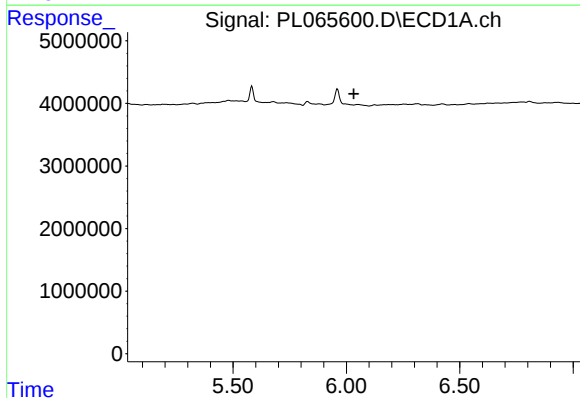


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.033 min
Response: 0
Conc: N.D.

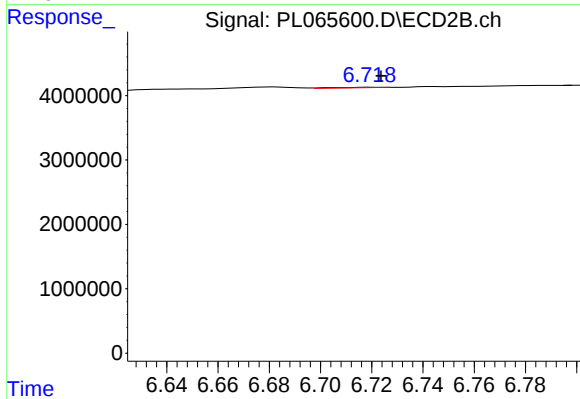

#27 Chlordane-5


R.T.: 6.720 min
Delta R.T.: -0.004 min
Response: 101523
Conc: 1.27 ng/ml

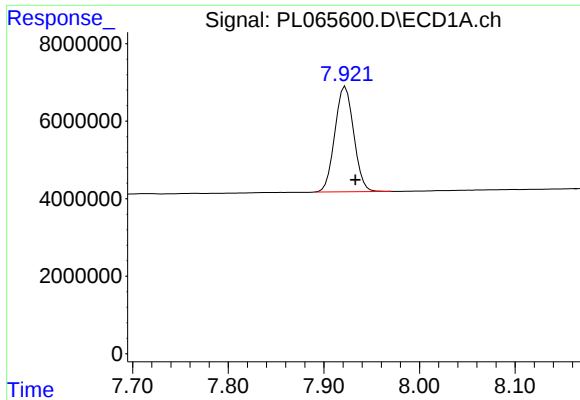

#28 Decachlorobiphenyl

R.T.: 7.922 min
Delta R.T.: -0.010 min
Response: 37255851
Conc: 15.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

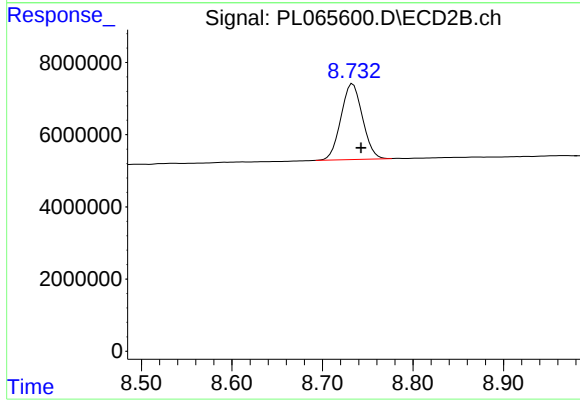

#28 Decachlorobiphenyl

R.T.: 8.733 min
Delta R.T.: -0.009 min
Response: 34804410
Conc: 17.56 ng/ml