

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032621\
 Data File : PL065605.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2021 19:05
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 07:46:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.284	3.784	51871421	56911753	21.843	20.735
28)	SA Decachlor...	7.923	8.734	45450390	43194393	18.812	21.792
Target Compounds							
4)	MA Heptachlor	0.000	4.947	0	929630	N.D.	0.279 #
6)	B beta-BHC	4.240	4.635	1480053	3329126	1.047	1.932 #
8)	B Heptachlo...	0.000	5.623	0	1313401	N.D.	0.454 #
14)	MA Endrin	5.764	0.000	1268270	0	0.508	N.D. #
15)	B Endosulfa...	0.000	6.642f	0	850376	N.D.	0.377 #
16)	A 4,4'-DDD	0.000	6.591	0	1512398	N.D.	0.688 #
17)	MA 4,4'-DDT	6.128	0.000	761237	0	0.402	N.D. #
18)	B Endrin al...	6.199	0.000	604783	0	0.315	N.D. #
21)	B Endrin ke...	0.000	7.474	0	357793	N.D.	0.152 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032621\
Data File : PL065605.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2021 19:05
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 07:46:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

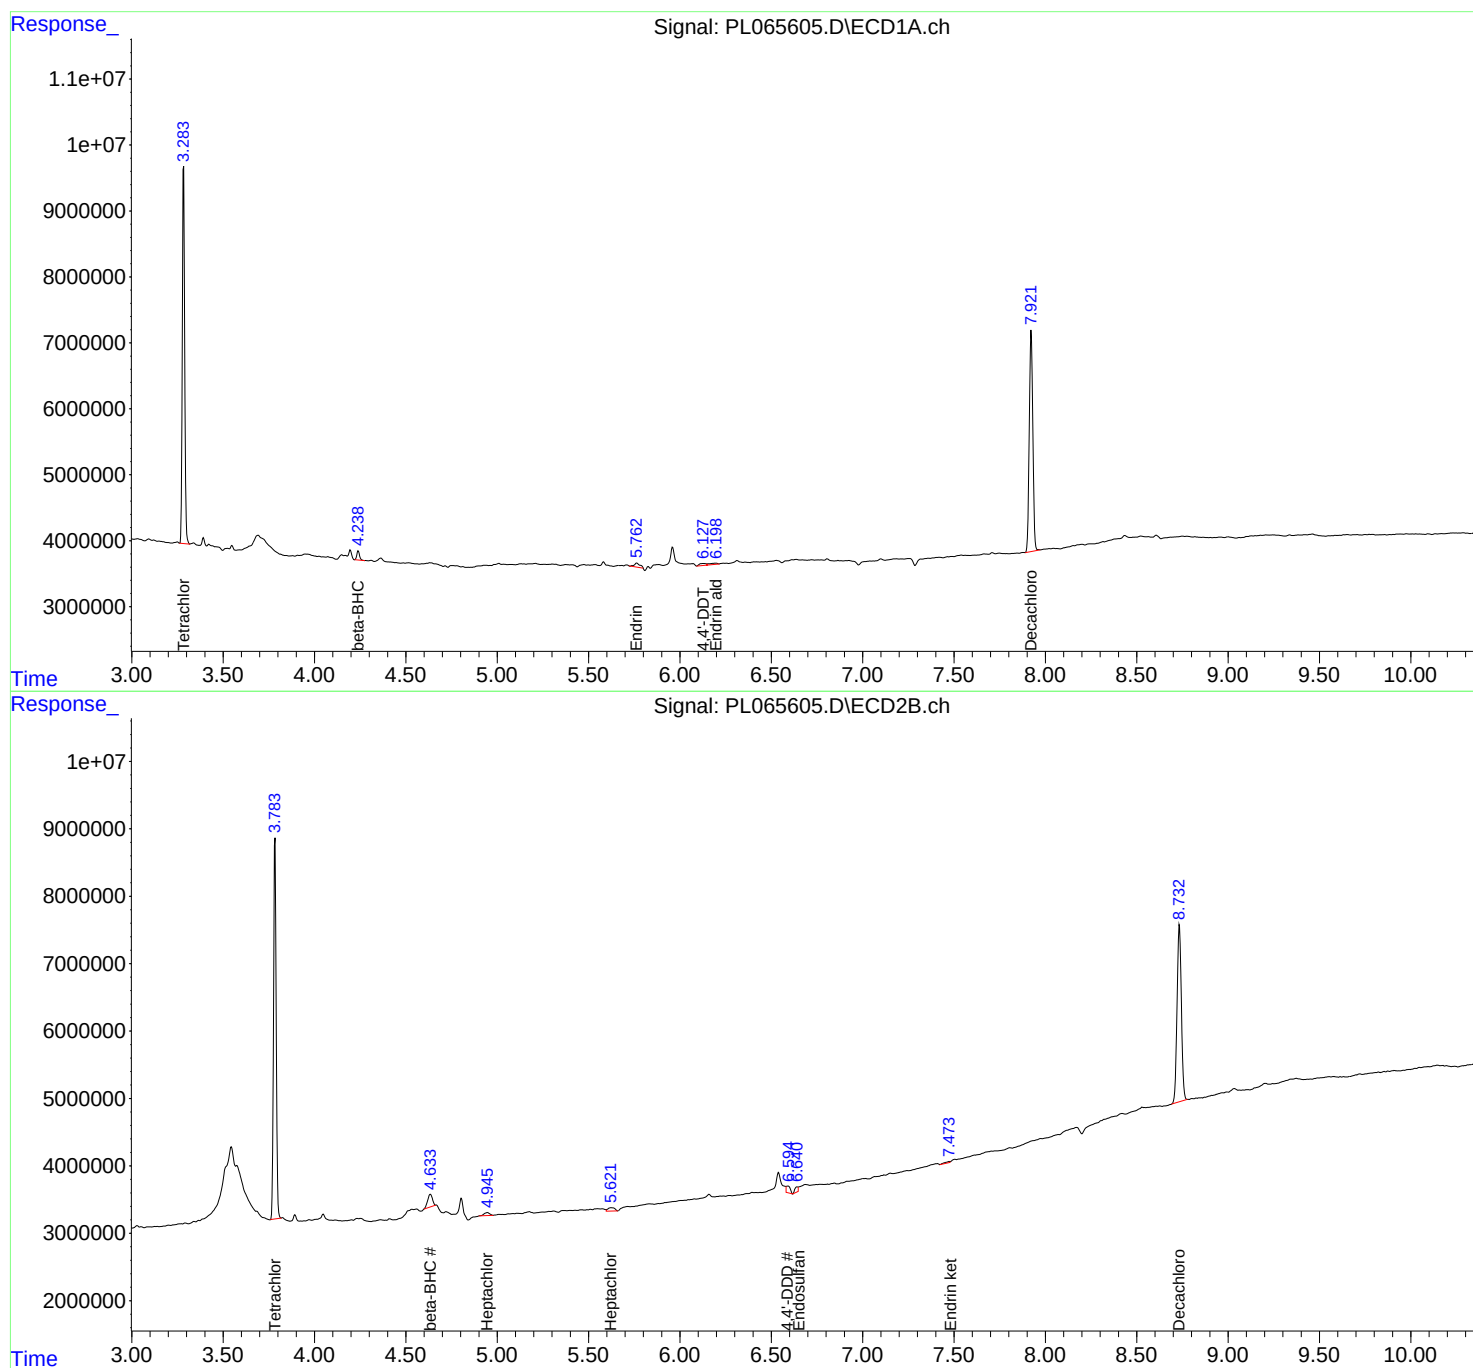


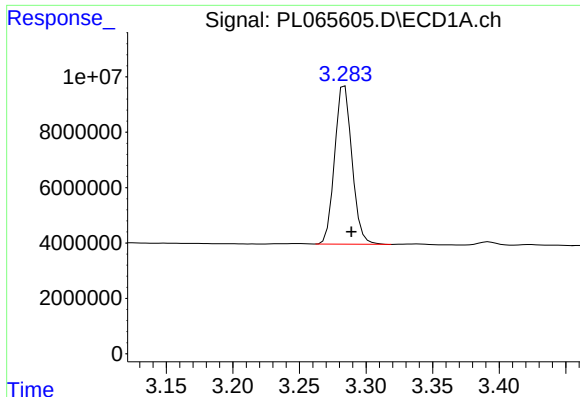

#1 Tetrachloro-m-xylene


R.T.: 3.284 min
Delta R.T.: -0.005 min
Response: 51871421
Conc: 21.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

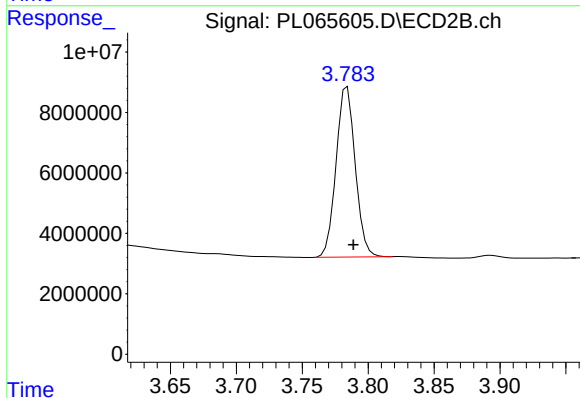


#1 Tetrachloro-m-xylene

R.T.: 3.784 min
Delta R.T.: -0.005 min
Response: 56911753
Conc: 20.73 ng/ml

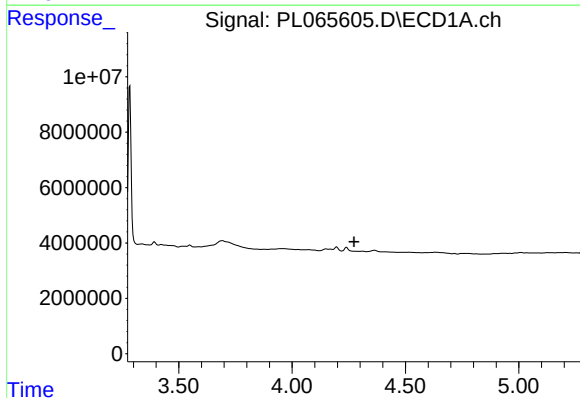


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.274 min
Response: 0
Conc: N.D.

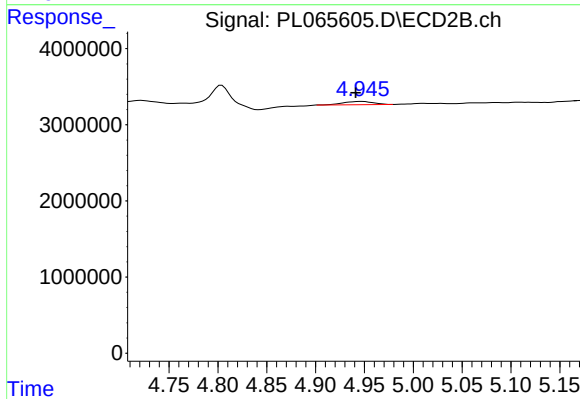

#4 Heptachlor


R.T.: 4.947 min
Delta R.T.: 0.006 min
Response: 929630
Conc: 0.28 ng/ml

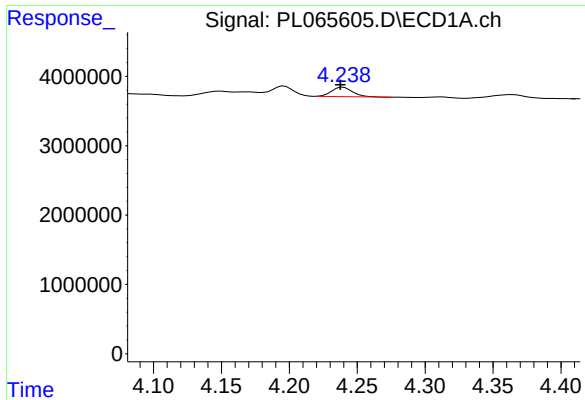

#6 beta-BHC


R.T.: 4.240 min
Delta R.T.: 0.002 min
Response: 1480053
Conc: 1.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

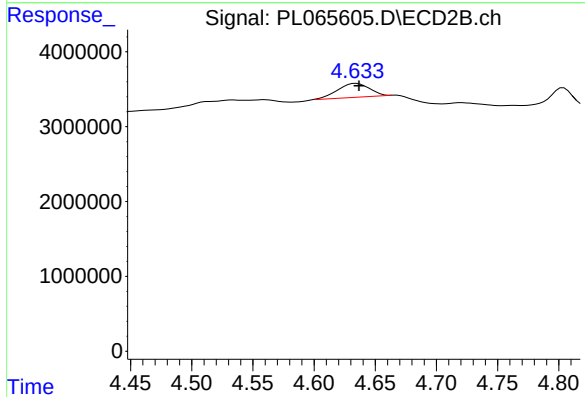


#6 beta-BHC

R.T.: 4.635 min
Delta R.T.: -0.002 min
Response: 3329126
Conc: 1.93 ng/ml

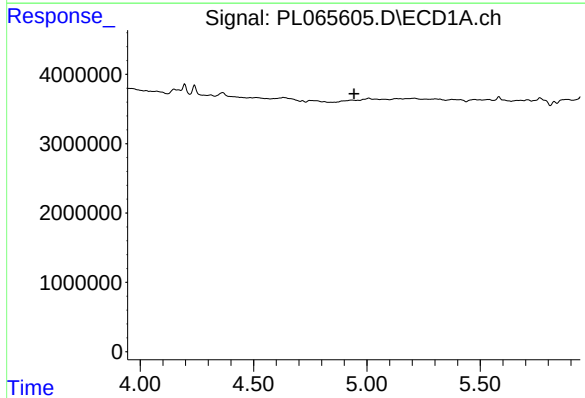


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.944 min
Response: 0
Conc: N.D.

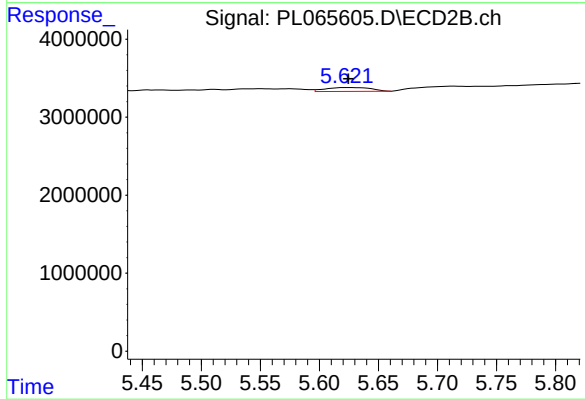

#8 Heptachlor epoxide


R.T.: 5.623 min
Delta R.T.: -0.002 min
Response: 1313401
Conc: 0.45 ng/ml

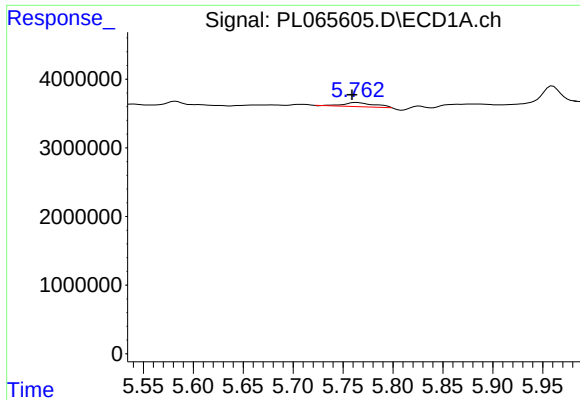

#14 Endrin


R.T.: 5.764 min
Delta R.T.: 0.005 min
Response: 1268270
Conc: 0.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

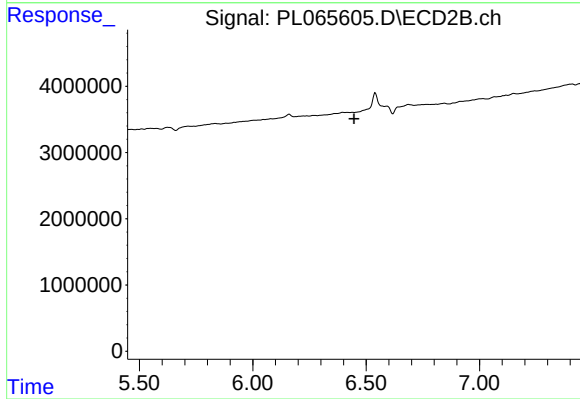


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.446 min
Response: 0
Conc: N.D.

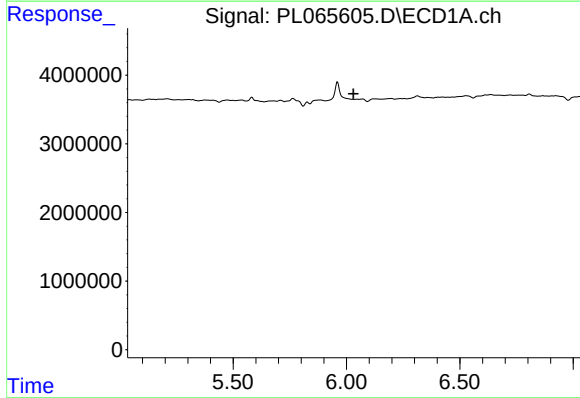


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.031 min
Response: 0
Conc: N.D.

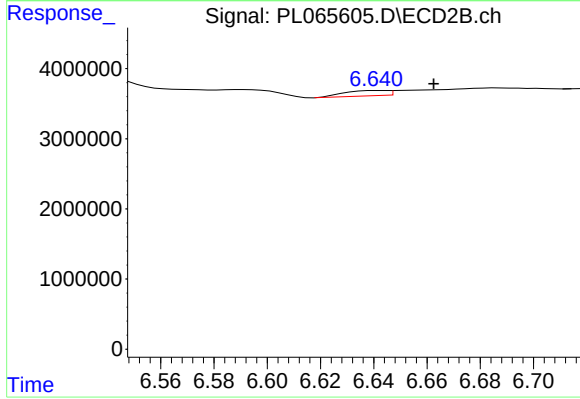

#15 Endosulfan II


R.T.: 6.642 min
Delta R.T.: -0.021 min
Response: 850376
Conc: 0.38 ng/ml

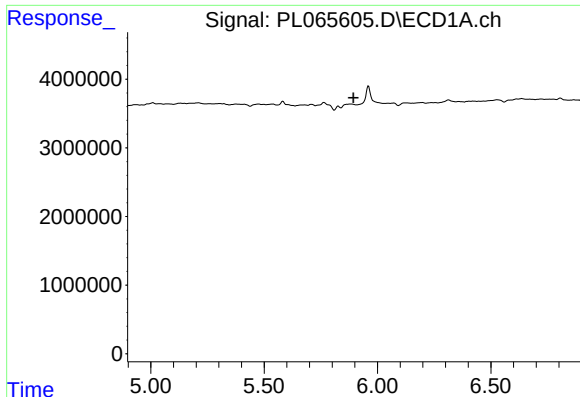

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.894 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

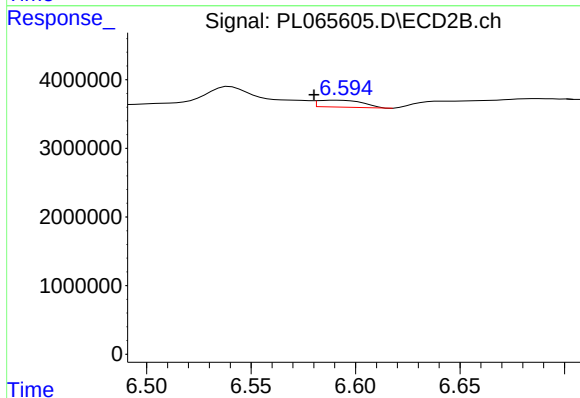


#16 4,4'-DDD

R.T.: 6.591 min
Delta R.T.: 0.011 min
Response: 1512398
Conc: 0.69 ng/ml

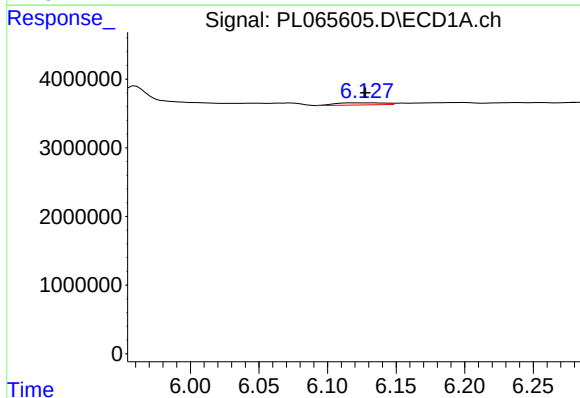


#17 4,4'-DDT

R.T.: 6.128 min
Delta R.T.: 0.000 min
Response: 761237
Conc: 0.40 ng/ml

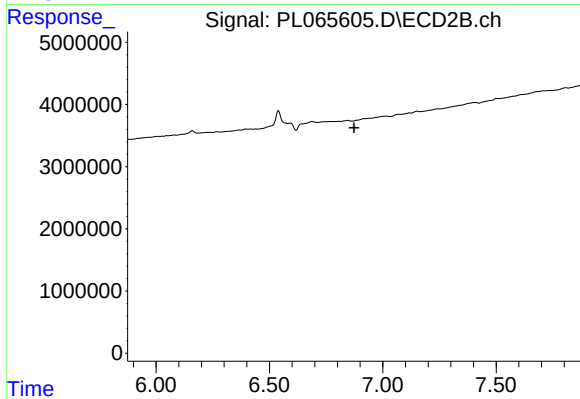

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.873 min
Response: 0
Conc: N.D.

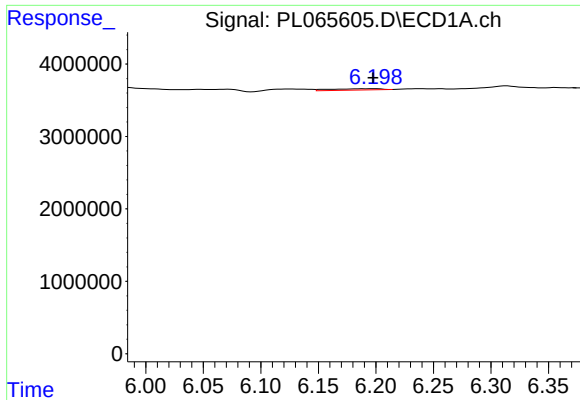

#18 Endrin aldehyde


R.T.: 6.199 min
Delta R.T.: 0.001 min
Response: 604783
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

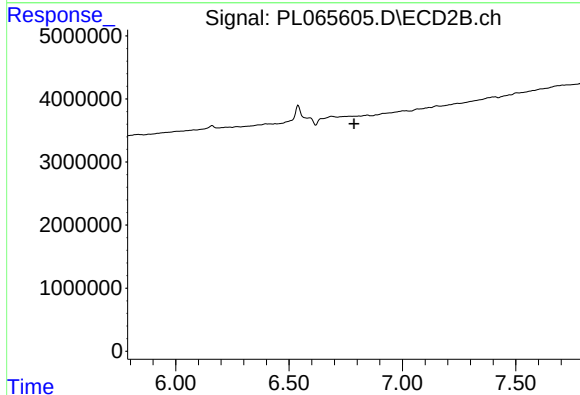


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.787 min
Response: 0
Conc: N.D.

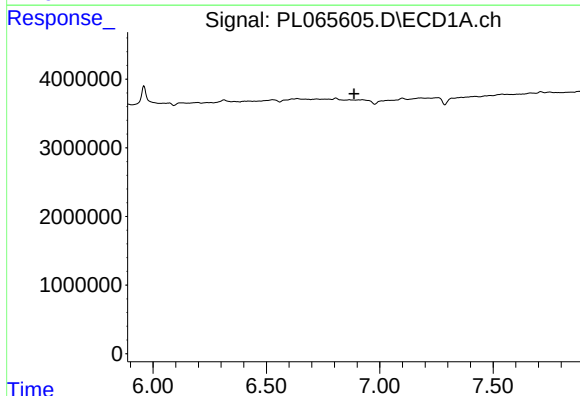


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.886 min
Response: 0
Conc: N.D.

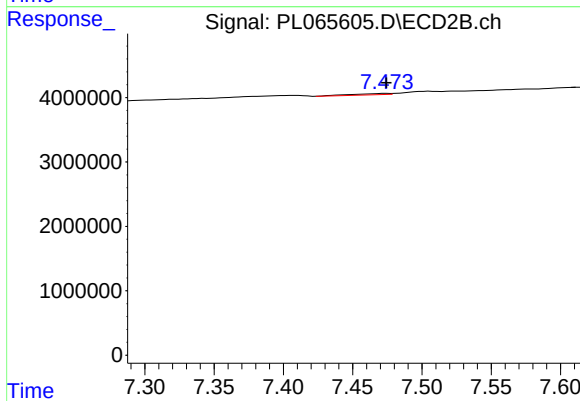

#21 Endrin ketone


R.T.: 7.474 min
Delta R.T.: 0.000 min
Response: 357793
Conc: 0.15 ng/ml

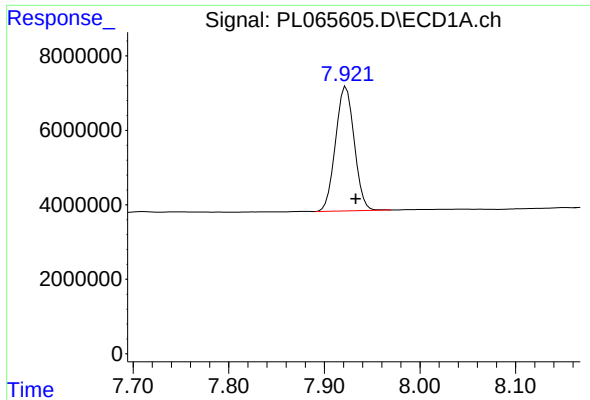

#28 Decachlorobiphenyl

R.T.: 7.923 min
Delta R.T.: -0.010 min
Response: 45450390
Conc: 18.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

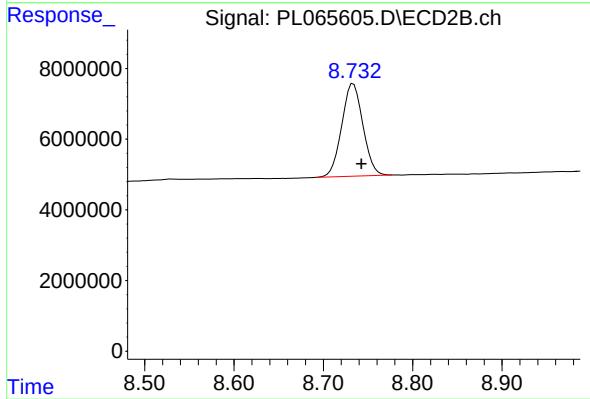

#28 Decachlorobiphenyl

R.T.: 8.734 min
Delta R.T.: -0.009 min
Response: 43194393
Conc: 21.79 ng/ml