

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032621\
 Data File : PL065582.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2021 11:56
 Operator : AR\AJ
 Sample : M1740-03RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TI-604RE

Manual Integrations
 APPROVED

Ankita
 3/30/2021 2:09:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:18:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.291	3.786	183.2E6	95090605	77.134m	34.645 #
28)	SA Decachlor...	7.924	8.735	15875473	12938370	6.571	6.528

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032621\
Data File : PL065582.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2021 11:56
Operator : AR\AJ
Sample : M1740-03RE
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TI-604RE


Manual Integrations
APPROVED

Ankita
3/30/2021 2:09:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:18:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

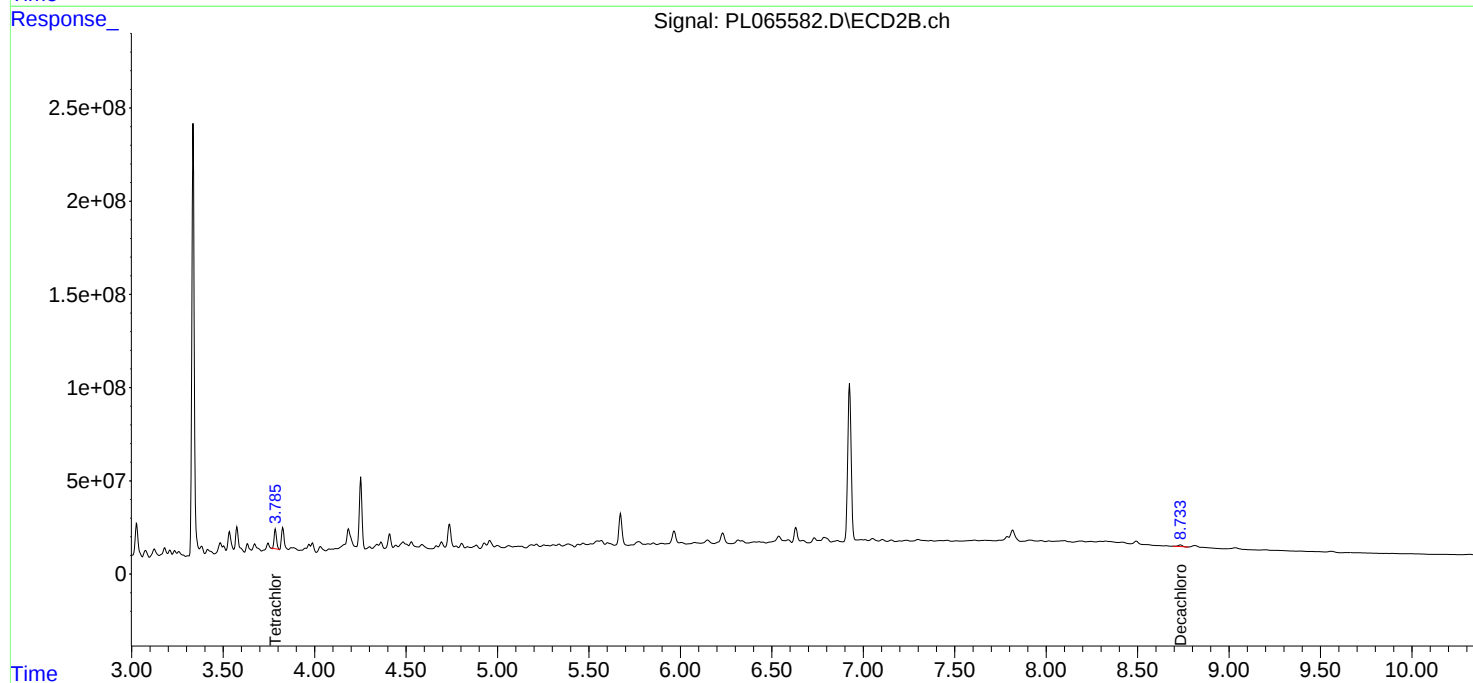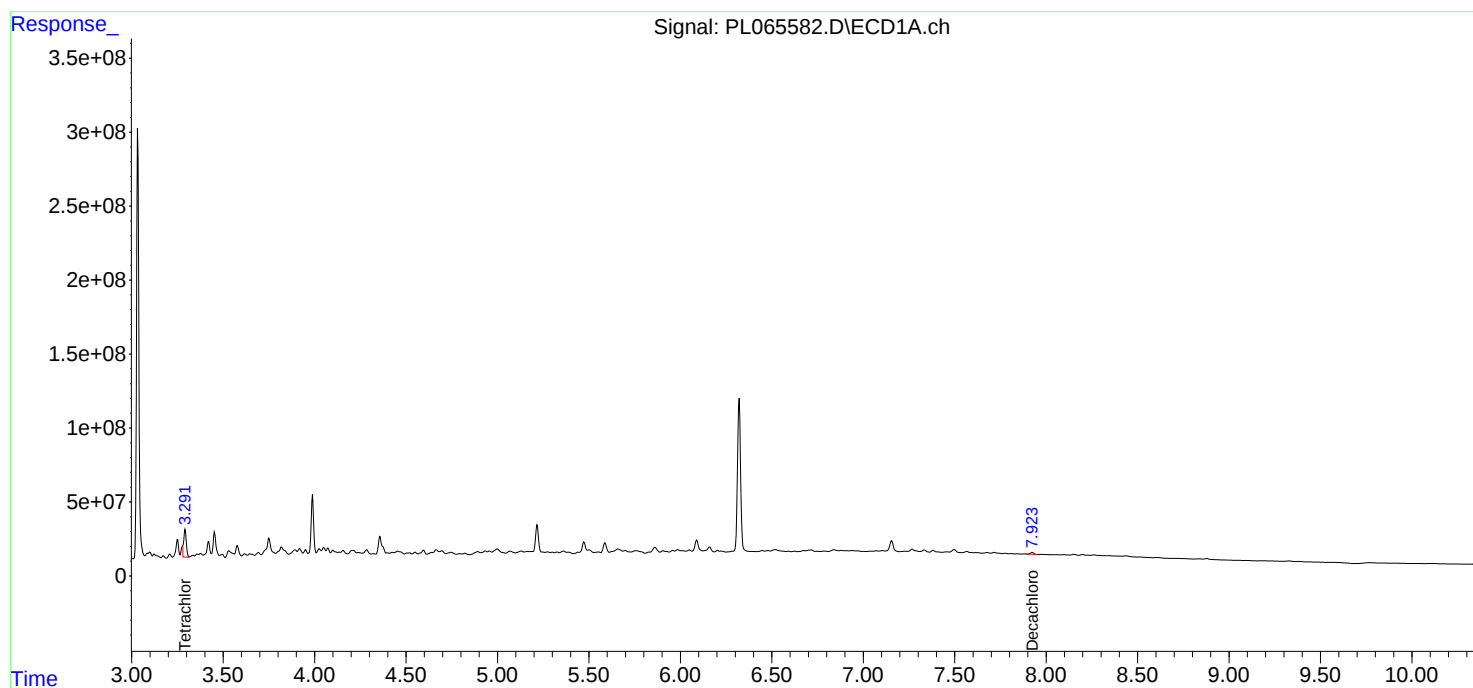

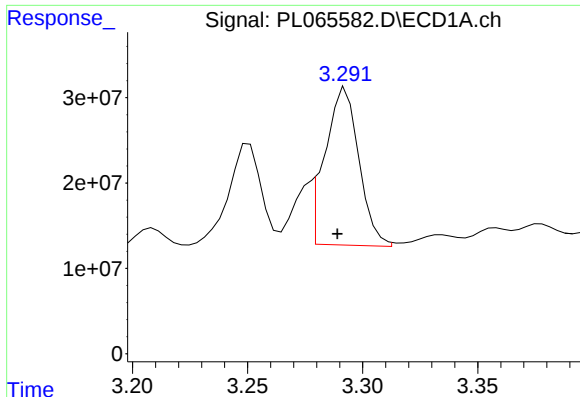


#1 Tetrachloro-m-xylene

R.T.: 3.291 min
Delta R.T.: 0.002 min
Response: 183175873
Conc: 77.13 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TI-604RE


Manual Integrations
APPROVED

Ankita
3/30/2021 2:09:44 PM

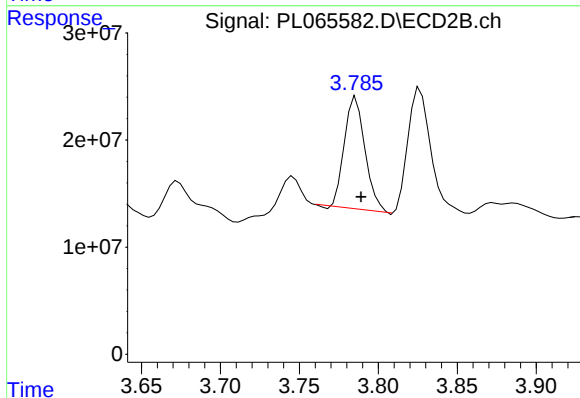


#1 Tetrachloro-m-xylene

R.T.: 3.786 min
Delta R.T.: -0.003 min
Response: 95090605
Conc: 34.64 ng/ml

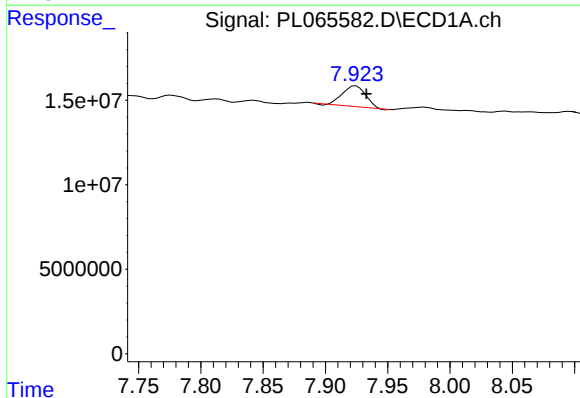

#28 Decachlorobiphenyl

R.T.: 7.924 min
Delta R.T.: -0.009 min
Response: 15875473
Conc: 6.57 ng/ml

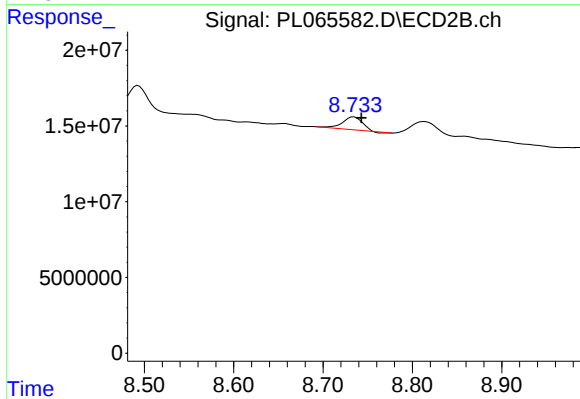

#28 Decachlorobiphenyl

R.T.: 8.735 min
Delta R.T.: -0.008 min
Response: 12938370
Conc: 6.53 ng/ml