

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032621\
 Data File : PL065615.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2021 21:28
 Operator : AR\AJ
 Sample : M1817-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PHC-326FB-002

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 07:48:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.283	3.784	32400416	35988211	13.643	13.112
28)	SA Decachlor...	7.921	8.734	27815450	25770604	11.513	13.002
Target Compounds							
12)	B 4,4'-DDE	5.378	6.078	1952750	2324710	0.742	0.933 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032621\
Data File : PL065615.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2021 21:28
Operator : AR\AJ
Sample : M1817-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PHC-326FB-002

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 07:48:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

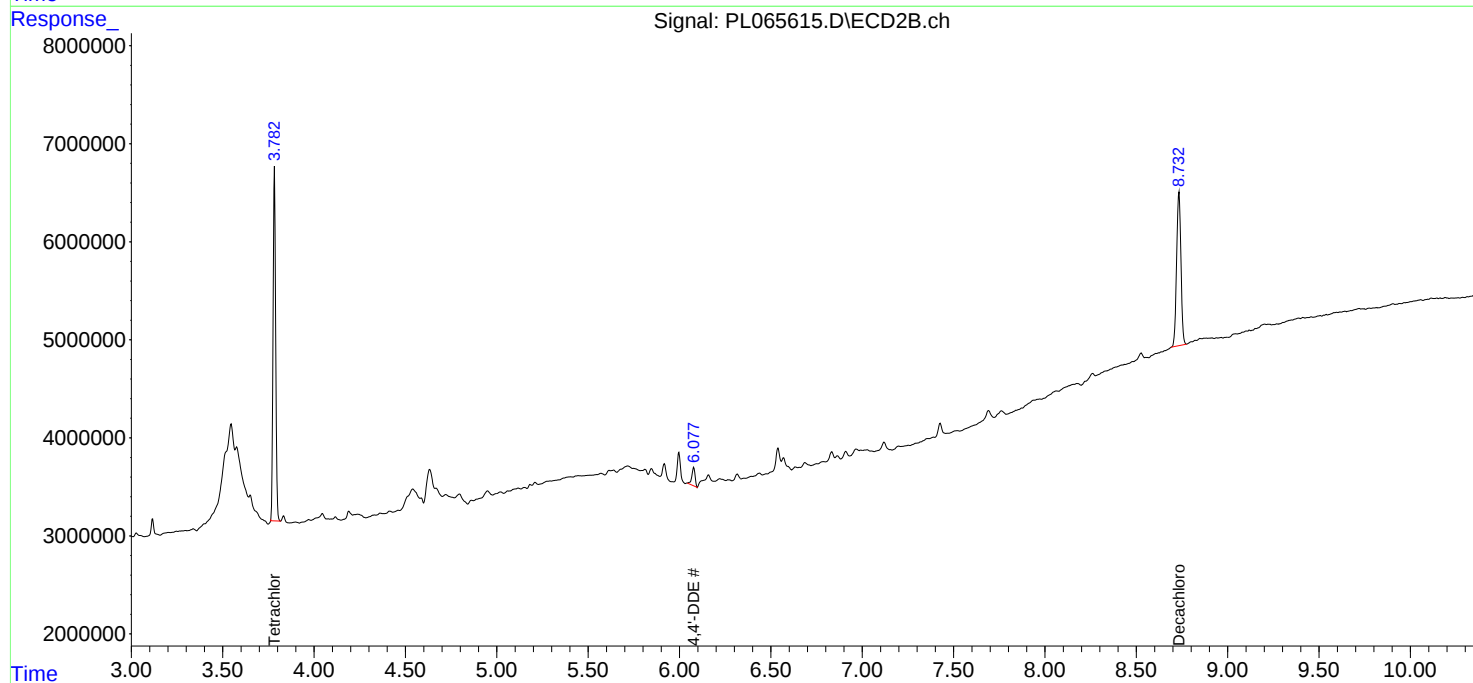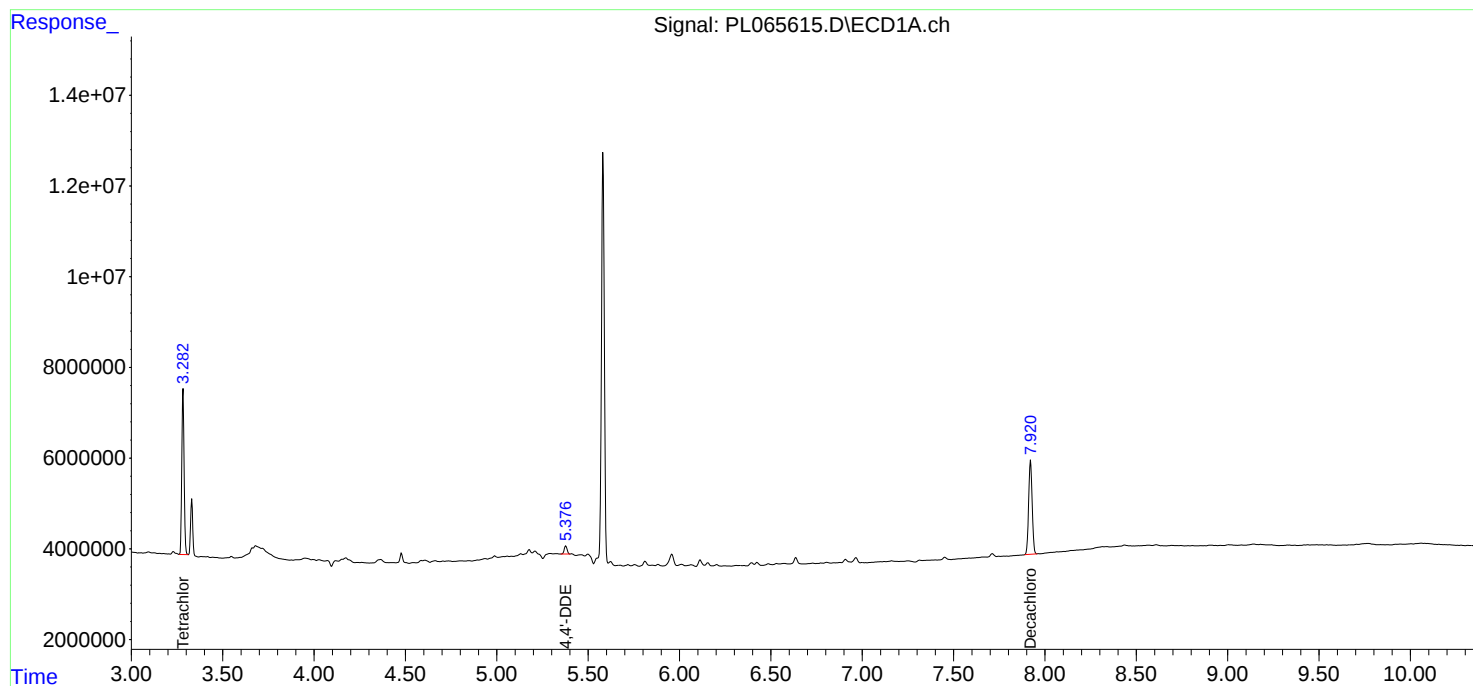


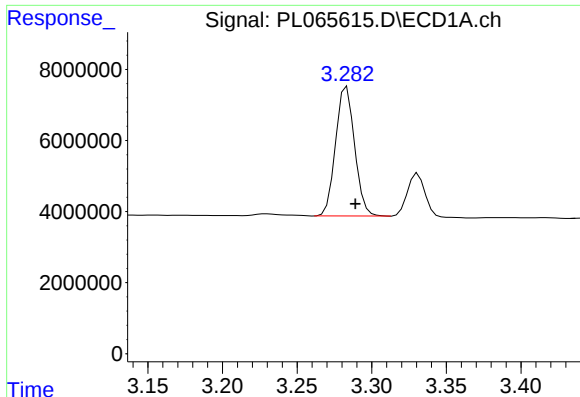

#1 Tetrachloro-m-xylene


R.T.: 3.283 min
Delta R.T.: -0.006 min
Response: 32400416
Conc: 13.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PHC-326FB-002

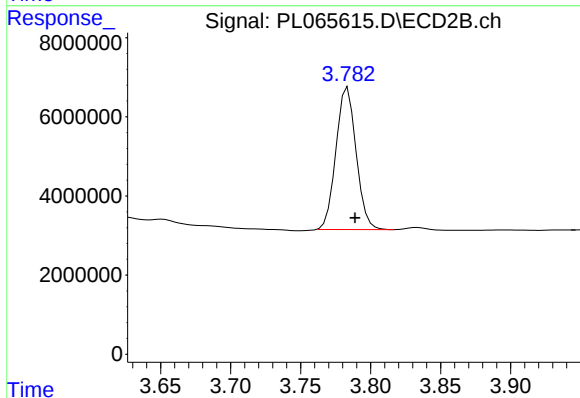


#1 Tetrachloro-m-xylene

R.T.: 3.784 min
Delta R.T.: -0.005 min
Response: 35988211
Conc: 13.11 ng/ml

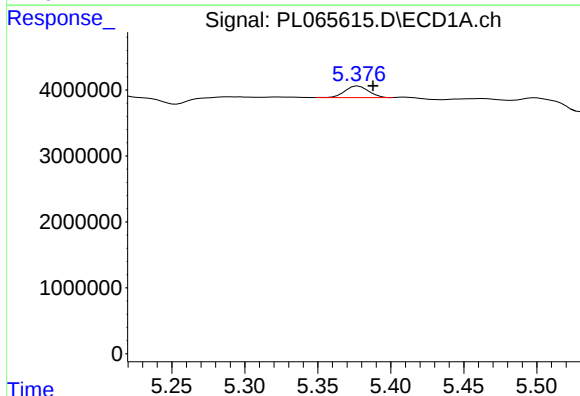


#12 4,4'-DDE

R.T.: 5.378 min
Delta R.T.: -0.010 min
Response: 1952750
Conc: 0.74 ng/ml

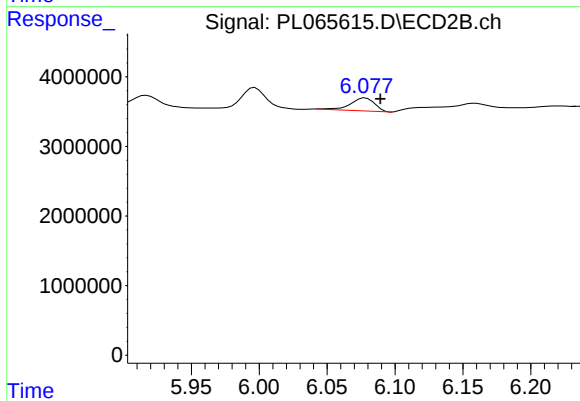

#12 4,4'-DDE


R.T.: 6.078 min
Delta R.T.: -0.011 min
Response: 2324710
Conc: 0.93 ng/ml

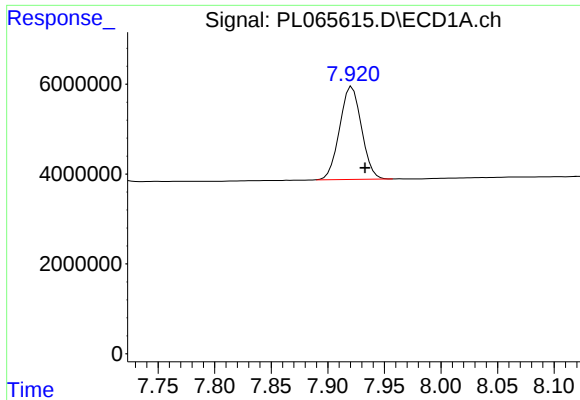

#28 Decachlorobiphenyl

R.T.: 7.921 min
Delta R.T.: -0.012 min
Response: 27815450
Conc: 11.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
PHC-326FB-002

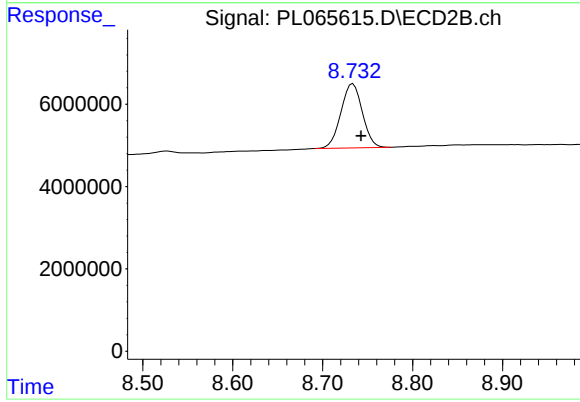

#28 Decachlorobiphenyl

R.T.: 8.734 min
Delta R.T.: -0.009 min
Response: 25770604
Conc: 13.00 ng/ml