

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032624\
 Data File : PL088778.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2024 13:30
 Operator : AR\AJ
 Sample : P1861-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HD-02-03252024

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/27/2024
 Supervised By :Ankita Jodhani 03/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 22:39:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:45:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.633	2.852	26413650	15064161	9.968	11.303
28)	SA Decachlor...	9.296	8.077	22659530	13525967	9.167	9.975
Target Compounds							
12)	B 4,4'-DDE	6.326	5.357	2698499	1093868	0.903m	0.750

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032624\
Data File : PL088778.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2024 13:30
Operator : AR\AJ
Sample : P1861-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HD-02-03252024


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/27/2024
Supervised By : Ankita Jodhani 03/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 22:39:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:45:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

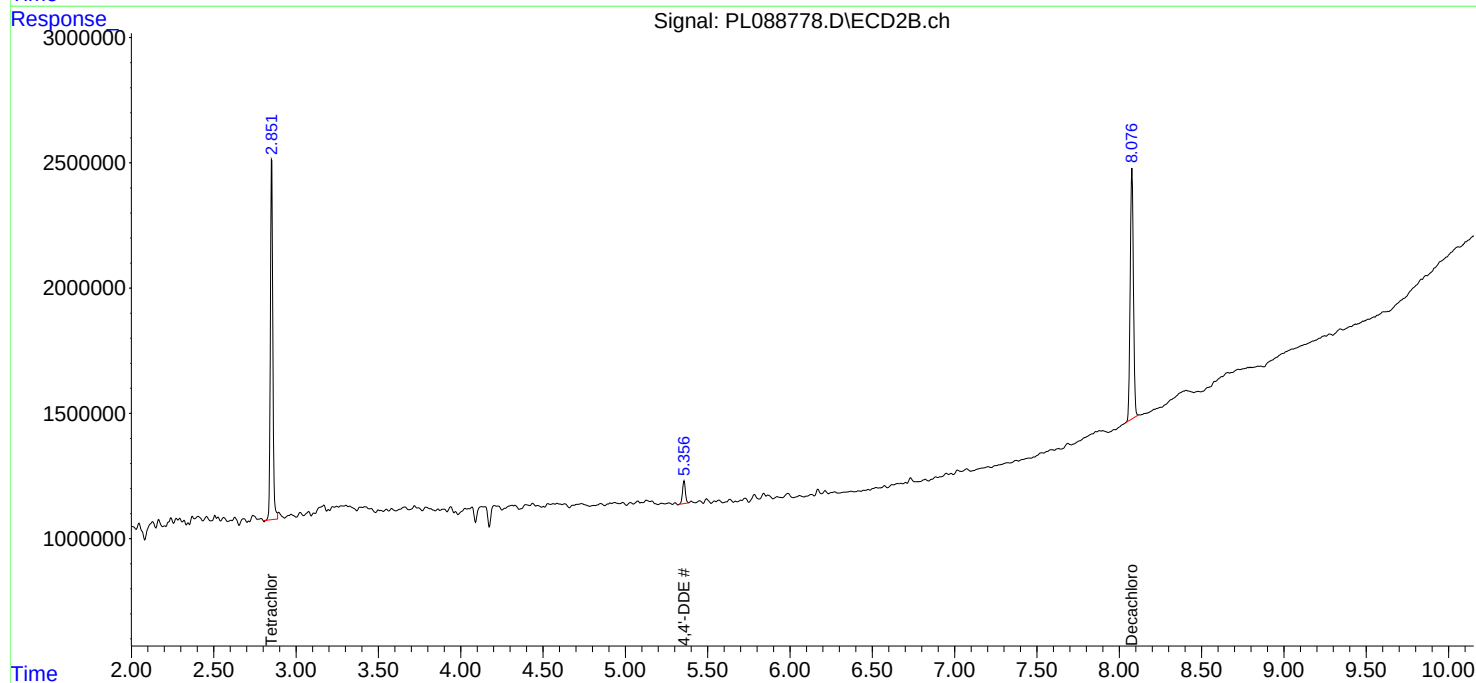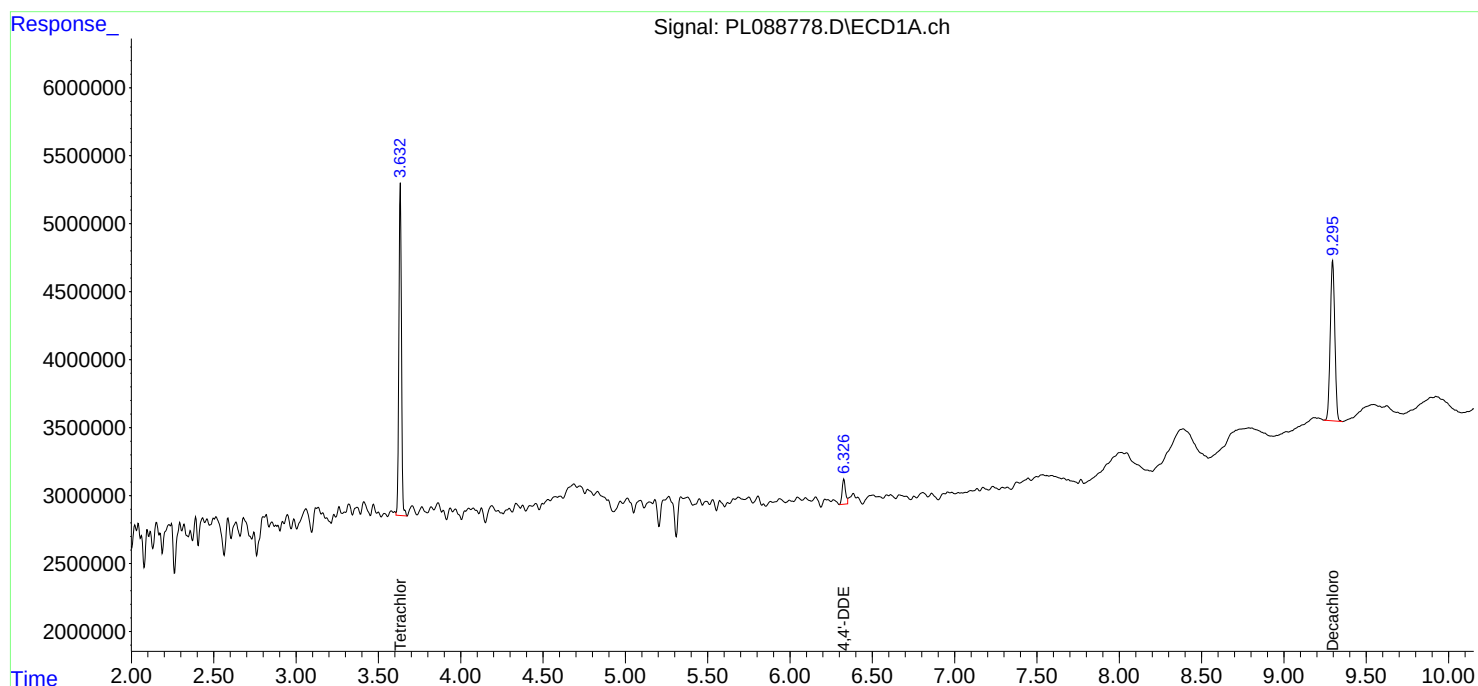

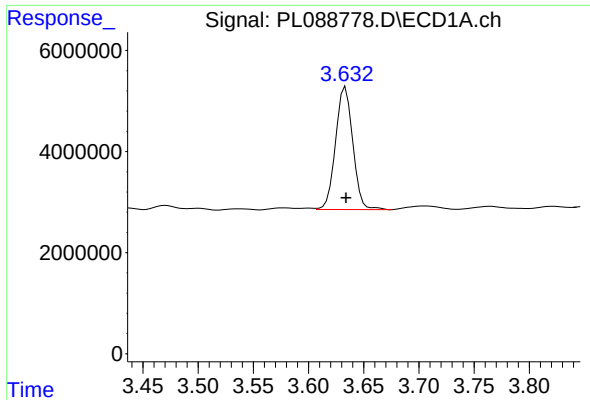


#1 Tetrachloro-m-xylene

R.T.: 3.633 min
Delta R.T.: 0.000 min
Response: 26413650
Conc: 9.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-02-03252024


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/27/2024
Supervised By :Ankita Jodhani 03/27/2024

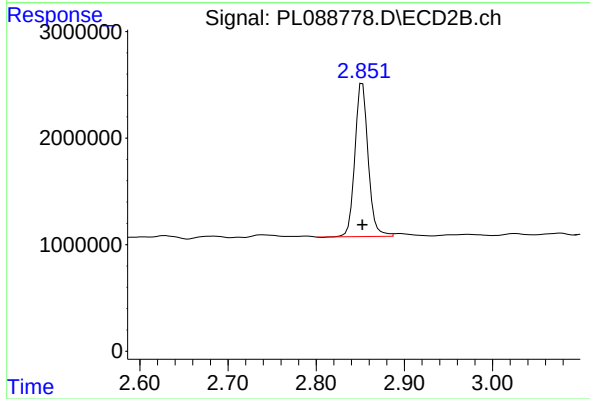


#1 Tetrachloro-m-xylene

R.T.: 2.852 min
Delta R.T.: 0.000 min
Response: 15064161
Conc: 11.30 ng/ml

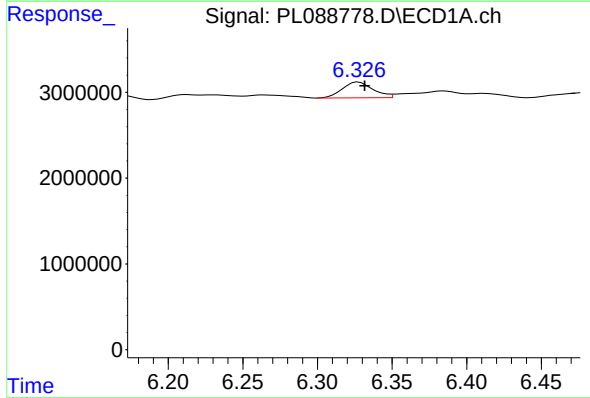


#12 4,4'-DDE

R.T.: 6.326 min
Delta R.T.: -0.005 min
Response: 2698499
Conc: 0.90 ng/ml m

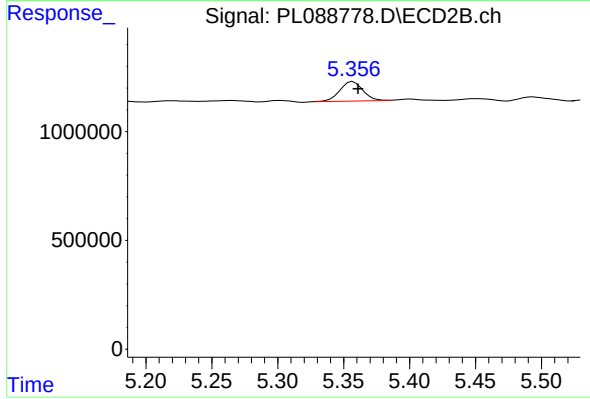

#12 4,4'-DDE

R.T.: 5.357 min
Delta R.T.: -0.004 min
Response: 1093868
Conc: 0.75 ng/ml

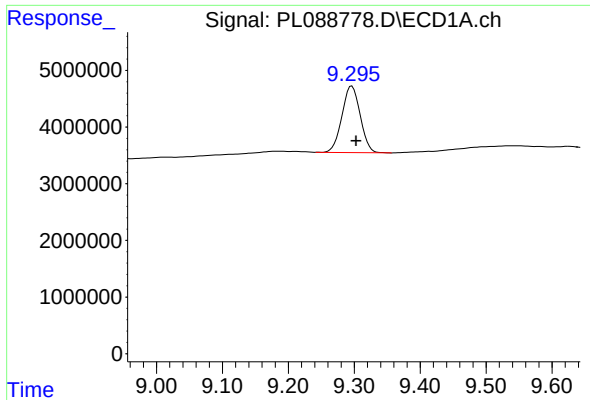


#28 Decachlorobiphenyl

R.T.: 9.296 min
Delta R.T.: -0.006 min
Response: 22659530
Conc: 9.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-02-03252024

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/27/2024
Supervised By :Ankita Jodhani 03/27/2024

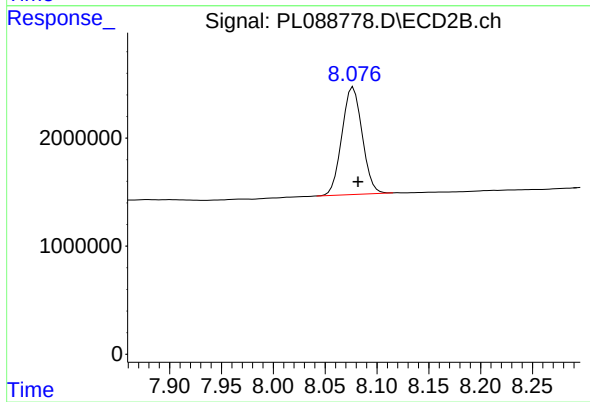

#28 Decachlorobiphenyl

R.T.: 8.077 min
Delta R.T.: -0.005 min
Response: 13525967
Conc: 9.98 ng/ml