

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032625\
 Data File : PL094881.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2025 17:31
 Operator : AR\AJ
 Sample : Q1637-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-02-032525

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 02:06:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.769	27982507	52444462	9.885	14.693 #
28)	SA Decachlor...	9.051	7.903	27236543	34711630	12.924	8.593 #
Target Compounds							
6)	B beta-BHC	4.542f	3.909	1909145	3952511	1.035	1.779 #
9)	A Endosulfan I	0.000	5.109f	0	8533098	N.D.	1.944 #
10)	B gamma-Chl...	5.935	0.000	19816317	0	5.881	N.D. #
11)	B alpha-Chl...	6.016	0.000	7701432	0	2.336	N.D. #
12)	B 4,4'-DDE	0.000	5.223	0	11505618	N.D.	2.475 #
23)	Chlordane-1	0.000	3.766	0	12238293	N.D.	81.031 #
24)	Chlordane-2	0.000	4.375f	0	9042114	N.D.	51.205 #
25)	Chlordane-3	5.935	0.000	19816317	0	39.647	N.D. #
26)	Chlordane-4	6.016	0.000	7701432	0	13.073	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032625\
Data File : PL094881.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2025 17:31
Operator : AR\AJ
Sample : Q1637-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EO-02-032525

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 02:06:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

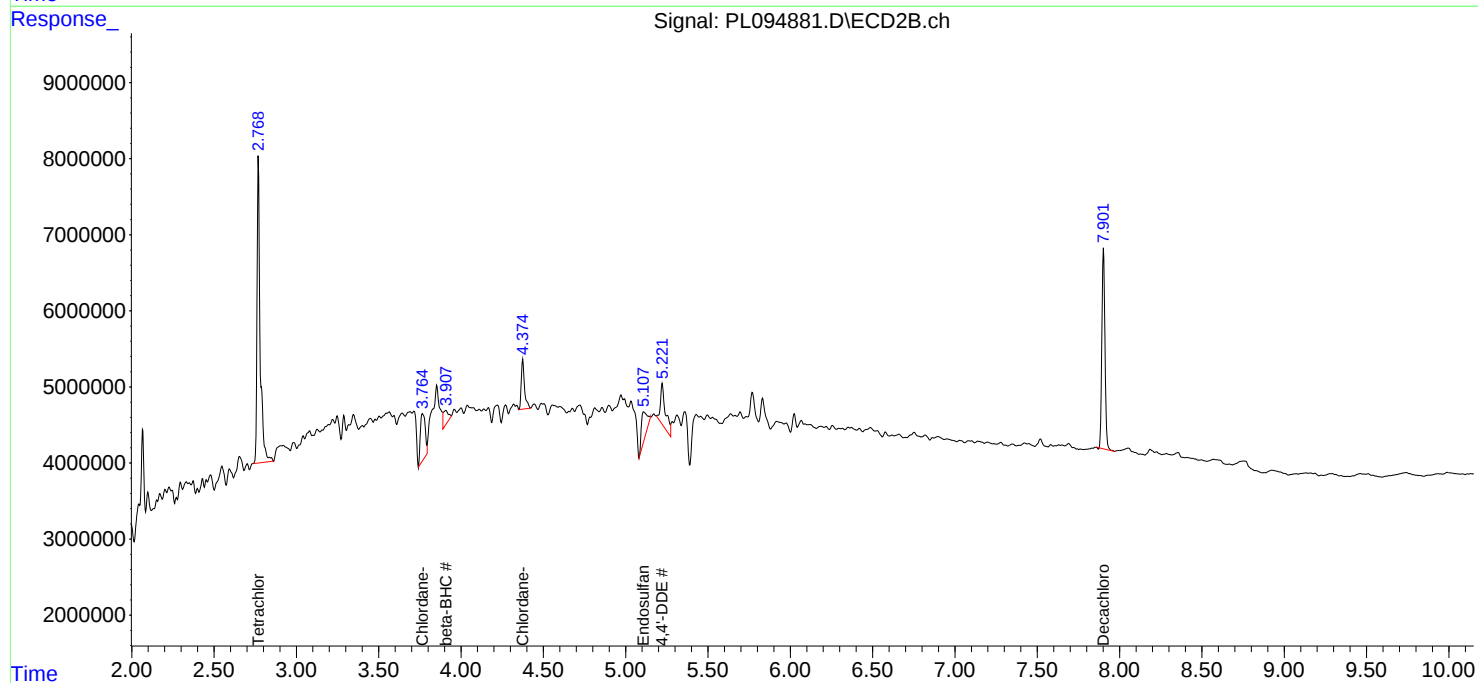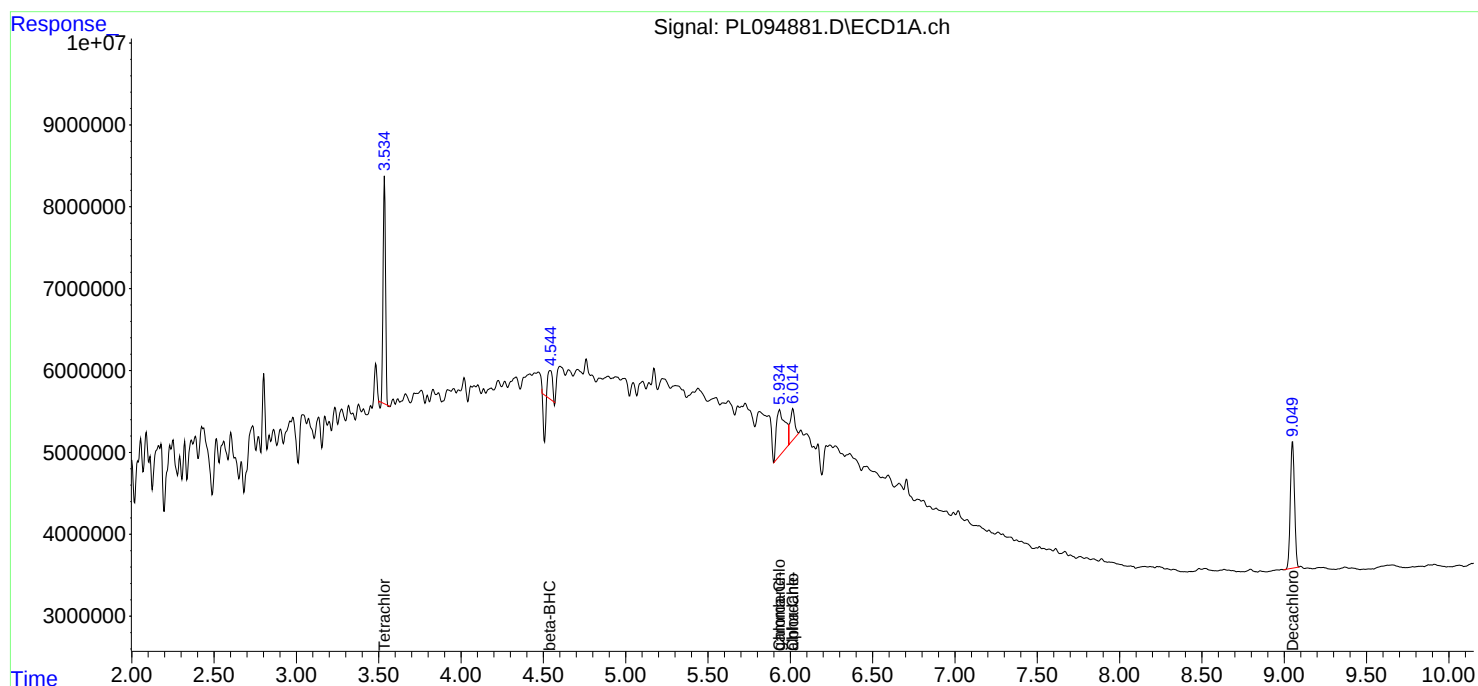


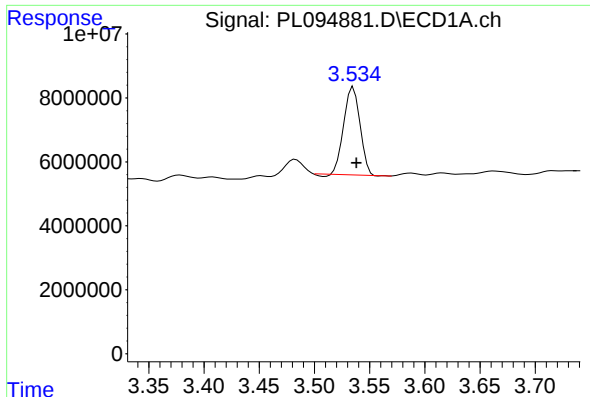

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: -0.003 min
Response: 27982507
Conc: 9.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-032525

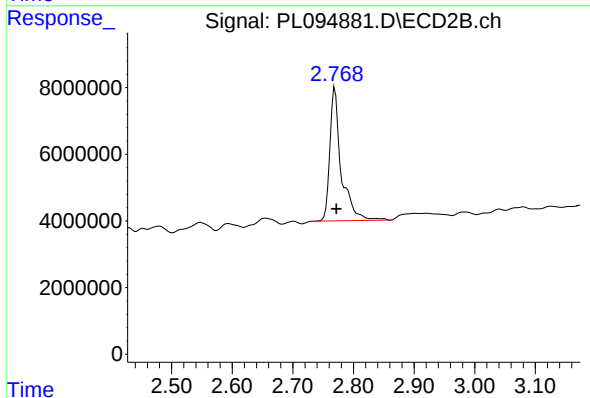


#1 Tetrachloro-m-xylene

R.T.: 2.769 min
Delta R.T.: -0.002 min
Response: 52444462
Conc: 14.69 ng/ml

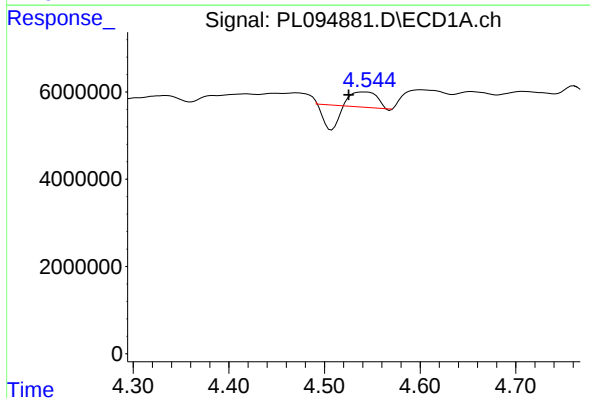


#6 beta-BHC

R.T.: 4.542 min
Delta R.T.: 0.016 min
Response: 1909145
Conc: 1.03 ng/ml

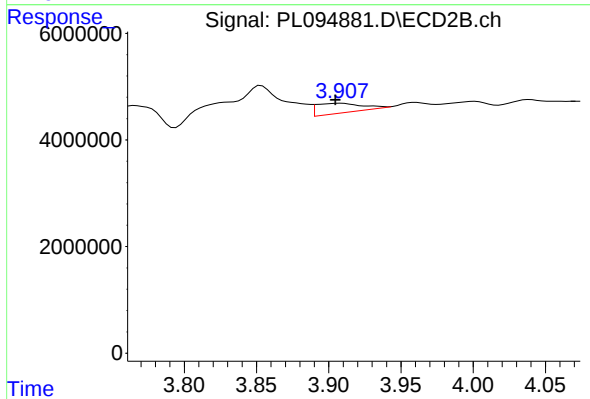

#6 beta-BHC


R.T.: 3.909 min
Delta R.T.: 0.004 min
Response: 3952511
Conc: 1.78 ng/ml

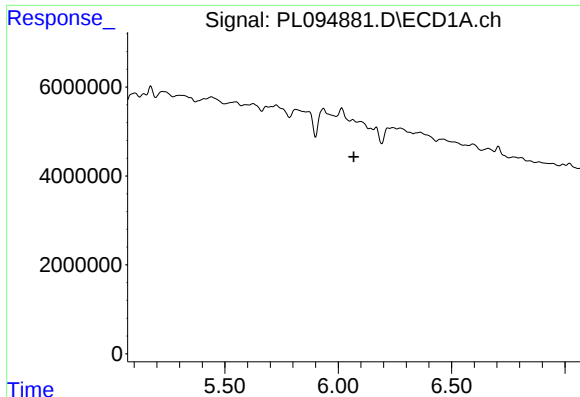

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EO-02-032525

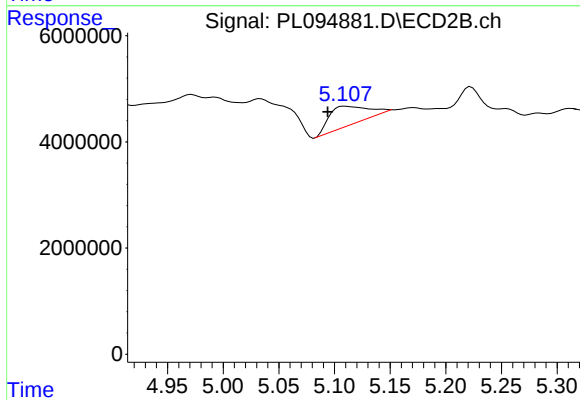


#9 Endosulfan I

R.T.: 5.109 min
Delta R.T.: 0.015 min
Response: 8533098
Conc: 1.94 ng/ml

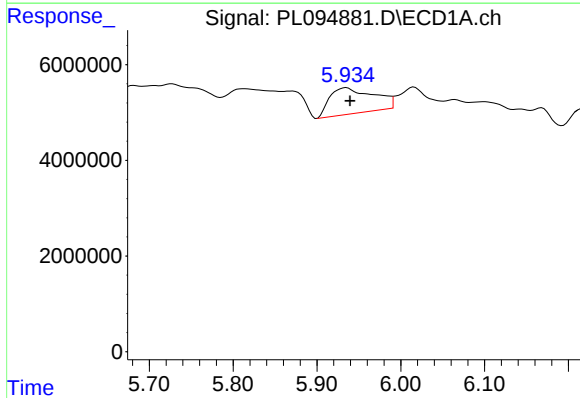


#10 gamma-Chlordane

R.T.: 5.935 min
Delta R.T.: -0.004 min
Response: 19816317
Conc: 5.88 ng/ml

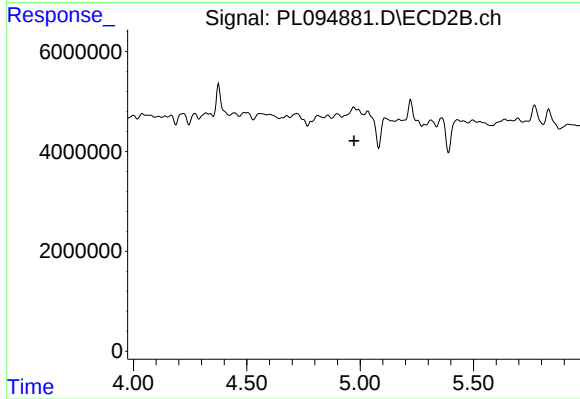

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 4.974 min
Response: 0
Conc: N.D.

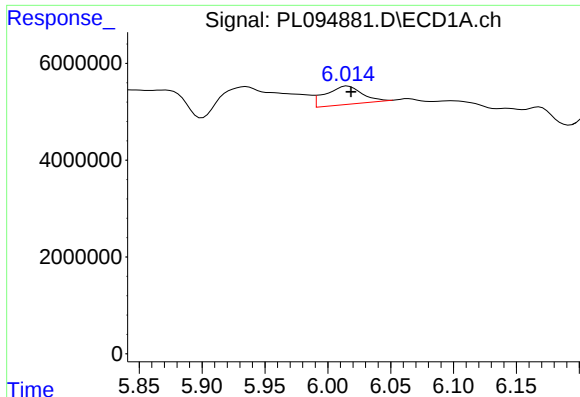

#11 alpha-Chlordane


R.T.: 6.016 min
Delta R.T.: -0.003 min
Response: 7701432
Conc: 2.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-032525

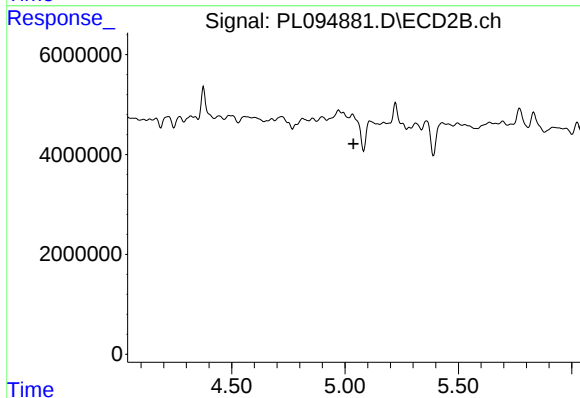


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.038 min
Response: 0
Conc: N.D.

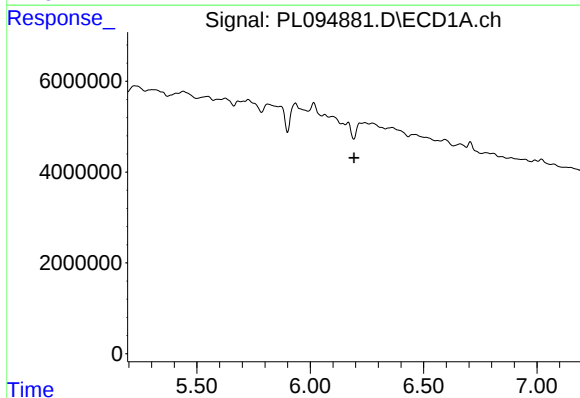


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.193 min
Response: 0
Conc: N.D.

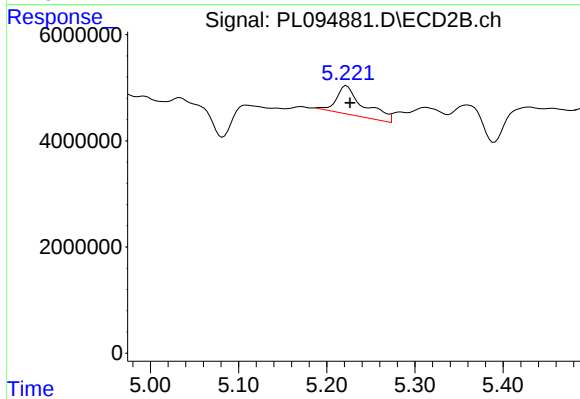

#12 4,4'-DDE


R.T.: 5.223 min
Delta R.T.: -0.004 min
Response: 11505618
Conc: 2.48 ng/ml

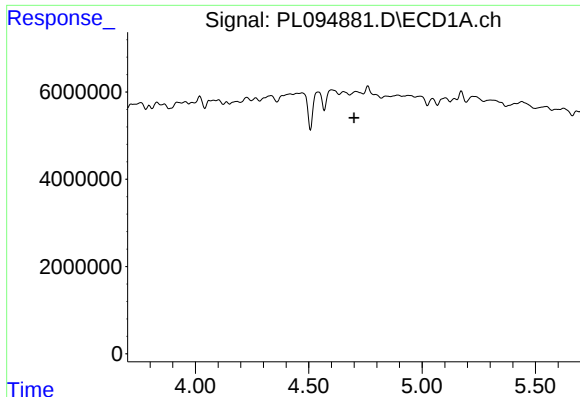

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.700 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EO-02-032525

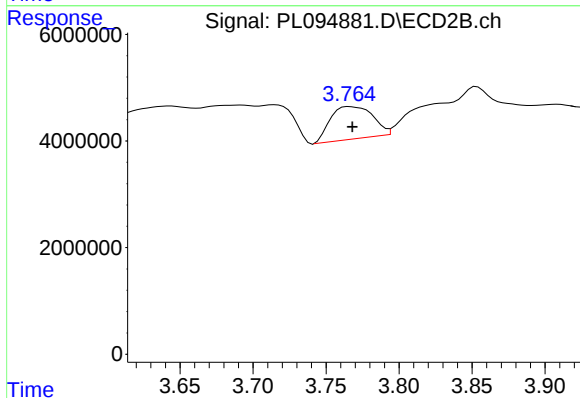


#23 Chlordane-1

R.T.: 3.766 min
Delta R.T.: -0.002 min
Response: 12238293
Conc: 81.03 ng/ml

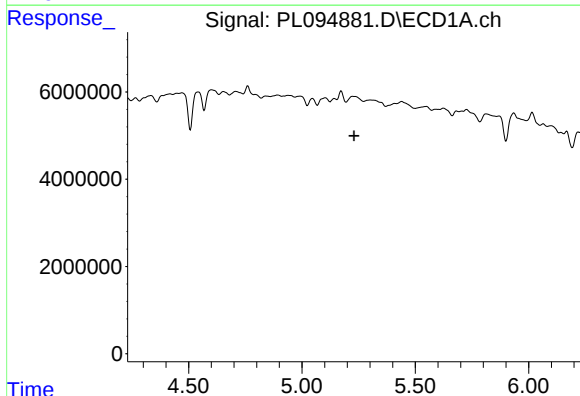


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.230 min
Response: 0
Conc: N.D.

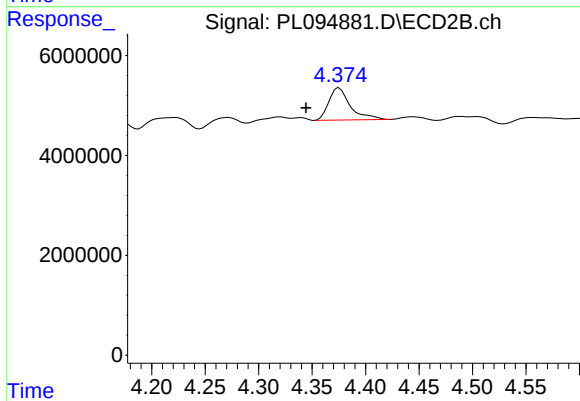

#24 Chlordane-2


R.T.: 4.375 min
Delta R.T.: 0.031 min
Response: 9042114
Conc: 51.20 ng/ml

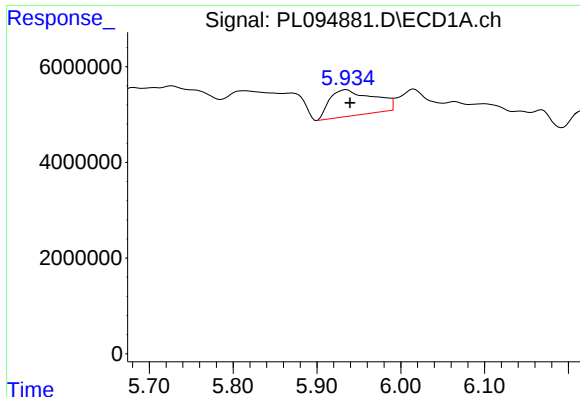

#25 Chlordane-3


R.T.: 5.935 min
Delta R.T.: -0.004 min
Response: 19816317
Conc: 39.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-032525

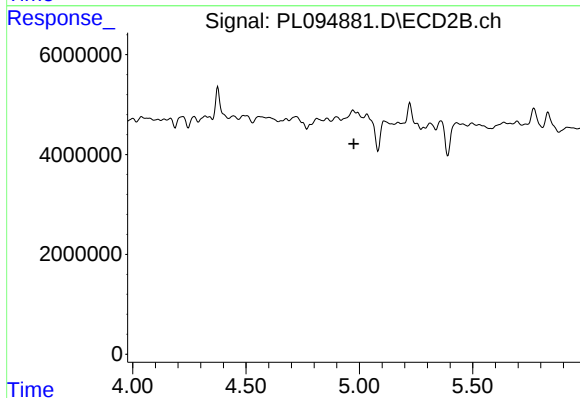


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

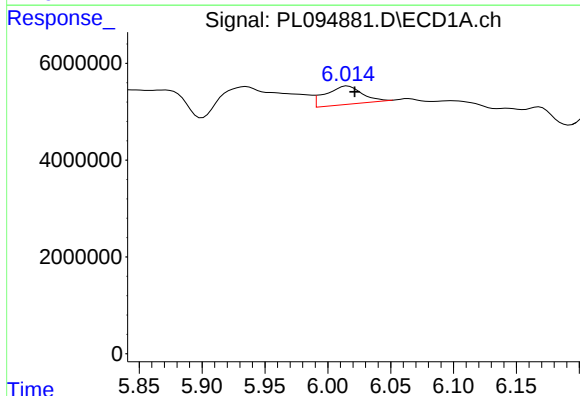


#26 Chlordane-4

R.T.: 6.016 min
Delta R.T.: -0.006 min
Response: 7701432
Conc: 13.07 ng/ml

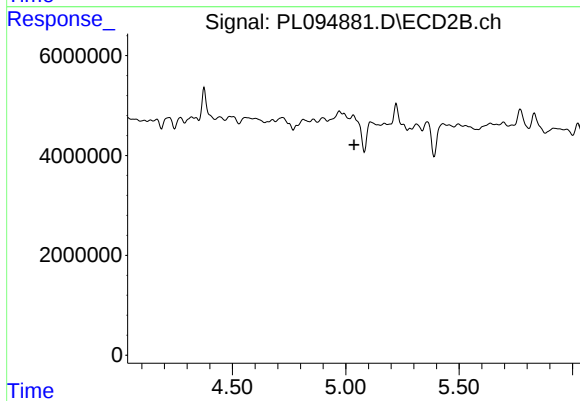

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

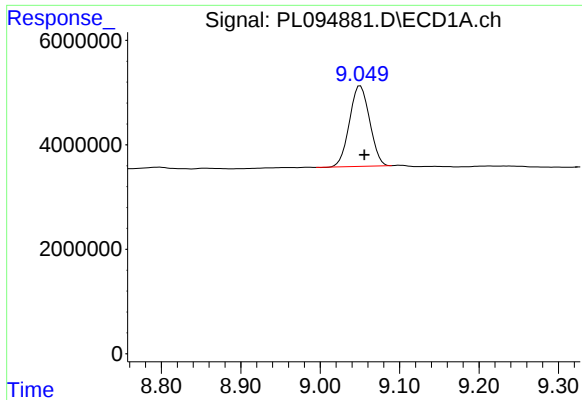

#28 Decachlorobiphenyl

R.T.: 9.051 min
Delta R.T.: -0.005 min
Response: 27236543
Conc: 12.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-032525

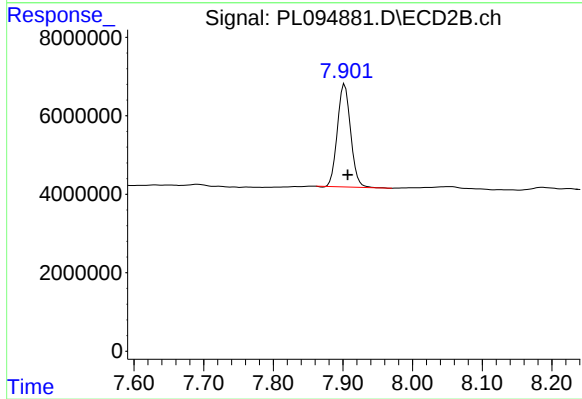

#28 Decachlorobiphenyl

R.T.: 7.903 min
Delta R.T.: -0.004 min
Response: 34711630
Conc: 8.59 ng/ml