

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032625\
 Data File : PL094888.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2025 19:07
 Operator : AR\AJ
 Sample : Q1625-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FRAC-TANK-A1291

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/27/2025
 Supervised By : mohammad ahmed 03/28/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 02:07:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.534	2.768	36966375	61566283	13.059m	17.249m#
28) SA Decachlor...	9.050	7.900	23248189	36786583	11.031	9.107m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032625\
Data File : PL094888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2025 19:07
Operator : AR\AJ
Sample : Q1625-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FRAC-TANK-A1291


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/27/2025
Supervised By : mohammad ahmed 03/28/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 02:07:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

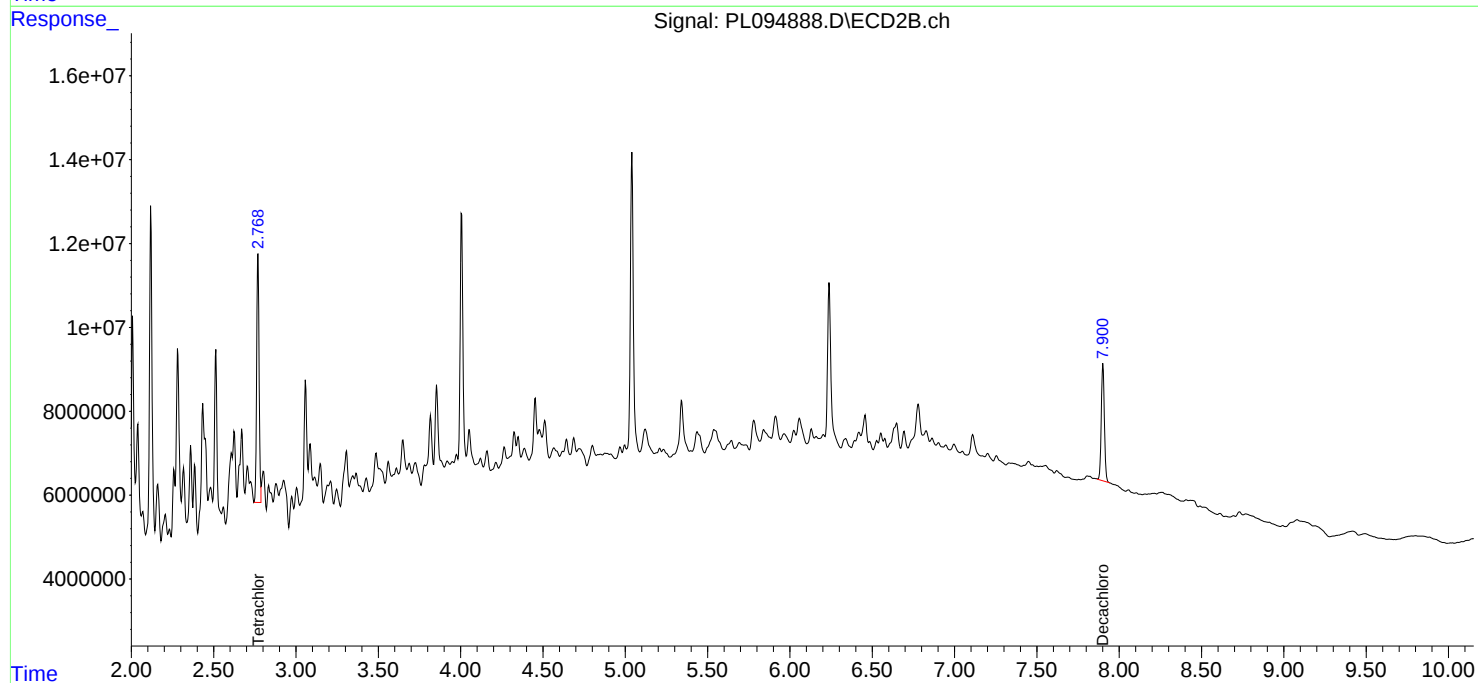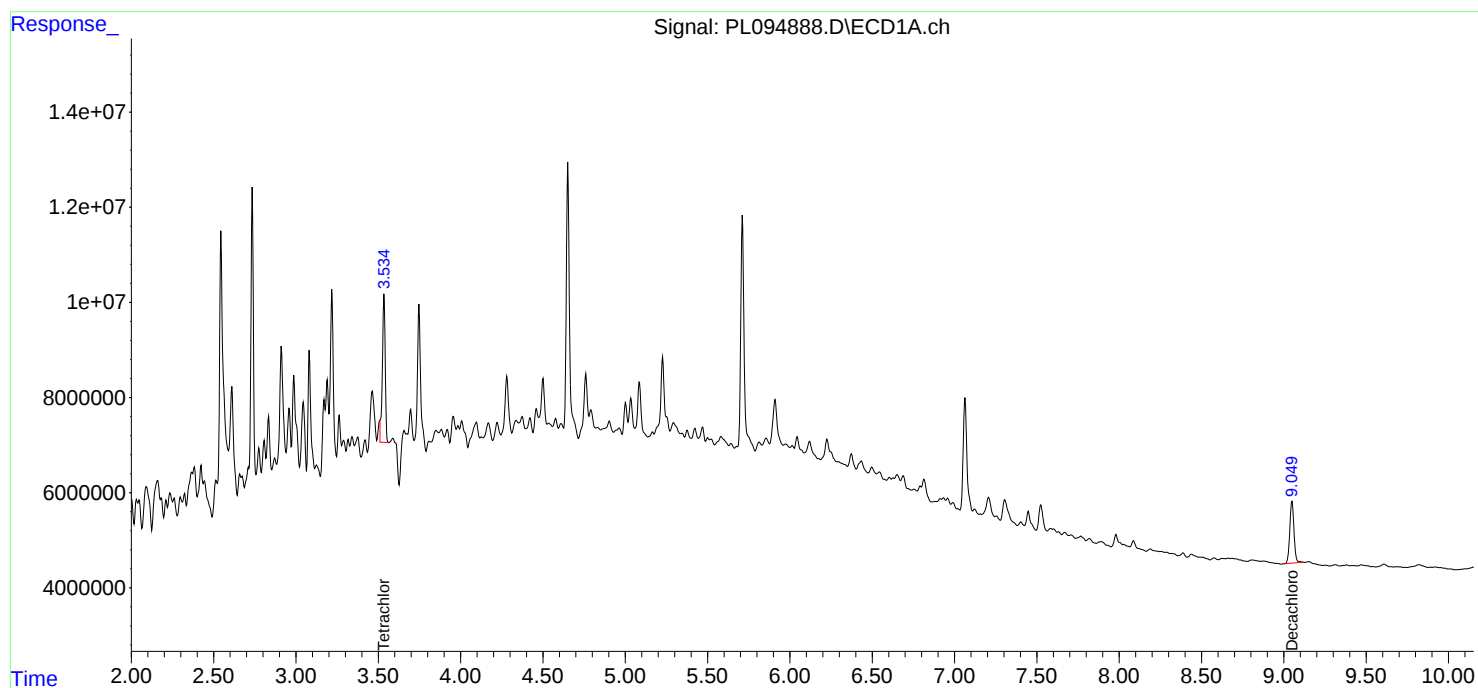

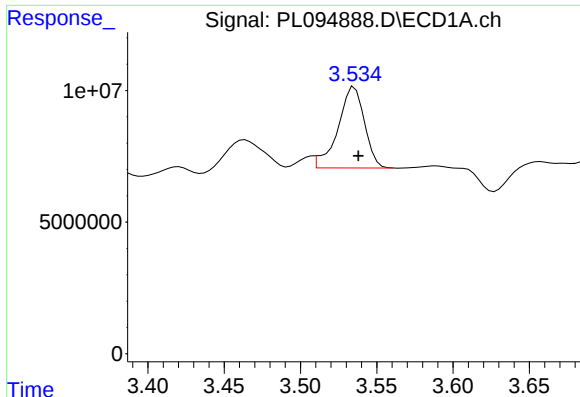


#1 Tetrachloro-m-xylene

R.T.: 3.534 min
Delta R.T.: -0.004 min
Response: 36966375
Conc: 13.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
FRAC-TANK-A1291


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/27/2025
Supervised By :mohammad ahmed 03/28/2025

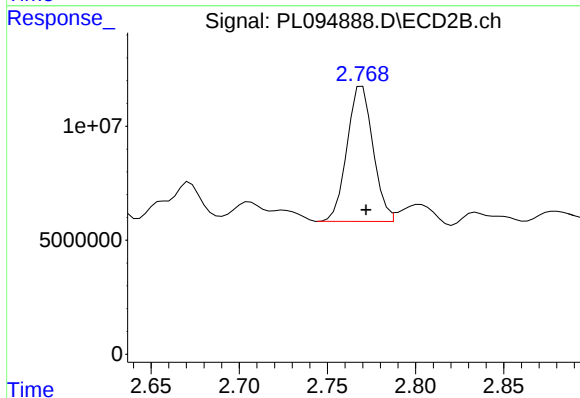


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: -0.004 min
Response: 61566283
Conc: 17.25 ng/ml m

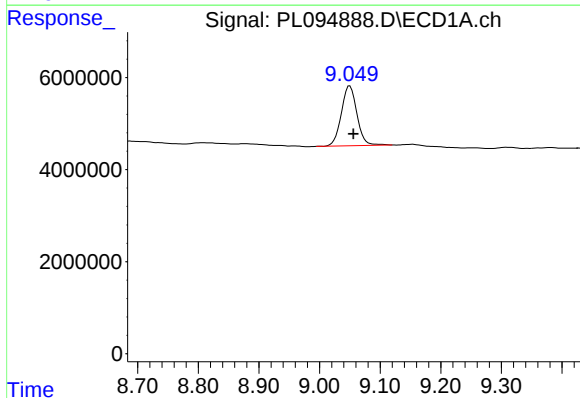

#28 Decachlorobiphenyl

R.T.: 9.050 min
Delta R.T.: -0.006 min
Response: 23248189
Conc: 11.03 ng/ml

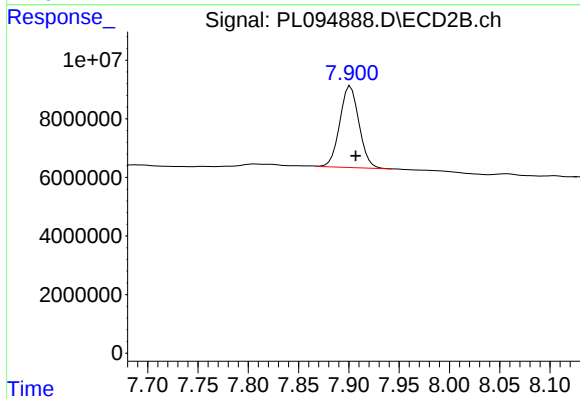

#28 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: -0.007 min
Response: 36786583
Conc: 9.11 ng/ml m