

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032719\
 Data File : PL046560.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2019 19:28
 Operator : AJ\SJ
 Sample : K1693-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-01-032519-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 01:13:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.977	80258367	25287784	11.033	11.045
28)	SA Decachlor...	8.034	9.027	85546413	28981878	10.171	12.500
Target Compounds							
6)	B beta-BHC	0.000	4.846f	0	1258019	N.D.	0.949 #
10)	B gamma-Chl...	0.000	6.082	0	4426296	N.D.	1.560 #
11)	B alpha-Chl...	0.000	6.154	0	7598474	N.D.	2.679 #
12)	B 4,4'-DDE	5.473	6.306	9794393	3478090	1.064	1.401 #
17)	MA 4,4'-DDT	6.219	7.098	10182804	3766342	1.344	1.796 #
24)	Chlordane-2	0.000	5.433	0	2931448	N.D.	25.096 #
25)	Chlordane-3	0.000	6.082	0	4426296	N.D.	11.609 #
26)	Chlordane-4	0.000	6.154	0	7598474	N.D.	16.467 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032719\
Data File : PL046560.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2019 19:28
Operator : AJ\SJ
Sample : K1693-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OR-01-032519-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 01:13:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

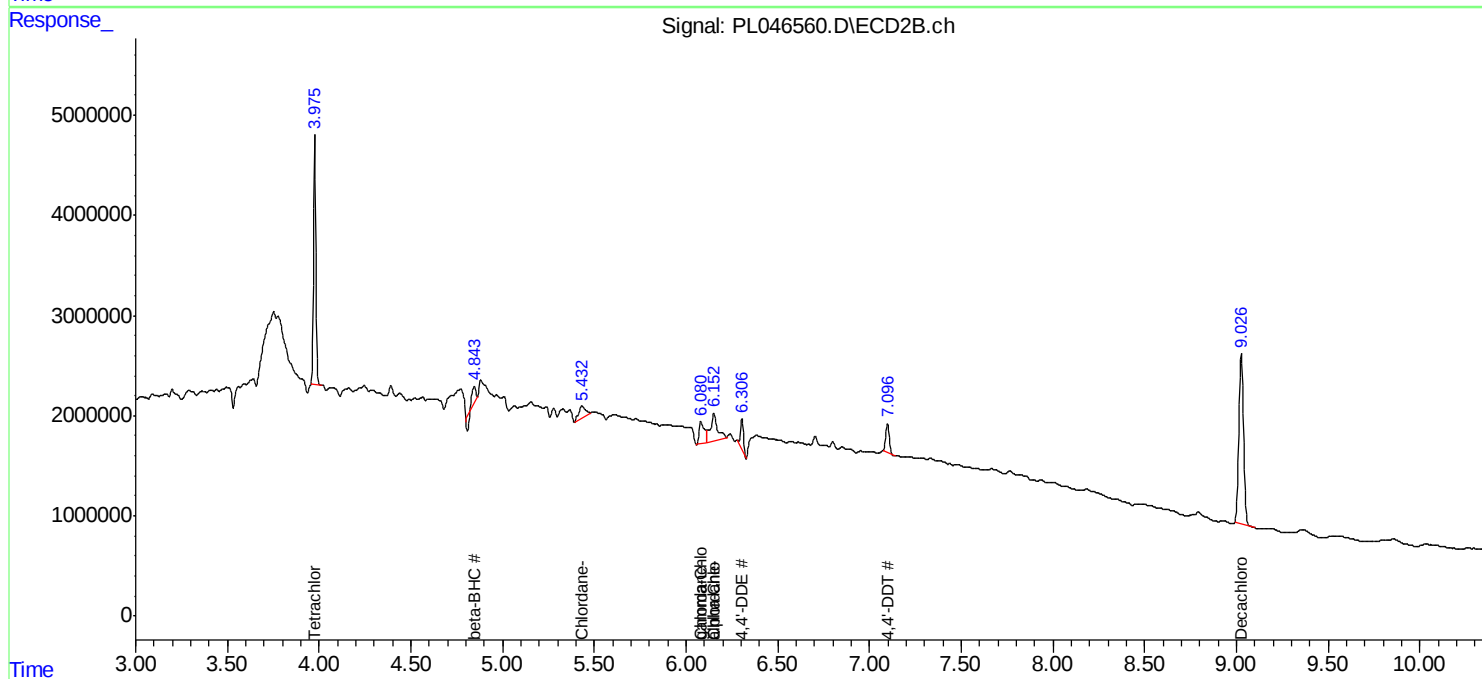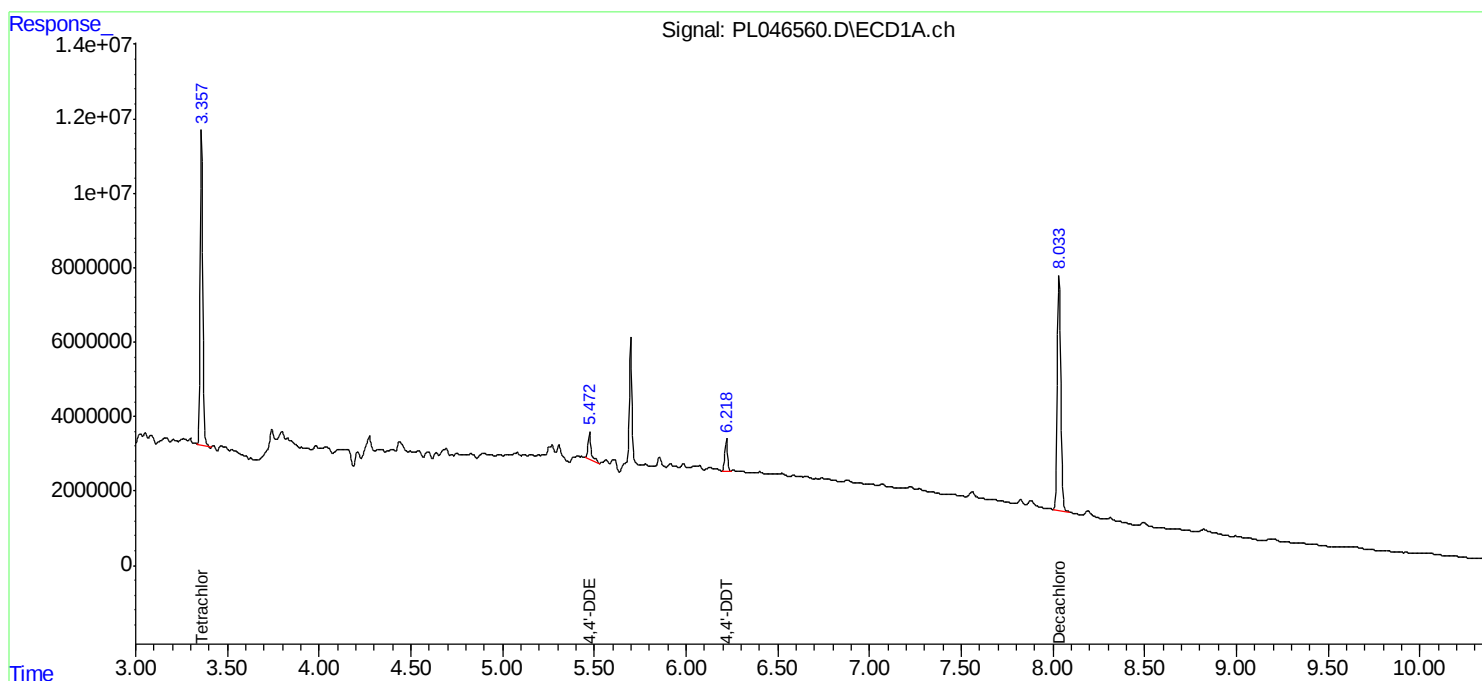


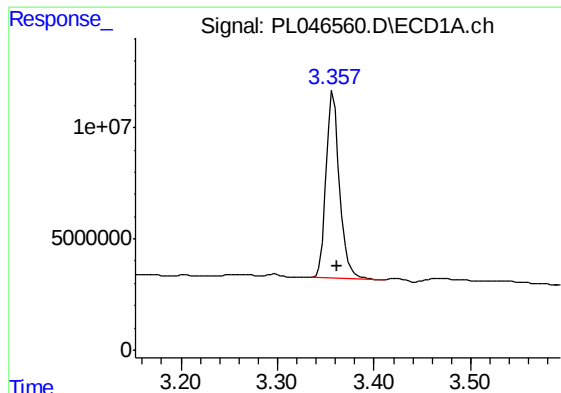

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 80258367
Conc: 11.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-01-032519-B

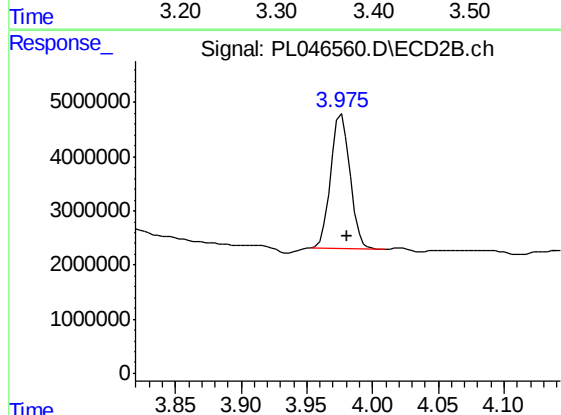


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.004 min
Response: 25287784
Conc: 11.04 ng/ml

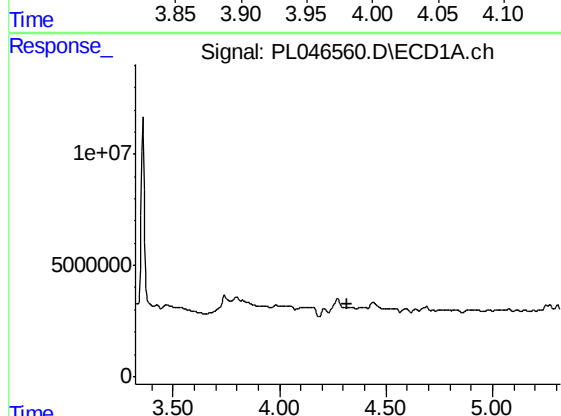


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.321 min
Response: 0
Conc: N.D.

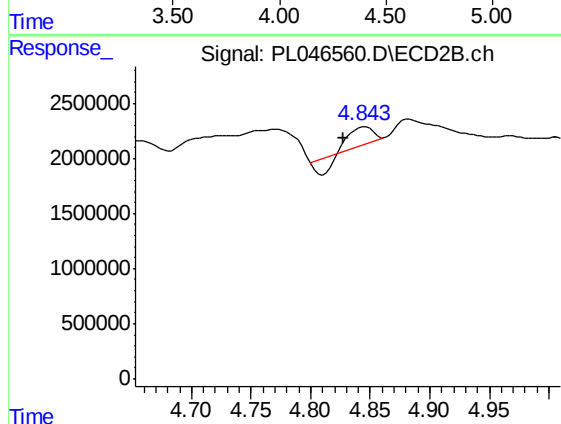

#6 beta-BHC


R.T.: 4.846 min
Delta R.T.: 0.018 min
Response: 1258019
Conc: 0.95 ng/ml

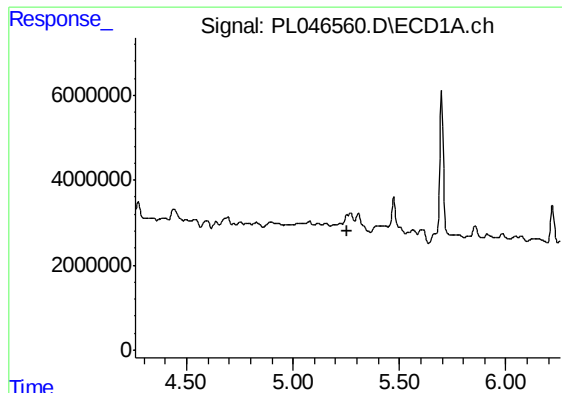

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.257 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-01-032519-B

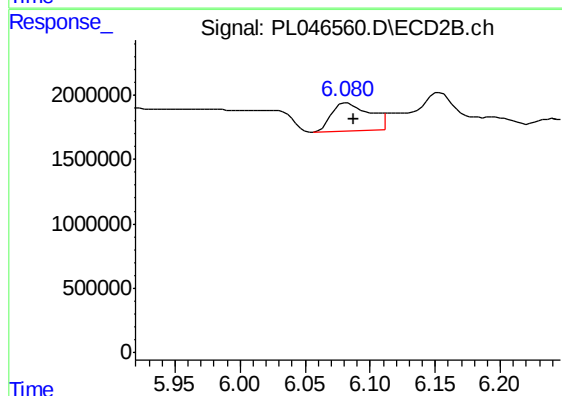


#10 gamma-Chlordane

R.T.: 6.082 min
Delta R.T.: -0.006 min
Response: 4426296
Conc: 1.56 ng/ml

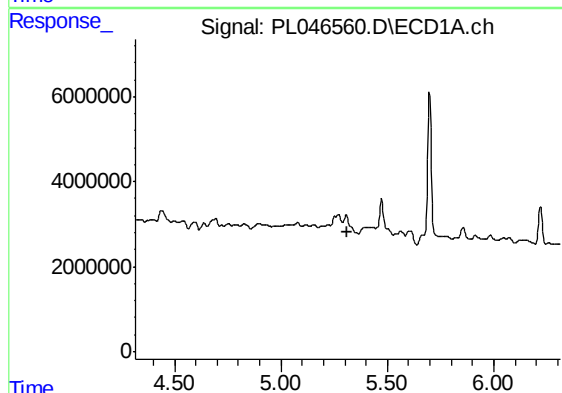


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.314 min
Response: 0
Conc: N.D.

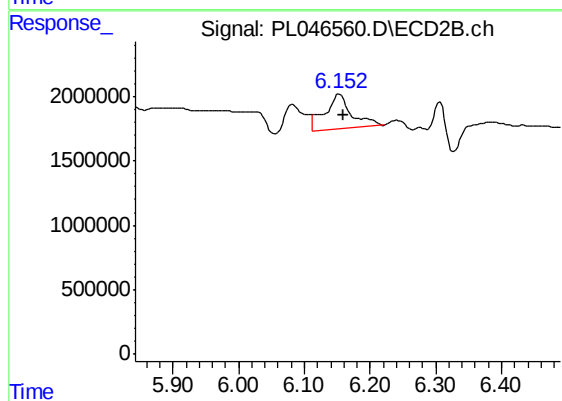

#11 alpha-Chlordane


R.T.: 6.154 min
Delta R.T.: -0.007 min
Response: 7598474
Conc: 2.68 ng/ml

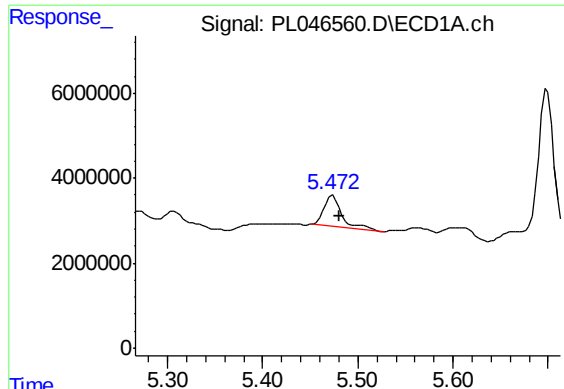

#12 4,4'-DDE


R.T.: 5.473 min
Delta R.T.: -0.007 min
Response: 9794393
Conc: 1.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-01-032519-B

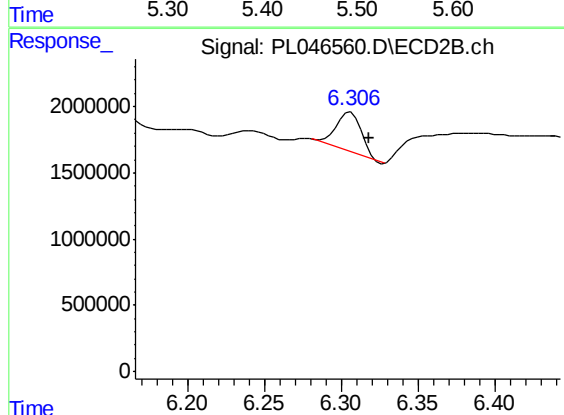


#12 4,4'-DDE

R.T.: 6.306 min
Delta R.T.: -0.011 min
Response: 3478090
Conc: 1.40 ng/ml

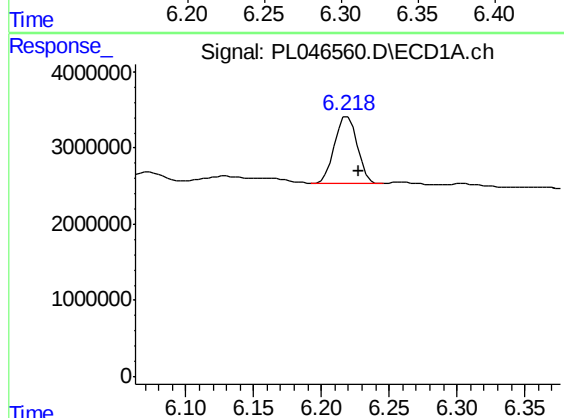


#17 4,4'-DDT

R.T.: 6.219 min
Delta R.T.: -0.008 min
Response: 10182804
Conc: 1.34 ng/ml

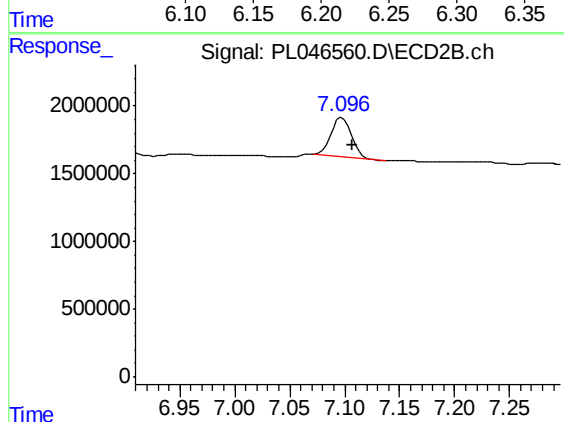

#17 4,4'-DDT


R.T.: 7.098 min
Delta R.T.: -0.009 min
Response: 3766342
Conc: 1.80 ng/ml

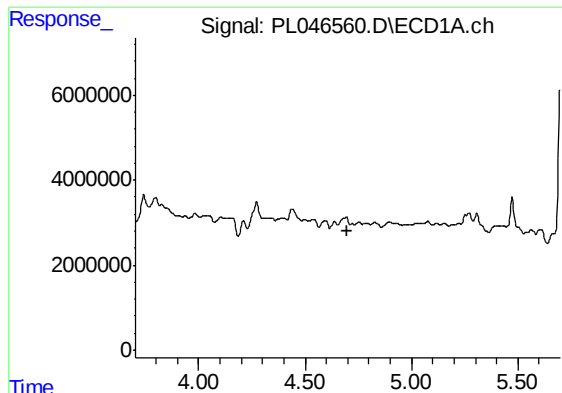

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.701 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-01-032519-B

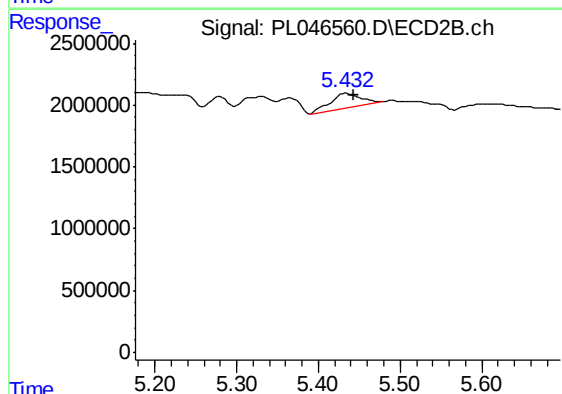


#24 Chlordane-2

R.T.: 5.433 min
Delta R.T.: -0.009 min
Response: 2931448
Conc: 25.10 ng/ml

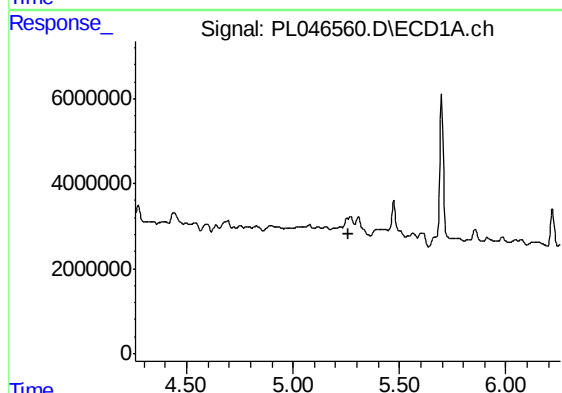


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

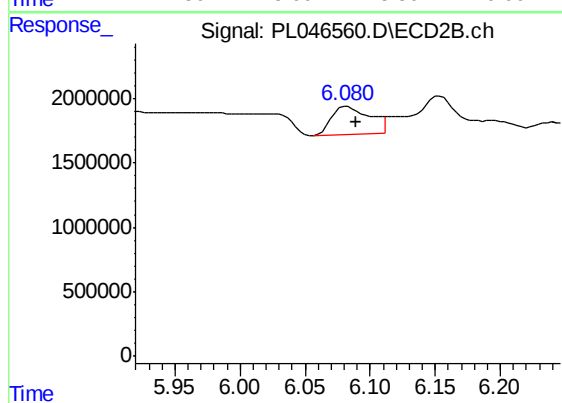

#25 Chlordane-3


R.T.: 6.082 min
Delta R.T.: -0.007 min
Response: 4426296
Conc: 11.61 ng/ml

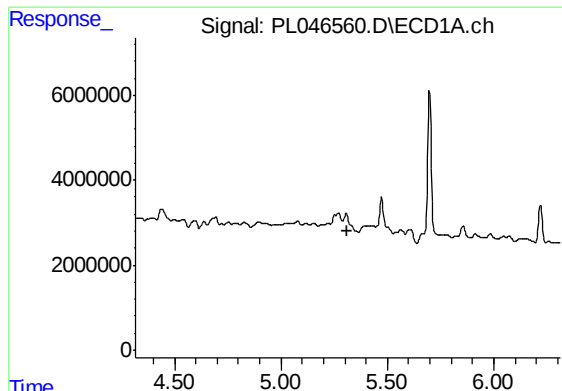

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-01-032519-B

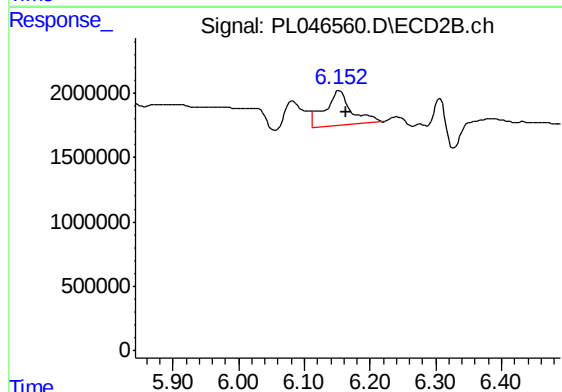


#26 Chlordane-4

R.T.: 6.154 min
Delta R.T.: -0.010 min
Response: 7598474
Conc: 16.47 ng/ml

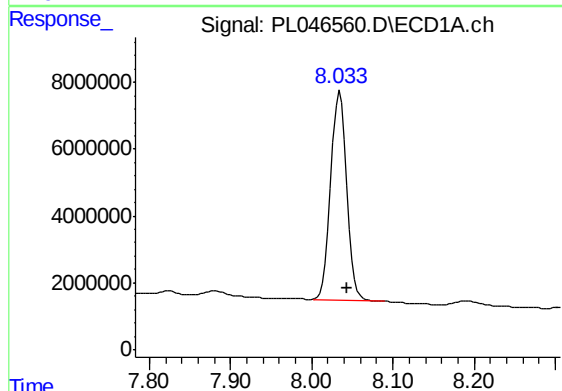

#28 Decachlorobiphenyl

R.T.: 8.034 min
Delta R.T.: -0.010 min
Response: 85546413
Conc: 10.17 ng/ml

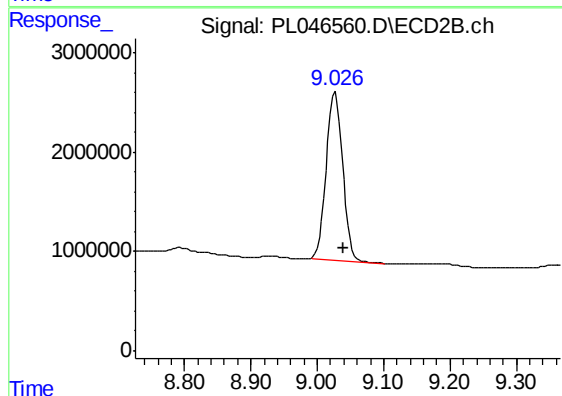

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: -0.013 min
Response: 28981878
Conc: 12.50 ng/ml