

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032719\
 Data File : PL046593.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2019 03:36
 Operator : AJ\SJ
 Sample : K2086-08
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CS-11

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 05:35:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.976	128.9E6	42183631	17.725	18.424
28)	SA Decachlor...	8.033	9.026	160.8E6	48335795	19.113	20.848
Target Compounds							
9)	A Endosulfan I	5.389f	0.000	17107366	0	1.819	N.D. #
10)	B gamma-Chl...	0.000	6.067f	0	4723886	N.D.	1.664 #
13)	MA Dieldrin	5.589f	0.000	9819552	0	0.978	N.D. #
25)	Chlordane-3	0.000	6.067f	0	4723886	N.D.	12.390 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032719\
Data File : PL046593.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2019 03:36
Operator : AJ\SJ
Sample : K2086-08
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CS-11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 05:35:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

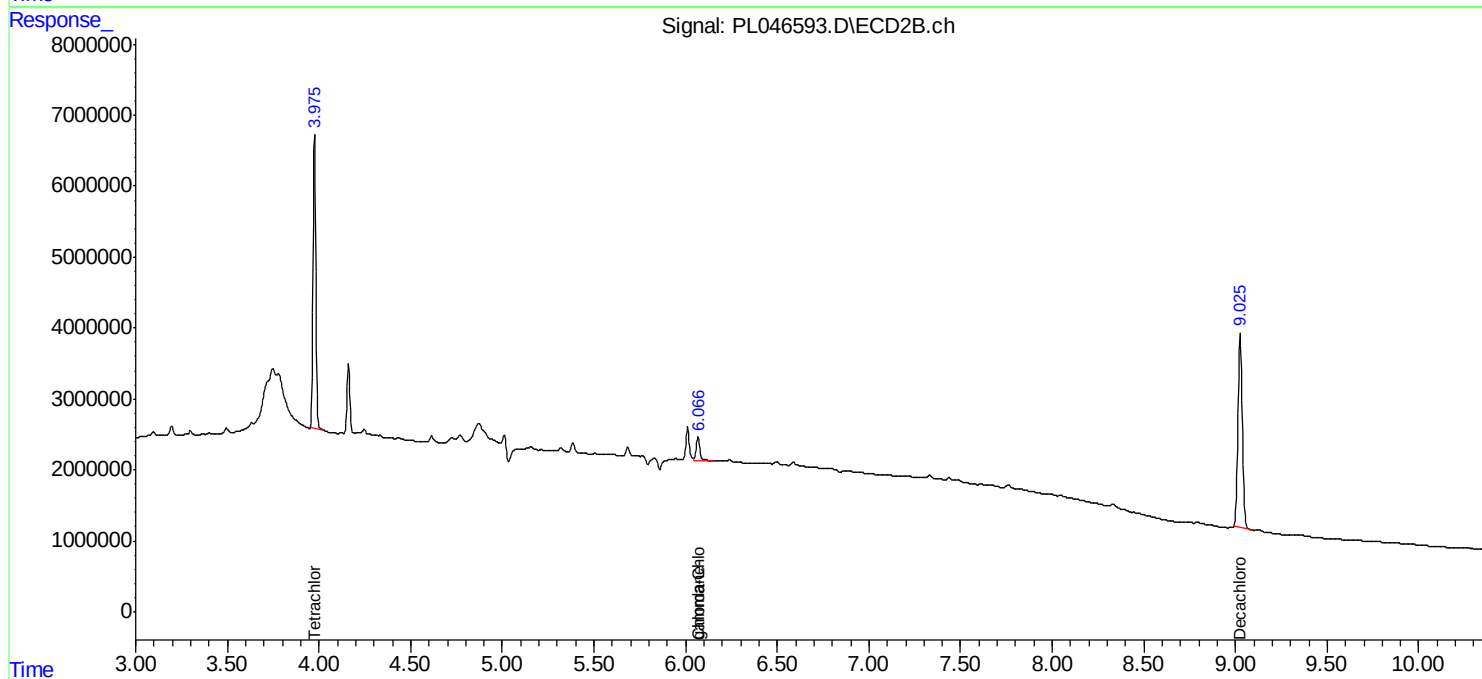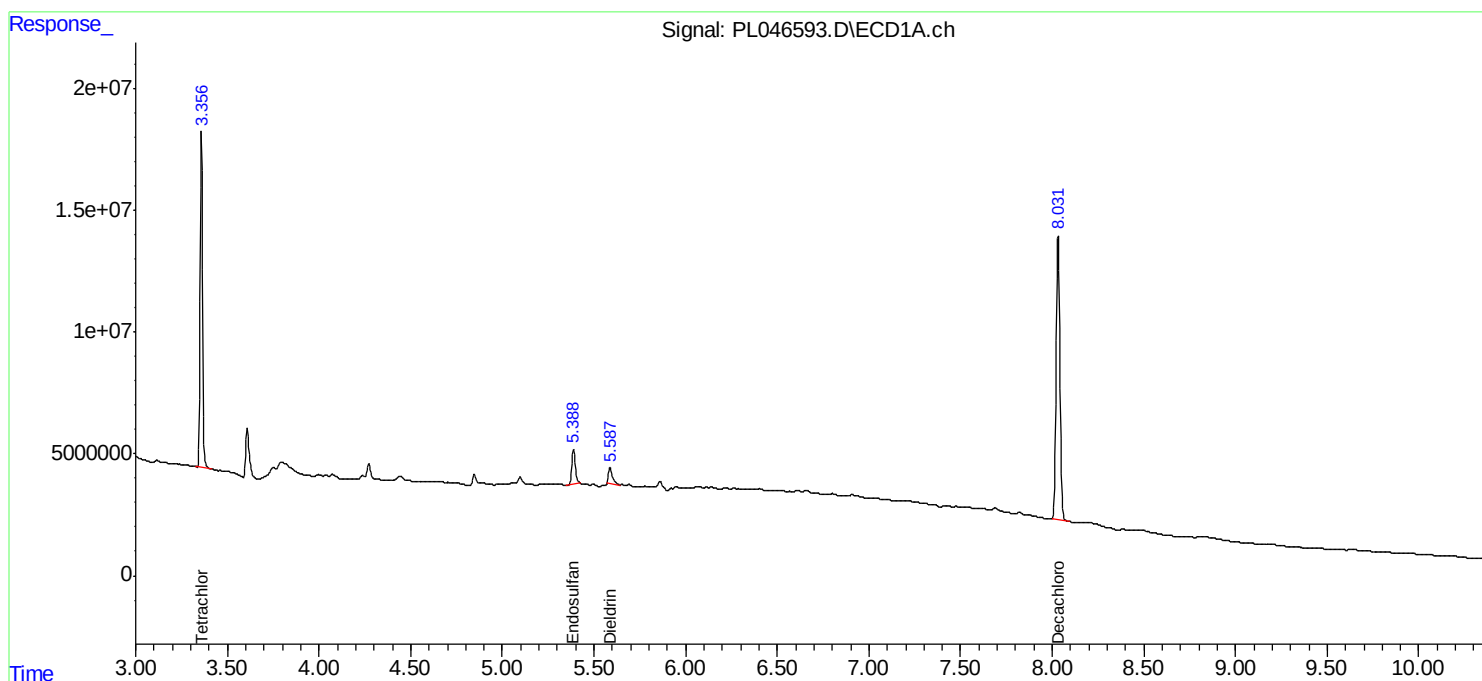


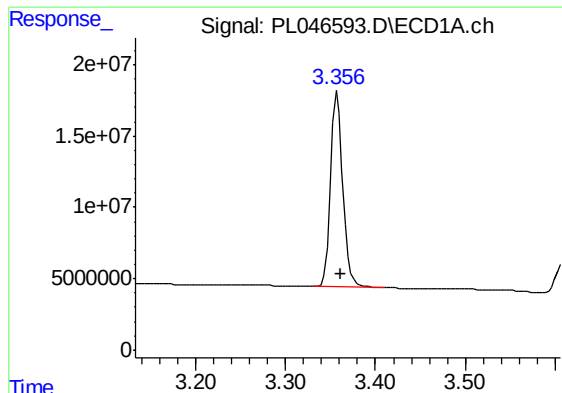

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 128946277
Conc: 17.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
CS-11

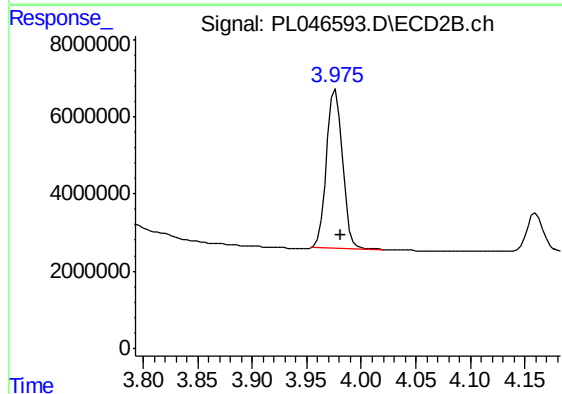


#1 Tetrachloro-m-xylene

R.T.: 3.976 min
Delta R.T.: -0.004 min
Response: 42183631
Conc: 18.42 ng/ml

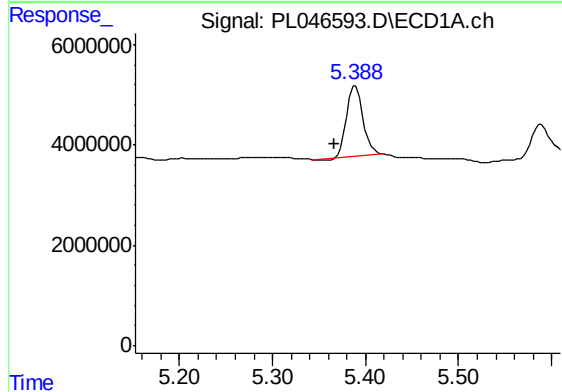


#9 Endosulfan I

R.T.: 5.389 min
Delta R.T.: 0.023 min
Response: 17107366
Conc: 1.82 ng/ml

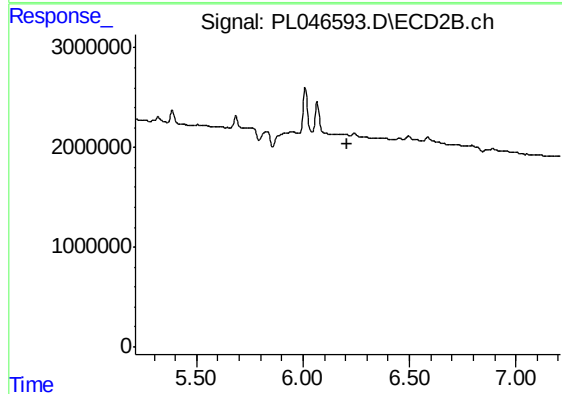

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.210 min
Response: 0
Conc: N.D.

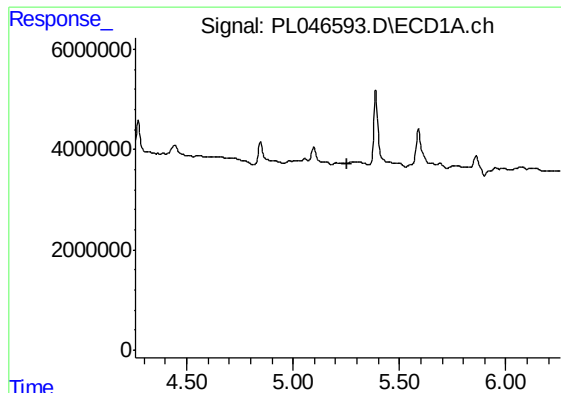

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.257 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CS-11

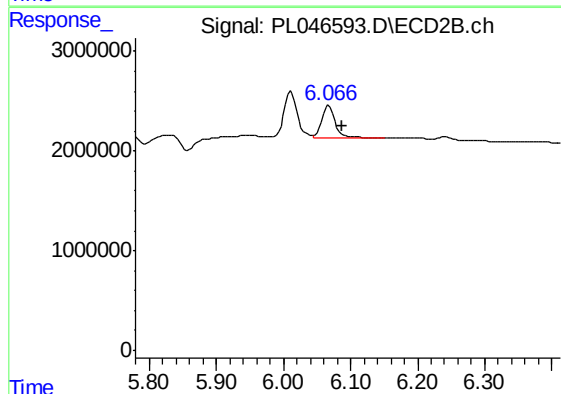


#10 gamma-Chlordane

R.T.: 6.067 min
Delta R.T.: -0.020 min
Response: 4723886
Conc: 1.66 ng/ml

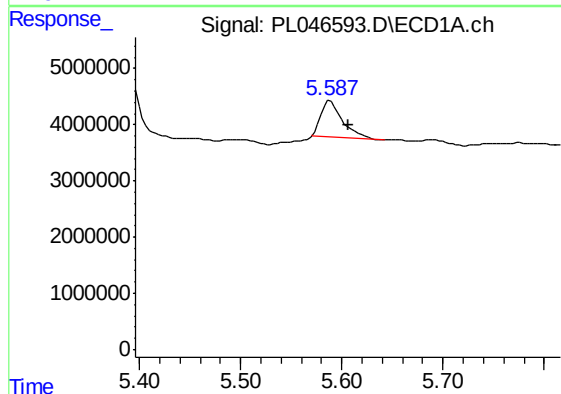


#13 Dieldrin

R.T.: 5.589 min
Delta R.T.: -0.018 min
Response: 9819552
Conc: 0.98 ng/ml

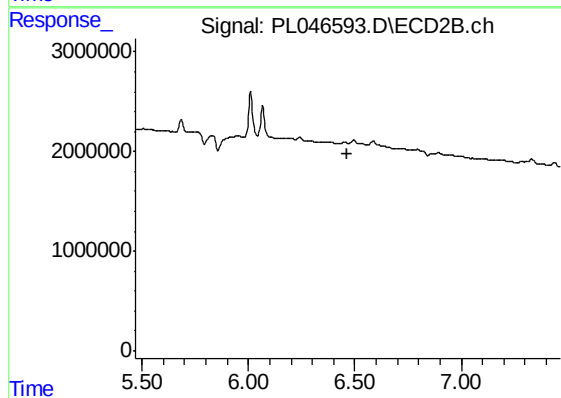

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.467 min
Response: 0
Conc: N.D.

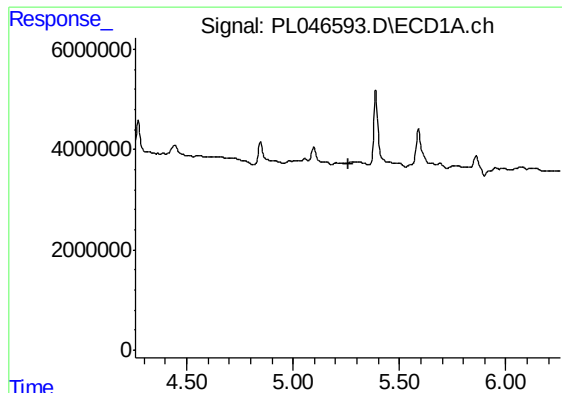

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CS-11

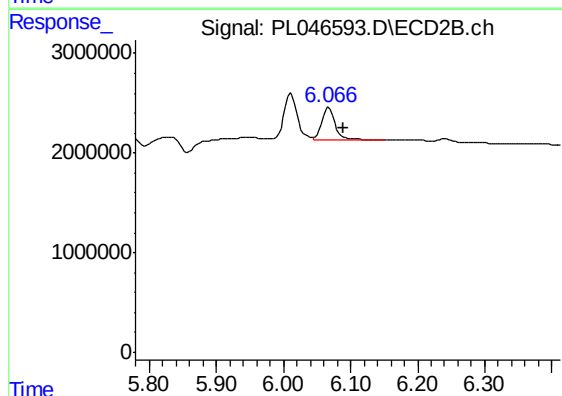


#25 Chlordane-3

R.T.: 6.067 min
Delta R.T.: -0.022 min
Response: 4723886
Conc: 12.39 ng/ml

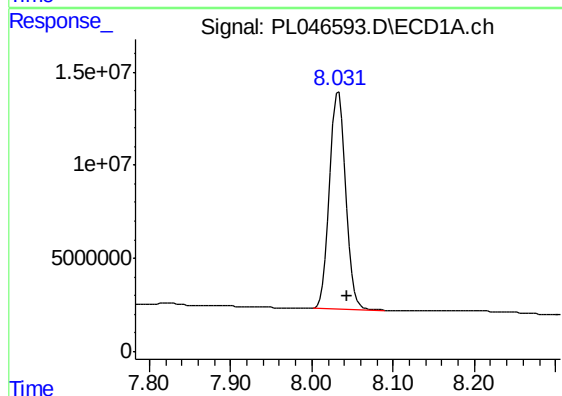

#28 Decachlorobiphenyl

R.T.: 8.033 min
Delta R.T.: -0.011 min
Response: 160762588
Conc: 19.11 ng/ml

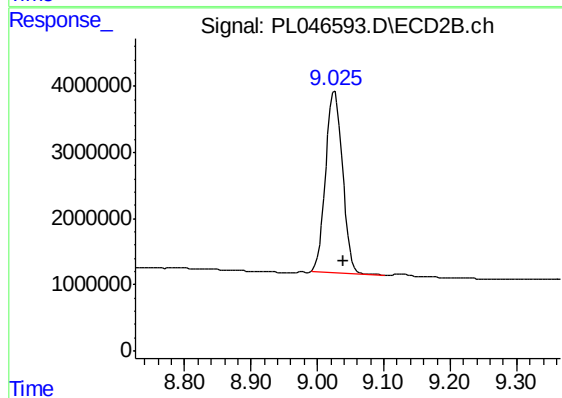

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.014 min
Response: 48335795
Conc: 20.85 ng/ml