

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032719\
 Data File : PL046597.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2019 04:33
 Operator : AJ\SJ
 Sample : K2086-10
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CS-13

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 05:36:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.976	130.9E6	41421032	17.994	18.091
28)	SA Decachlor...	8.033	9.026	152.6E6	43517536	18.146	18.770
Target Compounds							
3)	MA gamma-BHC...	4.073	4.631f	8004995	808299	0.745	0.270 #
9)	A Endosulfan I	5.390f	0.000	7431648	0	0.790	N.D. #
10)	B gamma-Chl...	0.000	6.067f	0	3544881	N.D.	1.249 #
13)	MA Dieldrin	5.590f	0.000	8366680	0	0.834	N.D. #
25)	Chlordane-3	0.000	6.067f	0	3544881	N.D.	9.298 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032719\
Data File : PL046597.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2019 04:33
Operator : AJ\SJ
Sample : K2086-10
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CS-13

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 05:36:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

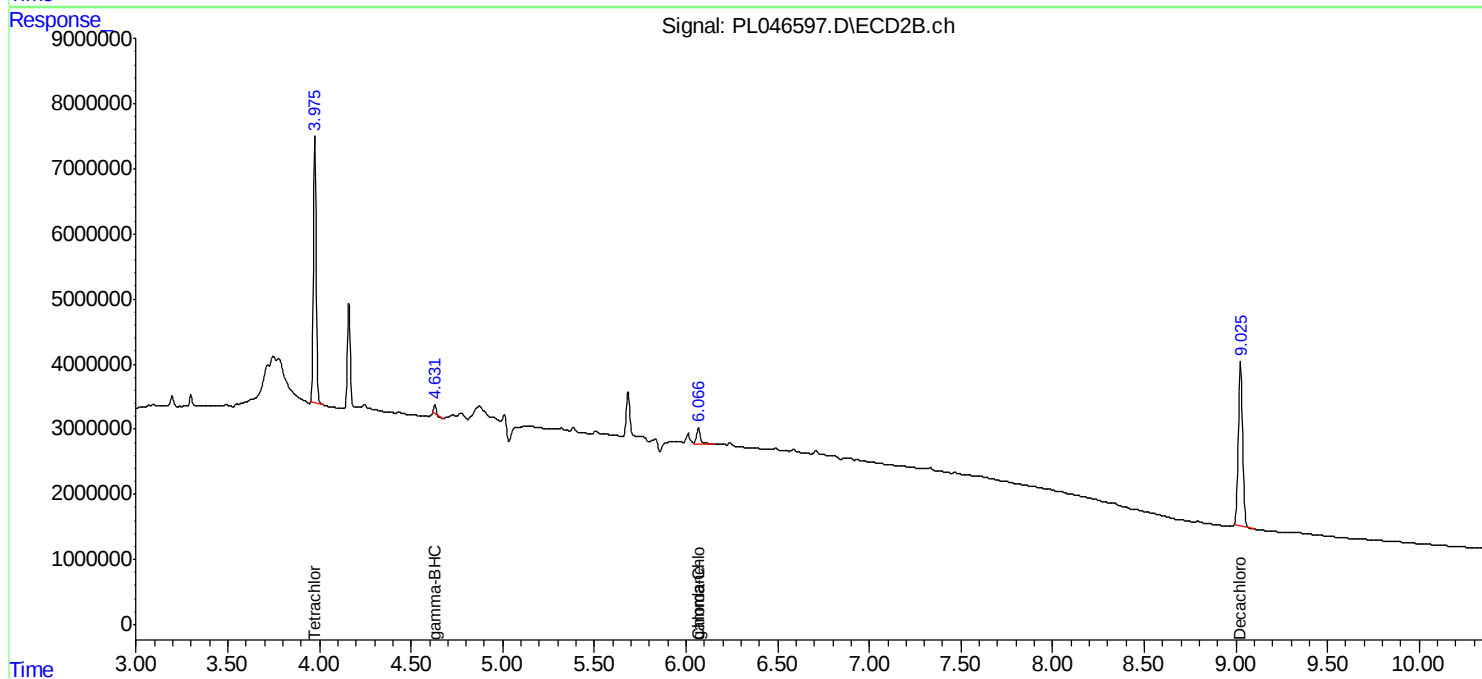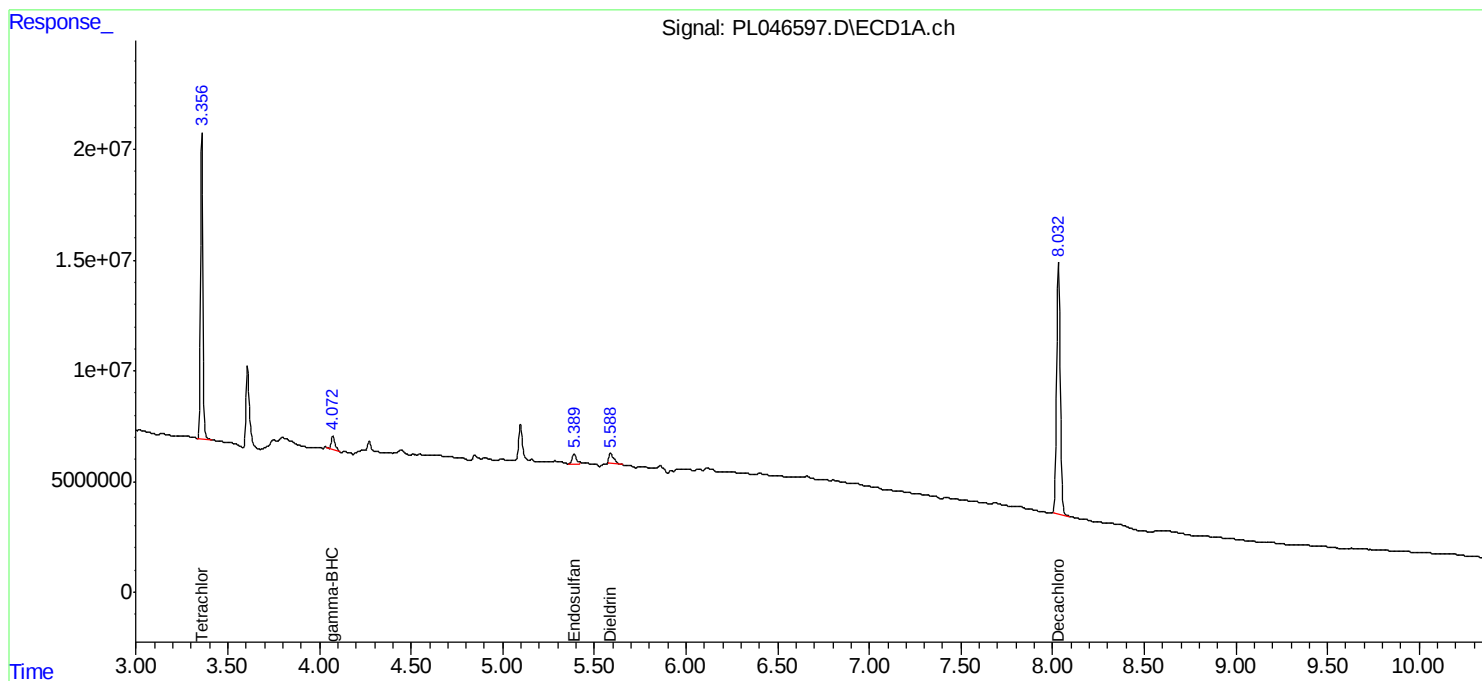


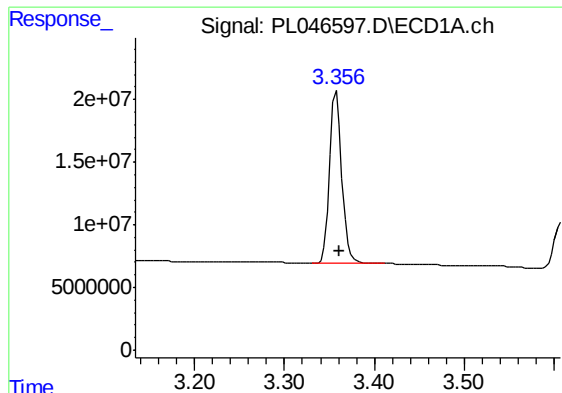

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 130900013
Conc: 17.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
CS-13

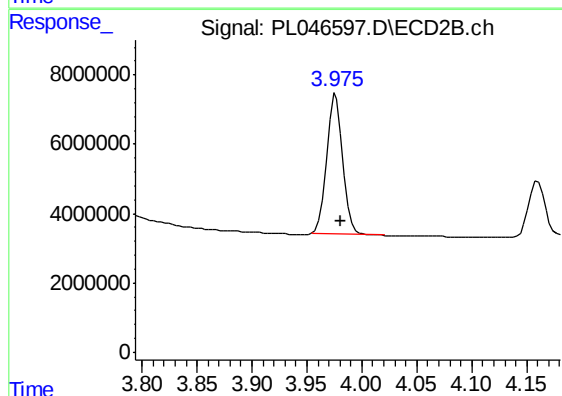


#1 Tetrachloro-m-xylene

R.T.: 3.976 min
Delta R.T.: -0.004 min
Response: 41421032
Conc: 18.09 ng/ml

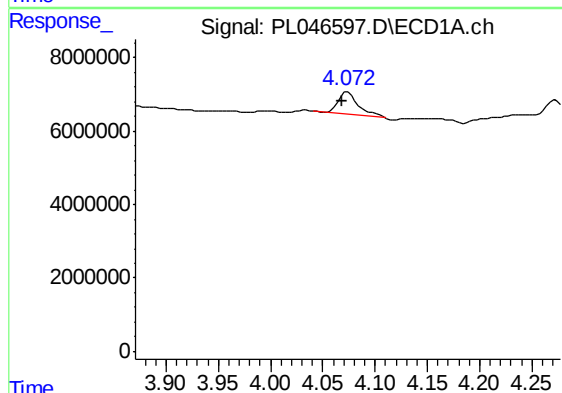


#3 gamma-BHC (Lindane)

R.T.: 4.073 min
Delta R.T.: 0.005 min
Response: 8004995
Conc: 0.75 ng/ml

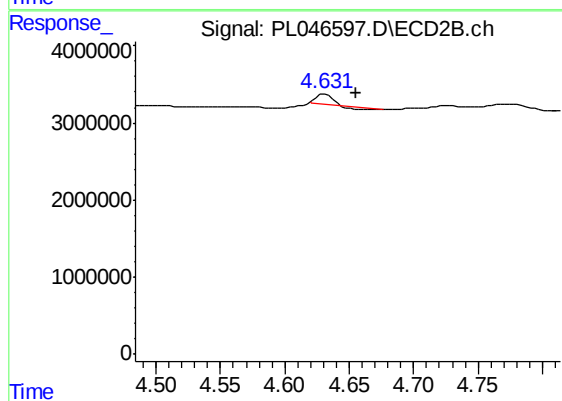

#3 gamma-BHC (Lindane)


R.T.: 4.631 min
Delta R.T.: -0.024 min
Response: 808299
Conc: 0.27 ng/ml

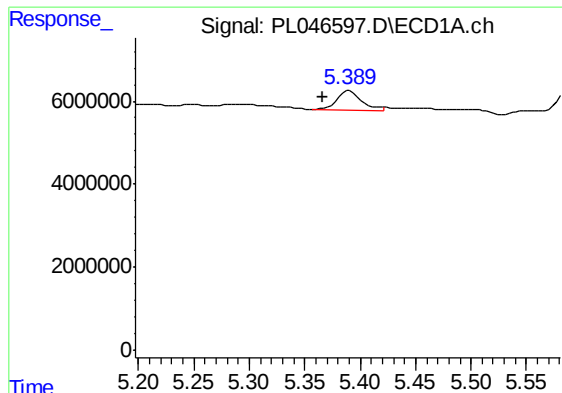

#9 Endosulfan I


R.T.: 5.390 min
Delta R.T.: 0.024 min
Response: 7431648
Conc: 0.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
CS-13

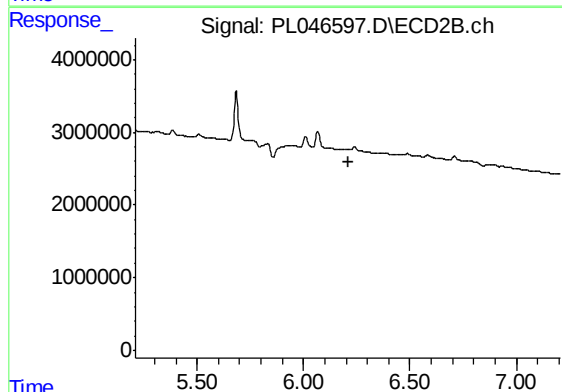


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.210 min
Response: 0
Conc: N.D.

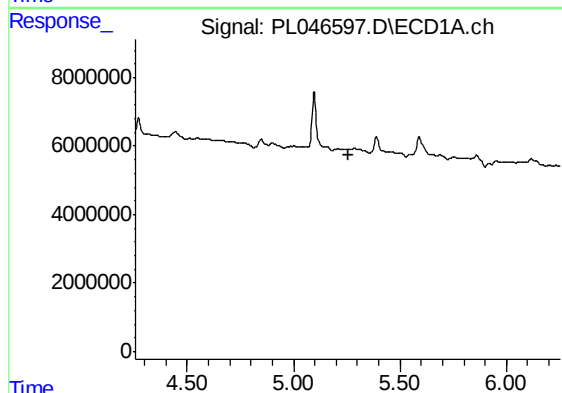


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.257 min
Response: 0
Conc: N.D.

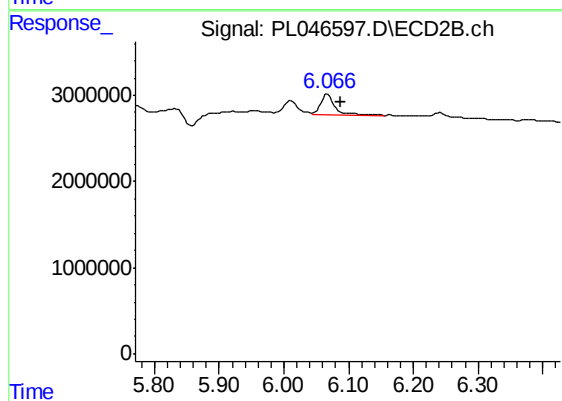

#10 gamma-Chlordane


R.T.: 6.067 min
Delta R.T.: -0.020 min
Response: 3544881
Conc: 1.25 ng/ml

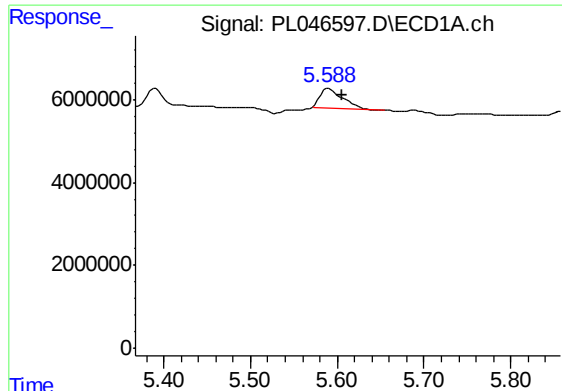

#13 Dieldrin


R.T.: 5.590 min
Delta R.T.: -0.017 min
Response: 8366680
Conc: 0.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
CS-13

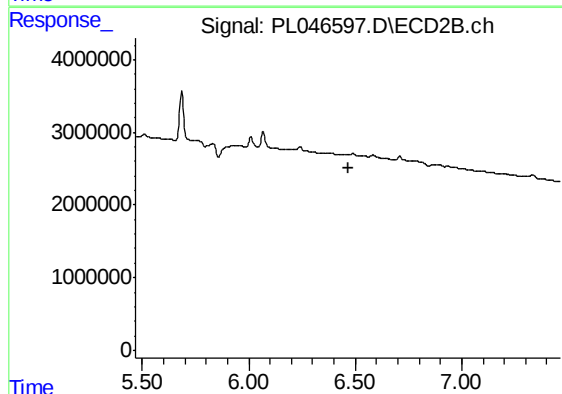


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.467 min
Response: 0
Conc: N.D.

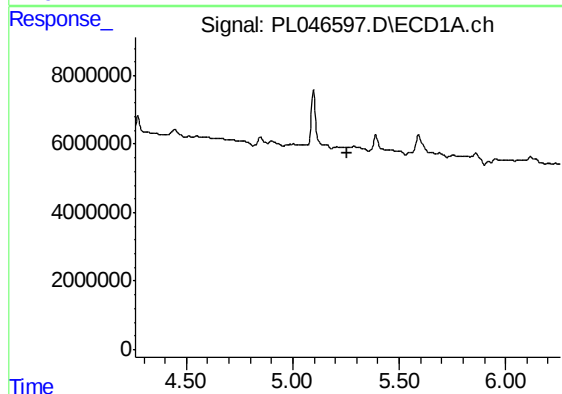


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

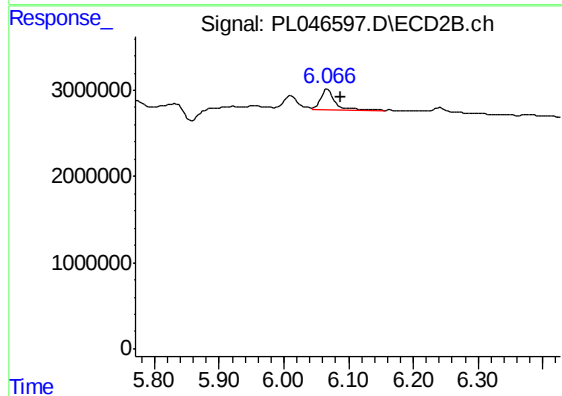

#25 Chlordane-3


R.T.: 6.067 min
Delta R.T.: -0.022 min
Response: 3544881
Conc: 9.30 ng/ml

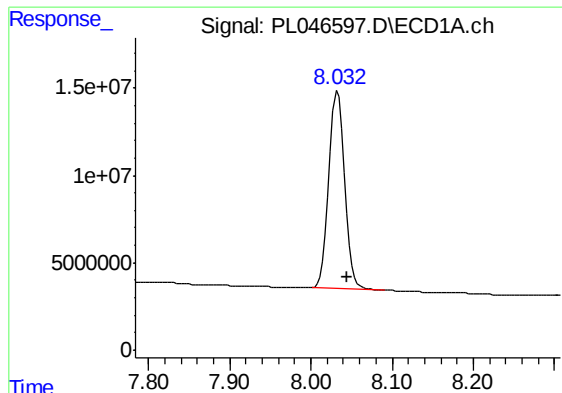

#28 Decachlorobiphenyl

R.T.: 8.033 min
Delta R.T.: -0.011 min
Response: 152627480
Conc: 18.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
CS-13

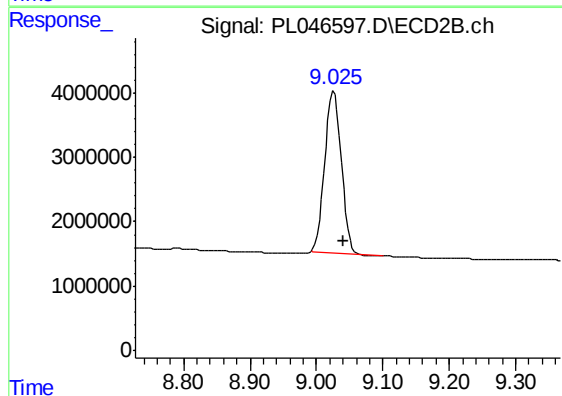

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.014 min
Response: 43517536
Conc: 18.77 ng/ml