

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032719\
 Data File : PL046598.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2019 04:47
 Operator : AJ\SJ
 Sample : K2086-11
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CS-14

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 05:36:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.976	135.7E6	42789615	18.653	18.689
28)	SA Decachlor...	8.034	9.026	161.1E6	45640688	19.153	19.686
Target Compounds							
10)	B gamma-Chl...	0.000	6.068f	0	3199722	N.D.	1.127 #
13)	MA Dieldrin	5.590f	0.000	8736721	0	0.871	N.D. #
23)	Chlordane-1	4.225f	0.000	5042935	0	14.996	N.D. #
25)	Chlordane-3	0.000	6.068f	0	3199722	N.D.	8.392 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032719\
Data File : PL046598.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2019 04:47
Operator : AJ\SJ
Sample : K2086-11
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CS-14

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 05:36:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

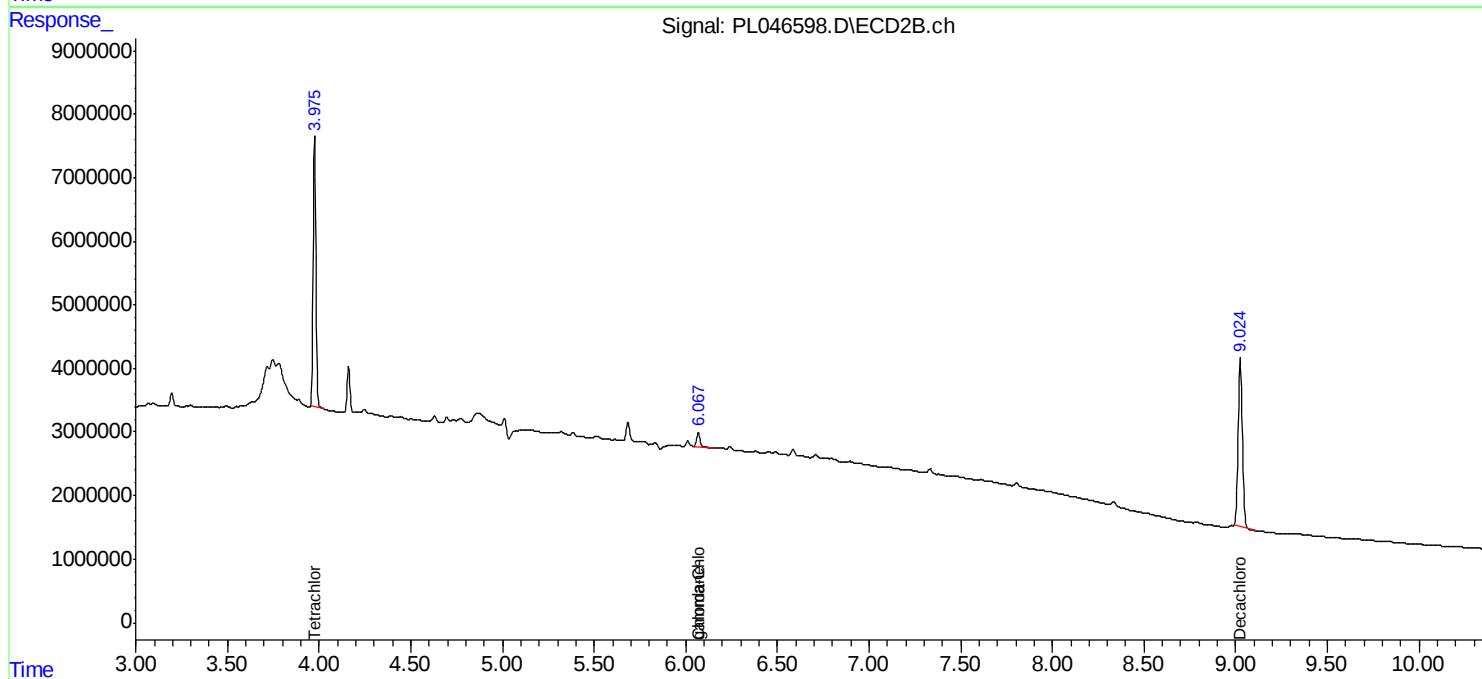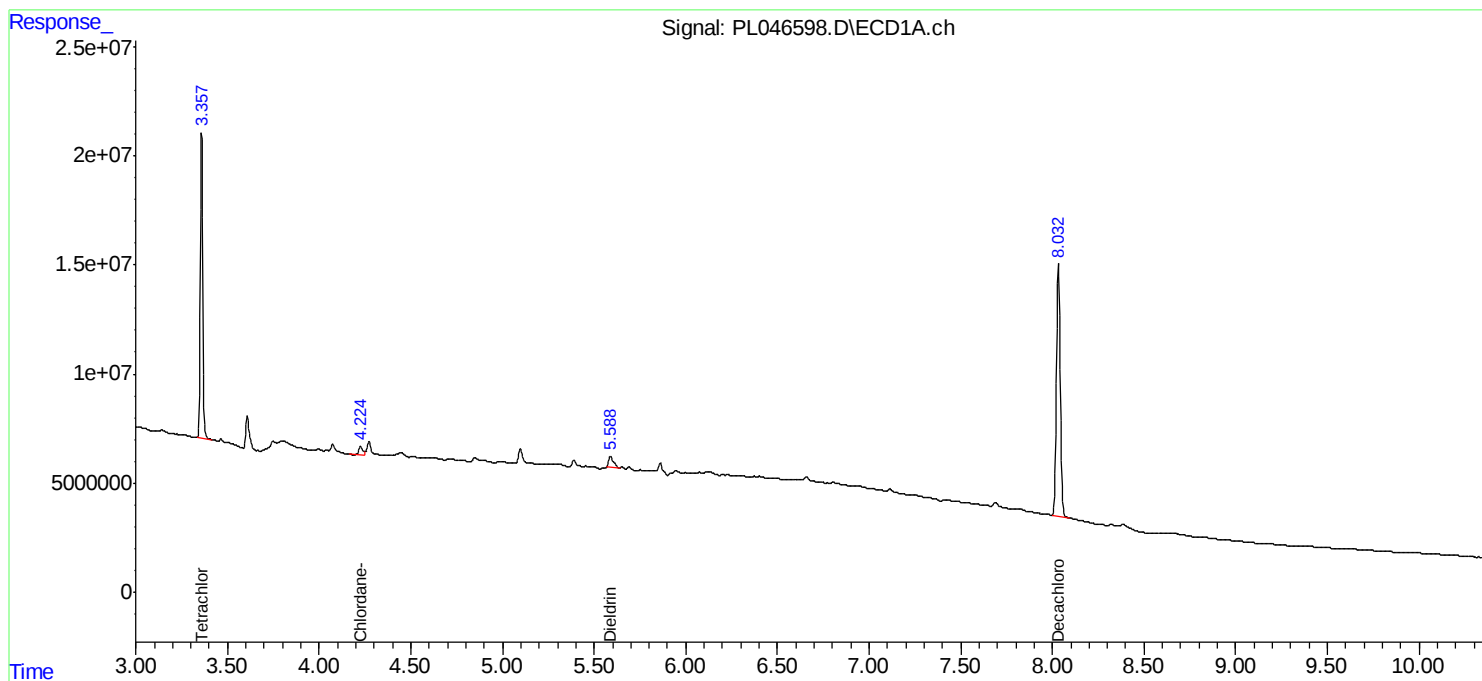


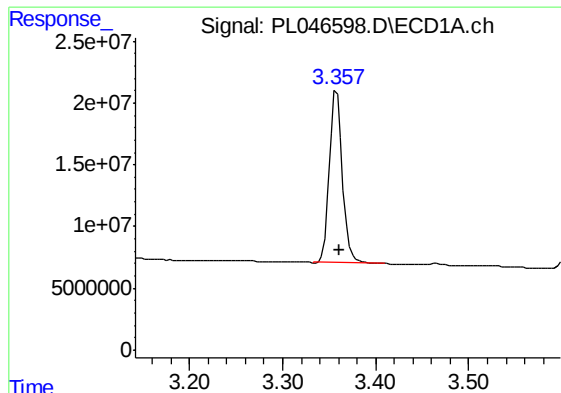

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 135696356
Conc: 18.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
CS-14

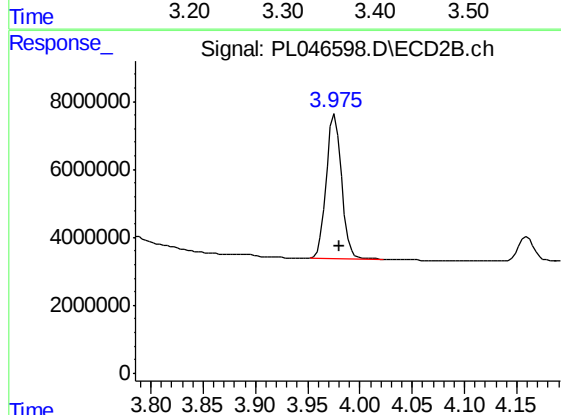


#1 Tetrachloro-m-xylene

R.T.: 3.976 min
Delta R.T.: -0.005 min
Response: 42789615
Conc: 18.69 ng/ml

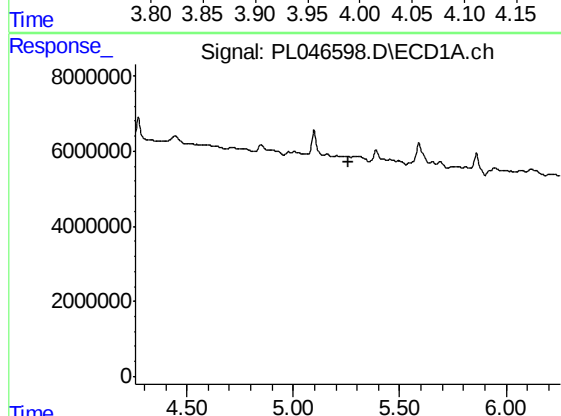


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.257 min
Response: 0
Conc: N.D.

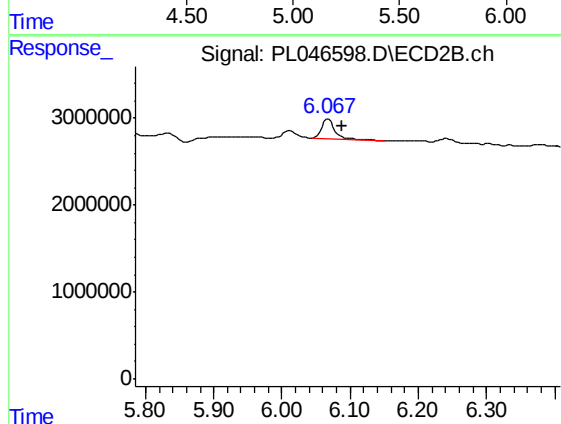

#10 gamma-Chlordane


R.T.: 6.068 min
Delta R.T.: -0.020 min
Response: 3199722
Conc: 1.13 ng/ml

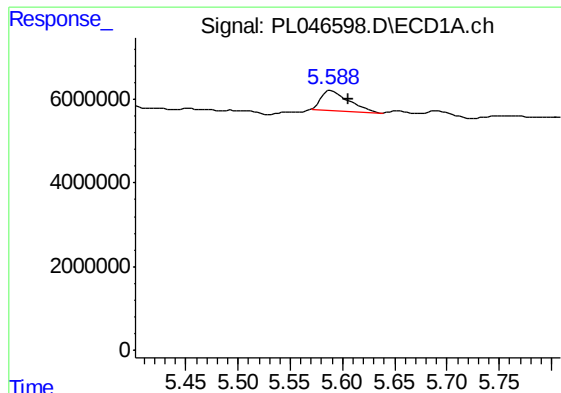

#13 Dieldrin


R.T.: 5.590 min
Delta R.T.: -0.017 min
Response: 8736721
Conc: 0.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
CS-14

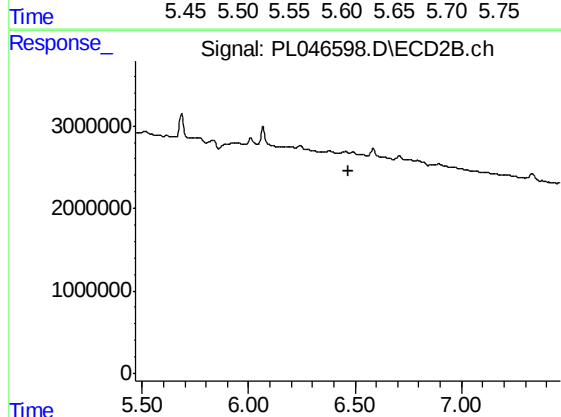


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.467 min
Response: 0
Conc: N.D.

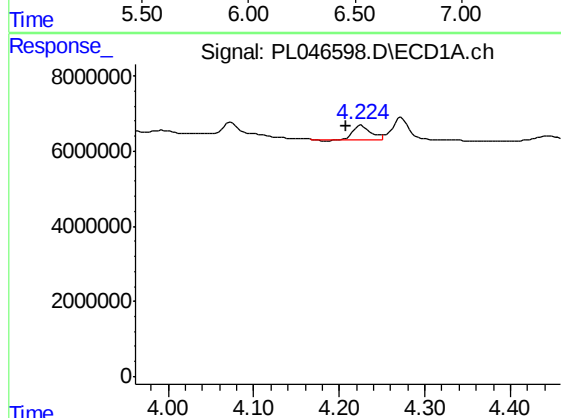


#23 Chlordane-1

R.T.: 4.225 min
Delta R.T.: 0.017 min
Response: 5042935
Conc: 15.00 ng/ml

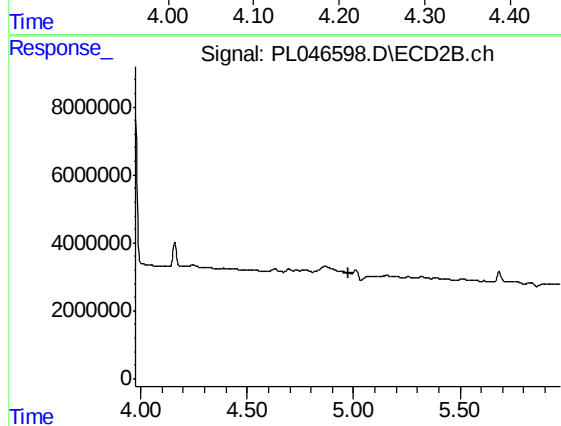

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

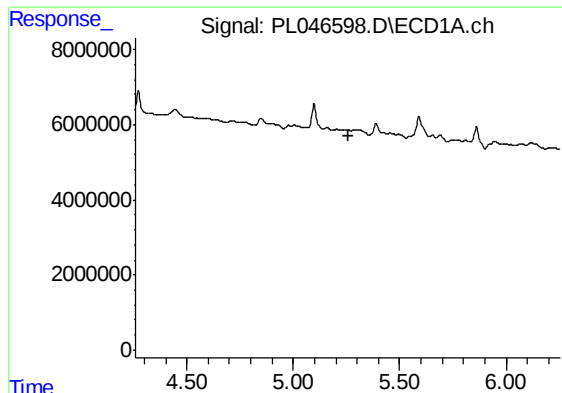

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CS-14

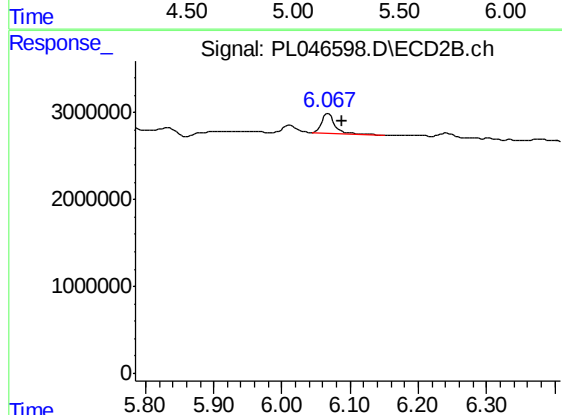


#25 Chlordane-3

R.T.: 6.068 min
Delta R.T.: -0.021 min
Response: 3199722
Conc: 8.39 ng/ml

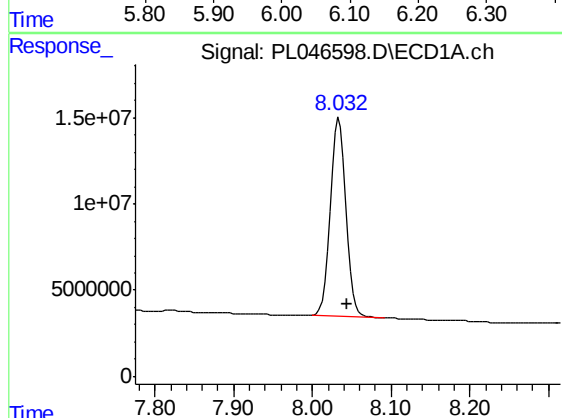

#28 Decachlorobiphenyl

R.T.: 8.034 min
Delta R.T.: -0.011 min
Response: 161093551
Conc: 19.15 ng/ml

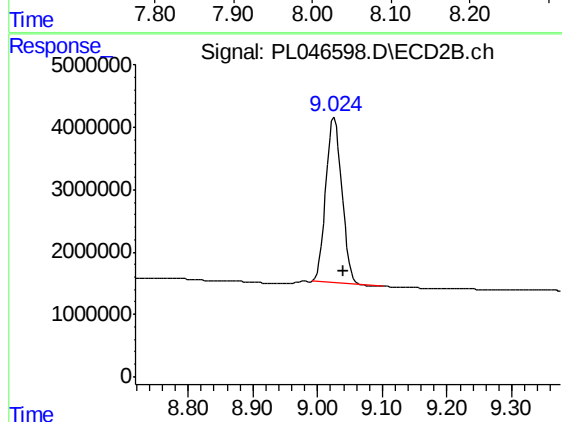

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.014 min
Response: 45640688
Conc: 19.69 ng/ml