

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032719\
 Data File : PL046526.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2019 09:32
 Operator : AJ\SJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 13:30:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.359	3.977	366.8E6	107.0E6	50.422	46.752
28)	SA Decachlor...	8.034	9.028	390.6E6	111.4E6	46.433	48.030
Target Compounds							
23)	Chlordane-1	4.204	4.969	150.9E6	53317176	448.591	492.687
24)	Chlordane-2	4.695	5.436	173.5E6	53601246	457.407	458.878
25)	Chlordane-3	5.252	6.081	519.2E6	177.5E6	466.186	465.678
26)	Chlordane-4	5.307	6.155	478.6E6	218.4E6	462.807	473.348
27)	Chlordane-5	6.131	6.957	156.6E6	40828493	458.955	454.469



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032719\
Data File : PL046526.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2019 09:32
Operator : AJ\SJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 13:30:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

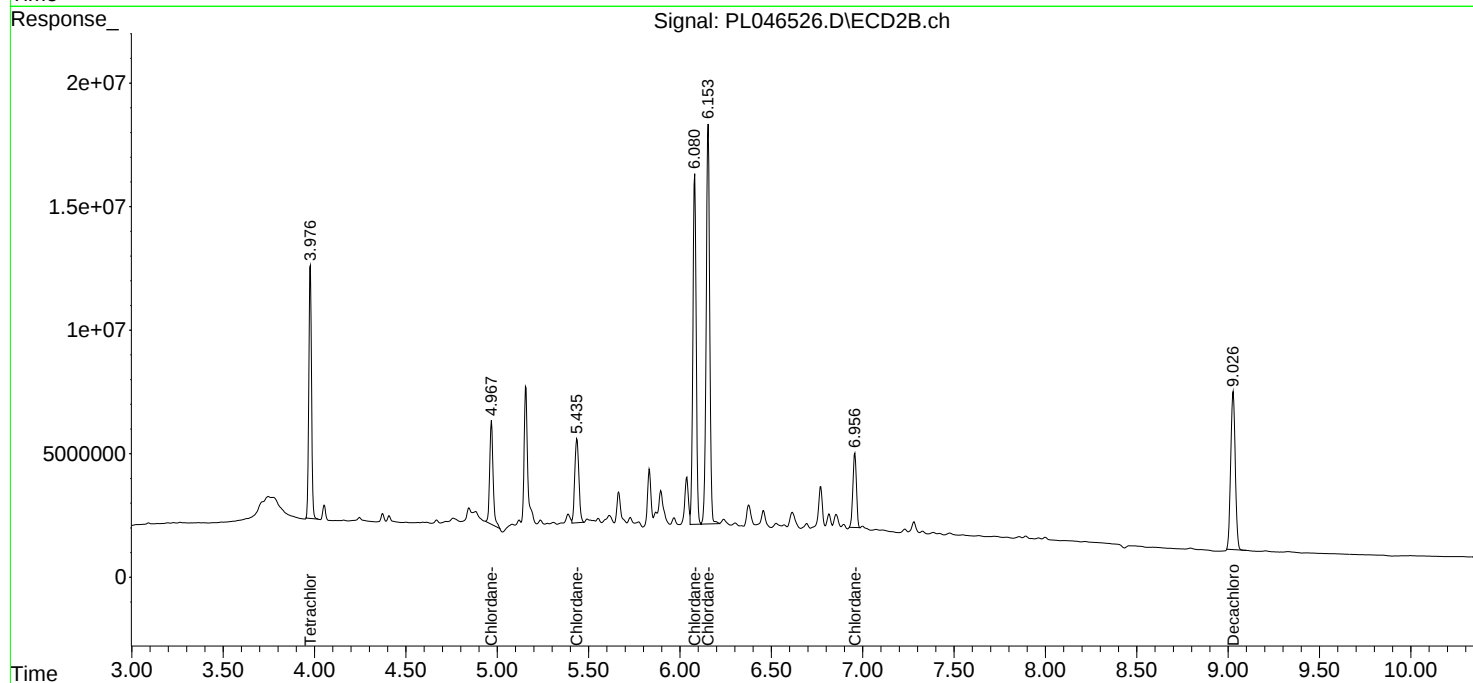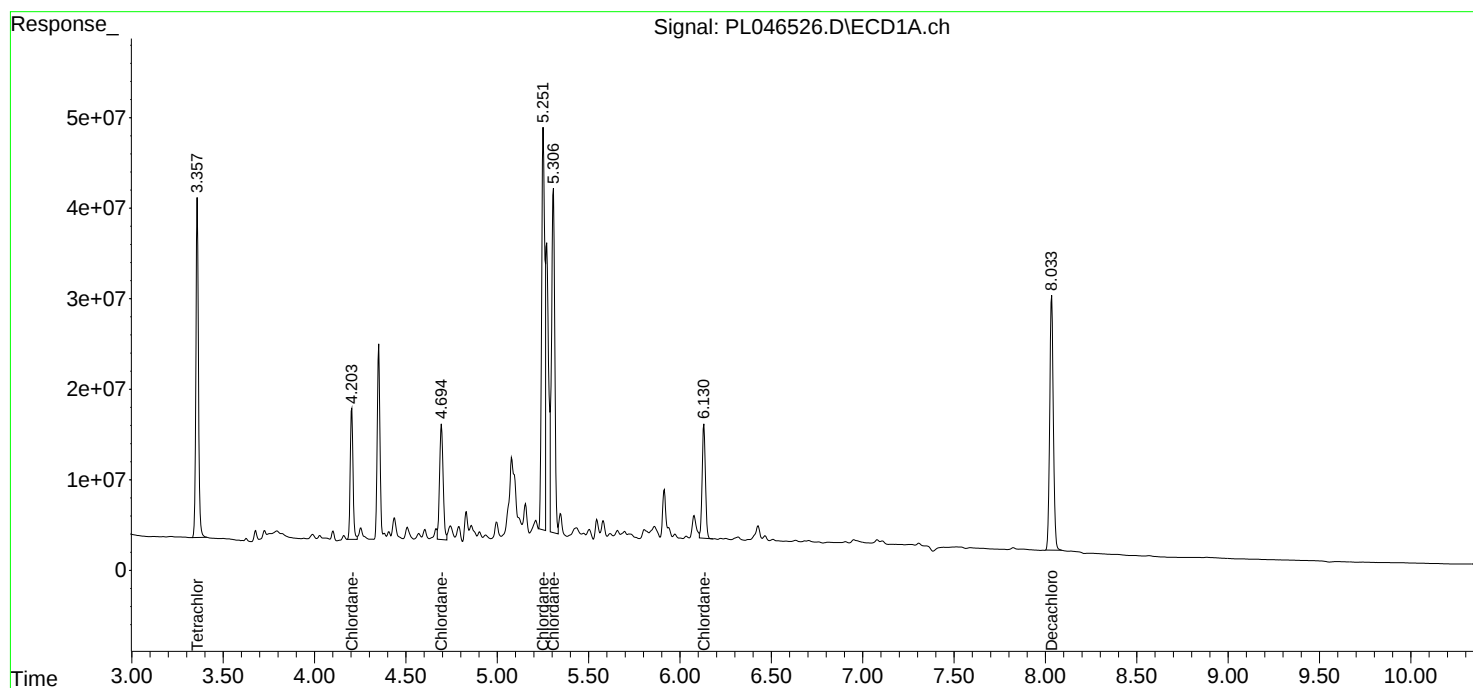


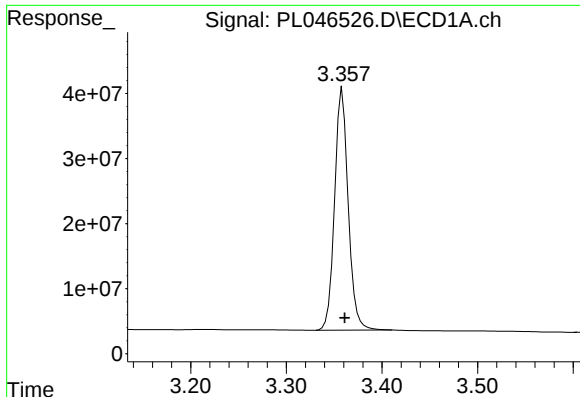

#1 Tetrachloro-m-xylene


R.T.: 3.359 min
Delta R.T.: -0.002 min
Response: 366799951
Conc: 50.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

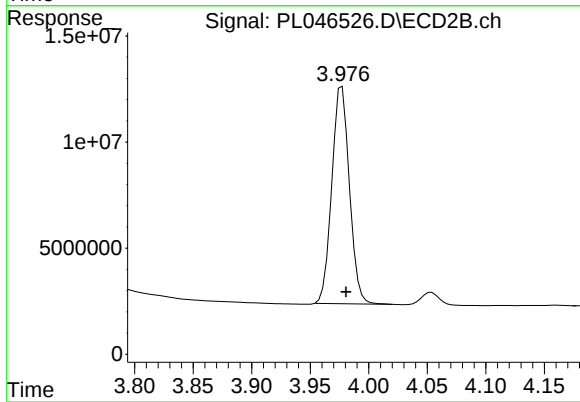


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.004 min
Response: 107043498
Conc: 46.75 ng/ml

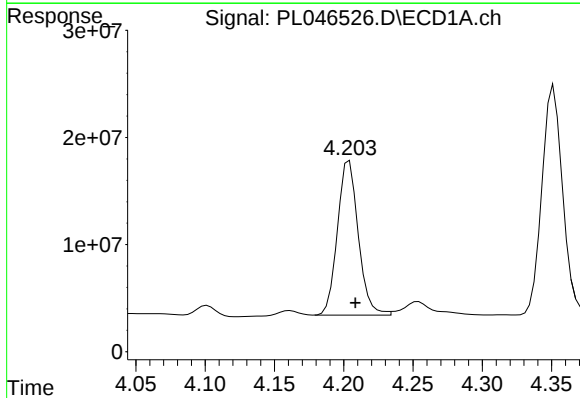


#23 Chlordane-1

R.T.: 4.204 min
Delta R.T.: -0.004 min
Response: 150859043
Conc: 448.59 ng/ml

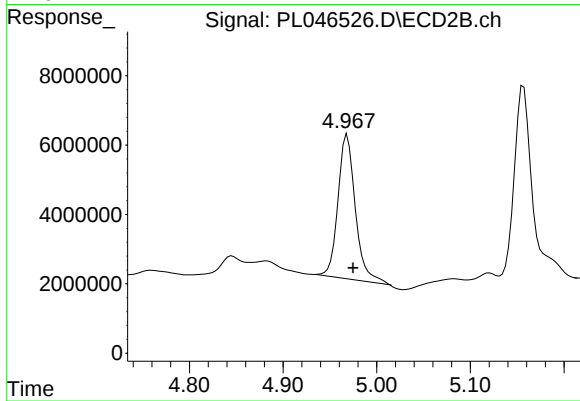

#23 Chlordane-1


R.T.: 4.969 min
Delta R.T.: -0.006 min
Response: 53317176
Conc: 492.69 ng/ml

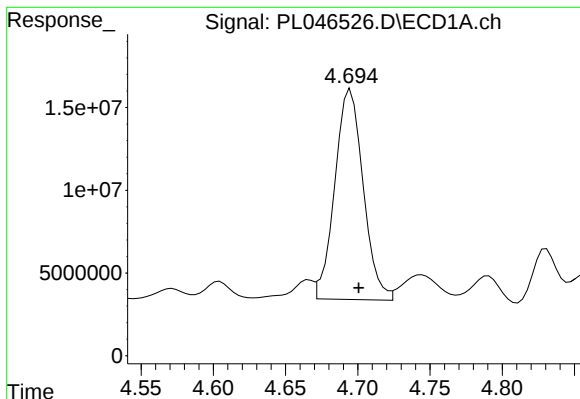

#24 Chlordane-2


R.T.: 4.695 min
Delta R.T.: -0.006 min
Response: 173549052
Conc: 457.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

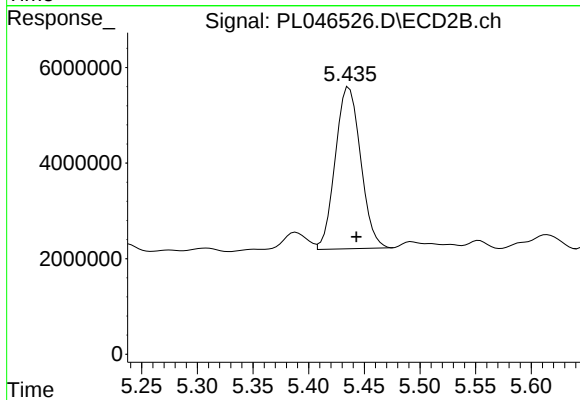


#24 Chlordane-2

R.T.: 5.436 min
Delta R.T.: -0.006 min
Response: 53601246
Conc: 458.88 ng/ml

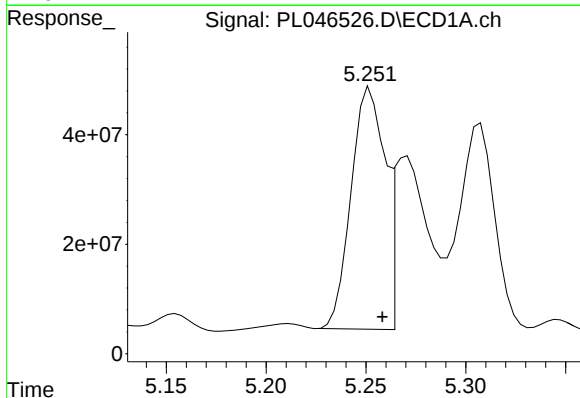


#25 Chlordane-3

R.T.: 5.252 min
Delta R.T.: -0.006 min
Response: 519178830
Conc: 466.19 ng/ml

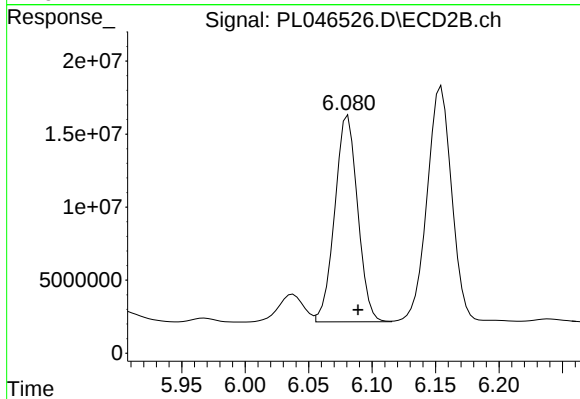

#25 Chlordane-3


R.T.: 6.081 min
Delta R.T.: -0.008 min
Response: 177547869
Conc: 465.68 ng/ml

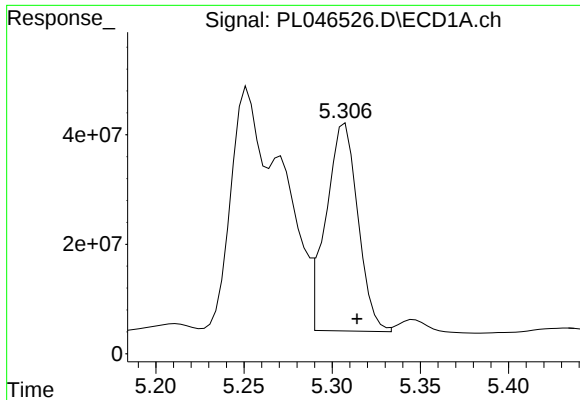

#26 Chlordane-4


R.T.: 5.307 min
Delta R.T.: -0.007 min
Response: 478570449
Conc: 462.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

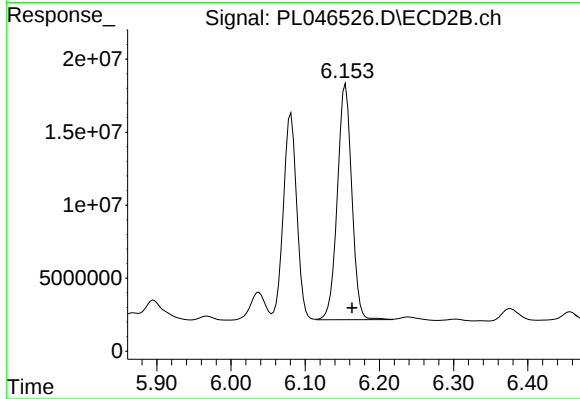


#26 Chlordane-4

R.T.: 6.155 min
Delta R.T.: -0.009 min
Response: 218414792
Conc: 473.35 ng/ml

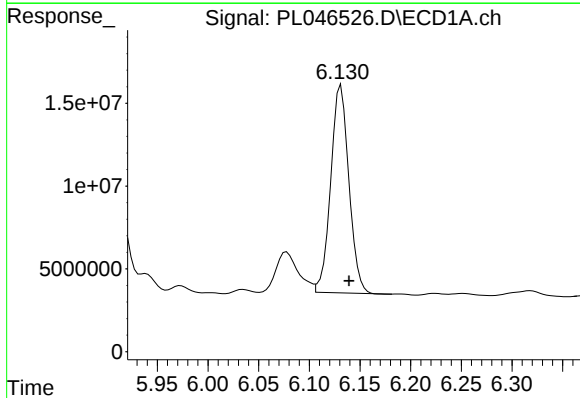


#27 Chlordane-5

R.T.: 6.131 min
Delta R.T.: -0.008 min
Response: 156626110
Conc: 458.95 ng/ml

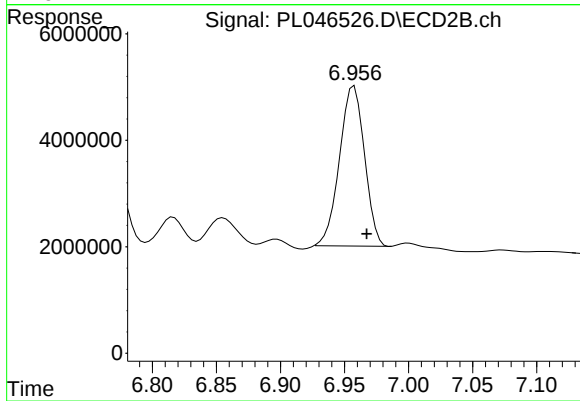

#27 Chlordane-5

R.T.: 6.957 min
Delta R.T.: -0.010 min
Response: 40828493
Conc: 454.47 ng/ml

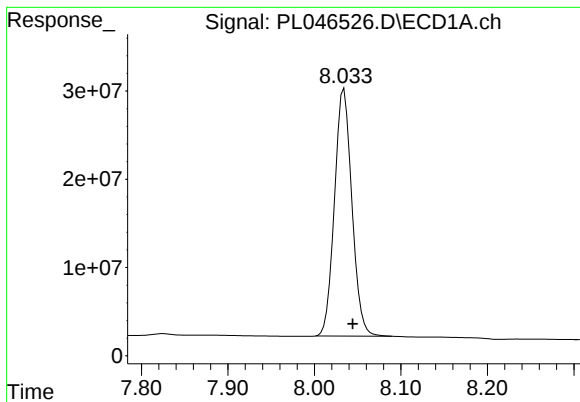

#28 Decachlorobiphenyl


R.T.: 8.034 min

Delta R.T.: -0.010 min

Response: 390552695

Conc: 46.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

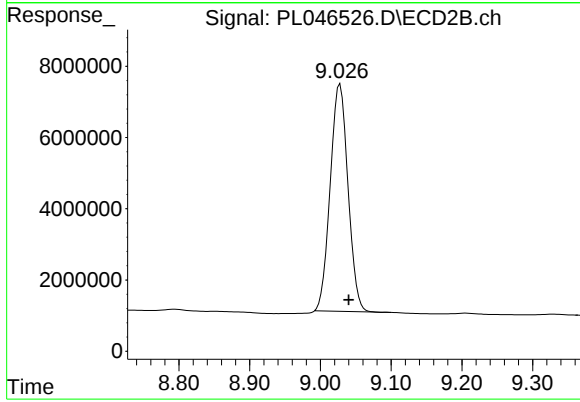

#28 Decachlorobiphenyl

R.T.: 9.028 min

Delta R.T.: -0.012 min

Response: 111356455

Conc: 48.03 ng/ml