

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032719\
 Data File : PL046536.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2019 11:55
 Operator : AJ\SJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 13:31:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.977	372.7E6	108.3E6	51.239	47.313
28)	SA Decachlor...	8.034	9.028	407.7E6	116.0E6	48.471	50.042
Target Compounds							
23)	Chlordane-1	4.204	4.968	158.9E6	53120399	472.377	490.869
24)	Chlordane-2	4.695	5.436	182.2E6	54978131	480.139	470.666
25)	Chlordane-3	5.252	6.081	535.9E6	184.8E6	481.245	484.662
26)	Chlordane-4	5.308	6.155	494.8E6	225.2E6	478.479	487.991
27)	Chlordane-5	6.132	6.958	162.7E6	42586035	476.711	474.033



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032719\
Data File : PL046536.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2019 11:55
Operator : AJ\SJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 13:31:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

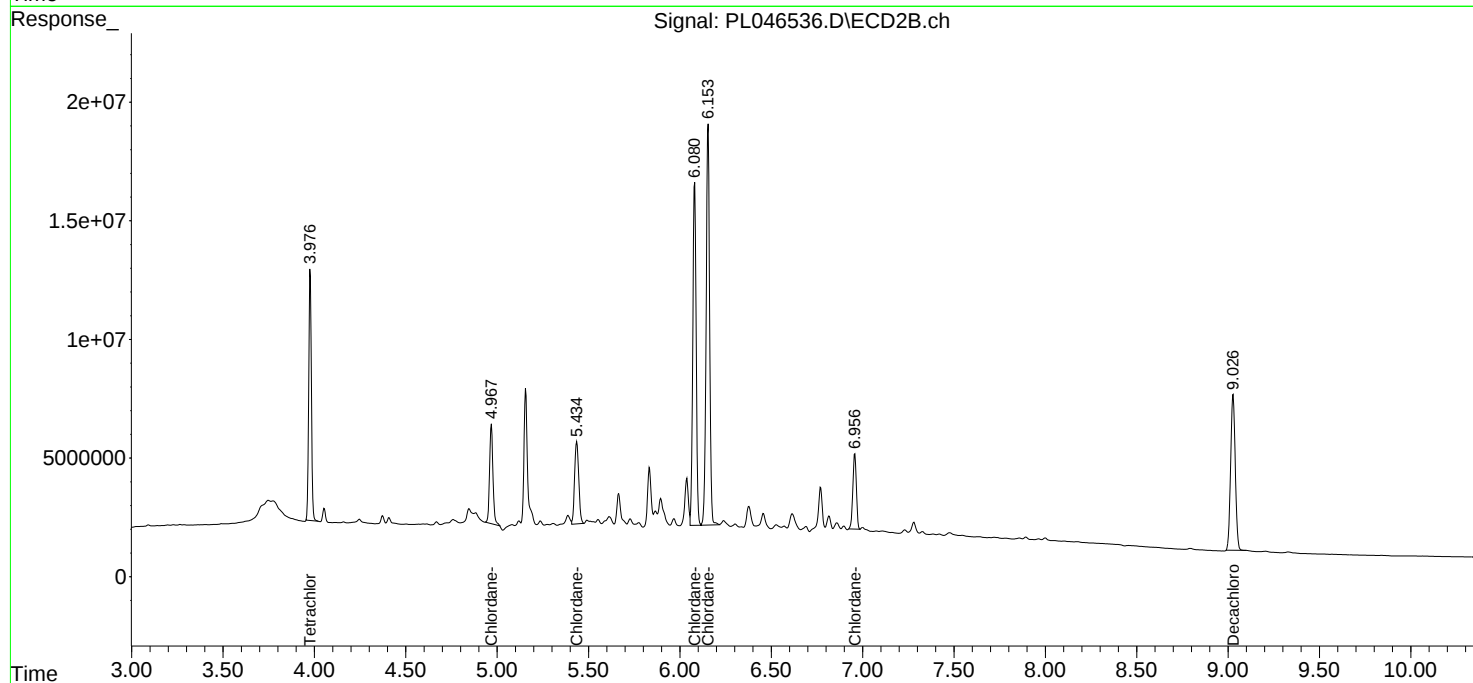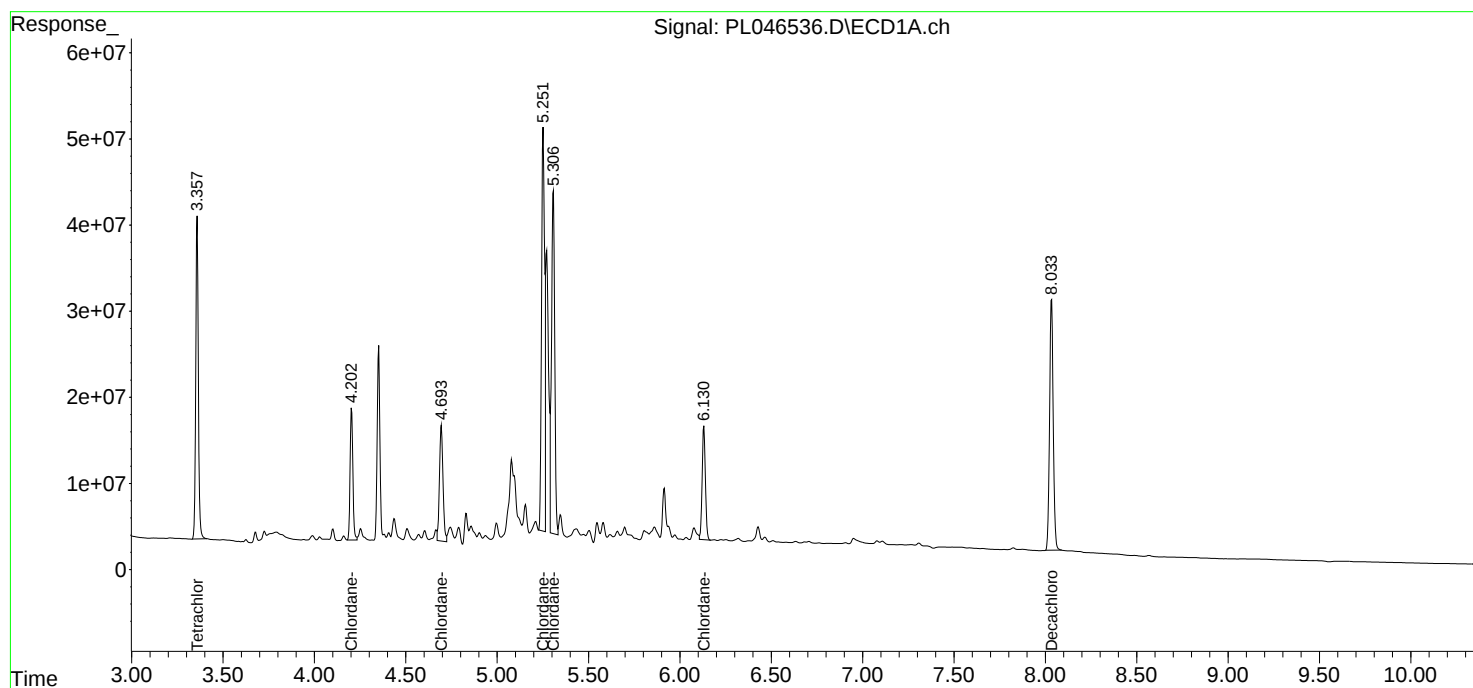


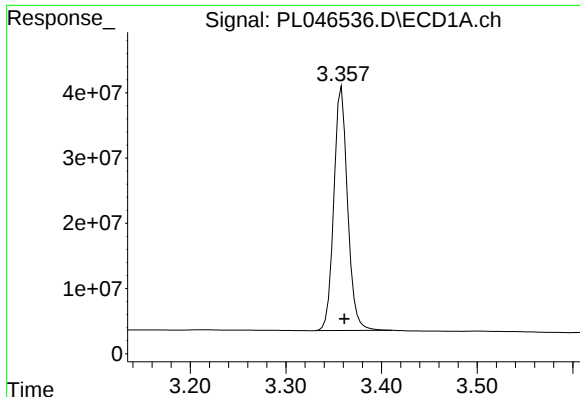

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 372744510
Conc: 51.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

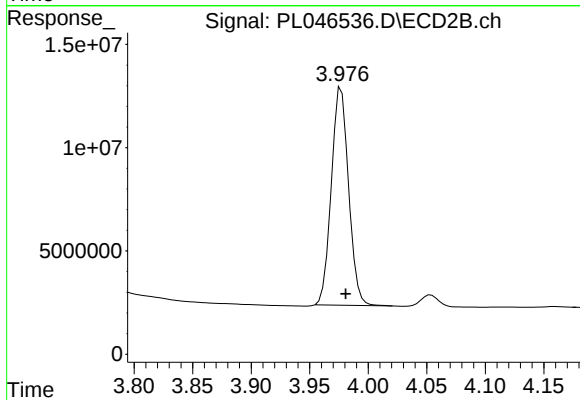


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.004 min
Response: 108327678
Conc: 47.31 ng/ml

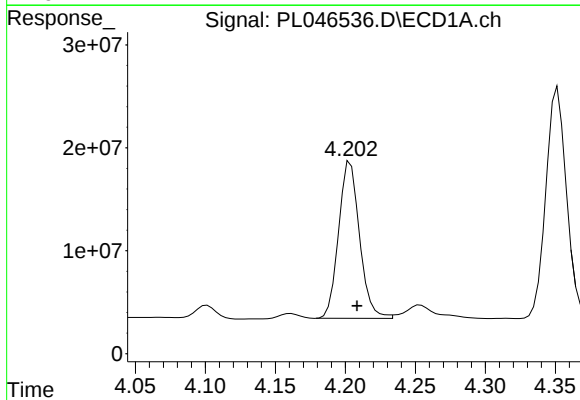


#23 Chlordane-1

R.T.: 4.204 min
Delta R.T.: -0.005 min
Response: 158858187
Conc: 472.38 ng/ml

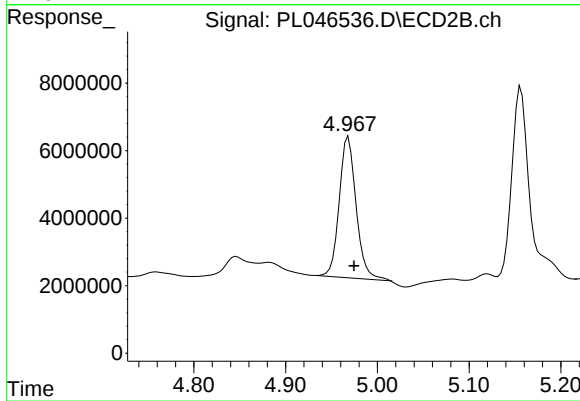

#23 Chlordane-1


R.T.: 4.968 min
Delta R.T.: -0.006 min
Response: 53120399
Conc: 490.87 ng/ml

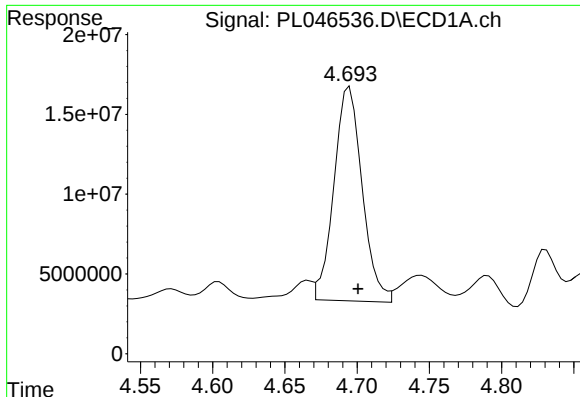

#24 Chlordane-2


R.T.: 4.695 min
Delta R.T.: -0.006 min
Response: 182173674
Conc: 480.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

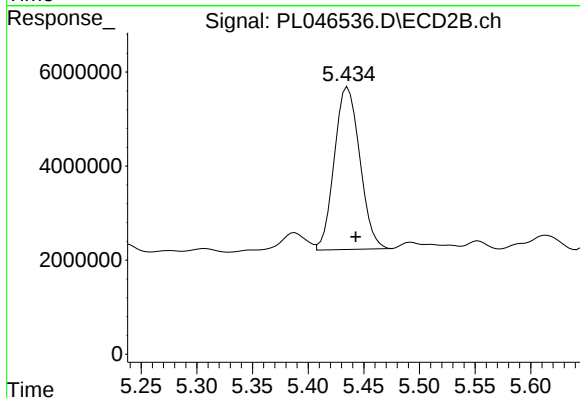


#24 Chlordane-2

R.T.: 5.436 min
Delta R.T.: -0.007 min
Response: 54978131
Conc: 470.67 ng/ml

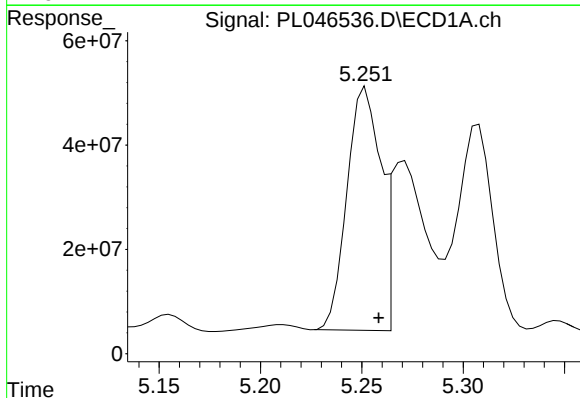


#25 Chlordane-3

R.T.: 5.252 min
Delta R.T.: -0.006 min
Response: 535949450
Conc: 481.24 ng/ml

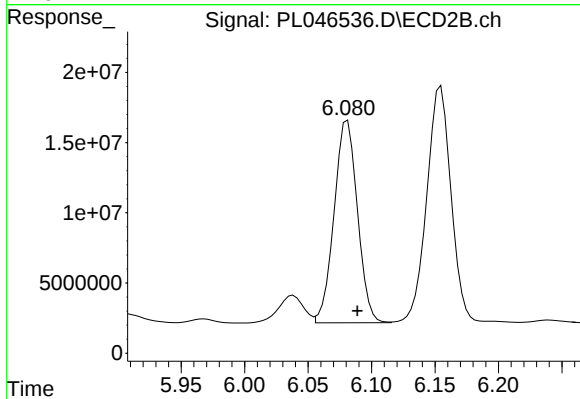

#25 Chlordane-3


R.T.: 6.081 min
Delta R.T.: -0.008 min
Response: 184785861
Conc: 484.66 ng/ml

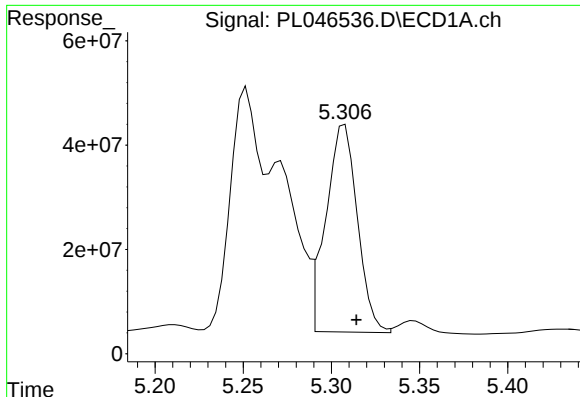

#26 Chlordane-4


R.T.: 5.308 min
Delta R.T.: -0.007 min
Response: 494775366
Conc: 478.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

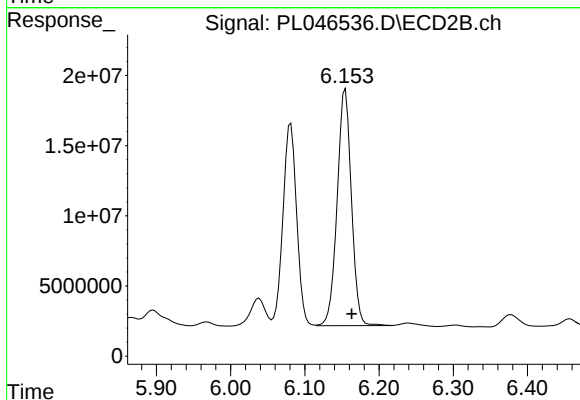


#26 Chlordane-4

R.T.: 6.155 min
Delta R.T.: -0.009 min
Response: 225171059
Conc: 487.99 ng/ml

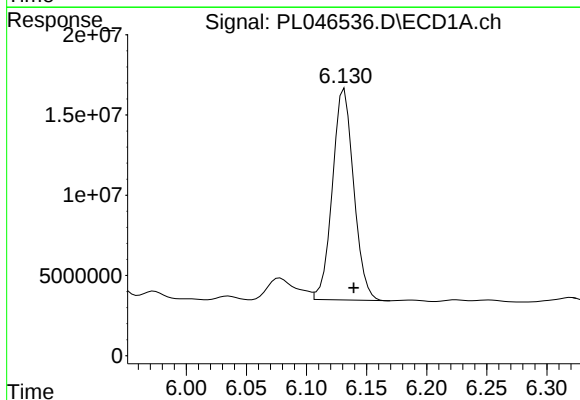


#27 Chlordane-5

R.T.: 6.132 min
Delta R.T.: -0.008 min
Response: 162685920
Conc: 476.71 ng/ml

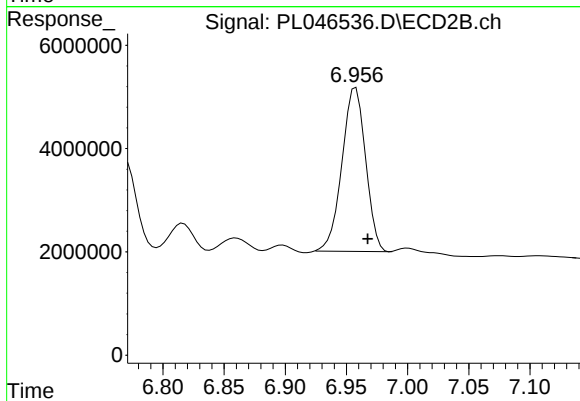

#27 Chlordane-5


R.T.: 6.958 min
Delta R.T.: -0.010 min
Response: 42586035
Conc: 474.03 ng/ml

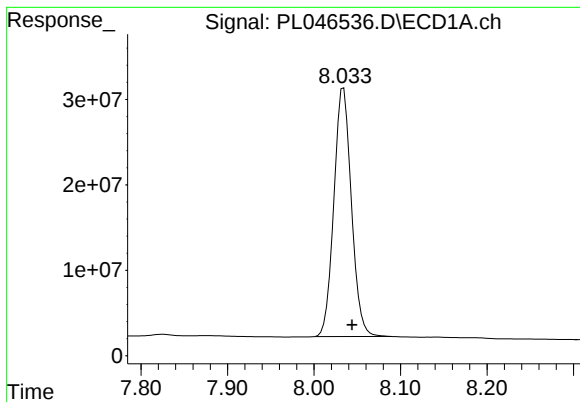

#28 Decachlorobiphenyl

R.T.: 8.034 min
Delta R.T.: -0.010 min
Response: 407689083
Conc: 48.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

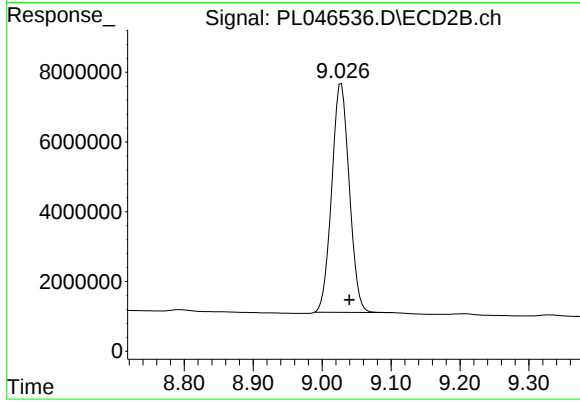

#28 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: -0.012 min
Response: 116021783
Conc: 50.04 ng/ml