

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032720\
 Data File : PL057647.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 13:28
 Operator : AJ\MA
 Sample : PB127848BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB127848BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 00:51:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	3.957	229.8E6	45685155	24.795	21.057
28)	SA Decachlor...	8.209	8.979	228.4E6	48271984	21.590	21.770
Target Compounds							
2)	A alpha-BHC	3.889	0.000	2727080	0	0.171	N.D. #
8)	B Heptachlo...	5.173	0.000	709500	0	0.055	N.D. #
11)	B alpha-Chl...	5.454	0.000	2487255	0	0.192	N.D. #
15)	B Endosulfa...	6.278	0.000	1496653	0	0.138	N.D. #
16)	A 4,4'-DDD	6.121	0.000	4060706	0	0.414	N.D. #
18)	B Endrin al...	6.454	0.000	177049	0	0.019	N.D. #
20)	A Methoxychlor	6.917	0.000	222944	0	0.042	N.D. #
22)	Mirex	7.334	0.000	851425	0	0.105	N.D. #
23)	Chlordane-1	4.356f	0.000	1737224	0	5.352	N.D. #
26)	Chlordane-4	5.454	0.000	2487255	0	2.594	N.D. #
27)	Chlordane-5	6.278	0.000	1496653	0	4.113	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032720\
Data File : PL057647.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 13:28
Operator : AJ\MA
Sample : PB127848BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB127848BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 00:51:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

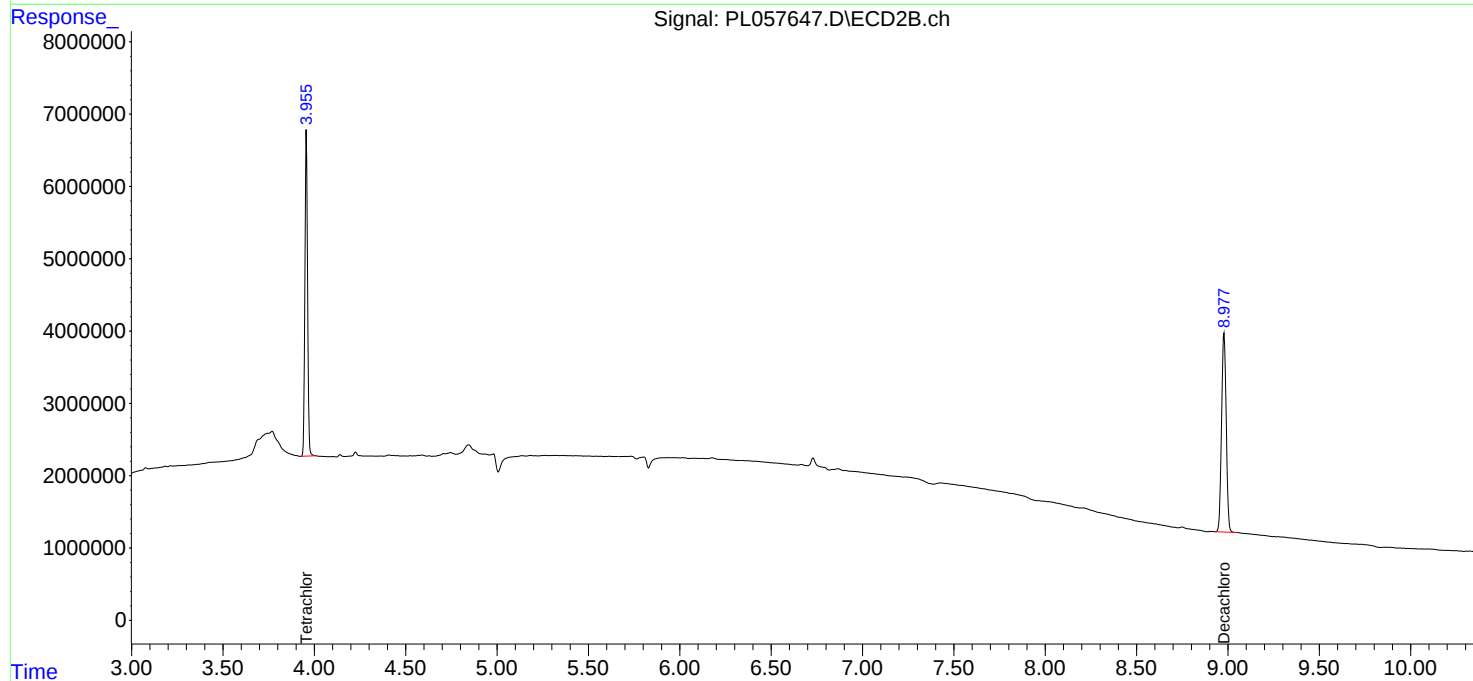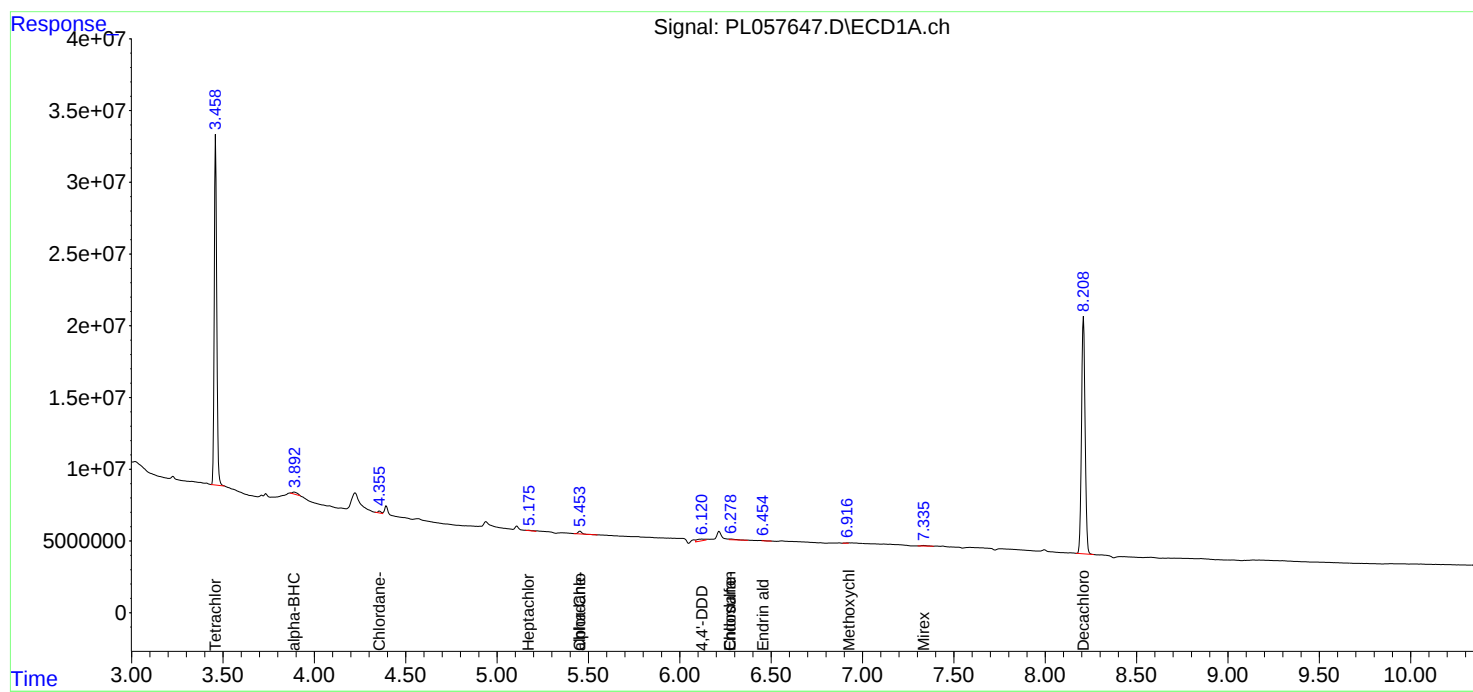


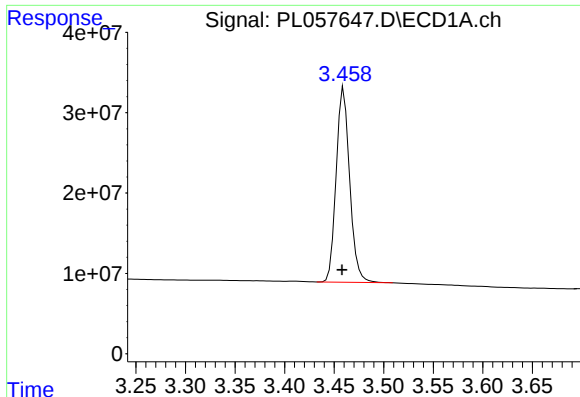

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.002 min
Response: 229831074
Conc: 24.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127848BL

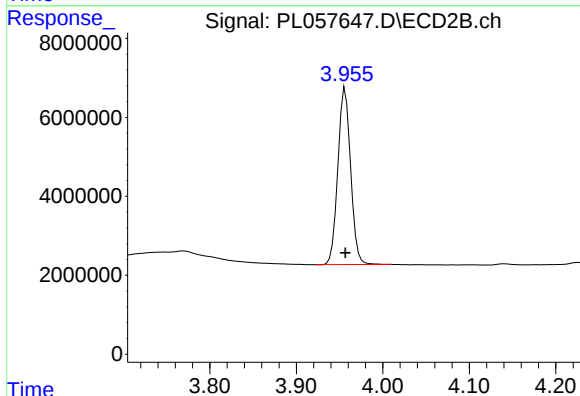


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 45685155
Conc: 21.06 ng/ml

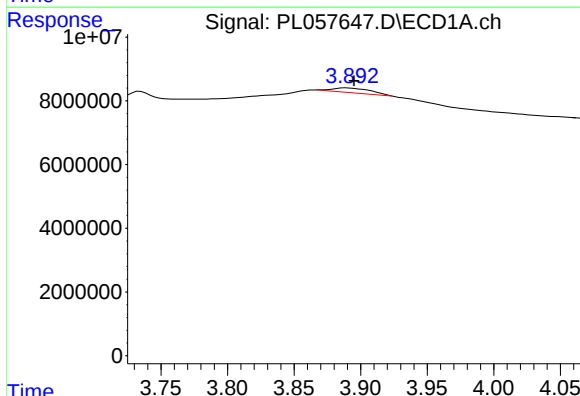


#2 alpha-BHC

R.T.: 3.889 min
Delta R.T.: -0.006 min
Response: 2727080
Conc: 0.17 ng/ml

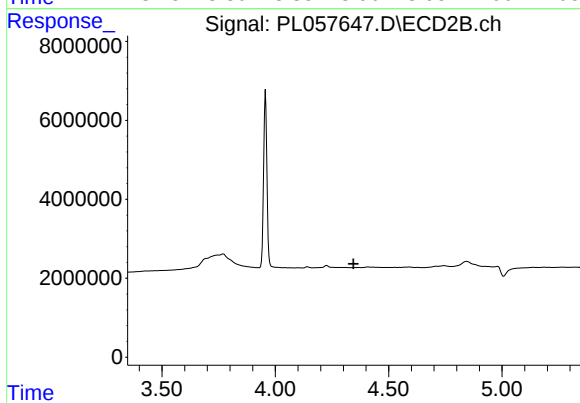

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

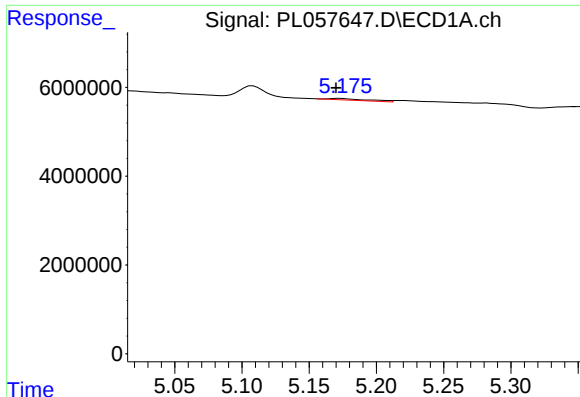

#8 Heptachlor epoxide


R.T.: 5.173 min
Delta R.T.: 0.003 min
Response: 709500
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127848BL

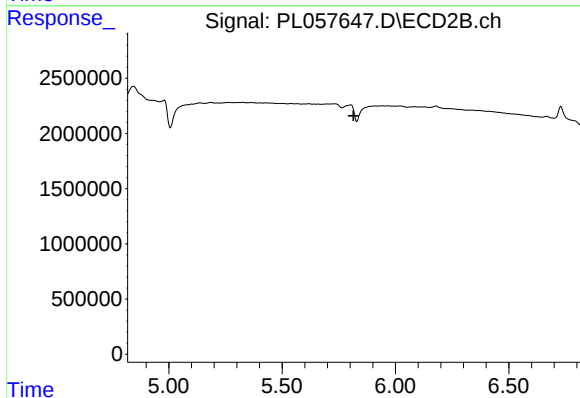


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.815 min
Response: 0
Conc: N.D.

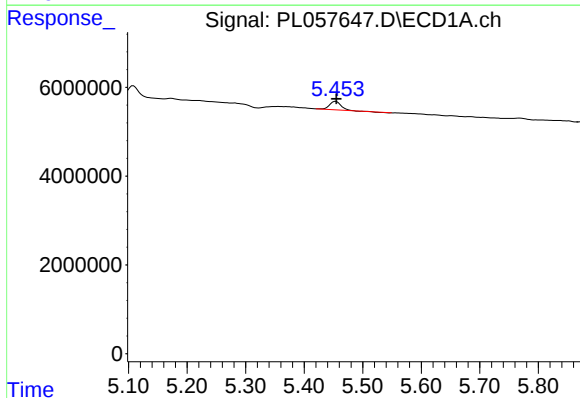


#11 alpha-Chlordane

R.T.: 5.454 min
Delta R.T.: 0.000 min
Response: 2487255
Conc: 0.19 ng/ml

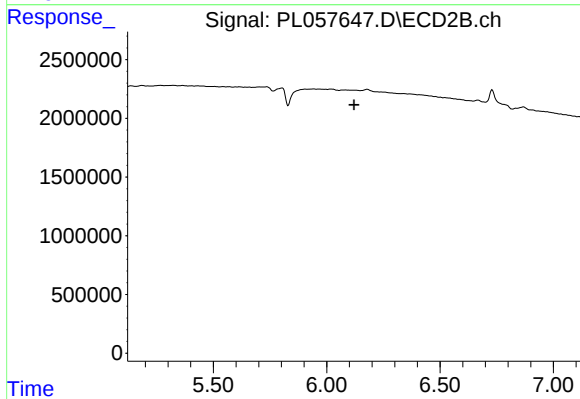

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.120 min
Response: 0
Conc: N.D.

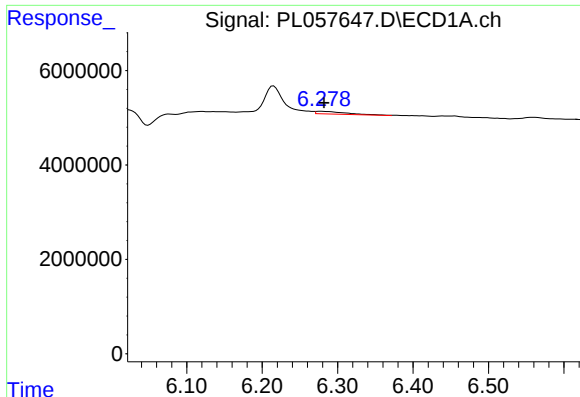

#15 Endosulfan II


R.T.: 6.278 min
Delta R.T.: -0.004 min
Response: 1496653
Conc: 0.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127848BL

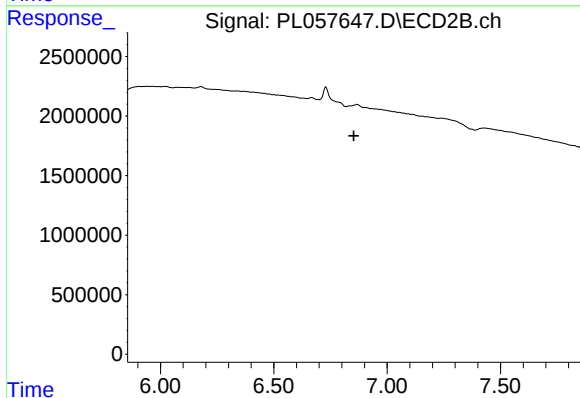


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.852 min
Response: 0
Conc: N.D.

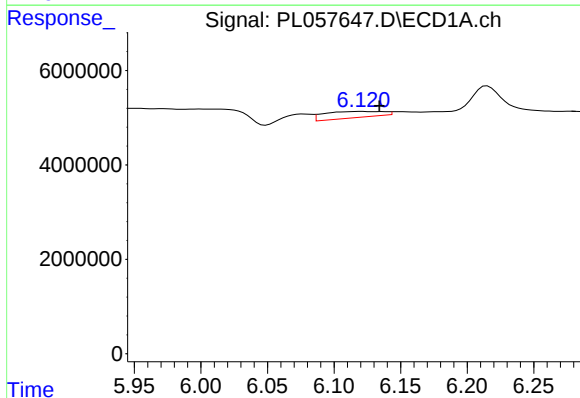


#16 4,4'-DDD

R.T.: 6.121 min
Delta R.T.: -0.013 min
Response: 4060706
Conc: 0.41 ng/ml

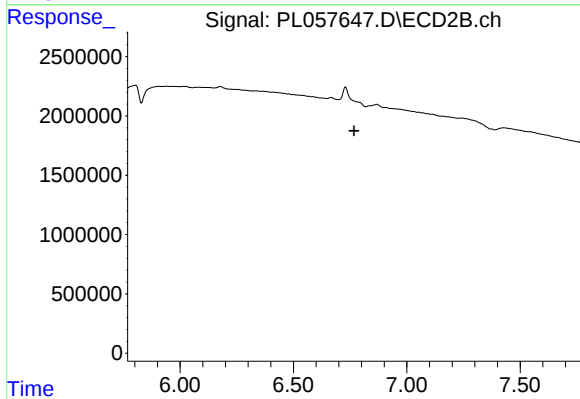

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.768 min
Response: 0
Conc: N.D.

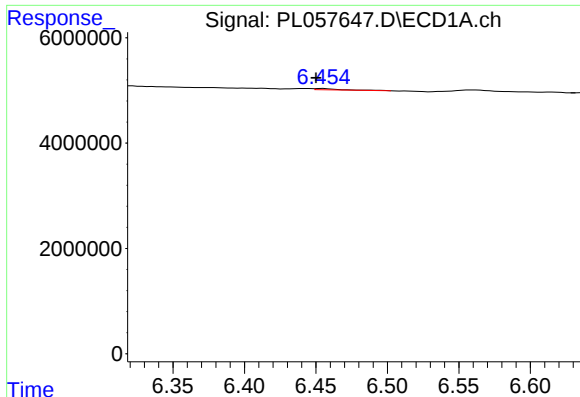

#18 Endrin aldehyde


R.T.: 6.454 min
Delta R.T.: 0.004 min
Response: 177049
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127848BL

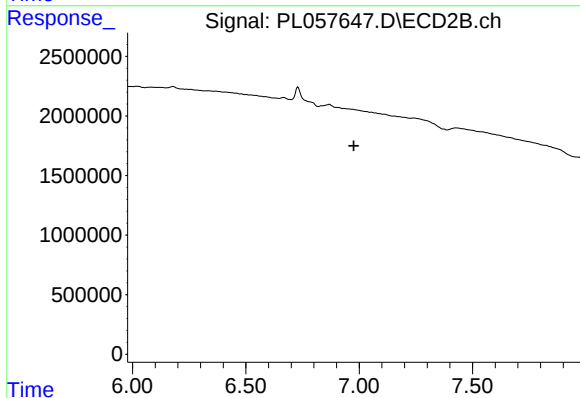


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.976 min
Response: 0
Conc: N.D.

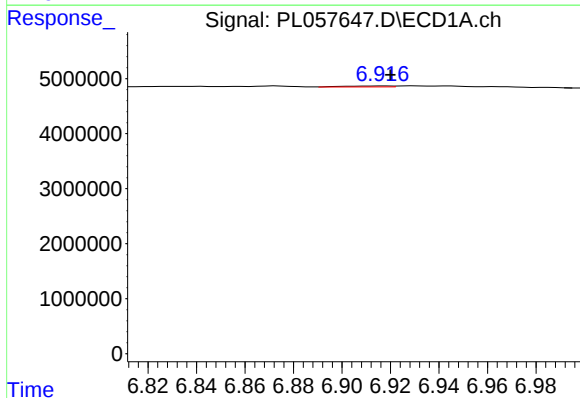


#20 Methoxychlor

R.T.: 6.917 min
Delta R.T.: -0.003 min
Response: 222944
Conc: 0.04 ng/ml

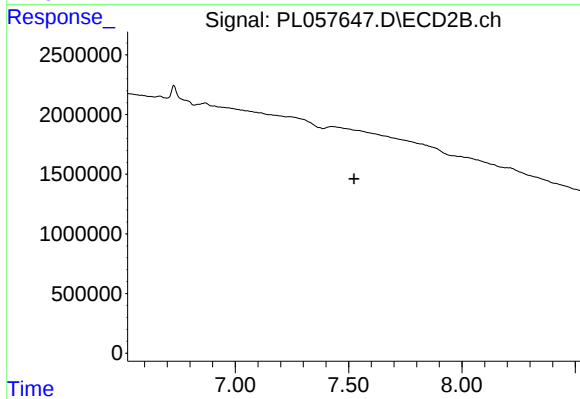

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.524 min
Response: 0
Conc: N.D.

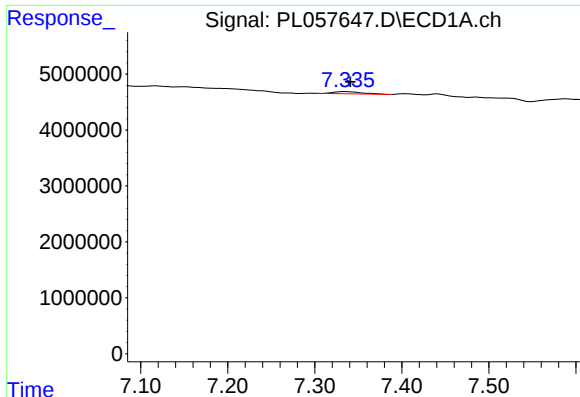

#22 Mirex


R.T.: 7.334 min
Delta R.T.: -0.007 min
Response: 851425
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127848BL

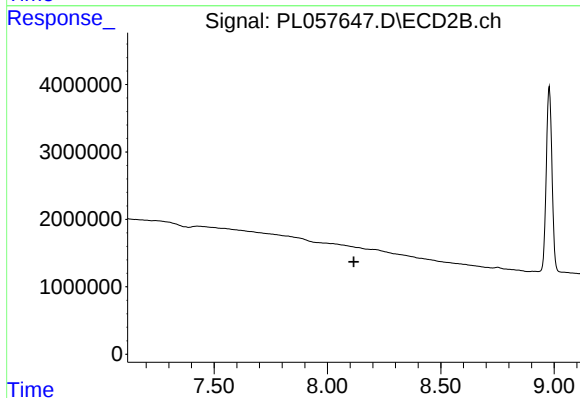


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

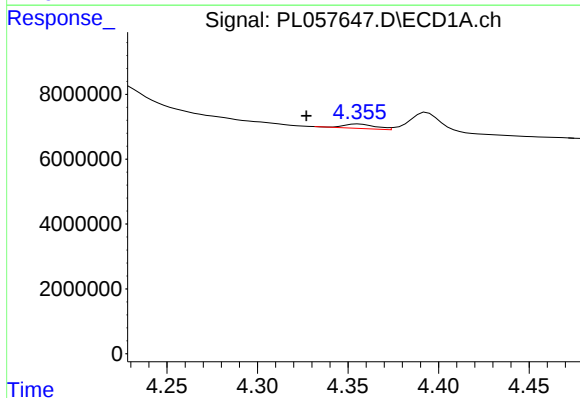


#23 Chlordane-1

R.T.: 4.356 min
Delta R.T.: 0.029 min
Response: 1737224
Conc: 5.35 ng/ml

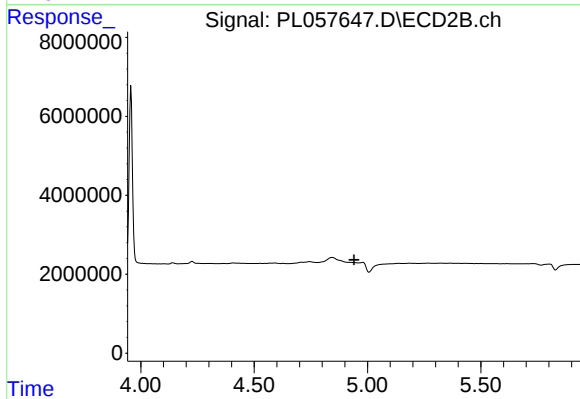

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

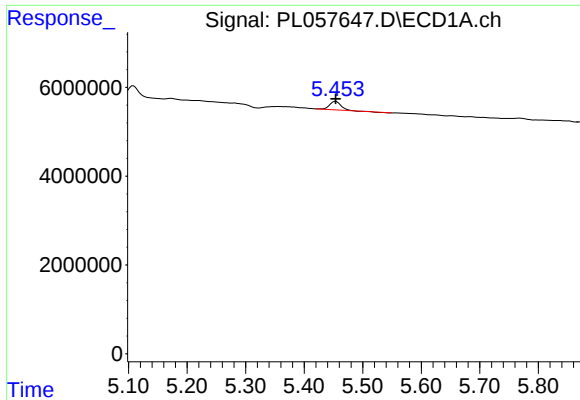

#26 Chlordane-4


R.T.: 5.454 min
Delta R.T.: 0.000 min
Response: 2487255
Conc: 2.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127848BL

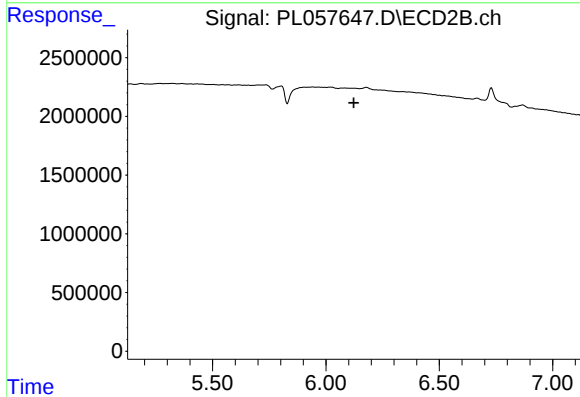


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.122 min
Response: 0
Conc: N.D.

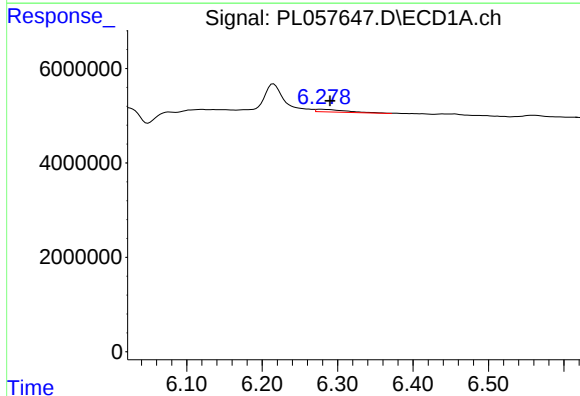


#27 Chlordane-5

R.T.: 6.278 min
Delta R.T.: -0.012 min
Response: 1496653
Conc: 4.11 ng/ml

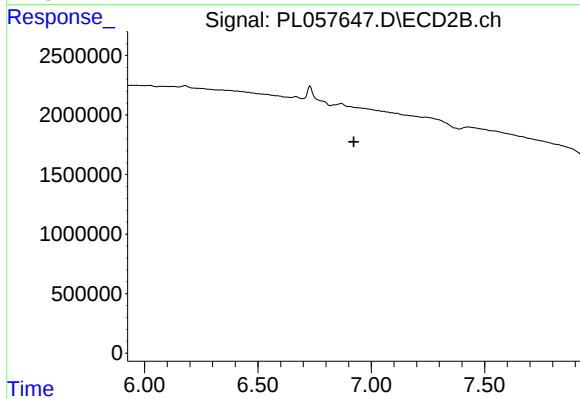

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

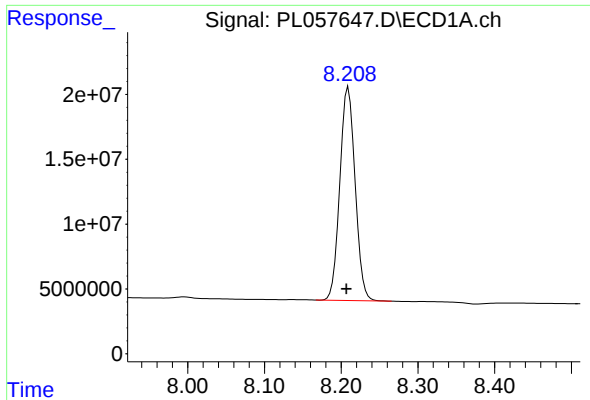

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.002 min
Response: 228449658
Conc: 21.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127848BL

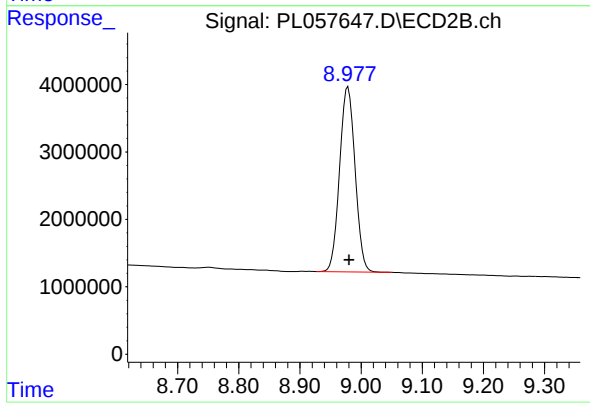

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.002 min
Response: 48271984
Conc: 21.77 ng/ml