

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032720\
 Data File : PL057659.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 16:51
 Operator : AJ\MA
 Sample : PB127868TB
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB127868TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 00:55:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.958	237.2E6	50538562	25.589	23.294
28)	SA Decachlor...	8.207	8.981	241.8E6	53096728	22.849	23.946
Target Compounds							
2)	A alpha-BHC	3.896	0.000	4994198	0	0.314	N.D. #
4)	MA Heptachlor	0.000	5.137	0	7530884	N.D.	2.392 #
10)	B gamma-Chl...	5.413f	0.000	772589	0	0.059	N.D. #
14)	MA Endrin	5.996	0.000	6698567	0	0.586	N.D. #
16)	A 4,4'-DDD	6.127	0.000	1356896	0	0.138	N.D. #
18)	B Endrin al...	6.447	0.000	253672	0	0.027	N.D. #
23)	Chlordane-1	4.356f	0.000	2778218	0	8.560	N.D. #
25)	Chlordane-3	5.413f	0.000	772589	0	0.685	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032720\
Data File : PL057659.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 16:51
Operator : AJ\MA
Sample : PB127868TB
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB127868TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 00:55:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

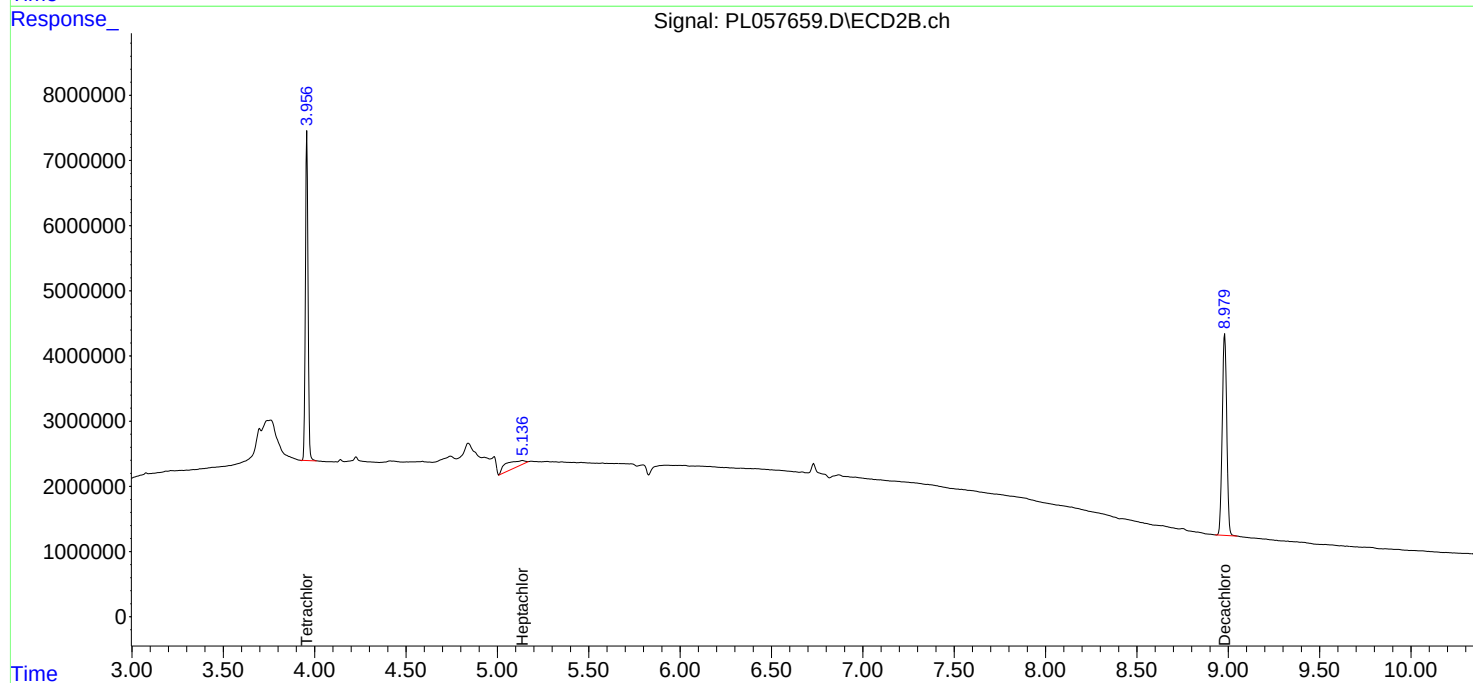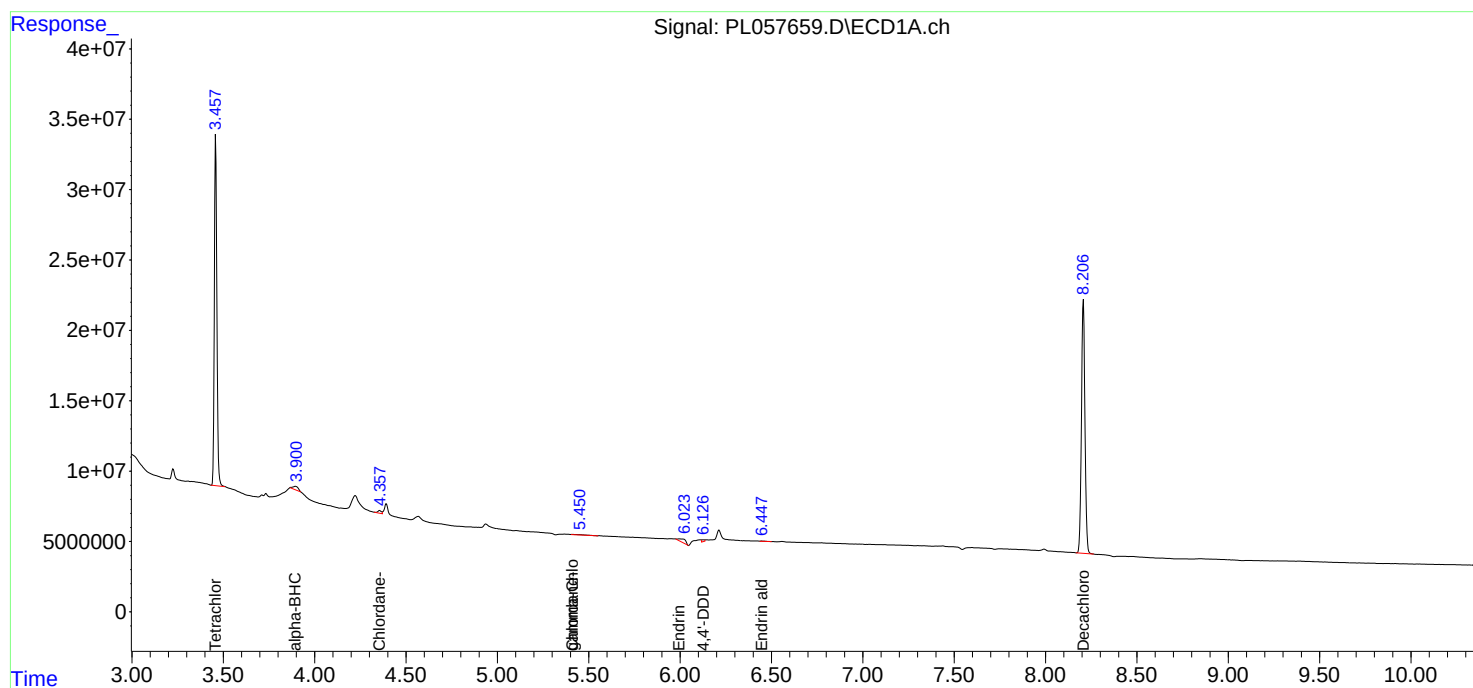


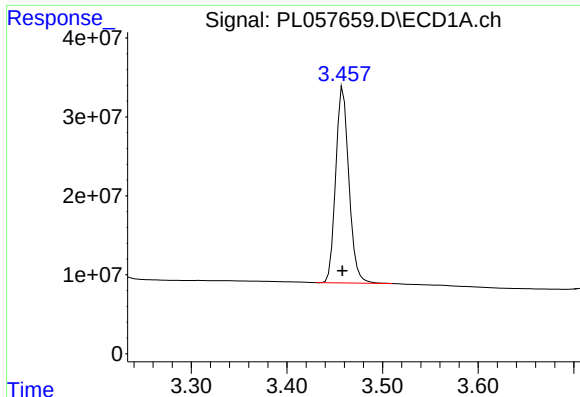

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 237195183
Conc: 25.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127868TB

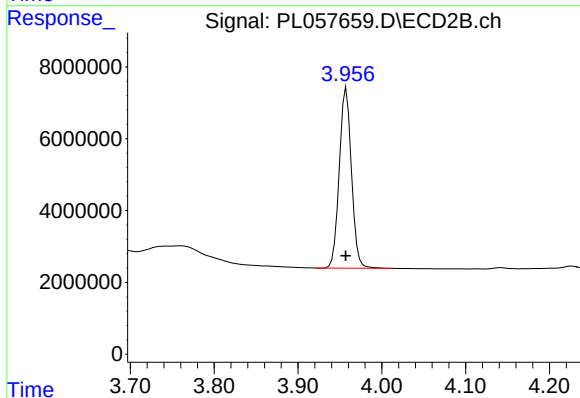


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 50538562
Conc: 23.29 ng/ml

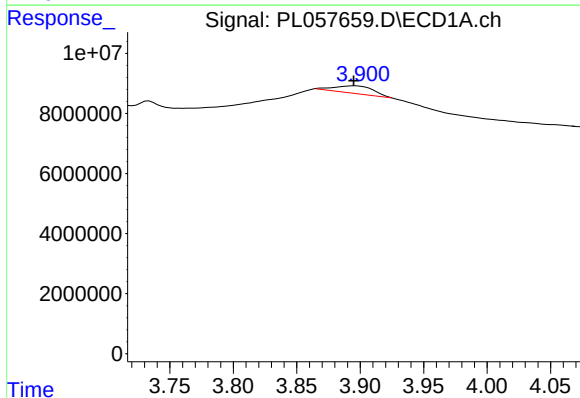


#2 alpha-BHC

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 4994198
Conc: 0.31 ng/ml

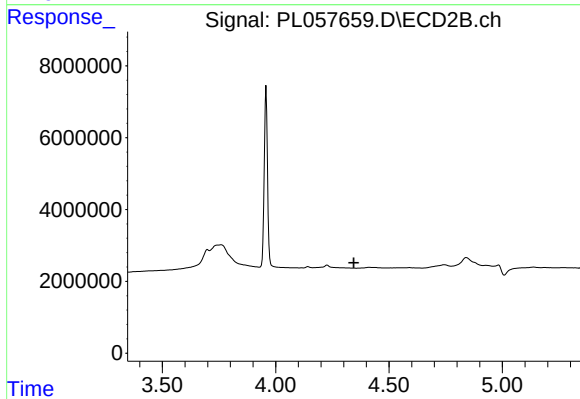

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

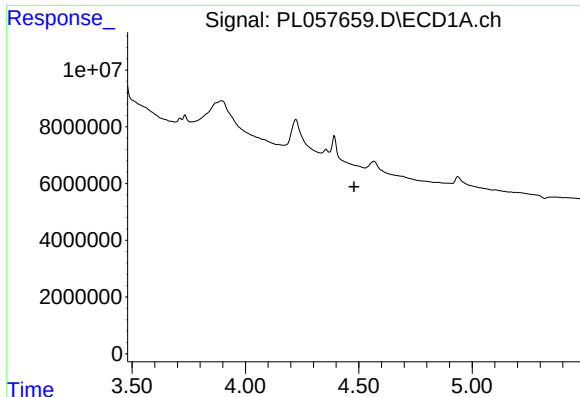

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB127868TB

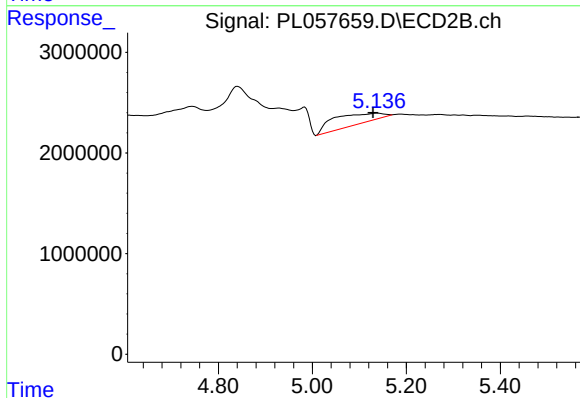


#4 Heptachlor

R.T.: 5.137 min
Delta R.T.: 0.008 min
Response: 7530884
Conc: 2.39 ng/ml

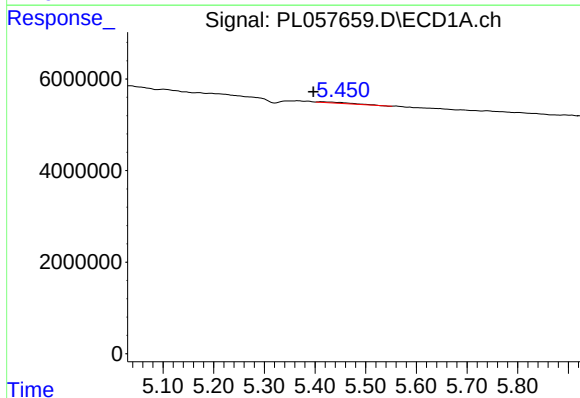


#10 gamma-Chlordane

R.T.: 5.413 min
Delta R.T.: 0.016 min
Response: 772589
Conc: 0.06 ng/ml

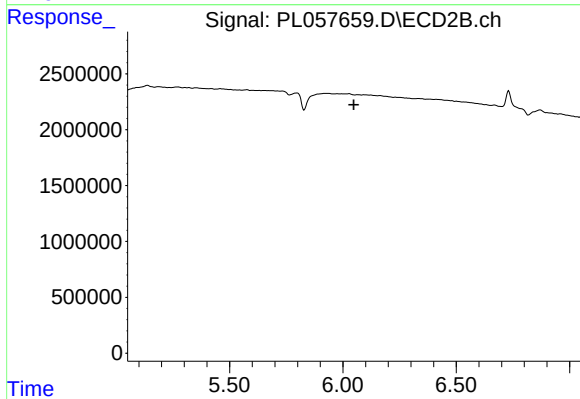

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

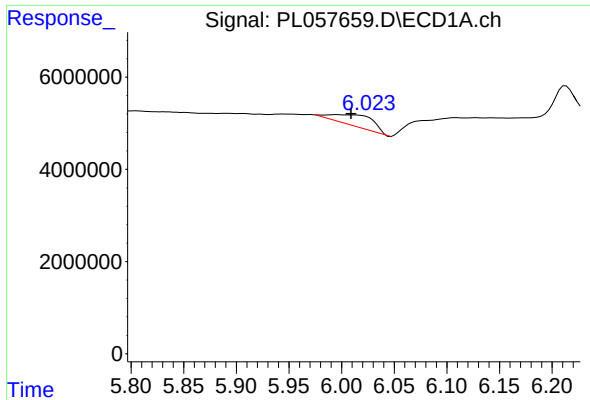

#14 Endrin


R.T.: 5.996 min
Delta R.T.: -0.013 min
Response: 6698567
Conc: 0.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127868TB

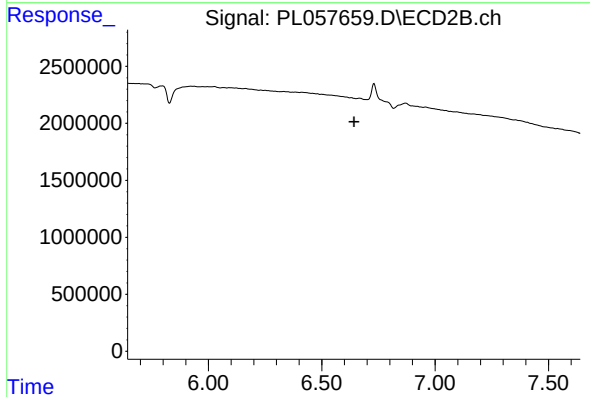


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.642 min
Response: 0
Conc: N.D.

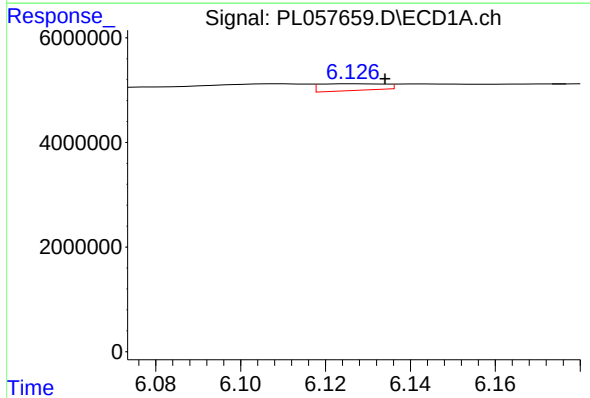


#16 4,4'-DDD

R.T.: 6.127 min
Delta R.T.: -0.007 min
Response: 1356896
Conc: 0.14 ng/ml

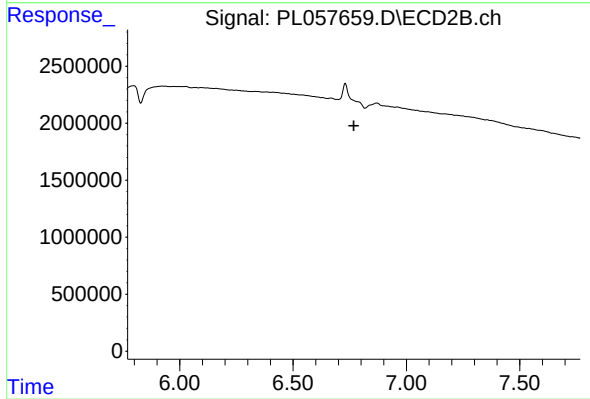

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.768 min
Response: 0
Conc: N.D.

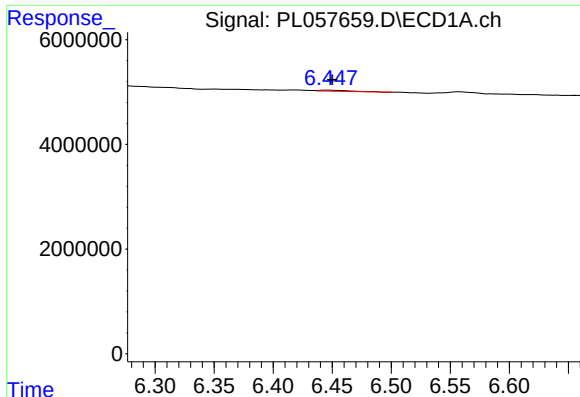

#18 Endrin aldehyde


R.T.: 6.447 min
Delta R.T.: -0.003 min
Response: 253672
Conc: 0.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127868TB

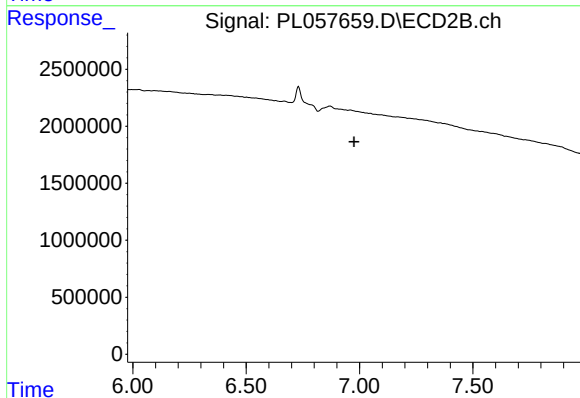


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.976 min
Response: 0
Conc: N.D.

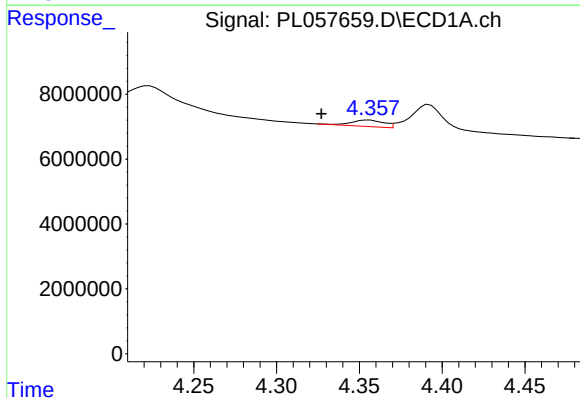


#23 Chlordane-1

R.T.: 4.356 min
Delta R.T.: 0.029 min
Response: 2778218
Conc: 8.56 ng/ml

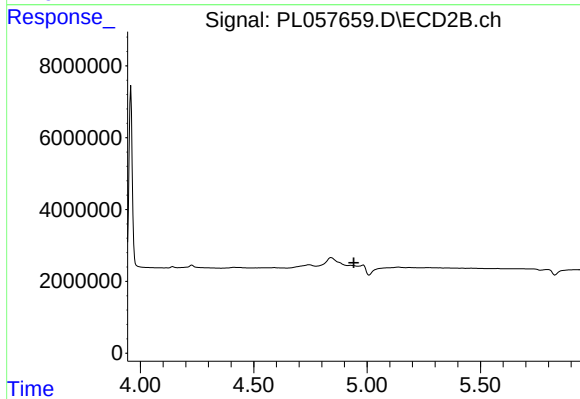

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

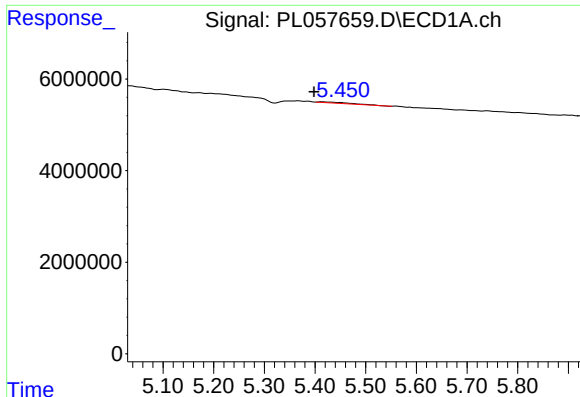

#25 Chlordane-3


R.T.: 5.413 min
Delta R.T.: 0.015 min
Response: 772589
Conc: 0.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127868TB

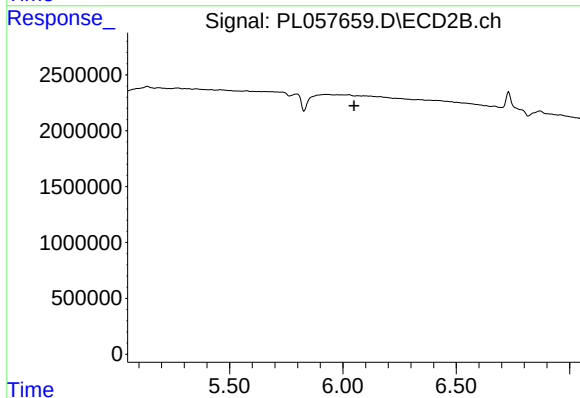


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

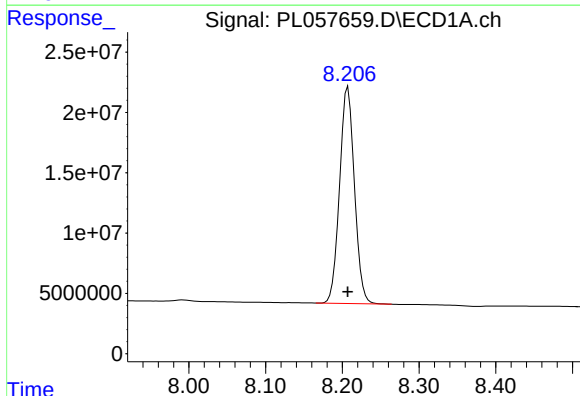

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 241766804
Conc: 22.85 ng/ml

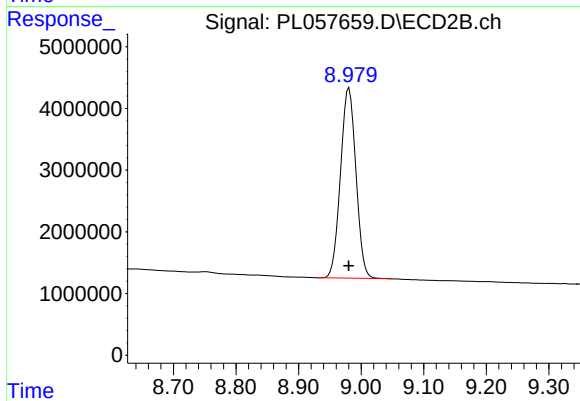

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: 0.000 min
Response: 53096728
Conc: 23.95 ng/ml