

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032720\
 Data File : PL057674.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 20:23
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 00:59:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.958	239.8E6	50936077	25.870	23.478
28)	SA Decachlor...	8.207	8.981	223.9E6	50552205	21.163	22.798
Target Compounds							
2)	A alpha-BHC	3.899	0.000	5147629	0	0.323	N.D. #
4)	MA Heptachlor	0.000	5.142	0	1228674	N.D.	0.390 #
14)	MA Endrin	6.015	0.000	701902	0	0.061	N.D. #
18)	B Endrin al...	6.448	0.000	132816	0	0.014	N.D. #
21)	B Endrin ke...	7.166	0.000	169739	0	0.015	N.D. #
22)	Mirex	7.339	0.000	224177	0	0.028	N.D. #
23)	Chlordane-1	4.356f	0.000	2577137	0	7.940	N.D. #
24)	Chlordane-2	4.845f	0.000	822302	0	2.263	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032720\
Data File : PL057674.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 20:23
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 00:59:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

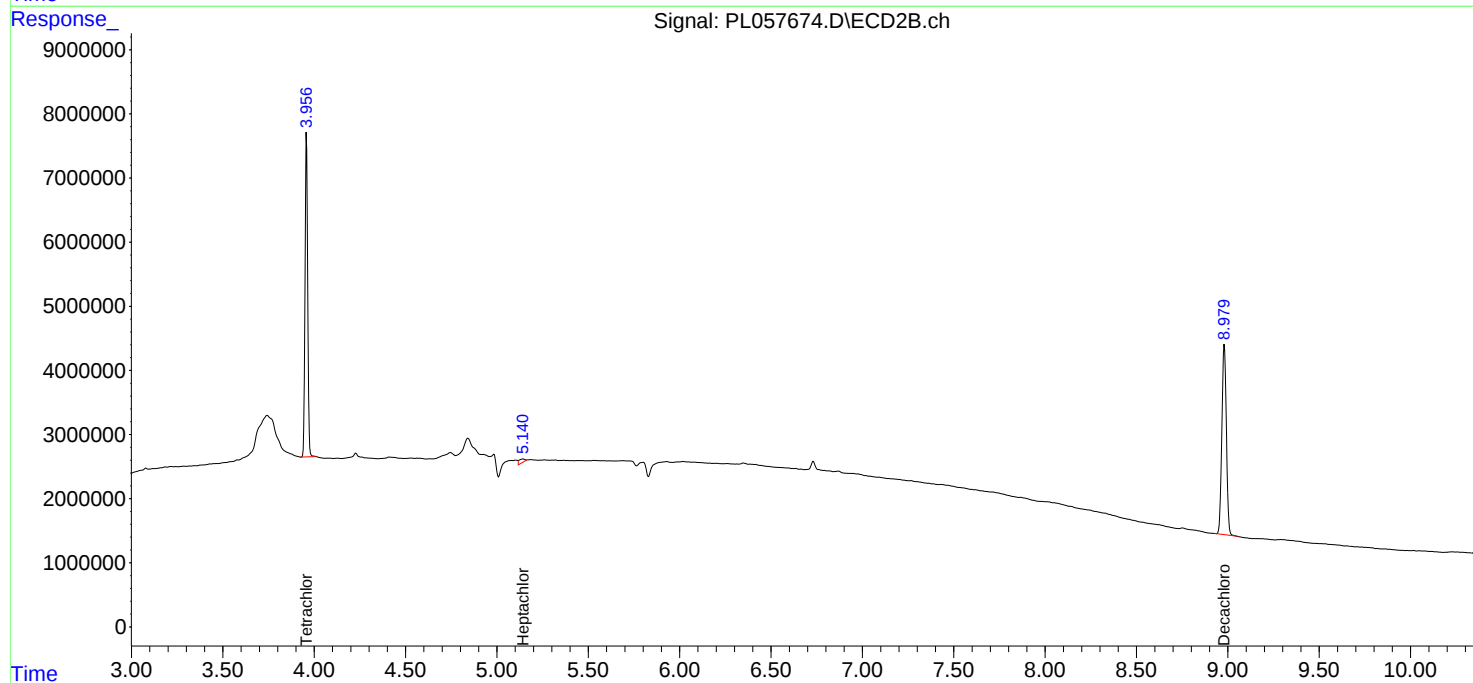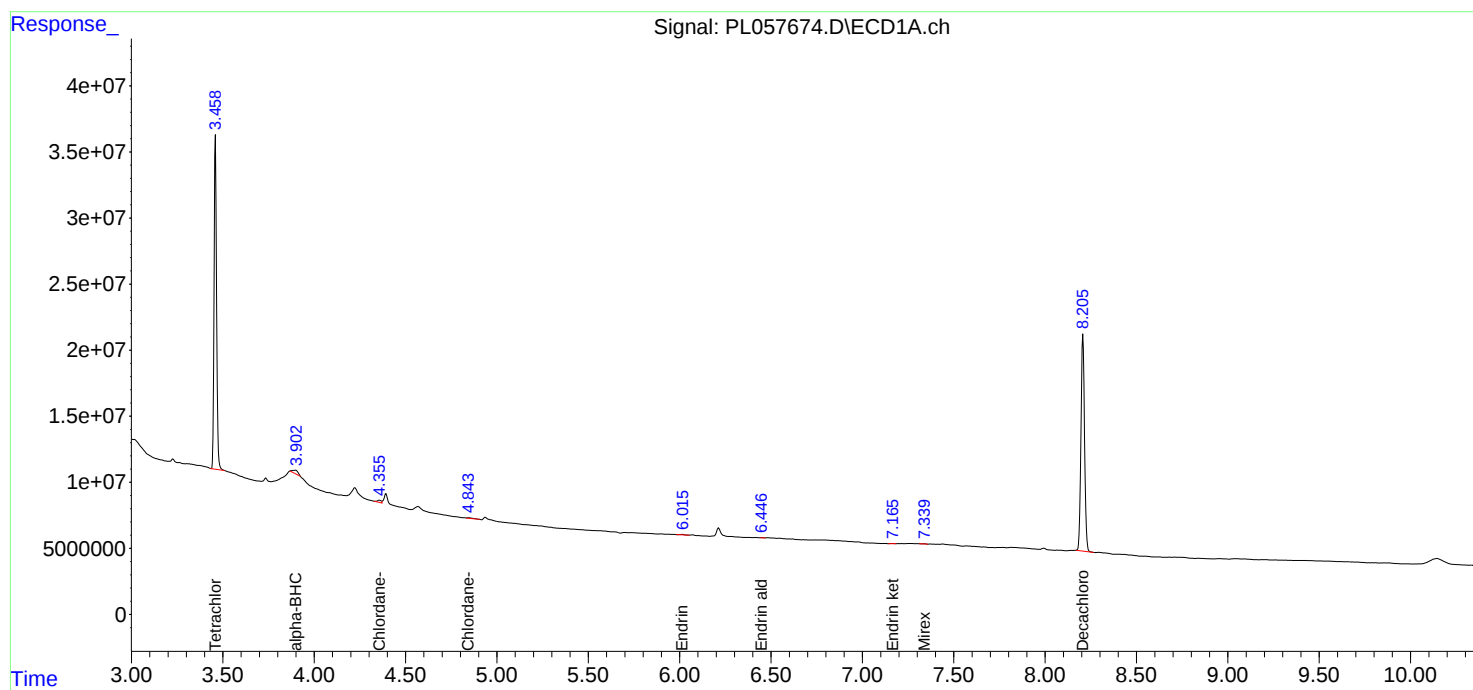


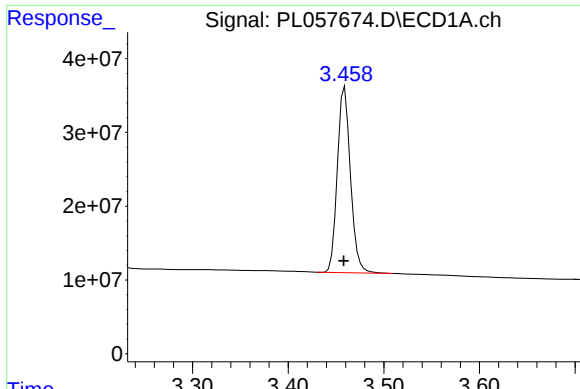

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.001 min
Response: 239795743
Conc: 25.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

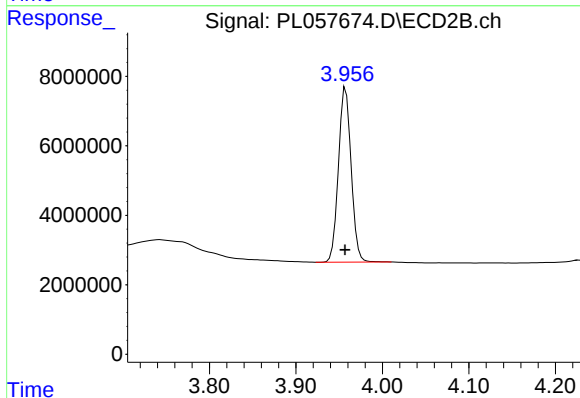


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 50936077
Conc: 23.48 ng/ml

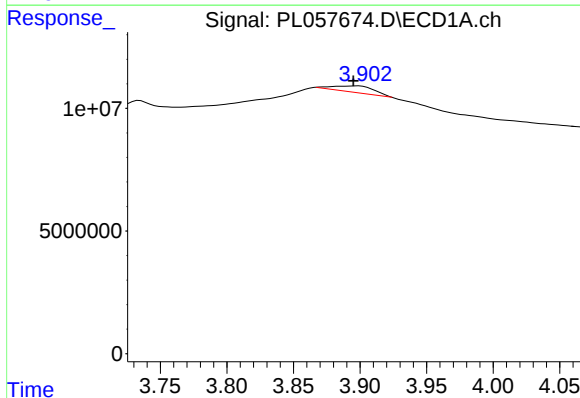


#2 alpha-BHC

R.T.: 3.899 min
Delta R.T.: 0.004 min
Response: 5147629
Conc: 0.32 ng/ml

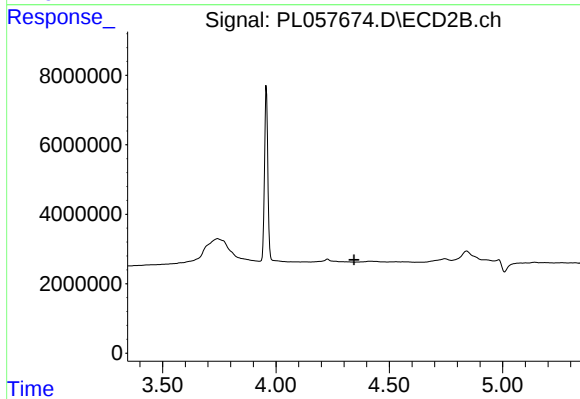

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.345 min
Response: 0
Conc: N.D.

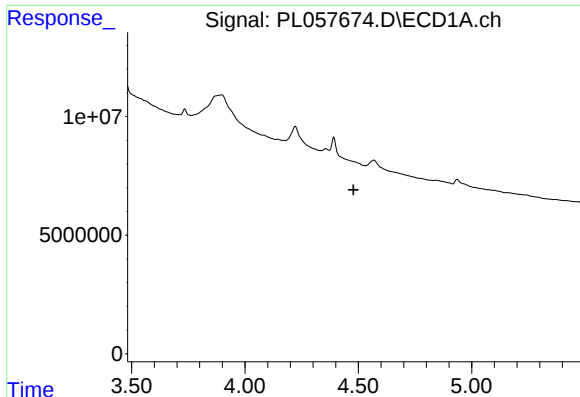

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

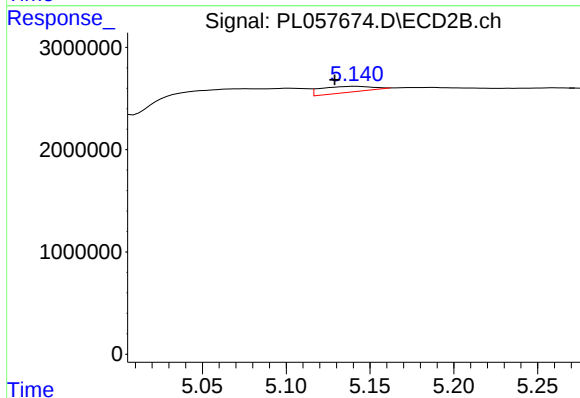


#4 Heptachlor

R.T.: 5.142 min
Delta R.T.: 0.013 min
Response: 1228674
Conc: 0.39 ng/ml

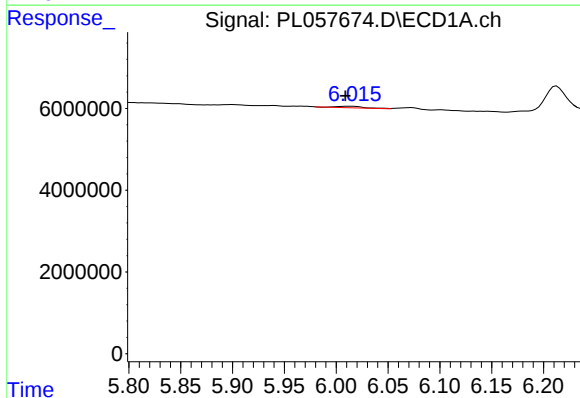


#14 Endrin

R.T.: 6.015 min
Delta R.T.: 0.006 min
Response: 701902
Conc: 0.06 ng/ml

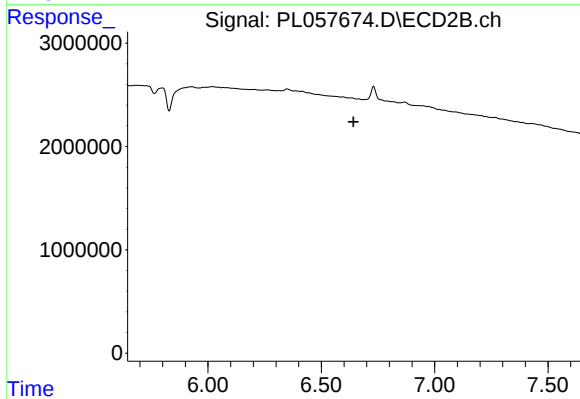

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.642 min
Response: 0
Conc: N.D.

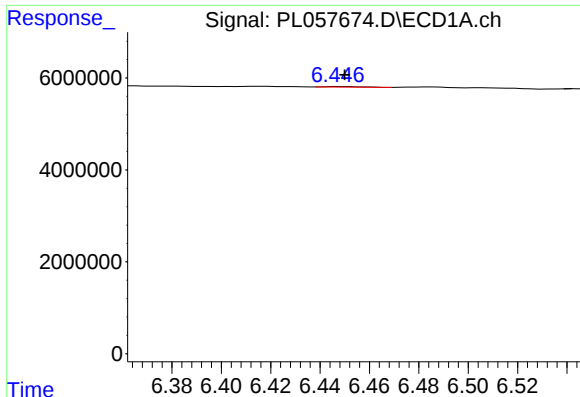

#18 Endrin aldehyde


R.T.: 6.448 min
Delta R.T.: -0.002 min
Response: 132816
Conc: 0.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

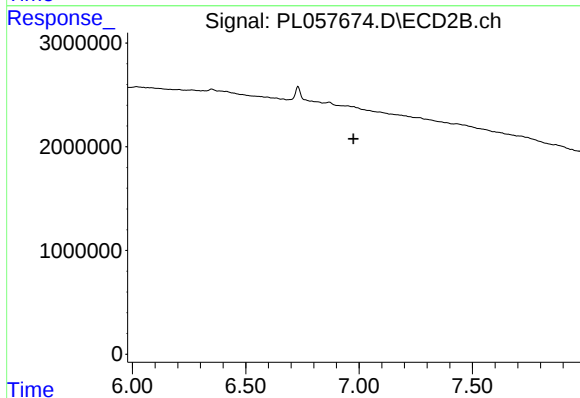


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.976 min
Response: 0
Conc: N.D.

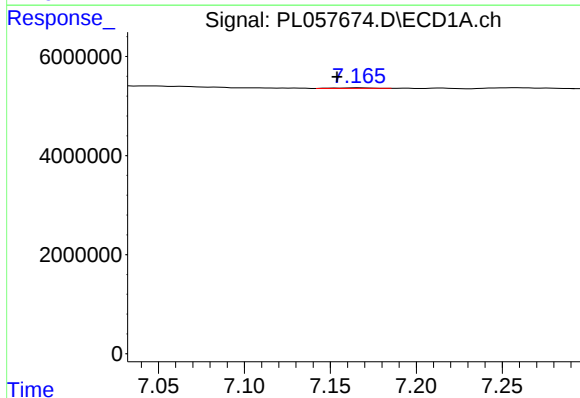


#21 Endrin ketone

R.T.: 7.166 min
Delta R.T.: 0.012 min
Response: 169739
Conc: 0.02 ng/ml

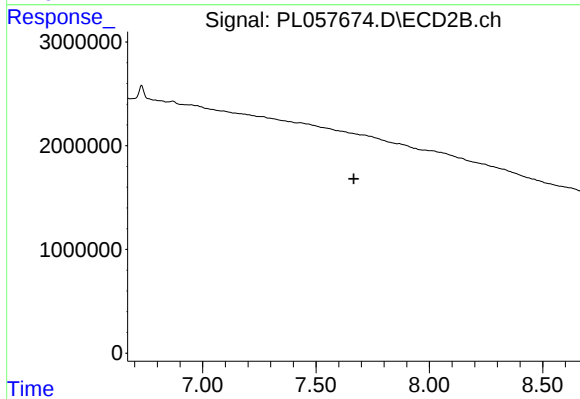

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.666 min
Response: 0
Conc: N.D.

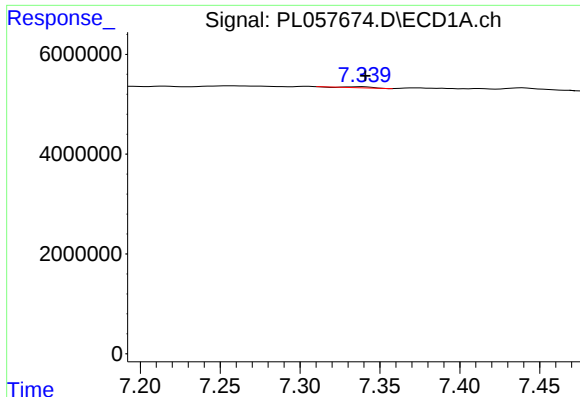

#22 Mirex


R.T.: 7.339 min
Delta R.T.: -0.002 min
Response: 224177
Conc: 0.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

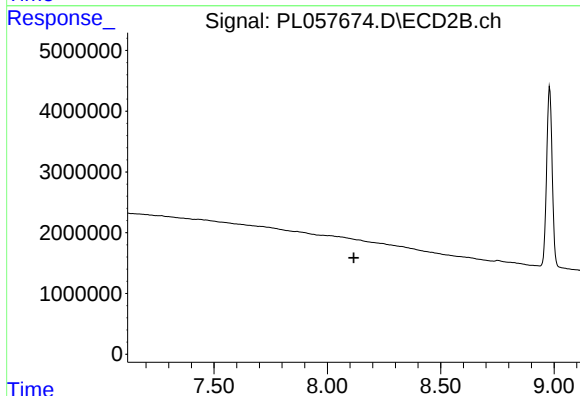


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

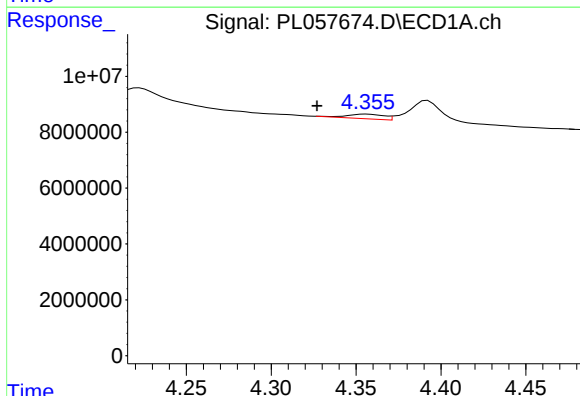


#23 Chlordane-1

R.T.: 4.356 min
Delta R.T.: 0.029 min
Response: 2577137
Conc: 7.94 ng/ml

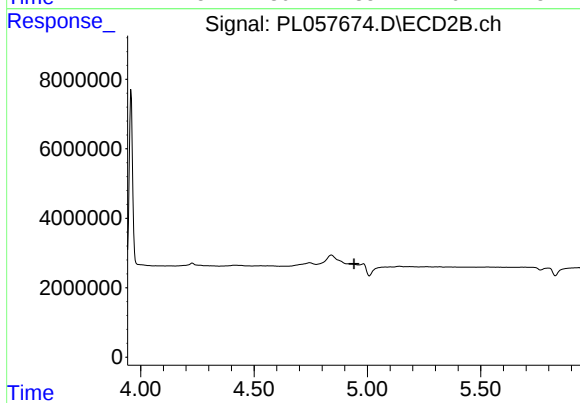

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

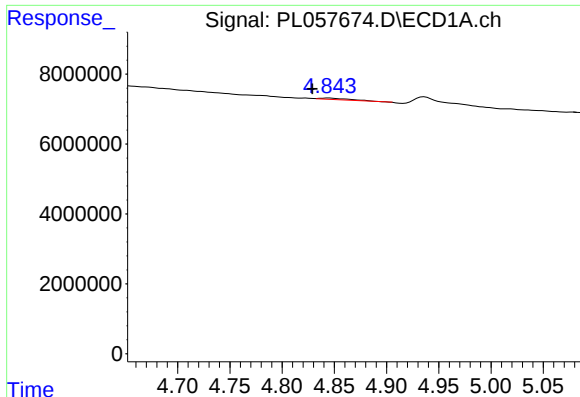

#24 Chlordane-2


R.T.: 4.845 min
Delta R.T.: 0.016 min
Response: 822302
Conc: 2.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

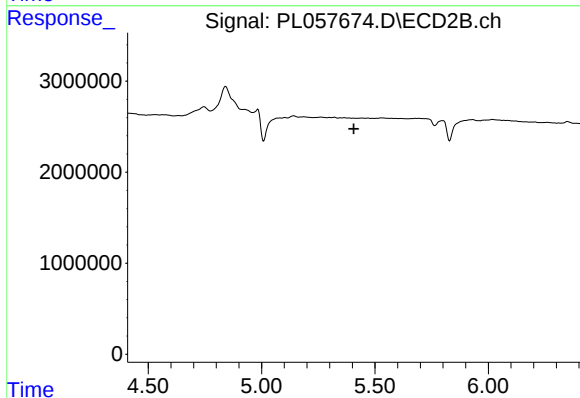


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.406 min
Response: 0
Conc: N.D.

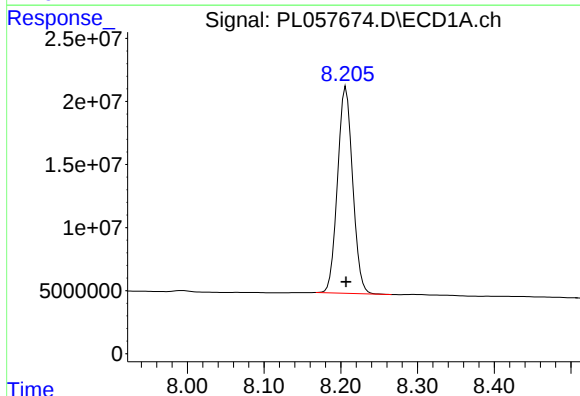

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 223931396
Conc: 21.16 ng/ml

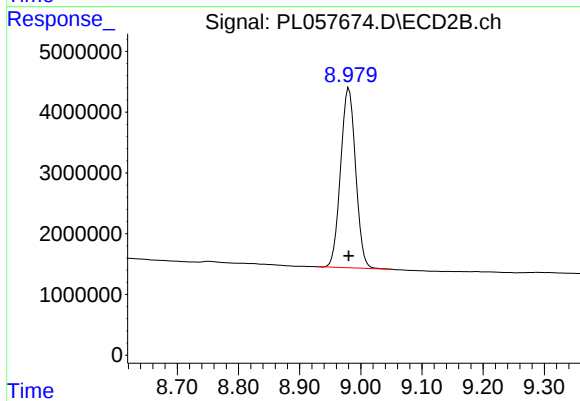

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: 0.000 min
Response: 50552205
Conc: 22.80 ng/ml