

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032819\
 Data File : PL046604.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2019 06:28
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 08:49:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

7) B	delta-BHC	4.512	0.000	4911081	0	0.485	N.D.	#
8) B	Heptachlo...	0.000	5.842	0	20248651	N.D.	7.678	#
9) A	Endosulfan I	0.000	6.200	0	2735751	N.D.	1.048	#
10) B	gamma-Chl...	0.000	6.079	0	29657320	N.D.	10.450	#
11) B	alpha-Chl...	0.000	6.152	0	7642610	N.D.	2.694	#
14) MA	Endrin	5.865	0.000	10843280	0	1.151	N.D.	#
25)	Chlordane-3	0.000	6.079	0	29657320	N.D.	77.786	#
26)	Chlordane-4	0.000	6.152	0	7642610	N.D.	16.563	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032819\
Data File : PL046604.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2019 06:28
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 08:49:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

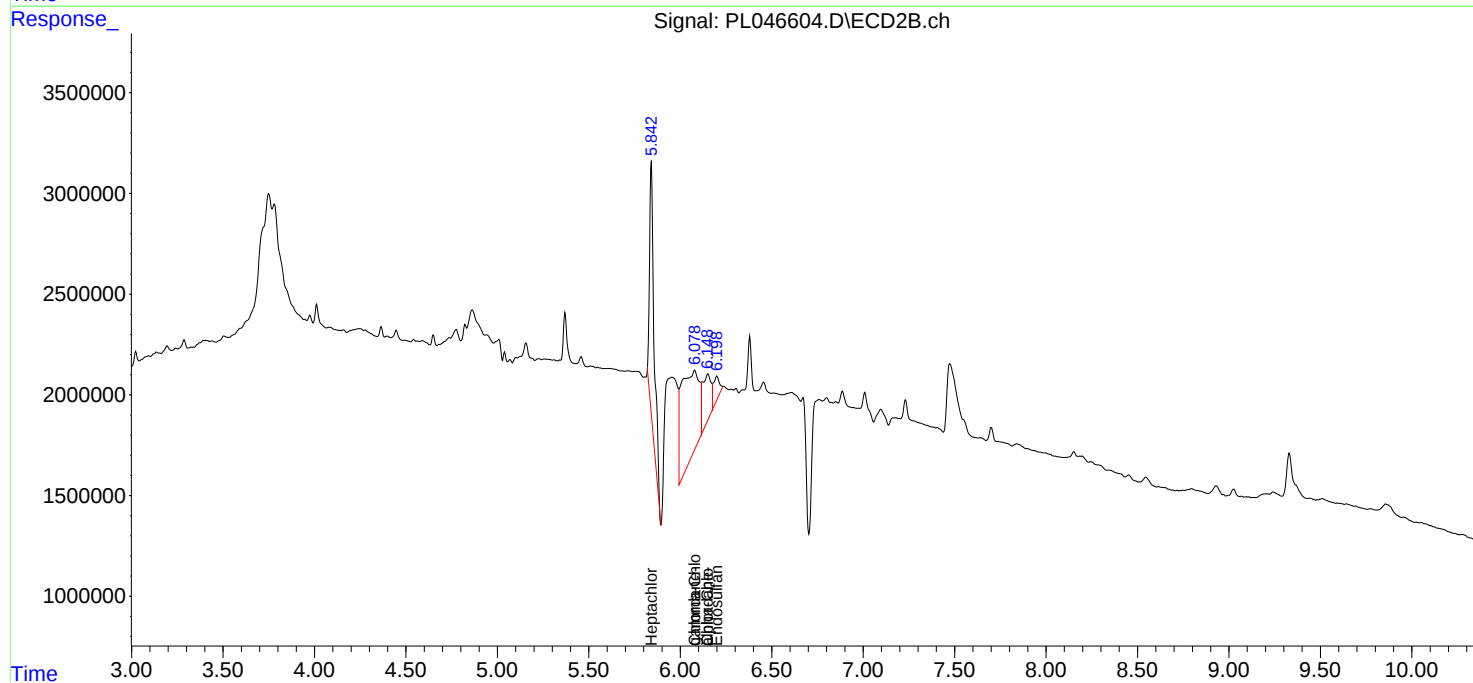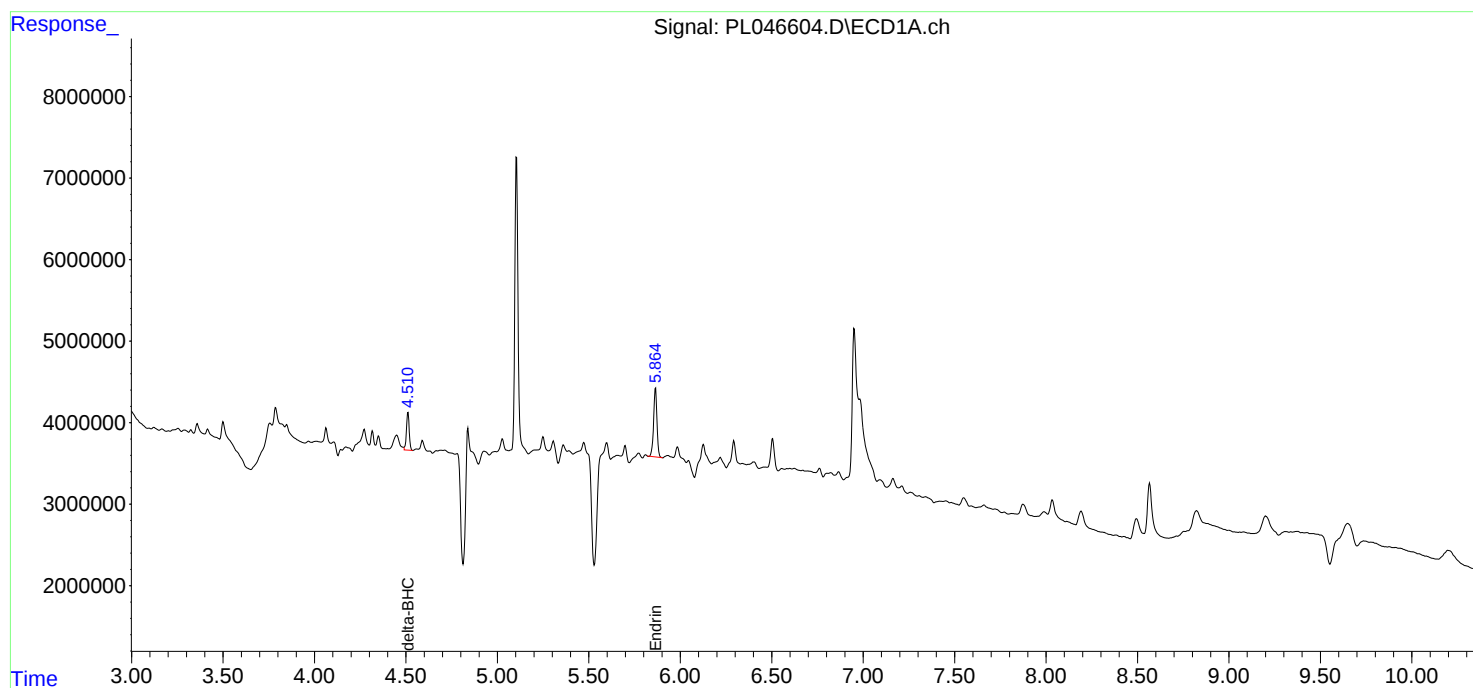


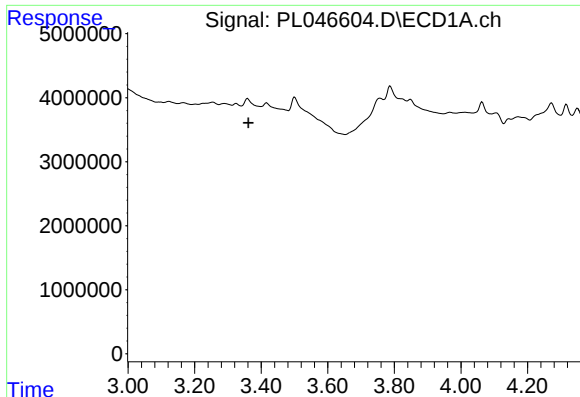

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.361 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

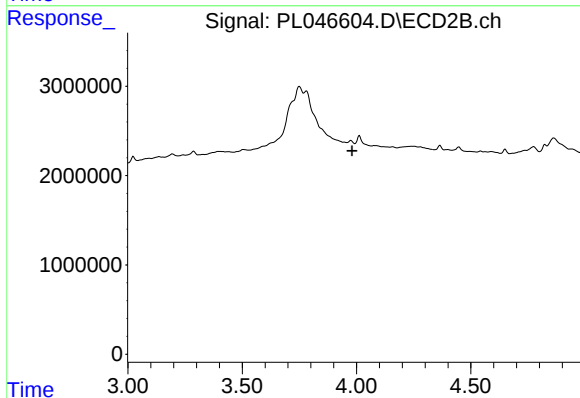


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.981 min
Response: 0
Conc: N.D.

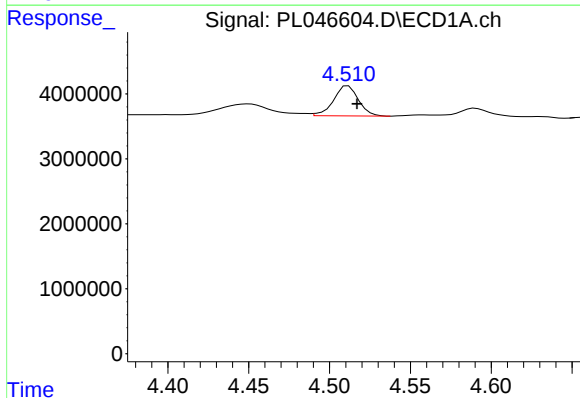


#7 delta-BHC

R.T.: 4.512 min
Delta R.T.: -0.005 min
Response: 4911081
Conc: 0.49 ng/ml

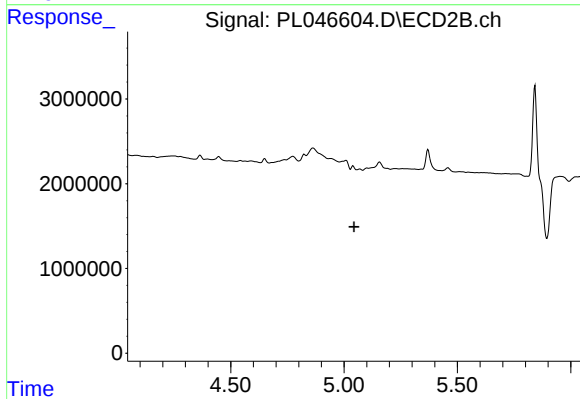

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 5.044 min
Response: 0
Conc: N.D.

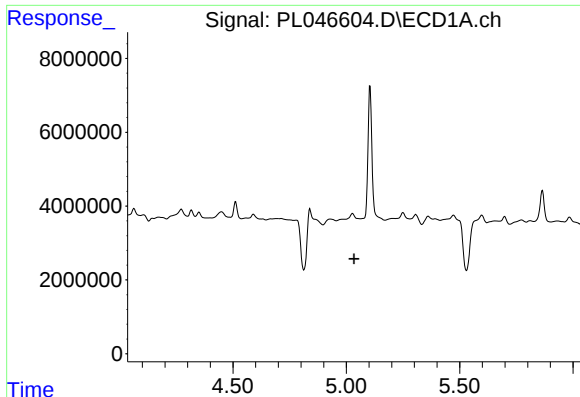

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.034 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

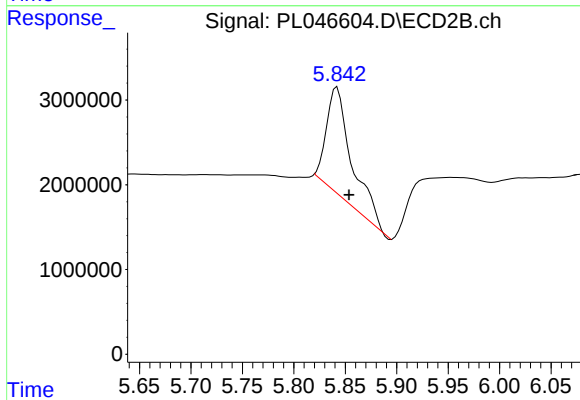


#8 Heptachlor epoxide

R.T.: 5.842 min
Delta R.T.: -0.011 min
Response: 20248651
Conc: 7.68 ng/ml

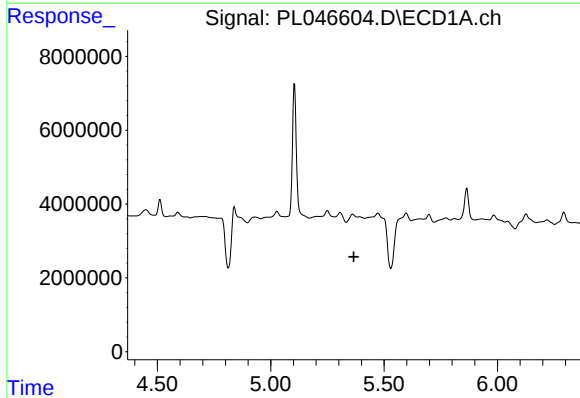


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.366 min
Response: 0
Conc: N.D.

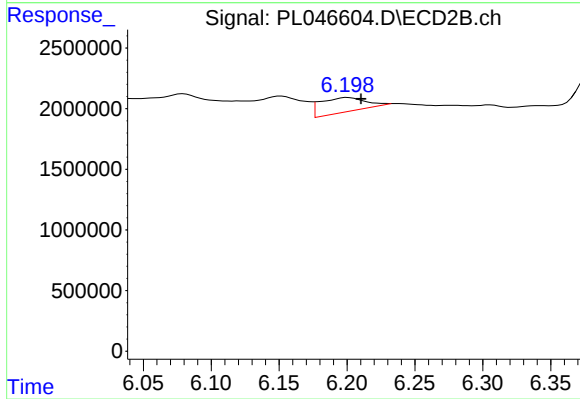

#9 Endosulfan I


R.T.: 6.200 min
Delta R.T.: -0.010 min
Response: 2735751
Conc: 1.05 ng/ml

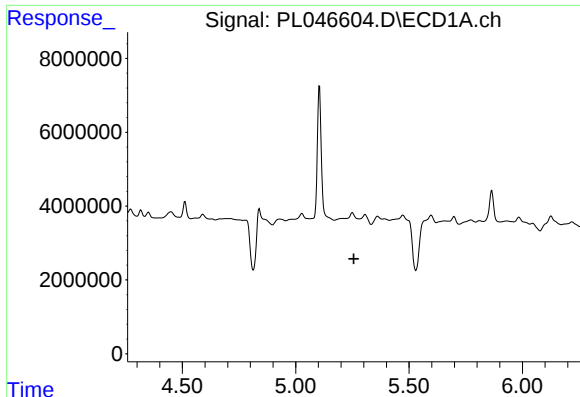

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.257 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

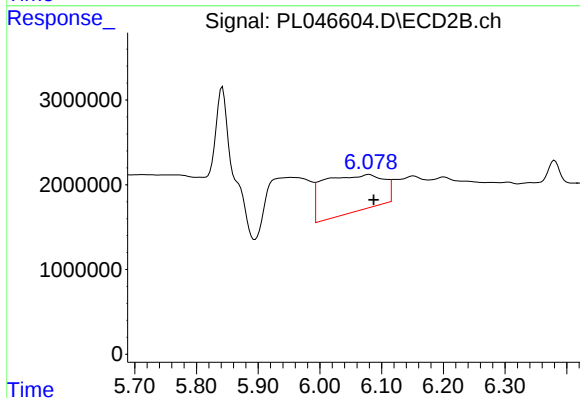


#10 gamma-Chlordane

R.T.: 6.079 min
Delta R.T.: -0.008 min
Response: 29657320
Conc: 10.45 ng/ml

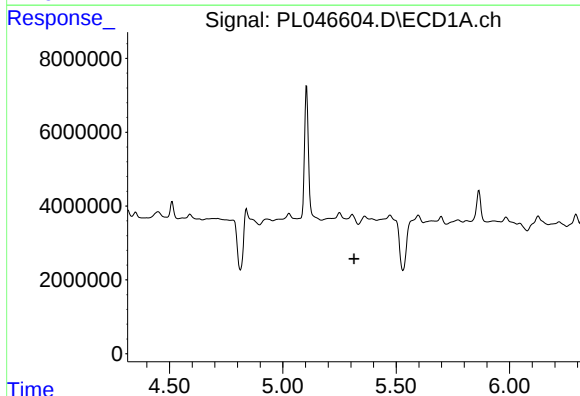


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.314 min
Response: 0
Conc: N.D.

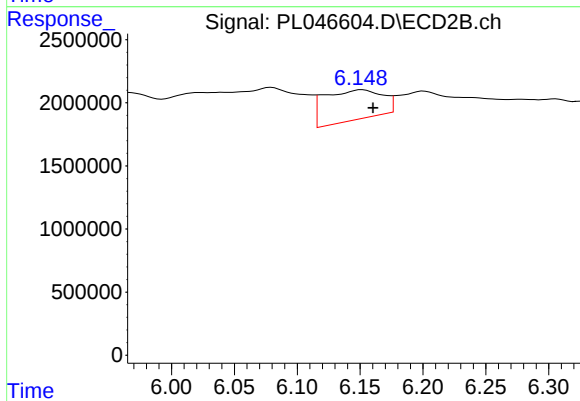

#11 alpha-Chlordane


R.T.: 6.152 min
Delta R.T.: -0.009 min
Response: 7642610
Conc: 2.69 ng/ml

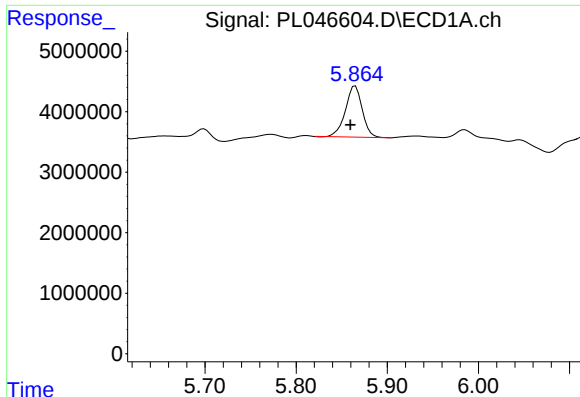

#14 Endrin


R.T.: 5.865 min
Delta R.T.: 0.005 min
Response: 10843280
Conc: 1.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

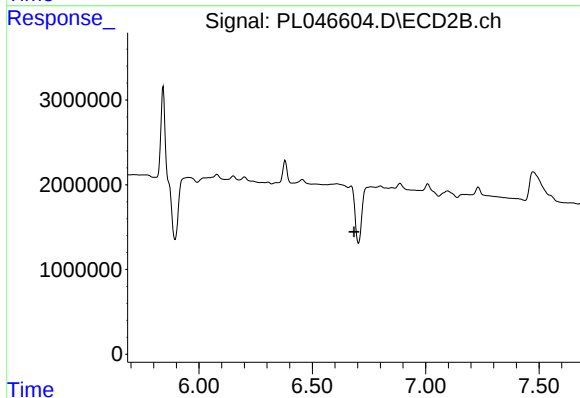


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.684 min
Response: 0
Conc: N.D.

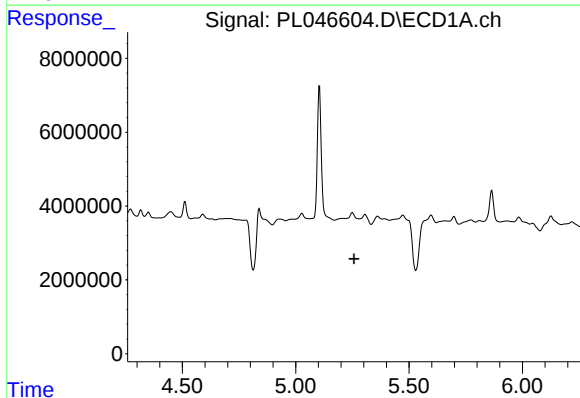


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

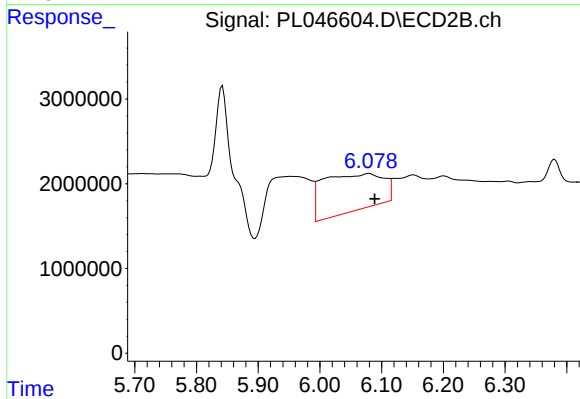

#25 Chlordane-3


R.T.: 6.079 min
Delta R.T.: -0.010 min
Response: 29657320
Conc: 77.79 ng/ml

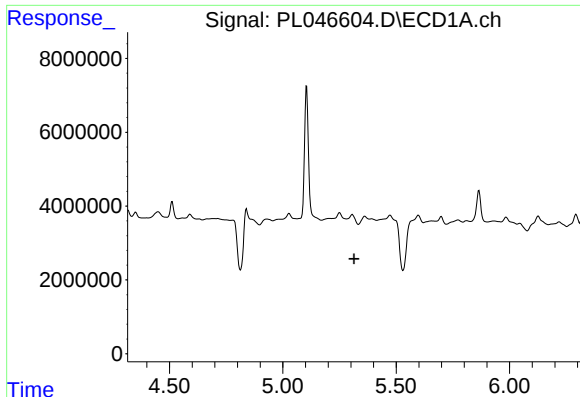

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

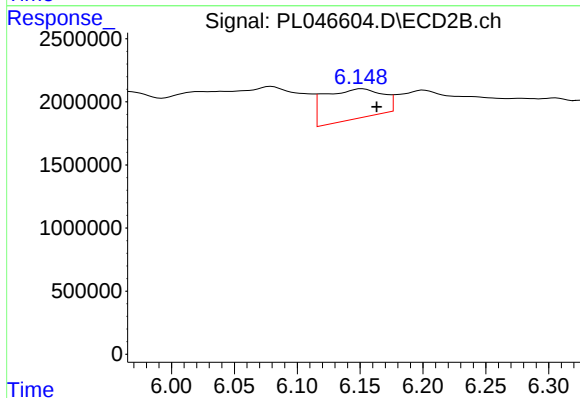


#26 Chlordane-4

R.T.: 6.152 min
Delta R.T.: -0.012 min
Response: 7642610
Conc: 16.56 ng/ml

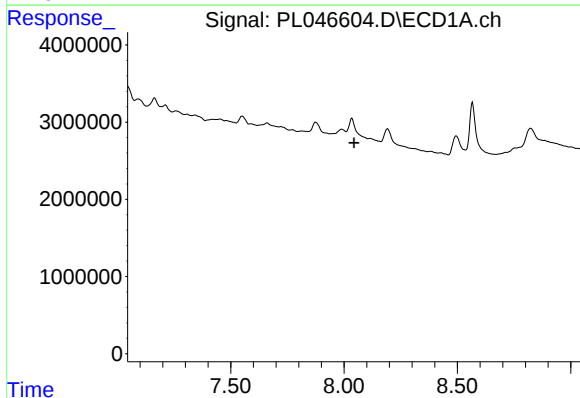

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.044 min
Response: 0
Conc: N.D.

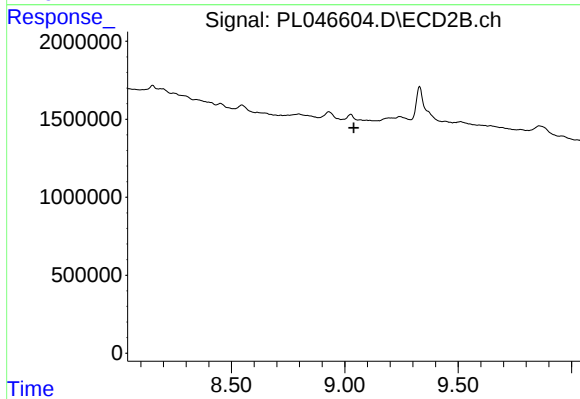

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.040 min
Response: 0
Conc: N.D.