

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032819\
 Data File : PL046640.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2019 16:47
 Operator : AJ\SJ
 Sample : K2086-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CS-14

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:13:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.977	85881634	28795366	11.806	12.577
28)	SA Decachlor...	8.036	9.031	136.8E6	38980439	16.262	16.813
Target Compounds							
9)	A Endosulfan I	5.392f	0.000	5778824	0	0.615	N.D. #
10)	B gamma-Chl...	0.000	6.072f	0	2404544	N.D.	0.847 #
25)	Chlordane-3	0.000	6.072f	0	2404544	N.D.	6.307 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032819\
Data File : PL046640.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2019 16:47
Operator : AJ\SJ
Sample : K2086-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CS-14

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:13:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

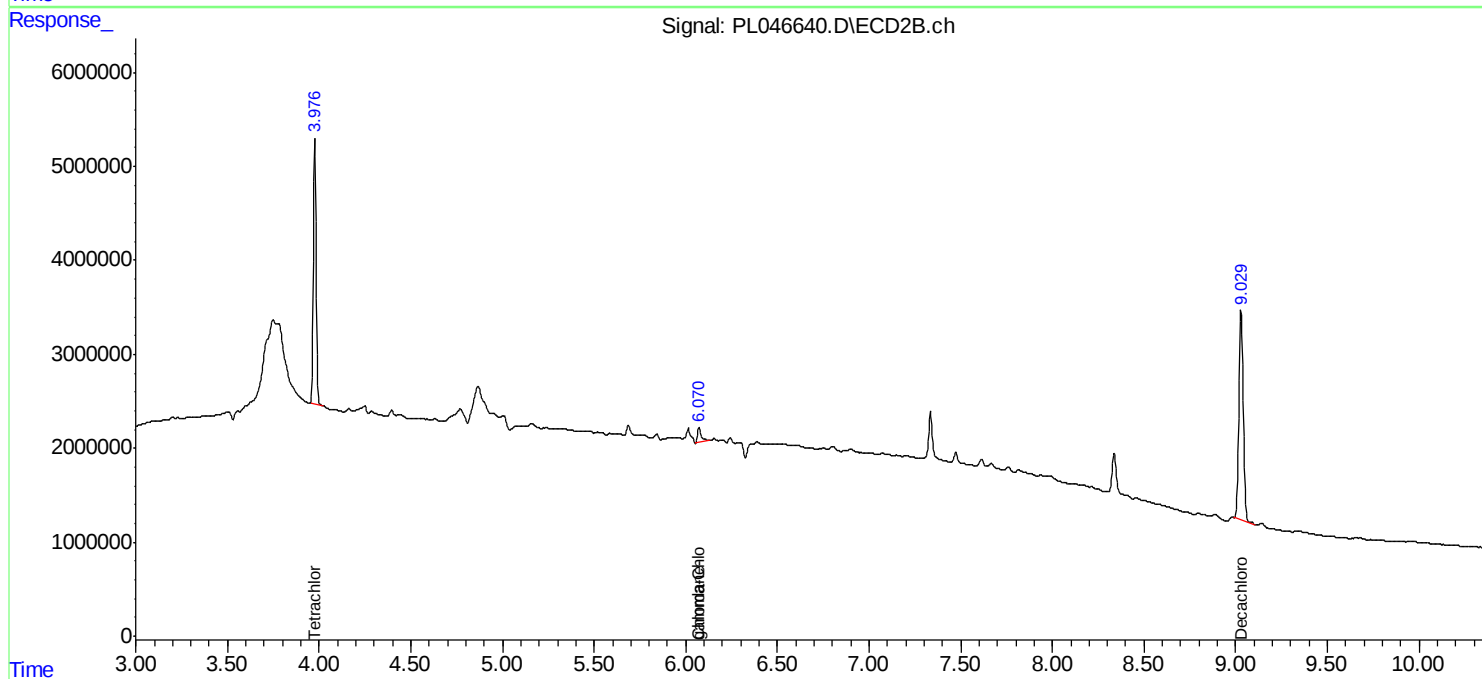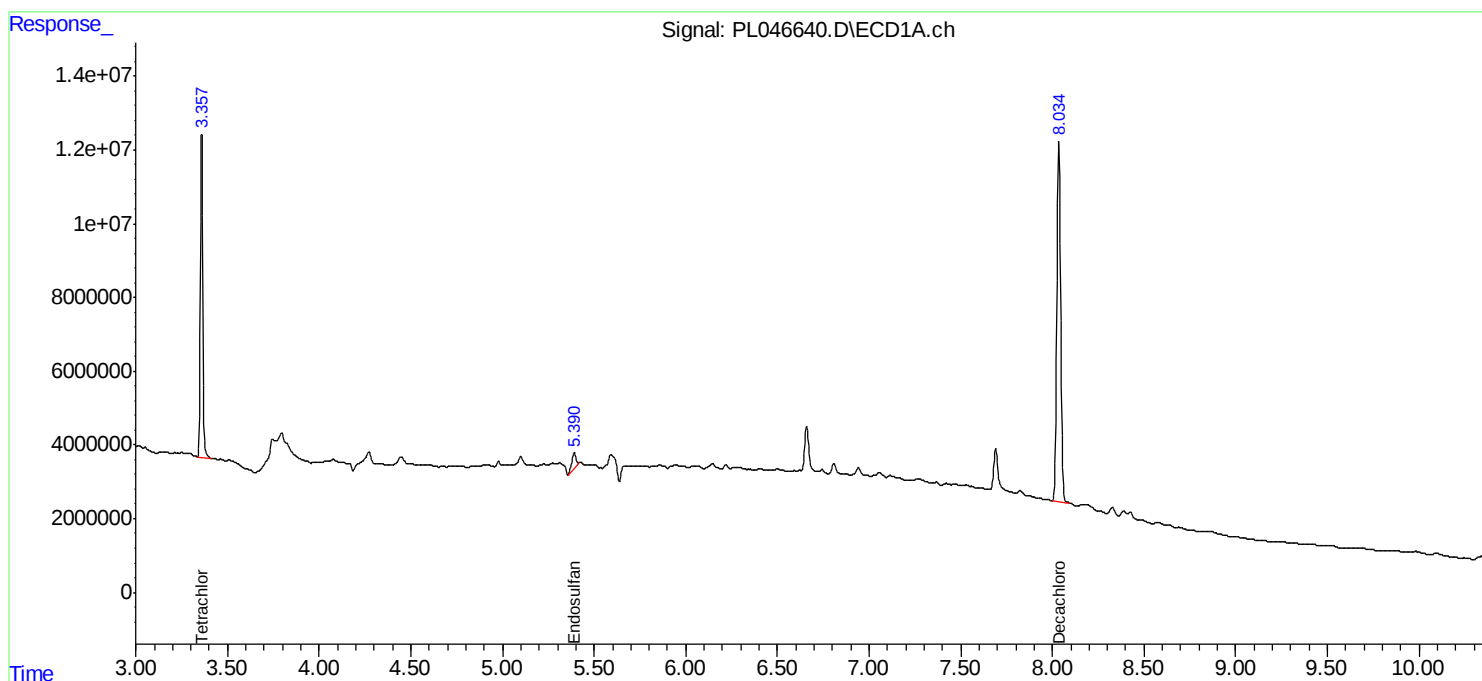


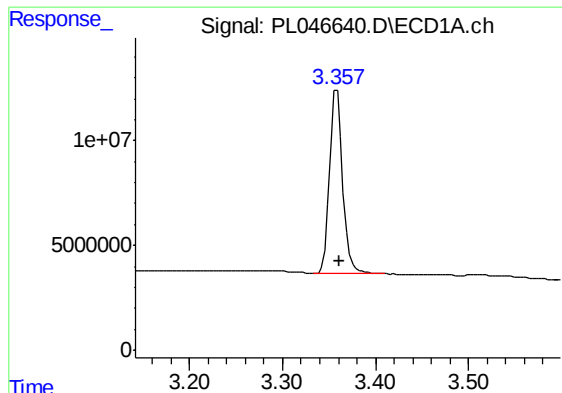

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 85881634
Conc: 11.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
CS-14

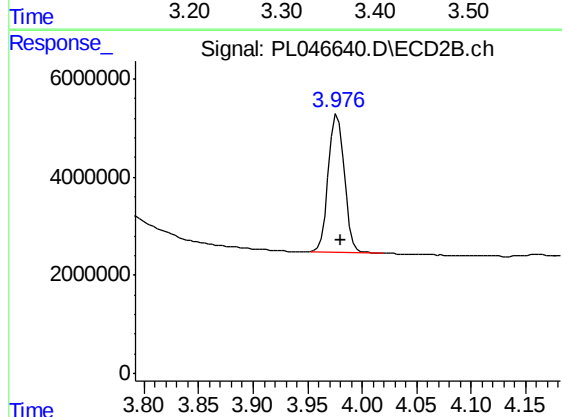


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.003 min
Response: 28795366
Conc: 12.58 ng/ml

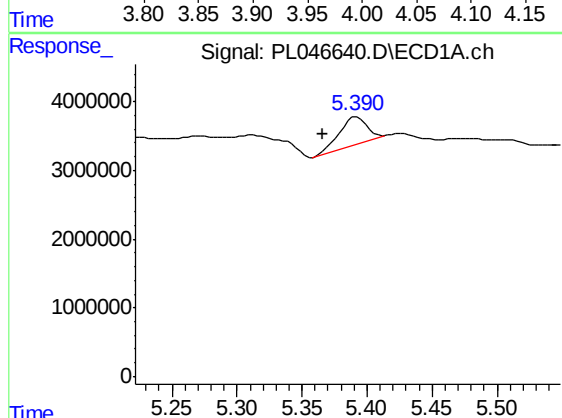


#9 Endosulfan I

R.T.: 5.392 min
Delta R.T.: 0.025 min
Response: 5778824
Conc: 0.61 ng/ml

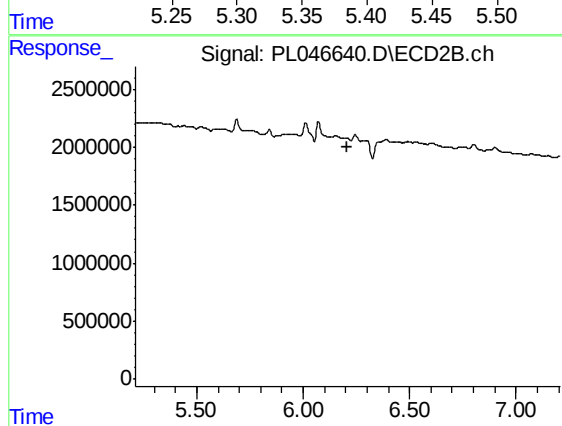

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.210 min
Response: 0
Conc: N.D.

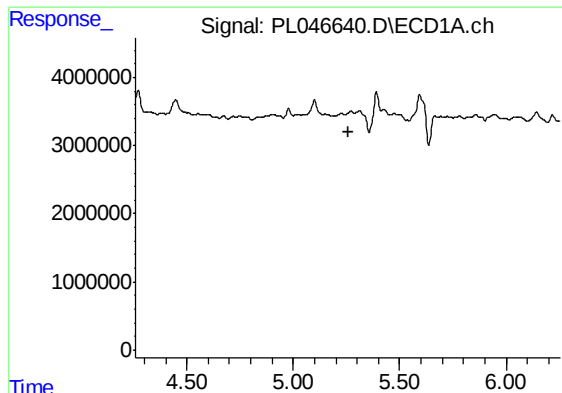

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.257 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CS-14

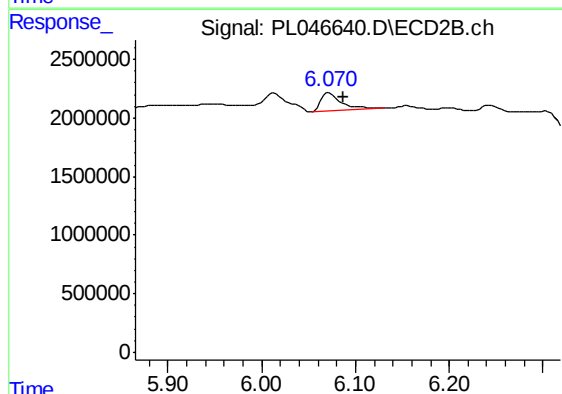


#10 gamma-Chlordane

R.T.: 6.072 min
Delta R.T.: -0.016 min
Response: 2404544
Conc: 0.85 ng/ml

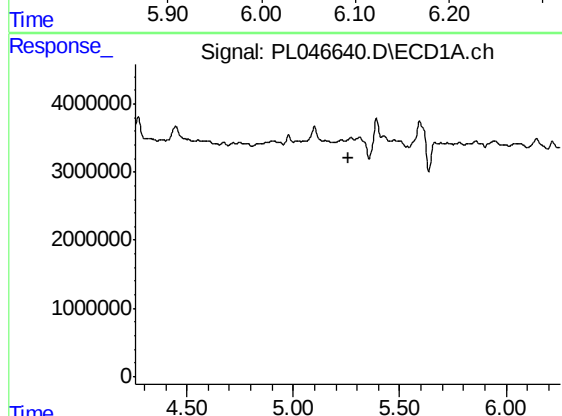


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

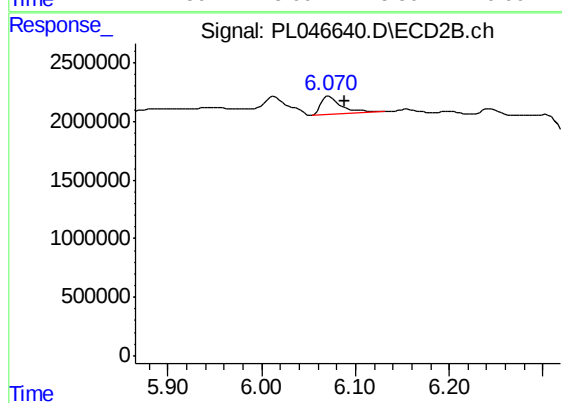

#25 Chlordane-3


R.T.: 6.072 min
Delta R.T.: -0.017 min
Response: 2404544
Conc: 6.31 ng/ml

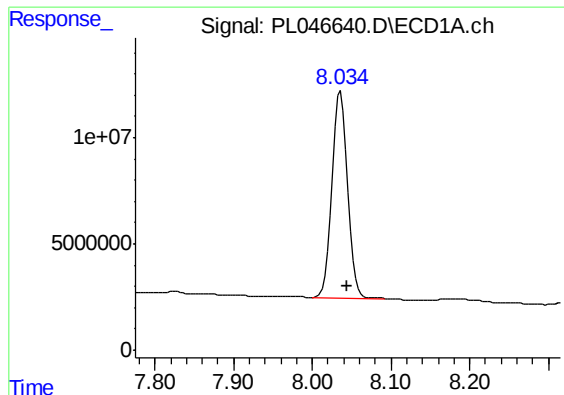

#28 Decachlorobiphenyl

R.T.: 8.036 min
Delta R.T.: -0.008 min
Response: 136778125
Conc: 16.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
CS-14

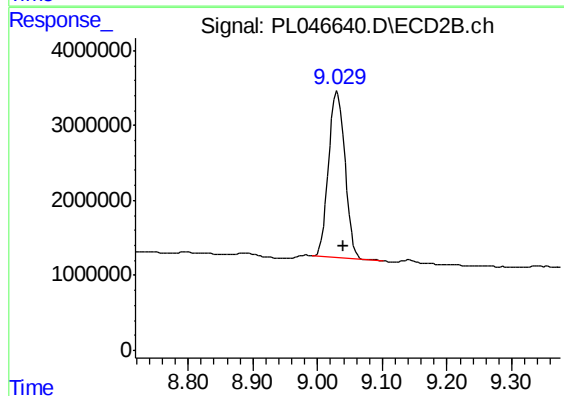

#28 Decachlorobiphenyl

R.T.: 9.031 min
Delta R.T.: -0.009 min
Response: 38980439
Conc: 16.81 ng/ml