

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032819\
 Data File : PL046644.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2019 17:45
 Operator : AJ\SJ
 Sample : K2090-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 P-5(0-10)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:14:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.977	61245764	20508207	8.419	8.957
28)	SA Decachlor...	8.035	9.029	71915925	21380982	8.550	9.222
Target Compounds							
2)	A alpha-BHC	3.795	0.000	11319662	0	0.971	N.D. #
10)	B gamma-Chl...	5.272	6.083	9484954	2184609	0.923	0.770
11)	B alpha-Chl...	0.000	6.156	0	6431226	N.D.	2.267 #
12)	B 4,4'-DDE	5.475	6.311	24331367	7784222	2.643	3.136
16)	A 4,4'-DDD	0.000	6.806	0	2105829	N.D.	1.047 #
17)	MA 4,4'-DDT	6.220	7.099	22093916	4171459	2.917	1.989 #
25)	Chlordane-3	5.272	6.083	9484954	2184609	8.517	5.730 #
26)	Chlordane-4	0.000	6.156	0	6431226	N.D.	13.938 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032819\
Data File : PL046644.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2019 17:45
Operator : AJ\SJ
Sample : K2090-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
P-5(0-10)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:14:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

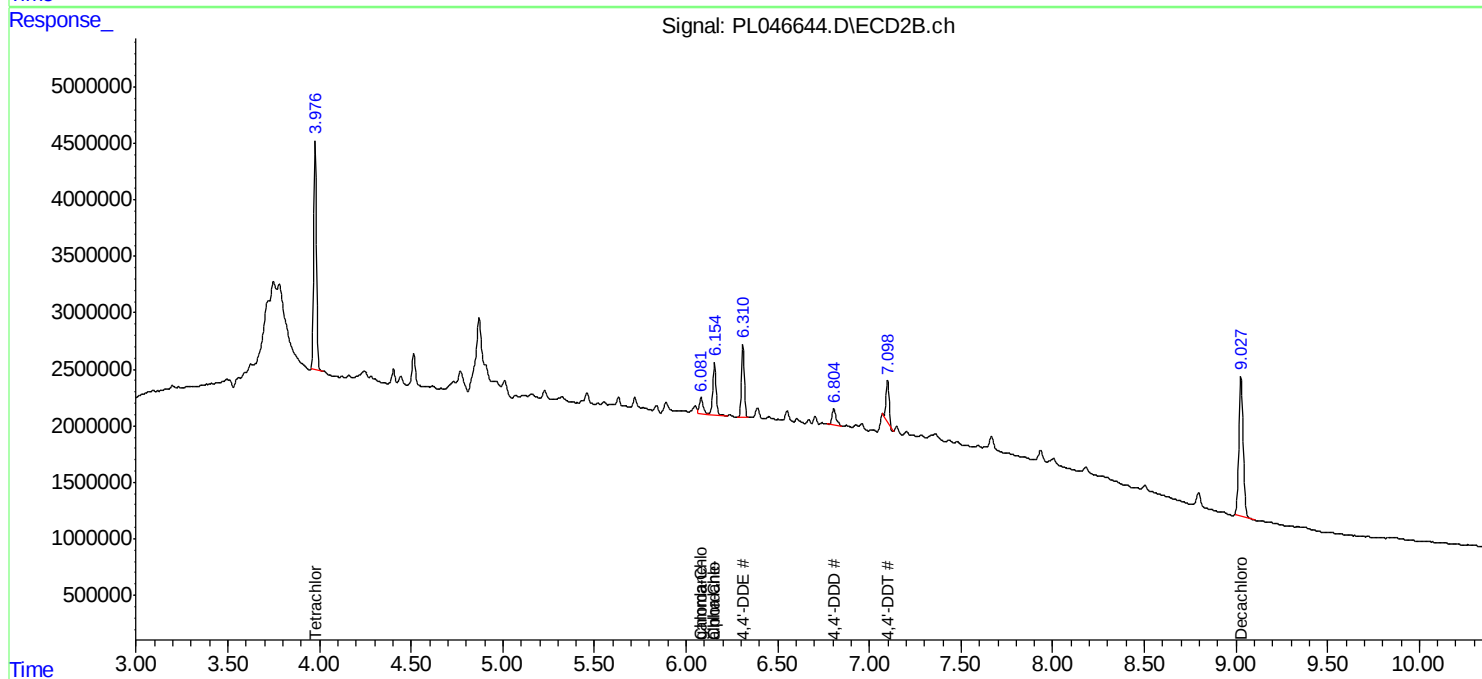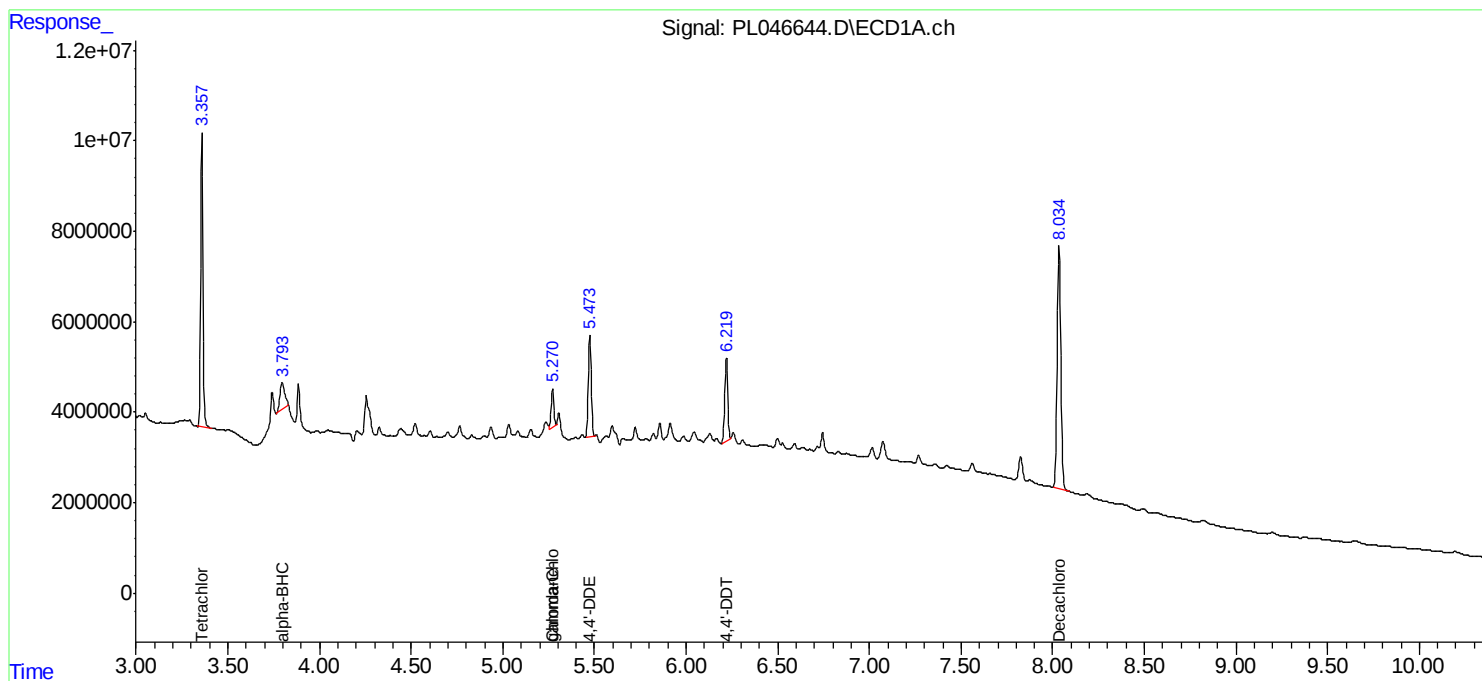


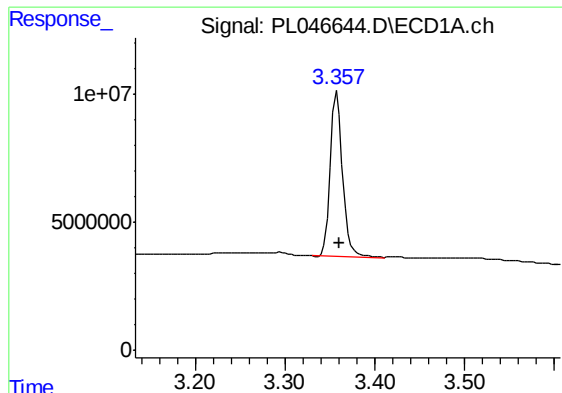

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 61245764
Conc: 8.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
P-5(0-10)

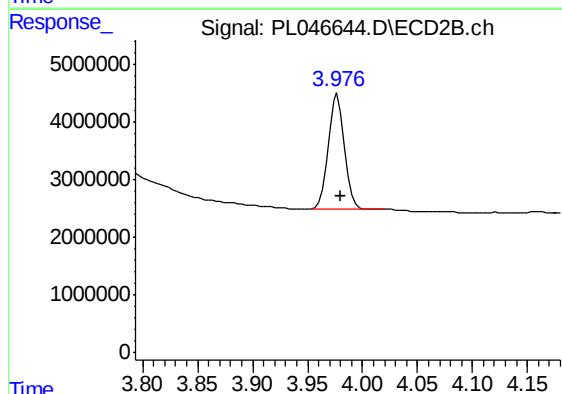


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.003 min
Response: 20508207
Conc: 8.96 ng/ml

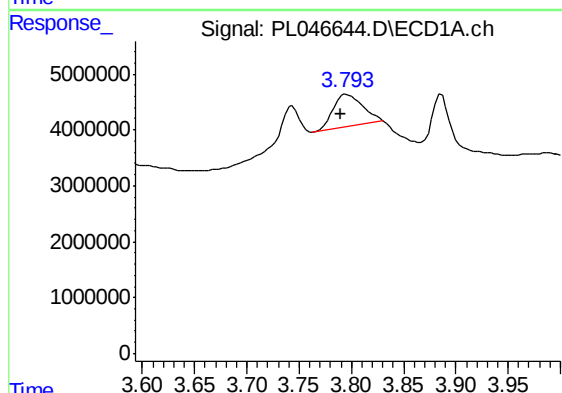


#2 alpha-BHC

R.T.: 3.795 min
Delta R.T.: 0.005 min
Response: 11319662
Conc: 0.97 ng/ml

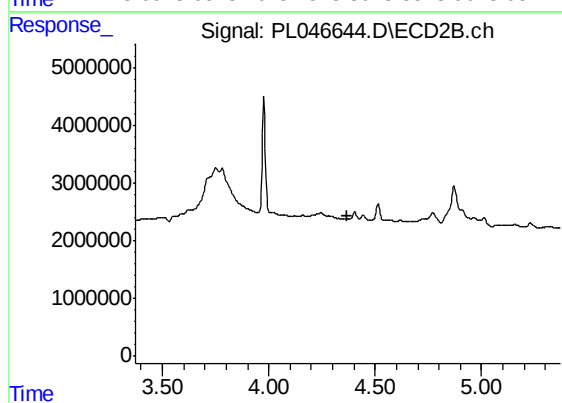

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.371 min
Response: 0
Conc: N.D.

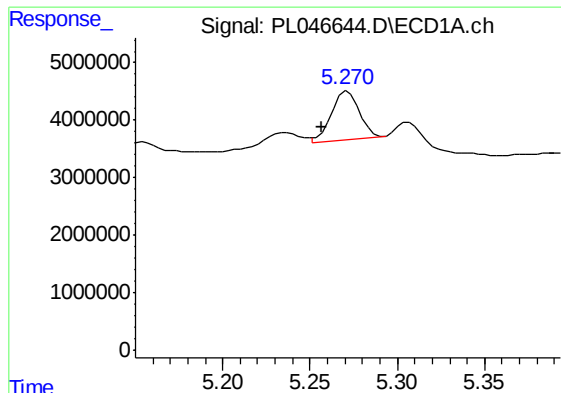

#10 gamma-Chlordane


R.T.: 5.272 min
Delta R.T.: 0.015 min
Response: 9484954
Conc: 0.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
P-5(0-10)

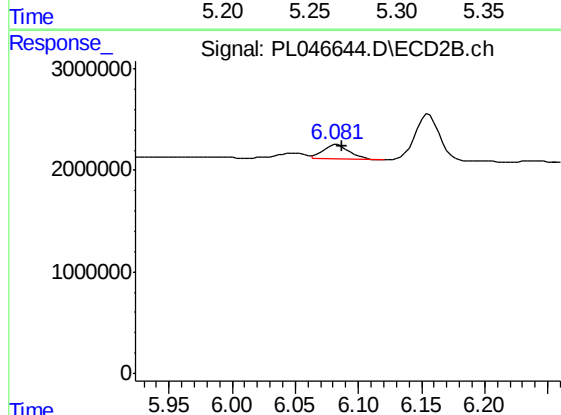


#10 gamma-Chlordane

R.T.: 6.083 min
Delta R.T.: -0.005 min
Response: 2184609
Conc: 0.77 ng/ml

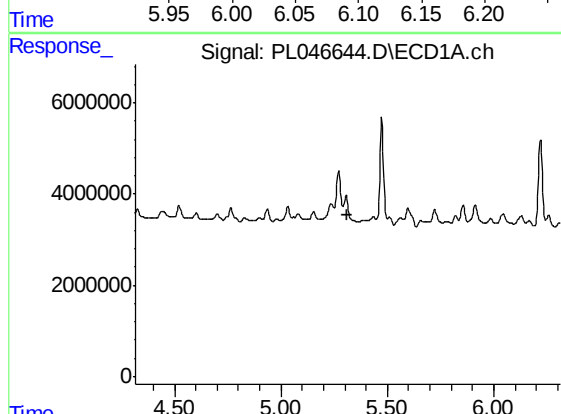


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.314 min
Response: 0
Conc: N.D.

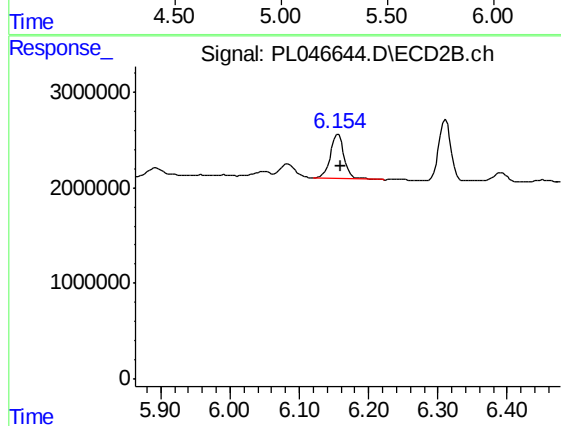

#11 alpha-Chlordane


R.T.: 6.156 min
Delta R.T.: -0.004 min
Response: 6431226
Conc: 2.27 ng/ml

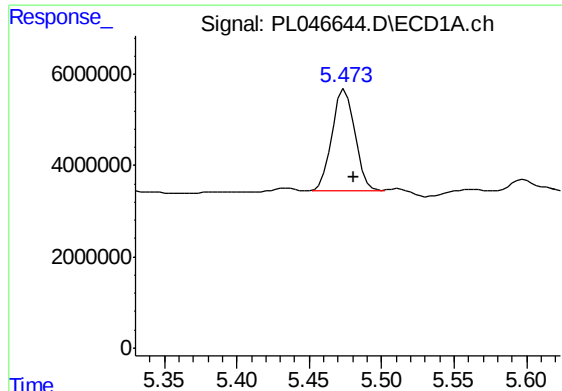

#12 4,4'-DDE


R.T.: 5.475 min
Delta R.T.: -0.006 min
Response: 24331367
Conc: 2.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
P-5(0-10)

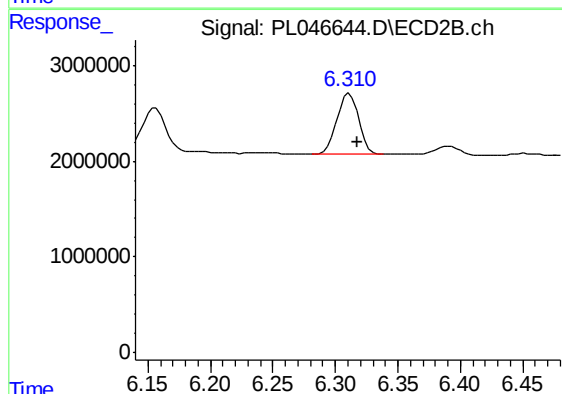


#12 4,4'-DDE

R.T.: 6.311 min
Delta R.T.: -0.007 min
Response: 7784222
Conc: 3.14 ng/ml

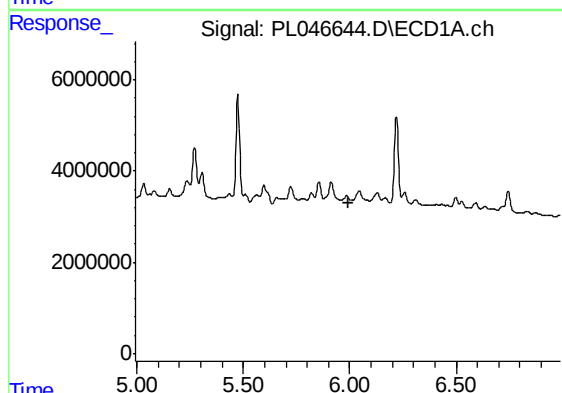


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.993 min
Response: 0
Conc: N.D.

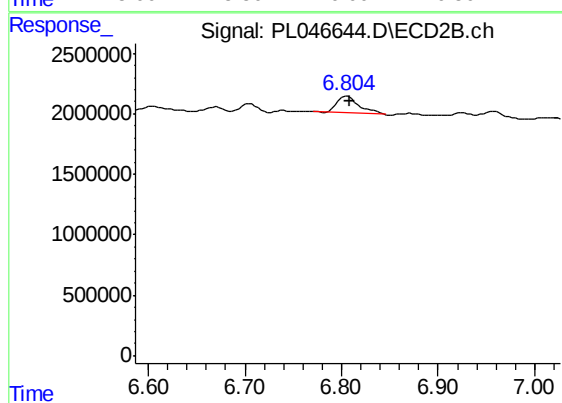

#16 4,4'-DDD


R.T.: 6.806 min
Delta R.T.: -0.003 min
Response: 2105829
Conc: 1.05 ng/ml

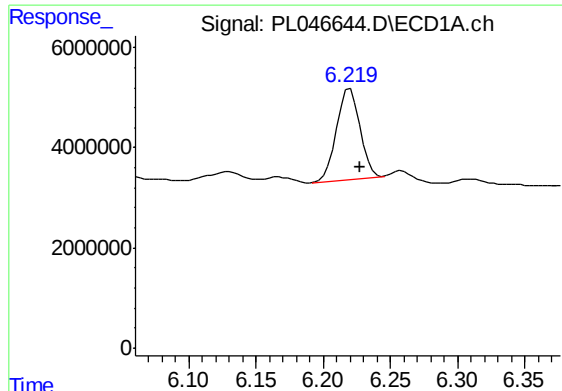

#17 4,4'-DDT


R.T.: 6.220 min
Delta R.T.: -0.008 min
Response: 22093916
Conc: 2.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
P-5(0-10)

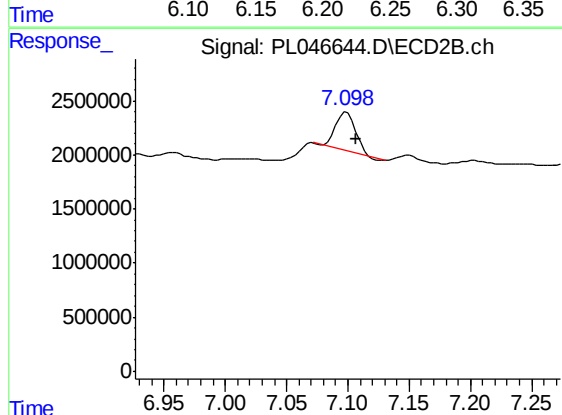


#17 4,4'-DDT

R.T.: 7.099 min
Delta R.T.: -0.008 min
Response: 4171459
Conc: 1.99 ng/ml

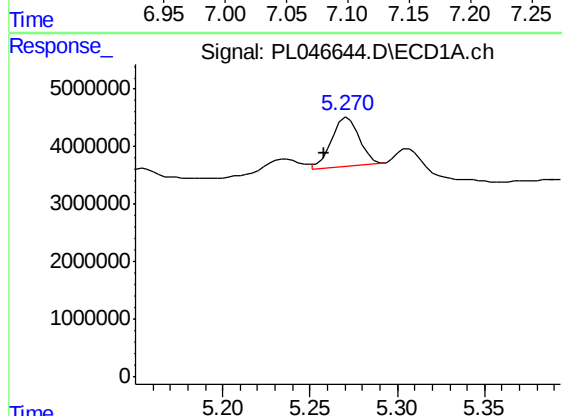


#25 Chlordane-3

R.T.: 5.272 min
Delta R.T.: 0.013 min
Response: 9484954
Conc: 8.52 ng/ml

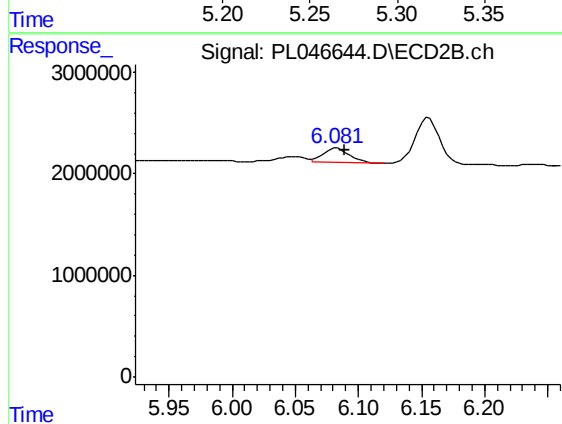

#25 Chlordane-3


R.T.: 6.083 min
Delta R.T.: -0.006 min
Response: 2184609
Conc: 5.73 ng/ml

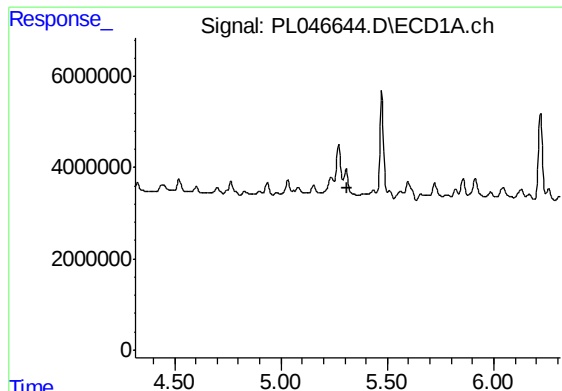

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
P-5(0-10)

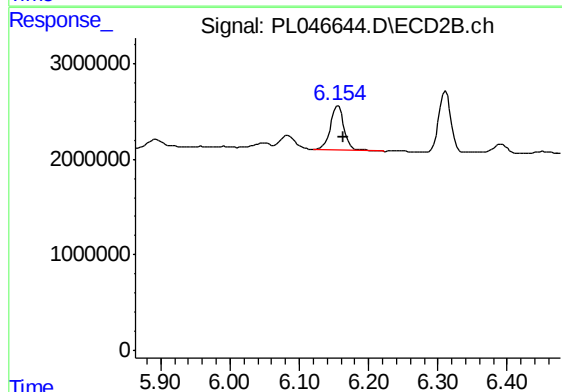


#26 Chlordane-4

R.T.: 6.156 min
Delta R.T.: -0.007 min
Response: 6431226
Conc: 13.94 ng/ml

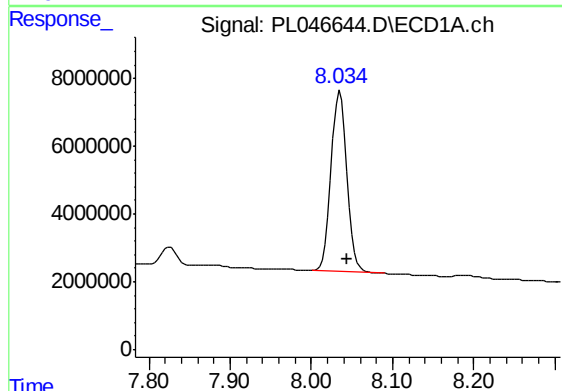

#28 Decachlorobiphenyl

R.T.: 8.035 min
Delta R.T.: -0.009 min
Response: 71915925
Conc: 8.55 ng/ml

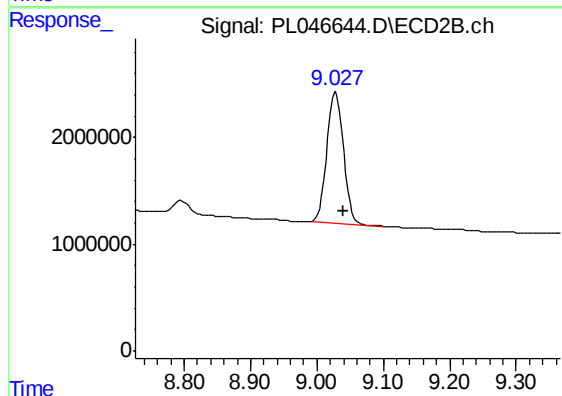

#28 Decachlorobiphenyl

R.T.: 9.029 min
Delta R.T.: -0.011 min
Response: 21380982
Conc: 9.22 ng/ml