

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032819\
 Data File : PL046647.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2019 18:28
 Operator : AJ\SJ
 Sample : K2086-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CS-13

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:15:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.977	71884556	24014222	9.882	10.488
28)	SA Decachlor...	8.035	9.028	118.4E6	34103822	14.076	14.710
Target Compounds							
2)	A alpha-BHC	3.795	0.000	5957551	0	0.511	N.D. #
9)	A Endosulfan I	5.391f	0.000	3674997	0	0.391	N.D. #
10)	B gamma-Chl...	0.000	6.082	0	2154780	N.D.	0.759 #
25)	Chlordane-3	0.000	6.082	0	2154780	N.D.	5.652 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032819\
Data File : PL046647.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2019 18:28
Operator : AJ\SJ
Sample : K2086-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CS-13

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:15:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

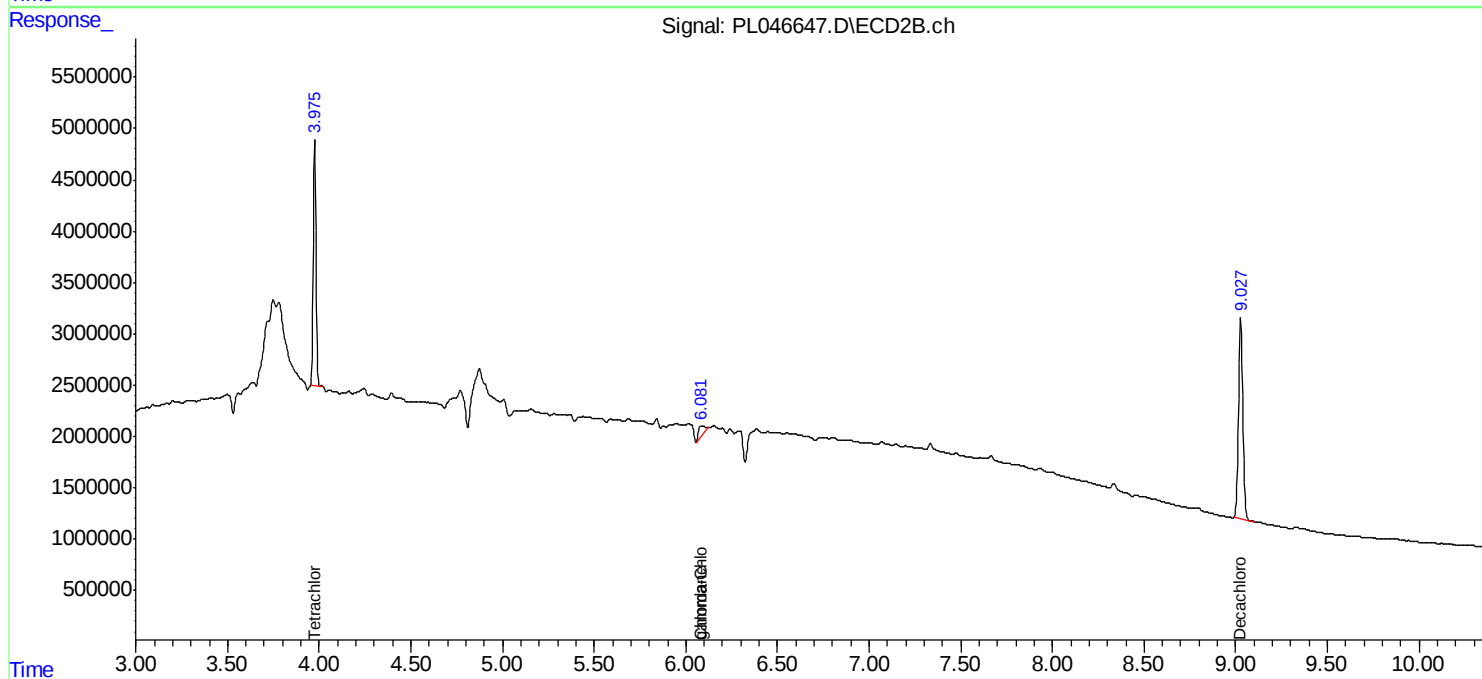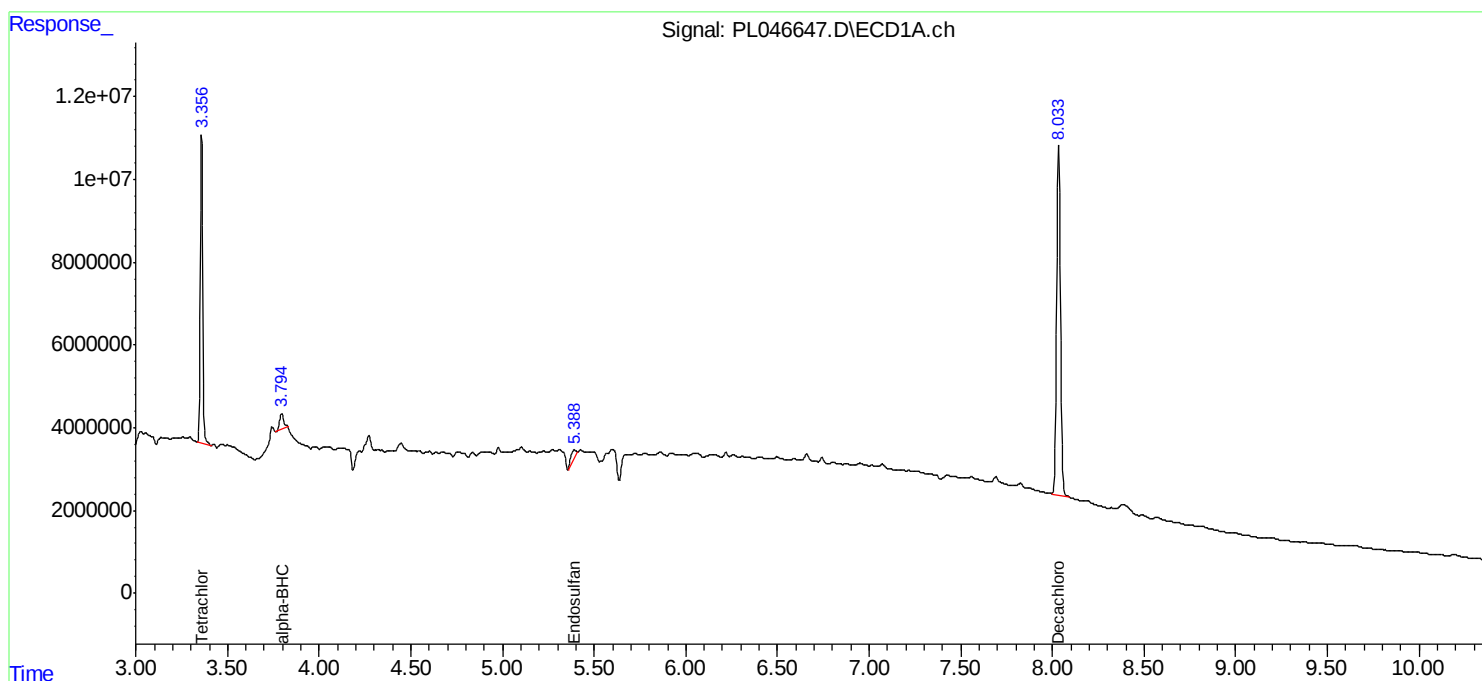


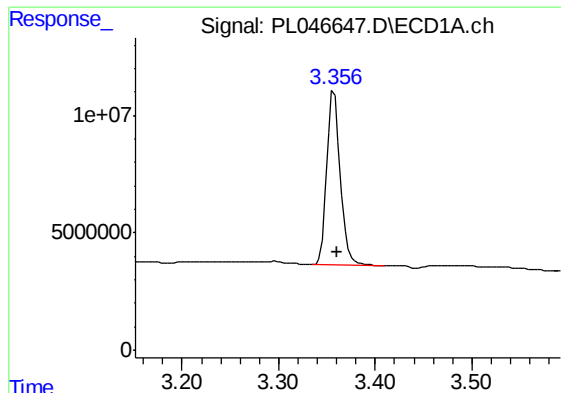

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 71884556
Conc: 9.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
CS-13

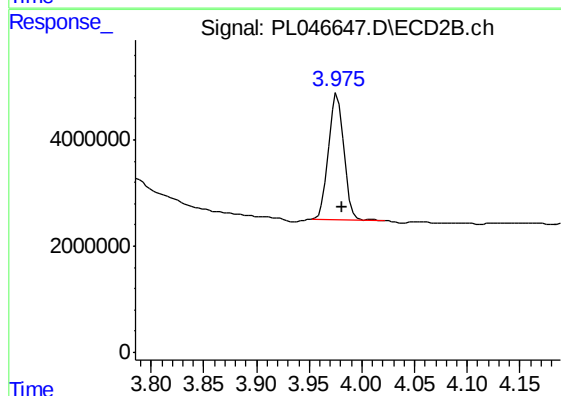


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.004 min
Response: 24014222
Conc: 10.49 ng/ml

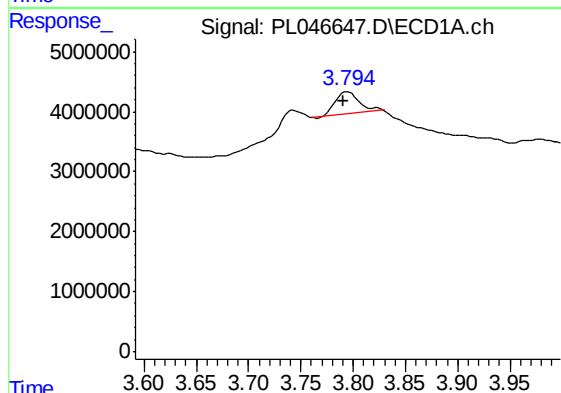


#2 alpha-BHC

R.T.: 3.795 min
Delta R.T.: 0.004 min
Response: 5957551
Conc: 0.51 ng/ml

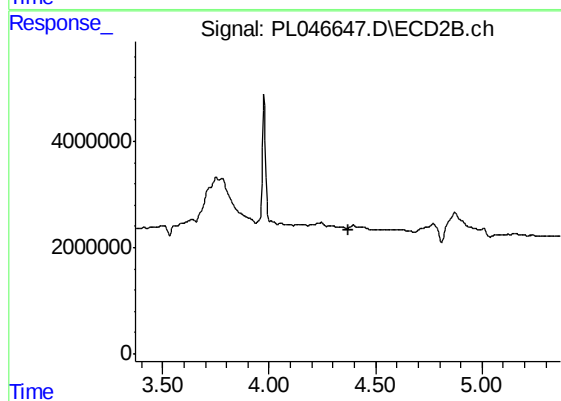

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.371 min
Response: 0
Conc: N.D.

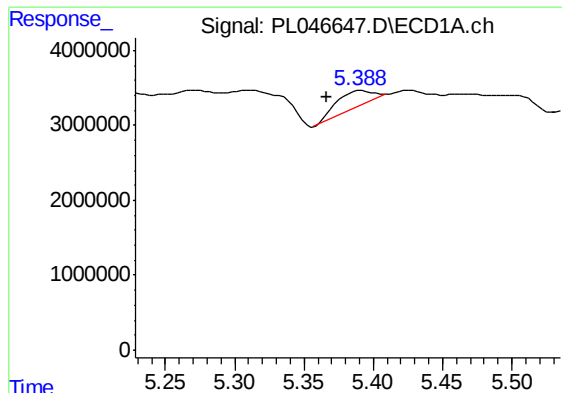

#9 Endosulfan I


R.T.: 5.391 min
Delta R.T.: 0.025 min
Response: 3674997
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
CS-13

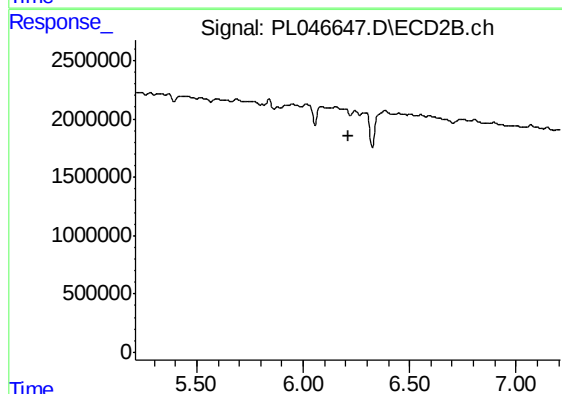


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.210 min
Response: 0
Conc: N.D.

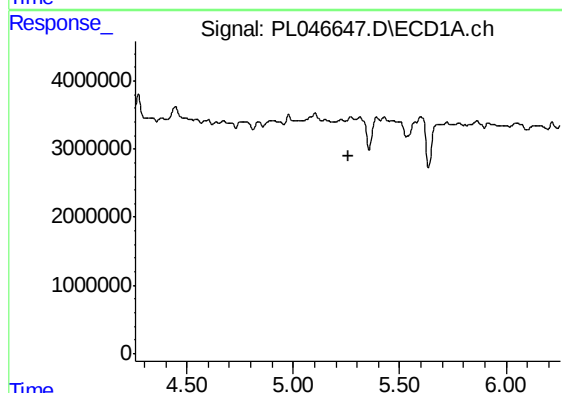


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.257 min
Response: 0
Conc: N.D.

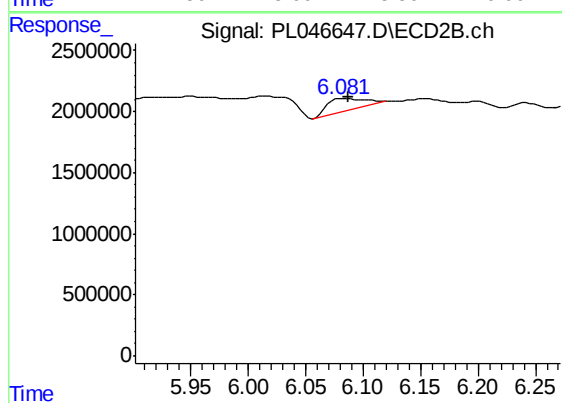

#10 gamma-Chlordane


R.T.: 6.082 min
Delta R.T.: -0.005 min
Response: 2154780
Conc: 0.76 ng/ml

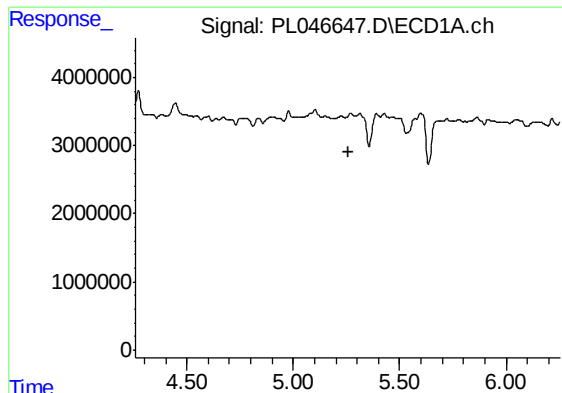

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CS-13

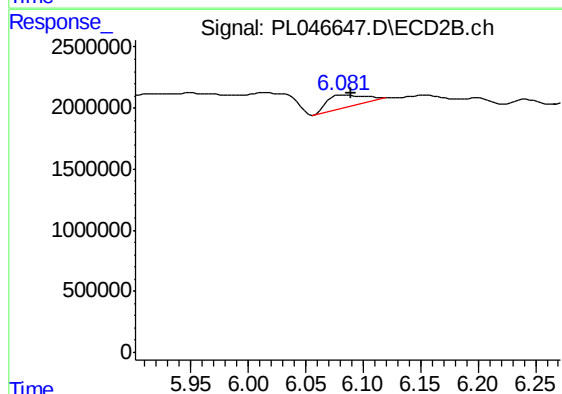


#25 Chlordane-3

R.T.: 6.082 min
Delta R.T.: -0.007 min
Response: 2154780
Conc: 5.65 ng/ml

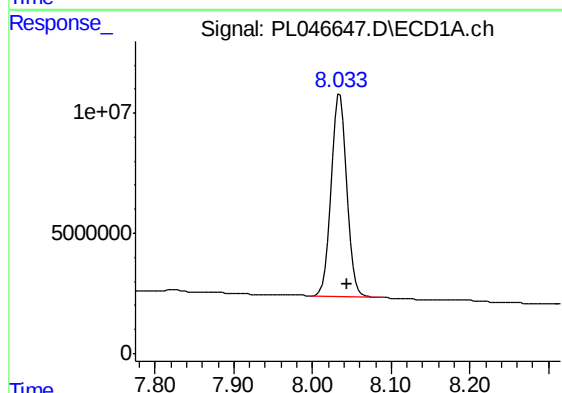

#28 Decachlorobiphenyl

R.T.: 8.035 min
Delta R.T.: -0.009 min
Response: 118391805
Conc: 14.08 ng/ml

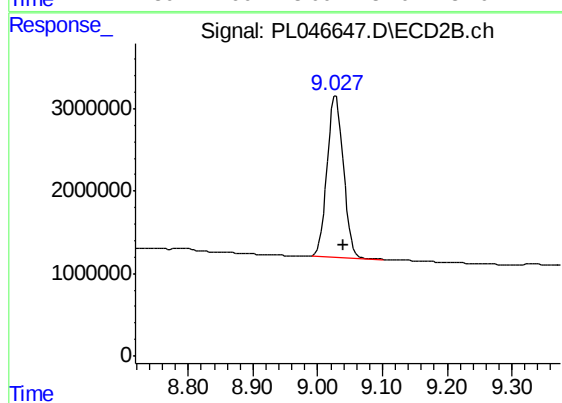

#28 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: -0.012 min
Response: 34103822
Conc: 14.71 ng/ml