

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032819\
 Data File : PL046664.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2019 22:46
 Operator : AJ\SJ
 Sample : K2107-11
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:18:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.358	3.977	124.8E6	40974018	17.151	17.896
28) SA Decachlor...	8.034	9.028	158.4E6	44507448	18.831	19.197
Target Compounds						
17) MA 4,4'-DDT	0.000	7.101	0	586995	N.D.	0.280 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032819\
Data File : PL046664.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2019 22:46
Operator : AJ\SJ
Sample : K2107-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:18:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

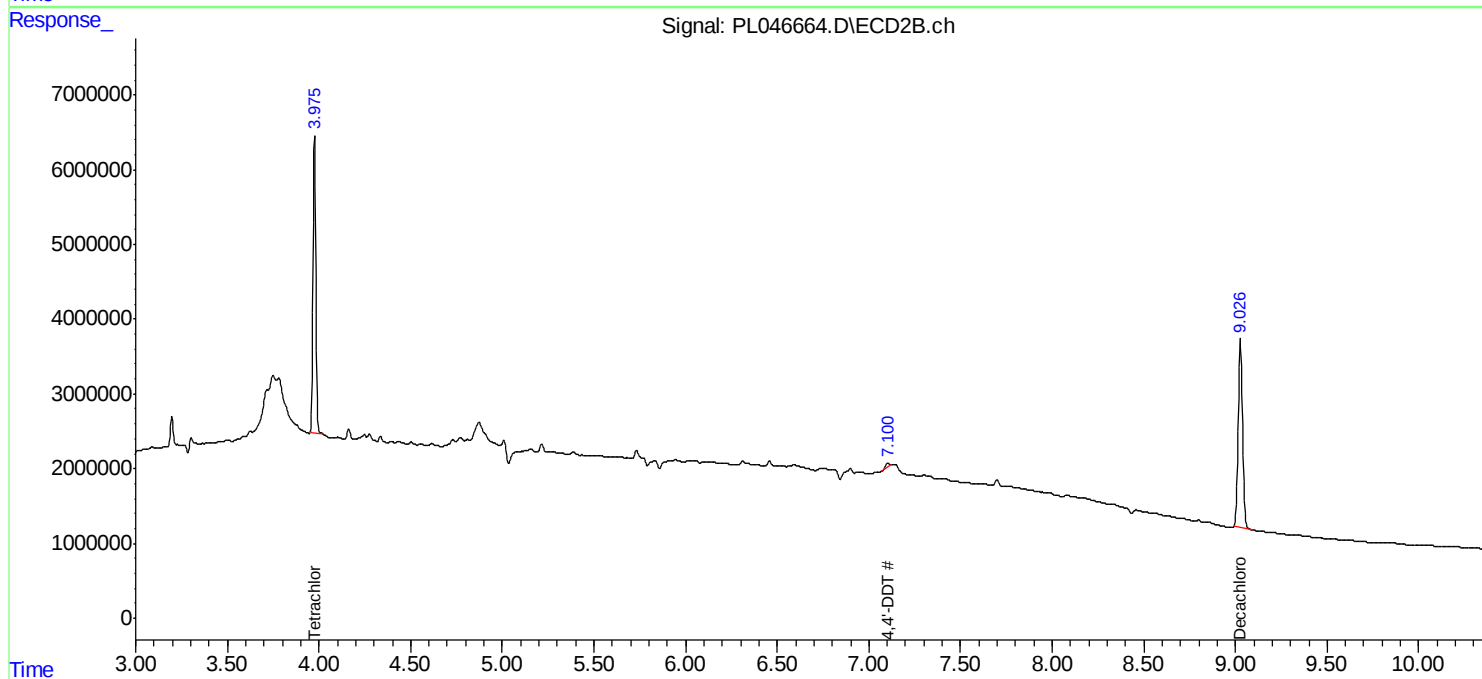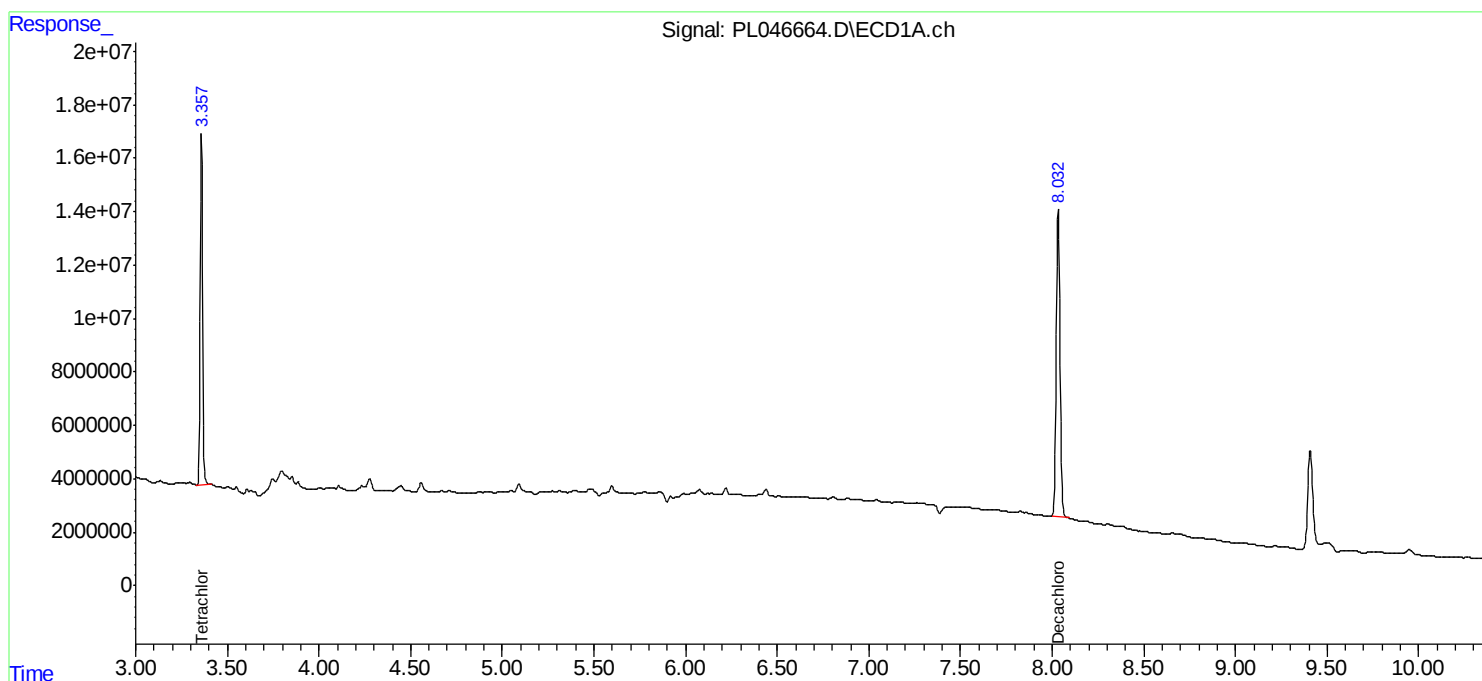


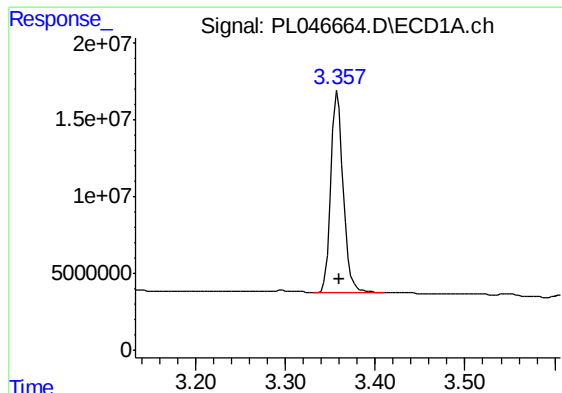

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 124770607
Conc: 17.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6

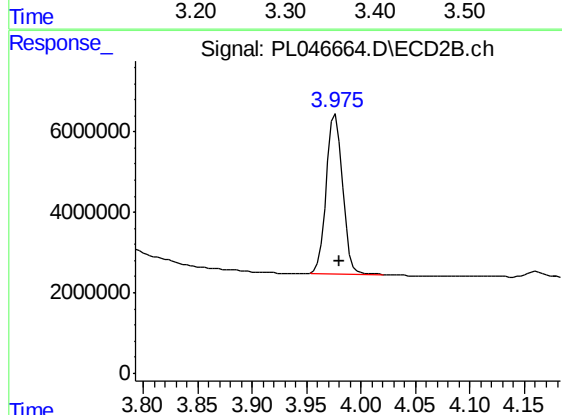


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.004 min
Response: 40974018
Conc: 17.90 ng/ml

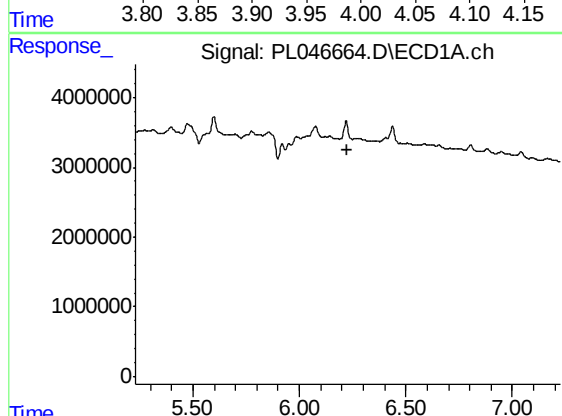


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.228 min
Response: 0
Conc: N.D.

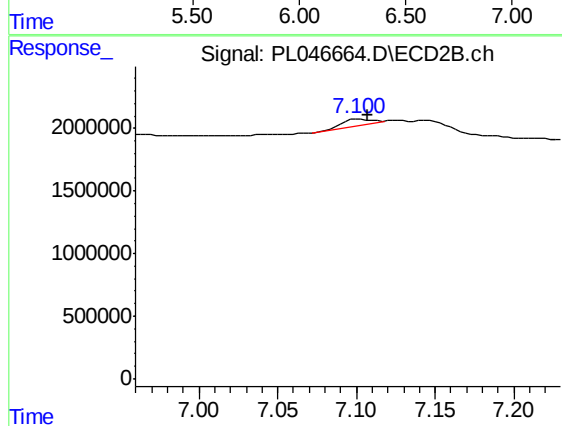

#17 4,4'-DDT


R.T.: 7.101 min
Delta R.T.: -0.005 min
Response: 586995
Conc: 0.28 ng/ml

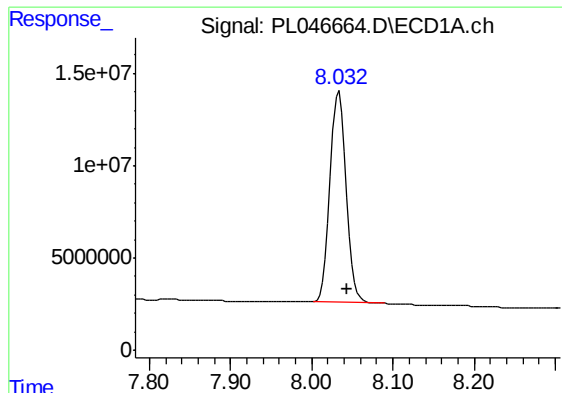

#28 Decachlorobiphenyl

R.T.: 8.034 min
Delta R.T.: -0.011 min
Response: 158386054
Conc: 18.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6

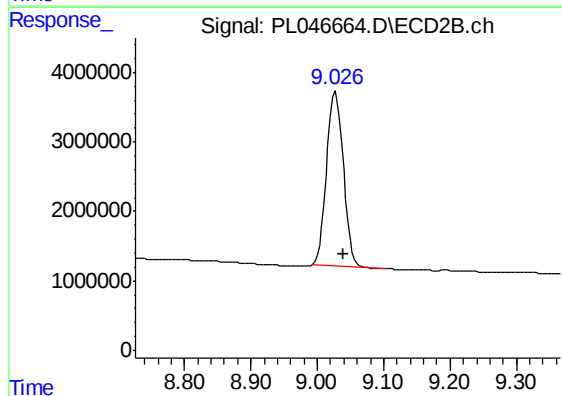

#28 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: -0.012 min
Response: 44507448
Conc: 19.20 ng/ml