

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032819\
 Data File : PL046697.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2019 06:56
 Operator : AJ\SJ
 Sample : K2097-02
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 08:19:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.977	47969653	16439713	6.594	7.180
28)	SA Decachlor...	8.035	9.030	63585465	18528144	7.560	7.992
Target Compounds							
2)	A alpha-BHC	0.000	4.392f	0	2401192	N.D.	0.747 #
8)	B Heptachlo...	0.000	5.877f	0	8761895	N.D.	3.322 #
12)	B 4,4'-DDE	5.474	6.311	7028983	2819017	0.763	1.136 #
16)	A 4,4'-DDD	0.000	6.807	0	7954192	N.D.	3.953 #
17)	MA 4,4'-DDT	6.217	0.000	33812086	0	4.464	N.D. #
18)	B Endrin al...	6.308	0.000	9605163	0	1.282	N.D. #
19)	B Endosulfa...	6.499	0.000	11875856	0	1.446	N.D. #
20)	A Methoxychlor	6.745f	0.000	10546488	0	2.482	N.D. #
21)	B Endrin ke...	7.015f	0.000	9500822	0	1.027	N.D. #
27)	Chlordane-5	6.168f	0.000	4856583	0	14.231	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032819\
Data File : PL046697.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2019 06:56
Operator : AJ\SJ
Sample : K2097-02
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 08:19:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

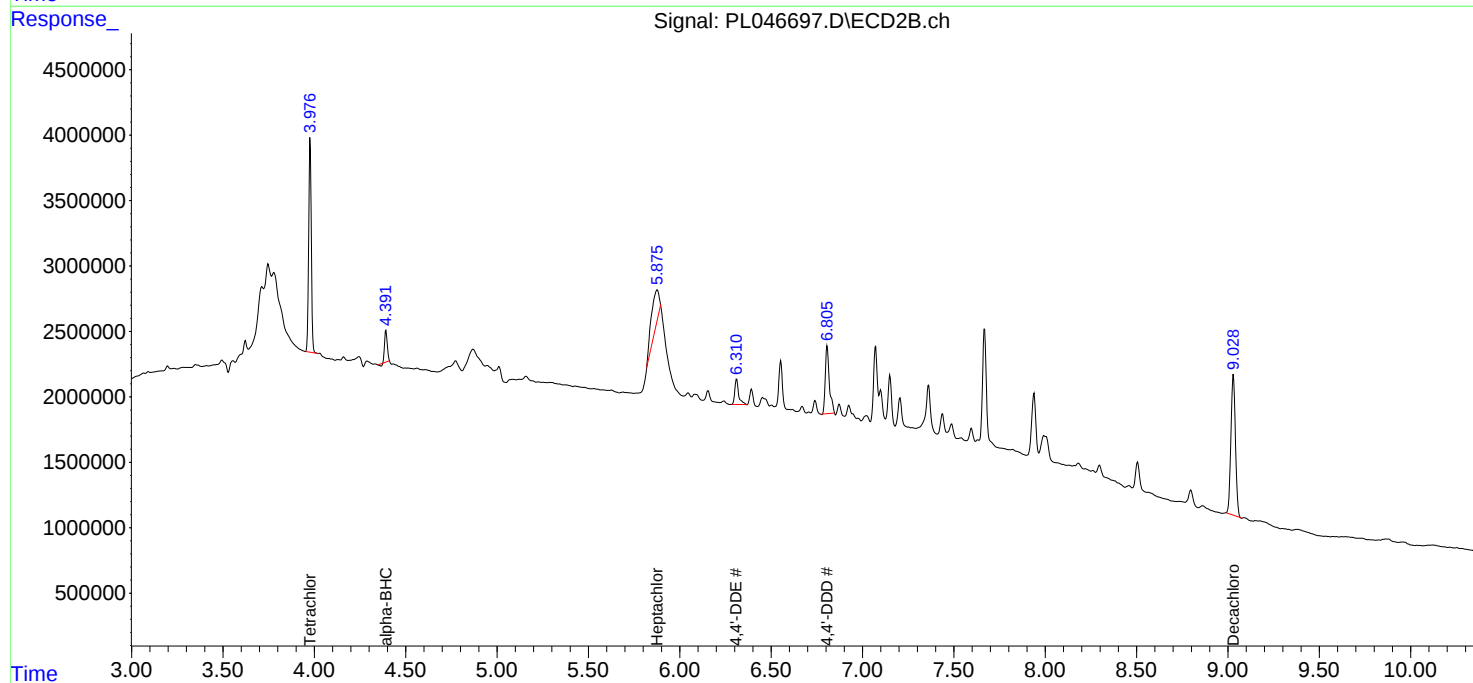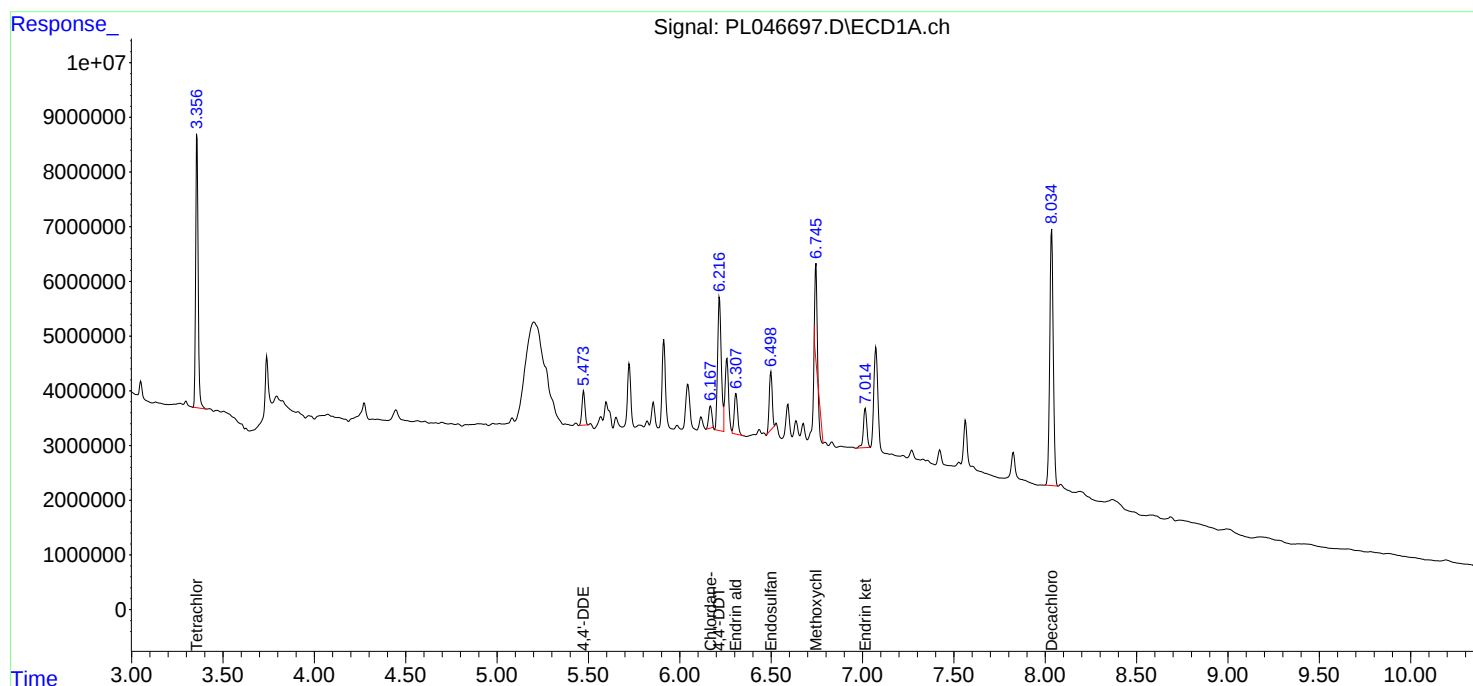


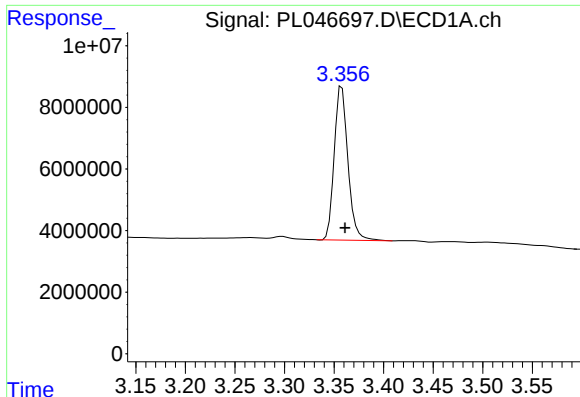

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 47969653
Conc: 6.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

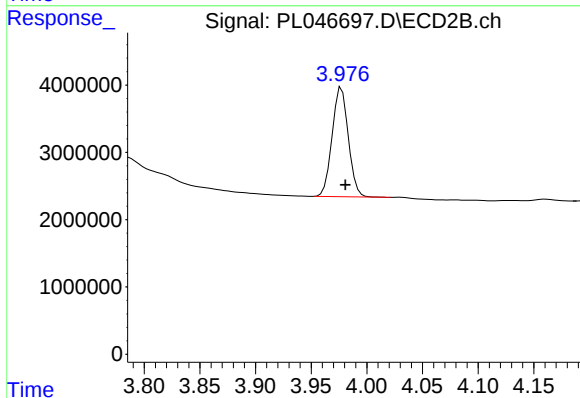


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.003 min
Response: 16439713
Conc: 7.18 ng/ml

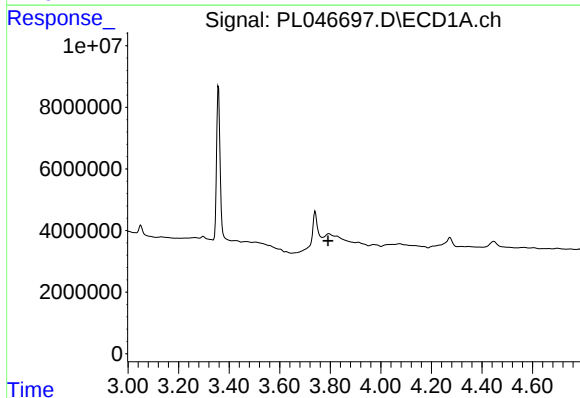


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.791 min
Response: 0
Conc: N.D.

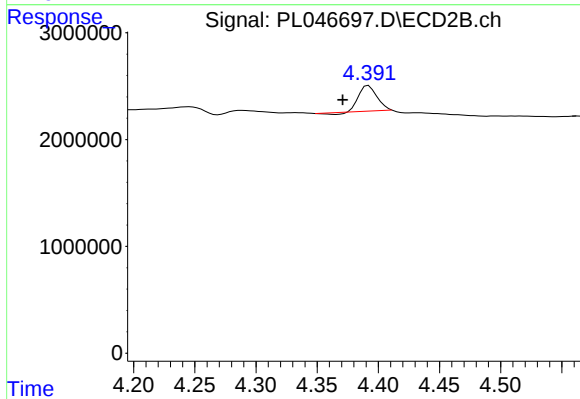

#2 alpha-BHC


R.T.: 4.392 min
Delta R.T.: 0.021 min
Response: 2401192
Conc: 0.75 ng/ml

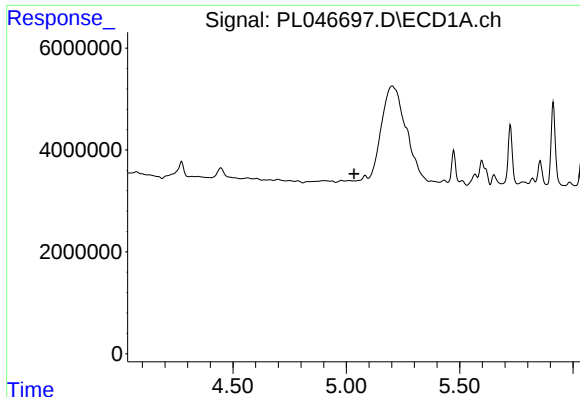

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.034 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

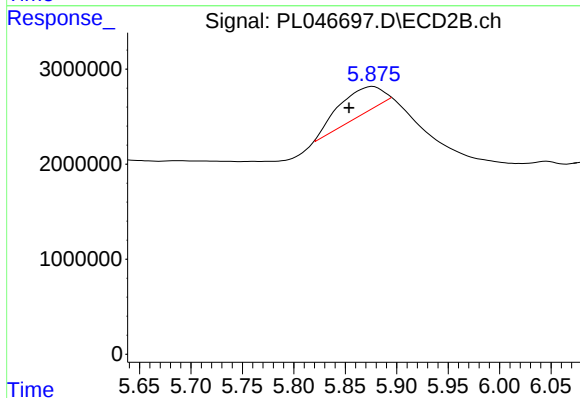


#8 Heptachlor epoxide

R.T.: 5.877 min
Delta R.T.: 0.023 min
Response: 8761895
Conc: 3.32 ng/ml

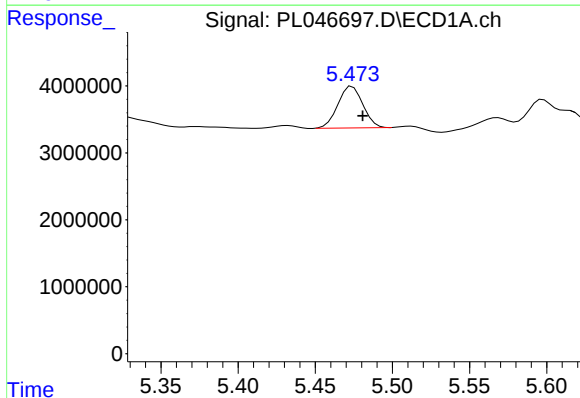


#12 4,4'-DDE

R.T.: 5.474 min
Delta R.T.: -0.007 min
Response: 7028983
Conc: 0.76 ng/ml

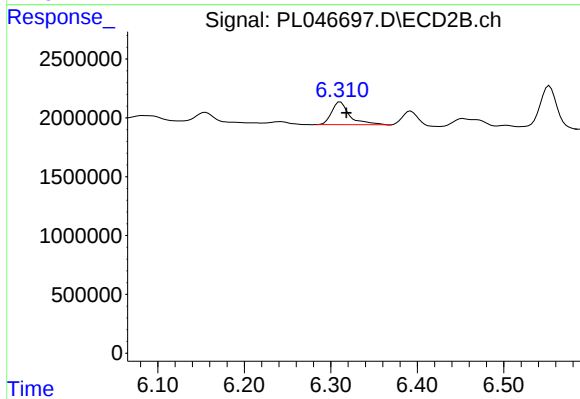

#12 4,4'-DDE


R.T.: 6.311 min
Delta R.T.: -0.007 min
Response: 2819017
Conc: 1.14 ng/ml

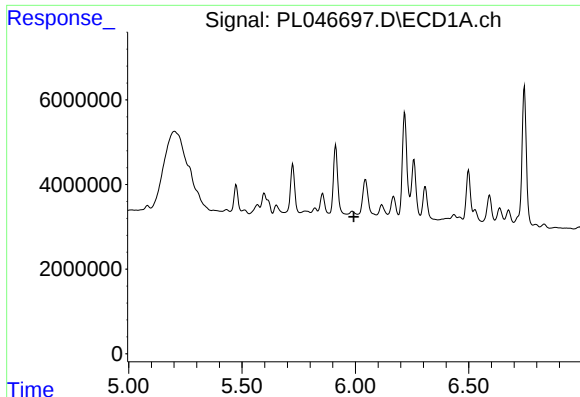

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.993 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

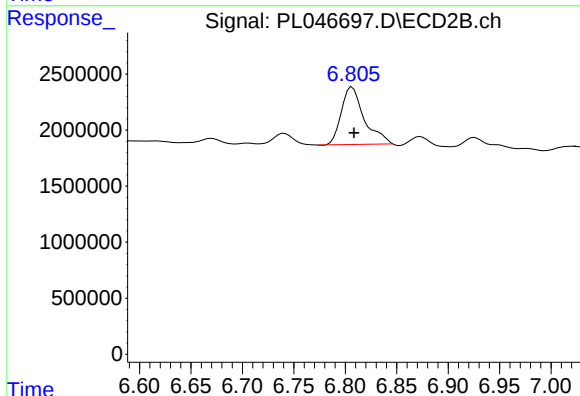


#16 4,4'-DDD

R.T.: 6.807 min
Delta R.T.: -0.002 min
Response: 7954192
Conc: 3.95 ng/ml

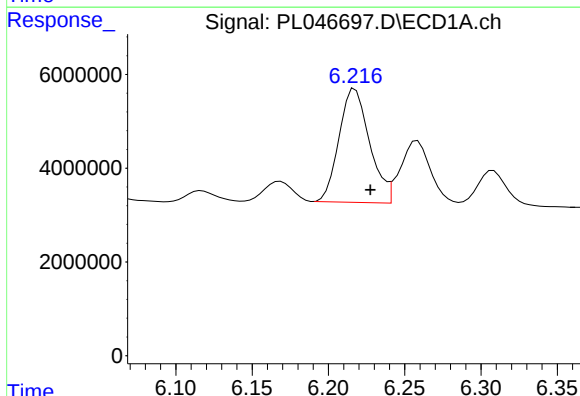


#17 4,4'-DDT

R.T.: 6.217 min
Delta R.T.: -0.010 min
Response: 33812086
Conc: 4.46 ng/ml

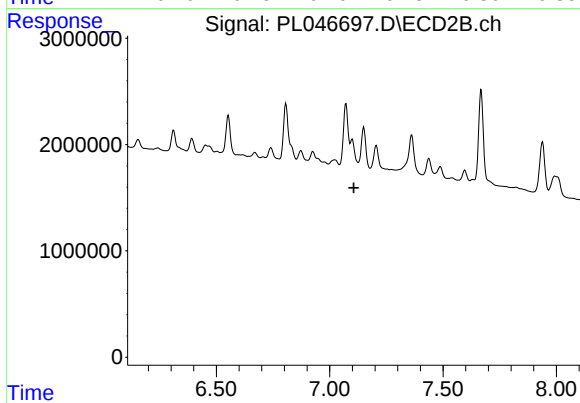

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.107 min
Response: 0
Conc: N.D.

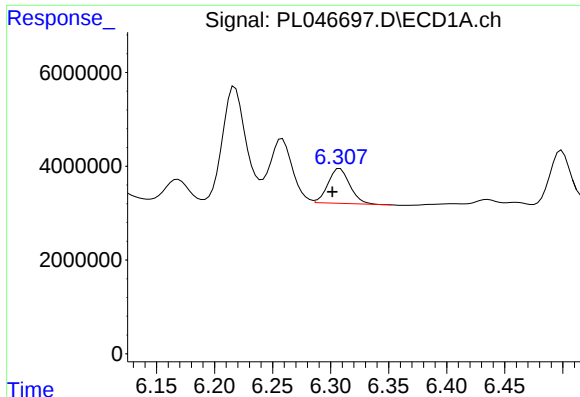

#18 Endrin aldehyde


R.T.: 6.308 min
Delta R.T.: 0.006 min
Response: 9605163
Conc: 1.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

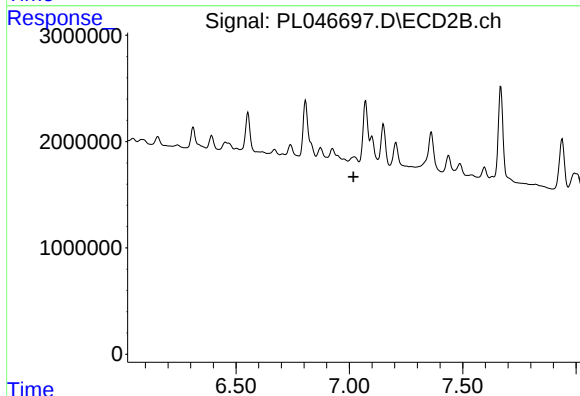


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.019 min
Response: 0
Conc: N.D.

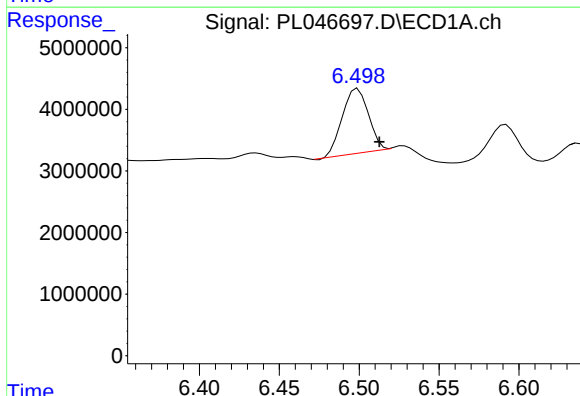


#19 Endosulfan Sulfate

R.T.: 6.499 min
Delta R.T.: -0.014 min
Response: 11875856
Conc: 1.45 ng/ml

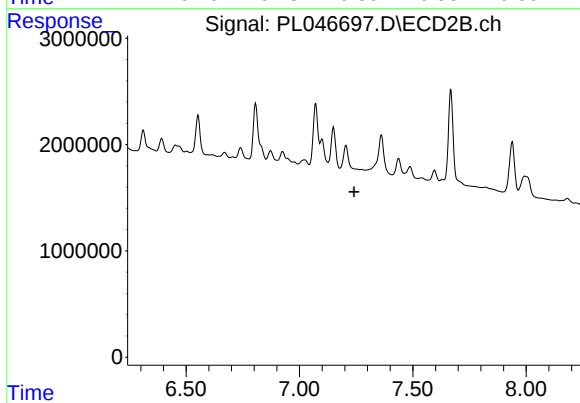

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.242 min
Response: 0
Conc: N.D.

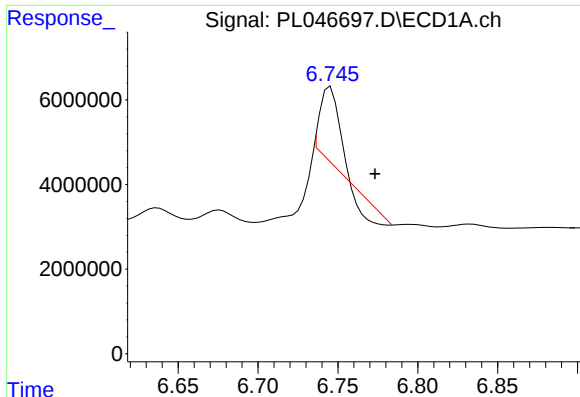

#20 Methoxychlor


R.T.: 6.745 min
Delta R.T.: -0.028 min
Response: 10546488
Conc: 2.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

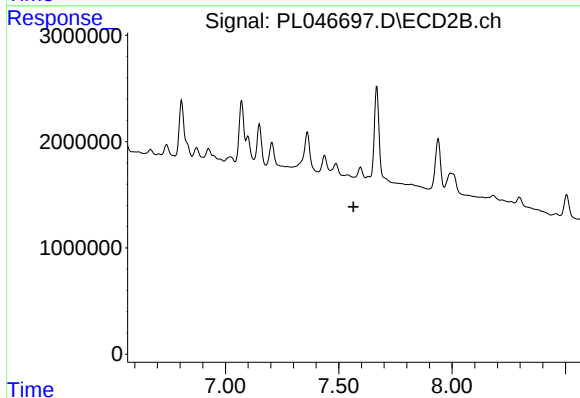


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.565 min
Response: 0
Conc: N.D.

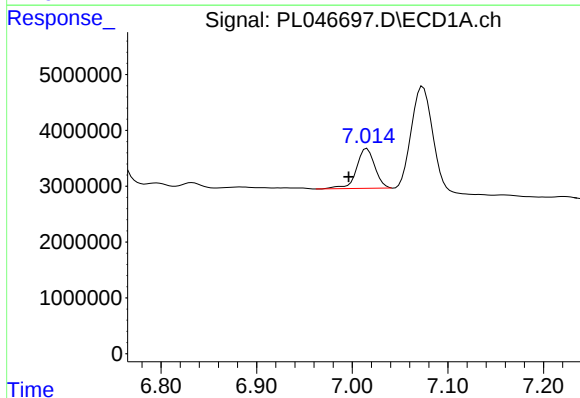


#21 Endrin ketone

R.T.: 7.015 min
Delta R.T.: 0.019 min
Response: 9500822
Conc: 1.03 ng/ml

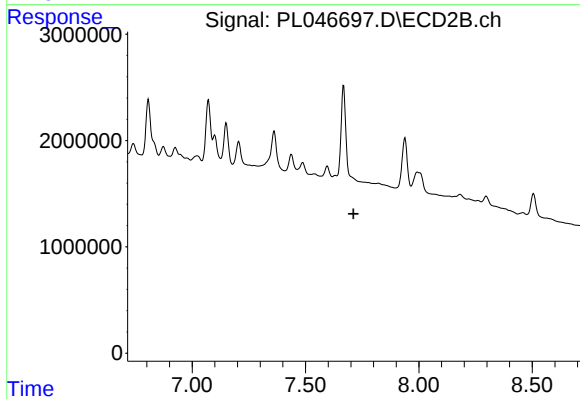

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.712 min
Response: 0
Conc: N.D.

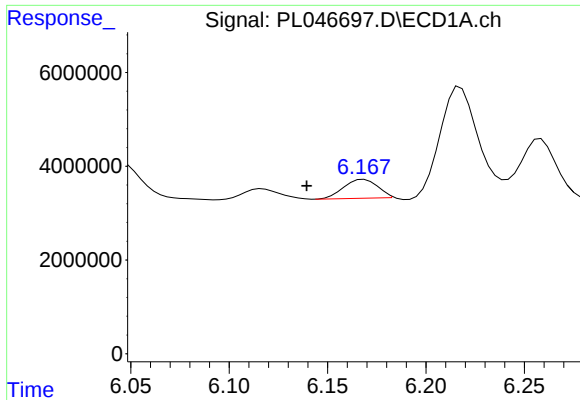

#27 Chlordane-5


R.T.: 6.168 min
Delta R.T.: 0.029 min
Response: 4856583
Conc: 14.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

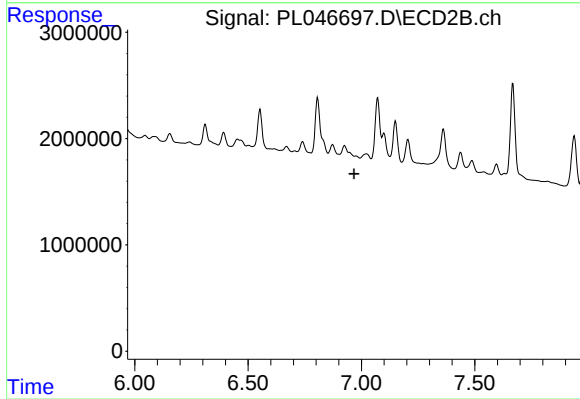


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.967 min
Response: 0
Conc: N.D.

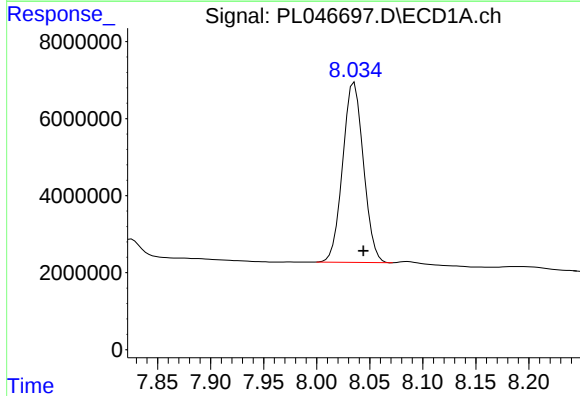

#28 Decachlorobiphenyl

R.T.: 8.035 min
Delta R.T.: -0.009 min
Response: 63585465
Conc: 7.56 ng/ml

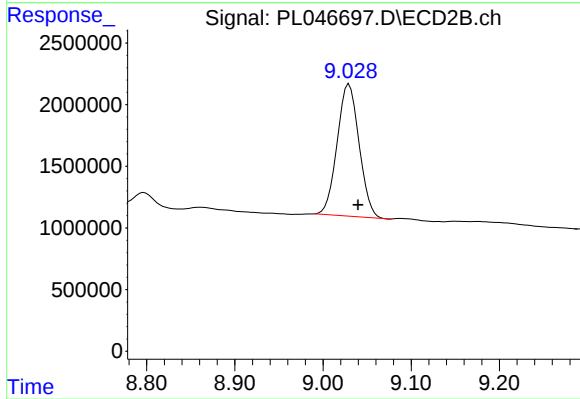

#28 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: -0.010 min
Response: 18528144
Conc: 7.99 ng/ml