

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032819\
 Data File : PL046608.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2019 07:39
 Operator : AJ\SJ
 Sample : MDL-CHL-S-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-CHL-S-06

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 08:50:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.977	151.4E6	48001276	20.806	20.965
28)	SA Decachlor...	8.034	9.028	189.5E6	54753583	22.529	23.616
Target Compounds							
23)	Chlordane-1	4.203	4.968	8850770	2932746	26.318	27.101
24)	Chlordane-2	4.695	5.435	11420165	3662527	30.099	31.355
25)	Chlordane-3	5.251	6.081	26624988	11218212	23.907	29.423
26)	Chlordane-4	5.307	6.154	25428116	14116411	24.591	30.593
27)	Chlordane-5	6.130	6.957	8217384	2464164	24.079	27.429



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032819\
Data File : PL046608.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2019 07:39
Operator : AJ\SJ
Sample : MDL-CHL-S-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-S-06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 08:50:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

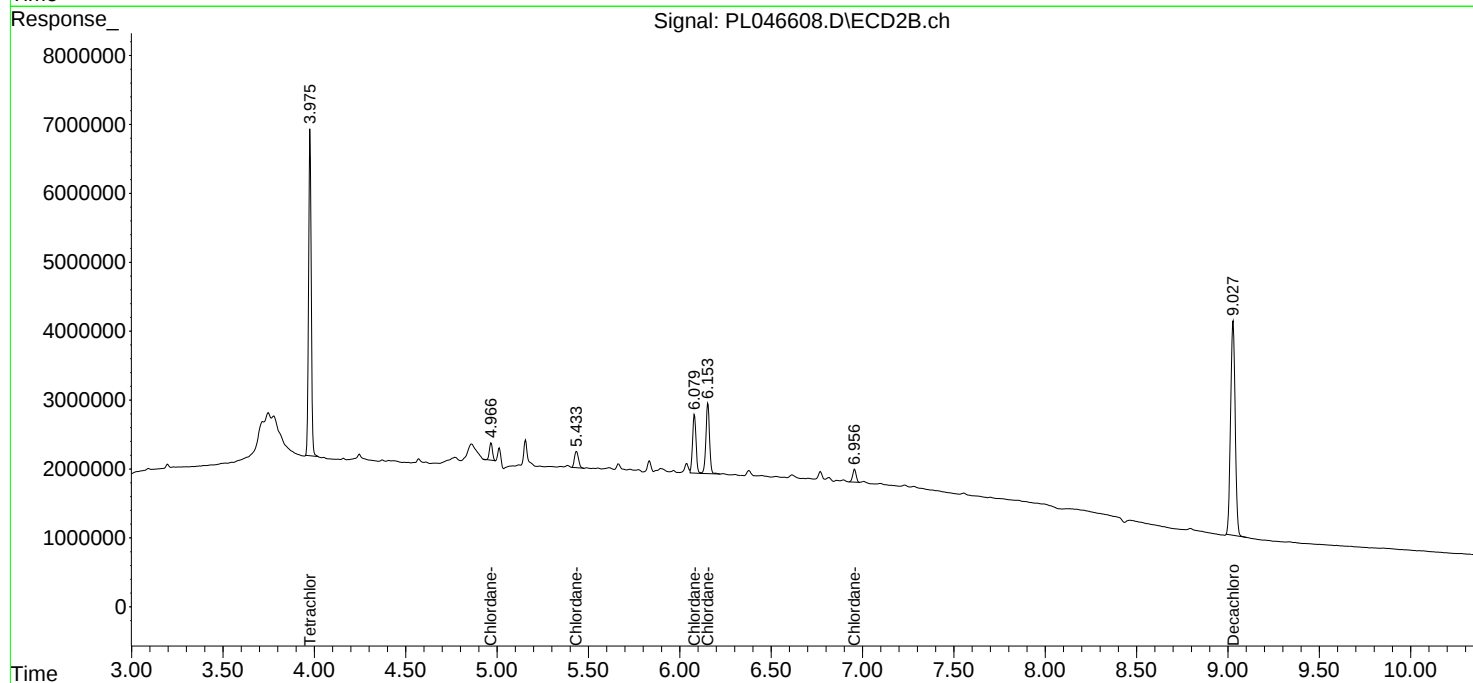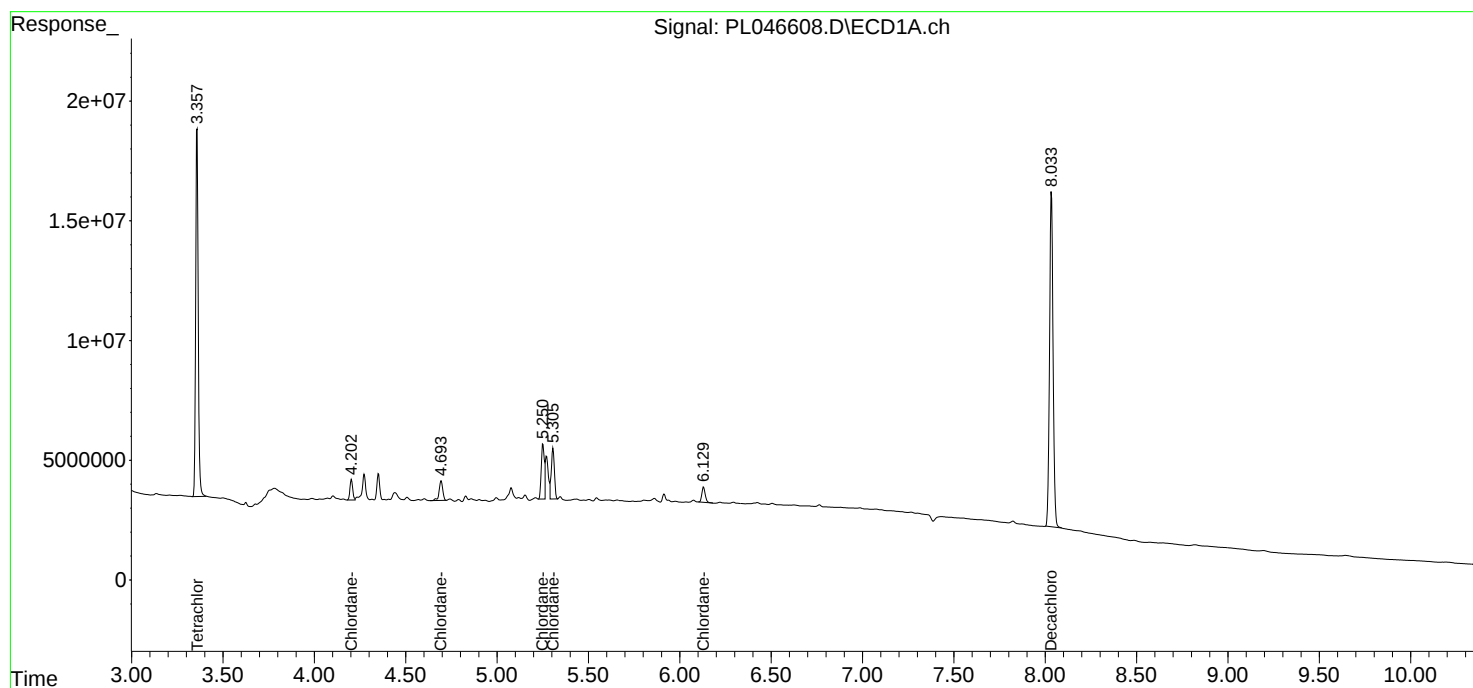


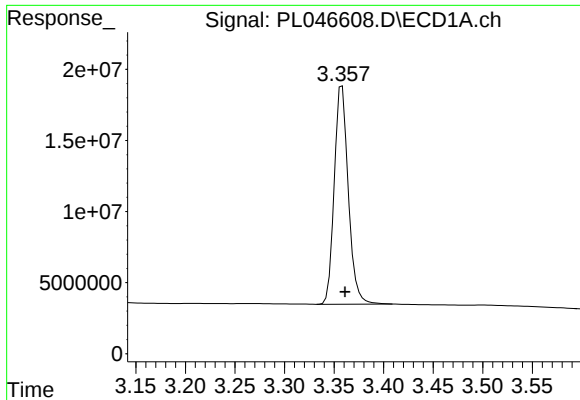

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 151359289
Conc: 20.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-S-06

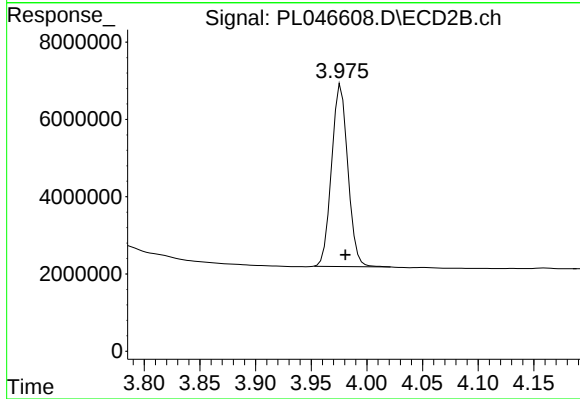


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.004 min
Response: 48001276
Conc: 20.96 ng/ml

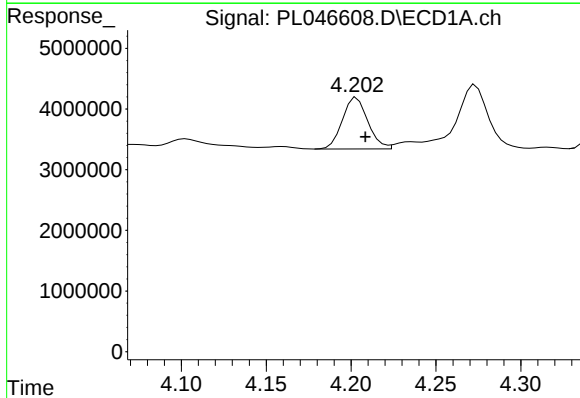


#23 Chlordane-1

R.T.: 4.203 min
Delta R.T.: -0.005 min
Response: 8850770
Conc: 26.32 ng/ml

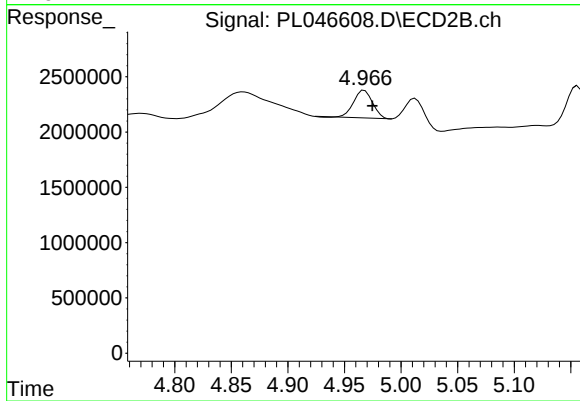

#23 Chlordane-1


R.T.: 4.968 min
Delta R.T.: -0.007 min
Response: 2932746
Conc: 27.10 ng/ml

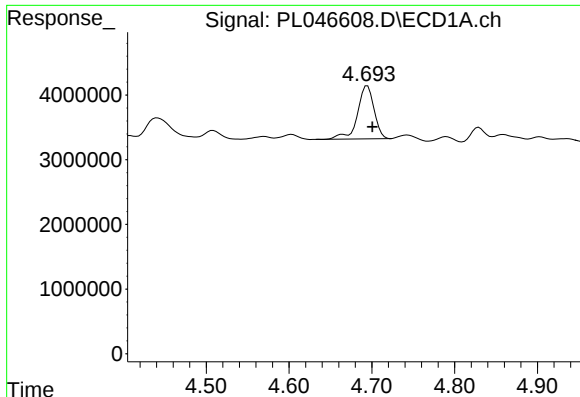

#24 Chlordane-2


R.T.: 4.695 min
Delta R.T.: -0.006 min
Response: 11420165
Conc: 30.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-S-06

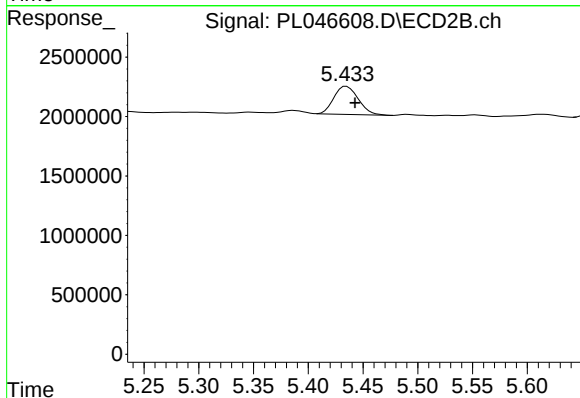


#24 Chlordane-2

R.T.: 5.435 min
Delta R.T.: -0.008 min
Response: 3662527
Conc: 31.35 ng/ml

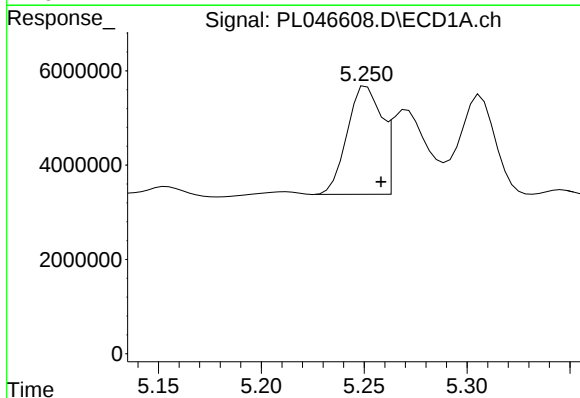


#25 Chlordane-3

R.T.: 5.251 min
Delta R.T.: -0.007 min
Response: 26624988
Conc: 23.91 ng/ml

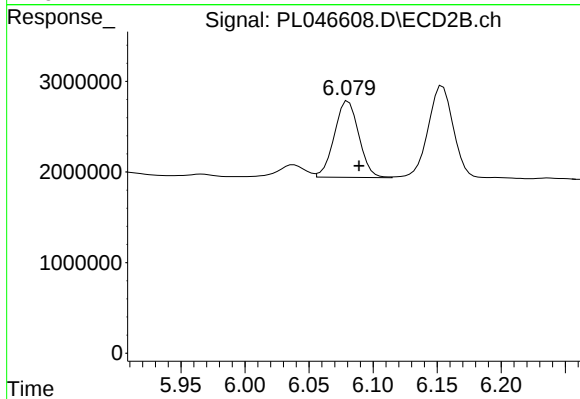

#25 Chlordane-3


R.T.: 6.081 min
Delta R.T.: -0.008 min
Response: 11218212
Conc: 29.42 ng/ml

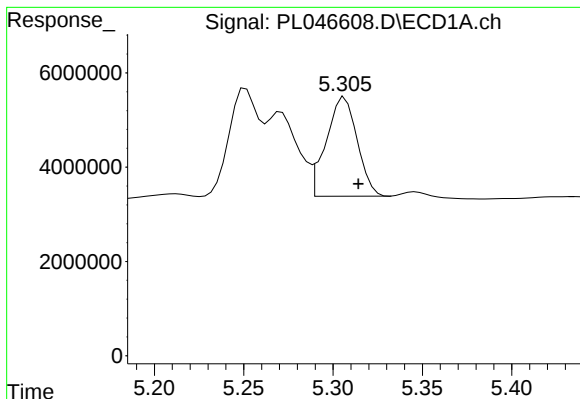

#26 Chlordane-4


R.T.: 5.307 min
Delta R.T.: -0.008 min
Response: 25428116
Conc: 24.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-S-06

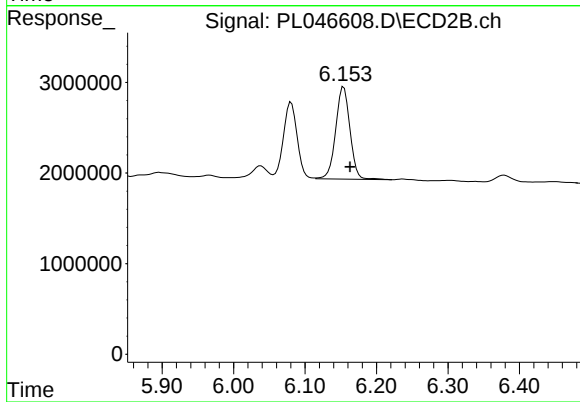


#26 Chlordane-4

R.T.: 6.154 min
Delta R.T.: -0.009 min
Response: 14116411
Conc: 30.59 ng/ml

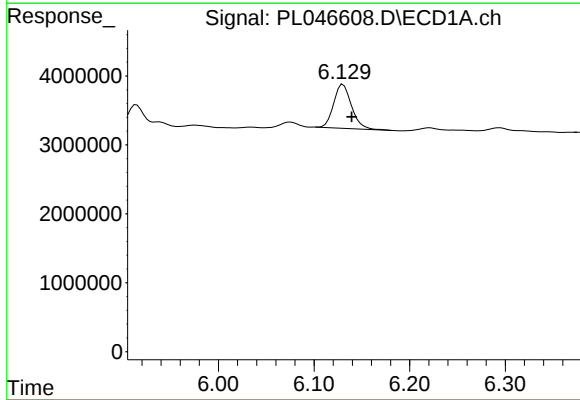


#27 Chlordane-5

R.T.: 6.130 min
Delta R.T.: -0.009 min
Response: 8217384
Conc: 24.08 ng/ml

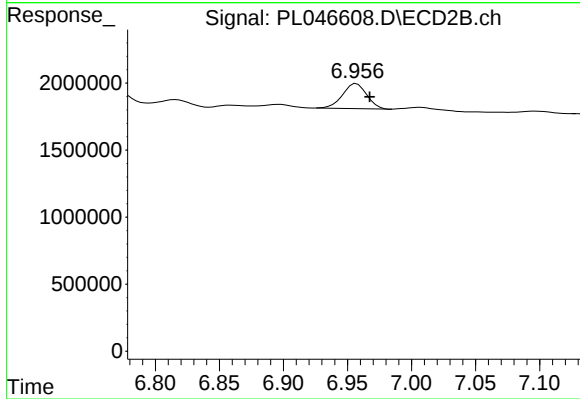

#27 Chlordane-5

R.T.: 6.957 min
Delta R.T.: -0.010 min
Response: 2464164
Conc: 27.43 ng/ml

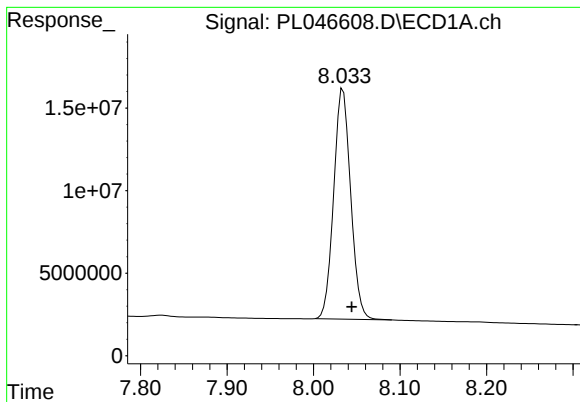

#28 Decachlorobiphenyl


R.T.: 8.034 min

Delta R.T.: -0.010 min

Response: 189489579

Conc: 22.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-S-06

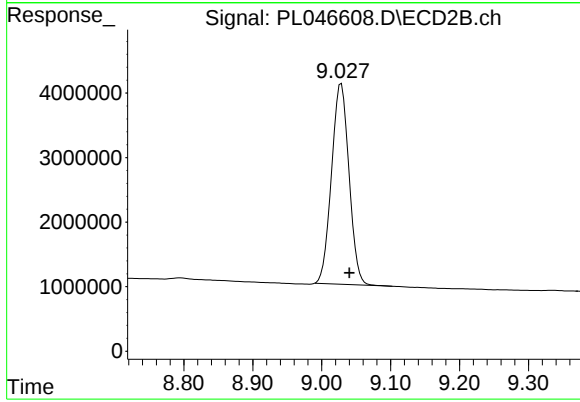

#28 Decachlorobiphenyl

R.T.: 9.028 min

Delta R.T.: -0.011 min

Response: 54753583

Conc: 23.62 ng/ml