

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032822\
 Data File : PL073703.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2022 14:13
 Operator : AR\AJ
 Sample : N2123-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20220388-COMP-CS-1

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/29/2022
 Supervised By : mohammad ahmed 03/30/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:46:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.643	5.490	2375393	10691428	7.416	6.514m
2) SA Decachlor...	10.418	11.336	3445406	10556331	6.776	5.903

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032822\
Data File : PL073703.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2022 14:13
Operator : AR\AJ
Sample : N2123-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20220388-COMP-CS-1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/29/2022
Supervised By : mohammad ahmed 03/30/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:46:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

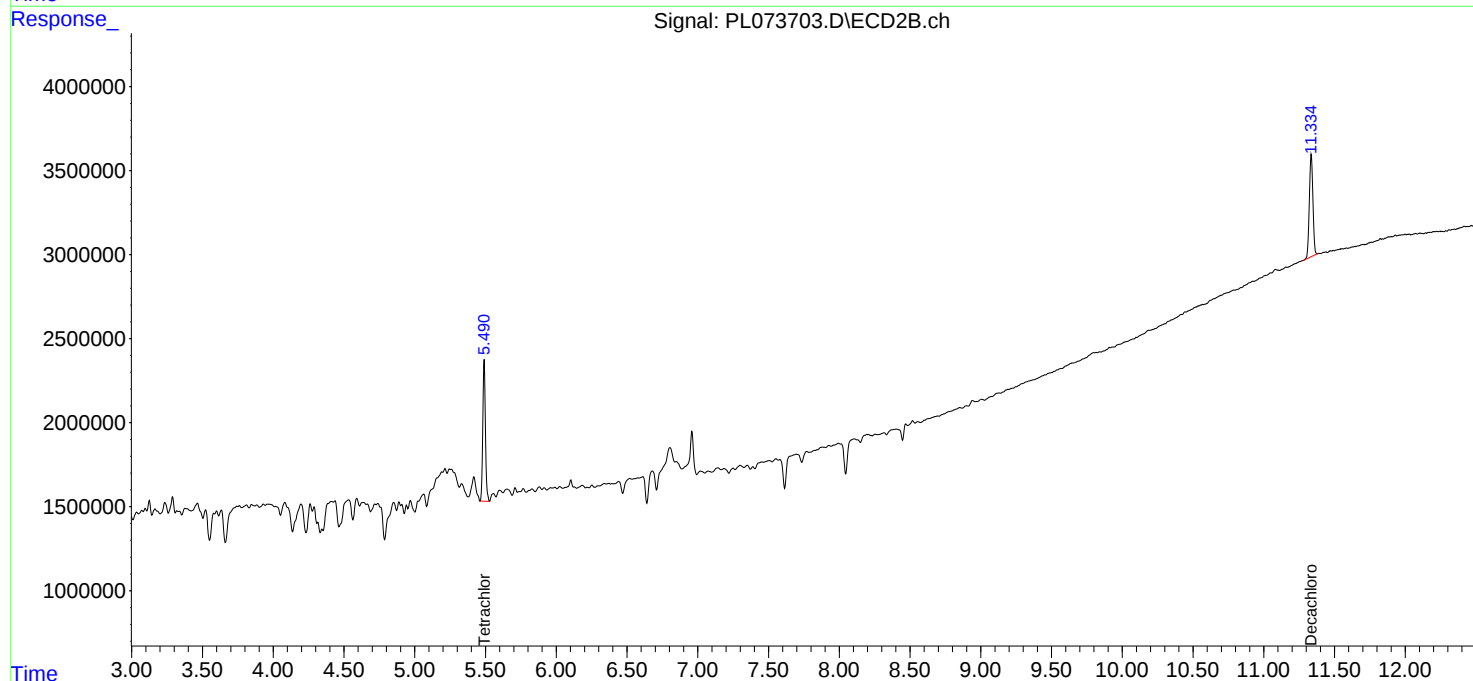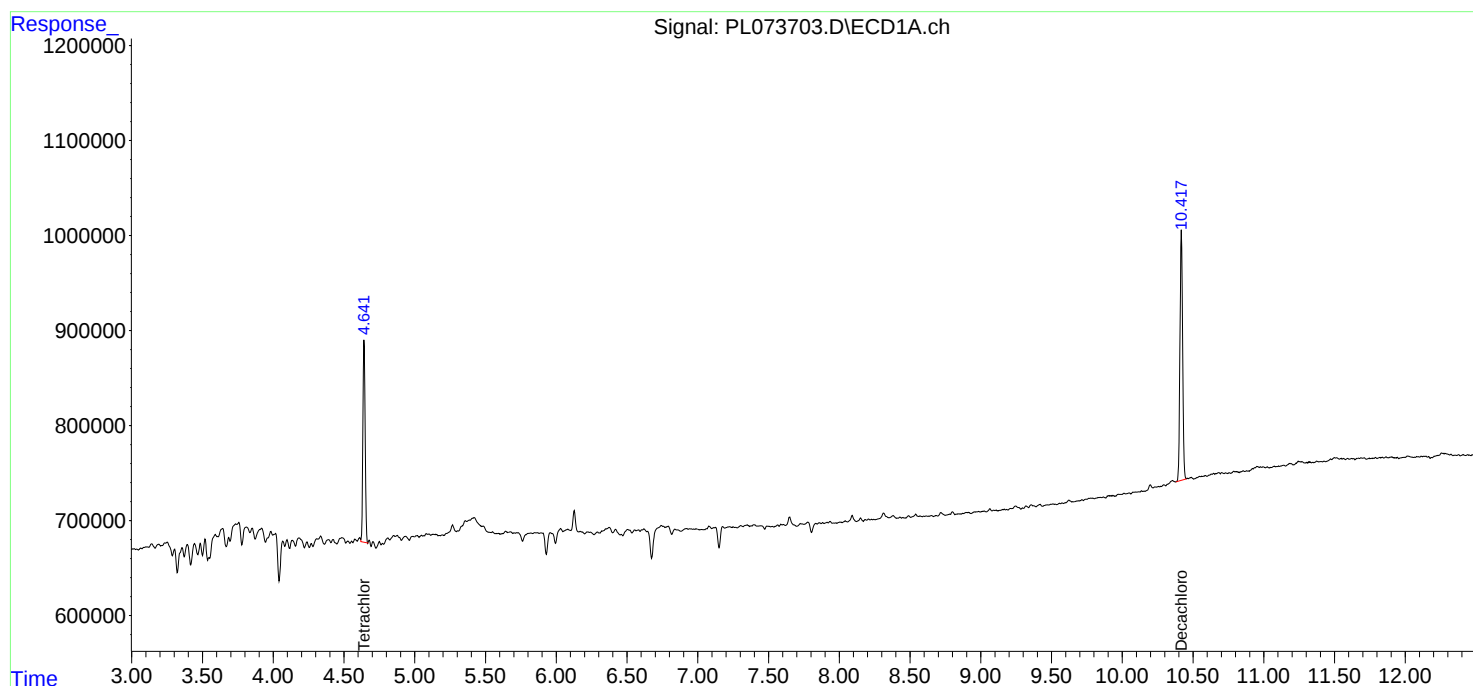

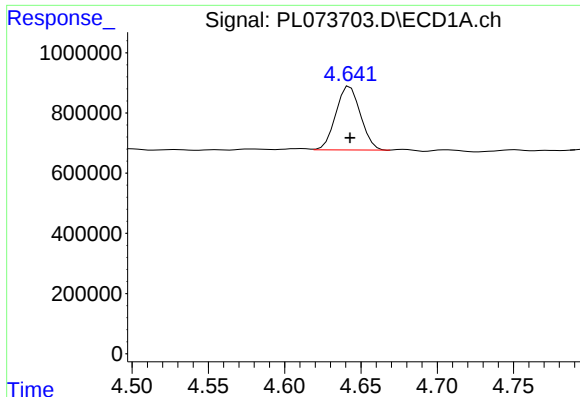


#1 Tetrachloro-m-xylene

R.T.: 4.643 min
Delta R.T.: 0.000 min
Response: 2375393
Conc: 7.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
20220388-COMP-CS-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/29/2022
Supervised By :mohammad ahmed 03/30/2022

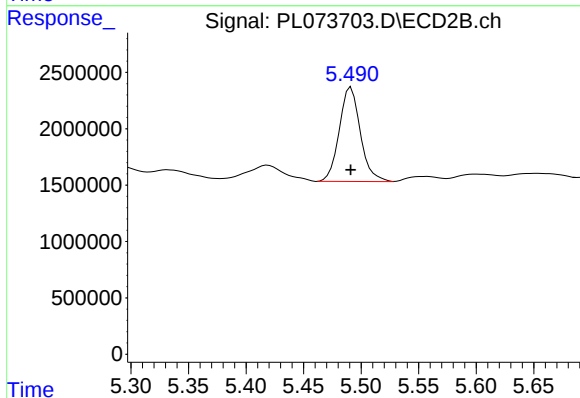


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: -0.001 min
Response: 10691428
Conc: 6.51 ng/ml m

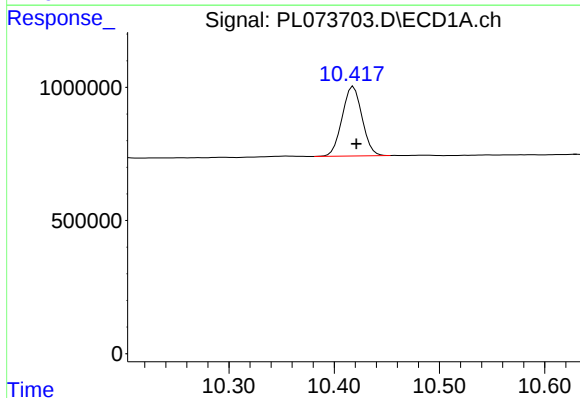

#28 Decachlorobiphenyl

R.T.: 10.418 min
Delta R.T.: -0.003 min
Response: 3445406
Conc: 6.78 ng/ml

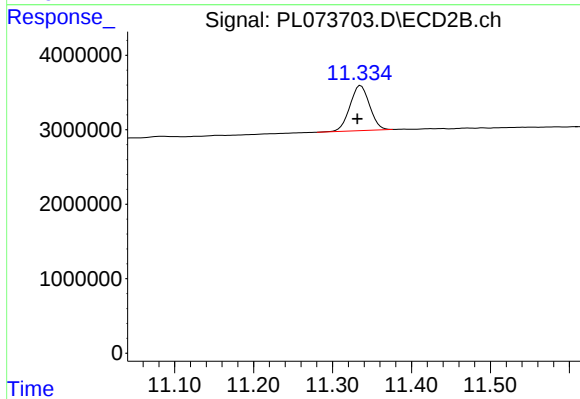

#28 Decachlorobiphenyl

R.T.: 11.336 min
Delta R.T.: 0.005 min
Response: 10556331
Conc: 5.90 ng/ml