

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032919\
 Data File : PL046739.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2019 17:31
 Operator : AJ\SJ
 Sample : K2138-07
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S6B(2-10)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 23:17:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.978	156.4E6	51512117	21.498	22.498
28)	SA Decachlor...	8.036	9.030	172.5E6	53036514	20.512	22.876
Target Compounds							
9)	A Endosulfan I	0.000	6.209	0	4181329	N.D.	1.602 #
11)	B alpha-Chl...	5.317	0.000	19710359	0	1.944	N.D. #
26)	Chlordane-4	5.317	0.000	19710359	0	19.061	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032919\
Data File : PL046739.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2019 17:31
Operator : AJ\SJ
Sample : K2138-07
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
S6B(2-10)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 23:17:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

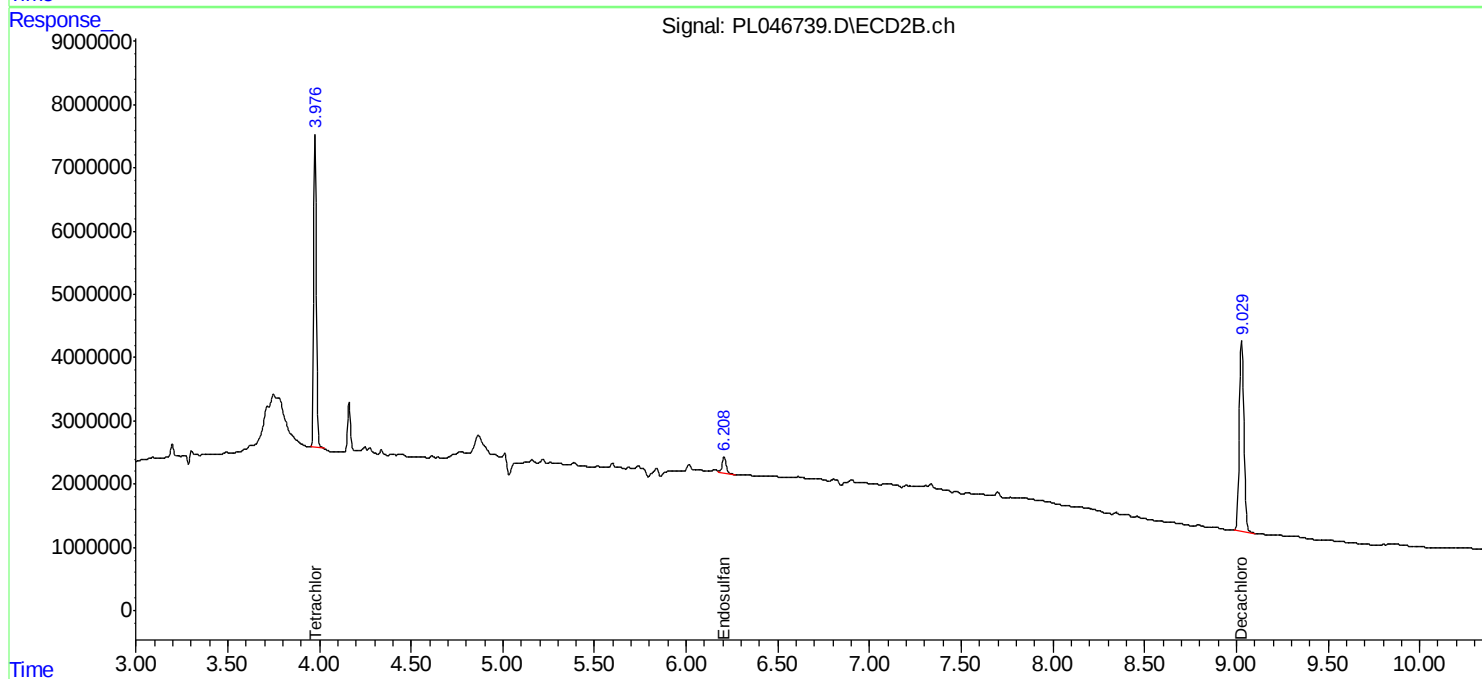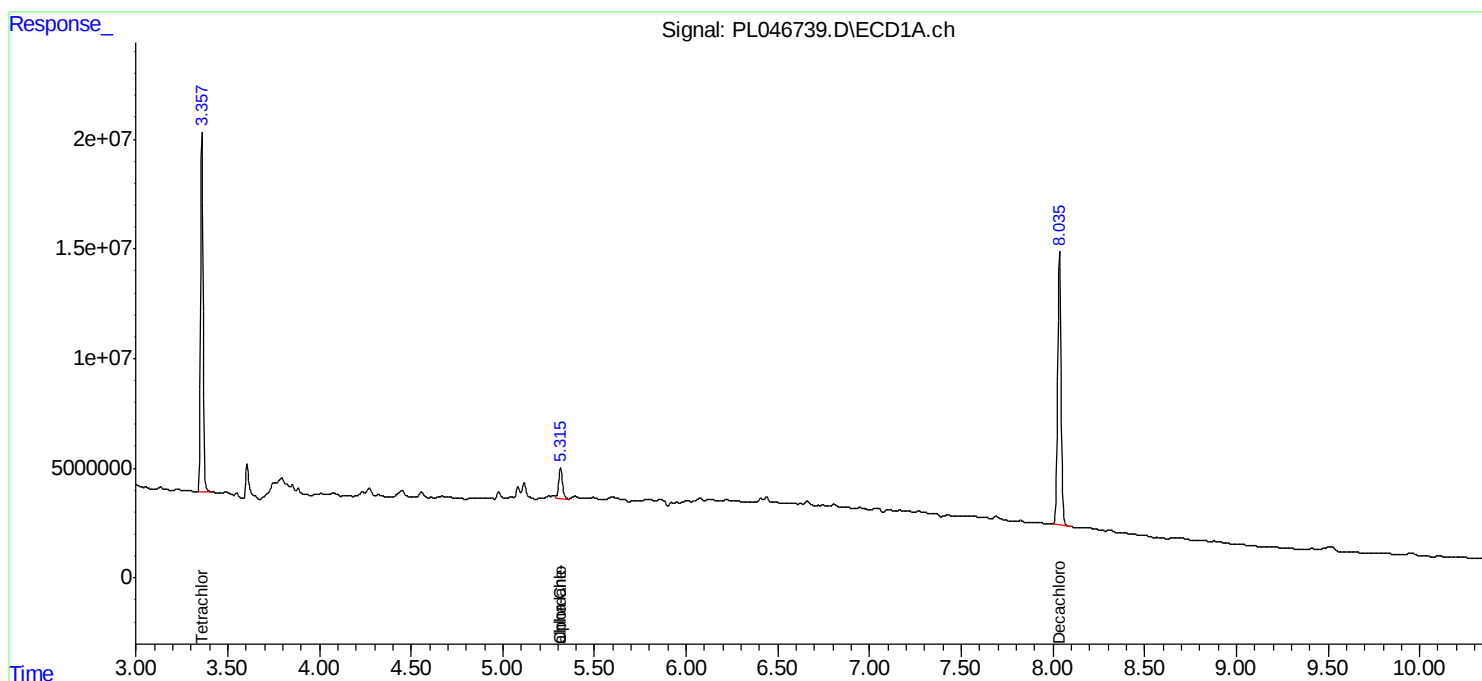


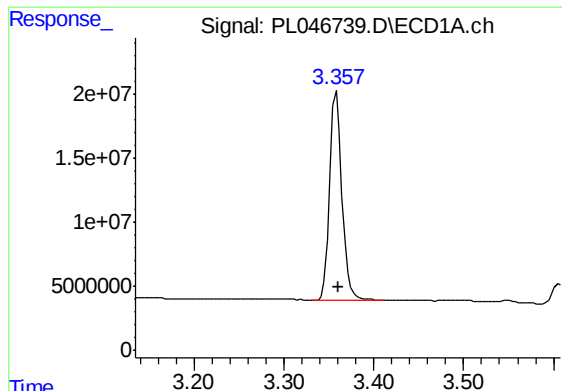

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 156392775
Conc: 21.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
S6B(2-10)COMP

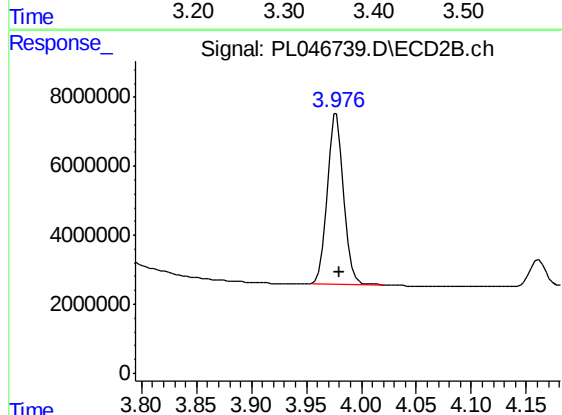


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.003 min
Response: 51512117
Conc: 22.50 ng/ml

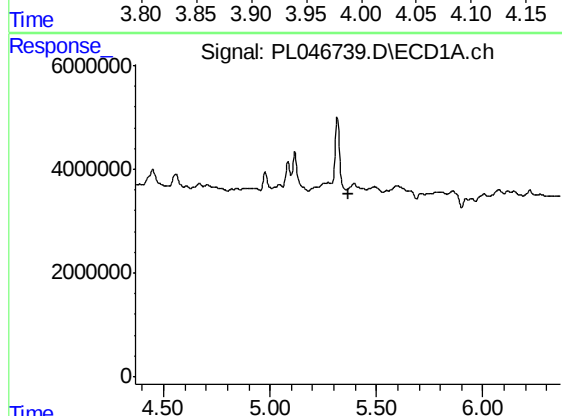


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.366 min
Response: 0
Conc: N.D.

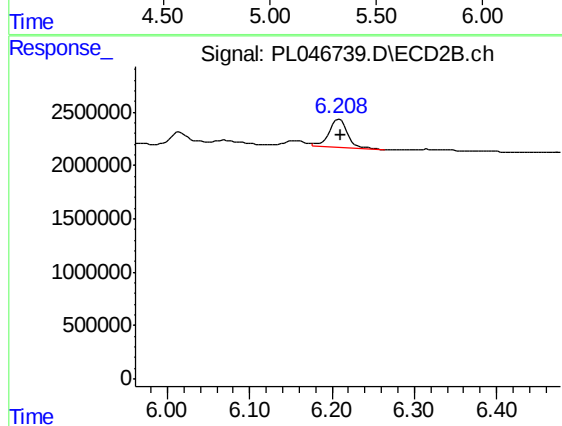

#9 Endosulfan I


R.T.: 6.209 min
Delta R.T.: -0.001 min
Response: 4181329
Conc: 1.60 ng/ml

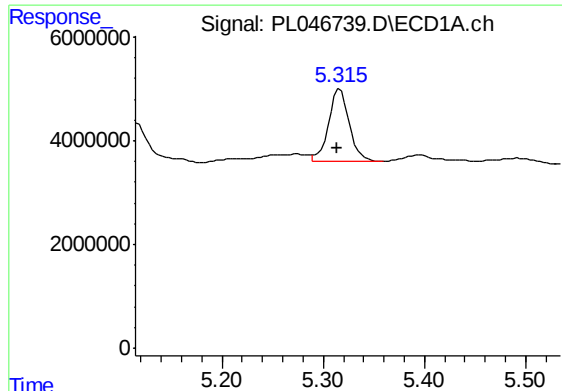

#11 alpha-Chlordane


R.T.: 5.317 min
Delta R.T.: 0.003 min
Response: 19710359
Conc: 1.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
S6B(2-10)COMP

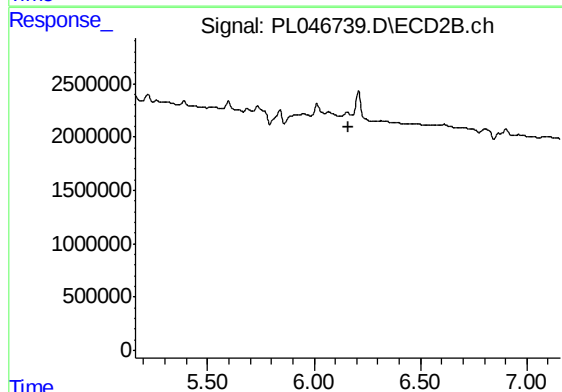


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.160 min
Response: 0
Conc: N.D.

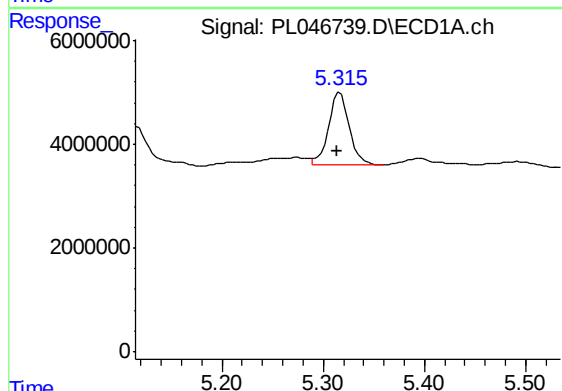


#26 Chlordane-4

R.T.: 5.317 min
Delta R.T.: 0.003 min
Response: 19710359
Conc: 19.06 ng/ml

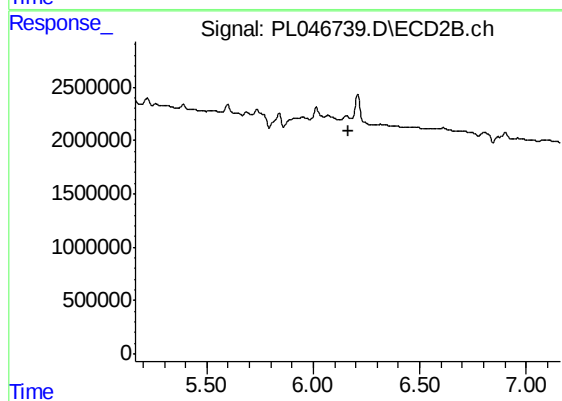

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.163 min
Response: 0
Conc: N.D.

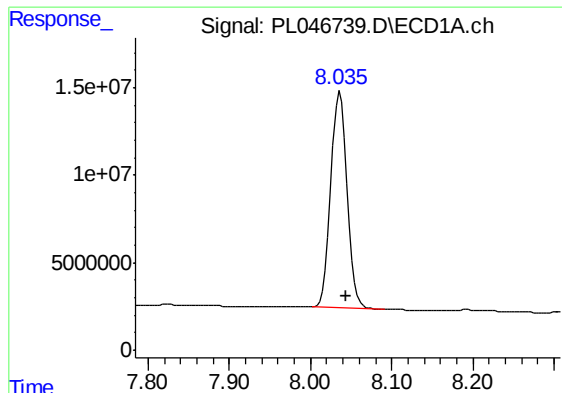

#28 Decachlorobiphenyl

R.T.: 8.036 min
Delta R.T.: -0.008 min
Response: 172529086
Conc: 20.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
S6B(2-10)COMP

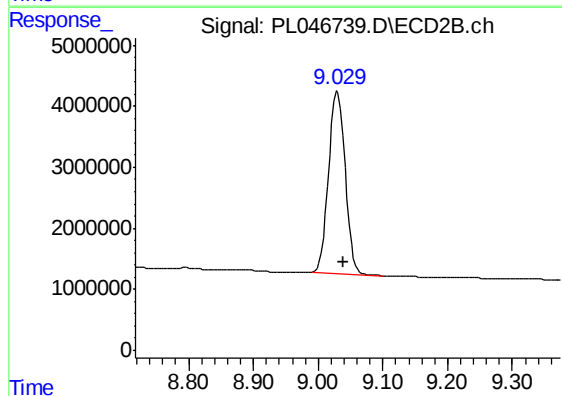

#28 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: -0.010 min
Response: 53036514
Conc: 22.88 ng/ml