

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032919\
 Data File : PL046745.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2019 18:57
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 23:18:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.358	3.977	131.3E6	43899930	18.051	19.174
28) SA Decachlor...	8.035	9.029	156.9E6	48045603	18.657	20.723
Target Compounds						
2) A alpha-BHC	3.795	0.000	10001481	0	0.858	N.D. #
8) B Heptachlo...	0.000	5.842	0	4002276	N.D.	1.518 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032919\
Data File : PL046745.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2019 18:57
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 23:18:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

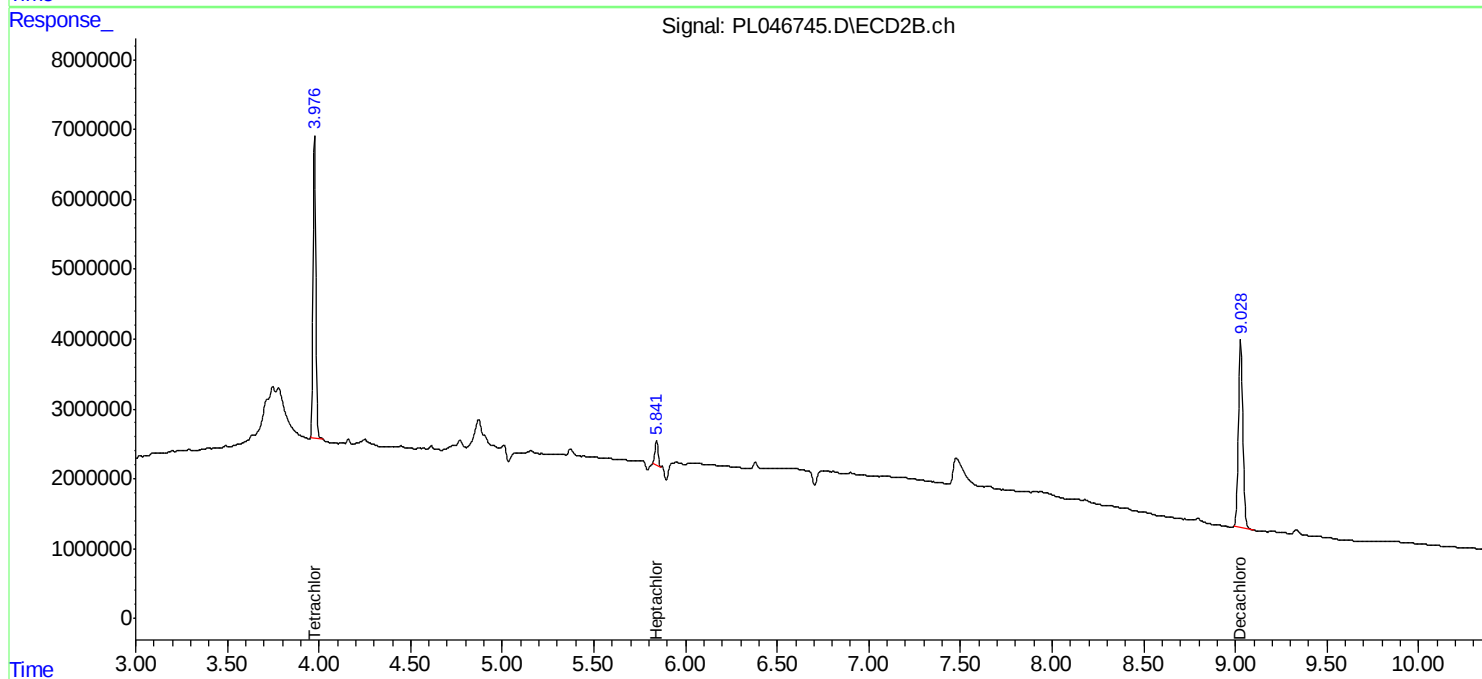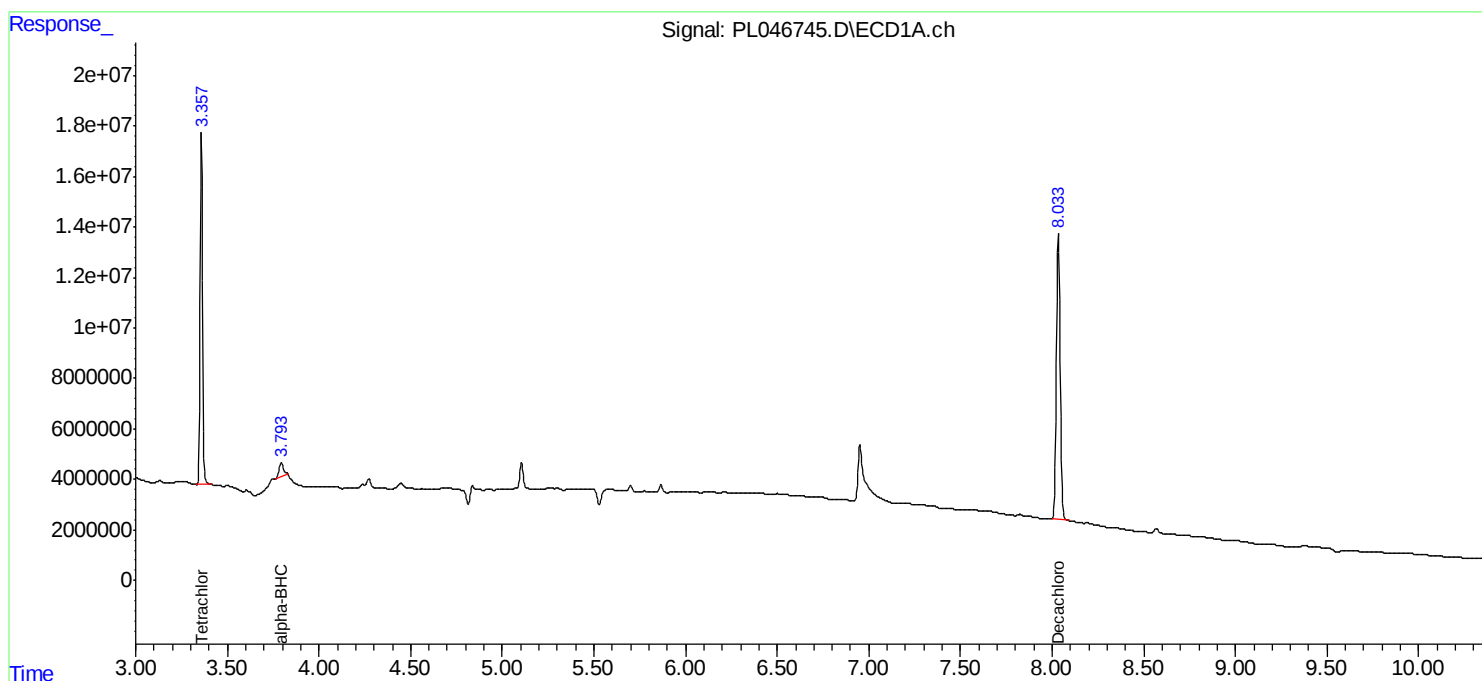


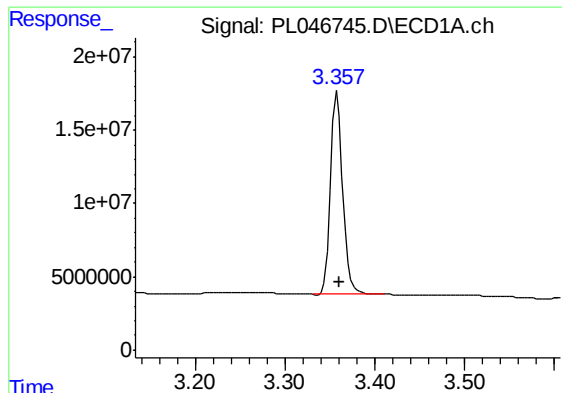

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 131311314
Conc: 18.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

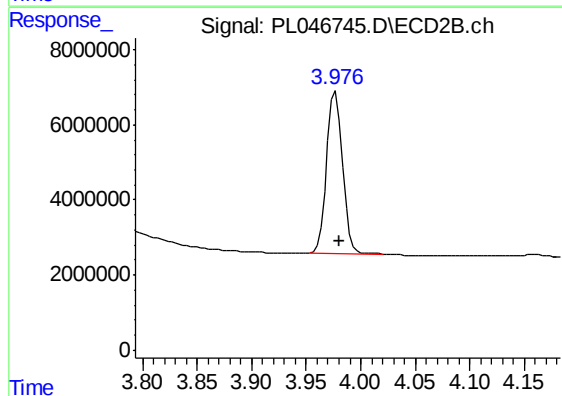


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.004 min
Response: 43899930
Conc: 19.17 ng/ml

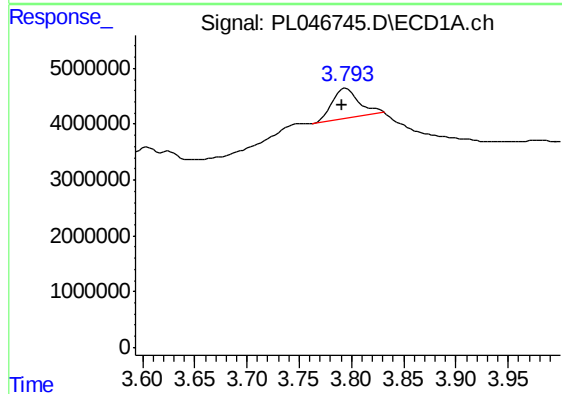


#2 alpha-BHC

R.T.: 3.795 min
Delta R.T.: 0.004 min
Response: 10001481
Conc: 0.86 ng/ml

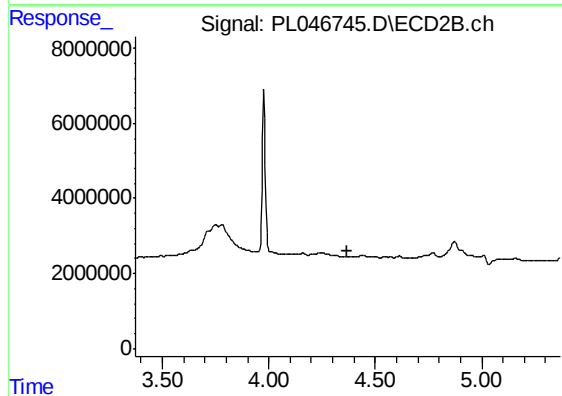

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.371 min
Response: 0
Conc: N.D.

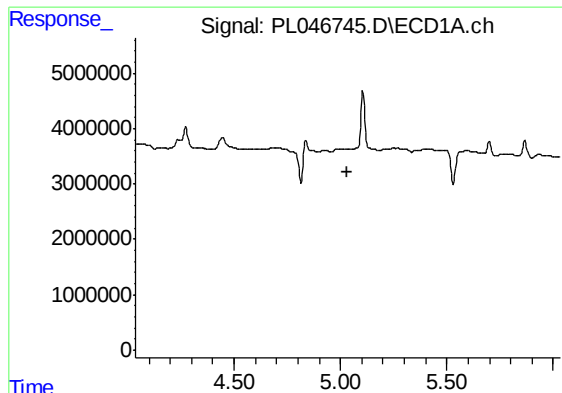

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.034 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

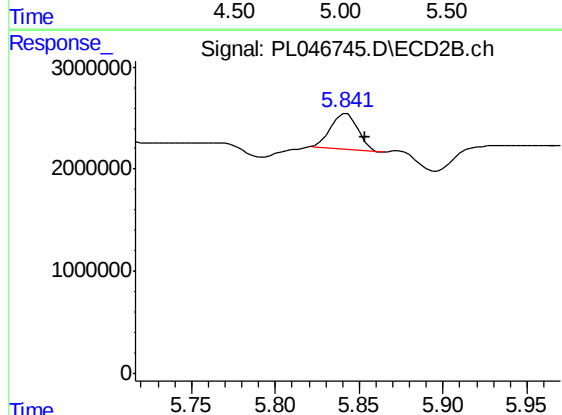


#8 Heptachlor epoxide

R.T.: 5.842 min
Delta R.T.: -0.011 min
Response: 4002276
Conc: 1.52 ng/ml

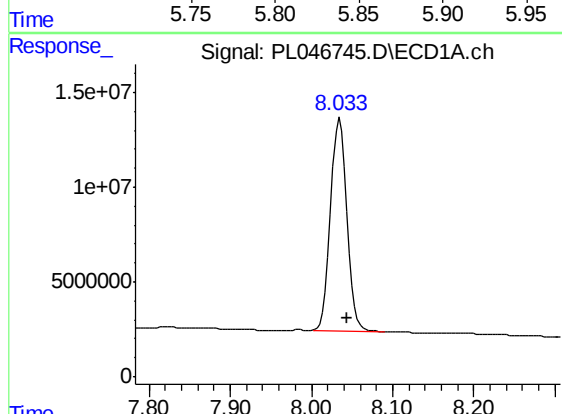

#28 Decachlorobiphenyl

R.T.: 8.035 min
Delta R.T.: -0.009 min
Response: 156927612
Conc: 18.66 ng/ml

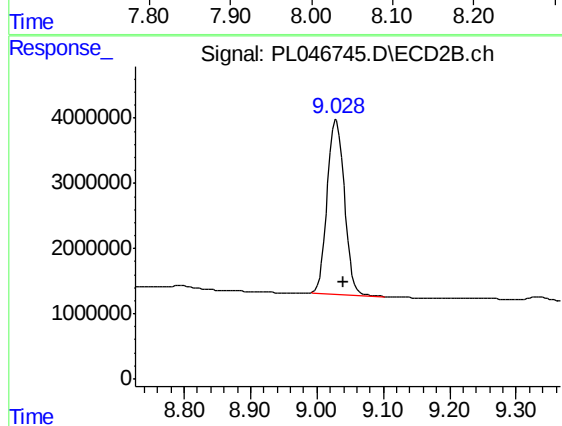

#28 Decachlorobiphenyl

R.T.: 9.029 min
Delta R.T.: -0.011 min
Response: 48045603
Conc: 20.72 ng/ml