

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032919\
 Data File : PL046777.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2019 02:37
 Operator : AJ\SJ
 Sample : K2124-04
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SAMPLE-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 03:17:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.977	151.4E6	49686022	20.818	21.701
28)	SA Decachlor...	8.034	9.028	160.6E6	47481029	19.091	20.479
Target Compounds							
6)	B beta-BHC	4.321	0.000	8655487	0	1.922	N.D. #
8)	B Heptachlo...	5.028	5.844	7201953	2888615	0.738	1.095 #
22)	Mirex	0.000	8.184f	0	1333473	N.D.	0.667 #
23)	Chlordane-1	4.203	4.968	5549136	1743190	16.501	16.108



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032919\
Data File : PL046777.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2019 02:37
Operator : AJ\SJ
Sample : K2124-04
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SAMPLE-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 03:17:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

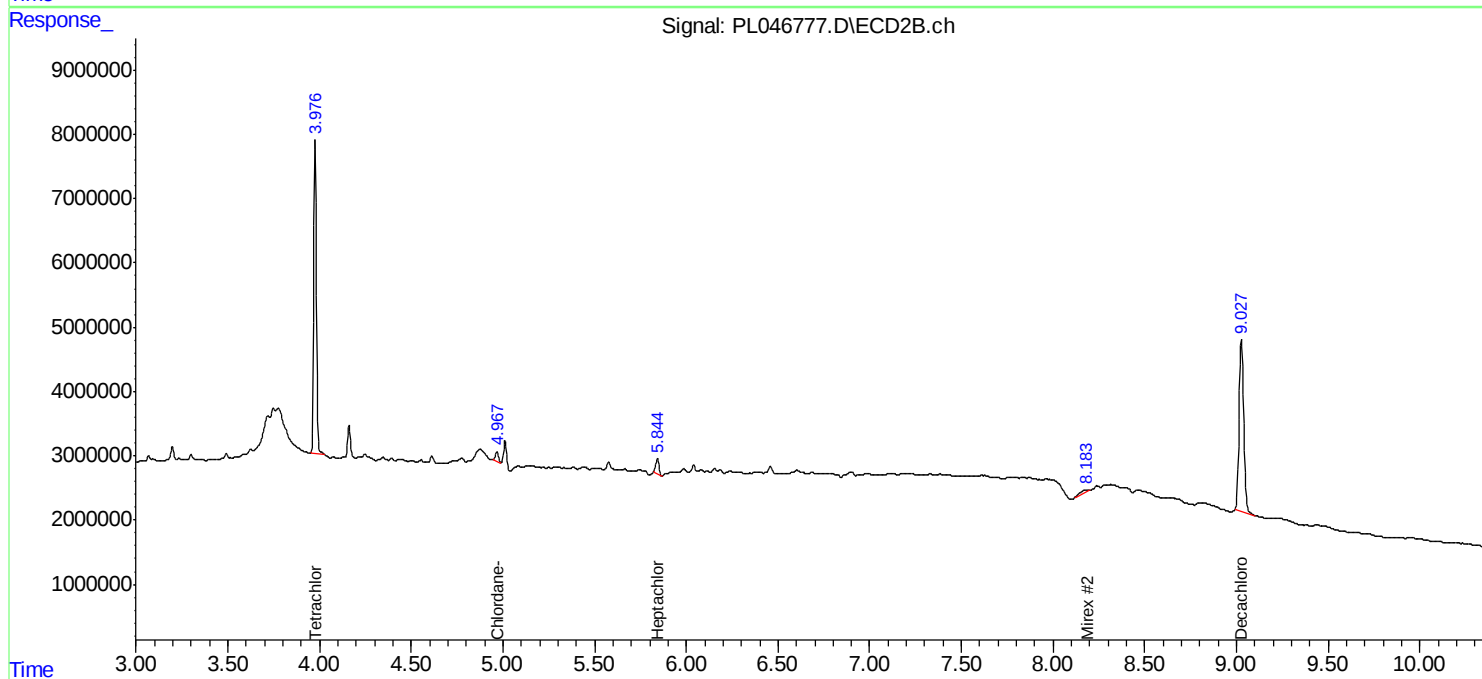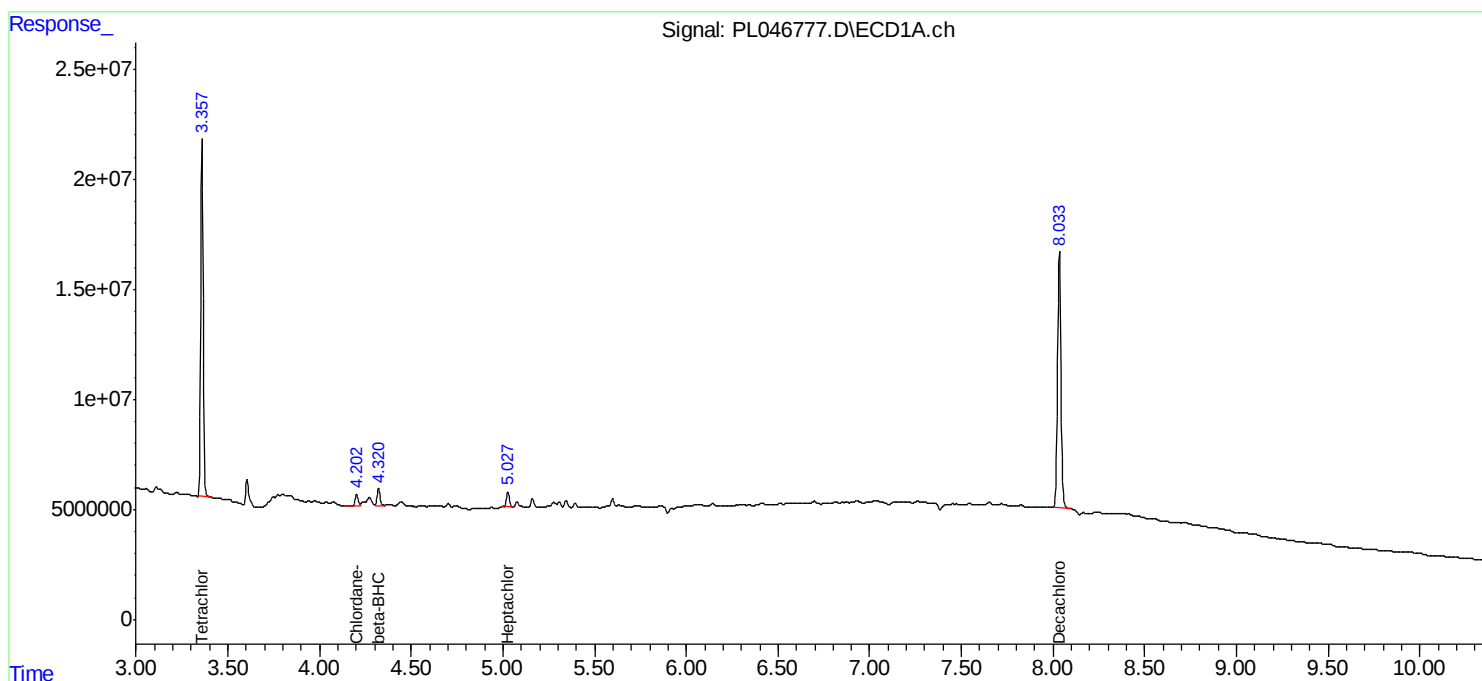


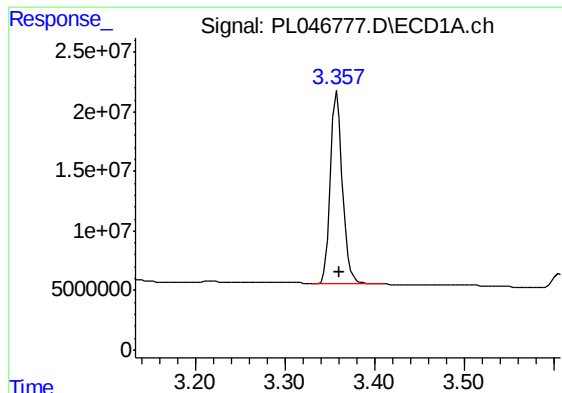

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 151446317
Conc: 20.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-2

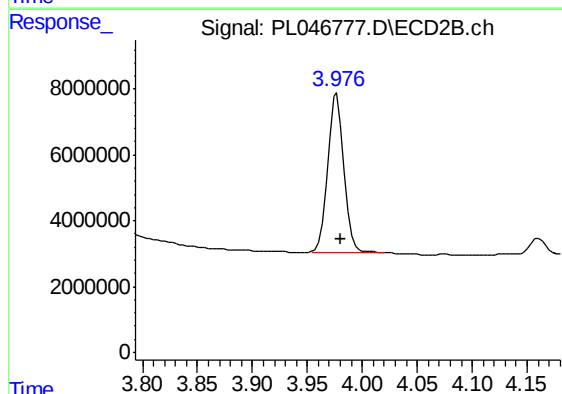


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.004 min
Response: 49686022
Conc: 21.70 ng/ml

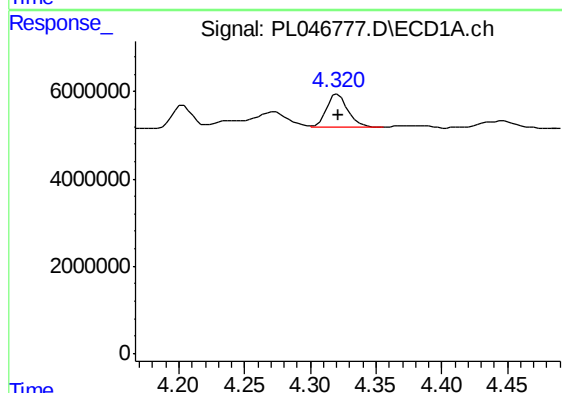


#6 beta-BHC

R.T.: 4.321 min
Delta R.T.: 0.000 min
Response: 8655487
Conc: 1.92 ng/ml

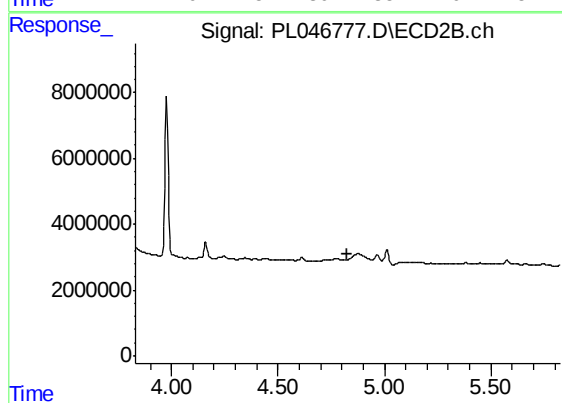

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.828 min
Response: 0
Conc: N.D.

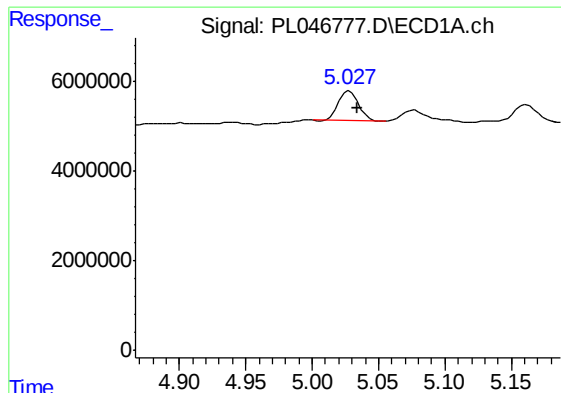

#8 Heptachlor epoxide


R.T.: 5.028 min
Delta R.T.: -0.006 min
Response: 7201953
Conc: 0.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-2

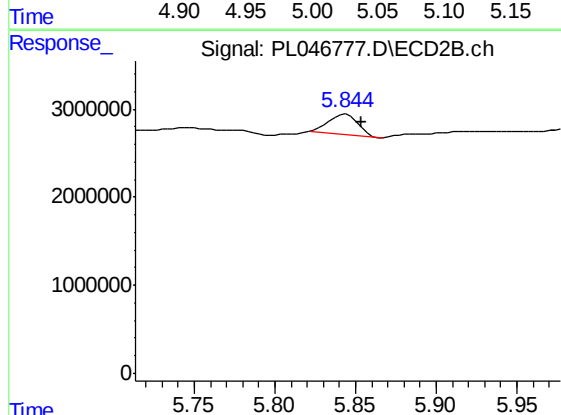


#8 Heptachlor epoxide

R.T.: 5.844 min
Delta R.T.: -0.009 min
Response: 2888615
Conc: 1.10 ng/ml

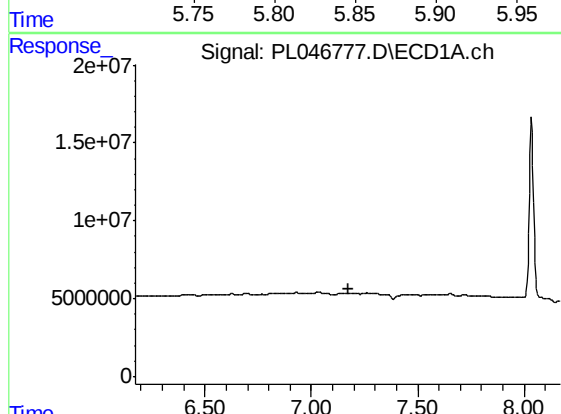


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.173 min
Response: 0
Conc: N.D.

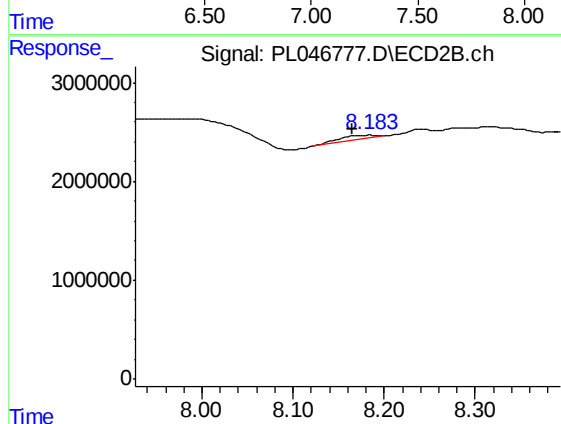

#22 Mirex


R.T.: 8.184 min
Delta R.T.: 0.020 min
Response: 1333473
Conc: 0.67 ng/ml

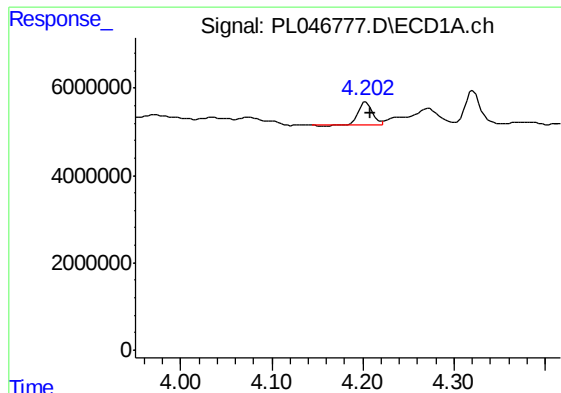

#23 Chlordane-1


R.T.: 4.203 min
Delta R.T.: -0.005 min
Response: 5549136
Conc: 16.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-2

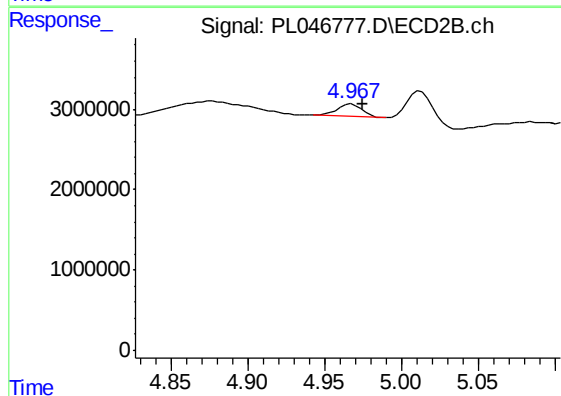


#23 Chlordane-1

R.T.: 4.968 min
Delta R.T.: -0.007 min
Response: 1743190
Conc: 16.11 ng/ml

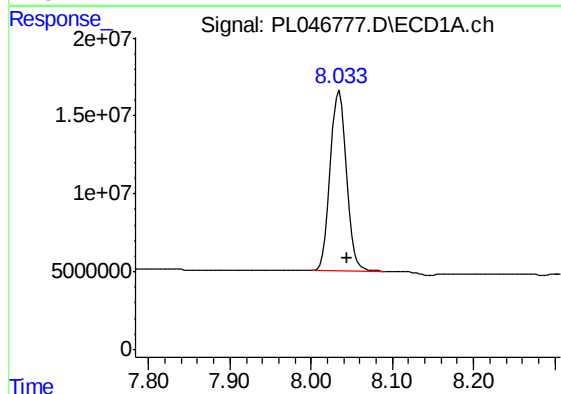

#28 Decachlorobiphenyl

R.T.: 8.034 min
Delta R.T.: -0.010 min
Response: 160579510
Conc: 19.09 ng/ml

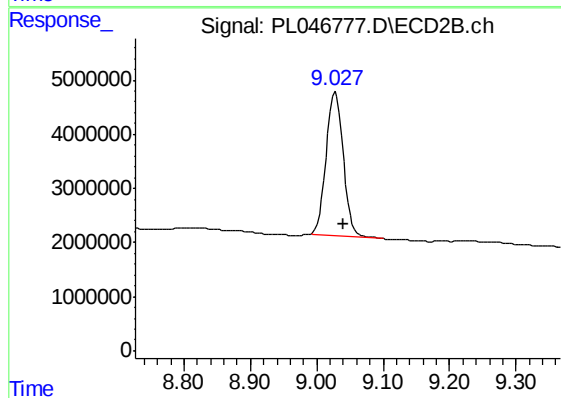

#28 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: -0.012 min
Response: 47481029
Conc: 20.48 ng/ml