

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032921\
 Data File : PL065626.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2021 10:21
 Operator : AR\AJ
 Sample : PB135377BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 12:32:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.283	3.783	46218652	48678066	19.462	17.735
28)	SA Decachlor...	7.920	8.732	42179327	38306391	17.458	19.326
Target Compounds							
4)	MA Heptachlor	0.000	4.948	0	498164	N.D.	0.149 #
5)	MB Aldrin	0.000	5.249	0	156371	N.D.	0.048 #
6)	B beta-BHC	0.000	4.635	0	4235506	N.D.	2.459 #
8)	B Heptachlo...	0.000	5.641f	0	329736	N.D.	0.114 #
15)	B Endosulfa...	0.000	6.681f	0	812063	N.D.	0.360 #
19)	B Endosulfa...	6.430f	0.000	341615	0	0.138	N.D. #
23)	Chlordane-1	4.148f	4.769	49072	385860	0.570	3.421 #
24)	Chlordane-2	0.000	5.221	0	363705	N.D.	3.339 #
27)	Chlordane-5	0.000	6.714	0	74787	N.D.	0.935 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032921\
Data File : PL065626.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2021 10:21
Operator : AR\AJ
Sample : PB135377BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 12:32:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

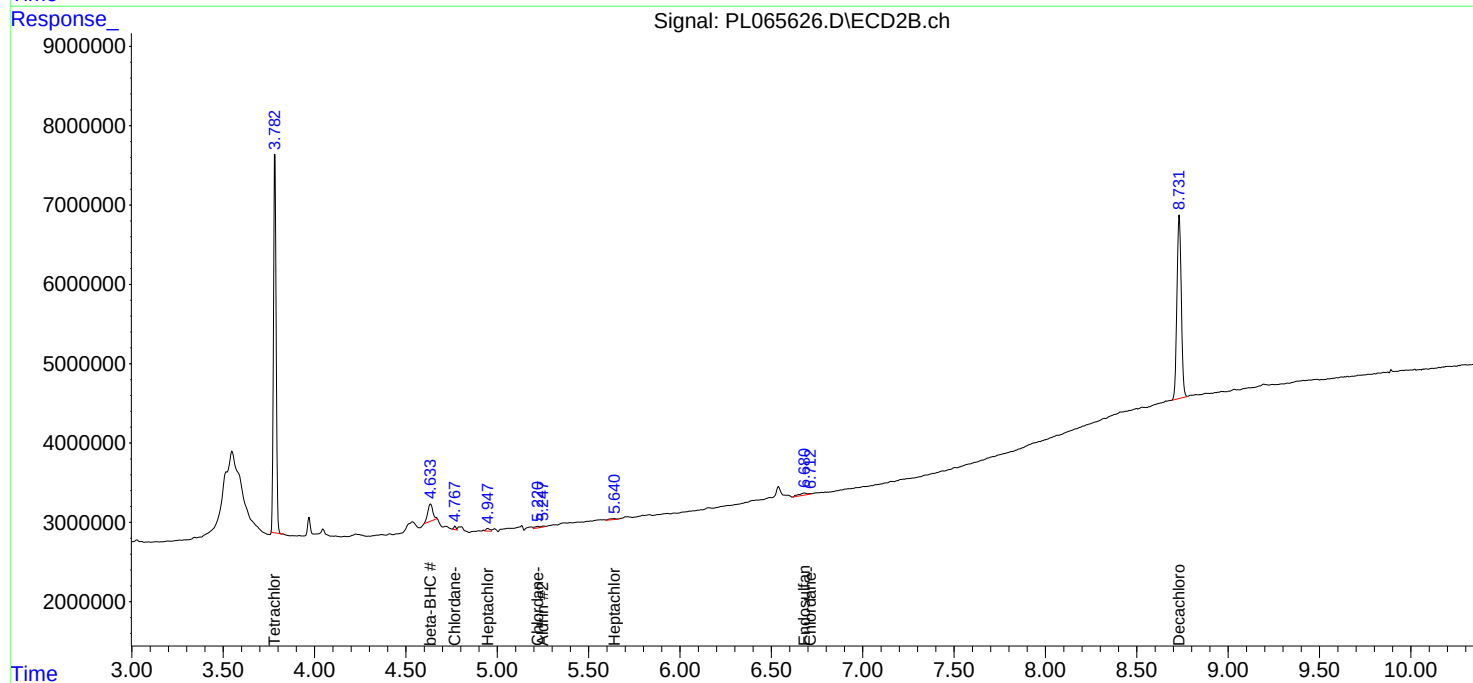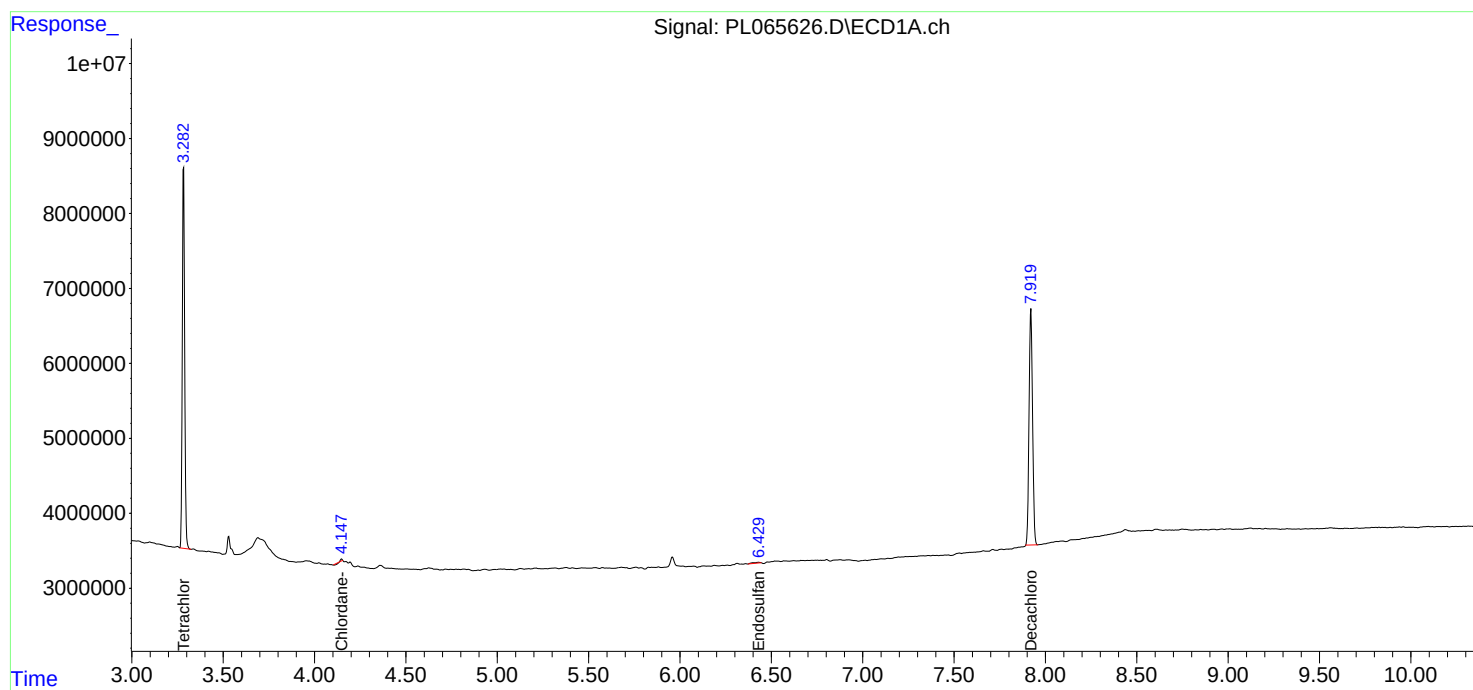


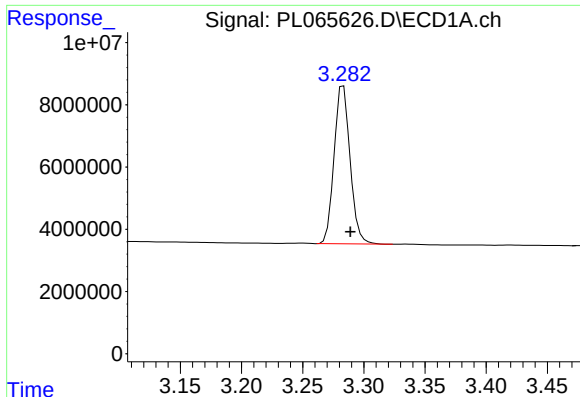

#1 Tetrachloro-m-xylene


R.T.: 3.283 min
Delta R.T.: -0.006 min
Response: 46218652
Conc: 19.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

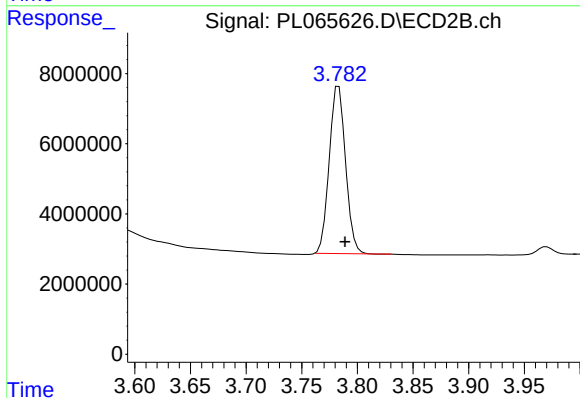


#1 Tetrachloro-m-xylene

R.T.: 3.783 min
Delta R.T.: -0.006 min
Response: 48678066
Conc: 17.74 ng/ml

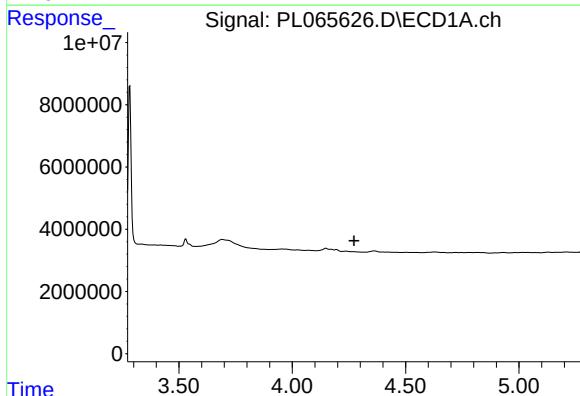


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.274 min
Response: 0
Conc: N.D.

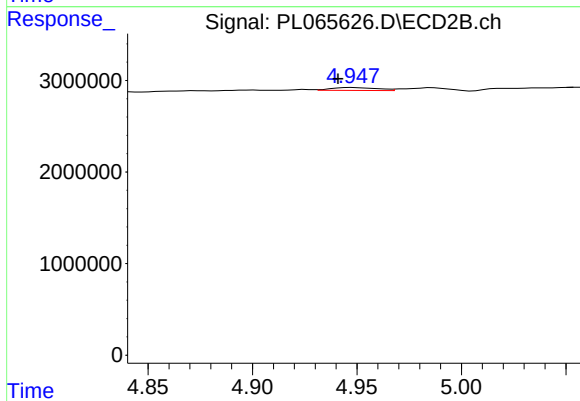

#4 Heptachlor


R.T.: 4.948 min
Delta R.T.: 0.007 min
Response: 498164
Conc: 0.15 ng/ml

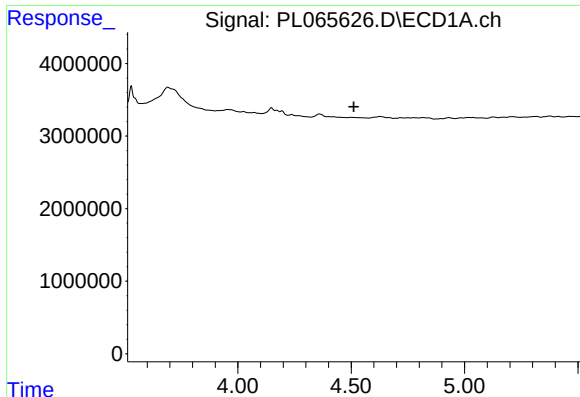

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

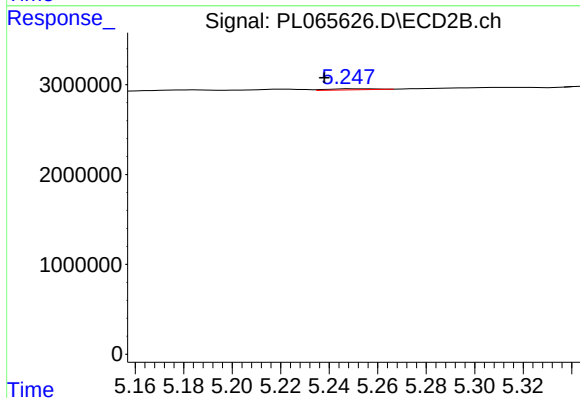


#5 Aldrin

R.T.: 5.249 min
Delta R.T.: 0.012 min
Response: 156371
Conc: 0.05 ng/ml

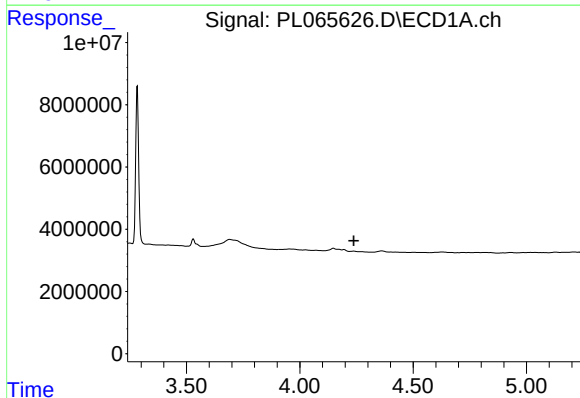


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.238 min
Response: 0
Conc: N.D.

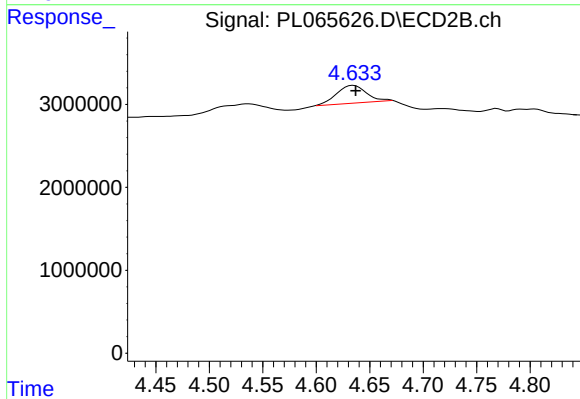

#6 beta-BHC


R.T.: 4.635 min
Delta R.T.: -0.002 min
Response: 4235506
Conc: 2.46 ng/ml

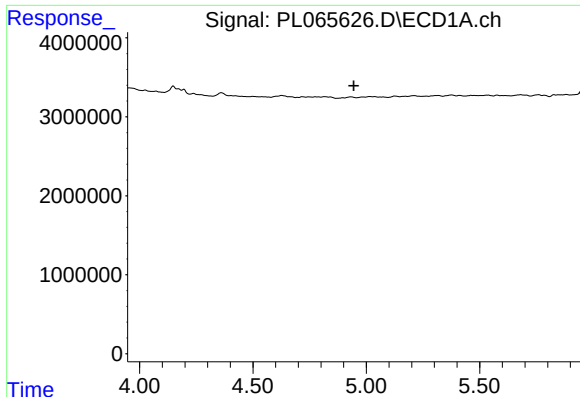

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.944 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

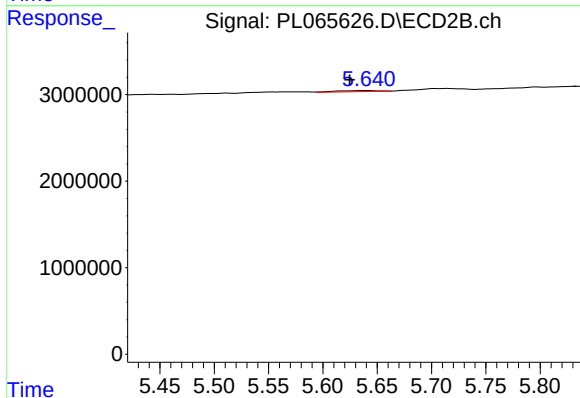


#8 Heptachlor epoxide

R.T.: 5.641 min
Delta R.T.: 0.016 min
Response: 329736
Conc: 0.11 ng/ml

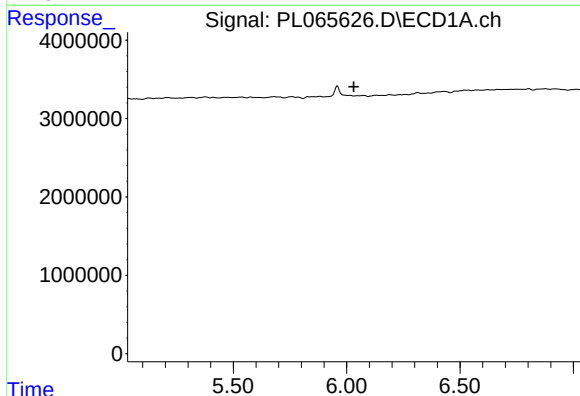


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.031 min
Response: 0
Conc: N.D.

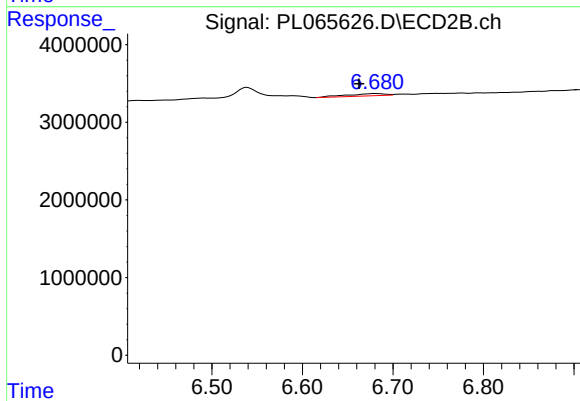

#15 Endosulfan II


R.T.: 6.681 min
Delta R.T.: 0.019 min
Response: 812063
Conc: 0.36 ng/ml

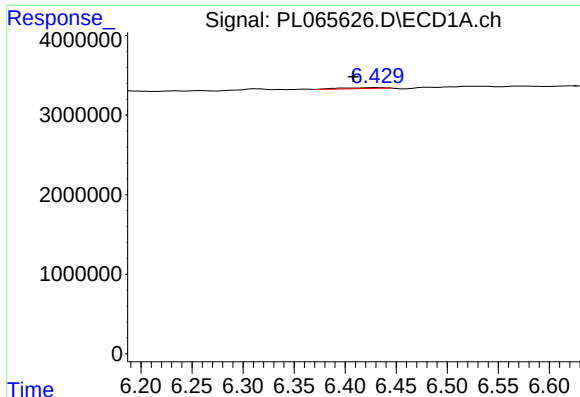

#19 Endosulfan Sulfate


R.T.: 6.430 min
Delta R.T.: 0.022 min
Response: 341615
Conc: 0.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

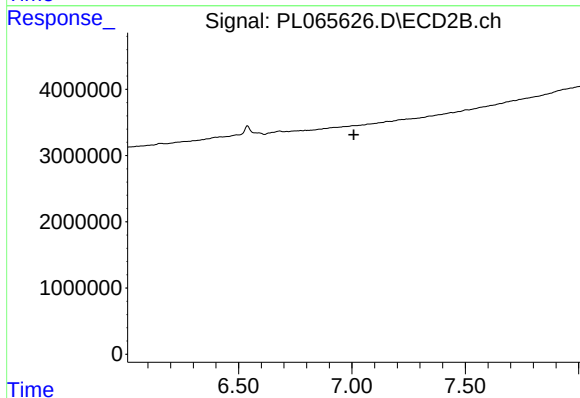


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.009 min
Response: 0
Conc: N.D.

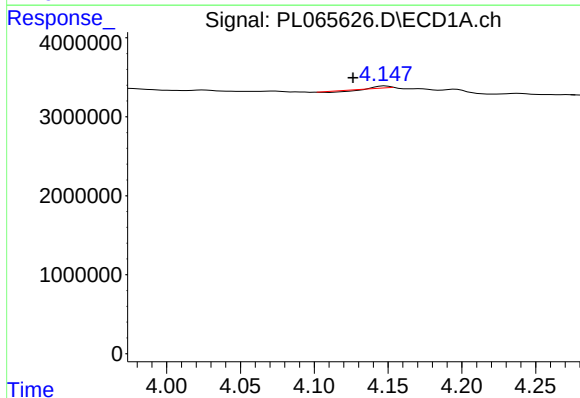


#23 Chlordane-1

R.T.: 4.148 min
Delta R.T.: 0.022 min
Response: 49072
Conc: 0.57 ng/ml

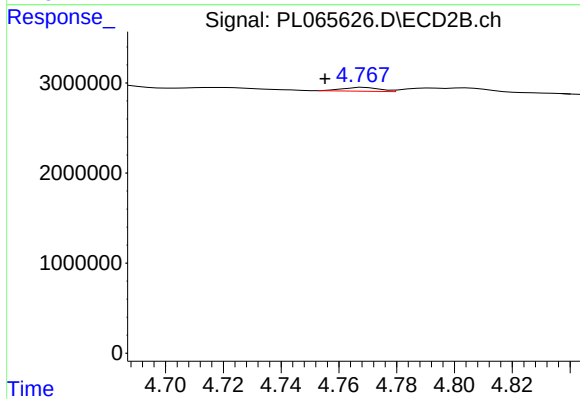

#23 Chlordane-1


R.T.: 4.769 min
Delta R.T.: 0.014 min
Response: 385860
Conc: 3.42 ng/ml

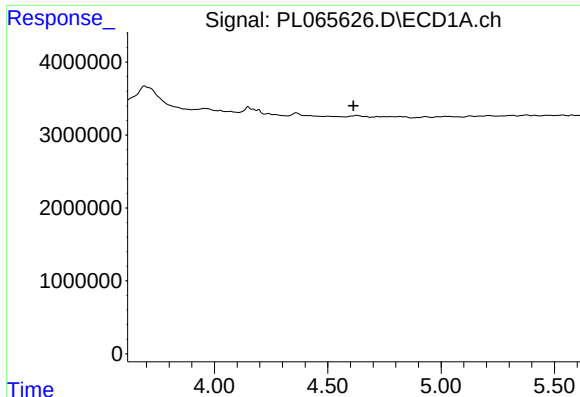

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.614 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

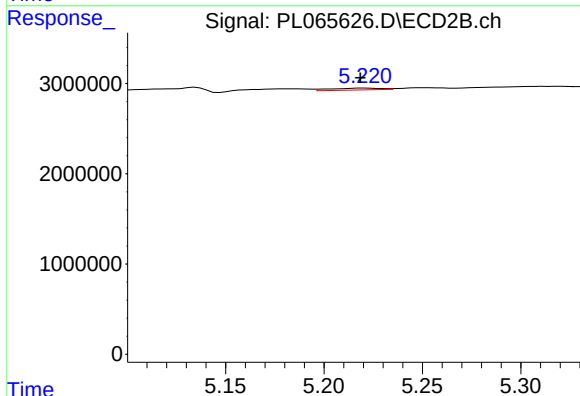


#24 Chlordane-2

R.T.: 5.221 min
Delta R.T.: 0.003 min
Response: 363705
Conc: 3.34 ng/ml

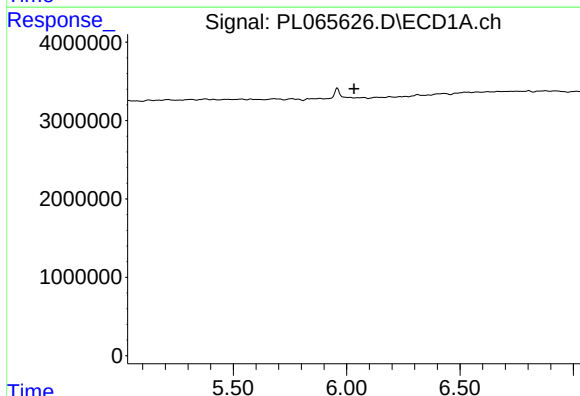


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.033 min
Response: 0
Conc: N.D.

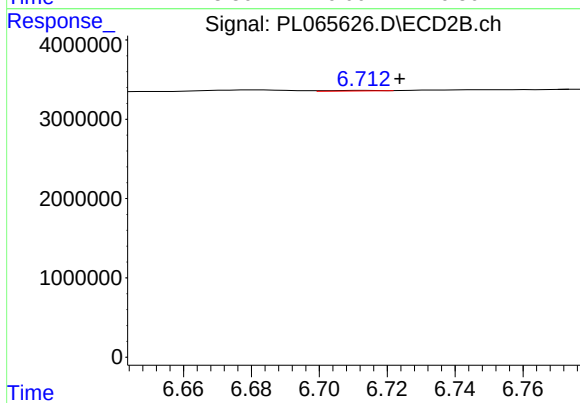

#27 Chlordane-5


R.T.: 6.714 min
Delta R.T.: -0.010 min
Response: 74787
Conc: 0.93 ng/ml

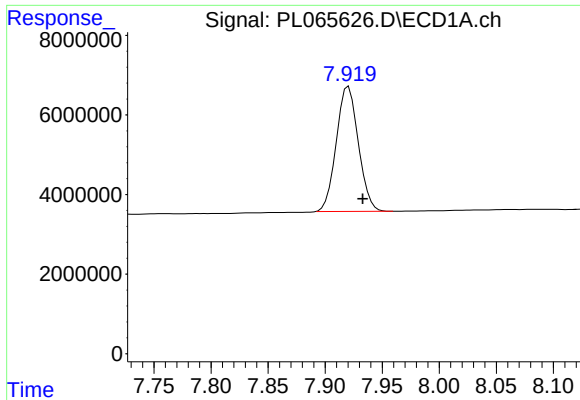

#28 Decachlorobiphenyl

R.T.: 7.920 min
Delta R.T.: -0.012 min
Response: 42179327
Conc: 17.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

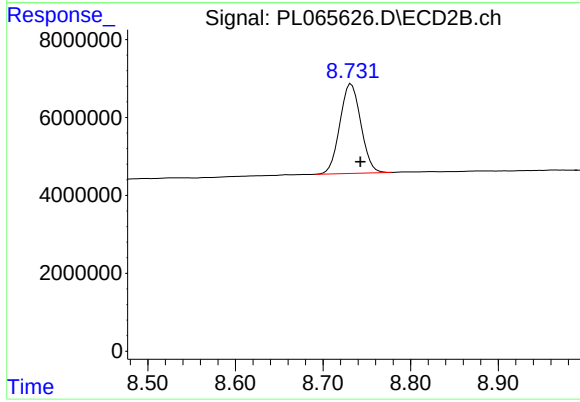

#28 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: -0.011 min
Response: 38306391
Conc: 19.33 ng/ml