

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032921\
 Data File : PL065630.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2021 11:18
 Operator : AR\AJ
 Sample : PB135379BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 12:33:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.283	3.783	44622836	47467557	18.790	17.294
28)	SA Decachlor...	7.919	8.732	41365413	37766678	17.121	19.054
Target Compounds							
4)	MA Heptachlor	0.000	4.944	0	677524	N.D.	0.203 #
6)	B beta-BHC	0.000	4.634	0	3412069	N.D.	1.981 #
9)	A Endosulfan I	0.000	5.978	0	28711	N.D.	0.011 #
11)	B alpha-Chl...	0.000	5.927	0	142892	N.D.	0.051 #
15)	B Endosulfa...	0.000	6.690f	0	204457	N.D.	0.091 #
21)	B Endrin ke...	0.000	7.501f	0	1441663	N.D.	0.611 #
23)	Chlordane-1	4.146f	0.000	173774	0	2.017	N.D. #
24)	Chlordane-2	4.629f	0.000	1141970	0	10.529	N.D. #
26)	Chlordane-4	0.000	5.927	0	142892	N.D.	0.297 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032921\
Data File : PL065630.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2021 11:18
Operator : AR\AJ
Sample : PB135379BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 12:33:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

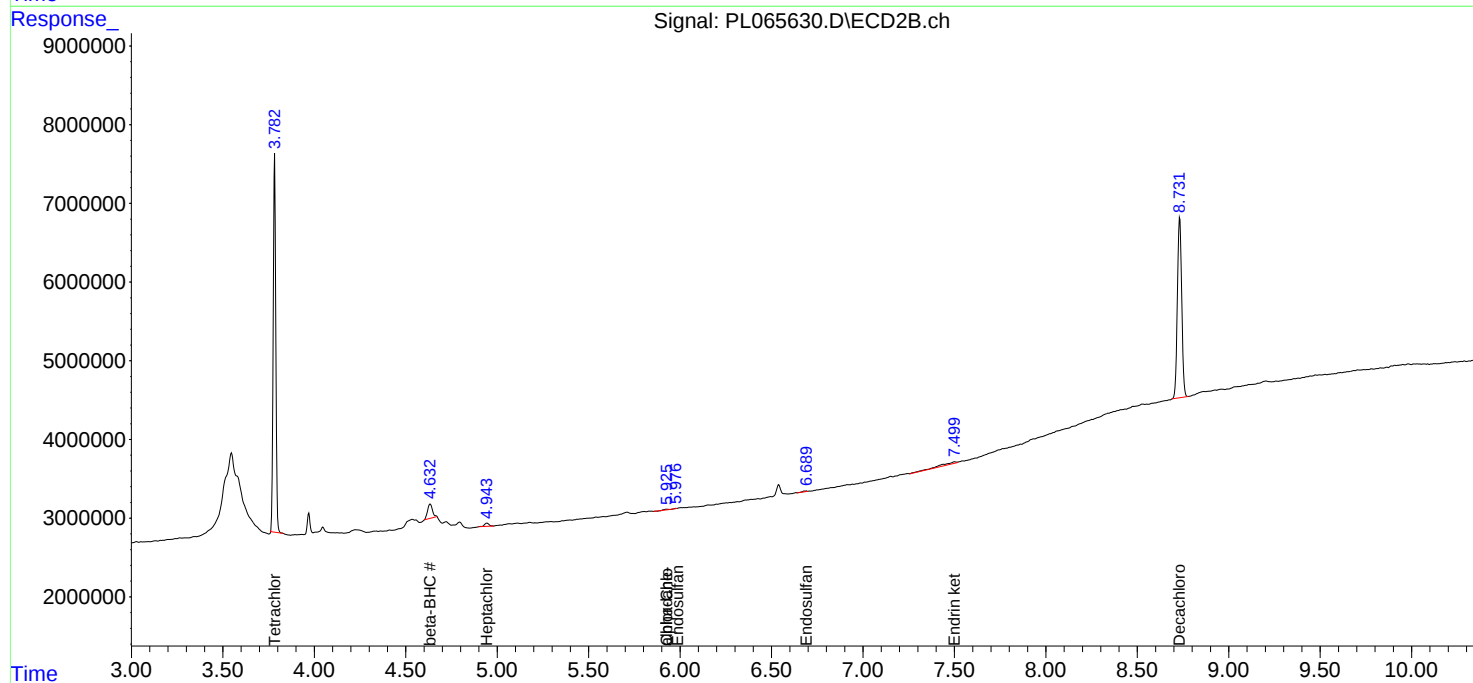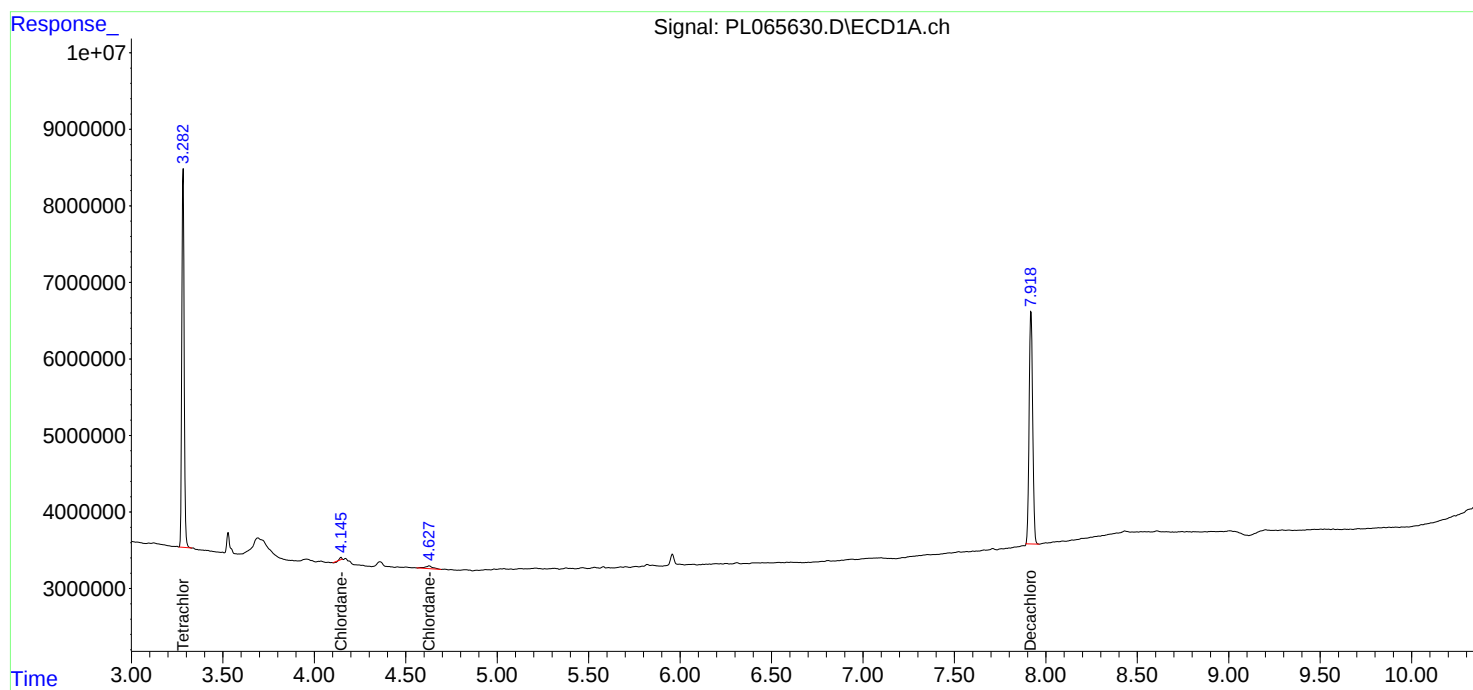


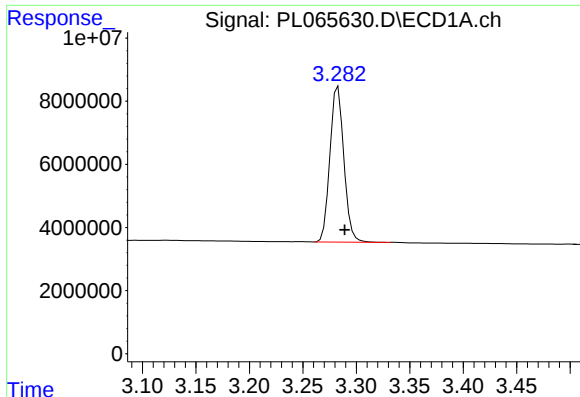

#1 Tetrachloro-m-xylene


R.T.: 3.283 min
Delta R.T.: -0.006 min
Response: 44622836
Conc: 18.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

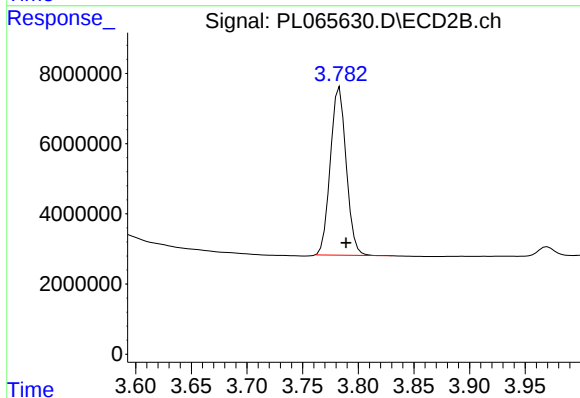


#1 Tetrachloro-m-xylene

R.T.: 3.783 min
Delta R.T.: -0.006 min
Response: 47467557
Conc: 17.29 ng/ml

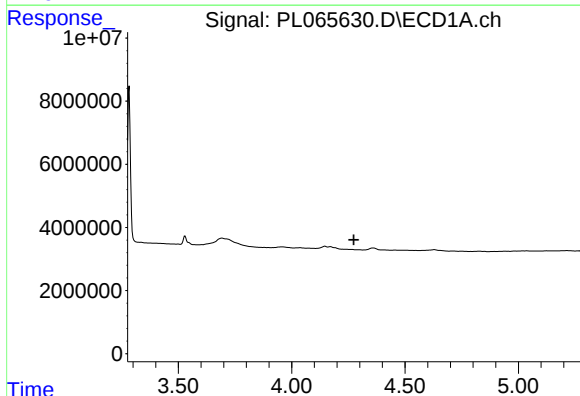


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.274 min
Response: 0
Conc: N.D.

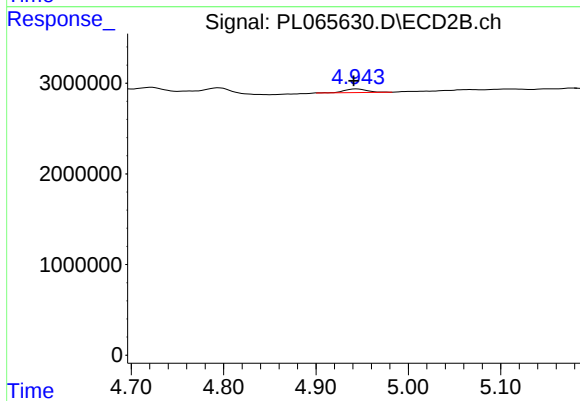

#4 Heptachlor

R.T.: 4.944 min
Delta R.T.: 0.003 min
Response: 677524
Conc: 0.20 ng/ml

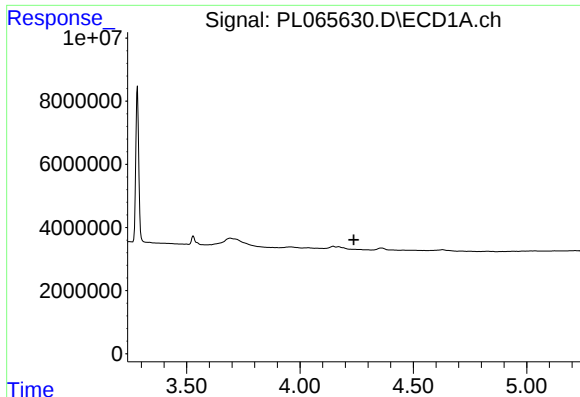

#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.238 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#6 beta-BHC


R.T.: 4.634 min
Delta R.T.: -0.003 min
Response: 3412069
Conc: 1.98 ng/ml

#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.271 min
Response: 0
Conc: N.D.

#9 Endosulfan I


R.T.: 5.978 min
Delta R.T.: 0.003 min
Response: 28711
Conc: 0.01 ng/ml

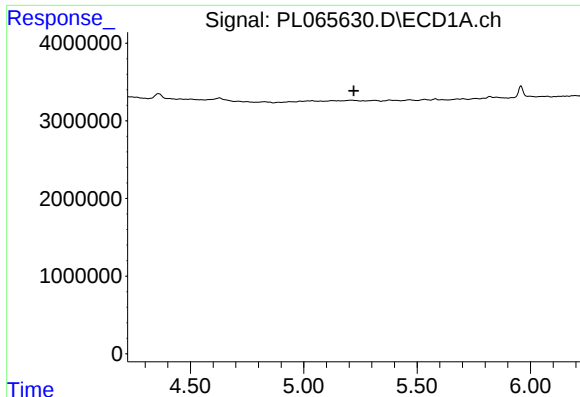

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

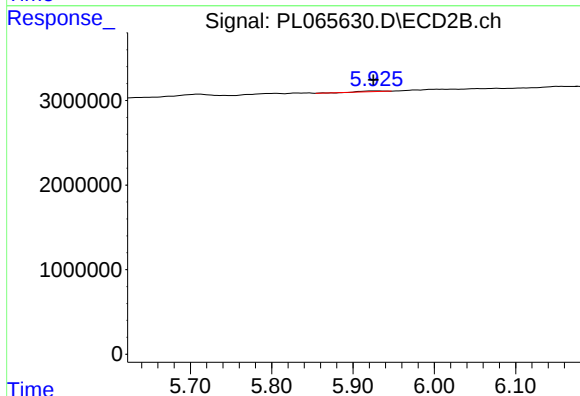


#11 alpha-Chlordane

R.T.: 5.927 min
Delta R.T.: 0.002 min
Response: 142892
Conc: 0.05 ng/ml

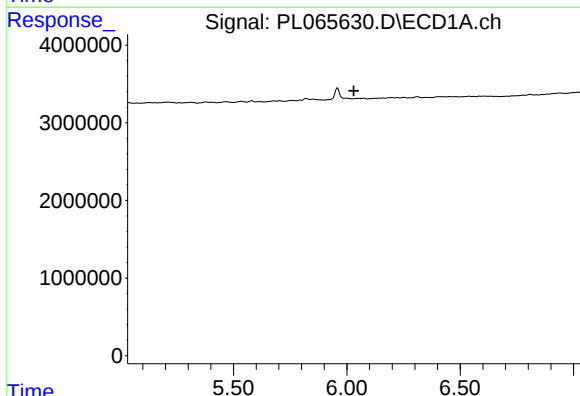


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.031 min
Response: 0
Conc: N.D.

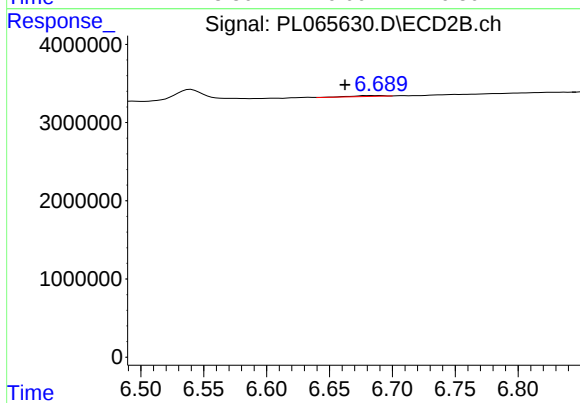

#15 Endosulfan II


R.T.: 6.690 min
Delta R.T.: 0.027 min
Response: 204457
Conc: 0.09 ng/ml

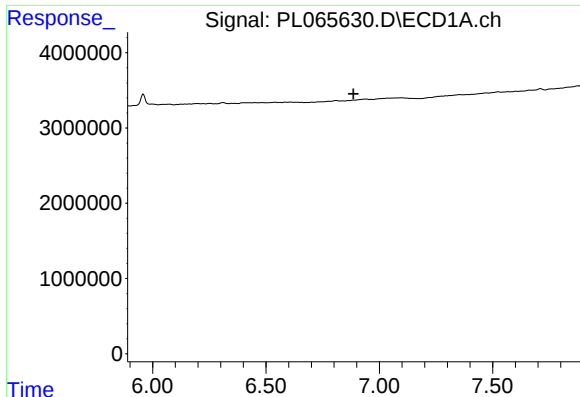

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.886 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

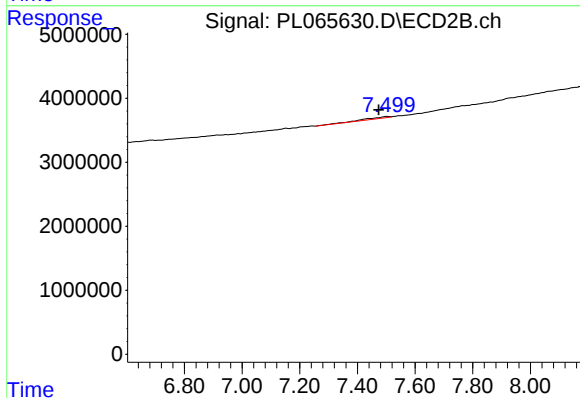


#21 Endrin ketone

R.T.: 7.501 min
Delta R.T.: 0.027 min
Response: 1441663
Conc: 0.61 ng/ml

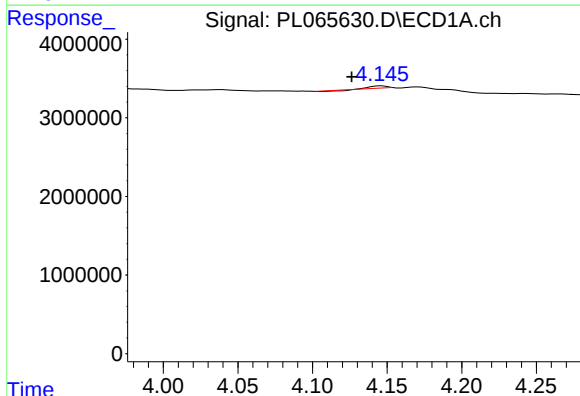


#23 Chlordane-1

R.T.: 4.146 min
Delta R.T.: 0.020 min
Response: 173774
Conc: 2.02 ng/ml

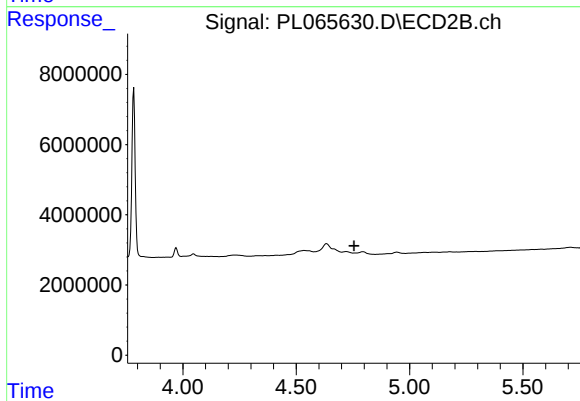

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.755 min
Response: 0
Conc: N.D.

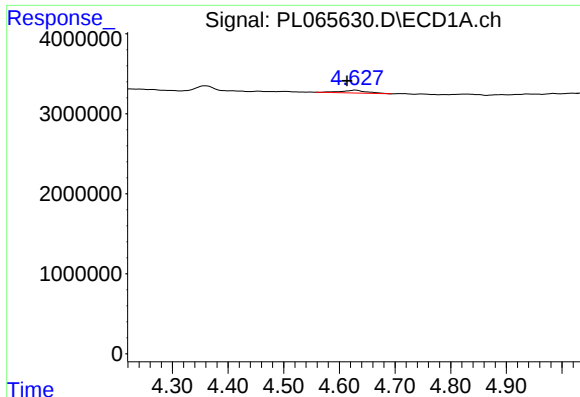

#24 Chlordane-2


R.T.: 4.629 min
Delta R.T.: 0.015 min
Response: 1141970
Conc: 10.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

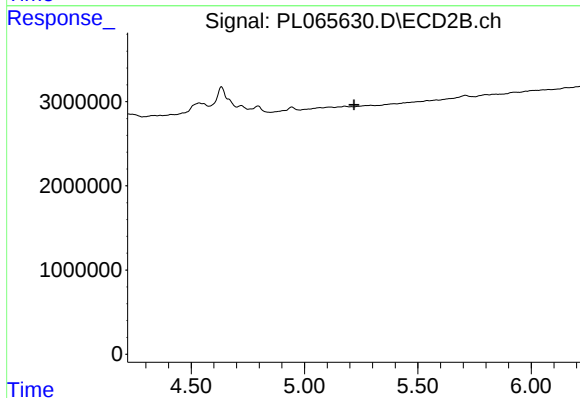


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.219 min
Response: 0
Conc: N.D.

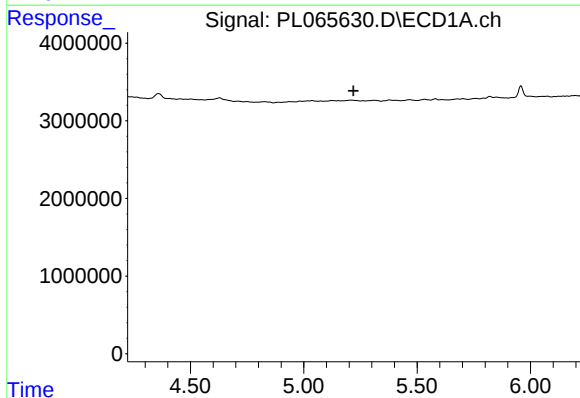


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.220 min
Response: 0
Conc: N.D.

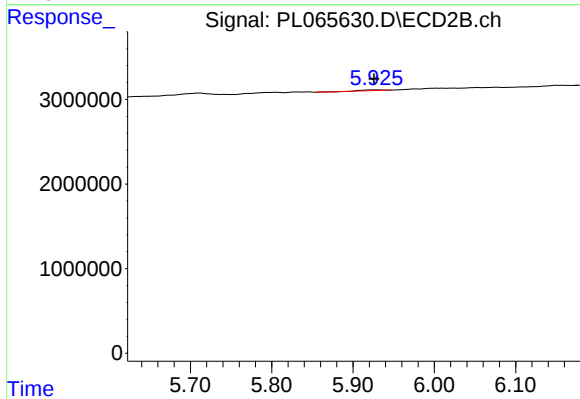

#26 Chlordane-4


R.T.: 5.927 min
Delta R.T.: 0.000 min
Response: 142892
Conc: 0.30 ng/ml

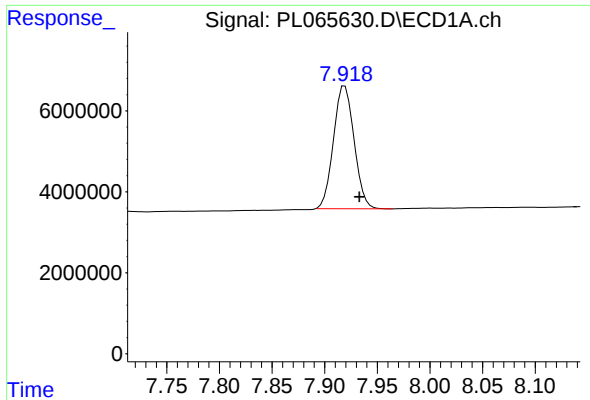

#28 Decachlorobiphenyl

R.T.: 7.919 min
Delta R.T.: -0.014 min
Response: 41365413
Conc: 17.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

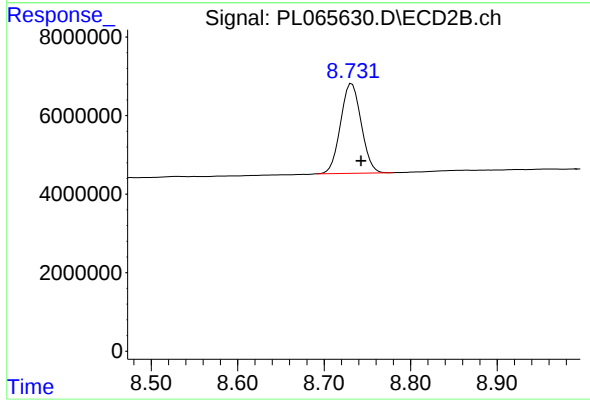

#28 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: -0.011 min
Response: 37766678
Conc: 19.05 ng/ml