

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032921\
 Data File : PL065639.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2021 14:26
 Operator : AR\AJ
 Sample : M1796-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 17:27:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.283	3.783	39937921	42048162	16.817	15.320
28)	SA Decachlor...	7.920	8.732	37181124	34359374	15.389	17.335
Target Compounds							
4)	MA Heptachlor	0.000	4.940	0	1058760	N.D.	0.318 #
6)	B beta-BHC	0.000	4.626	0	1331655	N.D.	0.773 #
8)	B Heptachlo...	0.000	5.619	0	3351405	N.D.	1.159 #
9)	A Endosulfan I	0.000	5.997f	0	608028	N.D.	0.231 #
15)	B Endosulfa...	0.000	6.679f	0	920768	N.D.	0.408 #
17)	MA 4,4'-DDT	0.000	6.874	0	347730	N.D.	0.177 #
19)	B Endosulfa...	6.419	0.000	444766	0	0.180	N.D. #
20)	A Methoxychlor	0.000	7.334	0	903423	N.D.	0.865 #
24)	Chlordane-2	4.627	0.000	1127438	0	10.395	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032921\
Data File : PL065639.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2021 14:26
Operator : AR\AJ
Sample : M1796-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 17:27:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

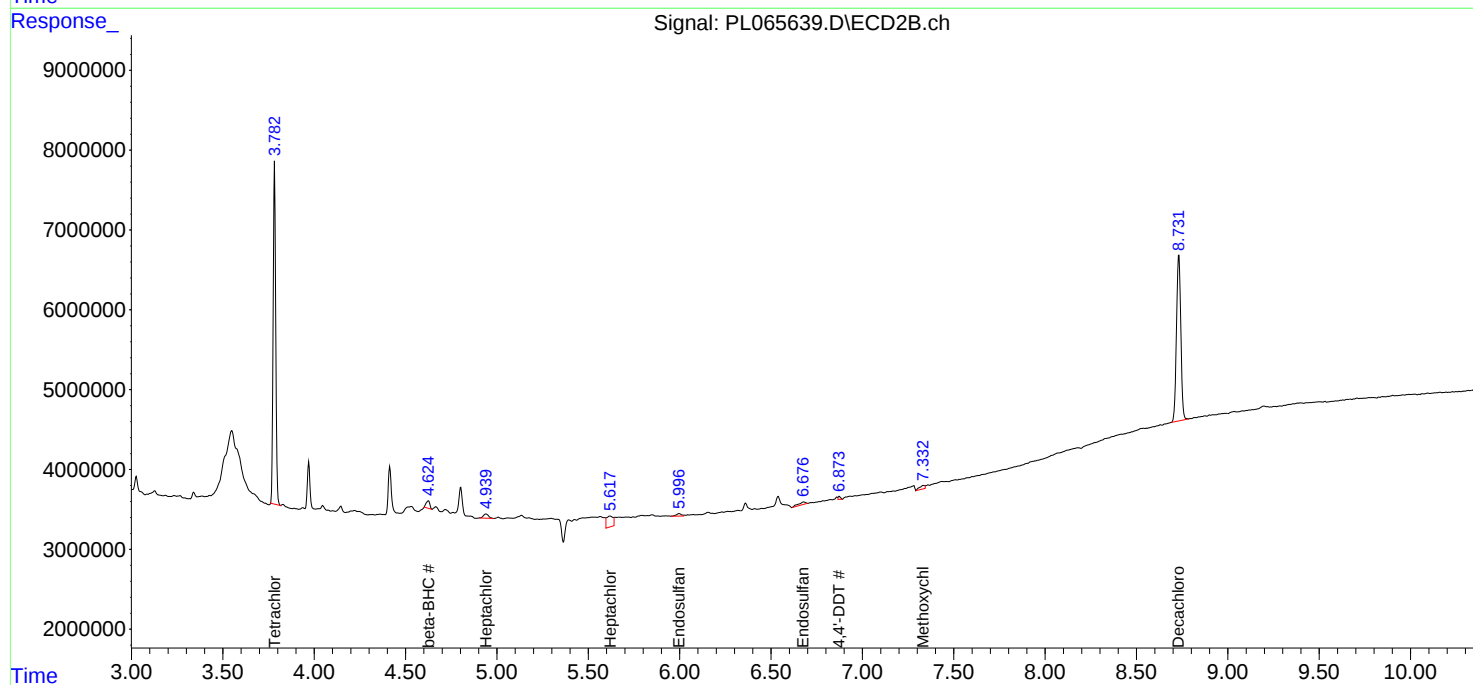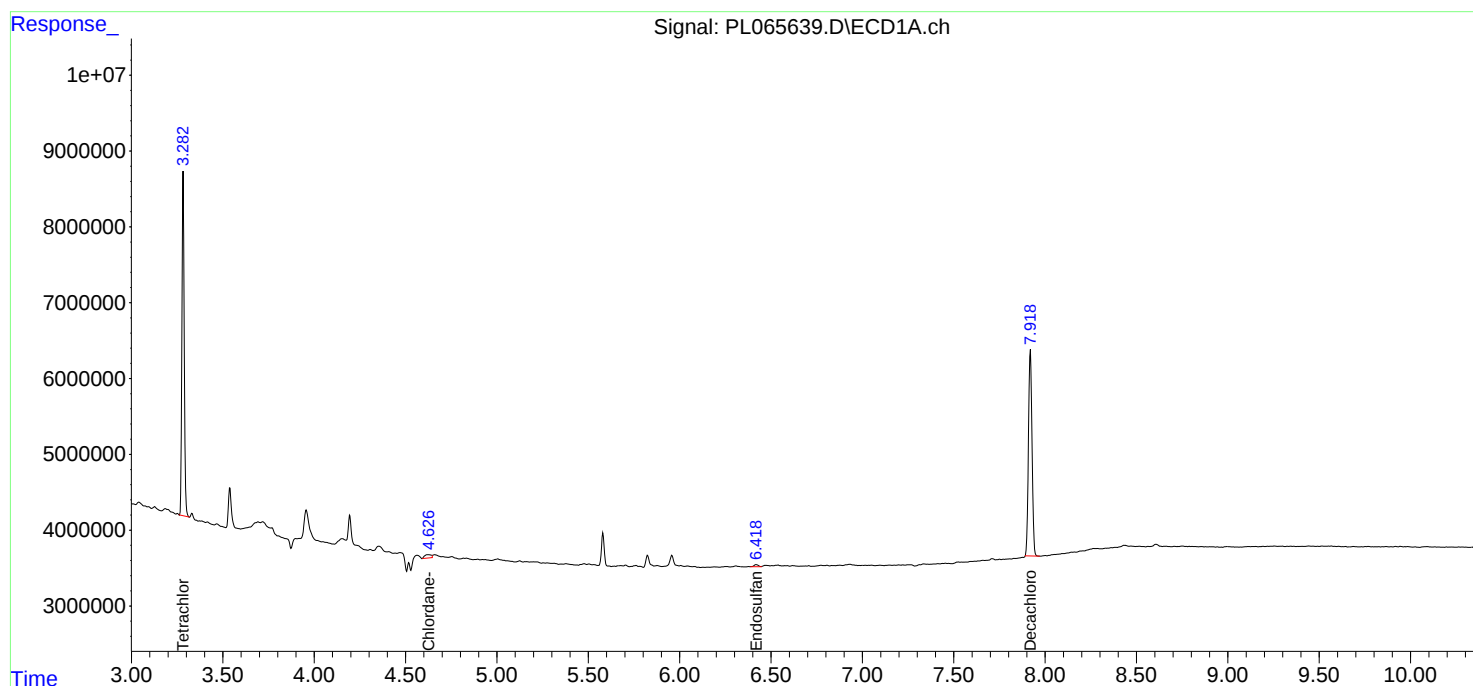


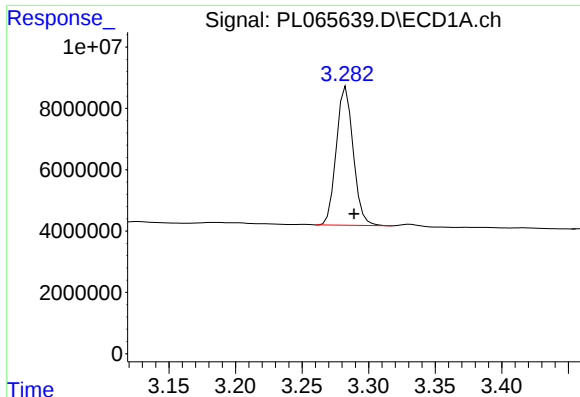

#1 Tetrachloro-m-xylene


R.T.: 3.283 min
Delta R.T.: -0.006 min
Response: 39937921
Conc: 16.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

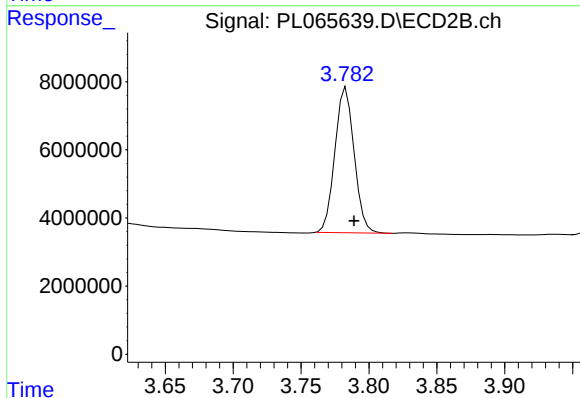


#1 Tetrachloro-m-xylene

R.T.: 3.783 min
Delta R.T.: -0.006 min
Response: 42048162
Conc: 15.32 ng/ml

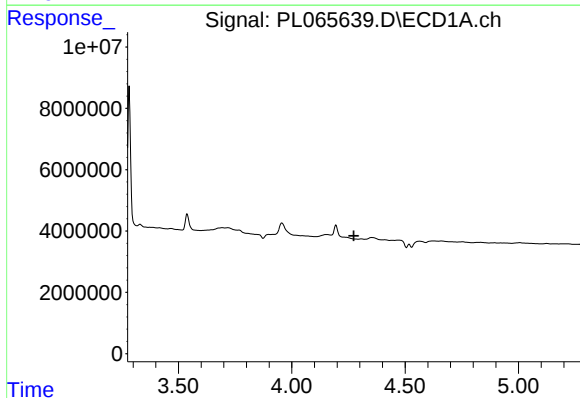


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.274 min
Response: 0
Conc: N.D.

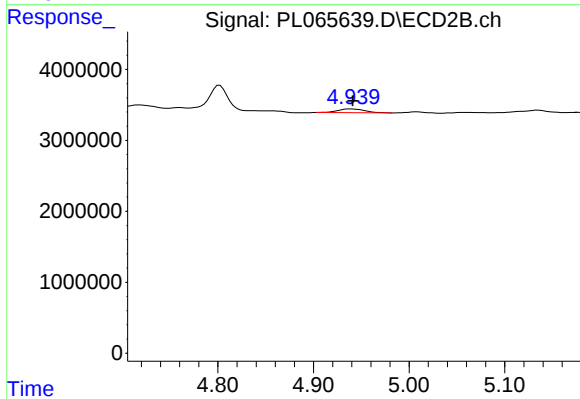

#4 Heptachlor


R.T.: 4.940 min
Delta R.T.: -0.001 min
Response: 1058760
Conc: 0.32 ng/ml

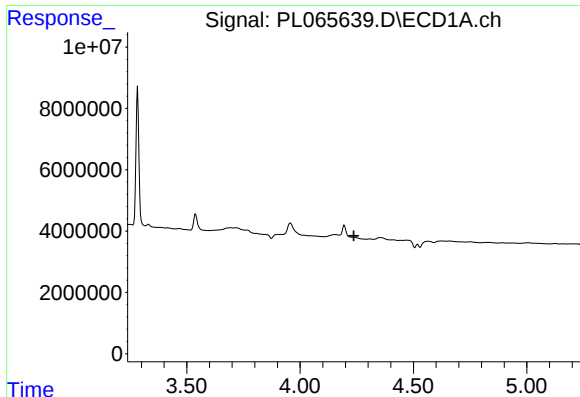

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.238 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

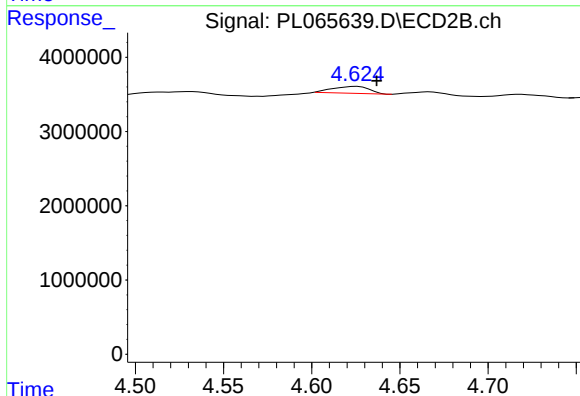


#6 beta-BHC

R.T.: 4.626 min
Delta R.T.: -0.011 min
Response: 1331655
Conc: 0.77 ng/ml

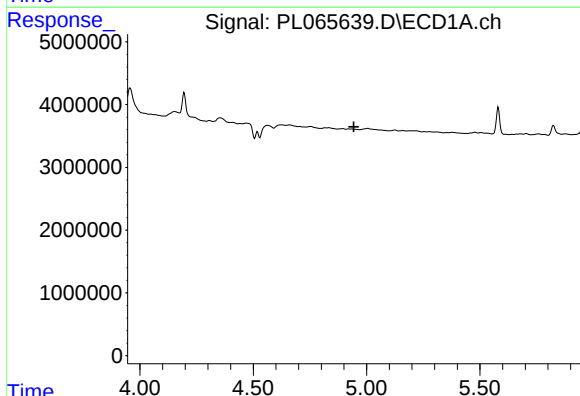


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.944 min
Response: 0
Conc: N.D.

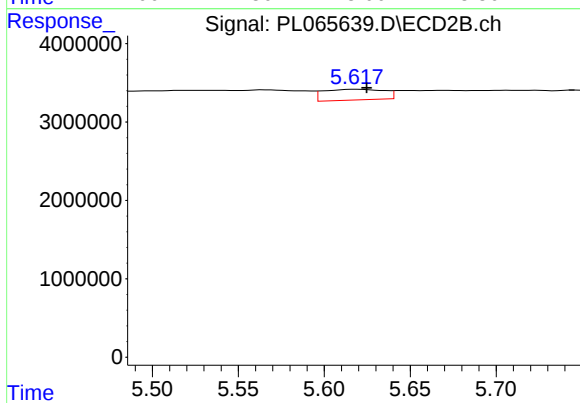

#8 Heptachlor epoxide


R.T.: 5.619 min
Delta R.T.: -0.006 min
Response: 3351405
Conc: 1.16 ng/ml

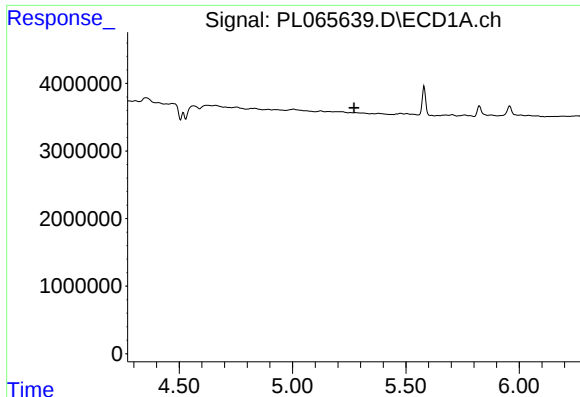

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.271 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

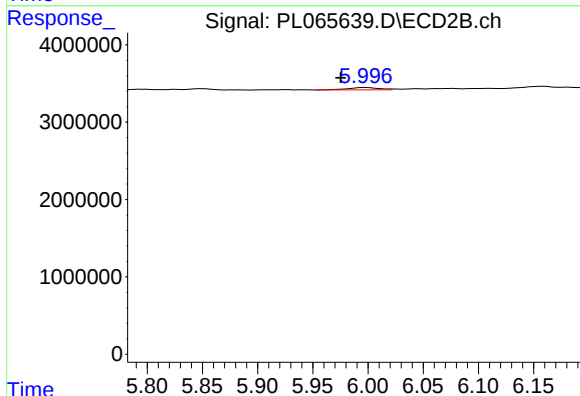


#9 Endosulfan I

R.T.: 5.997 min
Delta R.T.: 0.022 min
Response: 608028
Conc: 0.23 ng/ml

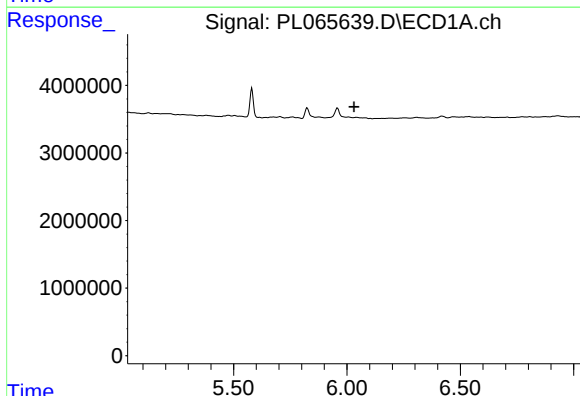


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.031 min
Response: 0
Conc: N.D.

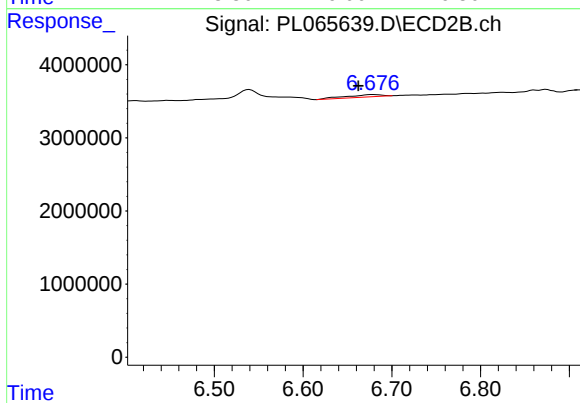

#15 Endosulfan II


R.T.: 6.679 min
Delta R.T.: 0.016 min
Response: 920768
Conc: 0.41 ng/ml

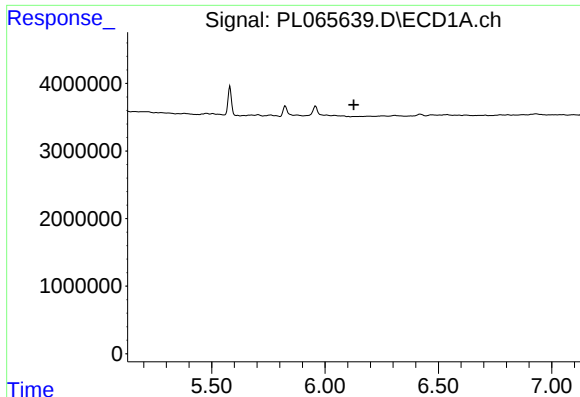

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.128 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

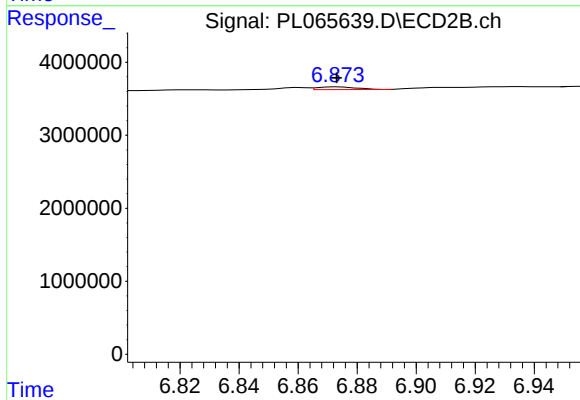


#17 4,4'-DDT

R.T.: 6.874 min
Delta R.T.: 0.000 min
Response: 347730
Conc: 0.18 ng/ml

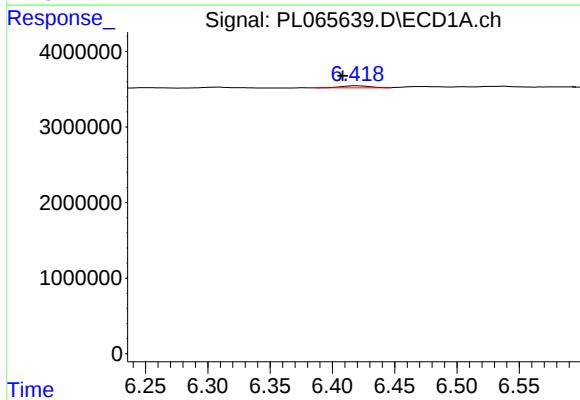


#19 Endosulfan Sulfate

R.T.: 6.419 min
Delta R.T.: 0.011 min
Response: 444766
Conc: 0.18 ng/ml

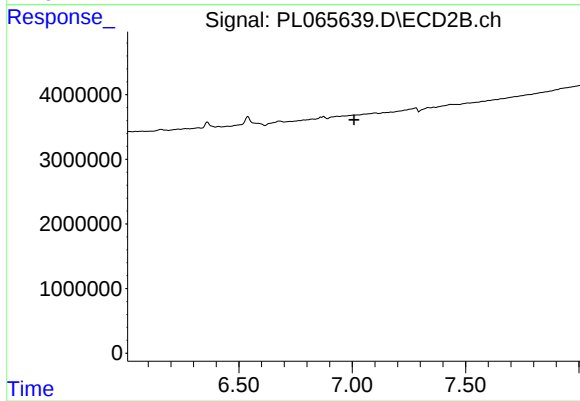

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.009 min
Response: 0
Conc: N.D.

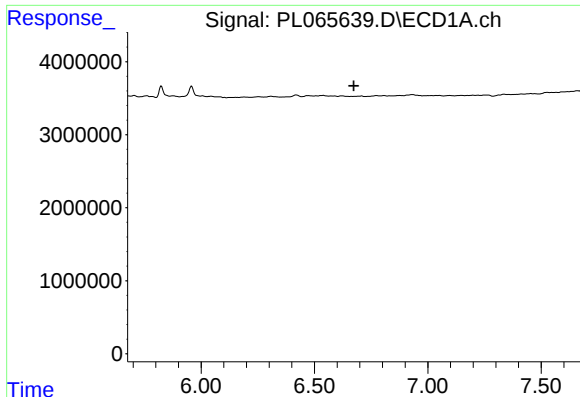

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.673 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

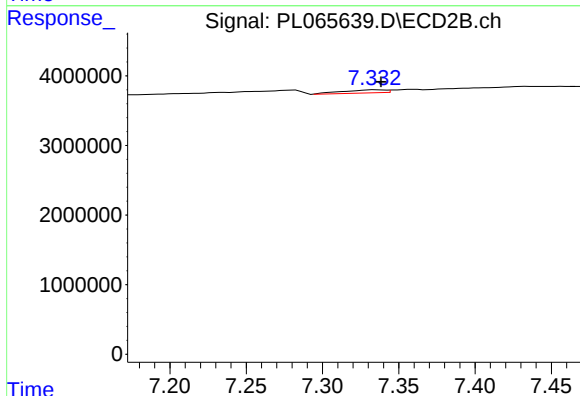


#20 Methoxychlor

R.T.: 7.334 min
Delta R.T.: -0.004 min
Response: 903423
Conc: 0.87 ng/ml

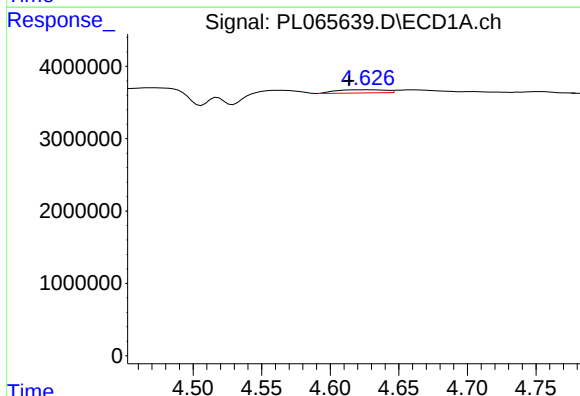


#24 Chlordane-2

R.T.: 4.627 min
Delta R.T.: 0.014 min
Response: 1127438
Conc: 10.39 ng/ml

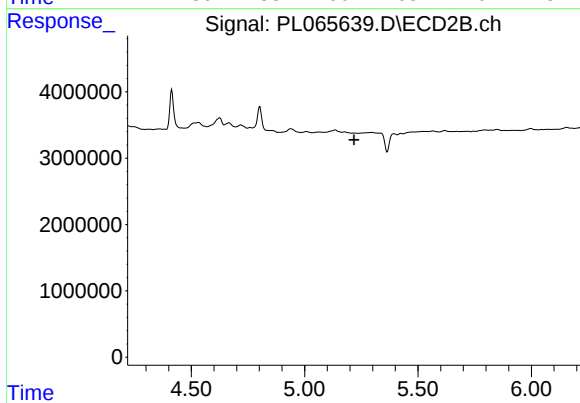

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.219 min
Response: 0
Conc: N.D.

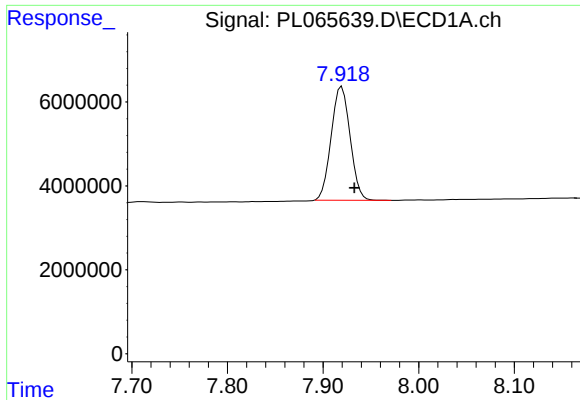

#28 Decachlorobiphenyl

R.T.: 7.920 min
Delta R.T.: -0.013 min
Response: 37181124
Conc: 15.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

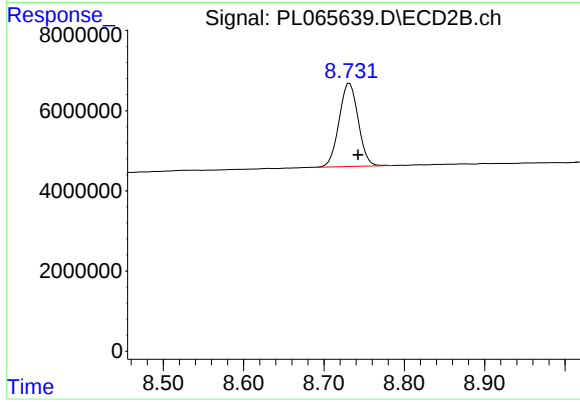

#28 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: -0.011 min
Response: 34359374
Conc: 17.33 ng/ml