

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032921\
 Data File : PL065633.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2021 12:01
 Operator : AR\AJ
 Sample : M1791-16
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EXTERIOR-SLAB-BRICK-1

Manual Integrations
 APPROVED

Ankita
 3/30/2021 2:08:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 13:33:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.283	3.781	38653289	42354289	16.277	15.431m
28)	SA Decachlor...	7.919	8.731	39109964	36125534	16.188	18.226

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032921\
Data File : PL065633.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2021 12:01
Operator : AR\AJ
Sample : M1791-16
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
EXTERIOR-SLAB-BRICK-1


Manual Integrations
APPROVED

Ankita
3/30/2021 2:08:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 13:33:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

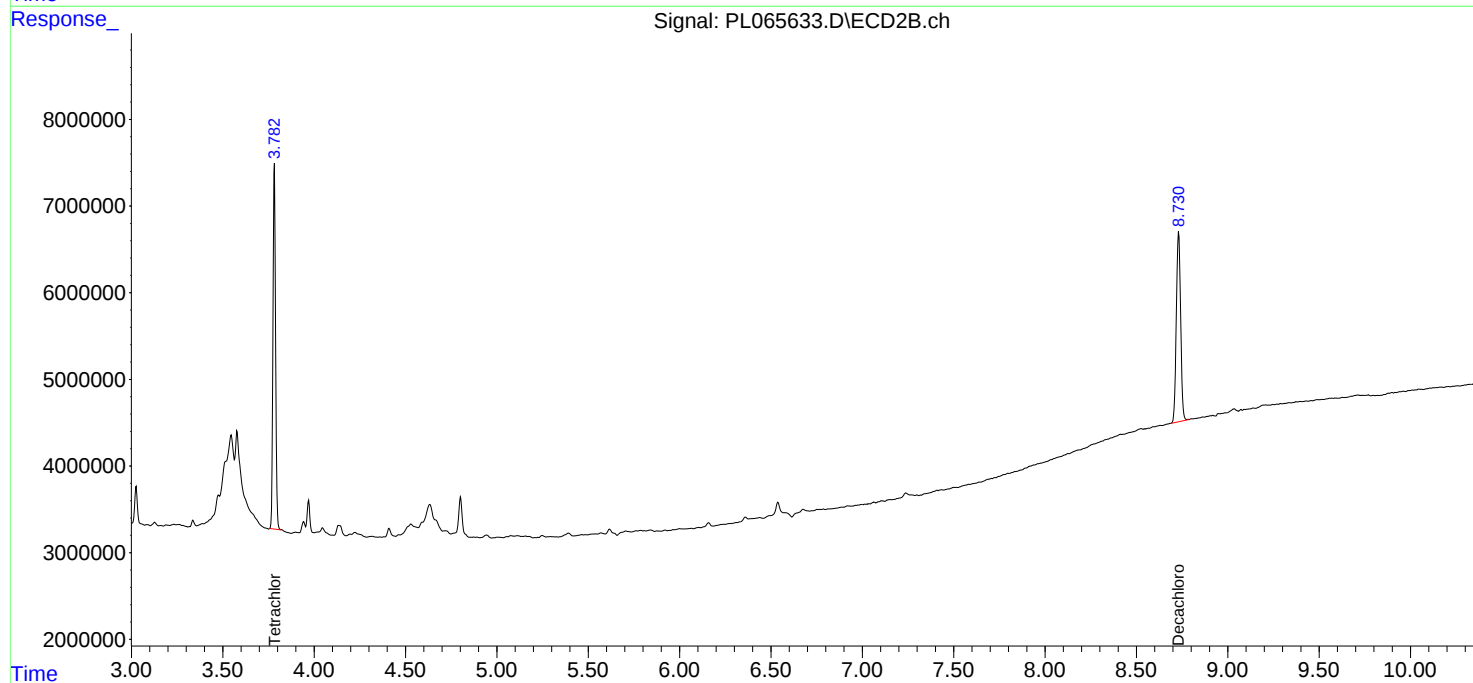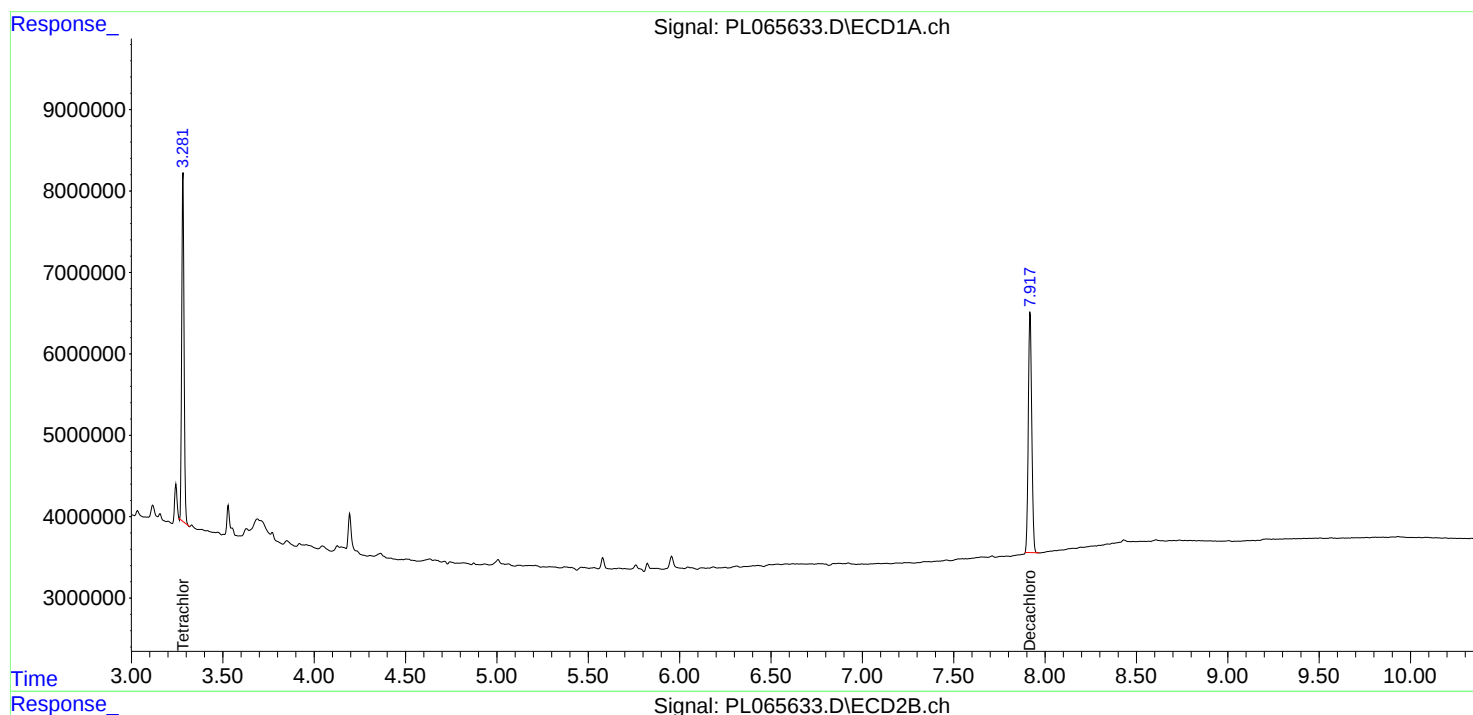

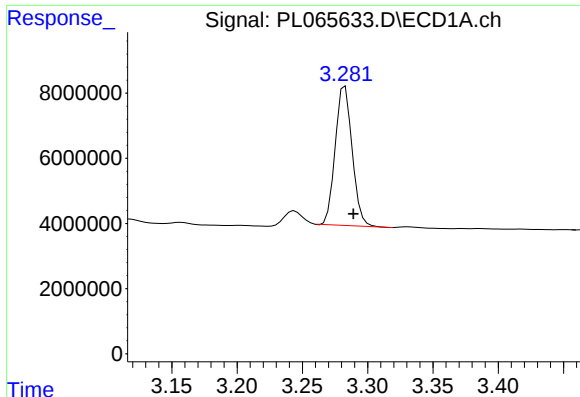


#1 Tetrachloro-m-xylene

R.T.: 3.283 min
Delta R.T.: -0.006 min
Response: 38653289
Conc: 16.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXTERIOR-SLAB-BRICK-1


Manual Integrations
APPROVED

Ankita
3/30/2021 2:08:10 PM

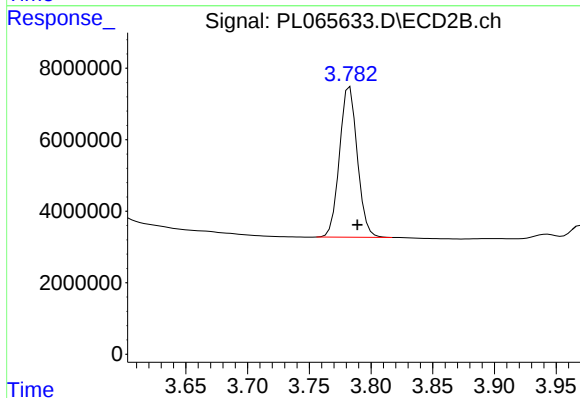


#1 Tetrachloro-m-xylene

R.T.: 3.781 min
Delta R.T.: -0.008 min
Response: 42354289
Conc: 15.43 ng/ml m

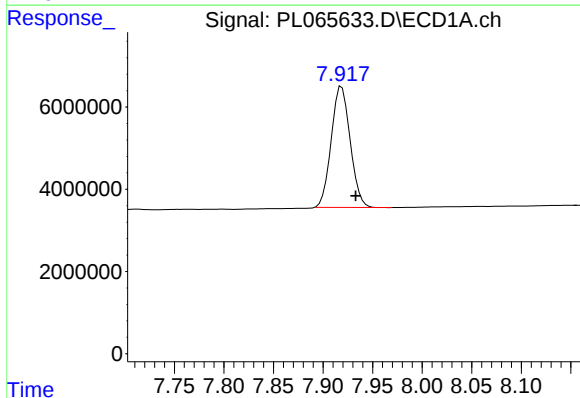

#28 Decachlorobiphenyl

R.T.: 7.919 min
Delta R.T.: -0.014 min
Response: 39109964
Conc: 16.19 ng/ml

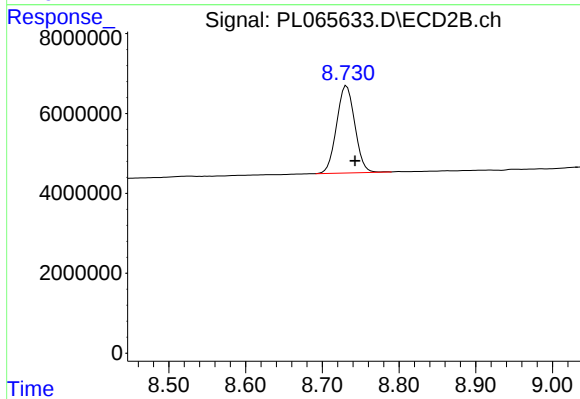

#28 Decachlorobiphenyl

R.T.: 8.731 min
Delta R.T.: -0.011 min
Response: 36125534
Conc: 18.23 ng/ml