

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032921\
 Data File : PL065649.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2021 17:19
 Operator : AR\AJ
 Sample : PB135375BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB135375BS

Manual Integrations
 APPROVED

Ankita
 3/30/2021 2:08:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 07:18:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.302	3.783	49556290	52248055	20.868	19.036
28)	SA Decachlor...	7.940	8.735	46385264	41979497	19.199m	21.179

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032921\
Data File : PL065649.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2021 17:19
Operator : AR\AJ
Sample : PB135375BL
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB135375BS


Manual Integrations
APPROVED

Ankita
3/30/2021 2:08:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 07:18:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

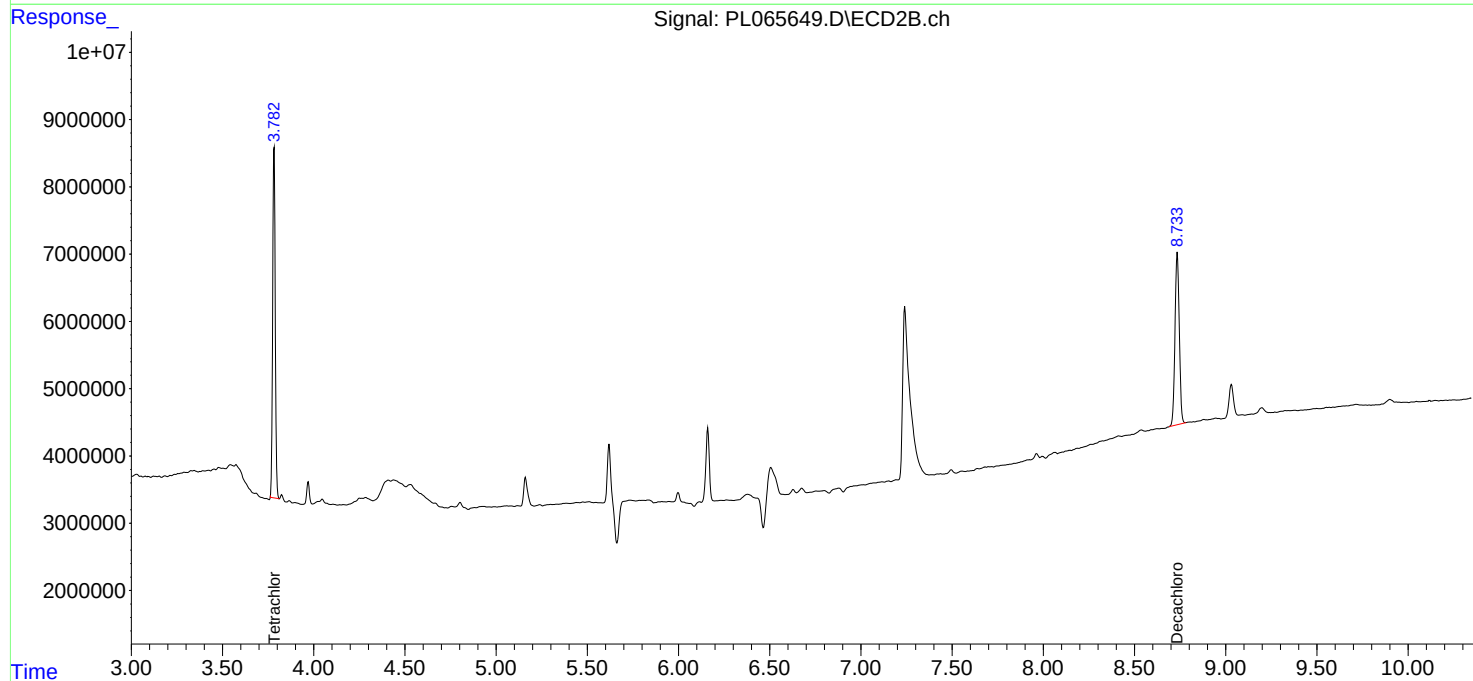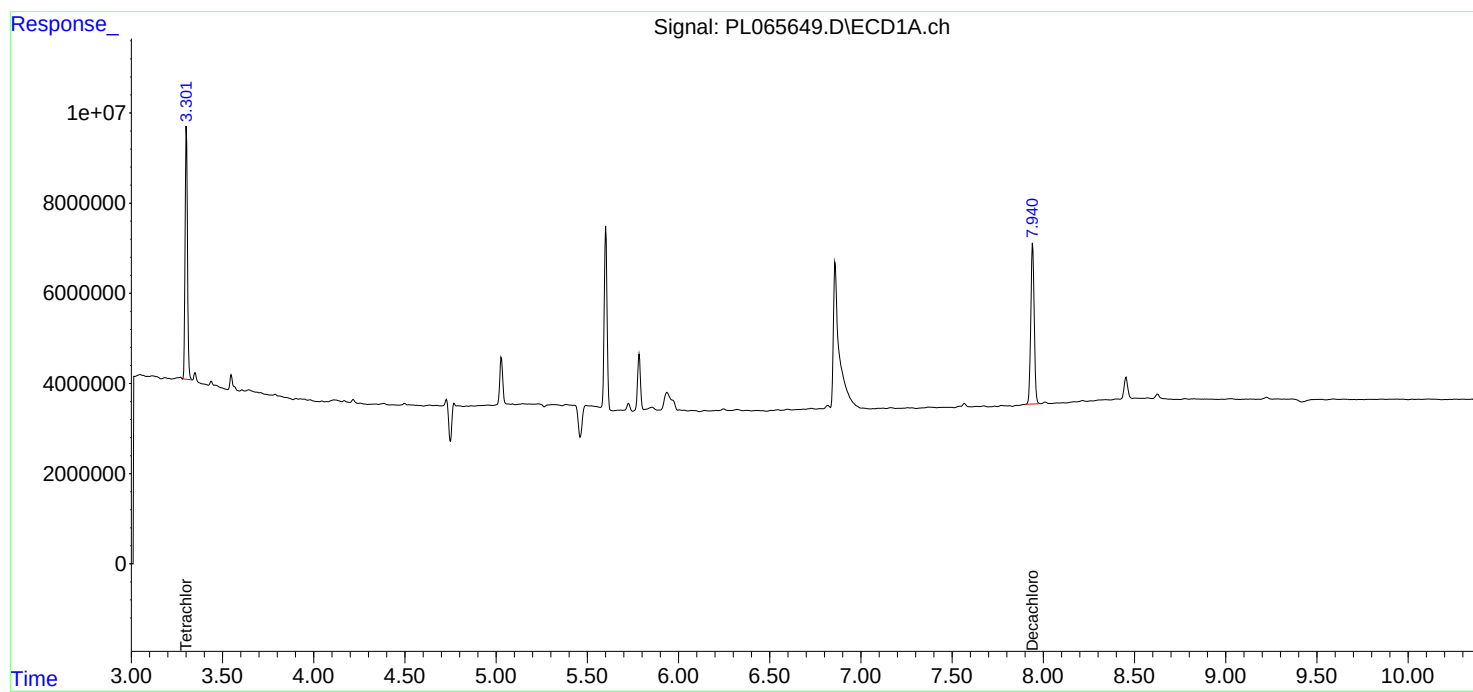

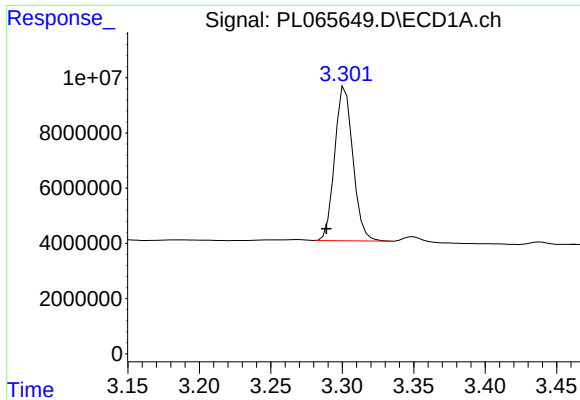


#1 Tetrachloro-m-xylene

R.T.: 3.302 min
Delta R.T.: 0.013 min
Response: 49556290
Conc: 20.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135375BS


Manual Integrations
APPROVED

Ankita
3/30/2021 2:08:15 PM

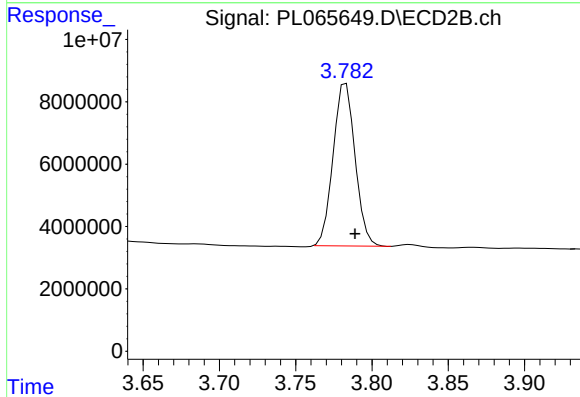


#1 Tetrachloro-m-xylene

R.T.: 3.783 min
Delta R.T.: -0.006 min
Response: 52248055
Conc: 19.04 ng/ml

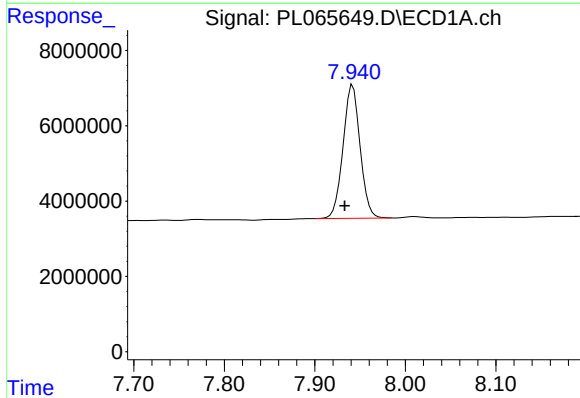

#28 Decachlorobiphenyl

R.T.: 7.940 min
Delta R.T.: 0.008 min
Response: 46385264
Conc: 19.20 ng/ml m

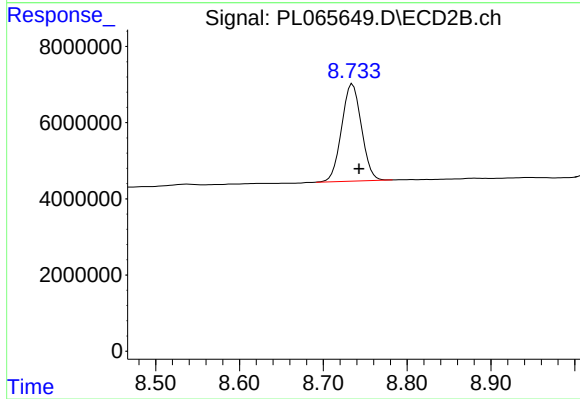

#28 Decachlorobiphenyl

R.T.: 8.735 min
Delta R.T.: -0.008 min
Response: 41979497
Conc: 21.18 ng/ml