

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032924\
 Data File : PL088833.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2024 15:28
 Operator : AR\AJ
 Sample : P1917-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CCM-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 00:35:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:45:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.634	2.851	55385696	30372472	20.901	22.789
28)	SA Decachlor...	9.305	8.081	43071208	28470792	17.424	20.997
Target Compounds							
4)	MA Heptachlor	5.037	4.050	1920737	874928	0.506	0.486



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032924\
Data File : PL088833.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2024 15:28
Operator : AR\AJ
Sample : P1917-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CCM-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 00:35:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:45:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

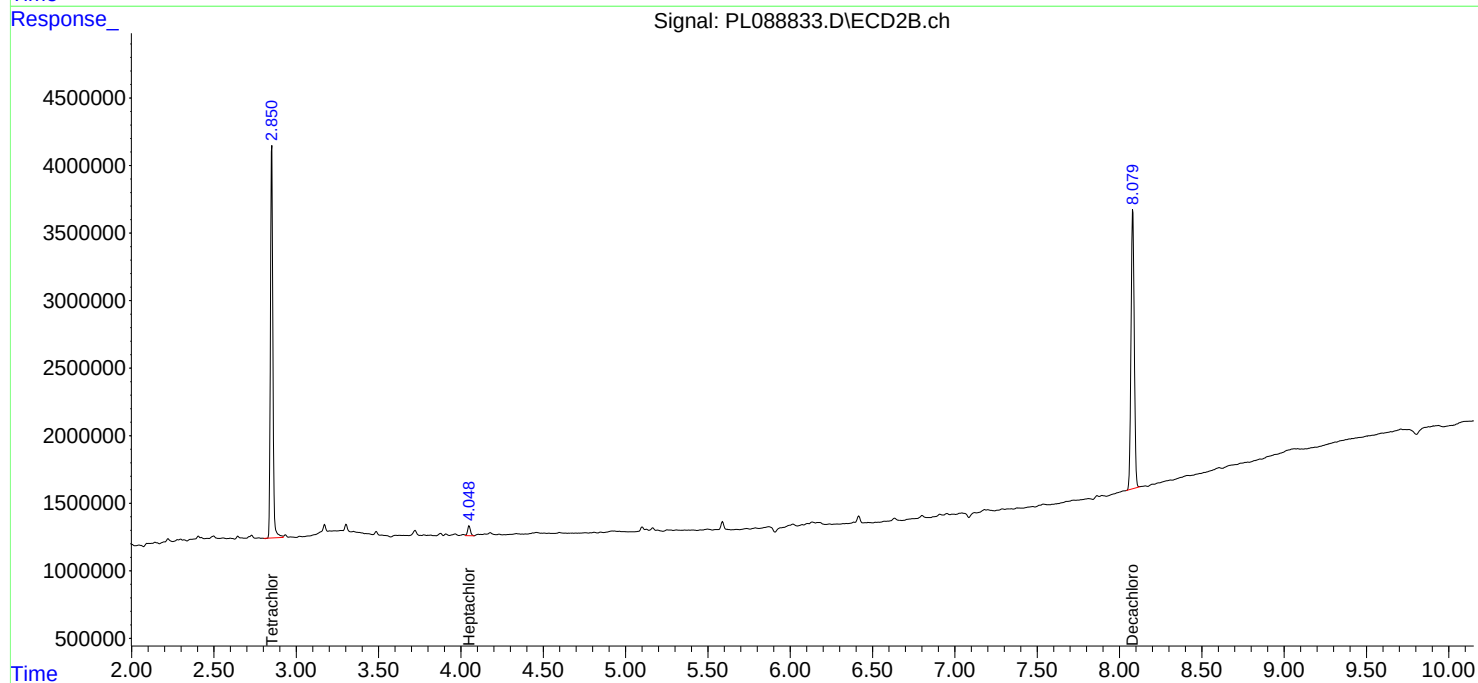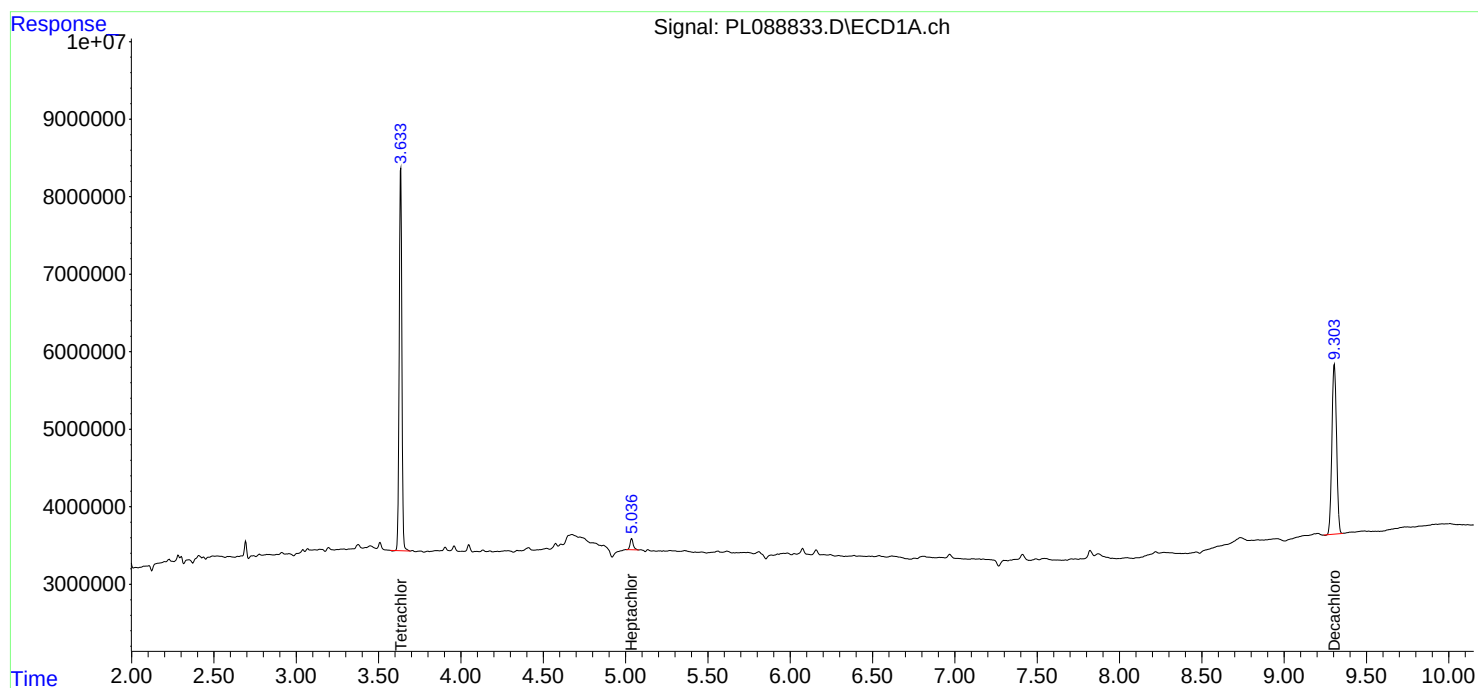


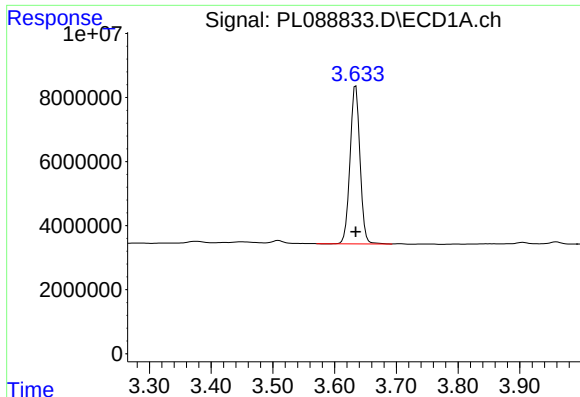

#1 Tetrachloro-m-xylene


R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 55385696
Conc: 20.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
CCM-2

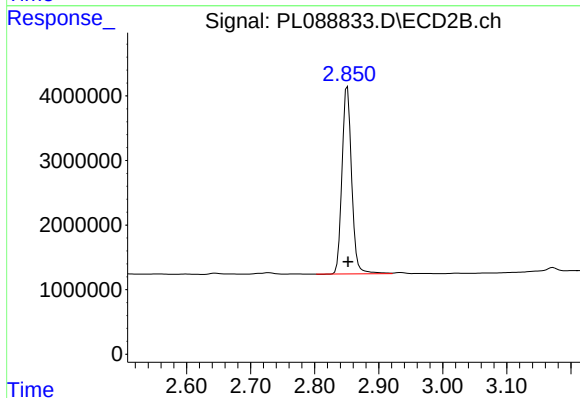


#1 Tetrachloro-m-xylene

R.T.: 2.851 min
Delta R.T.: -0.001 min
Response: 30372472
Conc: 22.79 ng/ml

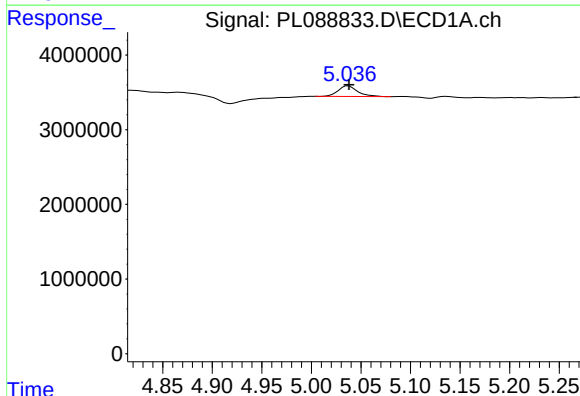


#4 Heptachlor

R.T.: 5.037 min
Delta R.T.: 0.000 min
Response: 1920737
Conc: 0.51 ng/ml

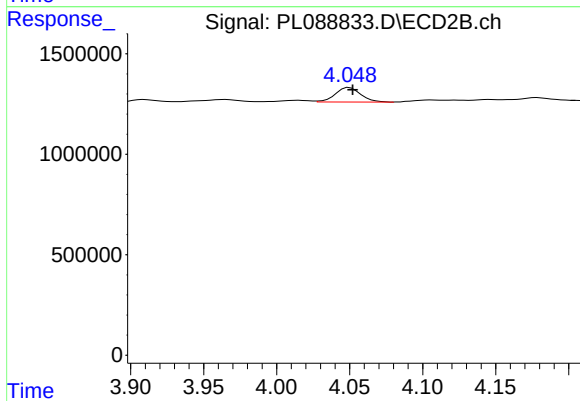

#4 Heptachlor


R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 874928
Conc: 0.49 ng/ml

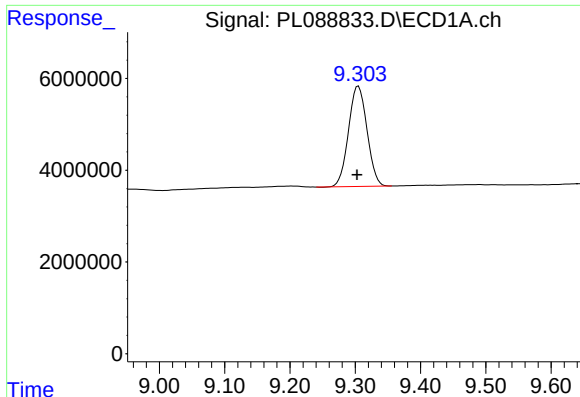

#28 Decachlorobiphenyl

R.T.: 9.305 min
Delta R.T.: 0.002 min
Response: 43071208
Conc: 17.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
CCM-2

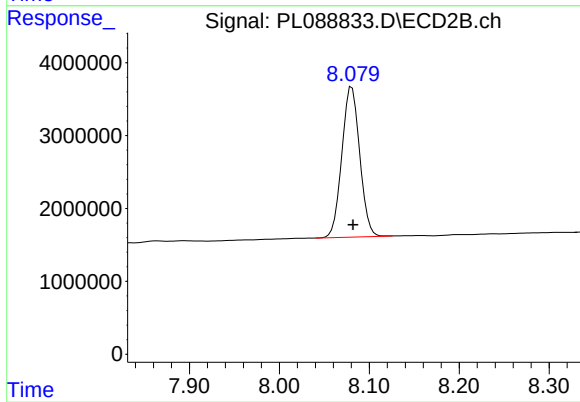

#28 Decachlorobiphenyl

R.T.: 8.081 min
Delta R.T.: -0.001 min
Response: 28470792
Conc: 21.00 ng/ml